

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071724\
 Data File : P0104796.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2024 12:37
 Operator : YP/AJ
 Sample : P3253-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ELZ-24-00058

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/18/2024
 Supervised By :Ankita Jodhani 07/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 01:42:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070224.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 02 16:29:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.428	3.542	158.0E6	60012503	17.649	18.394
2) SA Decachlor...	10.217	8.438	111.7E6	42720461	18.211m	20.371m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071724\
Data File : PO104796.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2024 12:37
Operator : YP/AJ
Sample : P3253-07
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ELZ-24-00058


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :Ankita Jodhani 07/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 01:42:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO070224.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 02 16:29:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

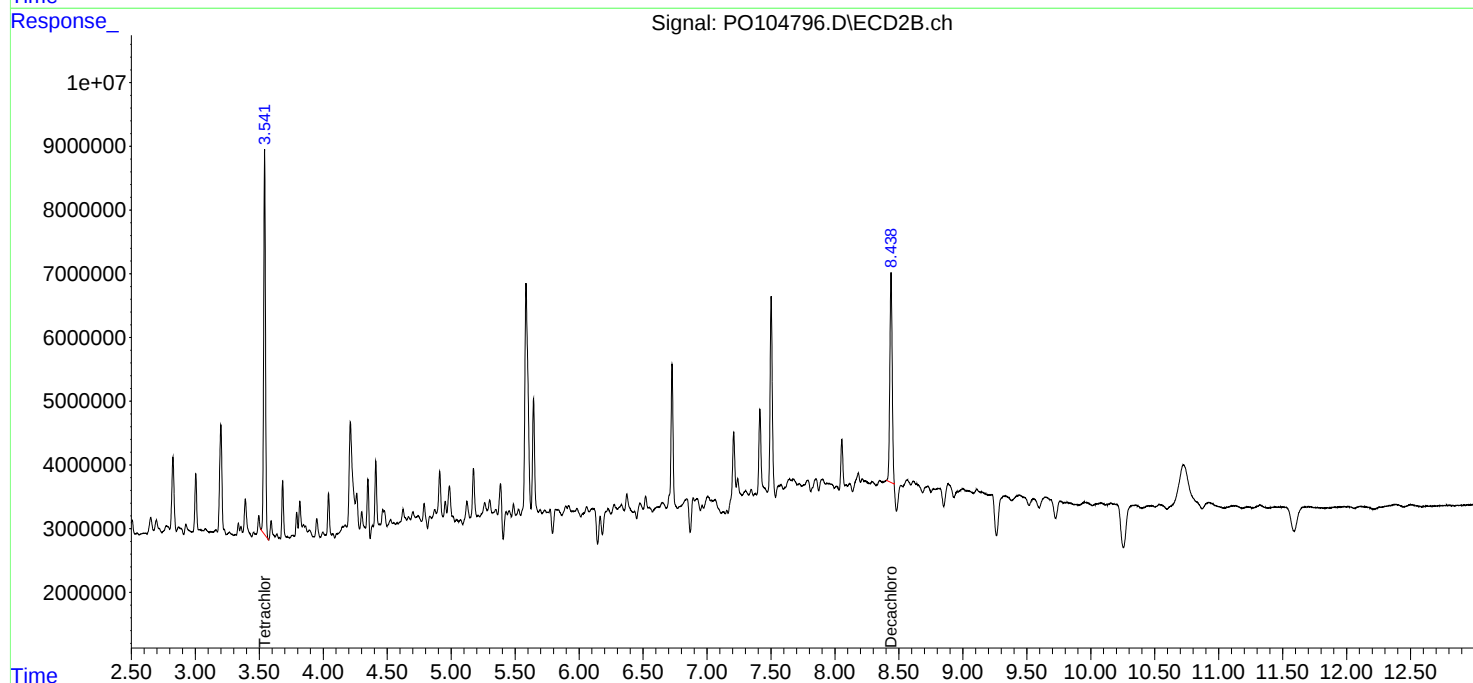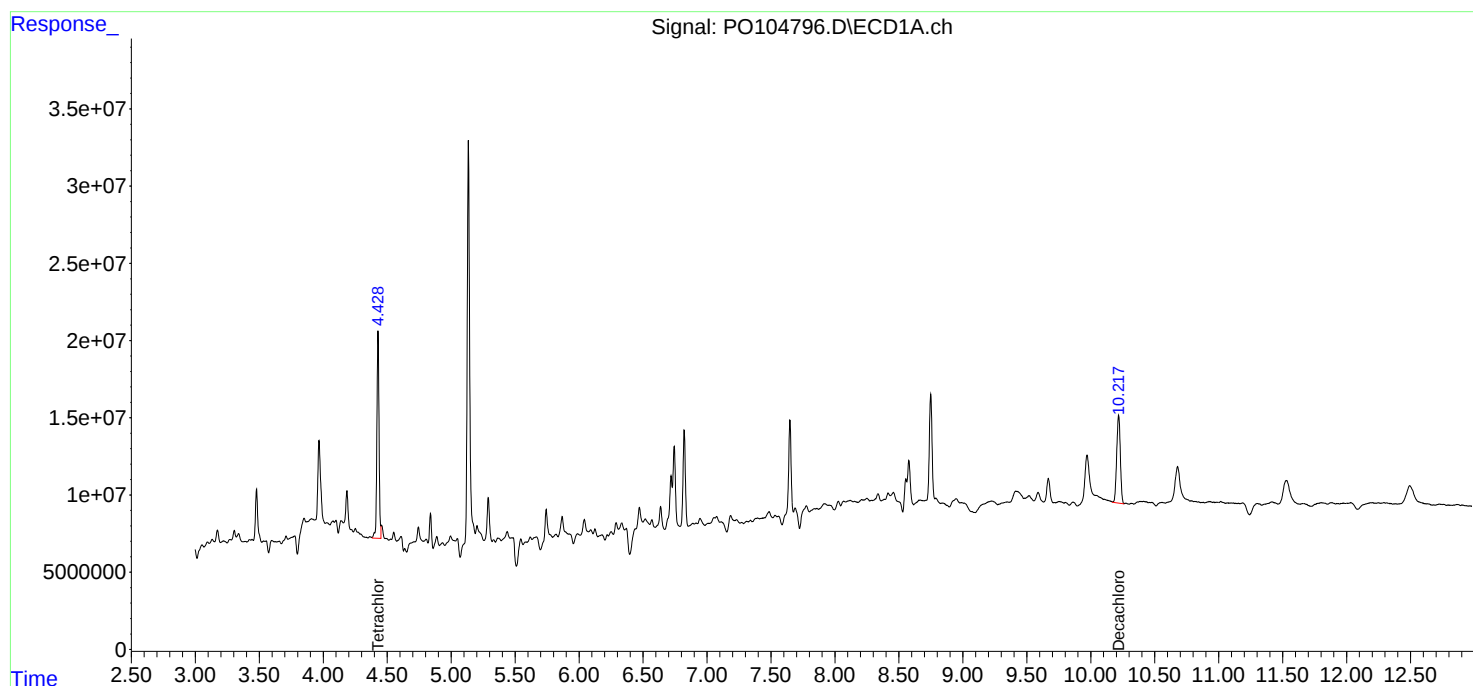

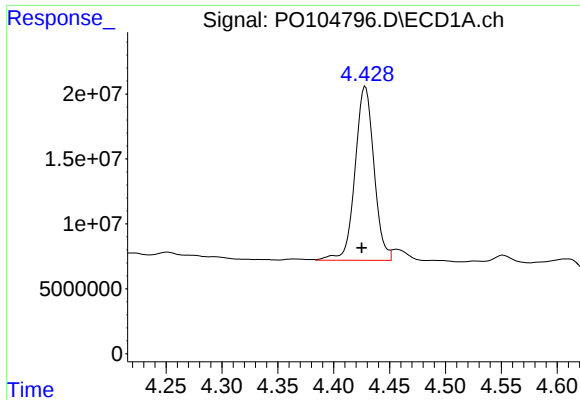


#1 Tetrachloro-m-xylene

R.T.: 4.428 min
Delta R.T.: 0.003 min
Response: 158021014
Conc: 17.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
ELZ-24-00058


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :Ankita Jodhani 07/19/2024

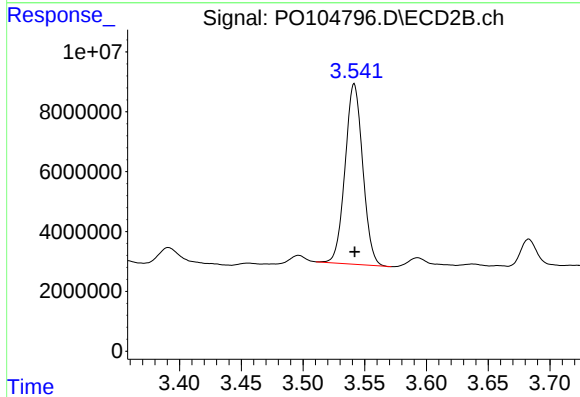


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: 0.000 min
Response: 60012503
Conc: 18.39 ng/ml

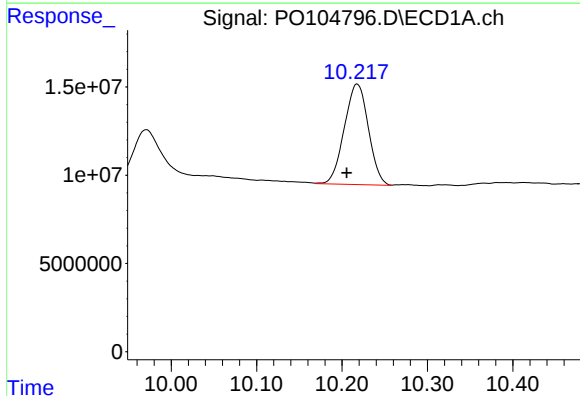

#2 Decachlorobiphenyl

R.T.: 10.217 min
Delta R.T.: 0.011 min
Response: 111679507
Conc: 18.21 ng/ml m

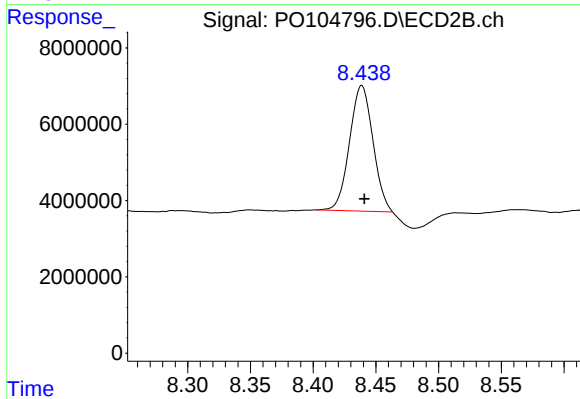

#2 Decachlorobiphenyl

R.T.: 8.438 min
Delta R.T.: -0.002 min
Response: 42720461
Conc: 20.37 ng/ml m