

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071724\
 Data File : P0104805.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2024 15:42
 Operator : YP/AJ
 Sample : P3254-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SOM-24-00069

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/18/2024
 Supervised By :Ankita Jodhani 07/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 01:46:31 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070224.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 02 16:29:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.418	3.543	180.1E6	41890825	20.121	12.840m#
2) SA Decachlor...	10.225	8.448	107.3E6	30073330	17.502m	14.340

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071724\
Data File : PO104805.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2024 15:42
Operator : YP/AJ
Sample : P3254-03
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SOM-24-00069


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :Ankita Jodhani 07/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 01:46:31 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO070224.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 02 16:29:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

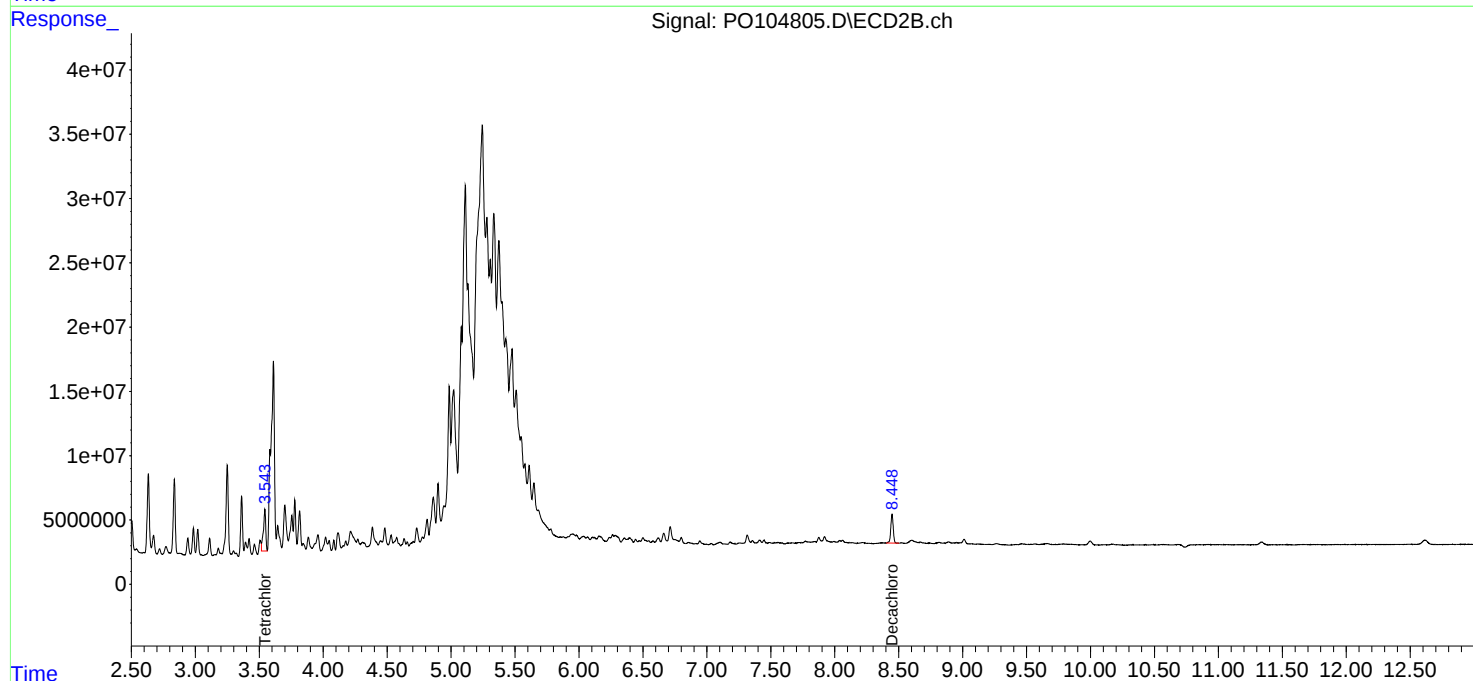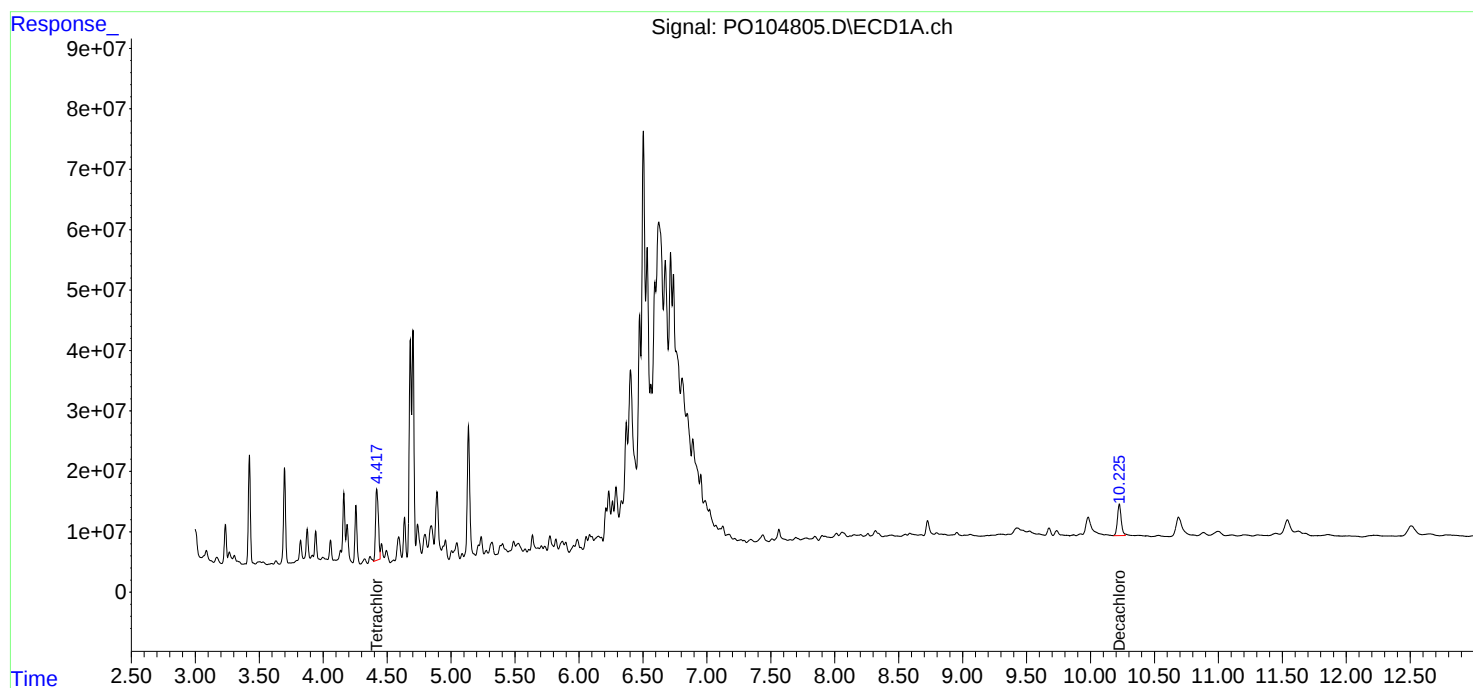

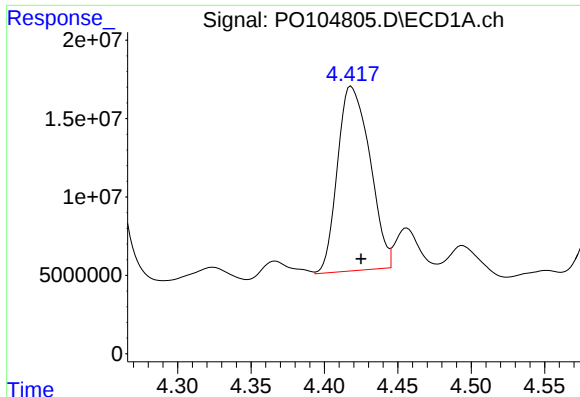


#1 Tetrachloro-m-xylene

R.T.: 4.418 min
Delta R.T.: -0.007 min
Response: 180148974
Conc: 20.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
SOM-24-00069


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/18/2024
Supervised By :Ankita Jodhani 07/19/2024

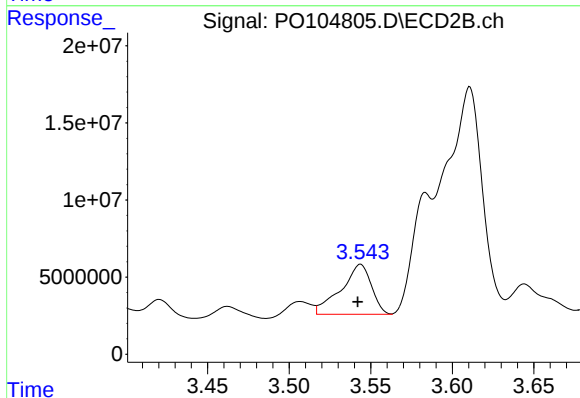


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: 0.001 min
Response: 41890825
Conc: 12.84 ng/ml m

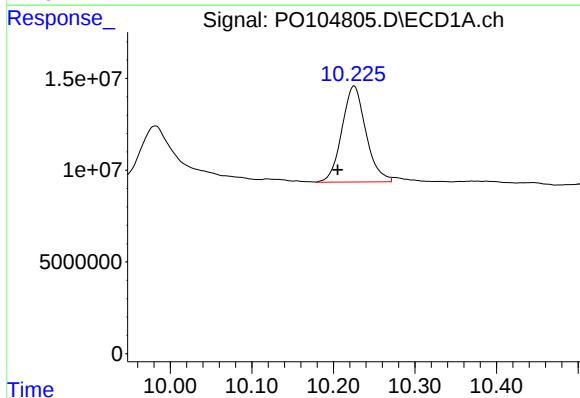

#2 Decachlorobiphenyl

R.T.: 10.225 min
Delta R.T.: 0.019 min
Response: 107333814
Conc: 17.50 ng/ml m

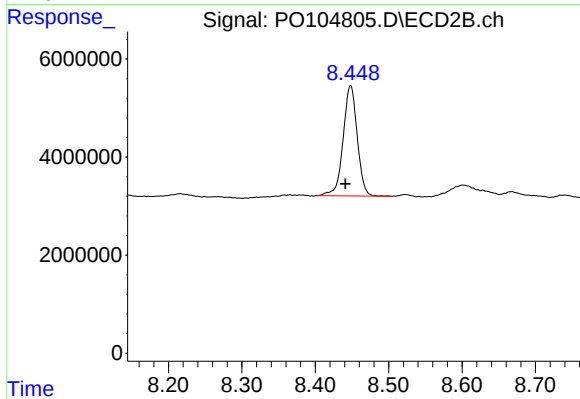

#2 Decachlorobiphenyl

R.T.: 8.448 min
Delta R.T.: 0.007 min
Response: 30073330
Conc: 14.34 ng/ml