

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0071725\
 Data File : P0112316.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2025 11:32
 Operator : YP/AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 01:17:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 10:50:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.686	3.679	304023	90356	0.031	0.014 #
2)	SA Decachlor...	8.699	8.669	422778	27240	0.062	0.016 #
Target Compounds							
3)	L1 AR-1016-1	4.750	4.755	-7068	244287	N.D.	1.096 #
4)	L1 AR-1016-2	4.777	4.784	581754	285732	1.170	0.868 #
5)	L1 AR-1016-3	4.828	4.943	323402	470445	0.999	2.769 #
6)	L1 AR-1016-4	4.956	4.998	4161994	912385	16.207	6.649 #
7)	L1 AR-1016-5	5.209	5.207	12941995	1202141	47.292	6.971 #
8)	L2 AR-1221-1	3.841f	3.876	946679	22494	8.118	0.273 #
9)	L2 AR-1221-2	0.000	3.952	0	82074	N.D.	1.383 #
10)	L2 AR-1221-3	0.000	4.033	0	19353	N.D.	0.103 #
11)	L3 AR-1232-1	0.000	4.033	0	19353	N.D.	0.129 #
12)	L3 AR-1232-2	4.544	4.755	1067790	244287	9.397	1.596 #
13)	L3 AR-1232-3	4.777	4.939	581754	322043	2.540	4.265 #
14)	L3 AR-1232-4	4.956	5.022	4161994	408553	36.414	6.191 #
15)	L3 AR-1232-5	5.014	5.190	5919621	1930146	80.649	25.992 #
16)	L4 AR-1242-1	4.750	4.744	-7068	253868	N.D.	1.310 #
17)	L4 AR-1242-2	4.777	4.755	581754	244287	1.366	0.862 #
18)	L4 AR-1242-3	4.828	4.939	323402	322043	1.182	2.211 #
19)	L4 AR-1242-4	4.956	5.022	4161994	408553	18.472	2.880 #
20)	L4 AR-1242-5	5.624	5.523	21090696	3887154	99.639	21.389 #
21)	L5 AR-1248-1	4.750	4.744	-7068	253868	N.D.	1.645 #
22)	L5 AR-1248-2	5.014	4.984	5919621	1699119	19.199	8.257 #
23)	L5 AR-1248-3	5.209	5.022	12941995	408553	31.774	1.902 #
24)	L5 AR-1248-4	5.551	5.190	15629727	1930146	27.081	7.460 #
25)	L5 AR-1248-5	5.624	5.590	21090696	1569651	54.037	6.265 #
26)	L6 AR-1254-1	5.551	5.523	15629727	3887154	25.410	10.198 #
27)	L6 AR-1254-2	5.705	5.681	3975465	768373	7.421	2.316 #
28)	L6 AR-1254-3	6.108	6.104	180837	14889002	0.215	30.887 #
29)	L6 AR-1254-4	6.364	6.330	2347048	2642650	4.879	10.137 #
30)	L6 AR-1254-5	6.763	6.729	4140.8E6	1927.6E6	5350.201	5409.132
31)	L7 AR-1260-1	6.252	6.248	174693	784994	0.349	2.798 #
32)	L7 AR-1260-2	6.442	6.408	9589298	6718671	12.991	19.761 #
33)	L7 AR-1260-3	6.843f	6.604	2118045	133503	3.231	0.484 #
34)	L7 AR-1260-4	7.076	7.031	4175677	764747	9.594	3.811 #
35)	L7 AR-1260-5	7.306	7.283	2195533	349256	1.739	0.780 #
36)	L8 AR-1262-1	6.843f	6.729f	2118045	1927.6E6	2.073	4732.332 #
37)	L8 AR-1262-2	7.594	7.283	2195533	349256	1.339	0.681 #
38)	L8 AR-1262-3	7.594	7.555	3117617	1927120	4.856	10.735 #
39)	L8 AR-1262-4	7.654	7.618	824680	121153	0.770	0.416 #
40)	L8 AR-1262-5	8.130	8.109	650192	23715	1.451	0.224 #
41)	L9 AR-1268-1	7.594	7.555	3117617	1927120	1.697	3.921 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071725\
 Data File : P0112316.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Jul 2025 11:32
 Operator : YP/AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 01:17:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 10:50:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	7.654	7.618	824680	121153	0.529	0.290 #
43) L9	AR-1268-3	7.863	7.816	1101167	78204	0.847	0.247 #
44) L9	AR-1268-4	8.130	8.109	650192	23715	1.353	0.213 #
45) L9	AR-1268-5	8.442	8.399	309245	21558	0.095	0.030 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071725\
Data File : PO112316.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Jul 2025 11:32
Operator : YP/AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 01:17:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 09 10:50:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

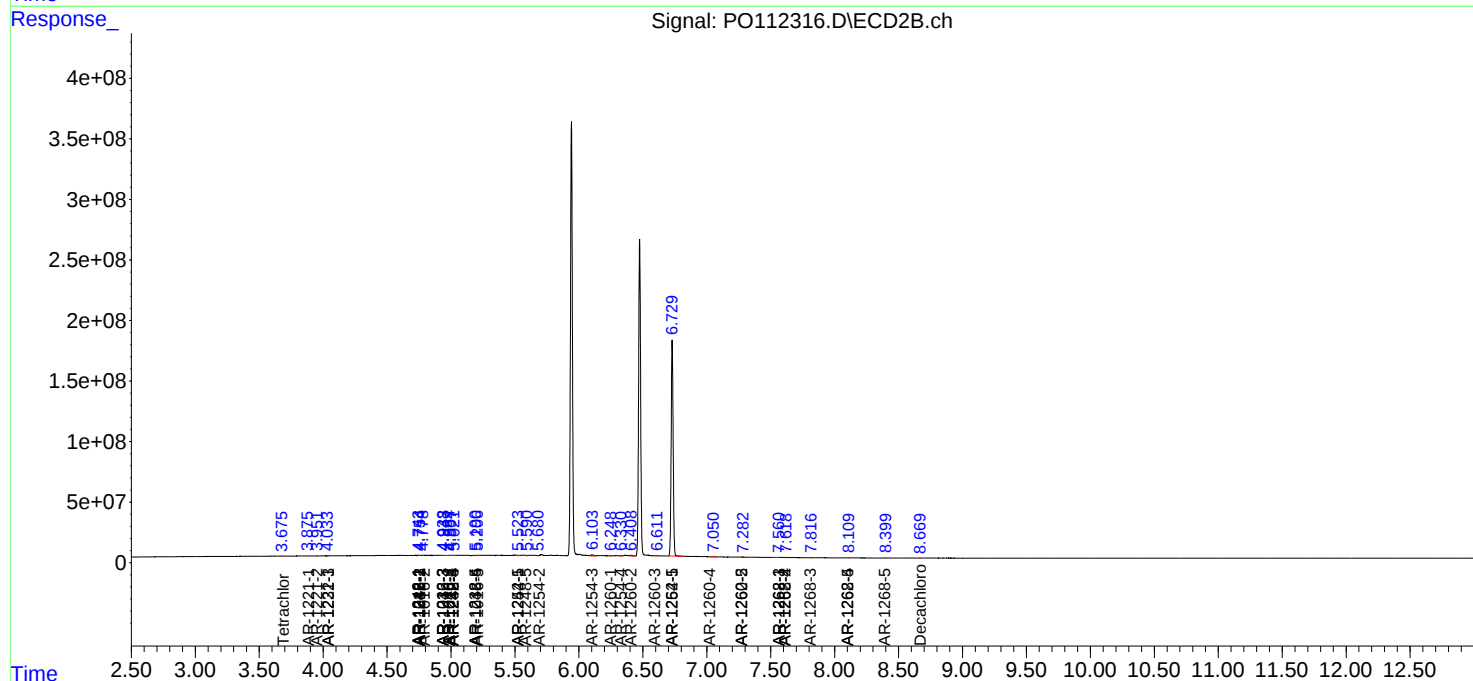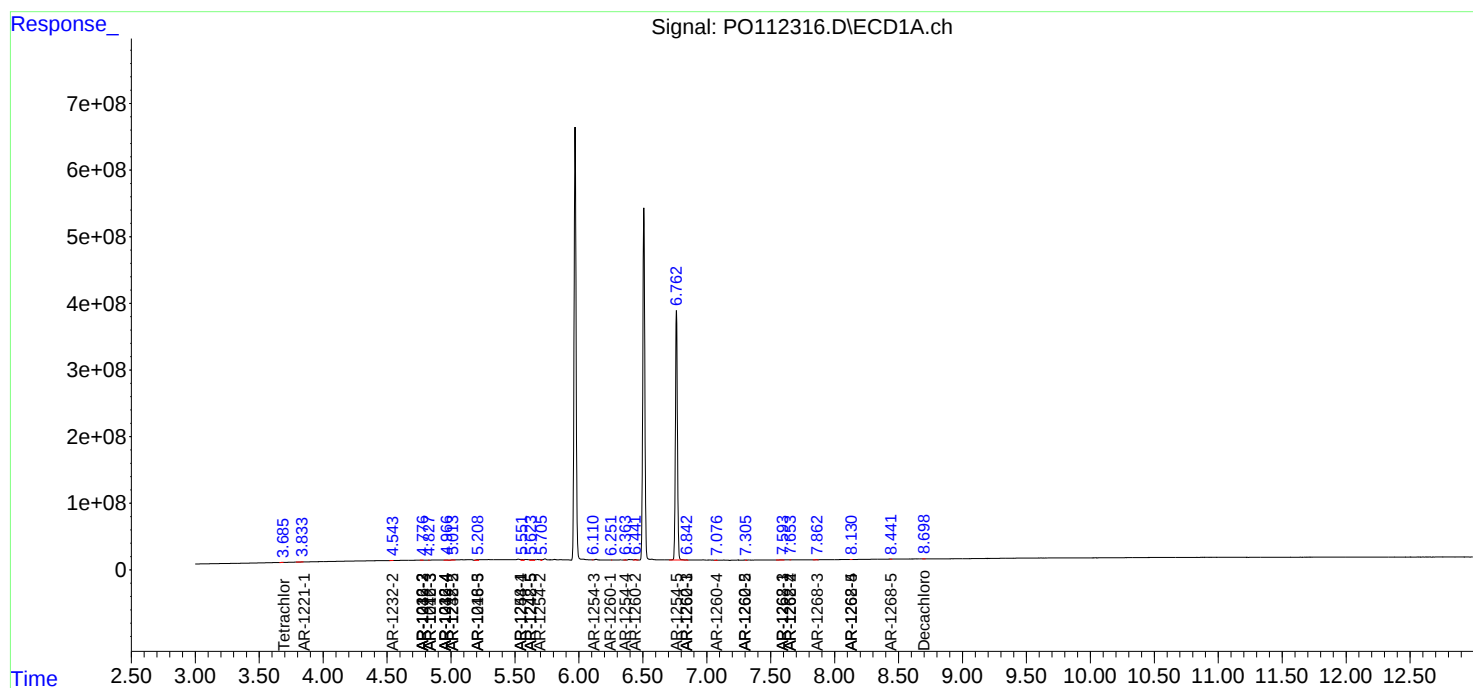


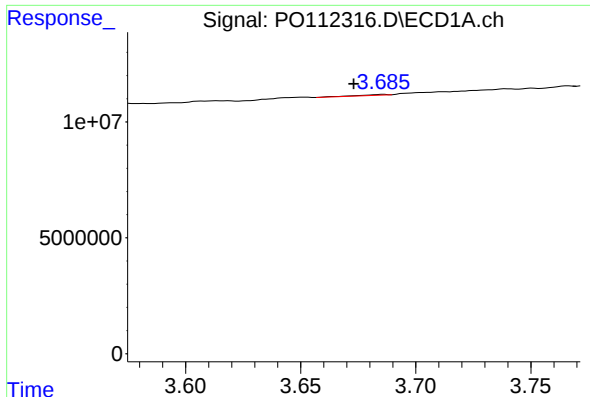

#1 Tetrachloro-m-xylene


R.T.: 3.686 min
Delta R.T.: 0.013 min
Response: 304023
Conc: 0.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

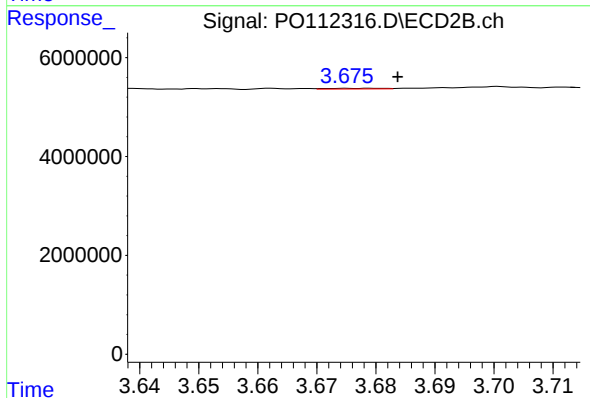


#1 Tetrachloro-m-xylene

R.T.: 3.679 min
Delta R.T.: -0.005 min
Response: 90356
Conc: 0.01 ng/ml

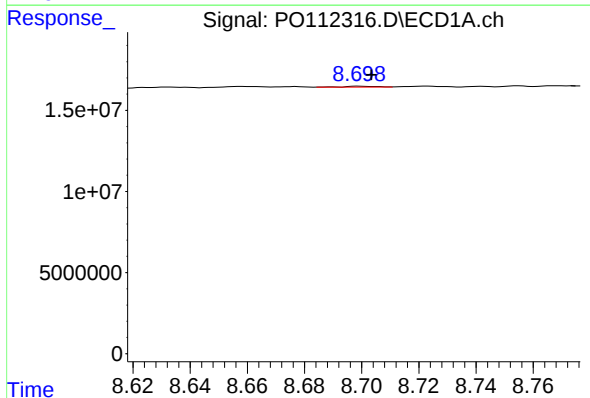


#2 Decachlorobiphenyl

R.T.: 8.699 min
Delta R.T.: -0.004 min
Response: 422778
Conc: 0.06 ng/ml

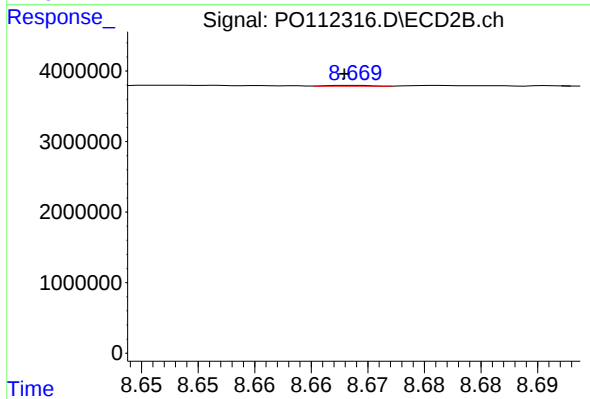

#2 Decachlorobiphenyl


R.T.: 8.669 min
Delta R.T.: 0.000 min
Response: 27240
Conc: 0.02 ng/ml

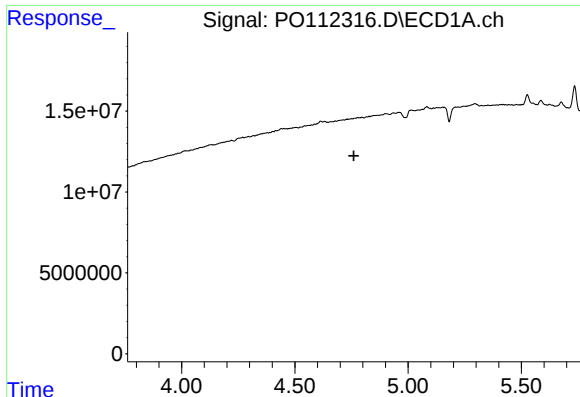

#3 AR-1016-1


R.T.: 4.750 min
Delta R.T.: -0.011 min
Response: -7068
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

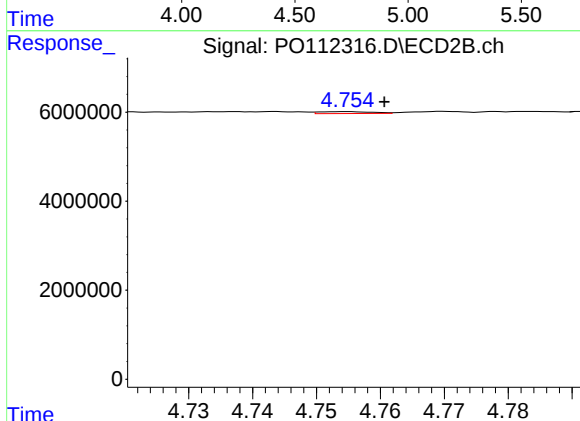


#3 AR-1016-1

R.T.: 4.755 min
Delta R.T.: -0.006 min
Response: 244287
Conc: 1.10 ng/ml

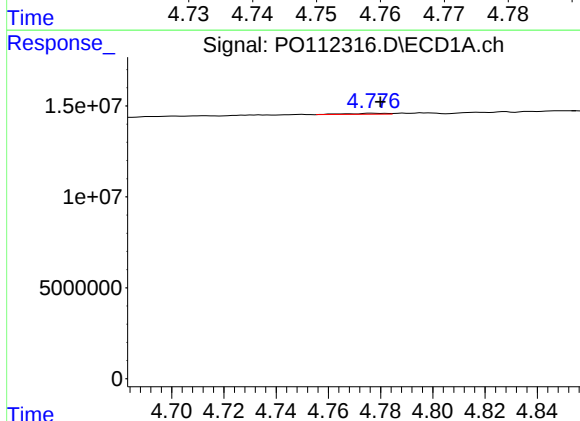


#4 AR-1016-2

R.T.: 4.777 min
Delta R.T.: -0.003 min
Response: 581754
Conc: 1.17 ng/ml

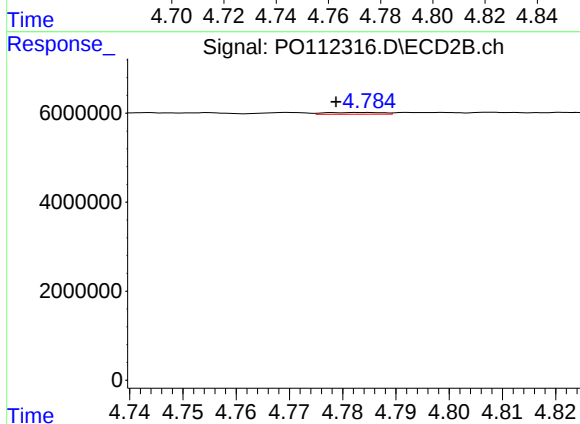

#4 AR-1016-2


R.T.: 4.784 min
Delta R.T.: 0.006 min
Response: 285732
Conc: 0.87 ng/ml

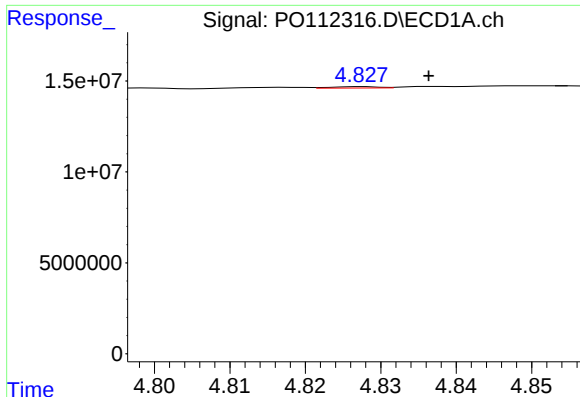

#5 AR-1016-3


R.T.: 4.828 min
Delta R.T.: -0.009 min
Response: 323402
Conc: 1.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

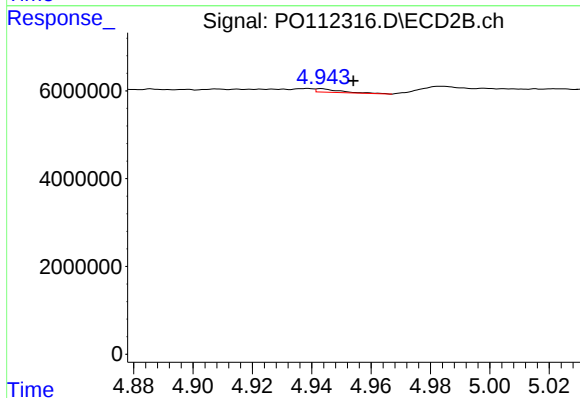


#5 AR-1016-3

R.T.: 4.943 min
Delta R.T.: -0.011 min
Response: 470445
Conc: 2.77 ng/ml

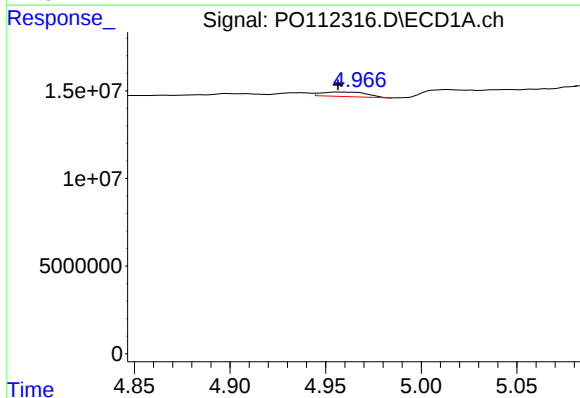


#6 AR-1016-4

R.T.: 4.956 min
Delta R.T.: 0.000 min
Response: 4161994
Conc: 16.21 ng/ml

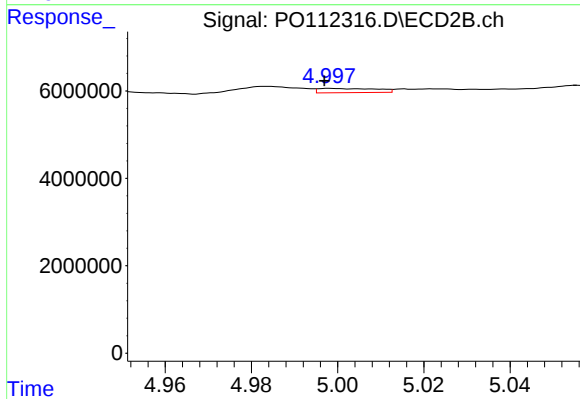

#6 AR-1016-4


R.T.: 4.998 min
Delta R.T.: 0.001 min
Response: 912385
Conc: 6.65 ng/ml

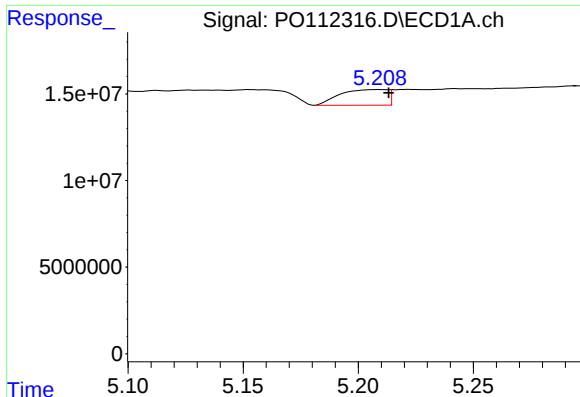

#7 AR-1016-5


R.T.: 5.209 min
Delta R.T.: -0.004 min
Response: 12941995
Conc: 47.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

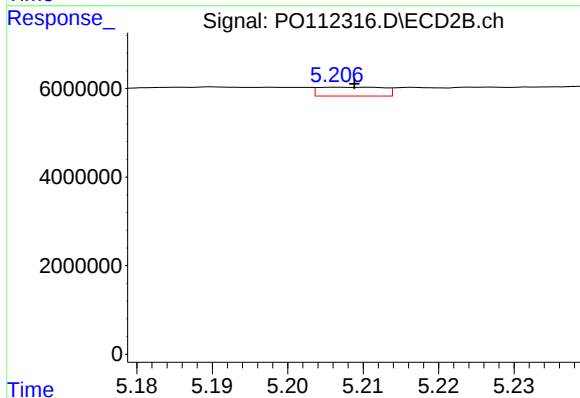


#7 AR-1016-5

R.T.: 5.207 min
Delta R.T.: -0.002 min
Response: 1202141
Conc: 6.97 ng/ml

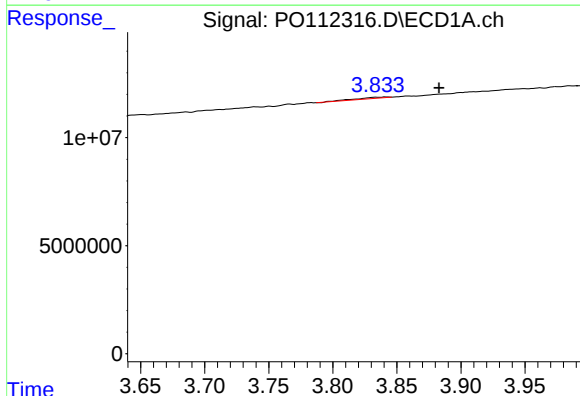


#8 AR-1221-1

R.T.: 3.841 min
Delta R.T.: -0.042 min
Response: 946679
Conc: 8.12 ng/ml

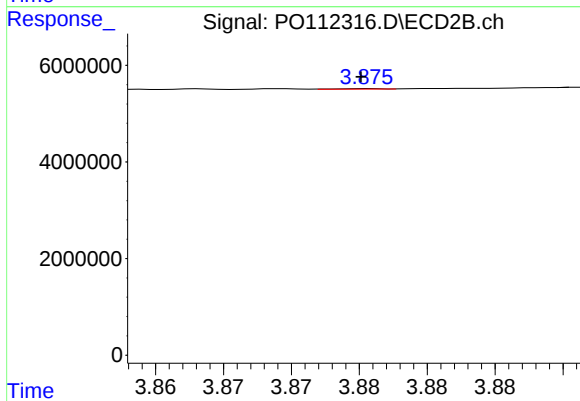

#8 AR-1221-1


R.T.: 3.876 min
Delta R.T.: 0.000 min
Response: 22494
Conc: 0.27 ng/ml

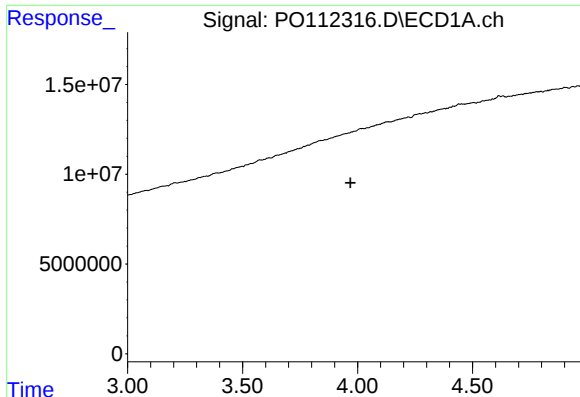

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 3.969 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

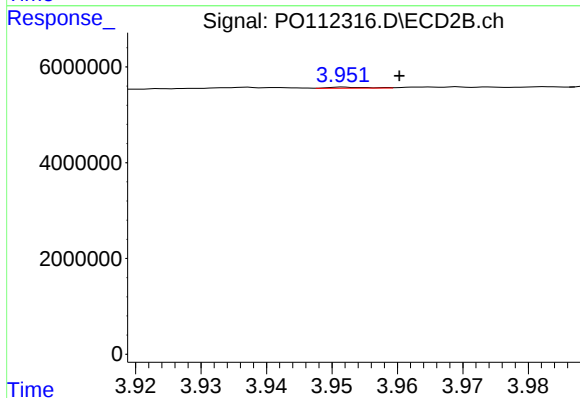


#9 AR-1221-2

R.T.: 3.952 min
Delta R.T.: -0.009 min
Response: 82074
Conc: 1.38 ng/ml

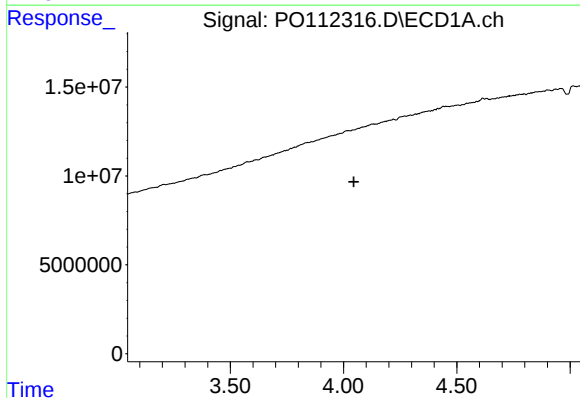


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T.: 4.045 min
Response: 0
Conc: N.D.

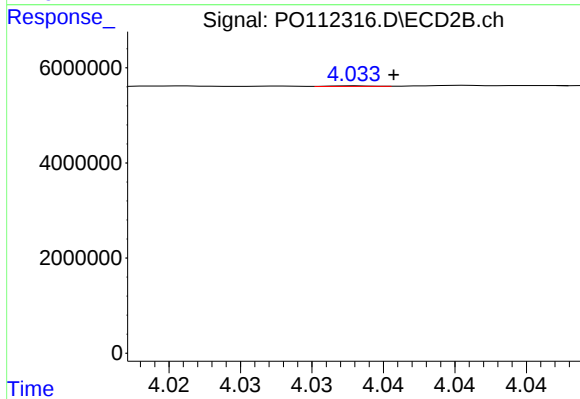

#10 AR-1221-3


R.T.: 4.033 min
Delta R.T.: -0.003 min
Response: 19353
Conc: 0.10 ng/ml

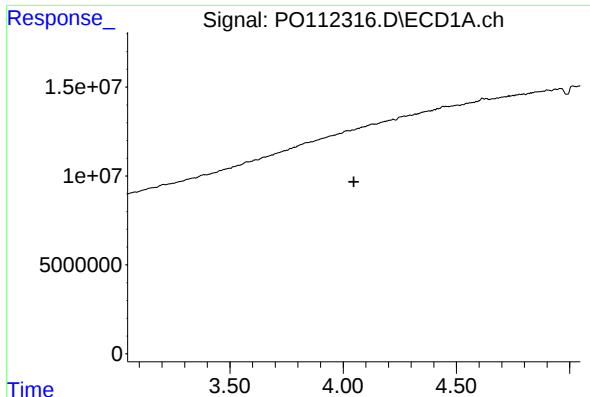

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 4.047 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

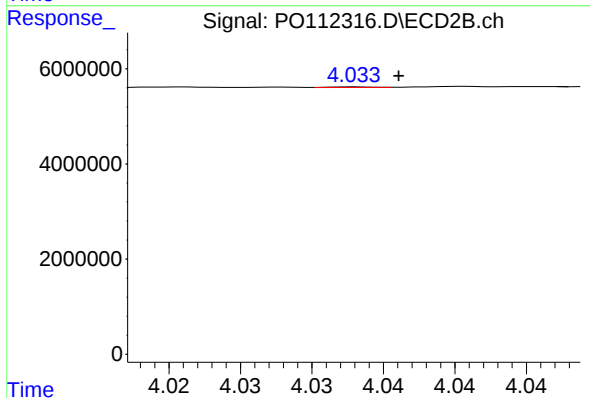


#11 AR-1232-1

R.T.: 4.033 min
Delta R.T.: -0.003 min
Response: 19353
Conc: 0.13 ng/ml

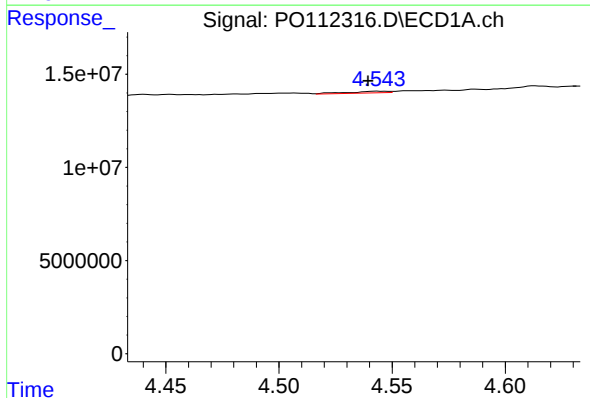


#12 AR-1232-2

R.T.: 4.544 min
Delta R.T.: 0.004 min
Response: 1067790
Conc: 9.40 ng/ml

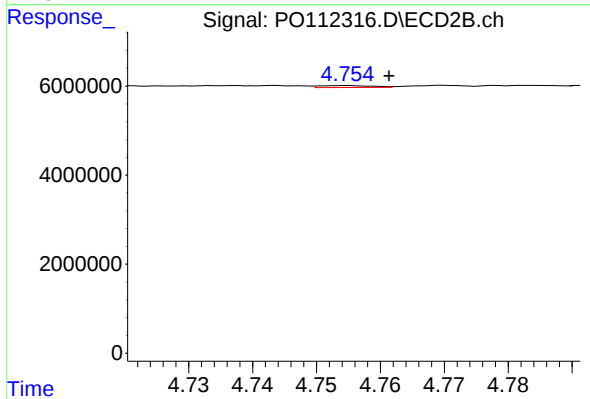

#12 AR-1232-2


R.T.: 4.755 min
Delta R.T.: -0.007 min
Response: 244287
Conc: 1.60 ng/ml

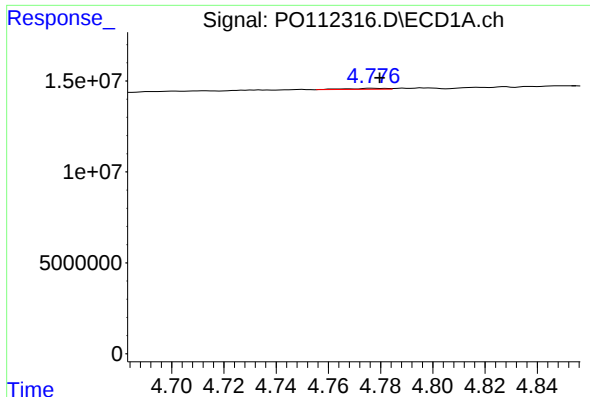

#13 AR-1232-3


R.T.: 4.777 min
Delta R.T.: -0.003 min
Response: 581754
Conc: 2.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

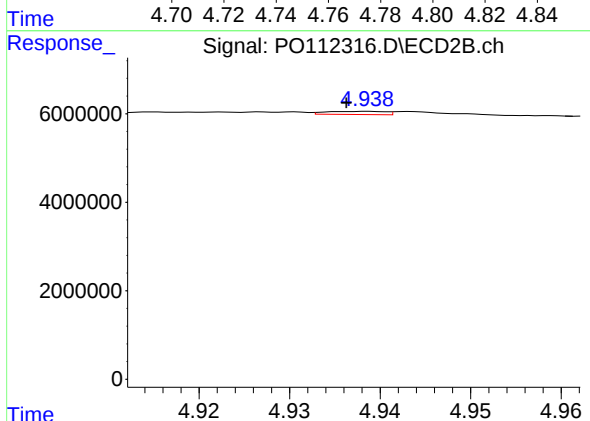


#13 AR-1232-3

R.T.: 4.939 min
Delta R.T.: 0.002 min
Response: 322043
Conc: 4.27 ng/ml

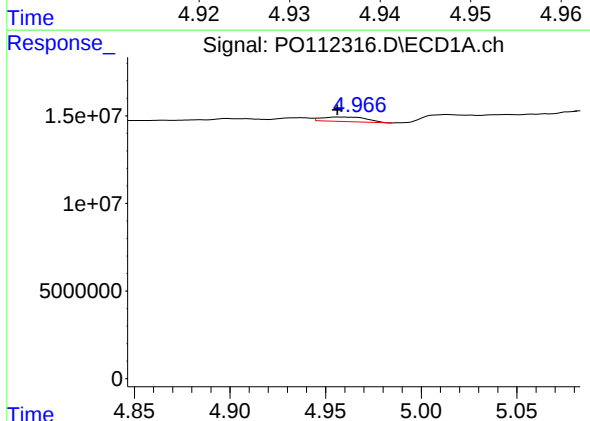


#14 AR-1232-4

R.T.: 4.956 min
Delta R.T.: 0.000 min
Response: 4161994
Conc: 36.41 ng/ml

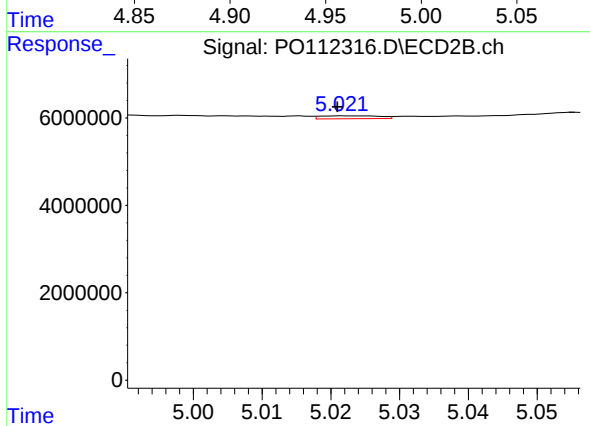

#14 AR-1232-4


R.T.: 5.022 min
Delta R.T.: 0.000 min
Response: 408553
Conc: 6.19 ng/ml

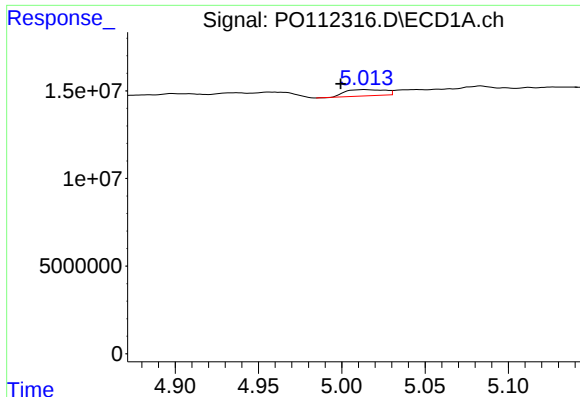

#15 AR-1232-5


R.T.: 5.014 min
Delta R.T.: 0.014 min
Response: 5919621
Conc: 80.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

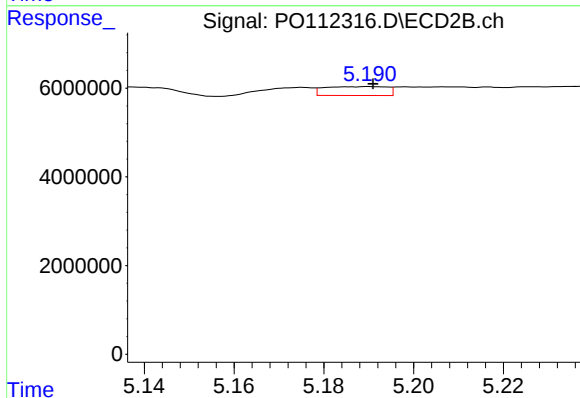


#15 AR-1232-5

R.T.: 5.190 min
Delta R.T.: 0.000 min
Response: 1930146
Conc: 25.99 ng/ml

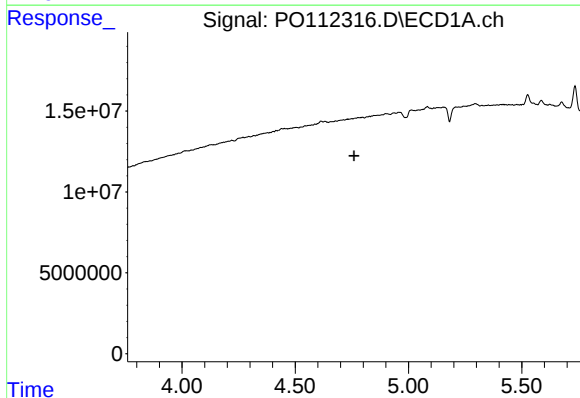


#16 AR-1242-1

R.T.: 4.750 min
Delta R.T.: -0.010 min
Response: -7068
Conc: N.D.

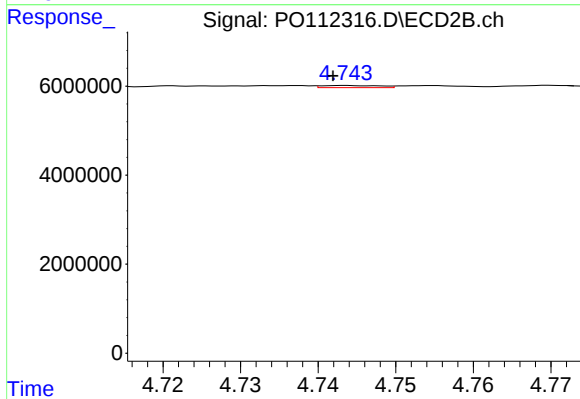

#16 AR-1242-1


R.T.: 4.744 min
Delta R.T.: 0.002 min
Response: 253868
Conc: 1.31 ng/ml

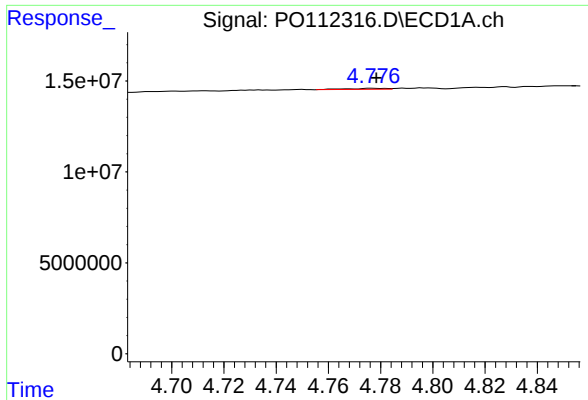

#17 AR-1242-2


R.T.: 4.777 min
Delta R.T.: -0.001 min
Response: 581754
Conc: 1.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

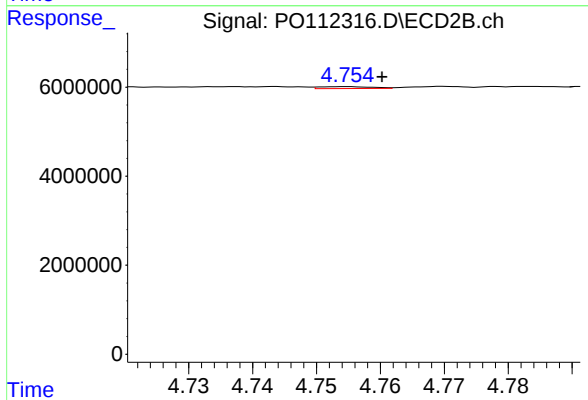


#17 AR-1242-2

R.T.: 4.755 min
Delta R.T.: -0.005 min
Response: 244287
Conc: 0.86 ng/ml

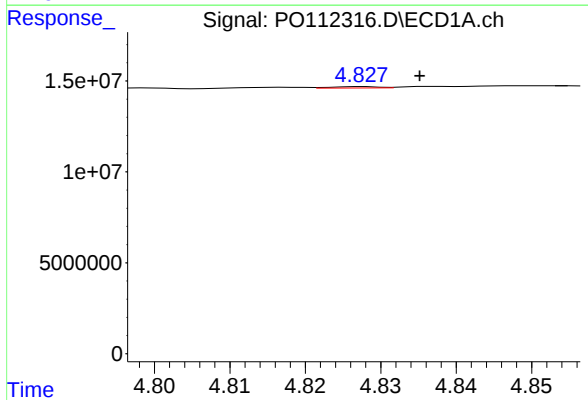


#18 AR-1242-3

R.T.: 4.828 min
Delta R.T.: -0.008 min
Response: 323402
Conc: 1.18 ng/ml

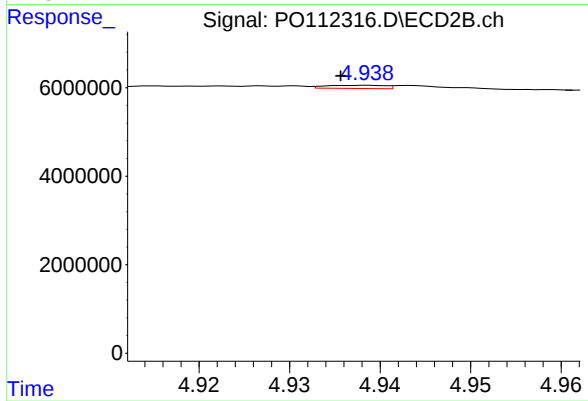

#18 AR-1242-3


R.T.: 4.939 min
Delta R.T.: 0.003 min
Response: 322043
Conc: 2.21 ng/ml

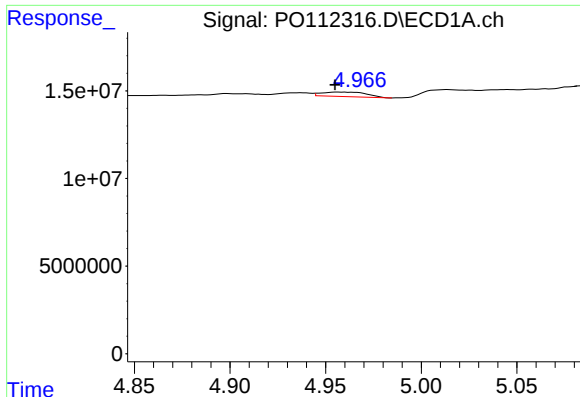

#19 AR-1242-4


R.T.: 4.956 min
Delta R.T.: 0.001 min
Response: 4161994
Conc: 18.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

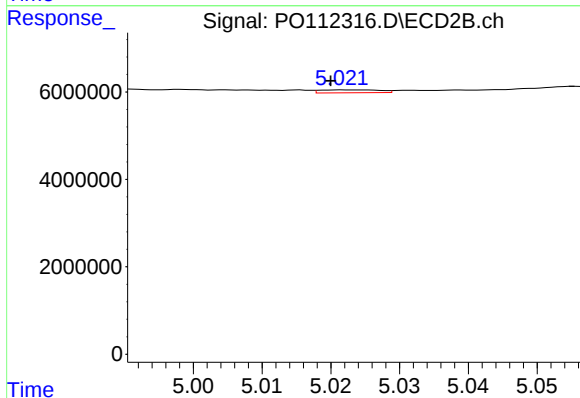


#19 AR-1242-4

R.T.: 5.022 min
Delta R.T.: 0.002 min
Response: 408553
Conc: 2.88 ng/ml

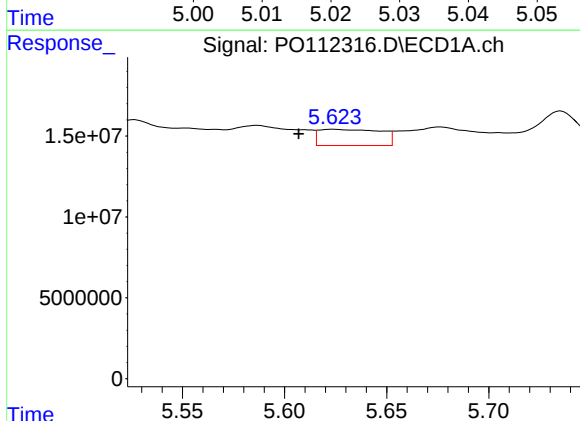


#20 AR-1242-5

R.T.: 5.624 min
Delta R.T.: 0.017 min
Response: 21090696
Conc: 99.64 ng/ml

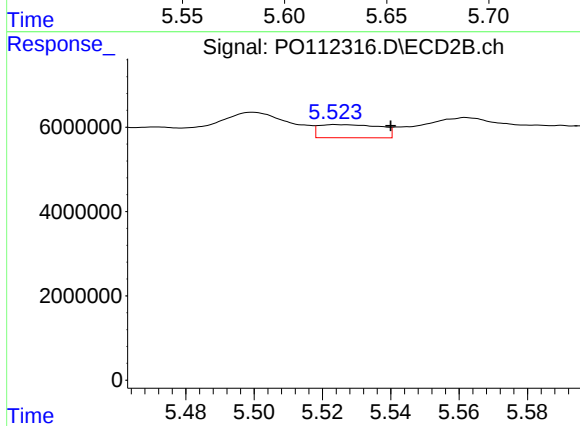

#20 AR-1242-5


R.T.: 5.523 min
Delta R.T.: -0.017 min
Response: 3887154
Conc: 21.39 ng/ml

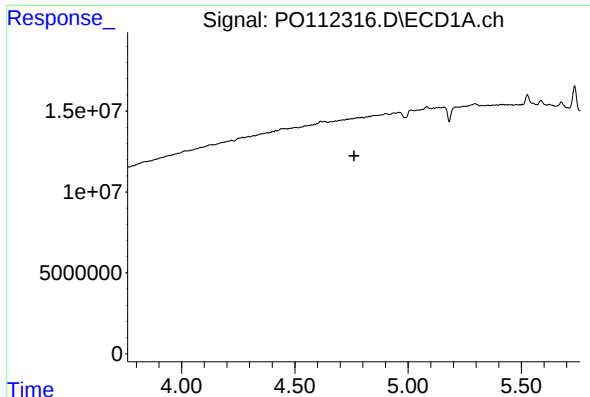

#21 AR-1248-1


R.T.: 4.750 min
Delta R.T.: -0.011 min
Response: -7068
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

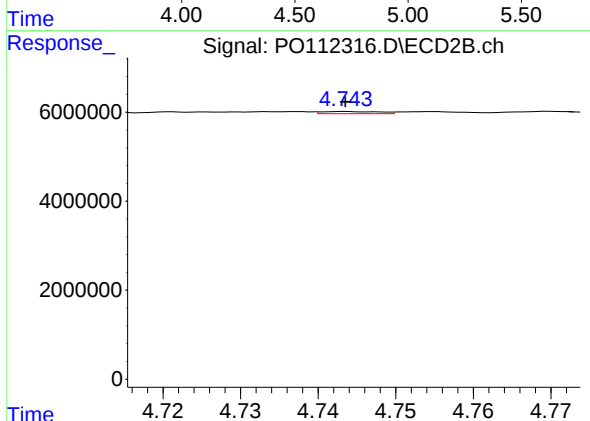


#21 AR-1248-1

R.T.: 4.744 min
Delta R.T.: 0.000 min
Response: 253868
Conc: 1.64 ng/ml

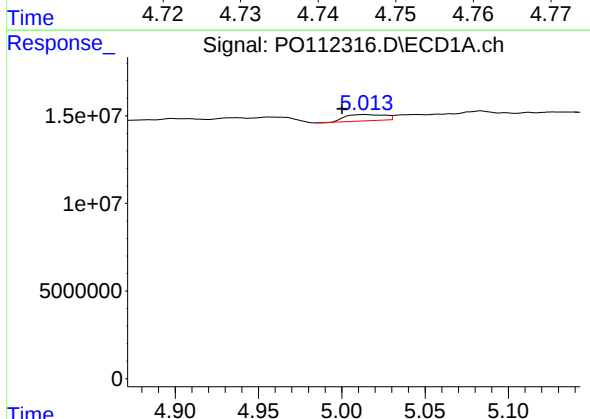


#22 AR-1248-2

R.T.: 5.014 min
Delta R.T.: 0.014 min
Response: 5919621
Conc: 19.20 ng/ml

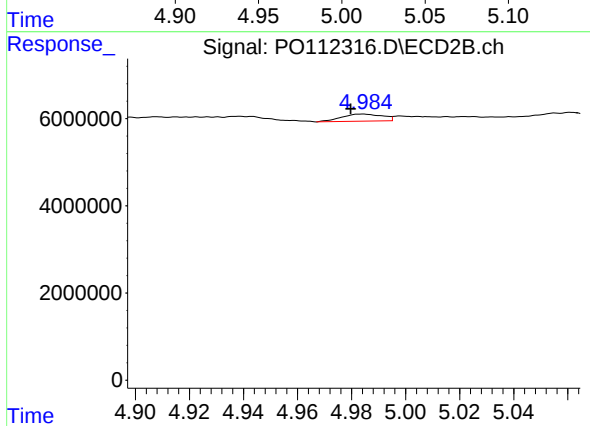

#22 AR-1248-2


R.T.: 4.984 min
Delta R.T.: 0.004 min
Response: 1699119
Conc: 8.26 ng/ml

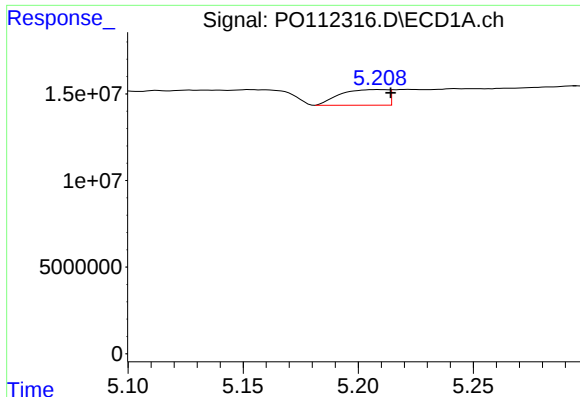

#23 AR-1248-3


R.T.: 5.209 min
Delta R.T.: -0.005 min
Response: 12941995
Conc: 31.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

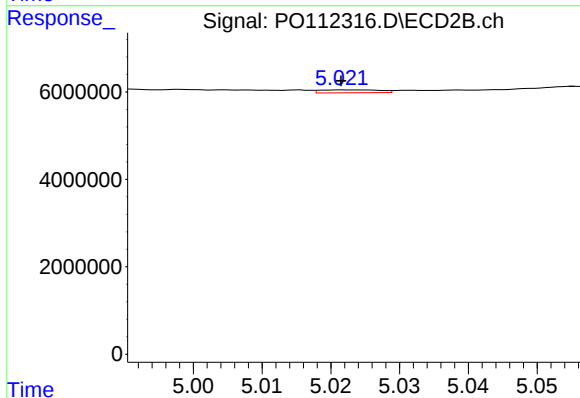


#23 AR-1248-3

R.T.: 5.022 min
Delta R.T.: 0.000 min
Response: 408553
Conc: 1.90 ng/ml

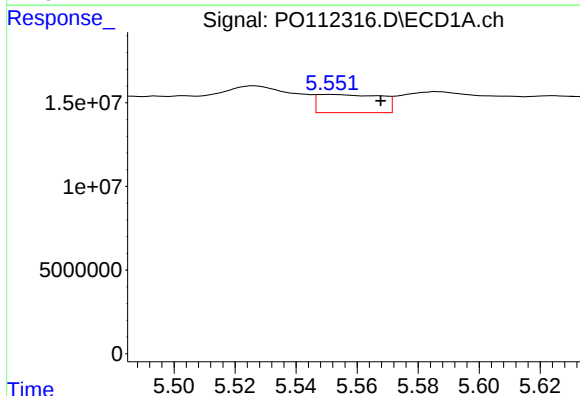


#24 AR-1248-4

R.T.: 5.551 min
Delta R.T.: -0.016 min
Response: 15629727
Conc: 27.08 ng/ml

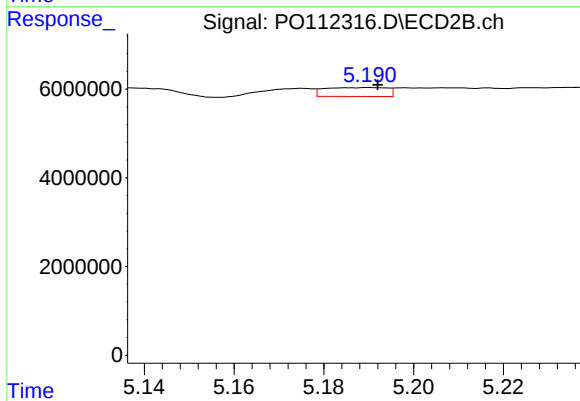

#24 AR-1248-4


R.T.: 5.190 min
Delta R.T.: -0.002 min
Response: 1930146
Conc: 7.46 ng/ml

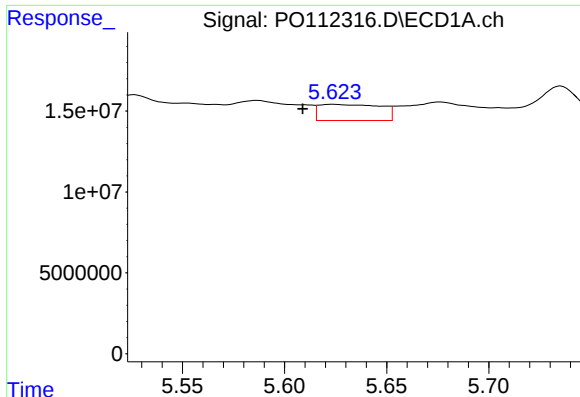

#25 AR-1248-5


R.T.: 5.624 min
Delta R.T.: 0.015 min
Response: 21090696
Conc: 54.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

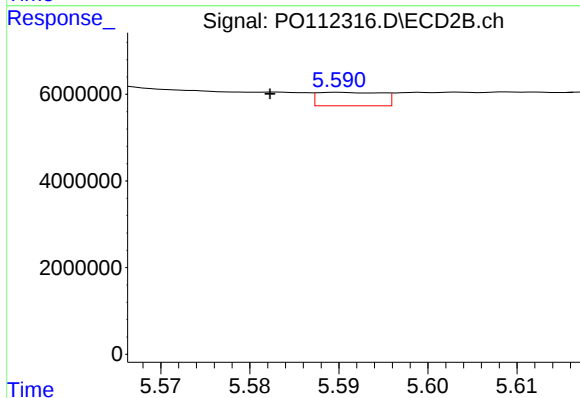


#25 AR-1248-5

R.T.: 5.590 min
Delta R.T.: 0.008 min
Response: 1569651
Conc: 6.26 ng/ml

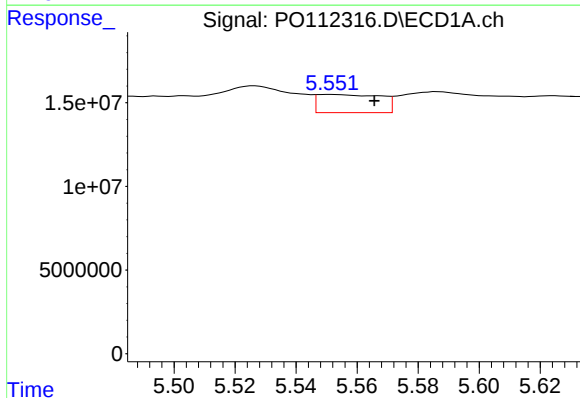


#26 AR-1254-1

R.T.: 5.551 min
Delta R.T.: -0.014 min
Response: 15629727
Conc: 25.41 ng/ml

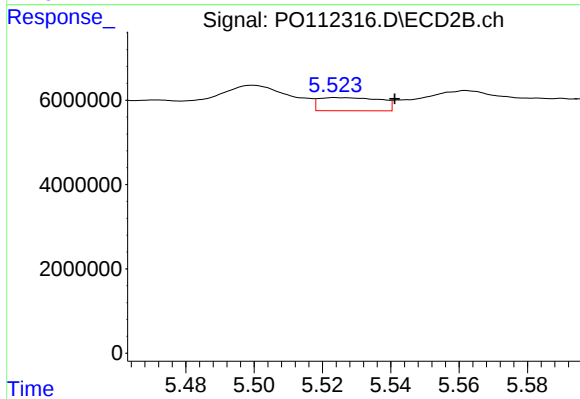

#26 AR-1254-1


R.T.: 5.523 min
Delta R.T.: -0.018 min
Response: 3887154
Conc: 10.20 ng/ml

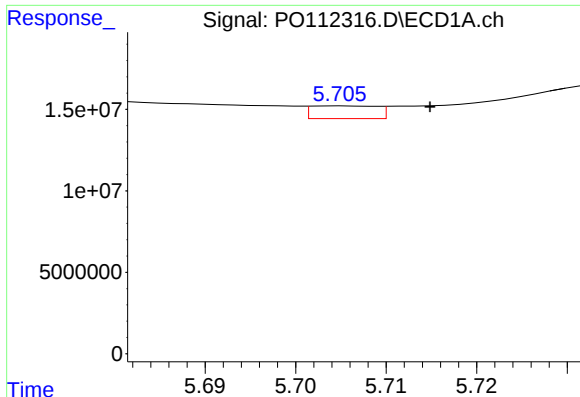

#27 AR-1254-2


R.T.: 5.705 min
Delta R.T.: -0.010 min
Response: 3975465
Conc: 7.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

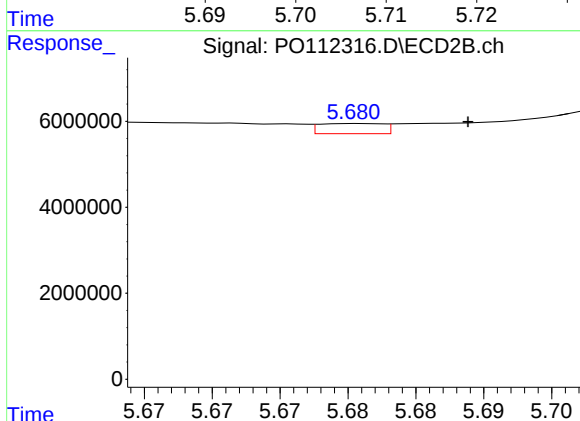


#27 AR-1254-2

R.T.: 5.681 min
Delta R.T.: -0.008 min
Response: 768373
Conc: 2.32 ng/ml

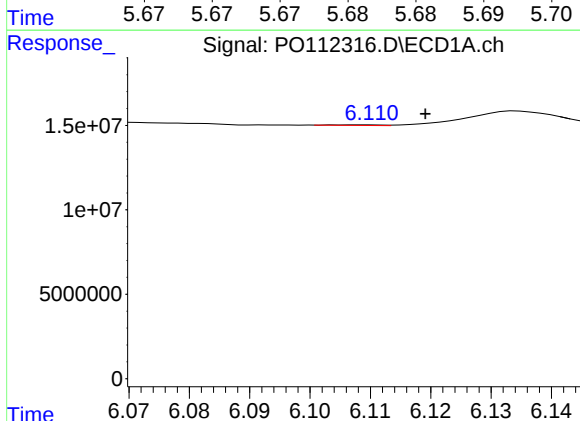


#28 AR-1254-3

R.T.: 6.108 min
Delta R.T.: -0.011 min
Response: 180837
Conc: 0.22 ng/ml

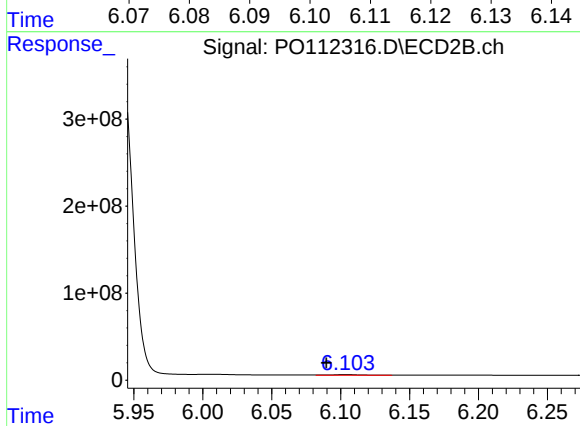

#28 AR-1254-3


R.T.: 6.104 min
Delta R.T.: 0.014 min
Response: 14889002
Conc: 30.89 ng/ml

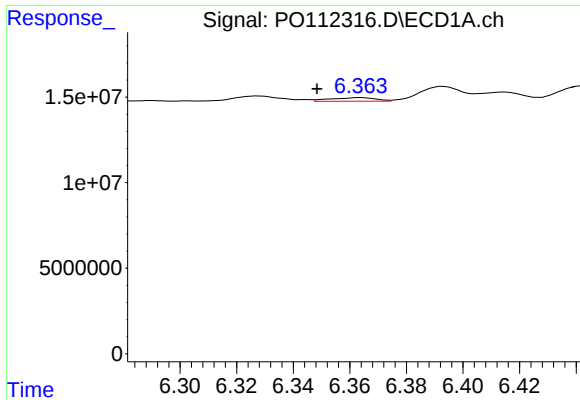

#29 AR-1254-4


R.T.: 6.364 min
Delta R.T.: 0.015 min
Response: 2347048
Conc: 4.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

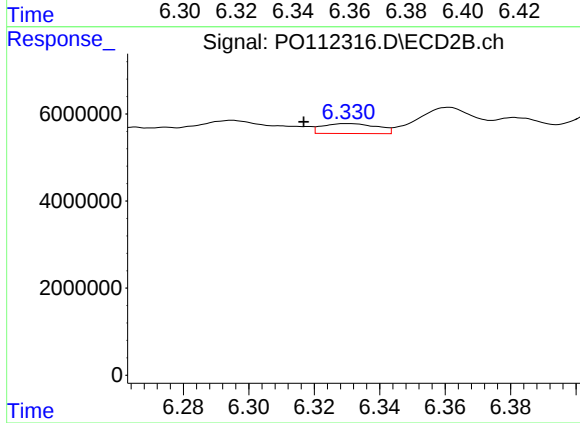


#29 AR-1254-4

R.T.: 6.330 min
Delta R.T.: 0.013 min
Response: 2642650
Conc: 10.14 ng/ml

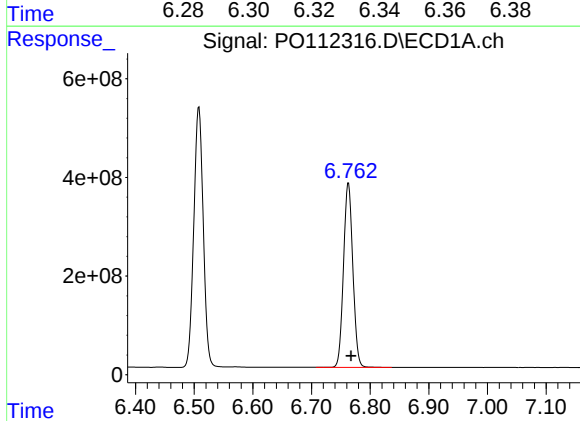


#30 AR-1254-5

R.T.: 6.763 min
Delta R.T.: -0.004 min
Response: 4140776794
Conc: 5350.20 ng/ml

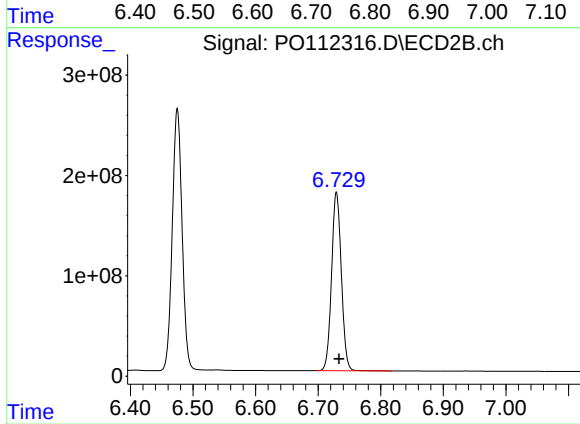

#30 AR-1254-5


R.T.: 6.729 min
Delta R.T.: -0.004 min
Response: 1927577698
Conc: 5409.13 ng/ml

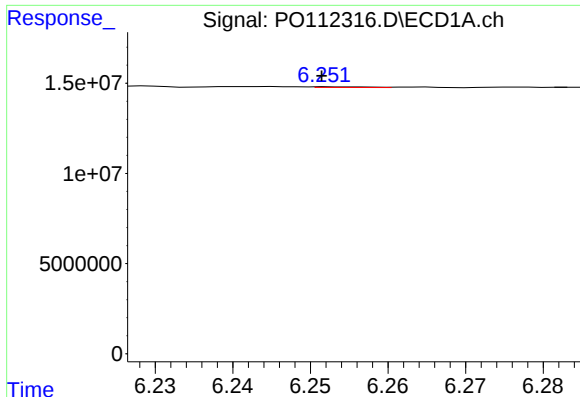

#31 AR-1260-1


R.T.: 6.252 min
Delta R.T.: 0.000 min
Response: 174693
Conc: 0.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

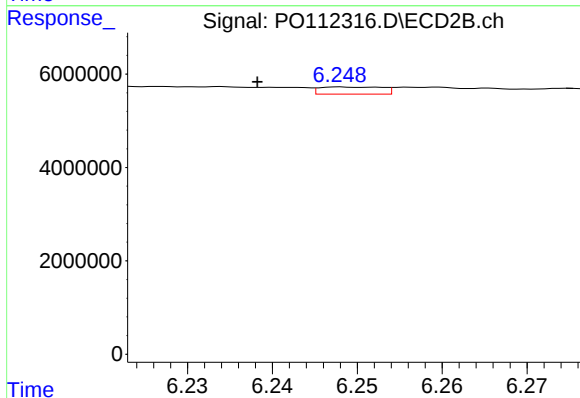


#31 AR-1260-1

R.T.: 6.248 min
Delta R.T.: 0.010 min
Response: 784994
Conc: 2.80 ng/ml

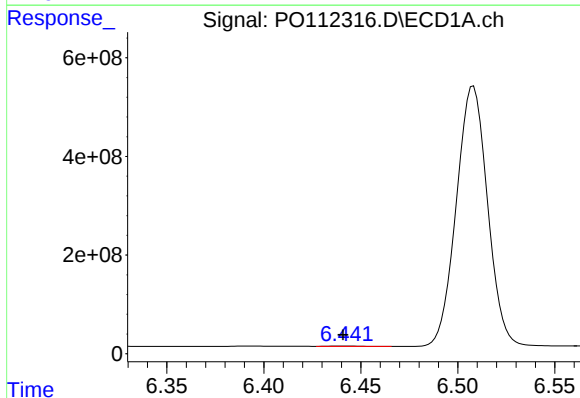


#32 AR-1260-2

R.T.: 6.442 min
Delta R.T.: 0.001 min
Response: 9589298
Conc: 12.99 ng/ml

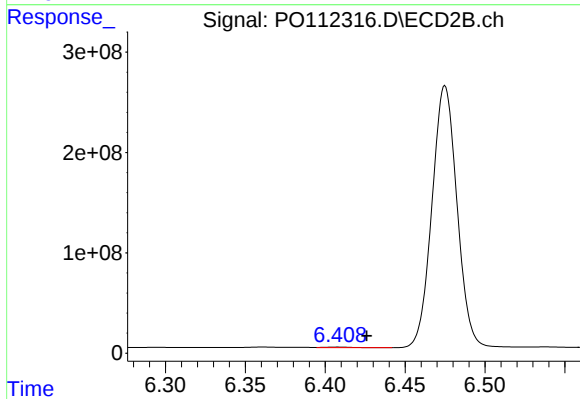

#32 AR-1260-2


R.T.: 6.408 min
Delta R.T.: -0.018 min
Response: 6718671
Conc: 19.76 ng/ml

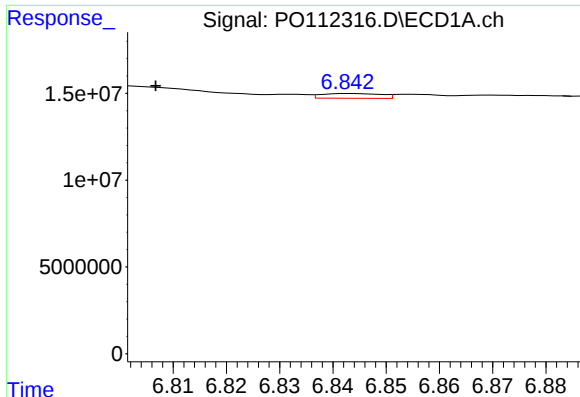

#33 AR-1260-3


R.T.: 6.843 min
Delta R.T.: 0.037 min
Response: 2118045
Conc: 3.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

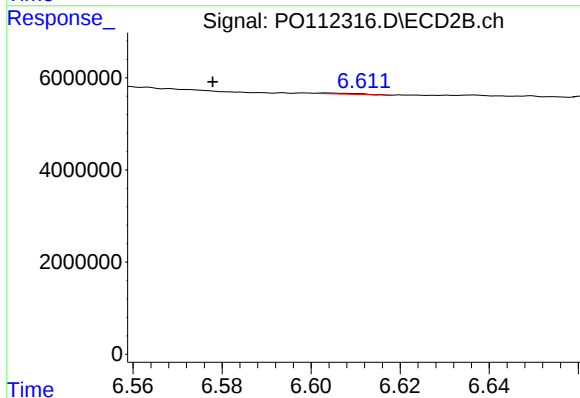


#33 AR-1260-3

R.T.: 6.604 min
Delta R.T.: 0.026 min
Response: 133503
Conc: 0.48 ng/ml

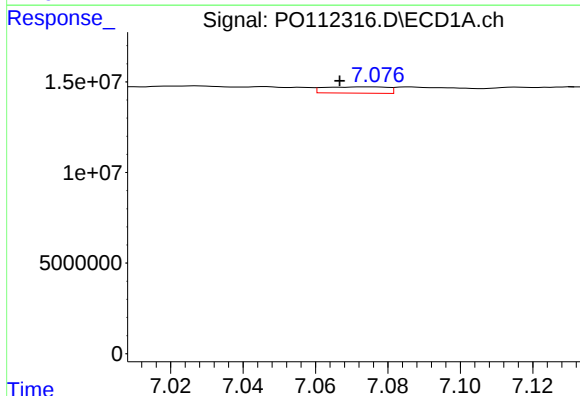


#34 AR-1260-4

R.T.: 7.076 min
Delta R.T.: 0.009 min
Response: 4175677
Conc: 9.59 ng/ml

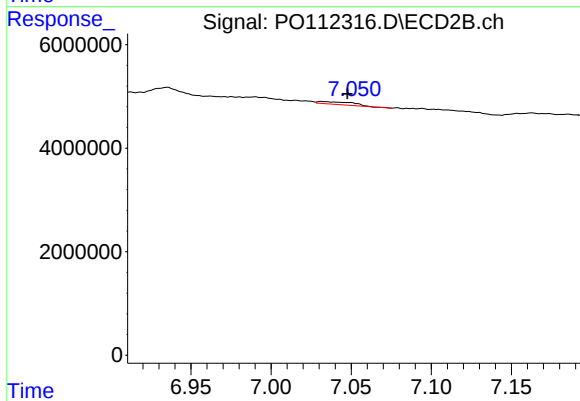

#34 AR-1260-4


R.T.: 7.031 min
Delta R.T.: -0.016 min
Response: 764747
Conc: 3.81 ng/ml

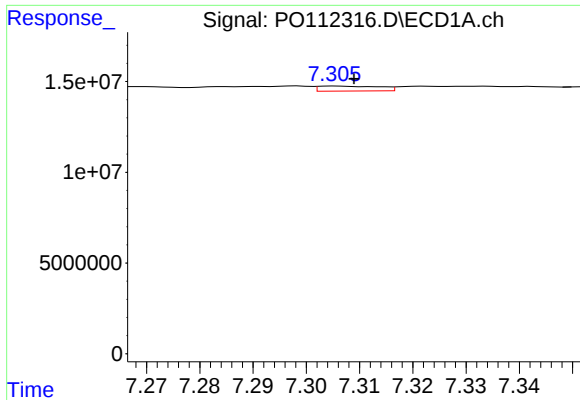

#35 AR-1260-5


R.T.: 7.306 min
Delta R.T.: -0.003 min
Response: 2195533
Conc: 1.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

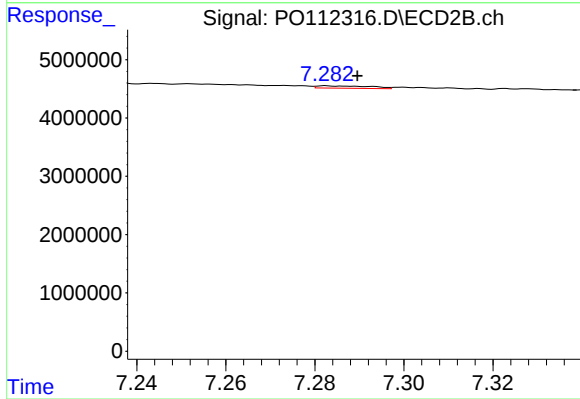


#35 AR-1260-5

R.T.: 7.283 min
Delta R.T.: -0.007 min
Response: 349256
Conc: 0.78 ng/ml

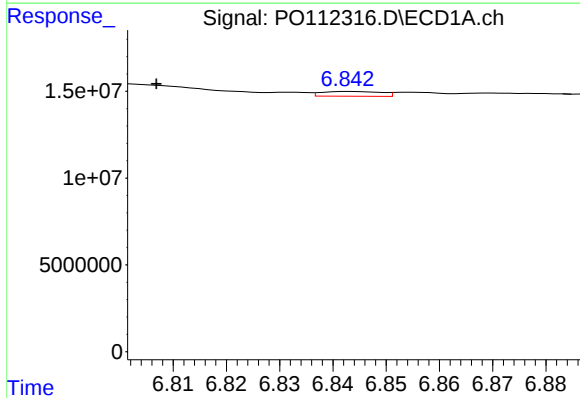


#36 AR-1262-1

R.T.: 6.843 min
Delta R.T.: 0.036 min
Response: 2118045
Conc: 2.07 ng/ml

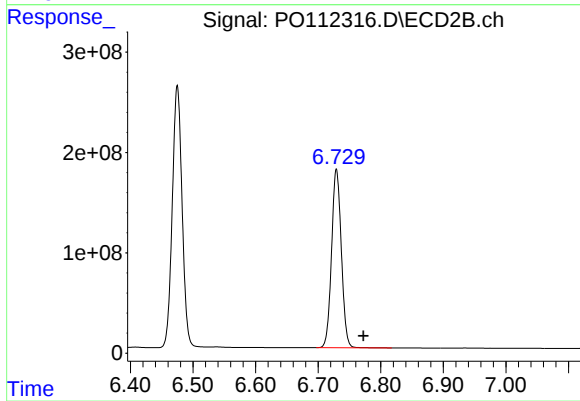

#36 AR-1262-1


R.T.: 6.729 min
Delta R.T.: -0.043 min
Response: 1927577698
Conc: 4732.33 ng/ml

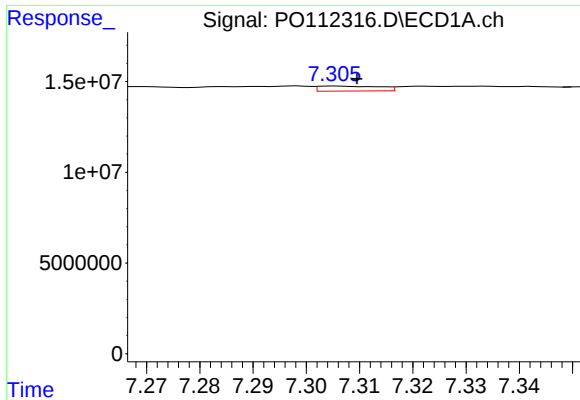

#37 AR-1262-2


R.T.: 7.306 min
Delta R.T.: -0.004 min
Response: 2195533
Conc: 1.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

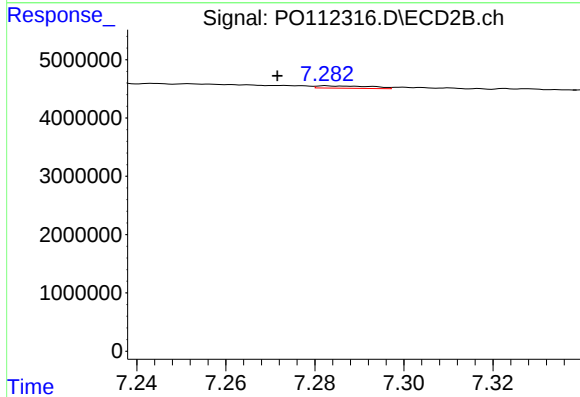


#37 AR-1262-2

R.T.: 7.283 min
Delta R.T.: 0.011 min
Response: 349256
Conc: 0.68 ng/ml

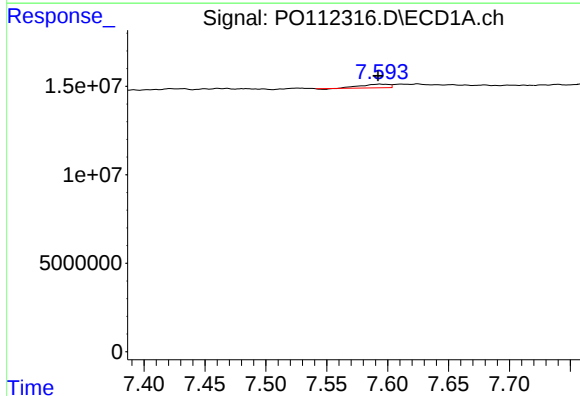


#38 AR-1262-3

R.T.: 7.594 min
Delta R.T.: 0.002 min
Response: 3117617
Conc: 4.86 ng/ml

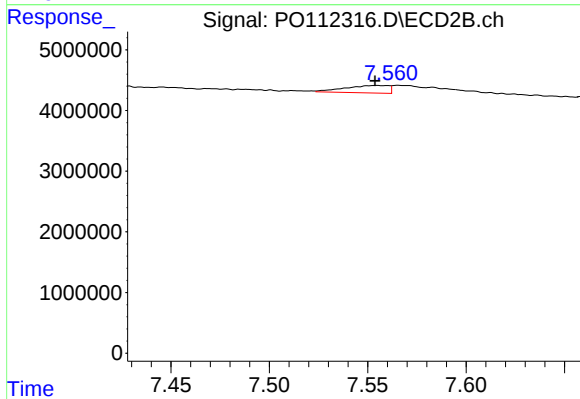

#38 AR-1262-3


R.T.: 7.555 min
Delta R.T.: 0.001 min
Response: 1927120
Conc: 10.73 ng/ml

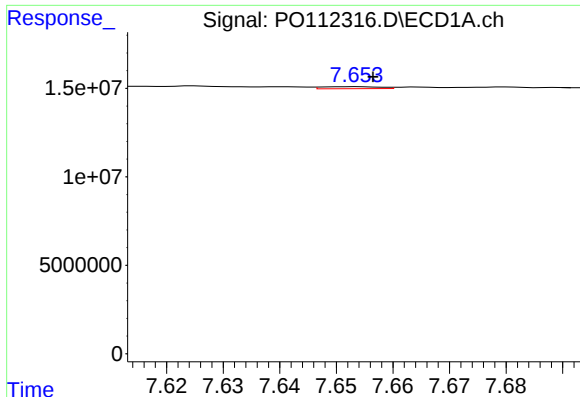

#39 AR-1262-4


R.T.: 7.654 min
Delta R.T.: -0.003 min
Response: 824680
Conc: 0.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

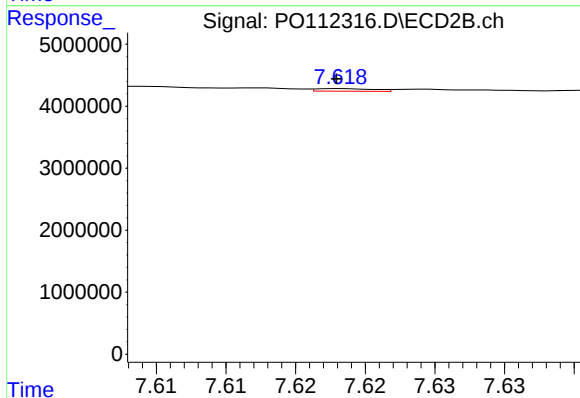


#39 AR-1262-4

R.T.: 7.618 min
Delta R.T.: 0.000 min
Response: 121153
Conc: 0.42 ng/ml

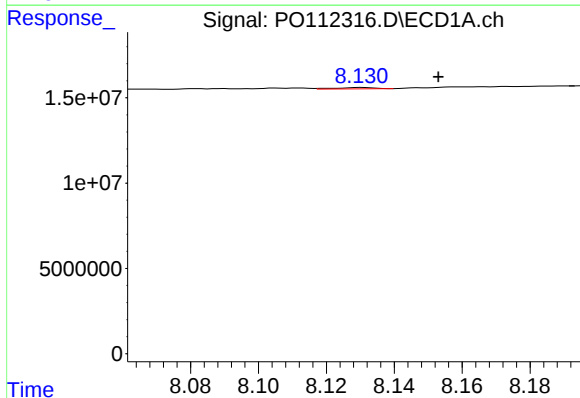


#40 AR-1262-5

R.T.: 8.130 min
Delta R.T.: -0.023 min
Response: 650192
Conc: 1.45 ng/ml

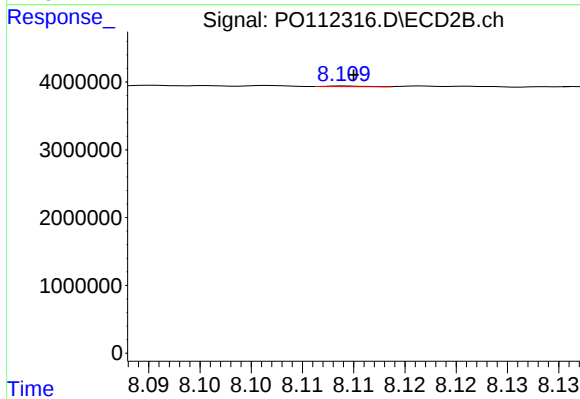

#40 AR-1262-5


R.T.: 8.109 min
Delta R.T.: 0.000 min
Response: 23715
Conc: 0.22 ng/ml

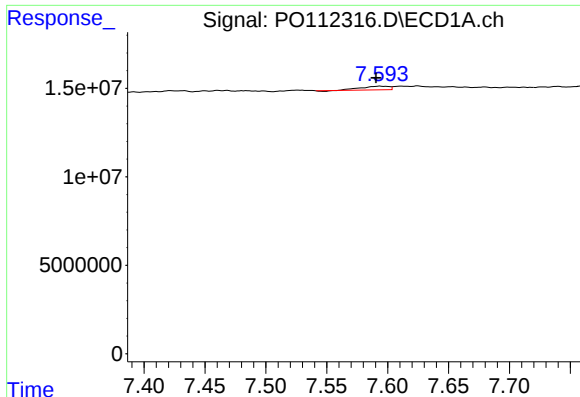

#41 AR-1268-1


R.T.: 7.594 min
Delta R.T.: 0.003 min
Response: 3117617
Conc: 1.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

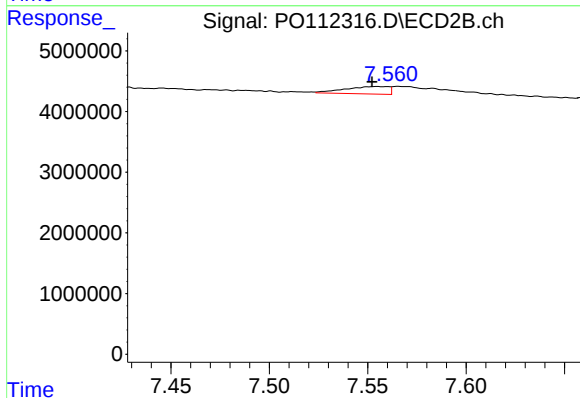


#41 AR-1268-1

R.T.: 7.555 min
Delta R.T.: 0.003 min
Response: 1927120
Conc: 3.92 ng/ml

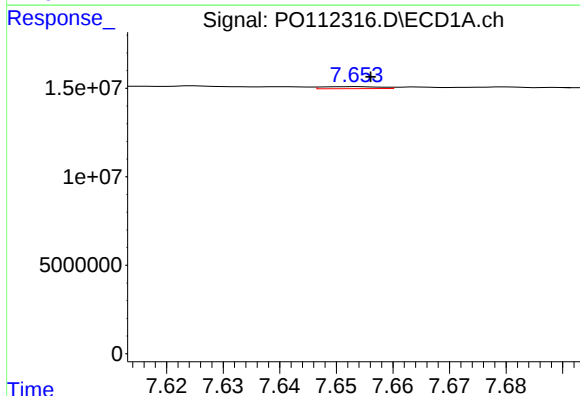


#42 AR-1268-2

R.T.: 7.654 min
Delta R.T.: -0.002 min
Response: 824680
Conc: 0.53 ng/ml

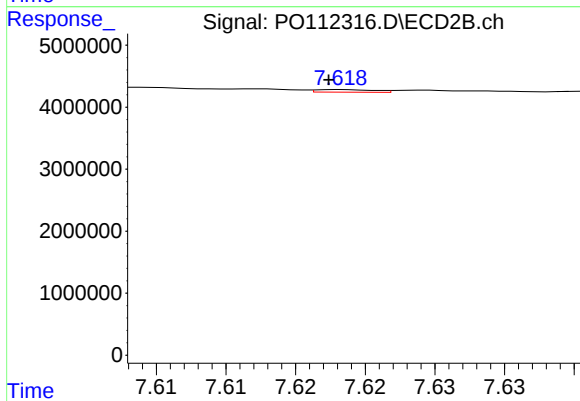

#42 AR-1268-2


R.T.: 7.618 min
Delta R.T.: 0.001 min
Response: 121153
Conc: 0.29 ng/ml

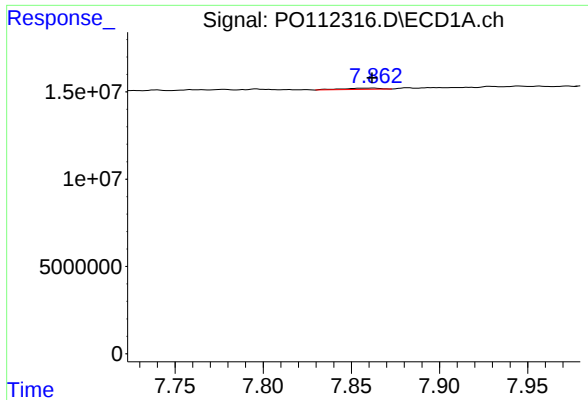

#43 AR-1268-3


R.T.: 7.863 min
Delta R.T.: 0.001 min
Response: 1101167
Conc: 0.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

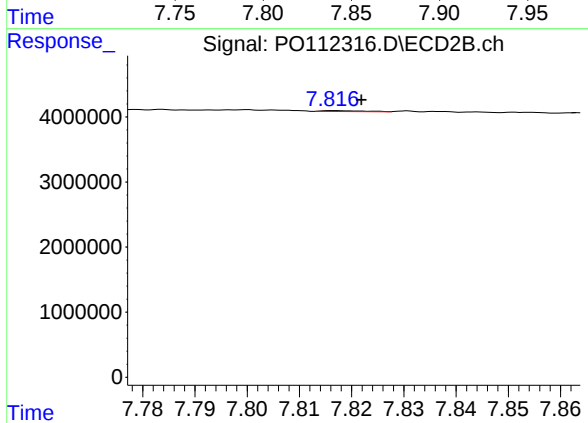


#43 AR-1268-3

R.T.: 7.816 min
Delta R.T.: -0.005 min
Response: 78204
Conc: 0.25 ng/ml

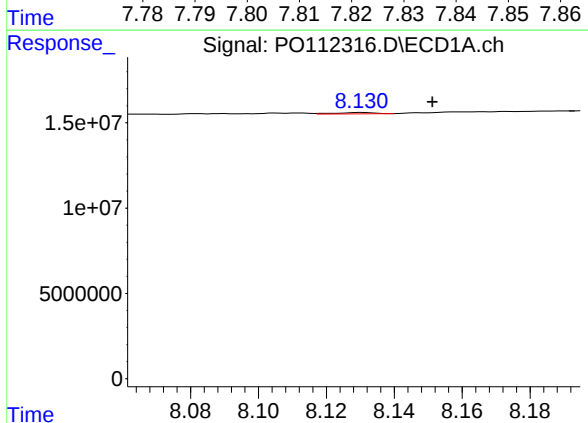


#44 AR-1268-4

R.T.: 8.130 min
Delta R.T.: -0.021 min
Response: 650192
Conc: 1.35 ng/ml

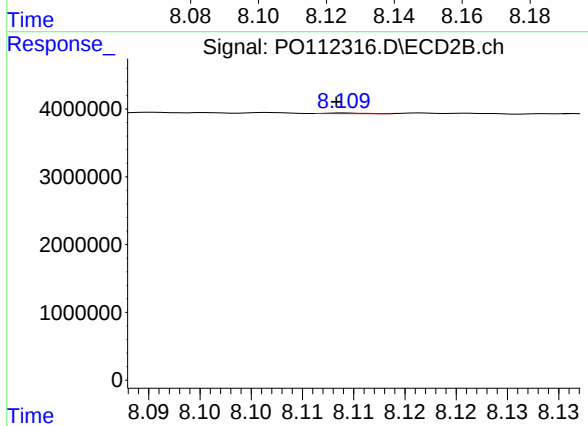

#44 AR-1268-4


R.T.: 8.109 min
Delta R.T.: 0.000 min
Response: 23715
Conc: 0.21 ng/ml

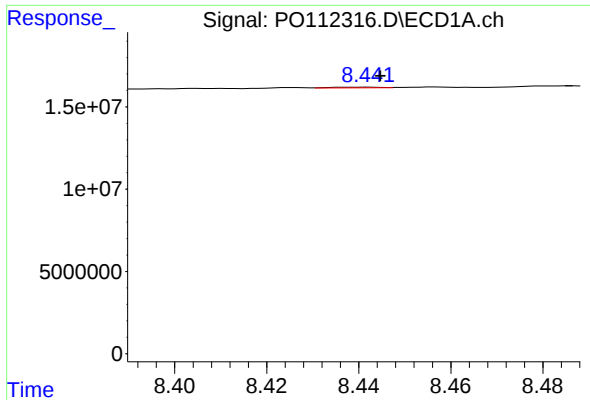

#45 AR-1268-5

R.T.: 8.442 min
Delta R.T.: -0.003 min
Response: 309245
Conc: 0.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

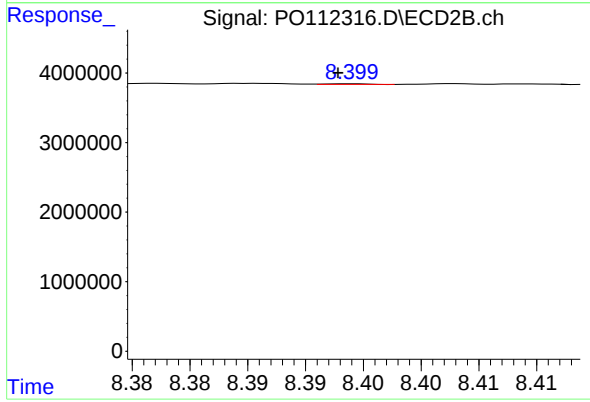

#45 AR-1268-5

R.T.: 8.399 min
Delta R.T.: 0.001 min
Response: 21558
Conc: 0.03 ng/ml