

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071819\
 Data File : P0058031.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Jul 2019 12:20
 Operator : SM/AJ
 Sample : K3845-01RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 K580-B7RE

Manual Integrations
 APPROVED

Ankita
 7/18/2019 2:37:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 13:20:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.205	3.540	877986	807072	25.909	25.163
2)	SA Decachlor...	9.725	8.446	1361882	862677	26.620	25.169
Target Compounds							
31)	L7 AR-1260-1	6.943	6.061	44917	34741	17.959m	17.154
32)	L7 AR-1260-2	7.198	6.248	68288	50992	19.423	19.829
33)	L7 AR-1260-3	7.552	6.399	40549	34216	13.810	15.002
34)	L7 AR-1260-4	7.773	6.864	33596	23620	12.298	12.199m
35)	L7 AR-1260-5	8.084	7.106	69983	54256	12.063	11.788

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071819\
Data File : PO058031.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Jul 2019 12:20
Operator : SM/AJ
Sample : K3845-01RE
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
K580-B7RE


Manual Integrations
APPROVED

Ankita
7/18/2019 2:37:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 13:20:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

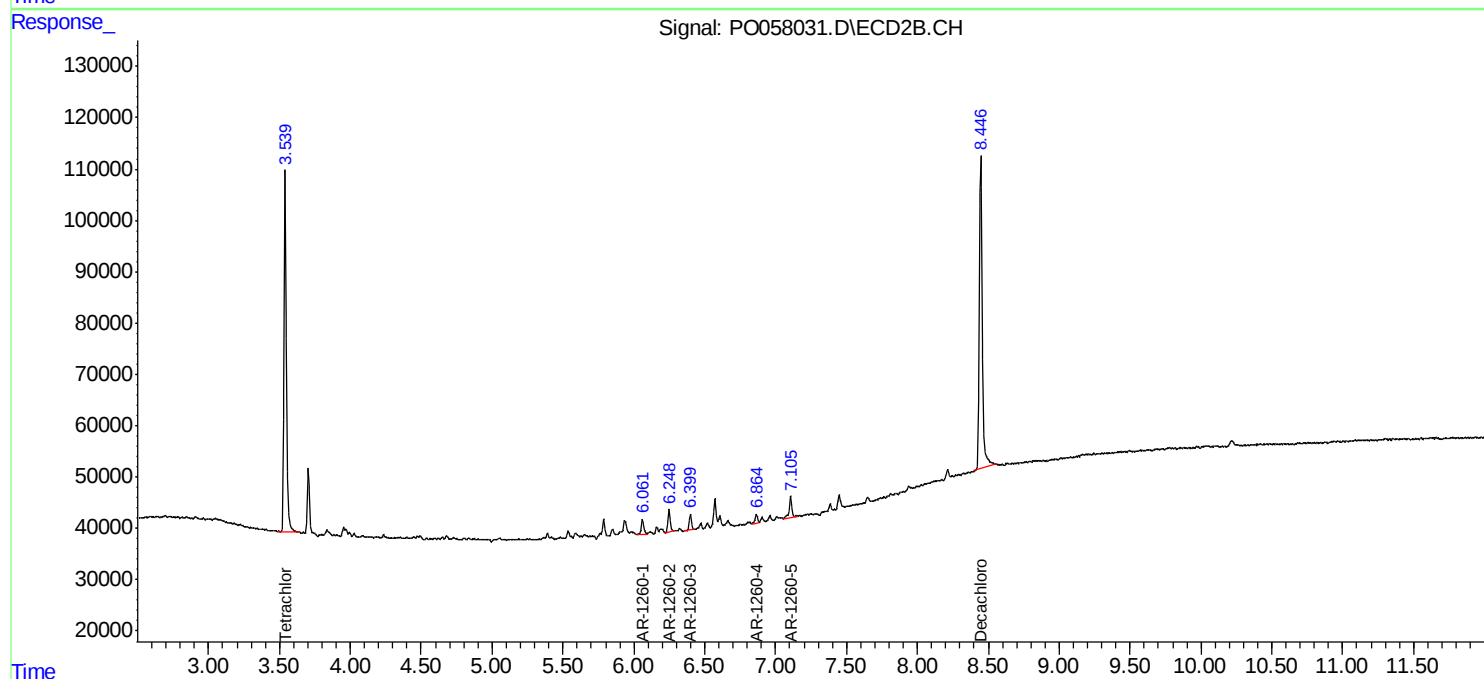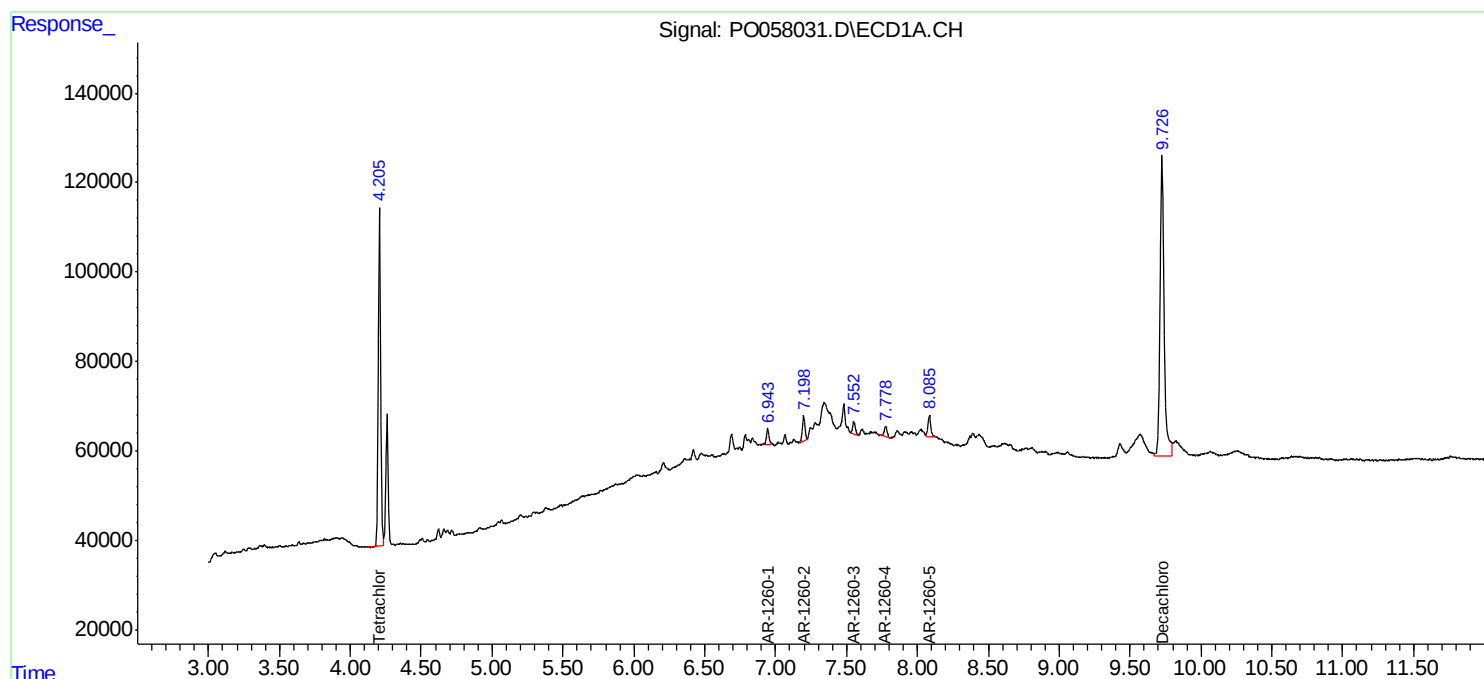

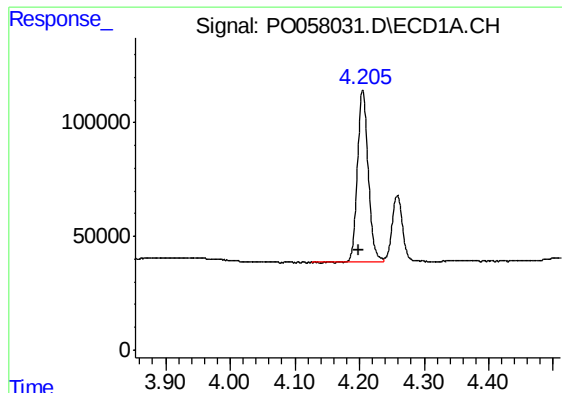


#1 Tetrachloro-m-xylene

R.T.: 4.205 min
Delta R.T.: 0.005 min
Response: 877986
Conc: 25.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
K580-B7RE


Manual Integrations
APPROVED

Ankita
7/18/2019 2:37:40 PM

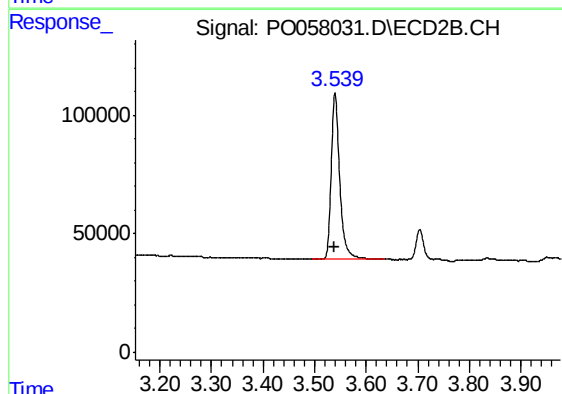


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: 0.000 min
Response: 807072
Conc: 25.16 ng/ml

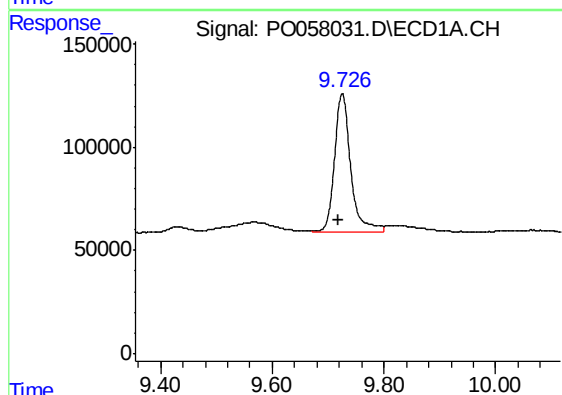


#2 Decachlorobiphenyl

R.T.: 9.725 min
Delta R.T.: 0.007 min
Response: 1361882
Conc: 26.62 ng/ml

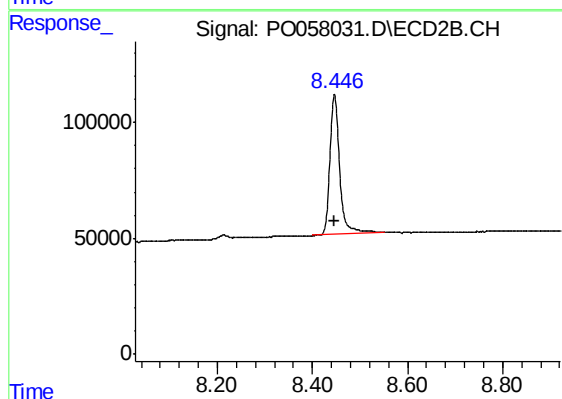

#2 Decachlorobiphenyl

R.T.: 8.446 min
Delta R.T.: 0.001 min
Response: 862677
Conc: 25.17 ng/ml

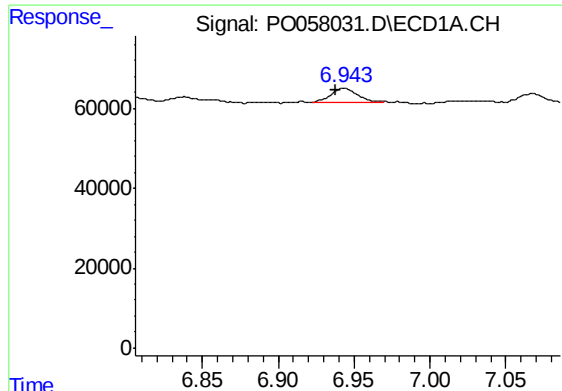


#31 AR-1260-1

R.T.: 6.943 min
Delta R.T.: 0.005 min
Response: 44917
Conc: 17.96 ng/ml m

Instrument :
ECD_O
ClientSampleId :
K580-B7RE


Manual Integrations
APPROVED

Ankita
7/18/2019 2:37:40 PM

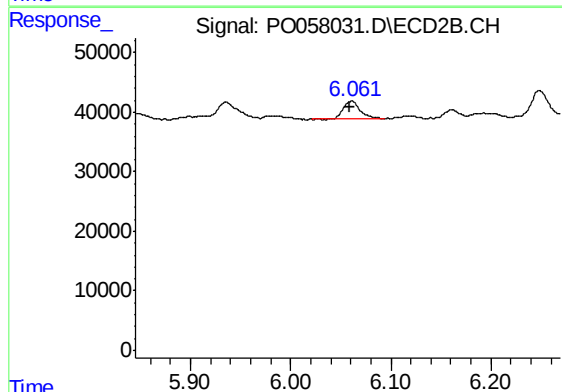


#31 AR-1260-1

R.T.: 6.061 min
Delta R.T.: 0.001 min
Response: 34741
Conc: 17.15 ng/ml

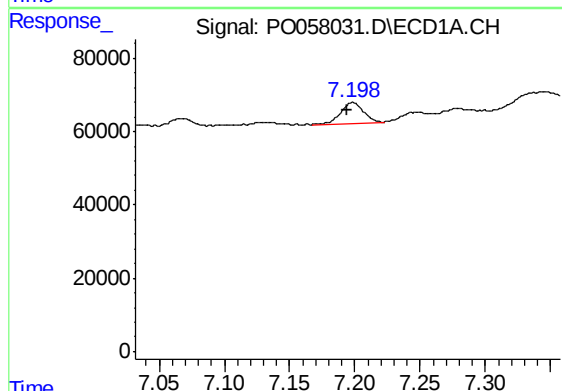


#32 AR-1260-2

R.T.: 7.198 min
Delta R.T.: 0.004 min
Response: 68288
Conc: 19.42 ng/ml

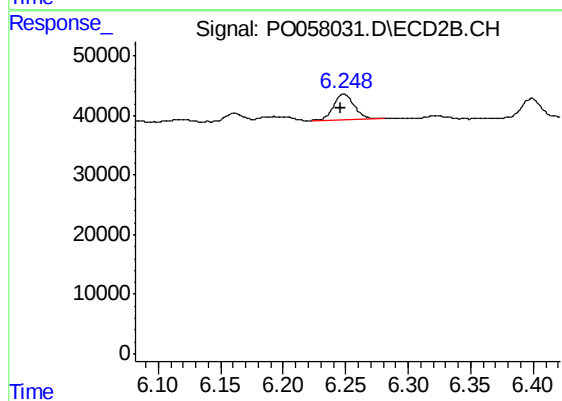

#32 AR-1260-2

R.T.: 6.248 min
Delta R.T.: 0.002 min
Response: 50992
Conc: 19.83 ng/ml

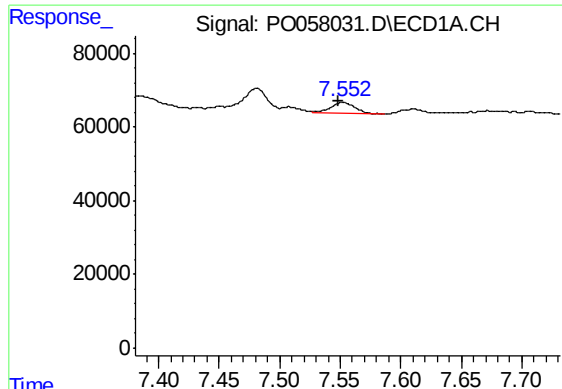


#33 AR-1260-3

R.T.: 7.552 min
Delta R.T.: 0.004 min
Response: 40549
Conc: 13.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
K580-B7RE


Manual Integrations
APPROVED

Ankita
7/18/2019 2:37:40 PM

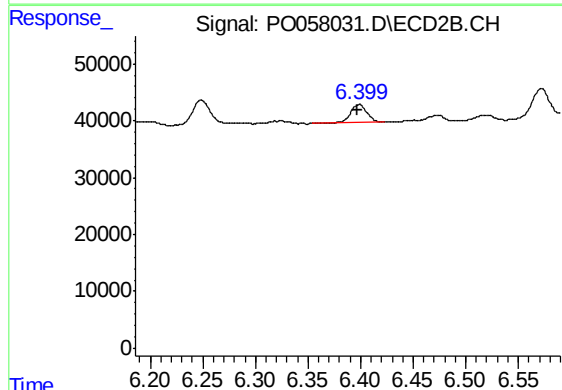


#33 AR-1260-3

R.T.: 6.399 min
Delta R.T.: 0.002 min
Response: 34216
Conc: 15.00 ng/ml

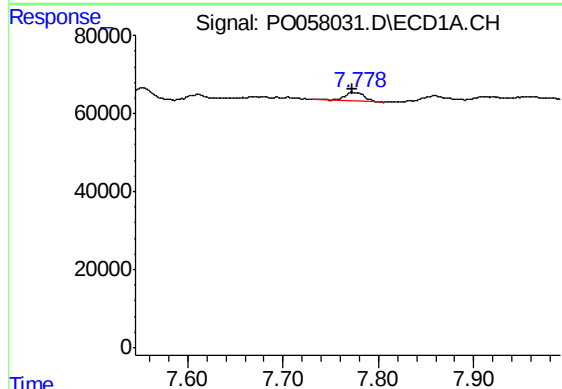


#34 AR-1260-4

R.T.: 7.773 min
Delta R.T.: 0.000 min
Response: 33596
Conc: 12.30 ng/ml

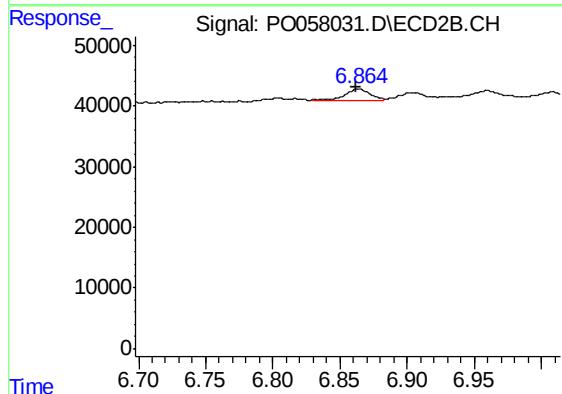

#34 AR-1260-4

R.T.: 6.864 min
Delta R.T.: 0.002 min
Response: 23620
Conc: 12.20 ng/ml m

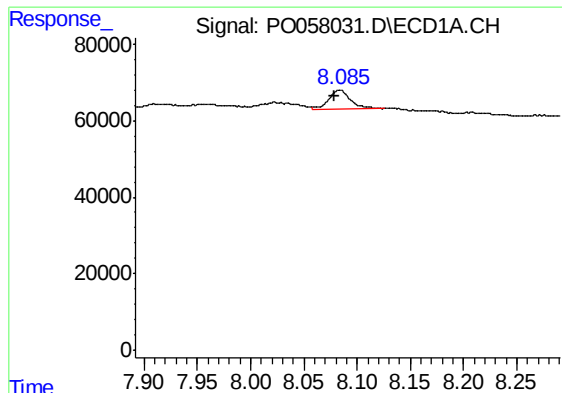


#35 AR-1260-5

R.T.: 8.084 min
Delta R.T.: 0.005 min
Response: 69983
Conc: 12.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
K580-B7RE

Manual Integrations
APPROVED

Ankita
7/18/2019 2:37:40 PM

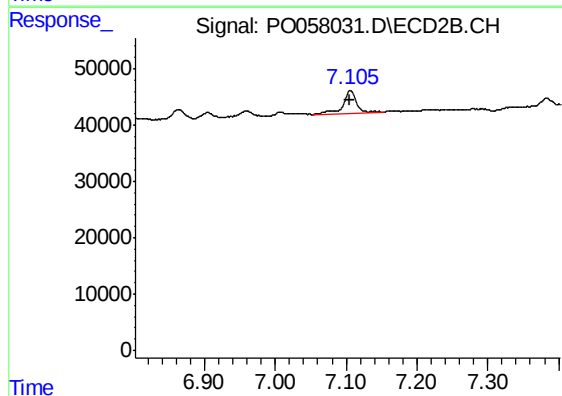

#35 AR-1260-5

R.T.: 7.106 min
Delta R.T.: 0.000 min
Response: 54256
Conc: 11.79 ng/ml