

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071819\
 Data File : P0058035.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Jul 2019 13:39
 Operator : SM/AJ
 Sample : K3849-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S12-06-B

Manual Integrations
 APPROVED

Ankita
 7/18/2019 2:37:46 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 17 14:29:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.200	3.539	892862	806889	26.348	25.157
2)	SA Decachlor...	9.716	8.444	1342376	901379	26.239	26.298m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071819\
Data File : PO058035.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Jul 2019 13:39
Operator : SM/AJ
Sample : K3849-04
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S12-06-B


Manual Integrations
APPROVED

Ankita
7/18/2019 2:37:46 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 17 14:29:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

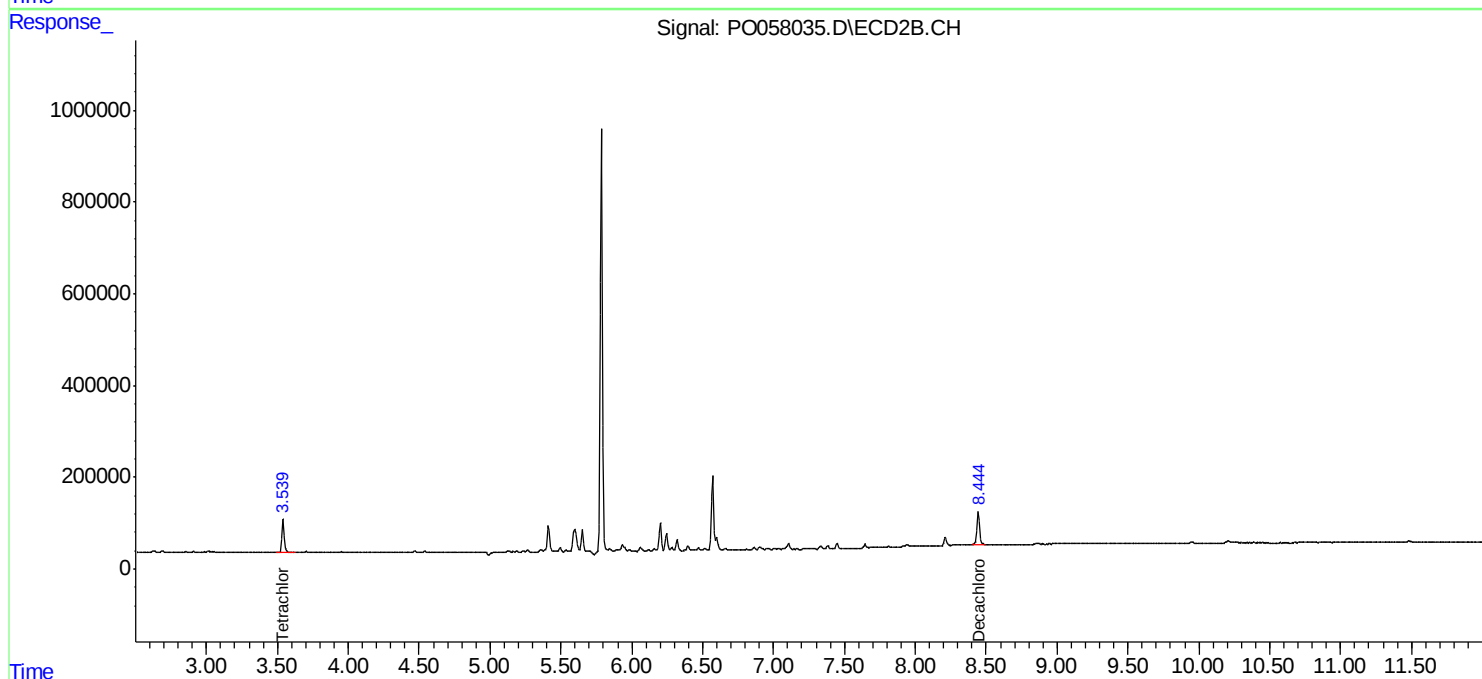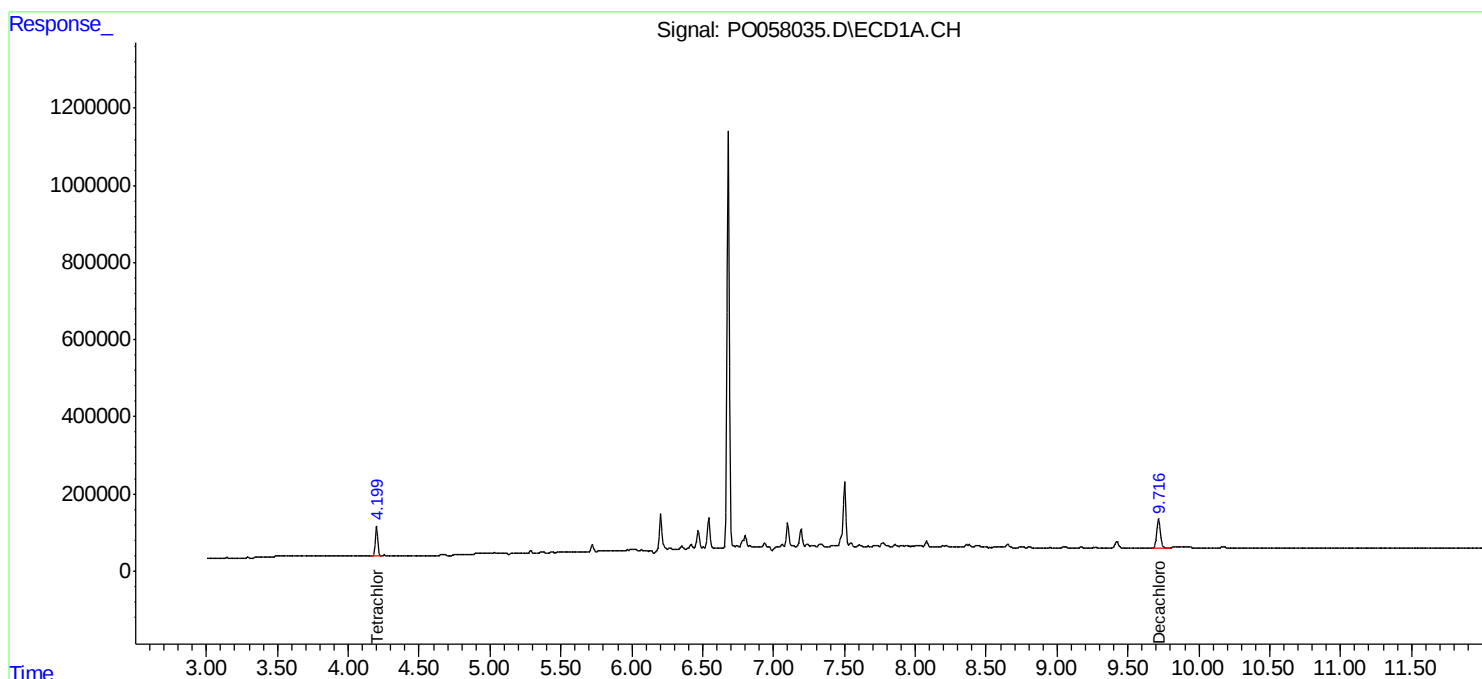

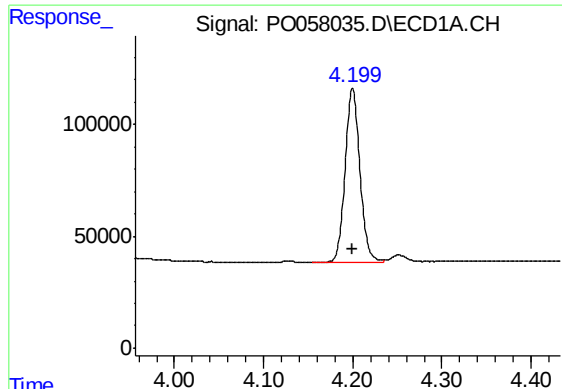


#1 Tetrachloro-m-xylene

R.T.: 4.200 min
Delta R.T.: 0.000 min
Response: 892862
Conc: 26.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
S12-06-B


Manual Integrations
APPROVED

Ankita
7/18/2019 2:37:46 PM

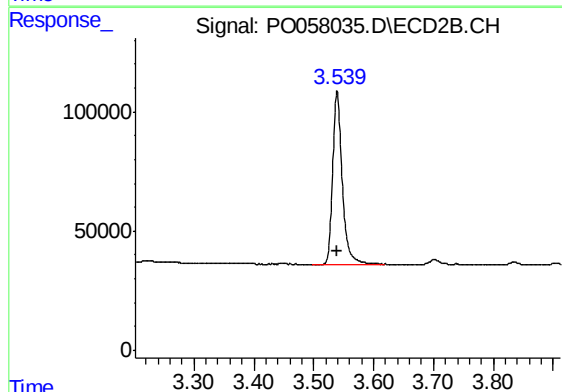


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 806889
Conc: 25.16 ng/ml

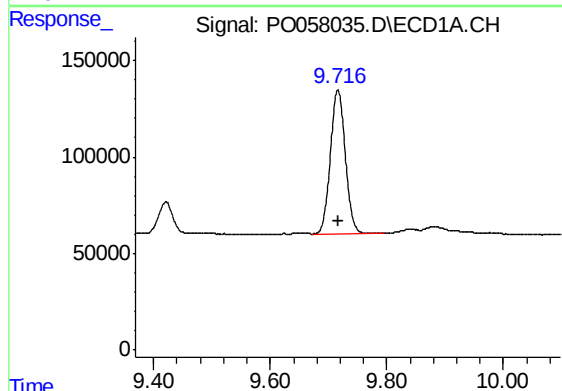

#2 Decachlorobiphenyl

R.T.: 9.716 min
Delta R.T.: -0.002 min
Response: 1342376
Conc: 26.24 ng/ml

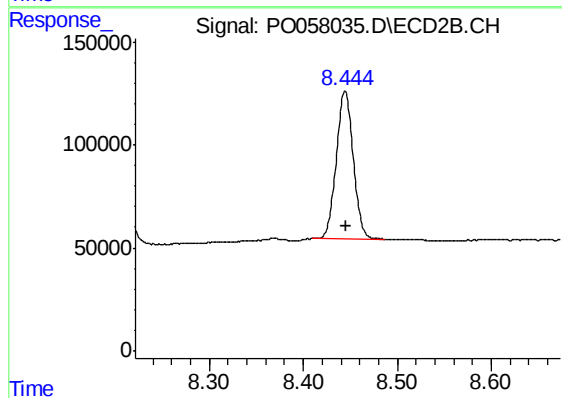

#2 Decachlorobiphenyl

R.T.: 8.444 min
Delta R.T.: -0.001 min
Response: 901379
Conc: 26.30 ng/ml m