

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071819\
 Data File : P0058080.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jul 2019 5:41
 Operator : SM/AJ
 Sample : K3840-01
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-SF-02-005-A

Manual Integrations
 APPROVED

Ankita
 7/18/2019 2:38:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 07:08:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.198	3.540	892576	787721	26.340	24.560
2) SA Decachlor...	9.713	8.443	892248	551094	17.441	16.078m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071819\
Data File : P0058080.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jul 2019 5:41
Operator : SM/AJ
Sample : K3840-01
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-SF-02-005-A


Manual Integrations
APPROVED

Ankita
7/18/2019 2:38:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 07:08:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

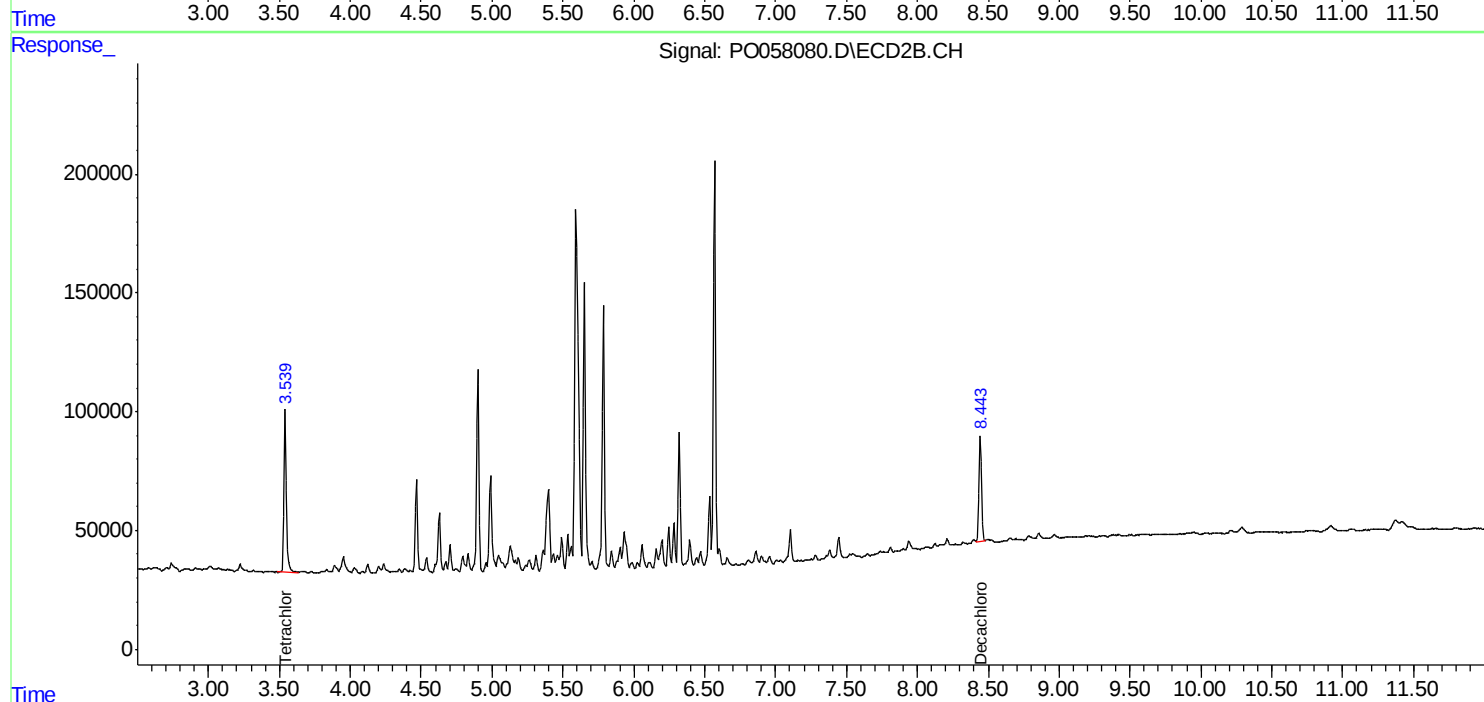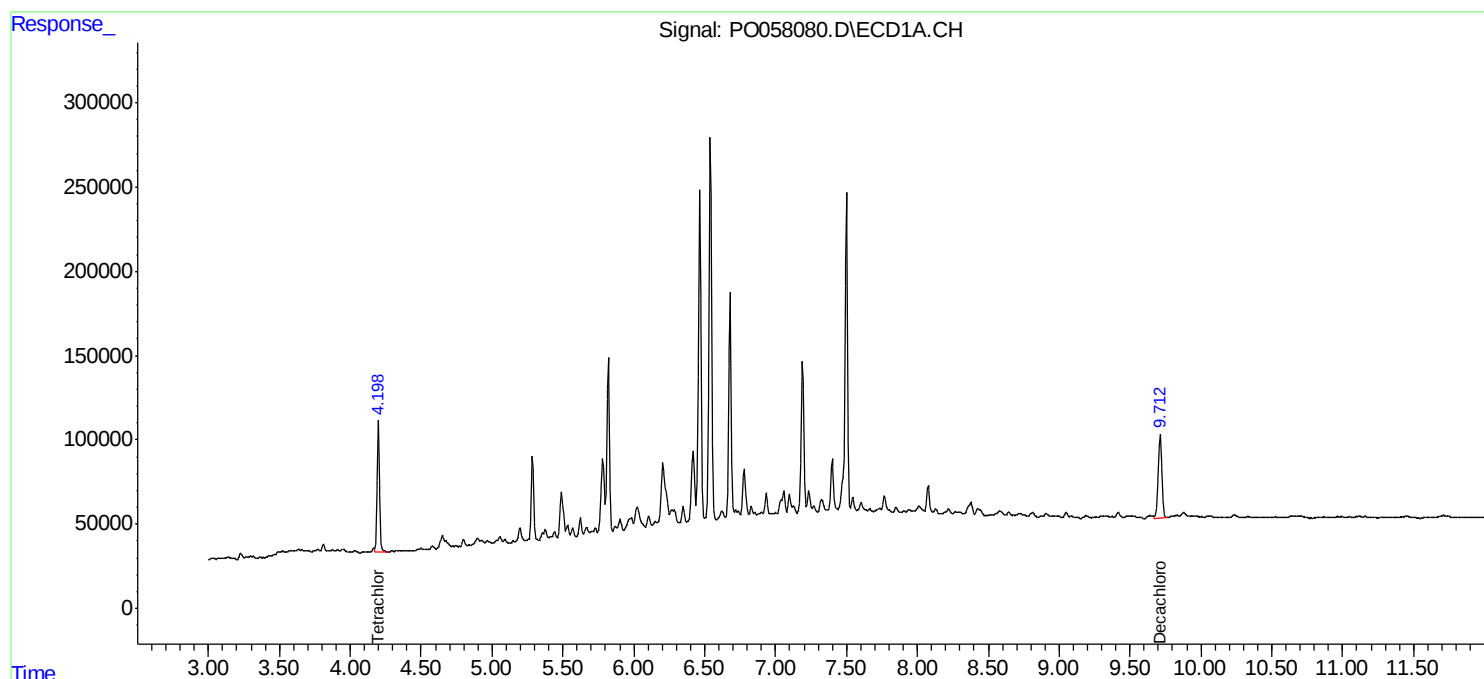

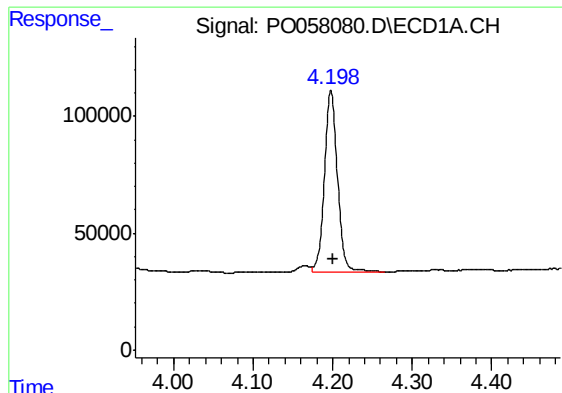


#1 Tetrachloro-m-xylene

R.T.: 4.198 min
Delta R.T.: -0.002 min
Response: 892576
Conc: 26.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-02-005-A


Manual Integrations
APPROVED

Ankita
7/18/2019 2:38:36 PM

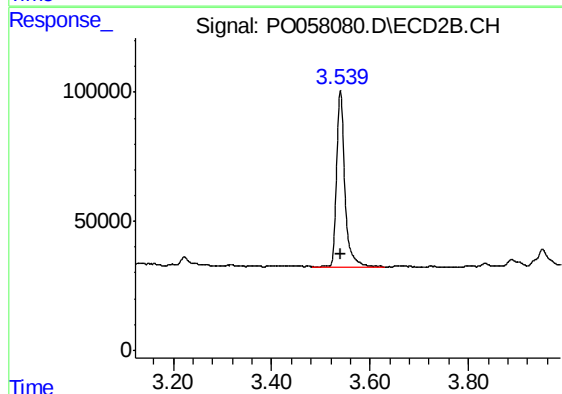


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: 0.000 min
Response: 787721
Conc: 24.56 ng/ml

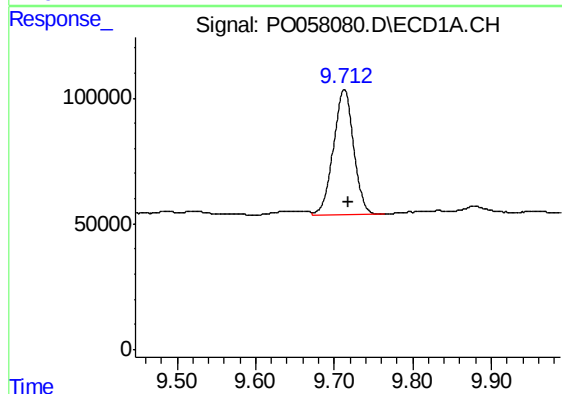

#2 Decachlorobiphenyl

R.T.: 9.713 min
Delta R.T.: -0.005 min
Response: 892248
Conc: 17.44 ng/ml

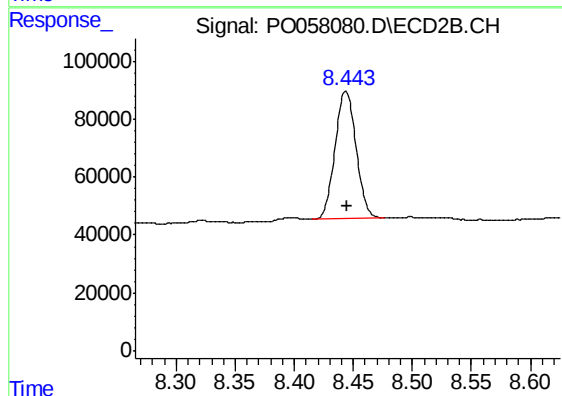

#2 Decachlorobiphenyl

R.T.: 8.443 min
Delta R.T.: -0.002 min
Response: 551094
Conc: 16.08 ng/ml m