

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071824\
 Data File : P0104846.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Jul 2024 20:27
 Operator : YP/AJ
 Sample : P3292-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 710

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/19/2024
 Supervised By :Ankita Jodhani 07/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 02:58:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070224.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 02 16:29:20 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.429	3.540	114.1E6	59428221	12.744	18.215m#
2) SA Decachlor...	10.219	8.441	56928893	11623629	9.283m	5.543 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071824\
Data File : PO104846.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Jul 2024 20:27
Operator : YP/AJ
Sample : P3292-02
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
710


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/19/2024
Supervised By :Ankita Jodhani 07/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 02:58:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO070224.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 02 16:29:20 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

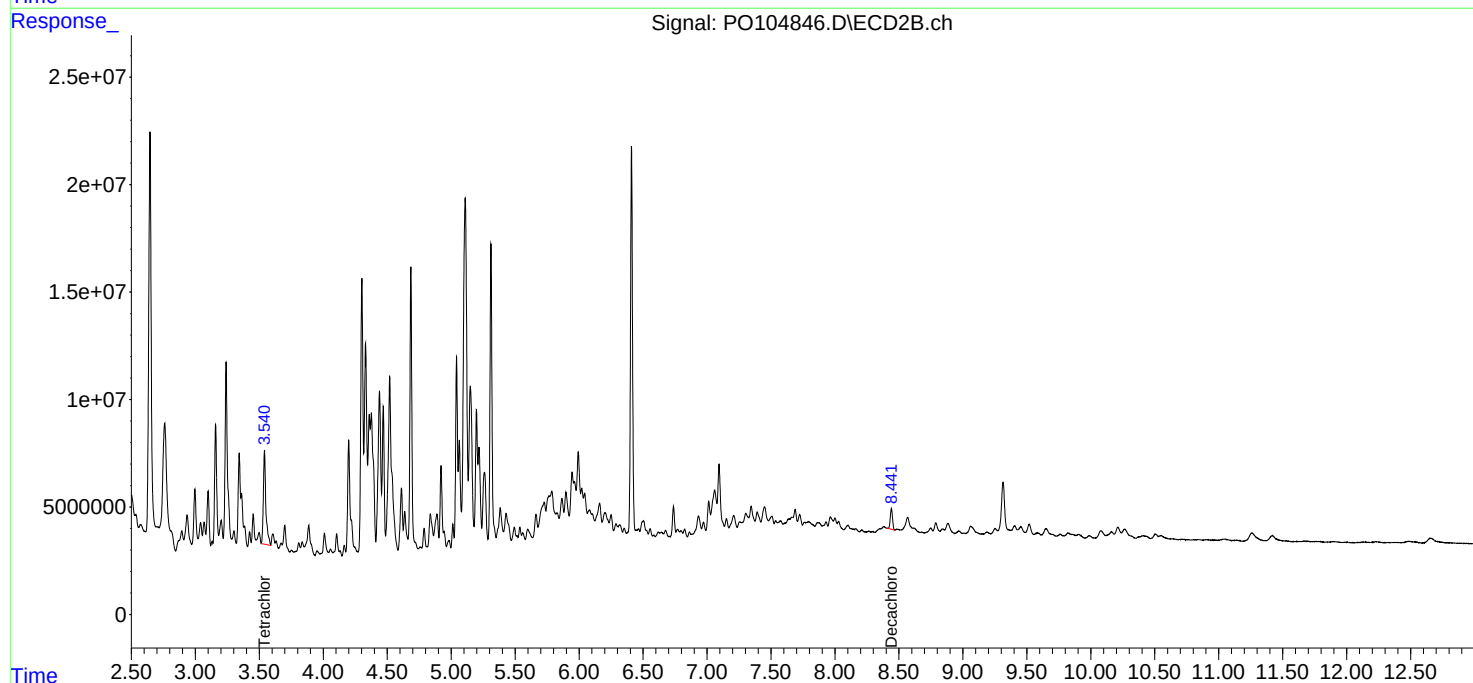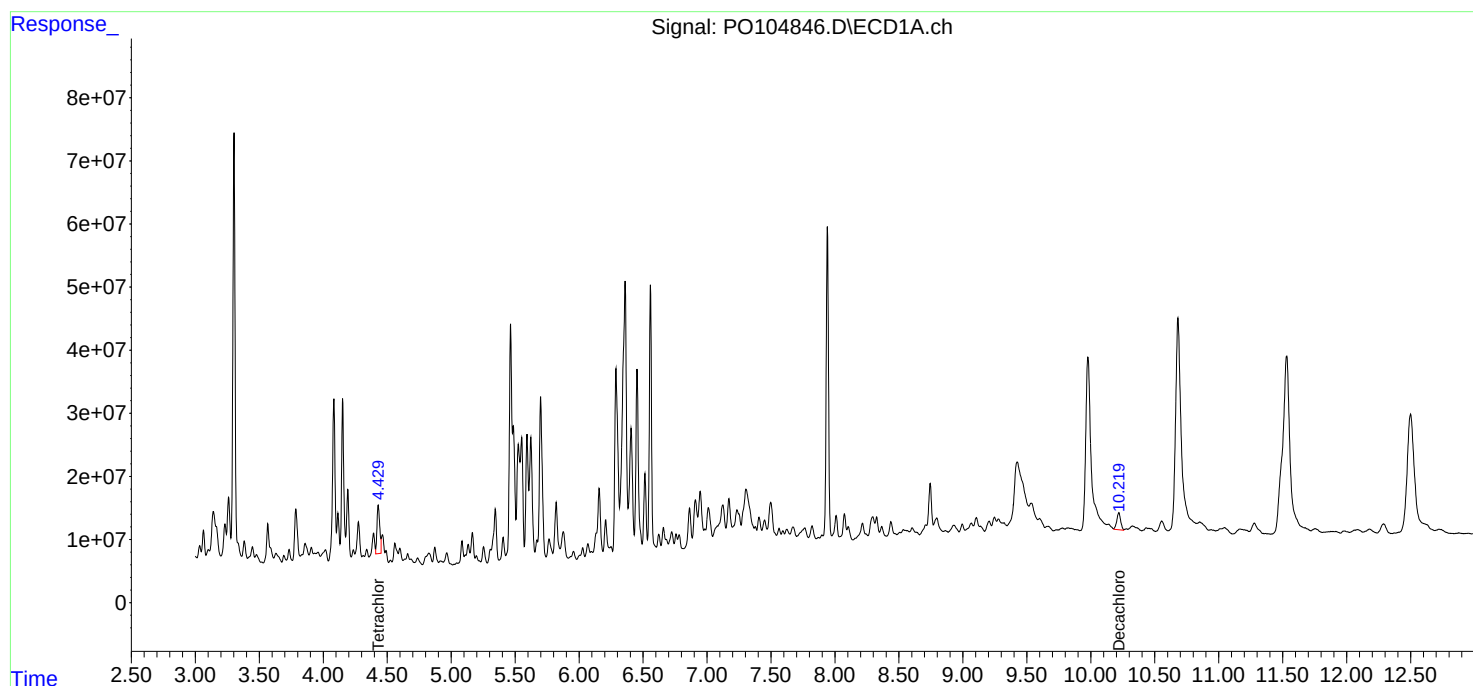

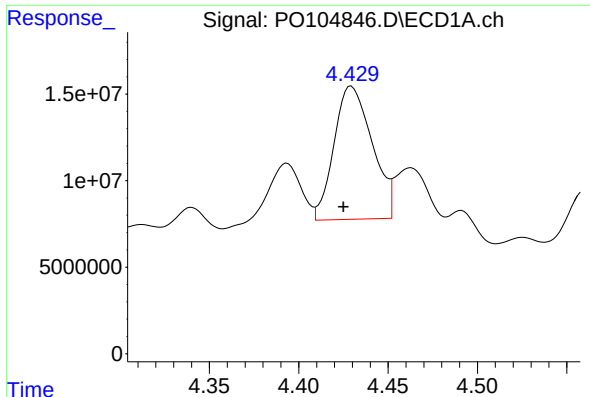


#1 Tetrachloro-m-xylene

R.T.: 4.429 min
Delta R.T.: 0.004 min
Response: 114104863
Conc: 12.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
710


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/19/2024
Supervised By :Ankita Jodhani 07/19/2024

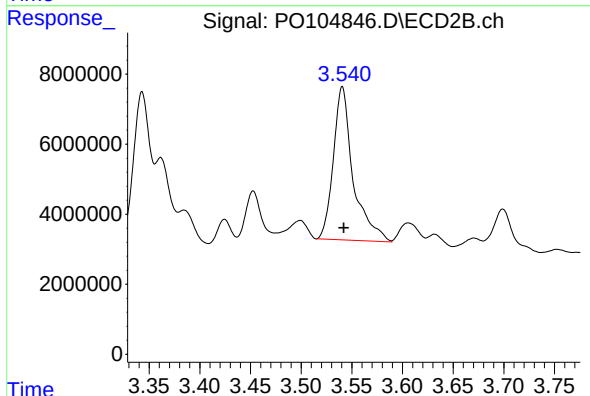


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: -0.002 min
Response: 59428221
Conc: 18.22 ng/ml m

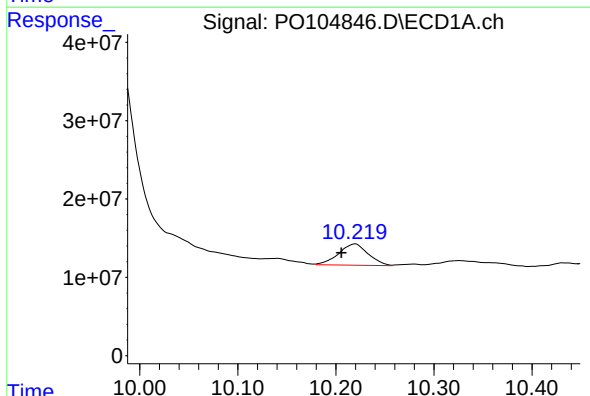

#2 Decachlorobiphenyl

R.T.: 10.219 min
Delta R.T.: 0.014 min
Response: 56928893
Conc: 9.28 ng/ml m

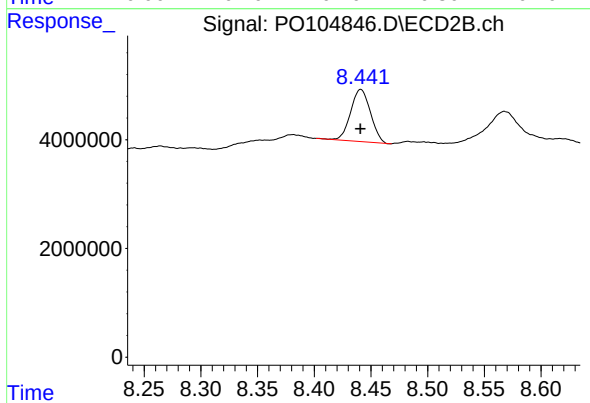

#2 Decachlorobiphenyl

R.T.: 8.441 min
Delta R.T.: 0.000 min
Response: 11623629
Conc: 5.54 ng/ml