

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071918\
Data File : P0046906.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jul 2018 3:23
Operator : SM/SJ
Sample : J4035-01
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MH-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 04:54:10 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071918.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 19 01:07:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.191	3.517	2545085	3317630	8.856	10.869
2)	SA Decachlor...	9.714	8.439	1847871	1810047	8.401	7.392

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071918\
Data File : P0046906.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jul 2018 3:23
Operator : SM/SJ
Sample : J4035-01
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MH-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 04:54:10 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071918.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 19 01:07:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

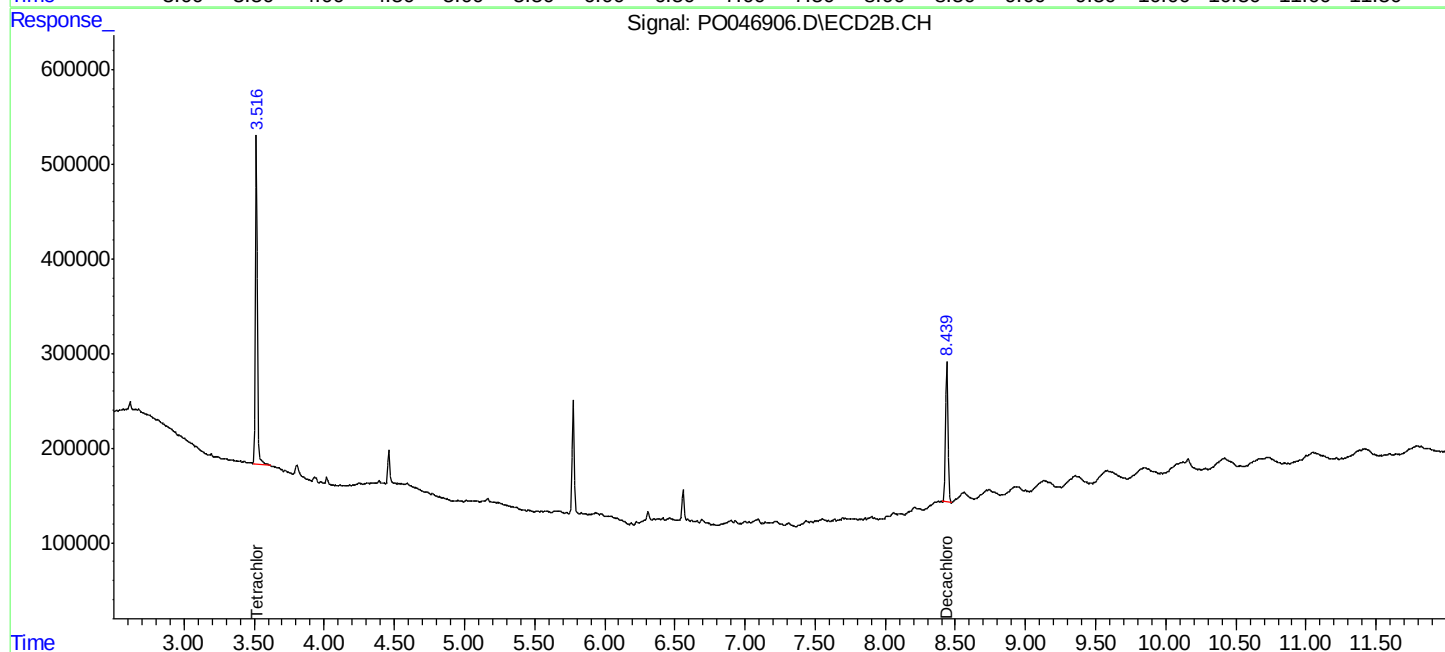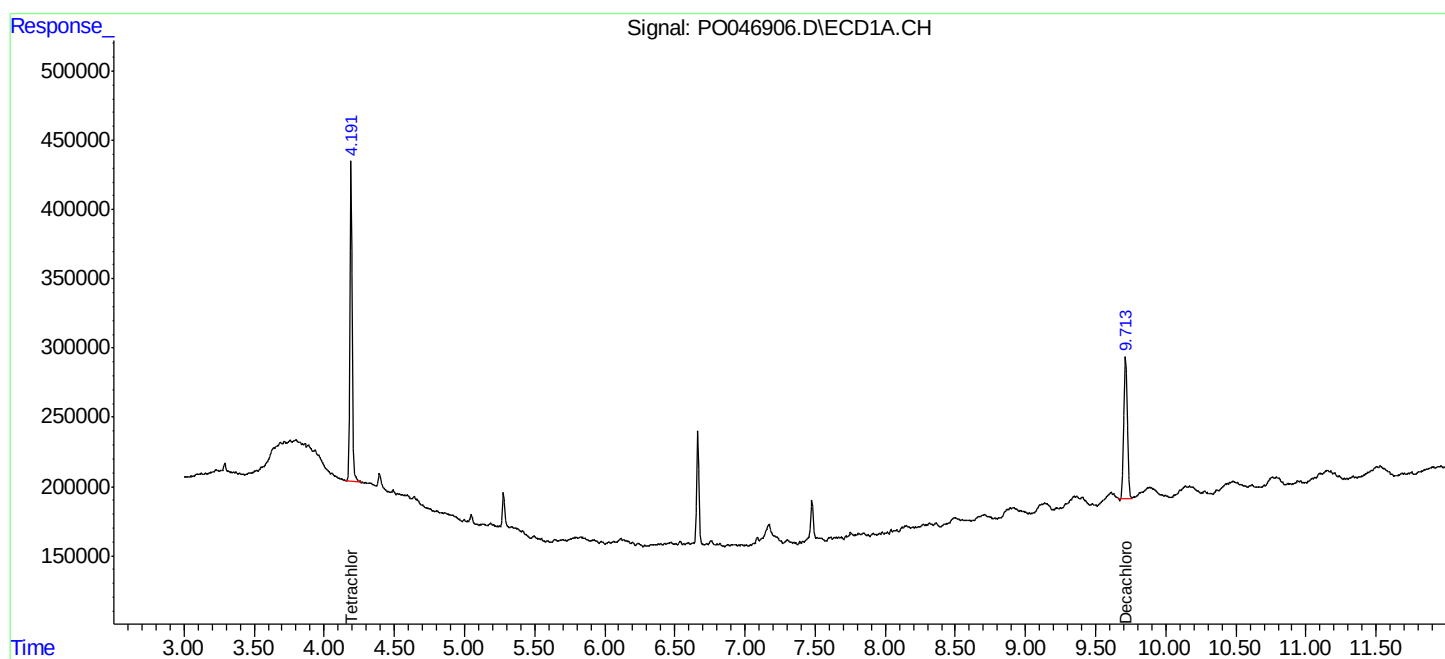


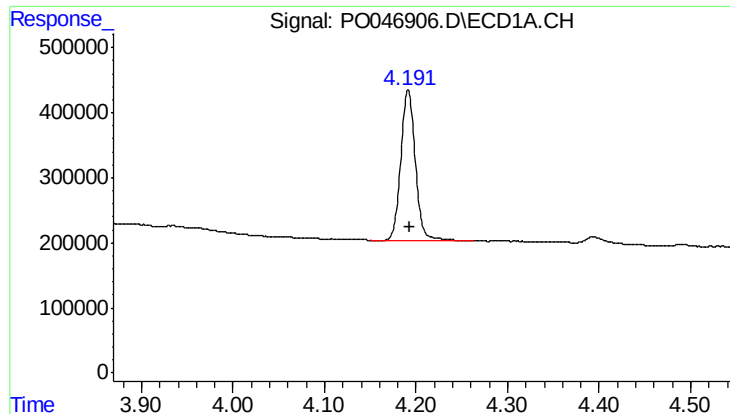

#1 Tetrachloro-m-xylene


R.T.: 4.191 min
Delta R.T.: -0.002 min
Response: 2545085
Conc: 8.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
MH-2

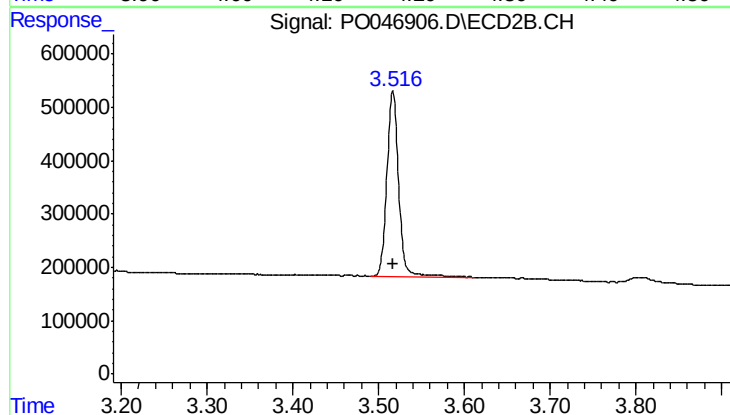


#1 Tetrachloro-m-xylene

R.T.: 3.517 min
Delta R.T.: 0.000 min
Response: 3317630
Conc: 10.87 ng/ml

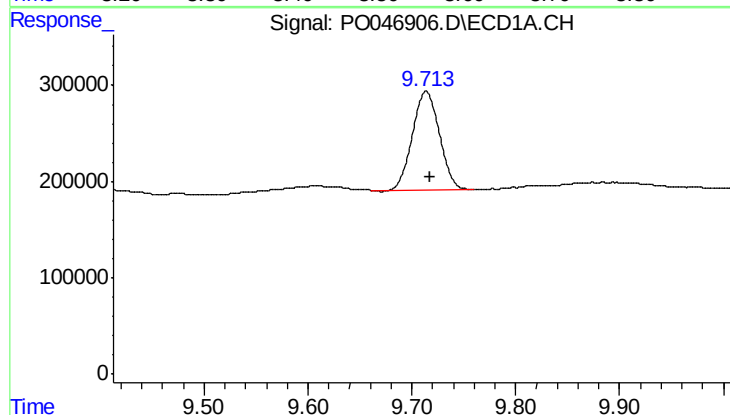

#2 Decachlorobiphenyl

R.T.: 9.714 min
Delta R.T.: -0.004 min
Response: 1847871
Conc: 8.40 ng/ml

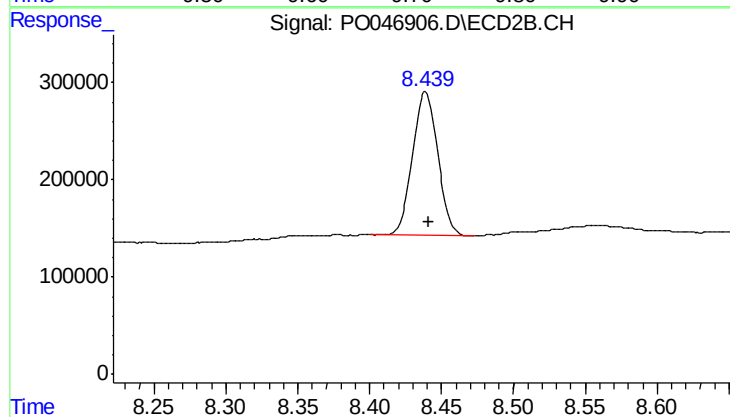

#2 Decachlorobiphenyl

R.T.: 8.439 min
Delta R.T.: -0.003 min
Response: 1810047
Conc: 7.39 ng/ml