

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0071918\
 Data File : P0046917.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jul 2018 6:34
 Operator : SM/SJ
 Sample : J4016-08
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB3-U-23-13

Manual Integrations
 APPROVED

Sohil
 7/19/2018 5:38:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 09:01:12 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0071918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 19 01:07:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.191	3.516	4122714	5084600	14.346m	16.657
2) SA Decachlor...	9.711	8.439	3029834	3058509	13.775	12.491

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071918\
Data File : P0046917.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jul 2018 6:34
Operator : SM/SJ
Sample : J4016-08
Misc :
ALS Vial : 40 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
SB3-U-23-13


Manual Integrations
APPROVED

Sohil
7/19/2018 5:38:47 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 09:01:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071918.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 19 01:07:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

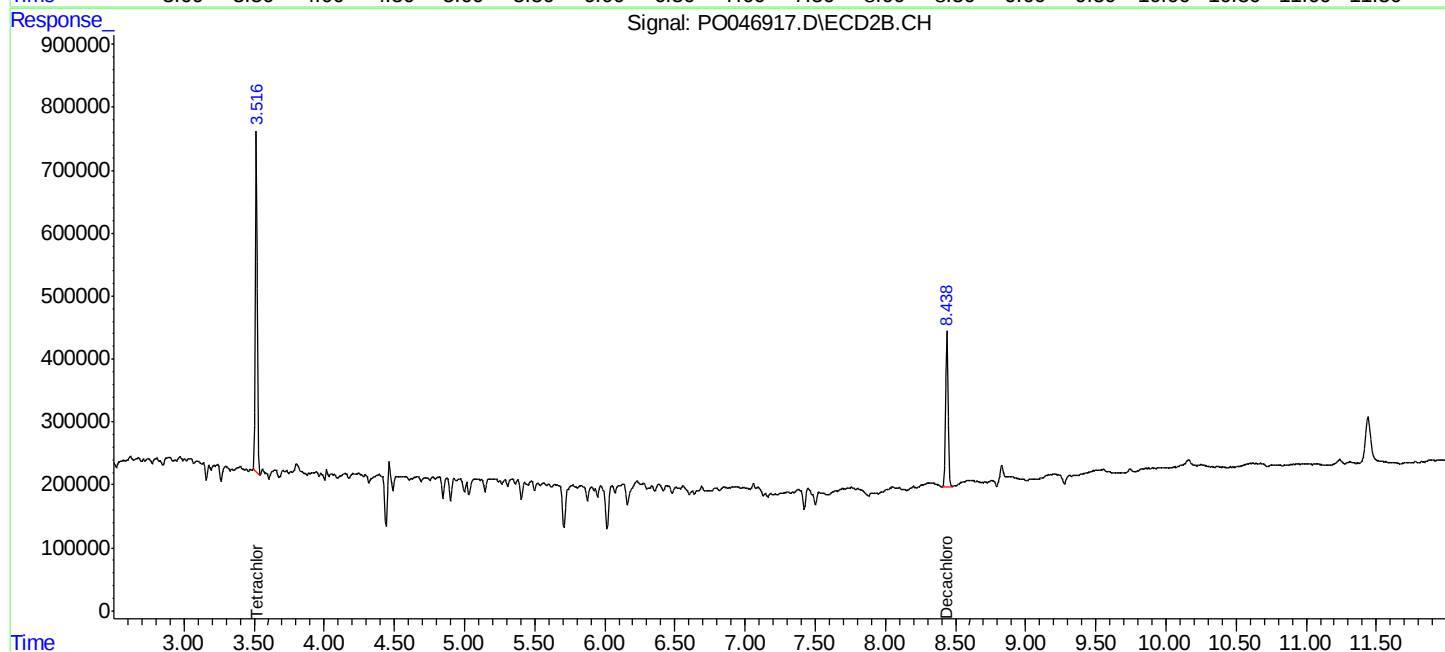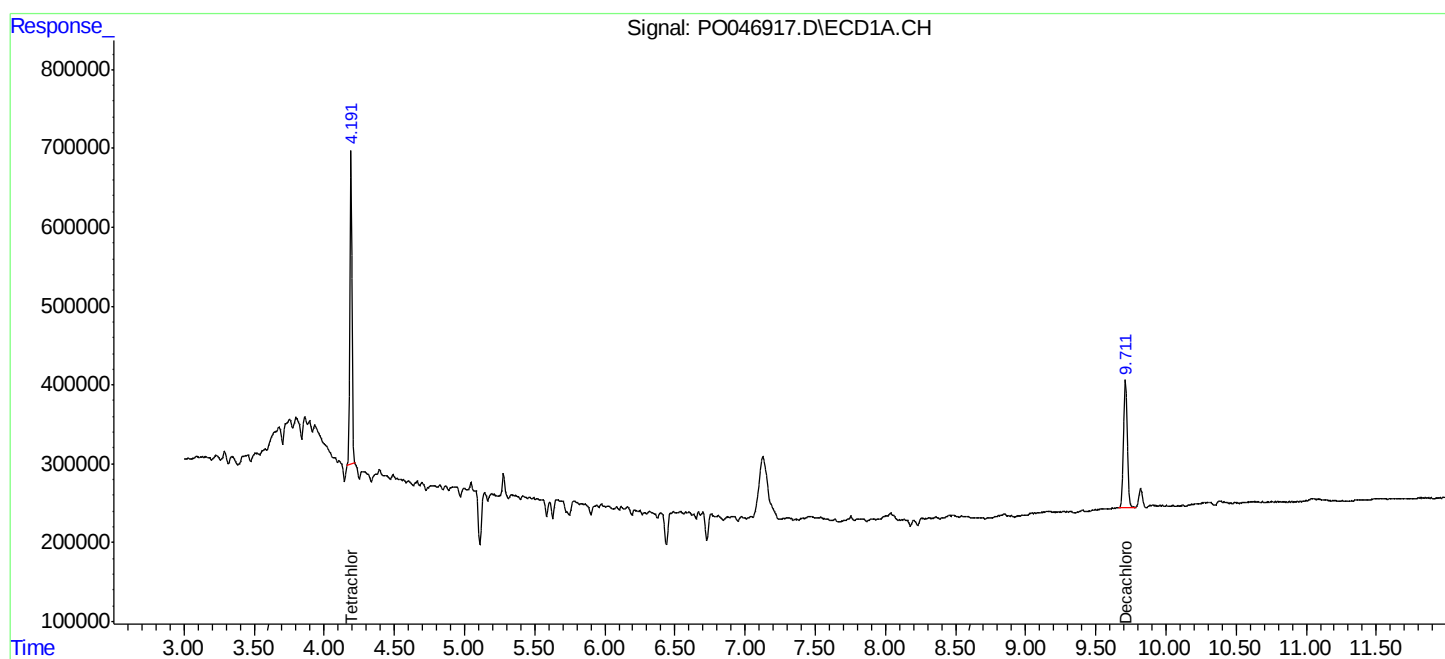

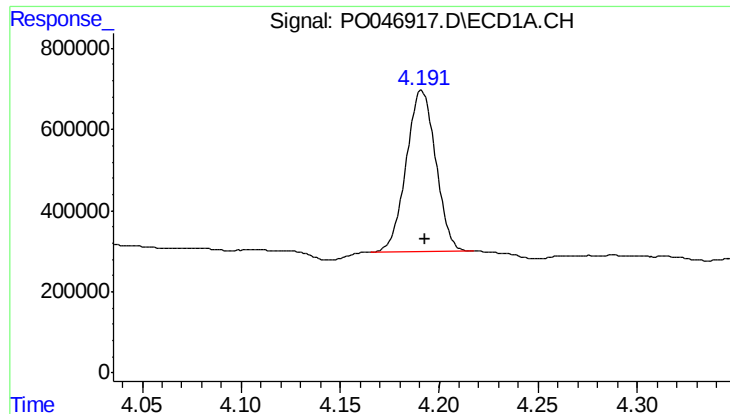


#1 Tetrachloro-m-xylene

R.T.: 4.191 min
Delta R.T.: -0.002 min
Response: 4122714
Conc: 14.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB3-U-23-13


Manual Integrations
APPROVED

Sohil
7/19/2018 5:38:47 PM

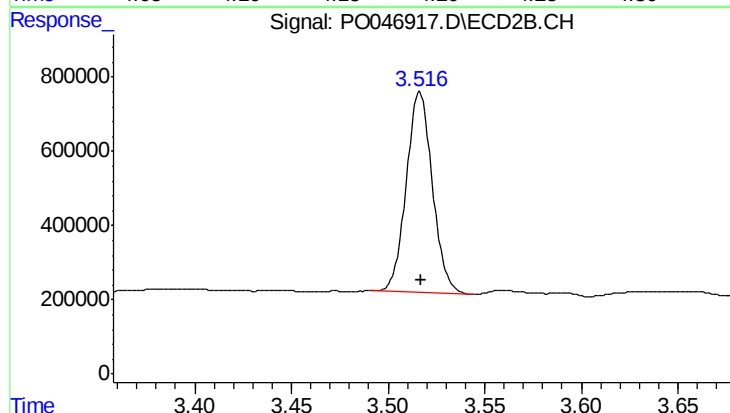


#1 Tetrachloro-m-xylene

R.T.: 3.516 min
Delta R.T.: 0.000 min
Response: 5084600
Conc: 16.66 ng/ml

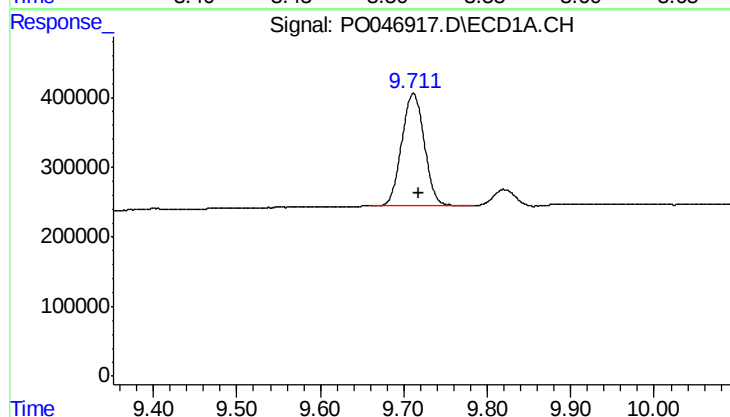

#2 Decachlorobiphenyl

R.T.: 9.711 min
Delta R.T.: -0.006 min
Response: 3029834
Conc: 13.78 ng/ml

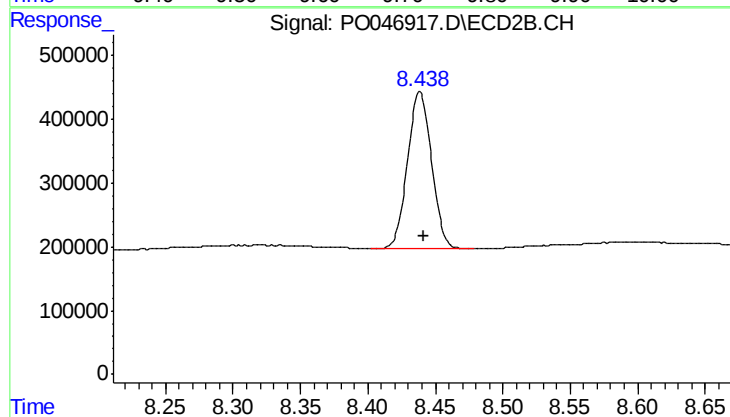

#2 Decachlorobiphenyl

R.T.: 8.439 min
Delta R.T.: -0.003 min
Response: 3058509
Conc: 12.49 ng/ml