

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071919\
 Data File : P0058086.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jul 2019 11:02
 Operator : SM/AJ
 Sample : K3622-05
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OR-03-071519-A

Manual Integrations
 APPROVED

Ankita
 7/21/2019 11:48:36 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 11:56:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.207	3.542	1128275	1009115	33.295	31.462
2) SA Decachlor...	9.722	8.447	1080571	702303	21.122m	20.490

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071919\
Data File : P0058086.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jul 2019 11:02
Operator : SM/AJ
Sample : K3622-05
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OR-03-071519-A


Manual Integrations
APPROVED

Ankita
7/21/2019 11:48:36 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 11:56:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

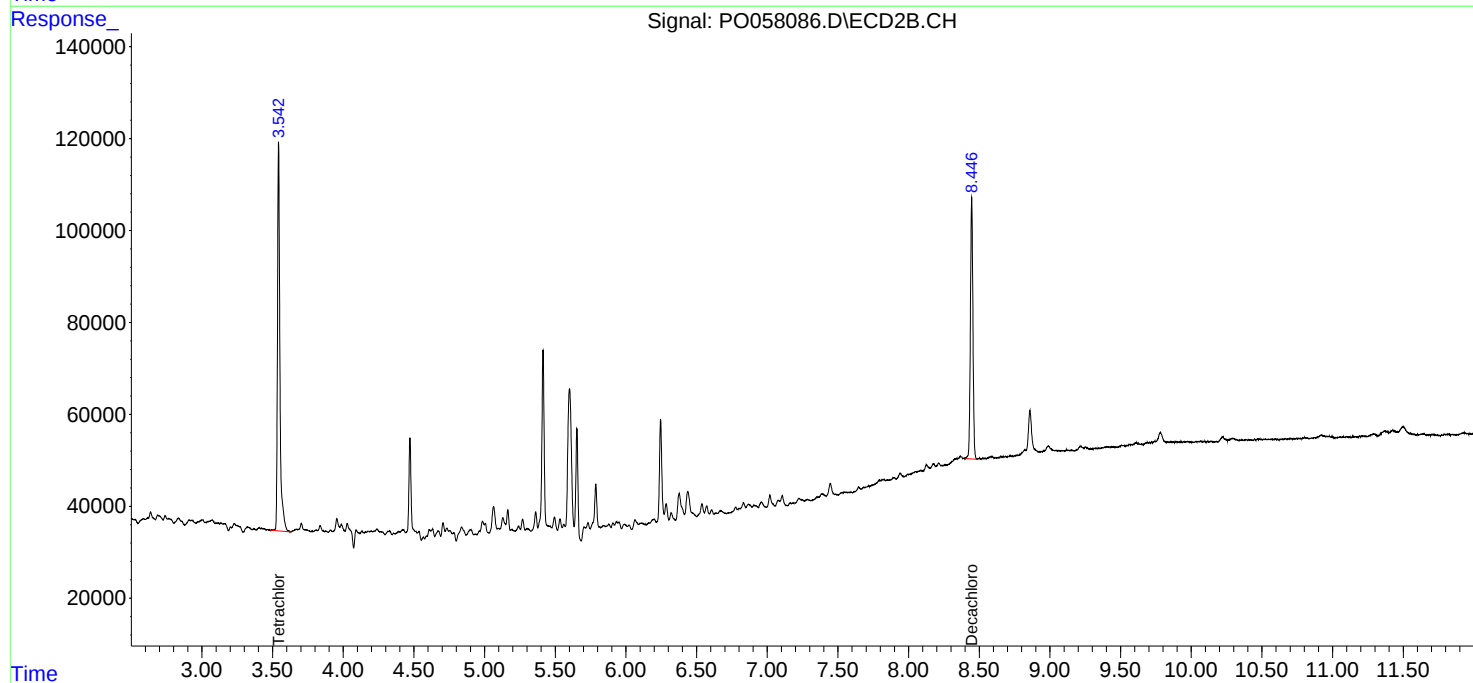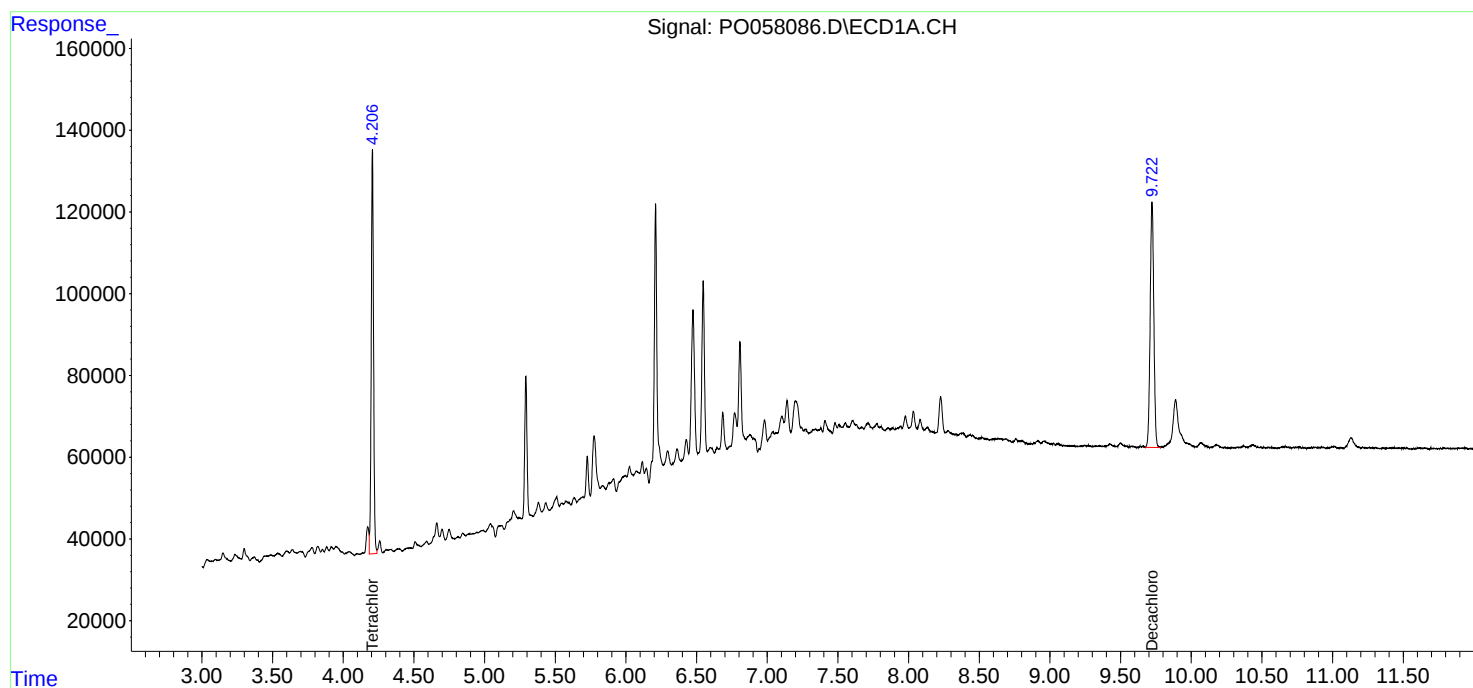

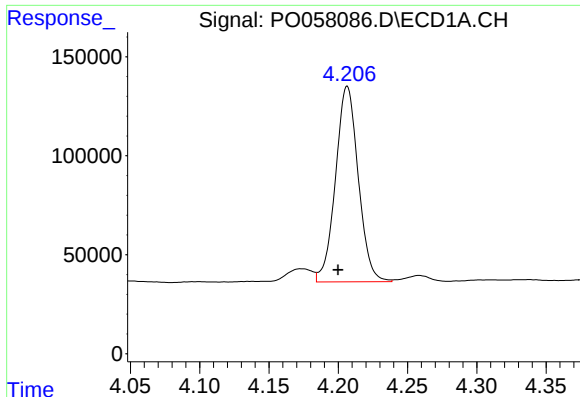


#1 Tetrachloro-m-xylene

R.T.: 4.207 min
Delta R.T.: 0.007 min
Response: 1128275
Conc: 33.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
OR-03-071519-A


Manual Integrations
APPROVED

Ankita
7/21/2019 11:48:36 AM

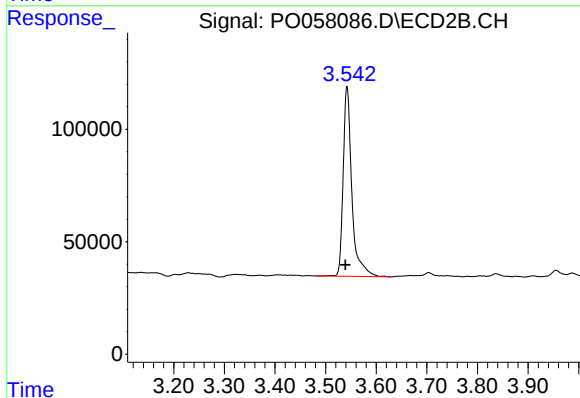


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: 0.003 min
Response: 1009115
Conc: 31.46 ng/ml

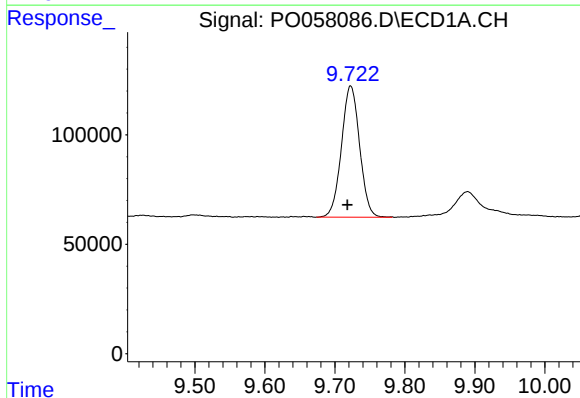

#2 Decachlorobiphenyl

R.T.: 9.722 min
Delta R.T.: 0.004 min
Response: 1080571
Conc: 21.12 ng/ml m

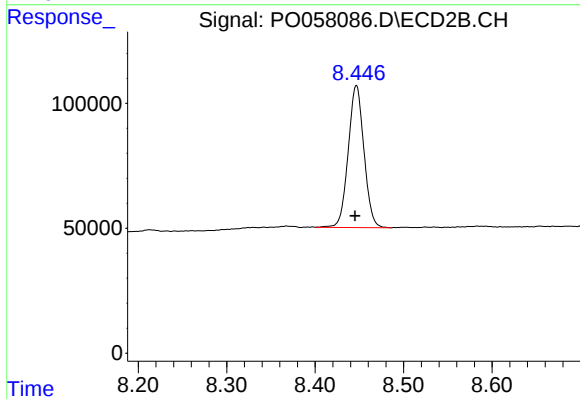

#2 Decachlorobiphenyl

R.T.: 8.447 min
Delta R.T.: 0.001 min
Response: 702303
Conc: 20.49 ng/ml