

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071919\
 Data File : P0058093.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jul 2019 13:33
 Operator : SM/AJ
 Sample : K3862-02DL 10X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S3-07-BDL

Manual Integrations
 APPROVED

Ankita
 7/21/2019 11:48:40 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 18 13:47:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.204	3.541	105280	94847	3.107m	2.957
2) SA Decachlor...	9.720	8.446	117254	77611	2.292	2.264
Target Compounds						
26) L6 AR-1254-1	6.201	5.389	313776	350904	159.667	172.227
27) L6 AR-1254-2	6.418	5.535	814268	471715	249.084	260.311
28) L6 AR-1254-3	6.782	5.933	1069237	987327	303.090	337.152
29) L6 AR-1254-4	7.065	6.160	1160220	782159	392.122	423.329
30) L6 AR-1254-5	7.480	6.571	1634695	1434954	556.919	527.850

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071919\
Data File : P0058093.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jul 2019 13:33
Operator : SM/AJ
Sample : K3862-02DL 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S3-07-BDL


Manual Integrations
APPROVED

Ankita
7/21/2019 11:48:40 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 18 13:47:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

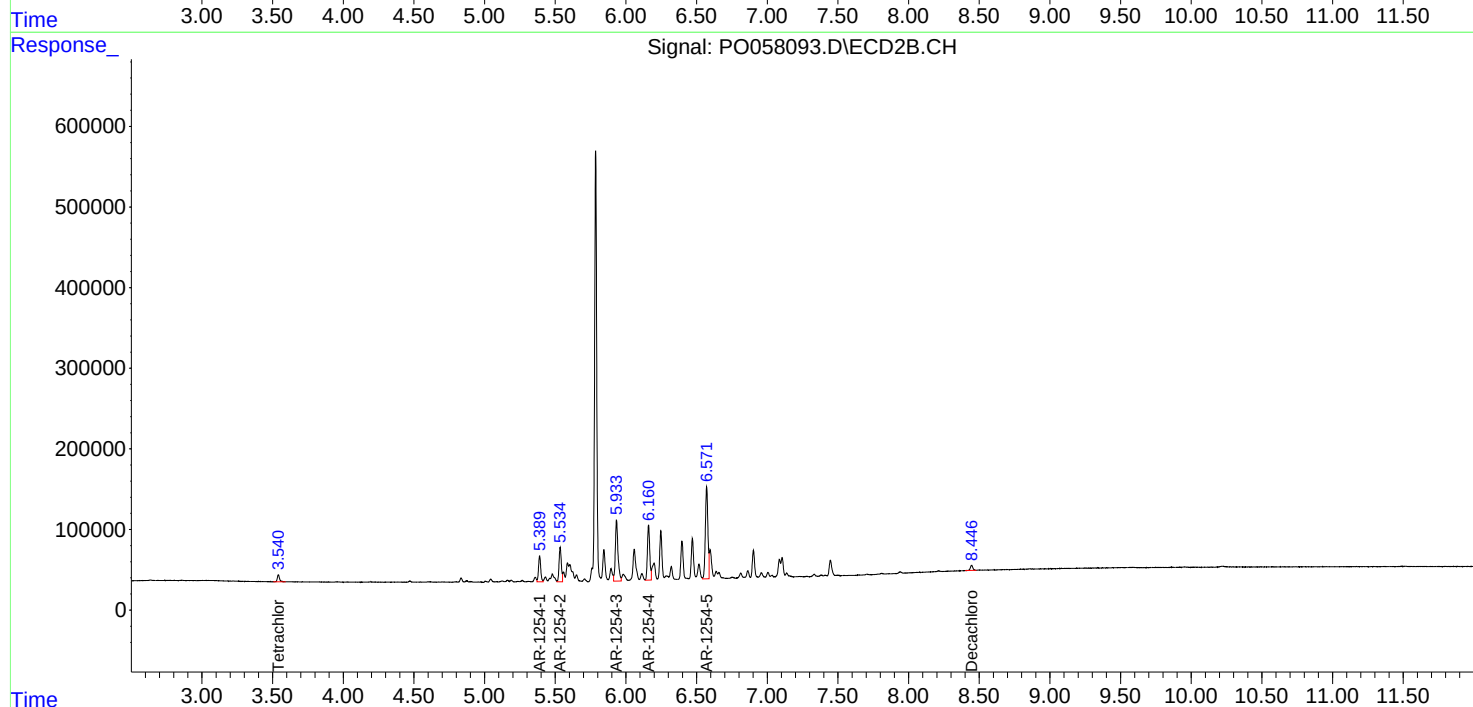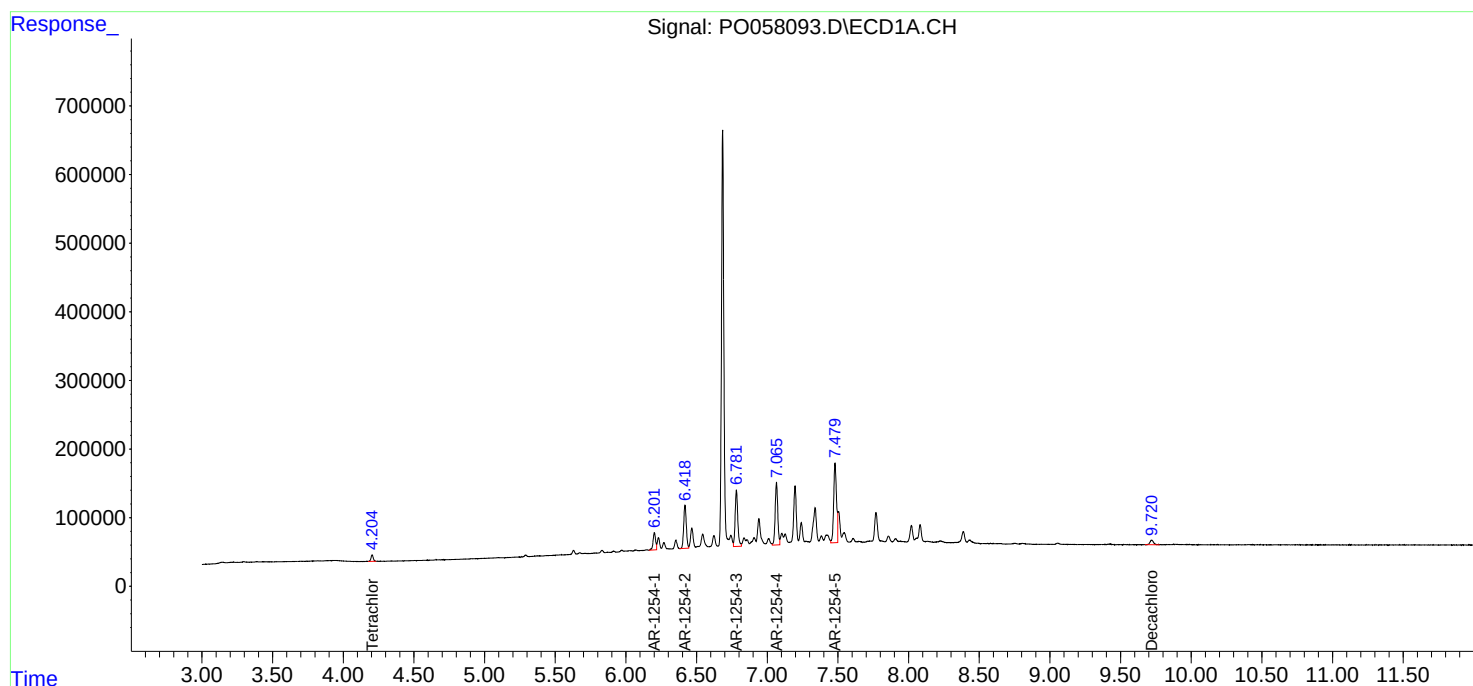

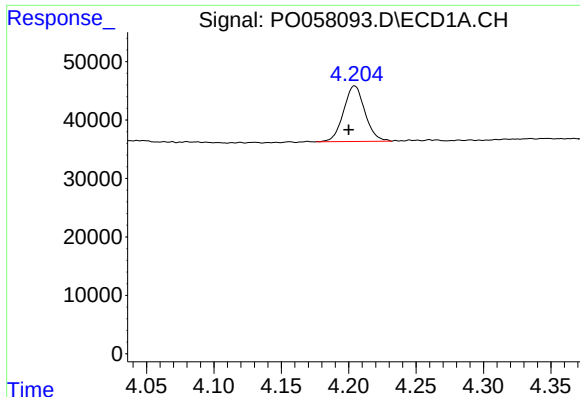


#1 Tetrachloro-m-xylene

R.T.: 4.204 min
Delta R.T.: 0.004 min
Response: 105280
Conc: 3.11 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S3-07-BDL


Manual Integrations
APPROVED

Ankita
7/21/2019 11:48:40 AM

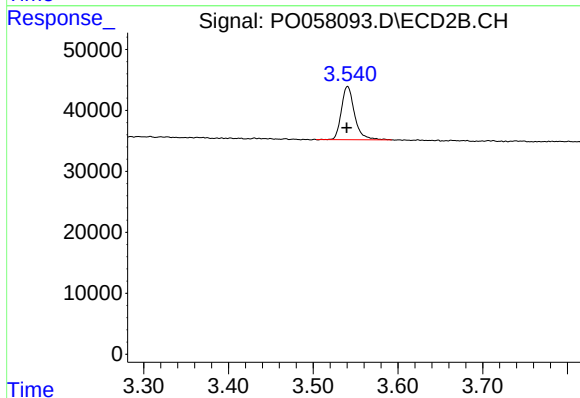


#1 Tetrachloro-m-xylene

R.T.: 3.541 min
Delta R.T.: 0.001 min
Response: 94847
Conc: 2.96 ng/ml

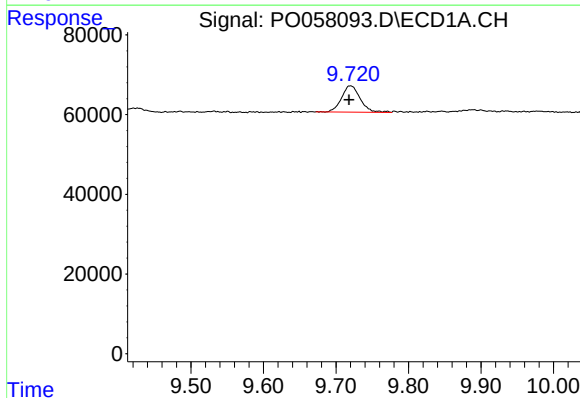


#2 Decachlorobiphenyl

R.T.: 9.720 min
Delta R.T.: 0.002 min
Response: 117254
Conc: 2.29 ng/ml

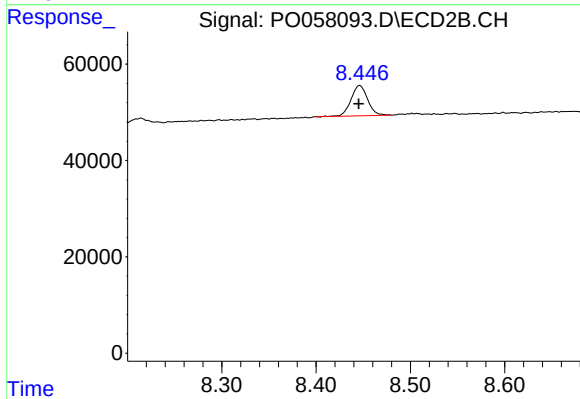

#2 Decachlorobiphenyl

R.T.: 8.446 min
Delta R.T.: 0.001 min
Response: 77611
Conc: 2.26 ng/ml

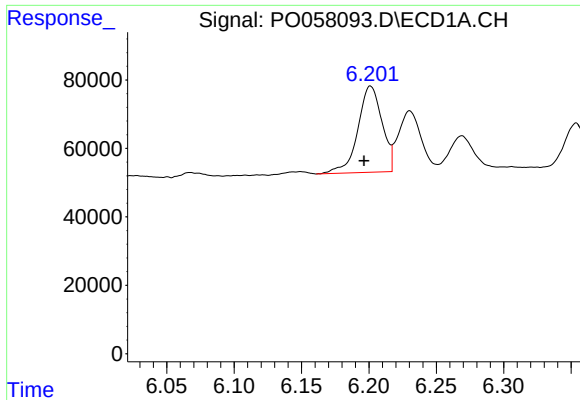


#26 AR-1254-1

R.T.: 6.201 min
Delta R.T.: 0.005 min
Response: 313776
Conc: 159.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
S3-07-BDL


Manual Integrations
APPROVED

Ankita
7/21/2019 11:48:40 AM

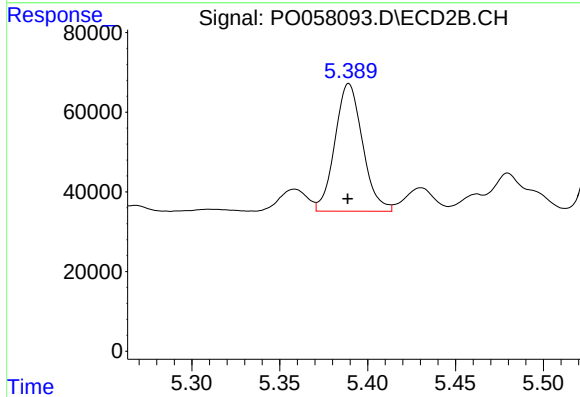


#26 AR-1254-1

R.T.: 5.389 min
Delta R.T.: 0.000 min
Response: 350904
Conc: 172.23 ng/ml

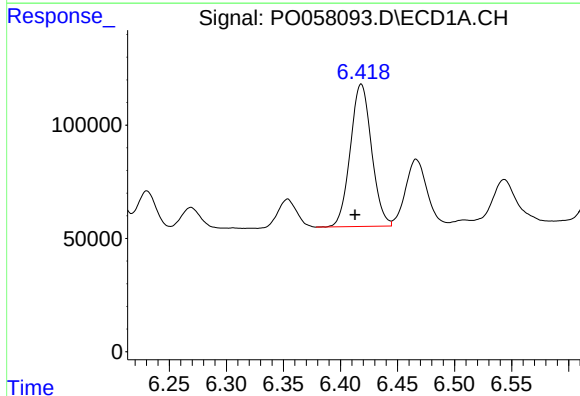


#27 AR-1254-2

R.T.: 6.418 min
Delta R.T.: 0.006 min
Response: 814268
Conc: 249.08 ng/ml

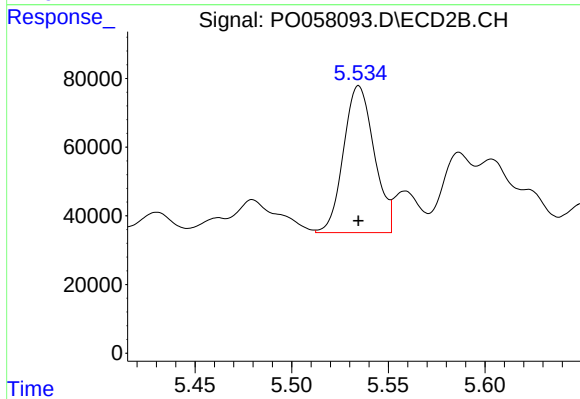

#27 AR-1254-2

R.T.: 5.535 min
Delta R.T.: 0.000 min
Response: 471715
Conc: 260.31 ng/ml

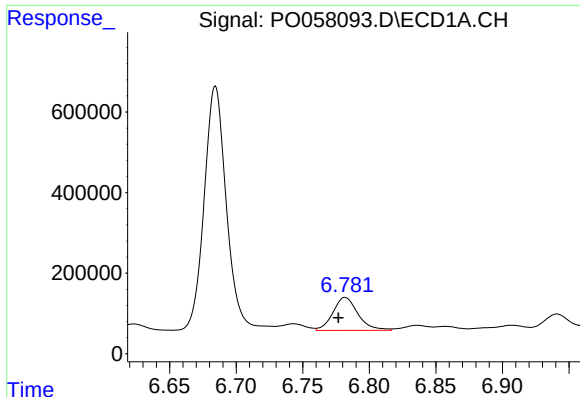


#28 AR-1254-3

R.T.: 6.782 min
Delta R.T.: 0.005 min
Response: 1069237
Conc: 303.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
S3-07-BDL


Manual Integrations
APPROVED

Ankita
7/21/2019 11:48:40 AM

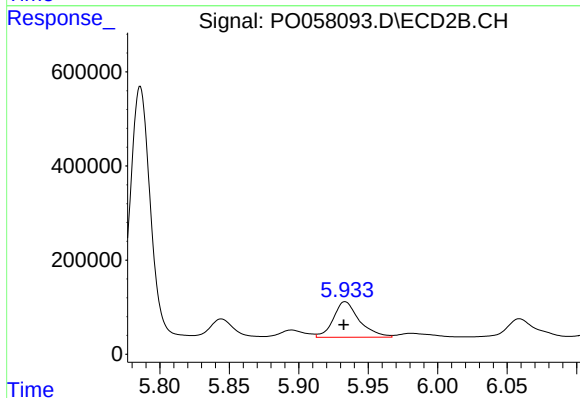


#28 AR-1254-3

R.T.: 5.933 min
Delta R.T.: 0.001 min
Response: 987327
Conc: 337.15 ng/ml

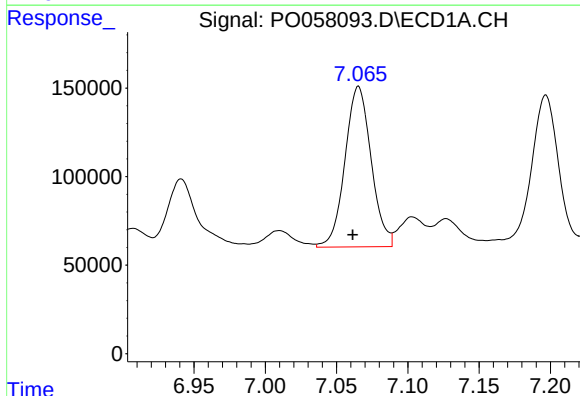


#29 AR-1254-4

R.T.: 7.065 min
Delta R.T.: 0.004 min
Response: 1160220
Conc: 392.12 ng/ml

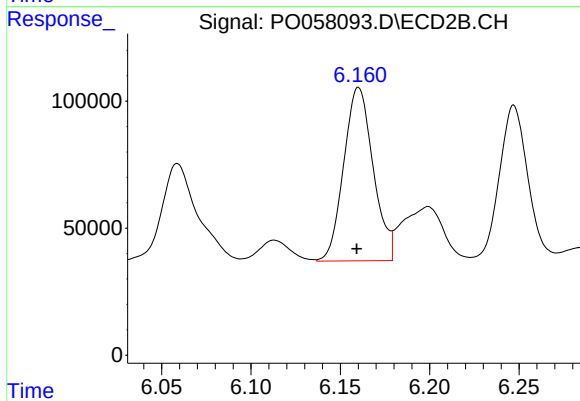

#29 AR-1254-4

R.T.: 6.160 min
Delta R.T.: 0.001 min
Response: 782159
Conc: 423.33 ng/ml

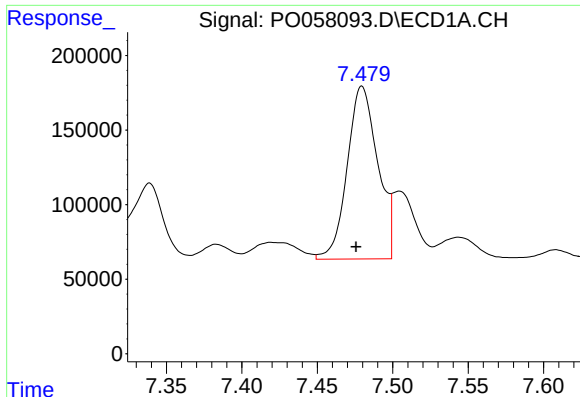


#30 AR-1254-5

R.T.: 7.480 min
Delta R.T.: 0.004 min
Response: 1634695
Conc: 556.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
S3-07-BDL

Manual Integrations
APPROVED

Ankita
7/21/2019 11:48:40 AM

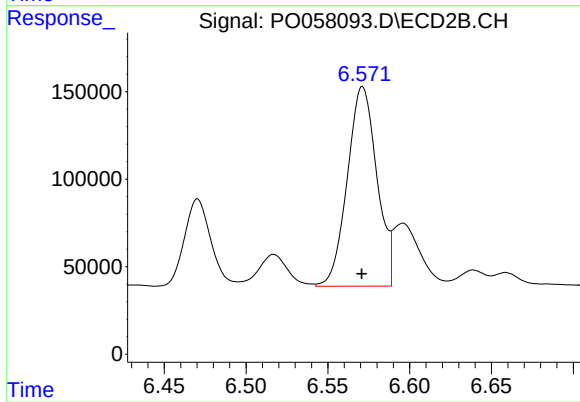

#30 AR-1254-5

R.T.: 6.571 min
Delta R.T.: 0.000 min
Response: 1434954
Conc: 527.85 ng/ml