

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071919\
 Data File : P0058115.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jul 2019 20:33
 Operator : SM/AJ
 Sample : K3889-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S3-06-S

Manual Integrations
 APPROVED

Ankita
 7/21/2019 11:49:30 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 05:48:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.196	3.540	781758	693084	23.070	21.609
2) SA Decachlor...	9.709	8.442	701652	478483	13.715	13.960
Target Compounds						
26) L6 AR-1254-1	6.191	5.387	75697	83435	38.519m	40.950
27) L6 AR-1254-2	6.411	5.533	467474	120632	143.000m	66.570 #
28) L6 AR-1254-3	6.774	5.930	402695	232160	114.149m	79.278m#
29) L6 AR-1254-4	7.056	6.158	199867	128739	67.550m	69.678
30) L6 AR-1254-5	7.470	6.569	431182	470313	146.898m	173.005

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071919\
Data File : P0058115.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jul 2019 20:33
Operator : SM/AJ
Sample : K3889-03
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S3-06-S


Manual Integrations
APPROVED

Ankita
7/21/2019 11:49:30 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 05:48:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

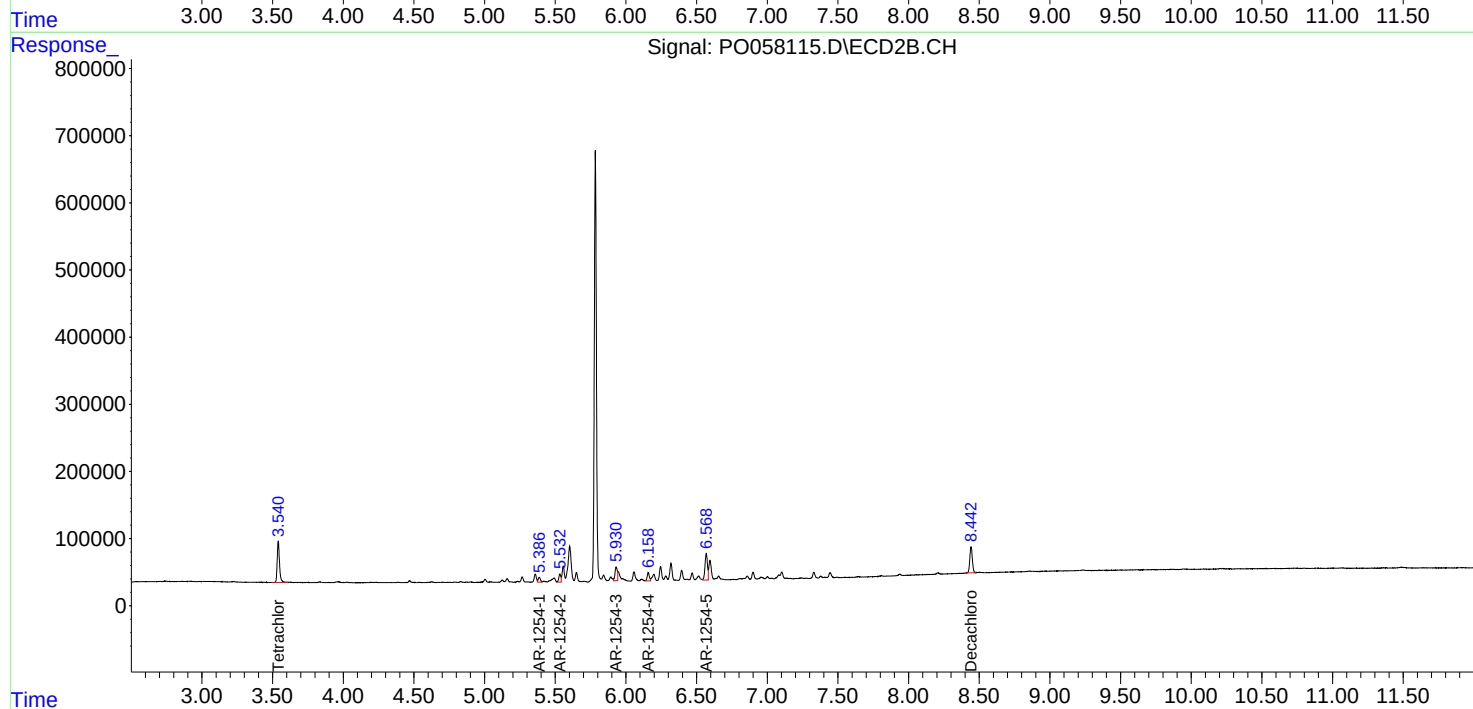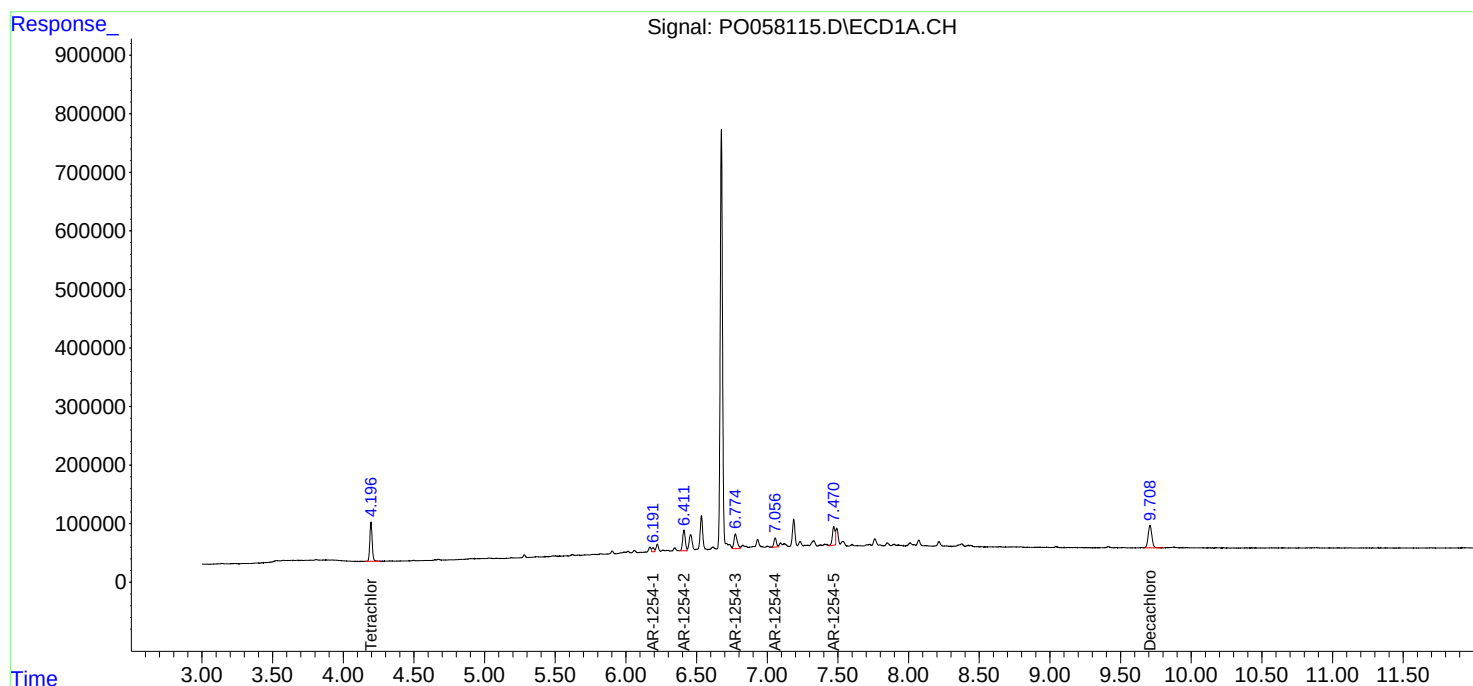

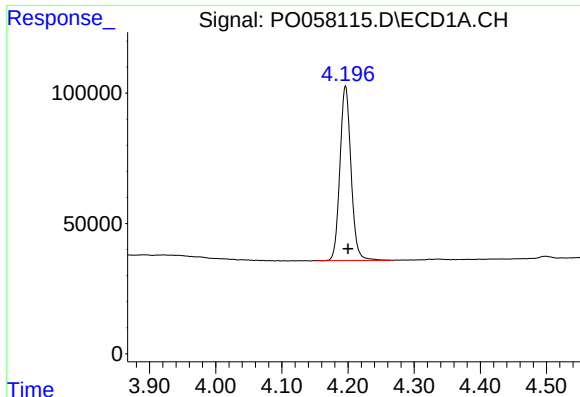


#1 Tetrachloro-m-xylene

R.T.: 4.196 min
Delta R.T.: -0.004 min
Response: 781758
Conc: 23.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
S3-06-S


Manual Integrations
APPROVED

Ankita
7/21/2019 11:49:30 AM

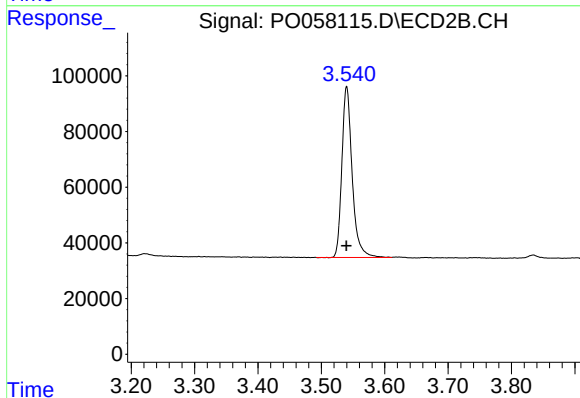


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: 0.000 min
Response: 693084
Conc: 21.61 ng/ml

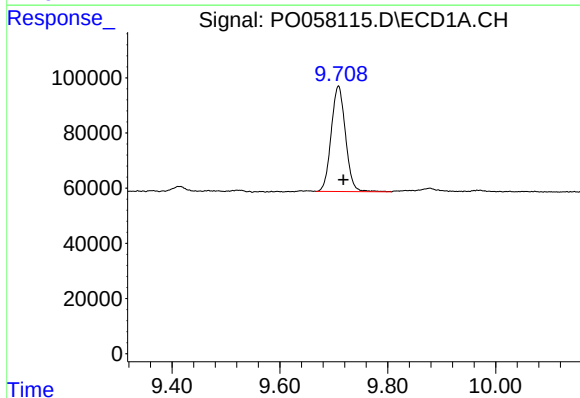


#2 Decachlorobiphenyl

R.T.: 9.709 min
Delta R.T.: -0.009 min
Response: 701652
Conc: 13.72 ng/ml

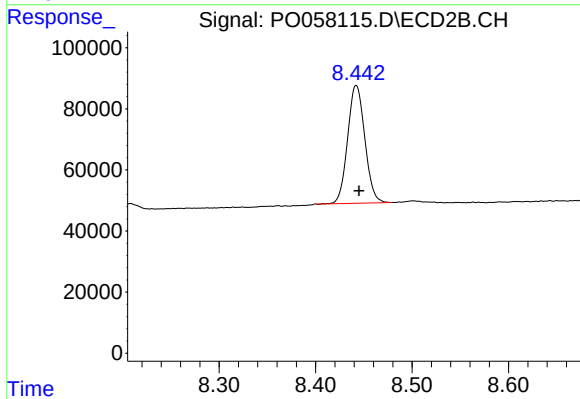

#2 Decachlorobiphenyl

R.T.: 8.442 min
Delta R.T.: -0.003 min
Response: 478483
Conc: 13.96 ng/ml

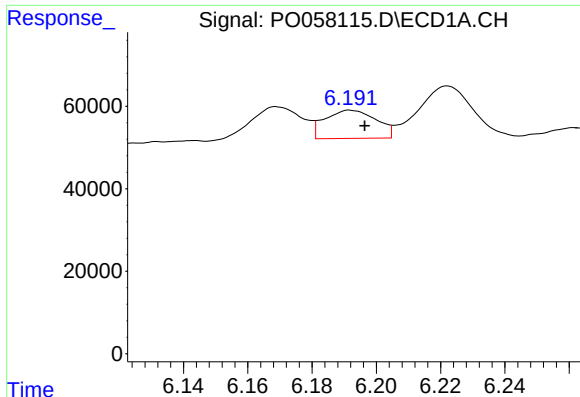


#26 AR-1254-1

R.T.: 6.191 min
Delta R.T.: -0.005 min
Response: 75697
Conc: 38.52 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S3-06-S


Manual Integrations
APPROVED

Ankita
7/21/2019 11:49:30 AM

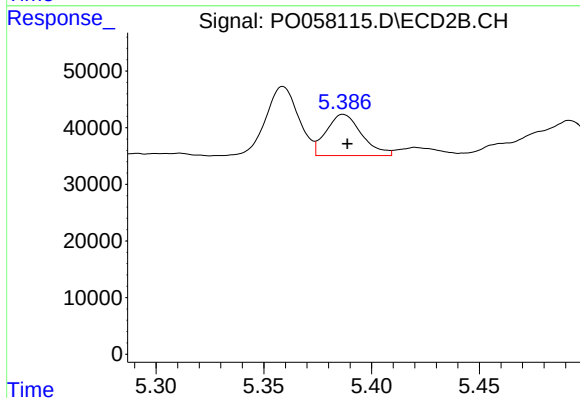


#26 AR-1254-1

R.T.: 5.387 min
Delta R.T.: -0.002 min
Response: 83435
Conc: 40.95 ng/ml

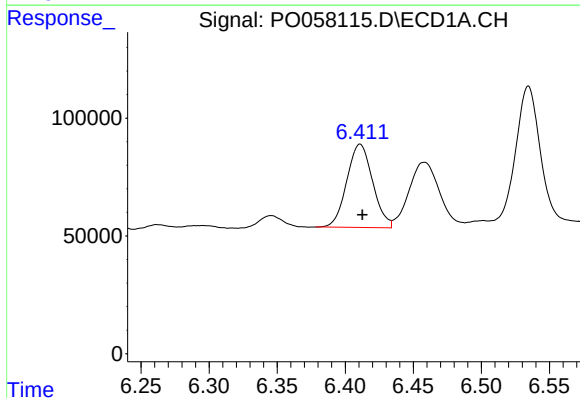


#27 AR-1254-2

R.T.: 6.411 min
Delta R.T.: -0.002 min
Response: 467474
Conc: 143.00 ng/ml m

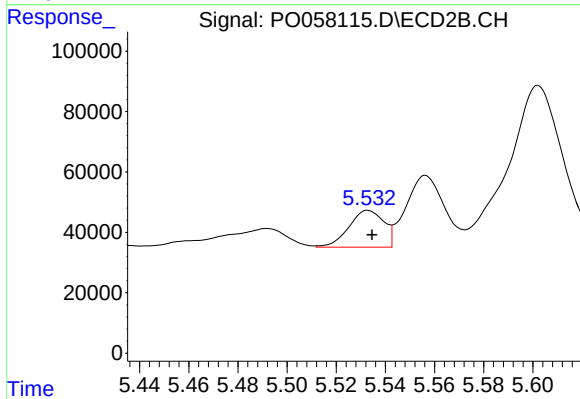

#27 AR-1254-2

R.T.: 5.533 min
Delta R.T.: -0.002 min
Response: 120632
Conc: 66.57 ng/ml

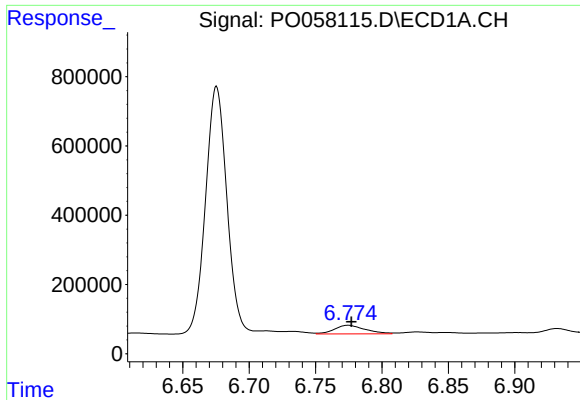


#28 AR-1254-3

R.T.: 6.774 min
Delta R.T.: -0.003 min
Response: 402695
Conc: 114.15 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S3-06-S


Manual Integrations
APPROVED

Ankita
7/21/2019 11:49:30 AM

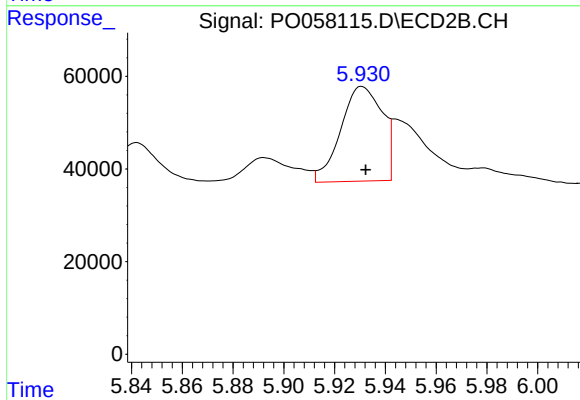


#28 AR-1254-3

R.T.: 5.930 min
Delta R.T.: -0.002 min
Response: 232160
Conc: 79.28 ng/ml m

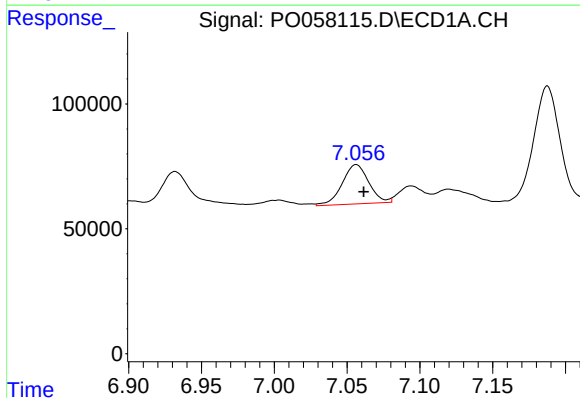


#29 AR-1254-4

R.T.: 7.056 min
Delta R.T.: -0.005 min
Response: 199867
Conc: 67.55 ng/ml m

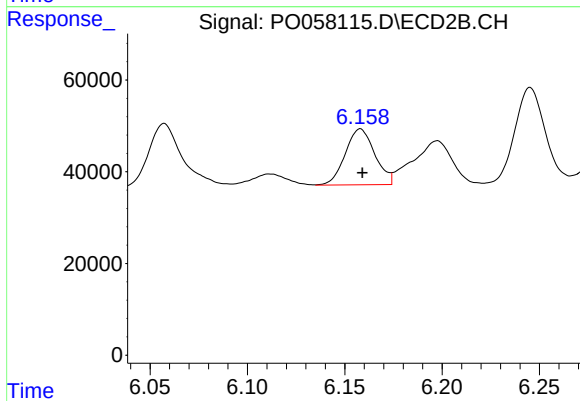

#29 AR-1254-4

R.T.: 6.158 min
Delta R.T.: -0.001 min
Response: 128739
Conc: 69.68 ng/ml

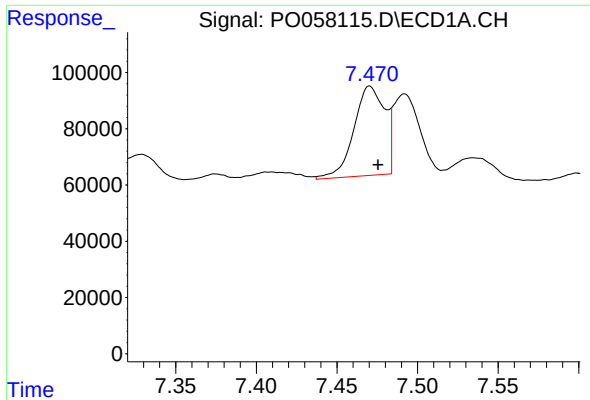


#30 AR-1254-5

R.T.: 7.470 min
Delta R.T.: -0.006 min
Response: 431182
Conc: 146.90 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S3-06-S

Manual Integrations
APPROVED

Ankita
7/21/2019 11:49:30 AM

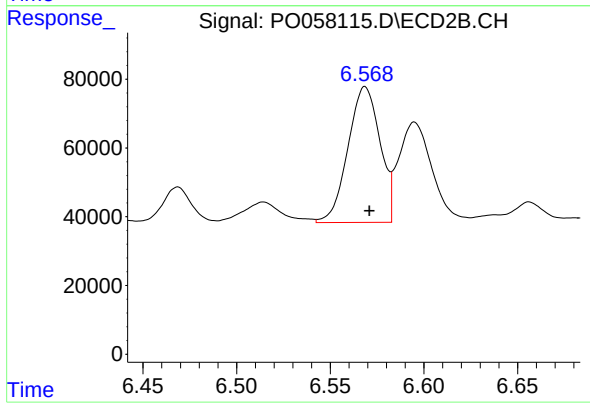

#30 AR-1254-5

R.T.: 6.569 min
Delta R.T.: -0.002 min
Response: 470313
Conc: 173.01 ng/ml