

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0071919\
 Data File : P0058120.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jul 2019 22:50
 Operator : SM/AJ
 Sample : K3889-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 S3-04-S

Manual Integrations
 APPROVED

Ankita
 7/21/2019 11:49:55 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 05:52:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.196	3.539	891547	783027	26.310	24.413
2)	SA Decachlor...	9.709	8.442	753034	519021	14.719	15.143
Target Compounds							
26)	L6 AR-1254-1	6.194	5.386	163293	152401	83.093	74.800
27)	L6 AR-1254-2	6.412	5.532	804312	195596	246.039	107.938 #
28)	L6 AR-1254-3	6.775	5.930	795288	453449	225.435	154.843m#
29)	L6 AR-1254-4	7.057	6.157	478326	251698	161.661	136.227
30)	L6 AR-1254-5	7.472	6.568	845307	869671	287.985	319.910

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071919\
Data File : P0058120.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jul 2019 22:50
Operator : SM/AJ
Sample : K3889-06
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S3-04-S


Manual Integrations
APPROVED

Ankita
7/21/2019 11:49:55 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 05:52:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

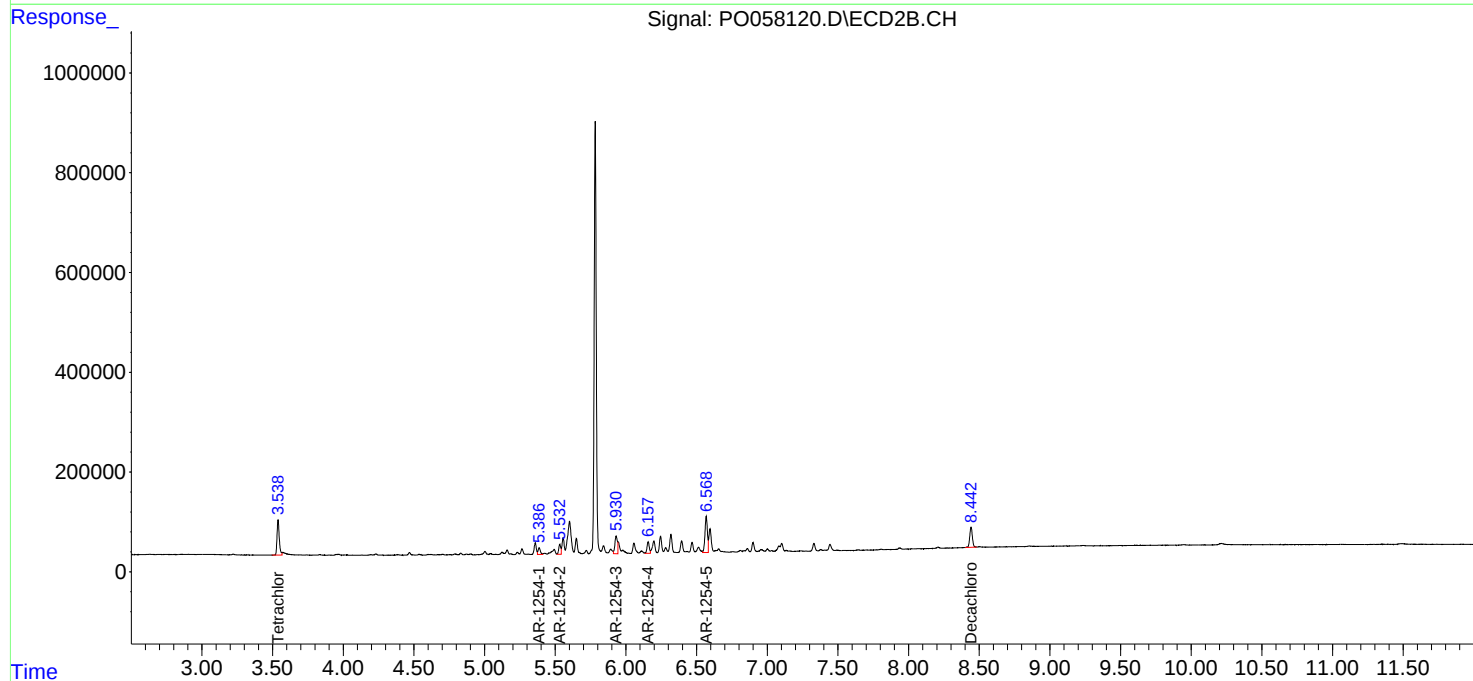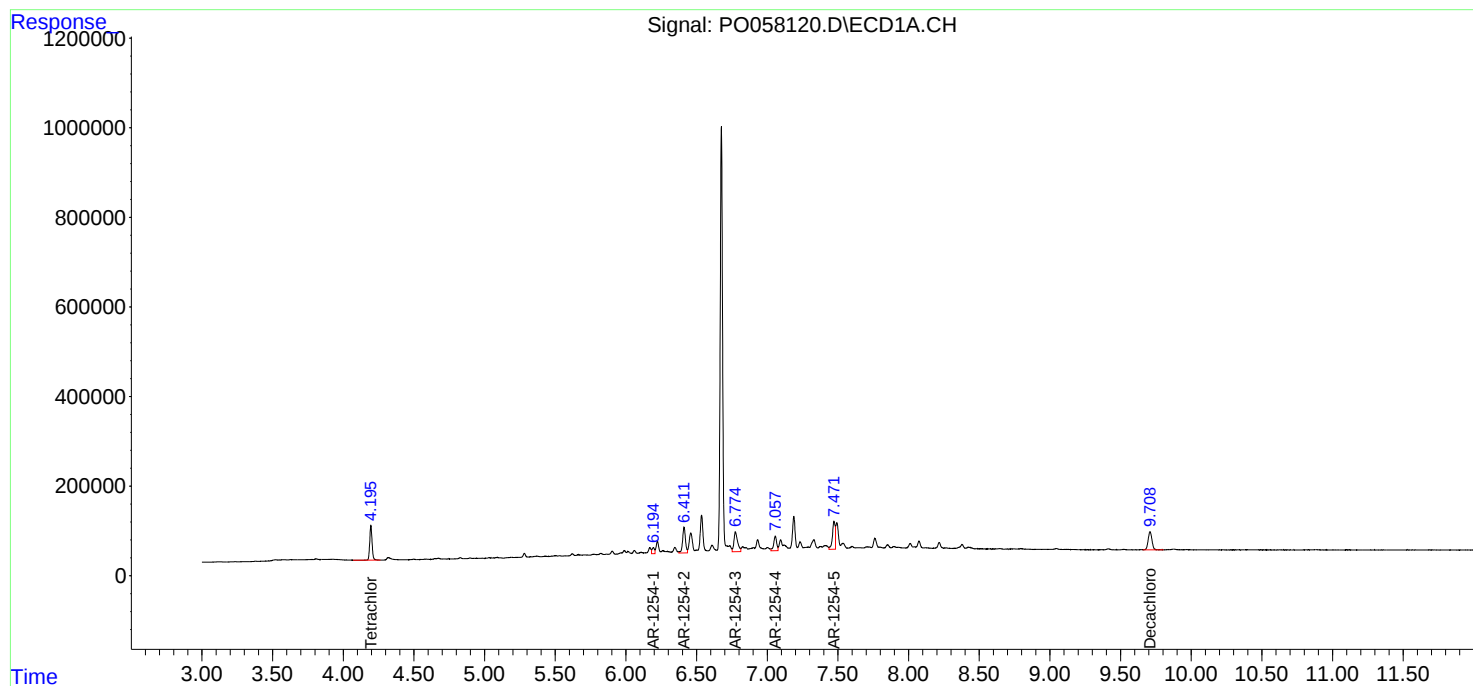

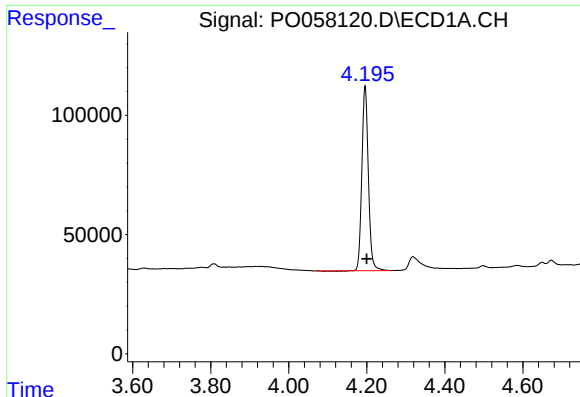


#1 Tetrachloro-m-xylene

R.T.: 4.196 min
Delta R.T.: -0.004 min
Response: 891547
Conc: 26.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
S3-04-S


Manual Integrations
APPROVED

Ankita
7/21/2019 11:49:55 AM

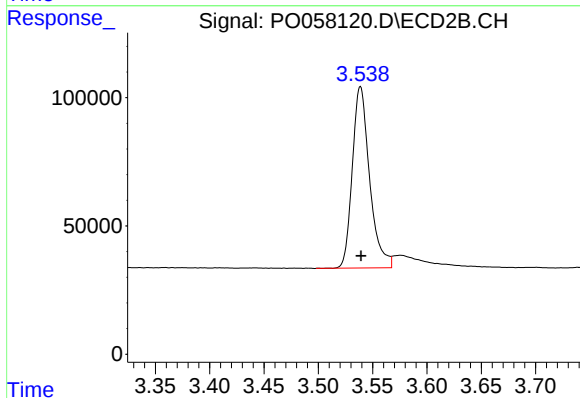


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 783027
Conc: 24.41 ng/ml

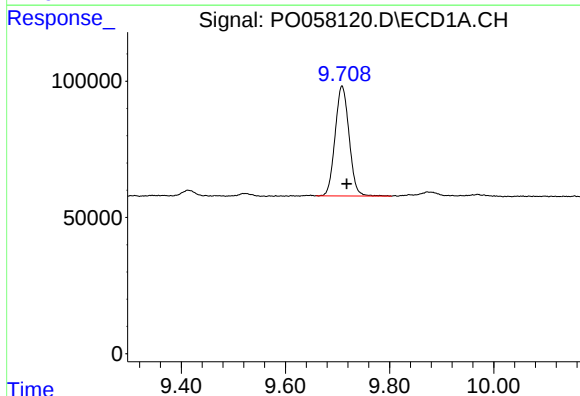


#2 Decachlorobiphenyl

R.T.: 9.709 min
Delta R.T.: -0.009 min
Response: 753034
Conc: 14.72 ng/ml

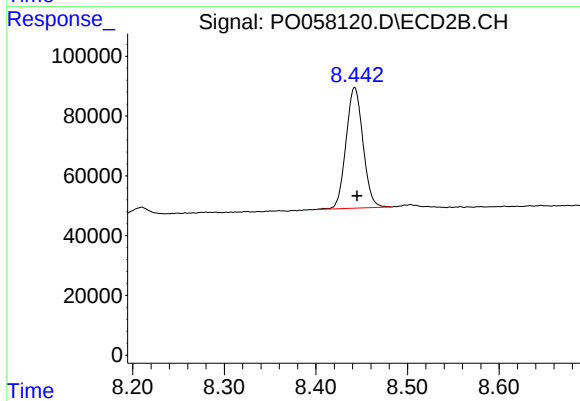

#2 Decachlorobiphenyl

R.T.: 8.442 min
Delta R.T.: -0.003 min
Response: 519021
Conc: 15.14 ng/ml

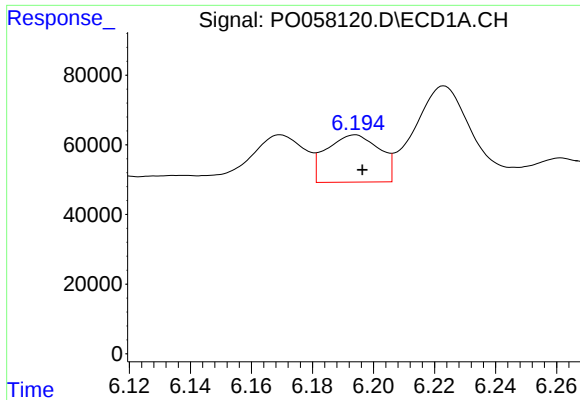


#26 AR-1254-1

R.T.: 6.194 min
Delta R.T.: -0.002 min
Response: 163293
Conc: 83.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
S3-04-S


Manual Integrations
APPROVED

Ankita
7/21/2019 11:49:55 AM

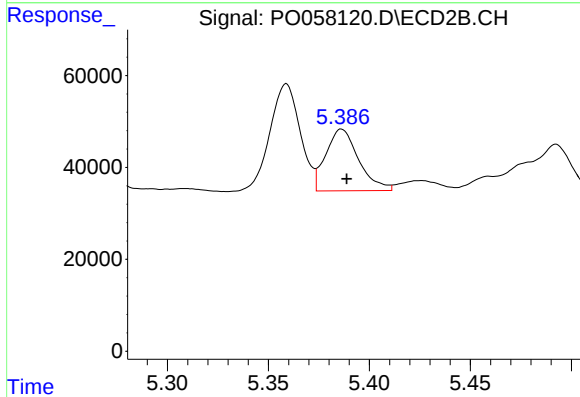


#26 AR-1254-1

R.T.: 5.386 min
Delta R.T.: -0.002 min
Response: 152401
Conc: 74.80 ng/ml

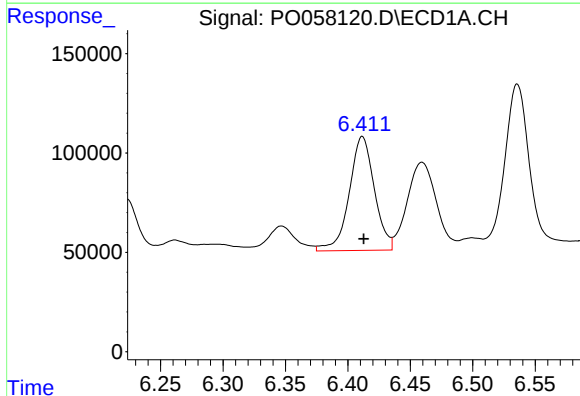


#27 AR-1254-2

R.T.: 6.412 min
Delta R.T.: -0.001 min
Response: 804312
Conc: 246.04 ng/ml

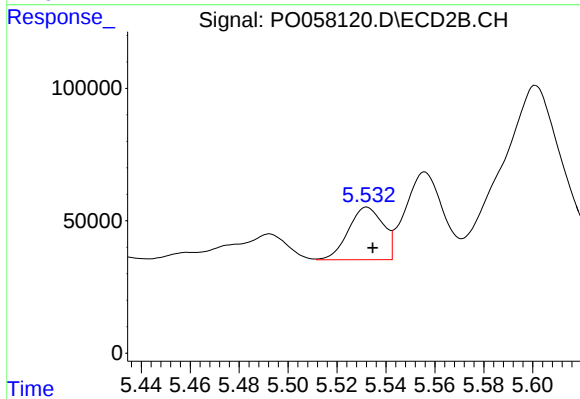

#27 AR-1254-2

R.T.: 5.532 min
Delta R.T.: -0.002 min
Response: 195596
Conc: 107.94 ng/ml

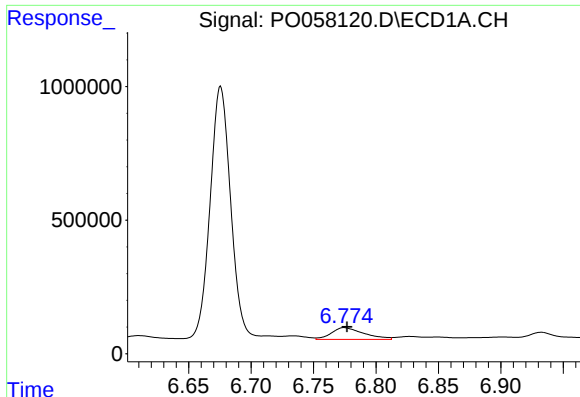


#28 AR-1254-3

R.T.: 6.775 min
Delta R.T.: -0.002 min
Response: 795288
Conc: 225.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
S3-04-S


Manual Integrations
APPROVED

Ankita
7/21/2019 11:49:55 AM

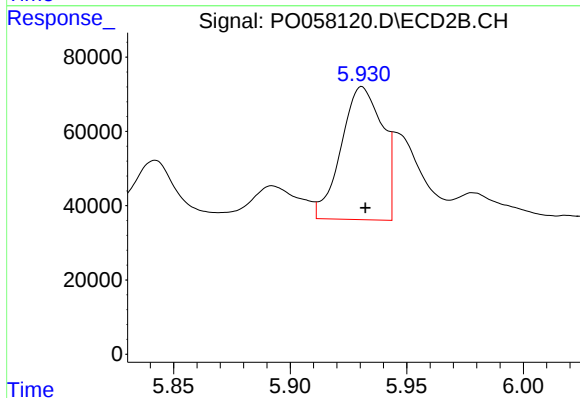


#28 AR-1254-3

R.T.: 5.930 min
Delta R.T.: -0.002 min
Response: 453449
Conc: 154.84 ng/ml m

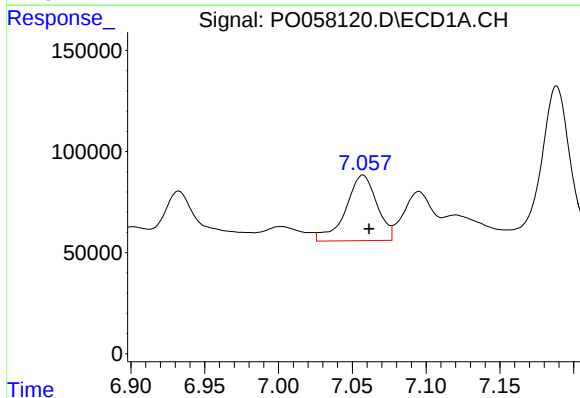


#29 AR-1254-4

R.T.: 7.057 min
Delta R.T.: -0.004 min
Response: 478326
Conc: 161.66 ng/ml

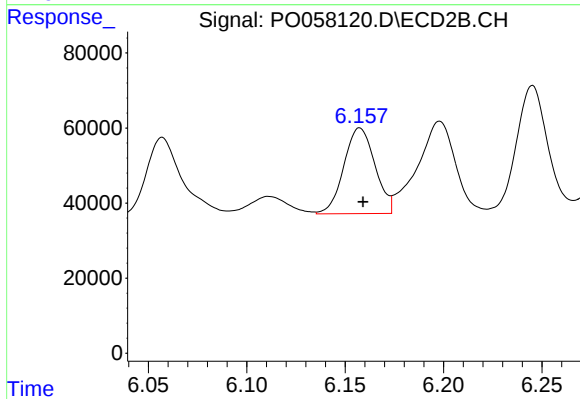

#29 AR-1254-4

R.T.: 6.157 min
Delta R.T.: -0.002 min
Response: 251698
Conc: 136.23 ng/ml

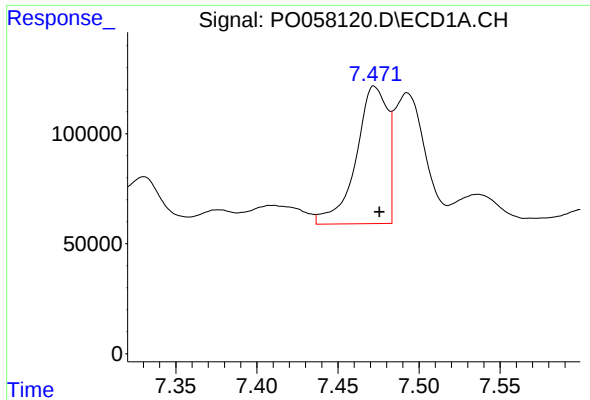


#30 AR-1254-5

R.T.: 7.472 min
Delta R.T.: -0.003 min
Response: 845307
Conc: 287.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
S3-04-S

Manual Integrations
APPROVED

Ankita
7/21/2019 11:49:55 AM

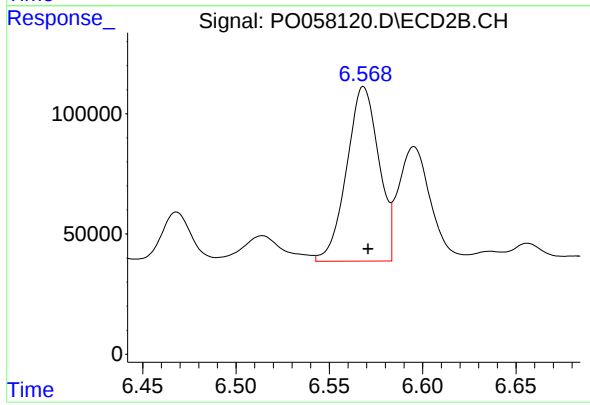

#30 AR-1254-5

R.T.: 6.568 min
Delta R.T.: -0.002 min
Response: 869671
Conc: 319.91 ng/ml