

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071919\
 Data File : P0058123.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Jul 2019 23:42
 Operator : SM/AJ
 Sample : K3894-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 K580-S6

Manual Integrations
 APPROVED

Ankita
 7/21/2019 11:49:59 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 05:54:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.197	3.539	816473	728402	24.094	22.710
2) SA Decachlor...	9.708	8.442	795941	660860	15.558m	19.281

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071919\
Data File : P0058123.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Jul 2019 23:42
Operator : SM/AJ
Sample : K3894-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
K580-S6


Manual Integrations
APPROVED

Ankita
7/21/2019 11:49:59 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 05:54:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

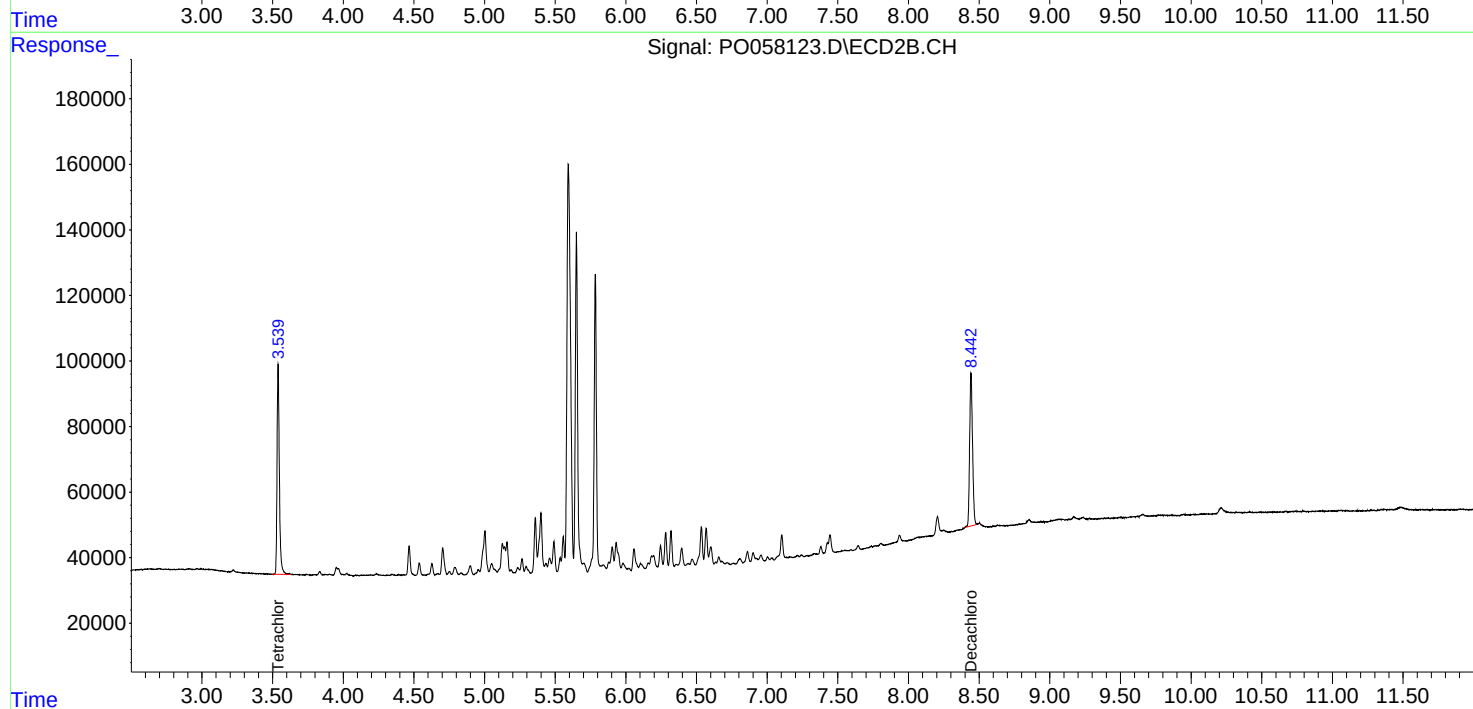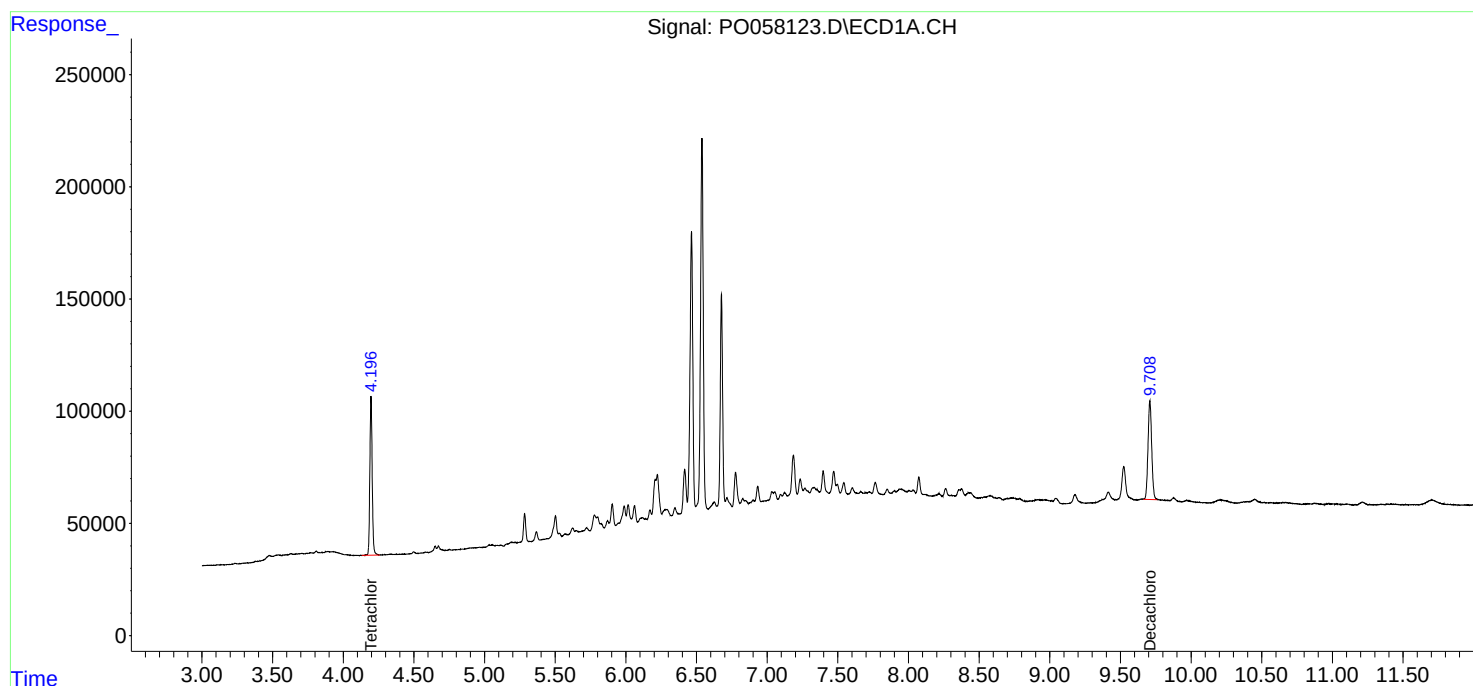

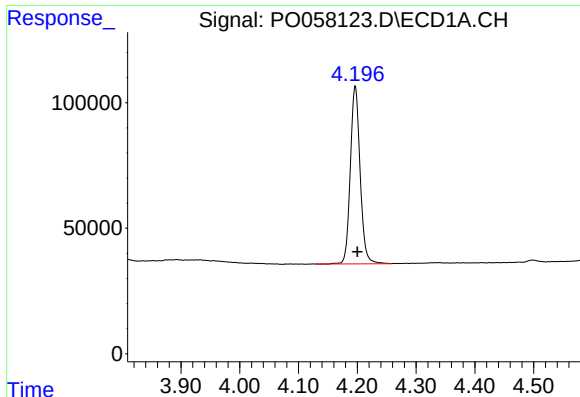


#1 Tetrachloro-m-xylene

R.T.: 4.197 min
Delta R.T.: -0.003 min
Response: 816473
Conc: 24.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
K580-S6


Manual Integrations
APPROVED

Ankita
7/21/2019 11:49:59 AM

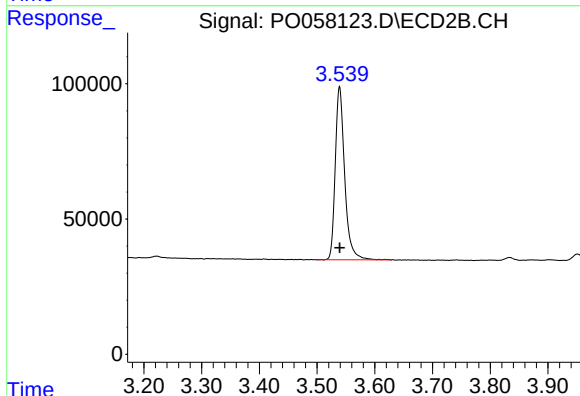


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 728402
Conc: 22.71 ng/ml

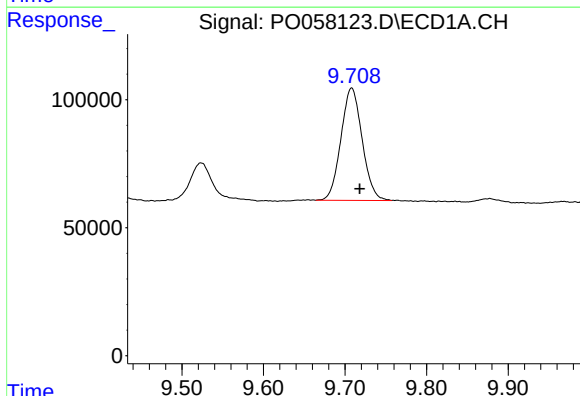

#2 Decachlorobiphenyl

R.T.: 9.708 min
Delta R.T.: -0.010 min
Response: 795941
Conc: 15.56 ng/ml m

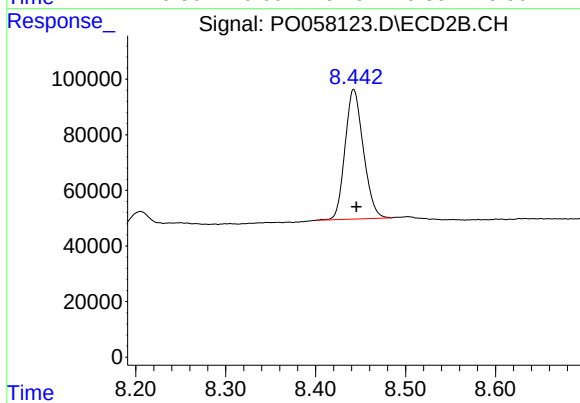

#2 Decachlorobiphenyl

R.T.: 8.442 min
Delta R.T.: -0.003 min
Response: 660860
Conc: 19.28 ng/ml