

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071919\
 Data File : P0058126.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jul 2019 00:33
 Operator : SM/AJ
 Sample : K3894-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 K580-S7

Manual Integrations
 APPROVED

Ankita
 7/21/2019 11:50:07 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 05:56:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.194	3.539	873793	787188	25.786	24.543
2) SA Decachlor...	9.706	8.444	845125	872137	16.519	25.445 #
Target Compounds						
26) L6 AR-1254-1	6.202	5.399	900636	879137	458.295m	431.489
27) L6 AR-1254-2	6.412	5.533	919867	368305	281.387m	203.245 #
28) L6 AR-1254-3	6.772	5.930	1345375	1138882	381.365m	388.904
29) L6 AR-1254-4	7.055	6.157	842942	466976	284.891m	252.742
30) L6 AR-1254-5	7.470	6.568	1611526	1371051	549.026m	504.343

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071919\
Data File : P0058126.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jul 2019 00:33
Operator : SM/AJ
Sample : K3894-02
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
K580-S7


Manual Integrations
APPROVED

Ankita
7/21/2019 11:50:07 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 05:56:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

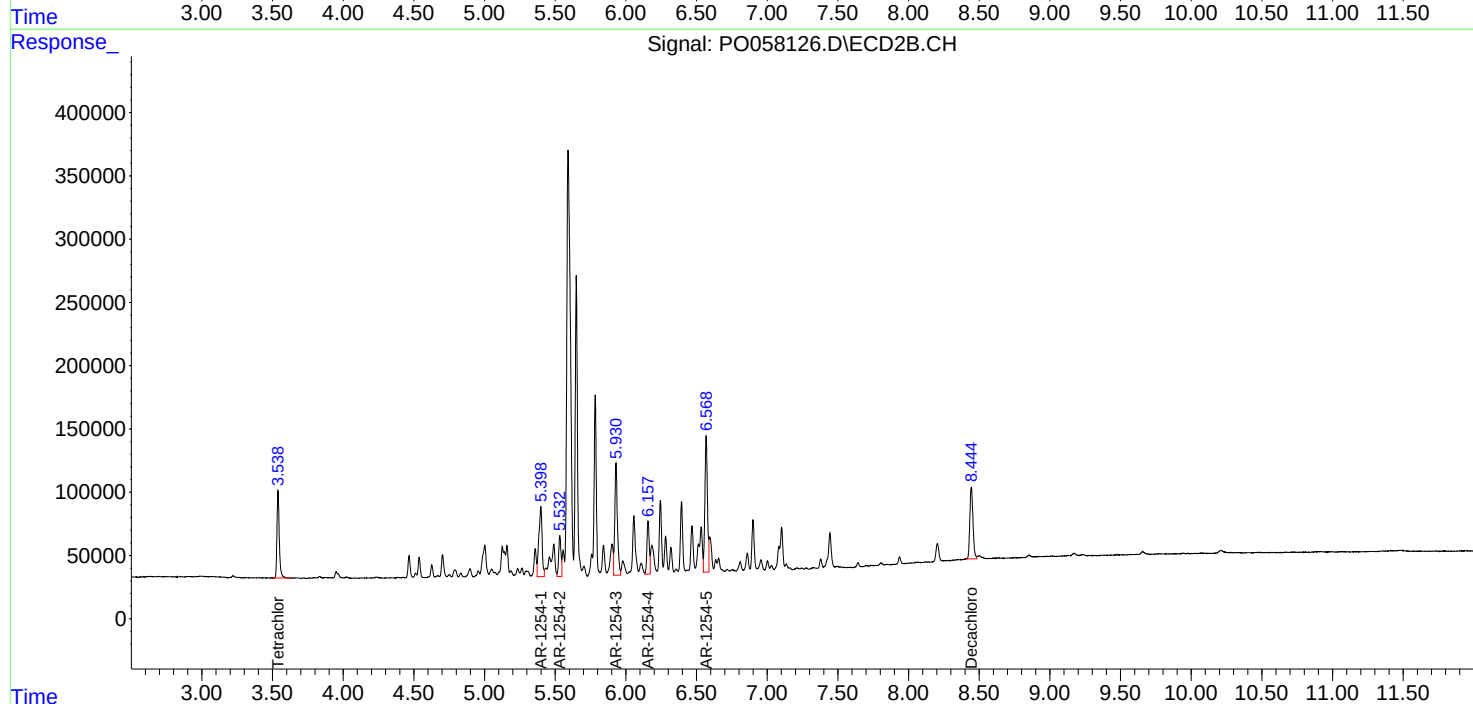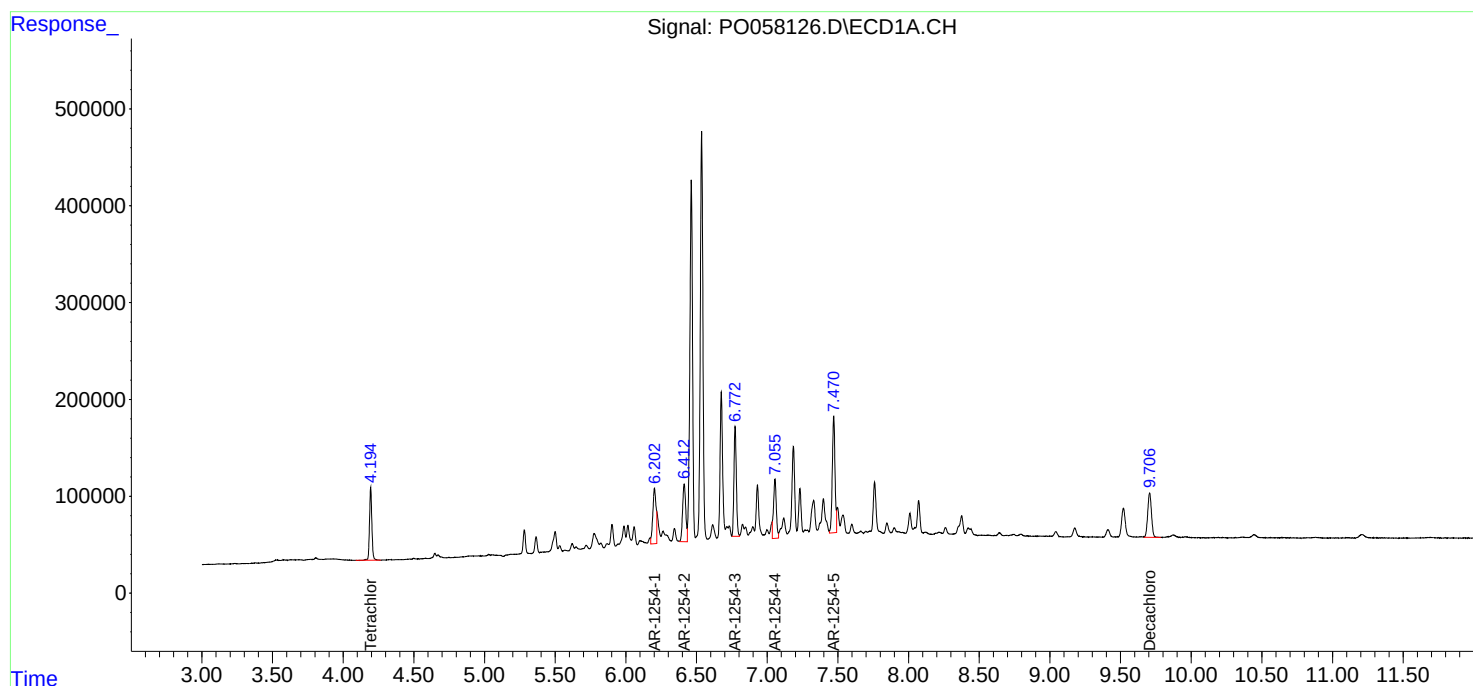

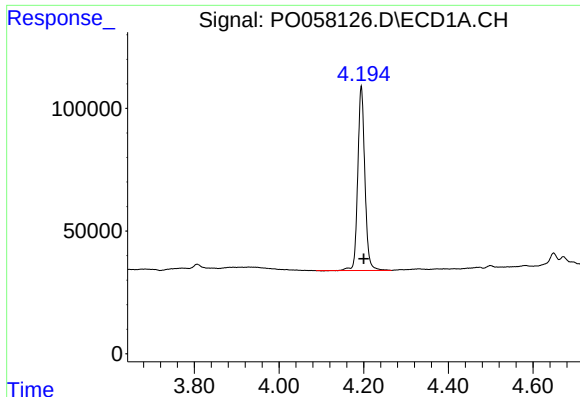


#1 Tetrachloro-m-xylene

R.T.: 4.194 min
Delta R.T.: -0.006 min
Response: 873793
Conc: 25.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
K580-S7


Manual Integrations
APPROVED

Ankita
7/21/2019 11:50:07 AM

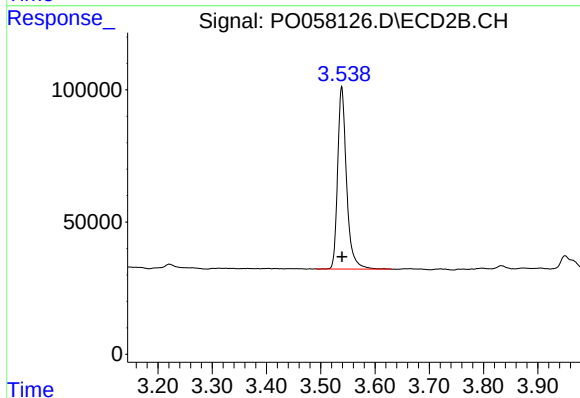


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 787188
Conc: 24.54 ng/ml

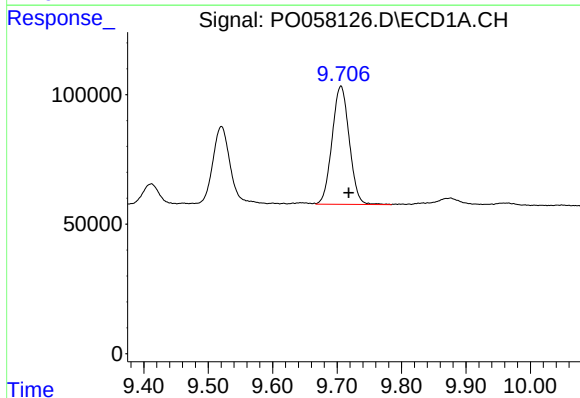


#2 Decachlorobiphenyl

R.T.: 9.706 min
Delta R.T.: -0.012 min
Response: 845125
Conc: 16.52 ng/ml

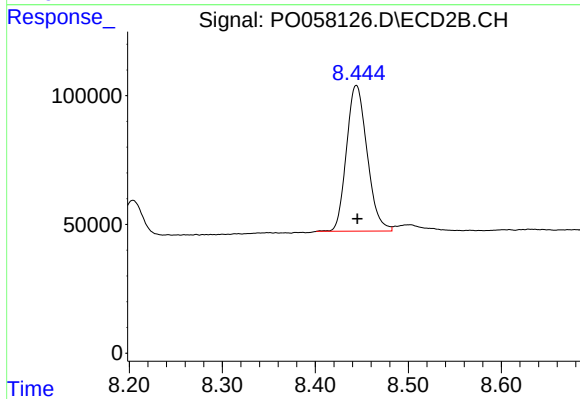

#2 Decachlorobiphenyl

R.T.: 8.444 min
Delta R.T.: -0.001 min
Response: 872137
Conc: 25.44 ng/ml

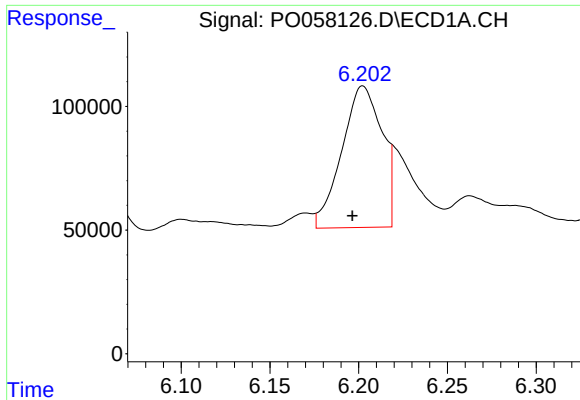


#26 AR-1254-1

R.T.: 6.202 min
Delta R.T.: 0.006 min
Response: 900636
Conc: 458.29 ng/ml m

Instrument :
ECD_O
ClientSampleId :
K580-S7


Manual Integrations
APPROVED

Ankita
7/21/2019 11:50:07 AM

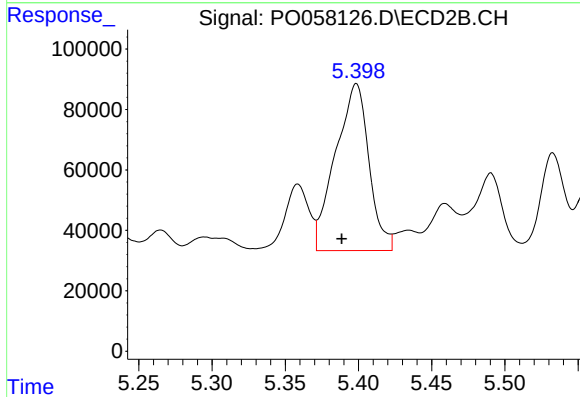


#26 AR-1254-1

R.T.: 5.399 min
Delta R.T.: 0.010 min
Response: 879137
Conc: 431.49 ng/ml

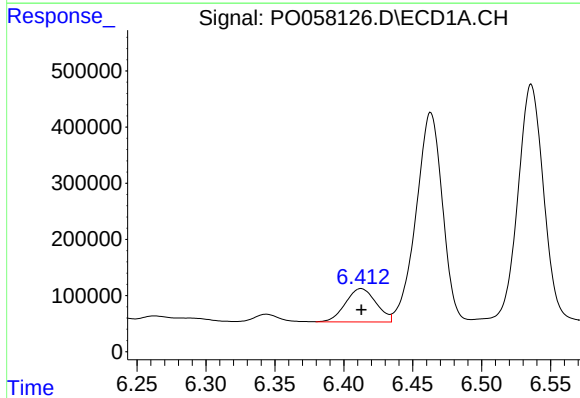


#27 AR-1254-2

R.T.: 6.412 min
Delta R.T.: 0.000 min
Response: 919867
Conc: 281.39 ng/ml m

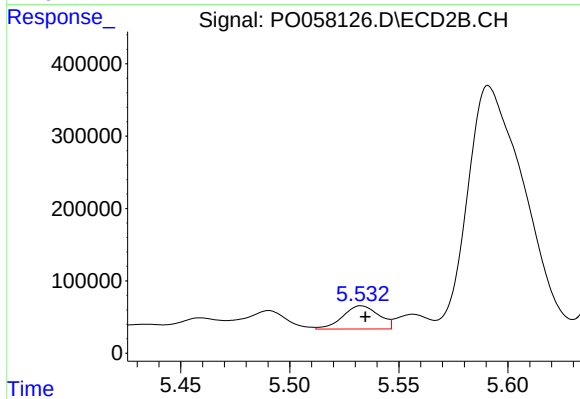

#27 AR-1254-2

R.T.: 5.533 min
Delta R.T.: -0.002 min
Response: 368305
Conc: 203.25 ng/ml

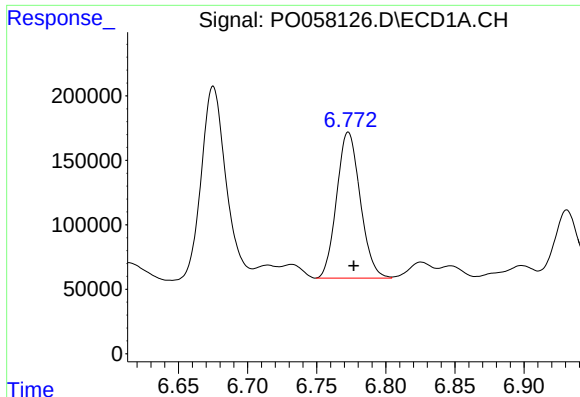


#28 AR-1254-3

R.T.: 6.772 min
Delta R.T.: -0.004 min
Response: 1345375
Conc: 381.36 ng/ml m

Instrument :
ECD_O
ClientSampleId :
K580-S7


Manual Integrations
APPROVED

Ankita
7/21/2019 11:50:07 AM

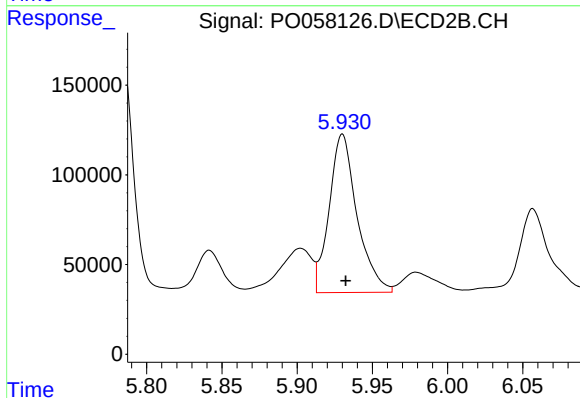


#28 AR-1254-3

R.T.: 5.930 min
Delta R.T.: -0.002 min
Response: 1138882
Conc: 388.90 ng/ml

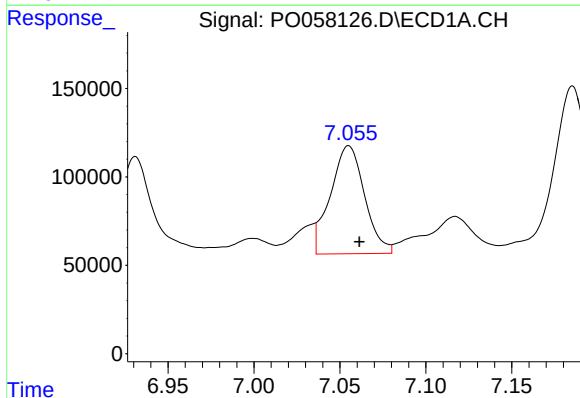


#29 AR-1254-4

R.T.: 7.055 min
Delta R.T.: -0.007 min
Response: 842942
Conc: 284.89 ng/ml m

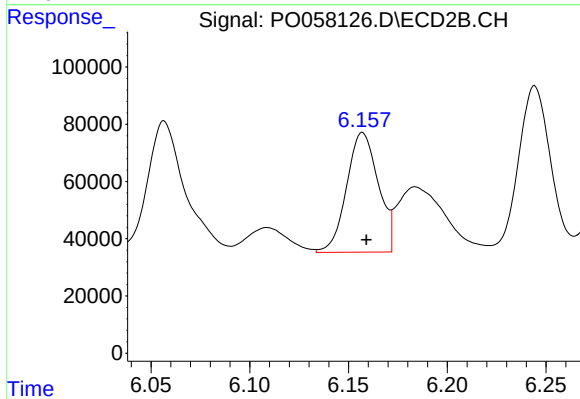

#29 AR-1254-4

R.T.: 6.157 min
Delta R.T.: -0.002 min
Response: 466976
Conc: 252.74 ng/ml

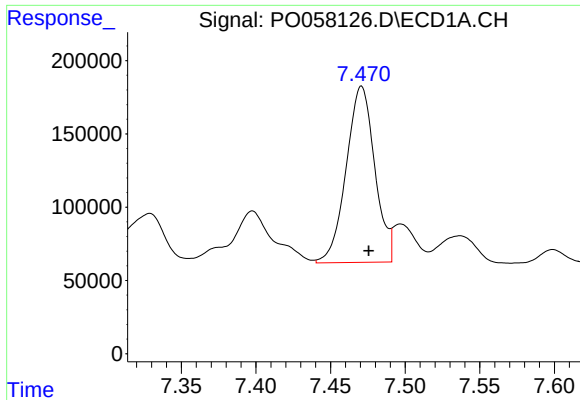


#30 AR-1254-5

R.T.: 7.470 min
Delta R.T.: -0.005 min
Response: 1611526
Conc: 549.03 ng/ml m

Instrument :
ECD_O
ClientSampleId :
K580-S7

Manual Integrations
APPROVED

Ankita
7/21/2019 11:50:07 AM

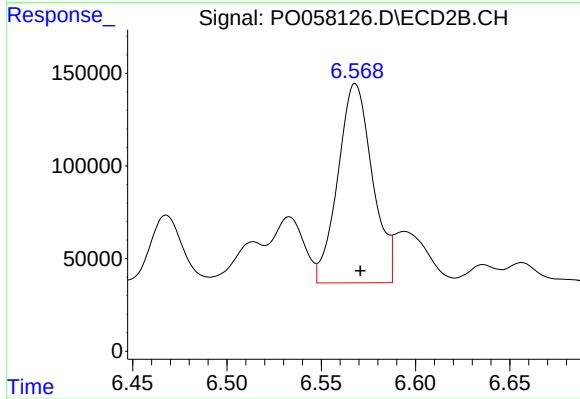

#30 AR-1254-5

R.T.: 6.568 min
Delta R.T.: -0.003 min
Response: 1371051
Conc: 504.34 ng/ml