

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071919\
 Data File : P0058130.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jul 2019 1:41
 Operator : SM/AJ
 Sample : K3894-06
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 K580-B13

Manual Integrations
 APPROVED

Ankita
 7/21/2019 11:50:36 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 05:59:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.196	3.540	962266	825335	28.396	25.733
2) SA Decachlor...	9.710	8.441	788426	556118	15.411	16.225
Target Compounds						
26) L6 AR-1254-1	6.194	5.385	39438	36224	20.068m	17.779m
27) L6 AR-1254-2	6.409	5.533	83242	39297	25.464	21.686m
28) L6 AR-1254-3	6.774	5.930	107671	93374	30.521	31.885
29) L6 AR-1254-4	7.057	6.157	79278	52867	26.794	28.613
30) L6 AR-1254-5	7.471	6.568	158802	130243	54.102	47.910

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071919\
Data File : PO058130.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jul 2019 1:41
Operator : SM/AJ
Sample : K3894-06
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
K580-B13


Manual Integrations
APPROVED

Ankita
7/21/2019 11:50:36 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 05:59:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

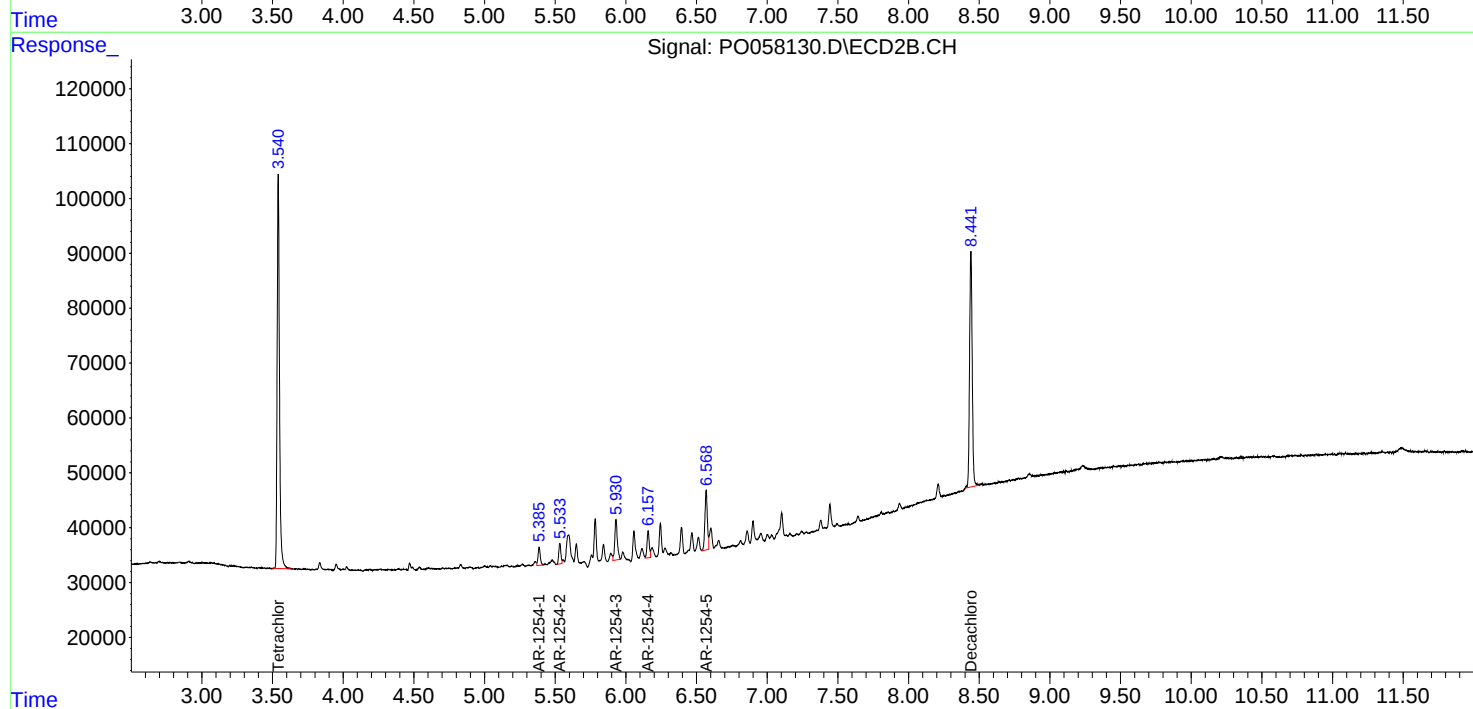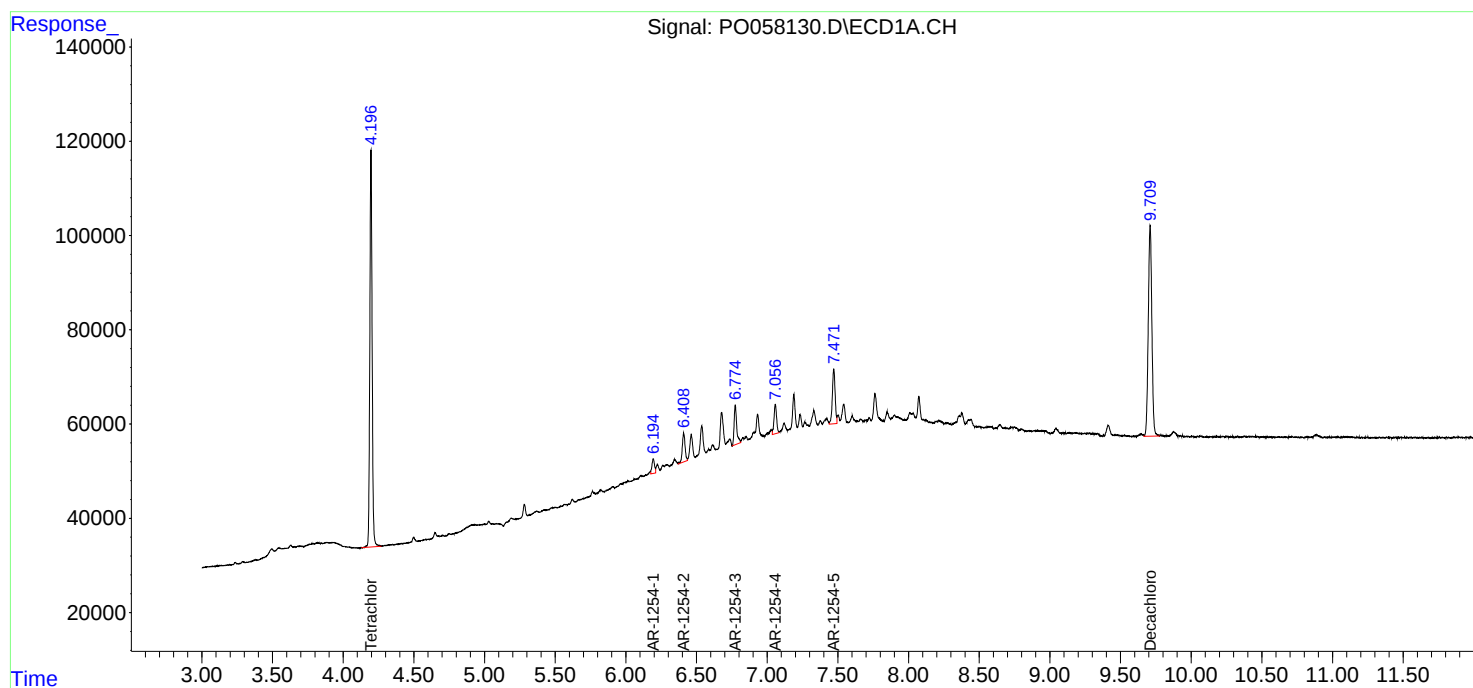

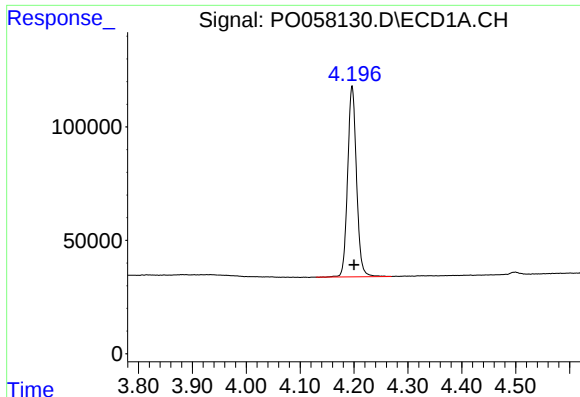


#1 Tetrachloro-m-xylene

R.T.: 4.196 min
Delta R.T.: -0.004 min
Response: 962266
Conc: 28.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
K580-B13


Manual Integrations
APPROVED

Ankita
7/21/2019 11:50:36 AM

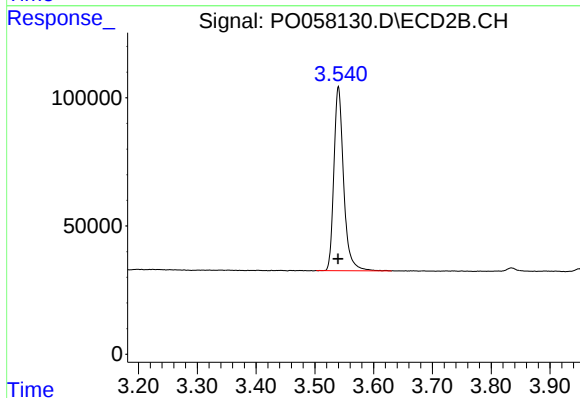


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: 0.000 min
Response: 825335
Conc: 25.73 ng/ml

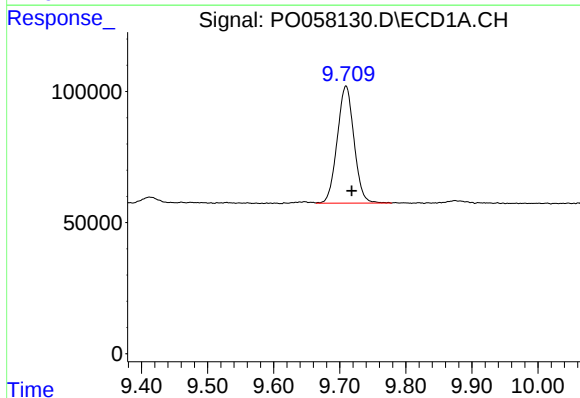


#2 Decachlorobiphenyl

R.T.: 9.710 min
Delta R.T.: -0.008 min
Response: 788426
Conc: 15.41 ng/ml

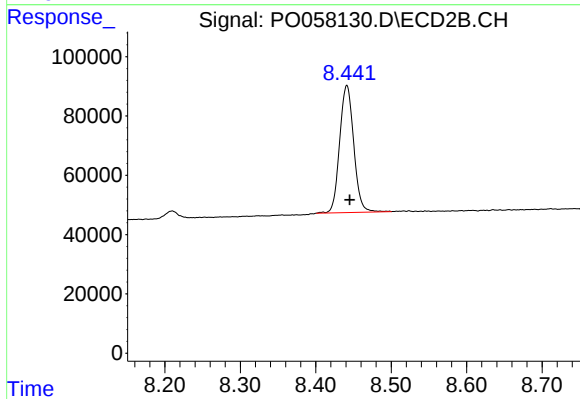

#2 Decachlorobiphenyl

R.T.: 8.441 min
Delta R.T.: -0.004 min
Response: 556118
Conc: 16.22 ng/ml

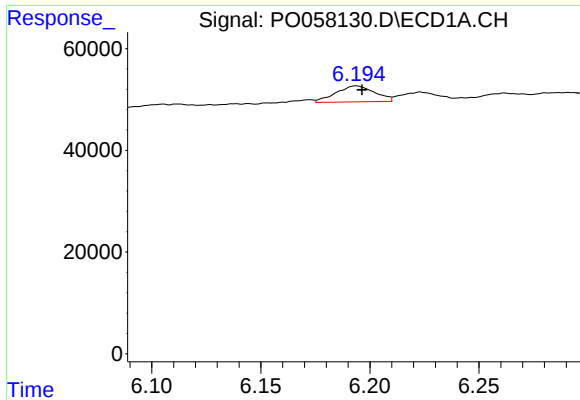


#26 AR-1254-1

R.T.: 6.194 min
Delta R.T.: -0.003 min
Response: 39438
Conc: 20.07 ng/ml m

Instrument :
ECD_O
ClientSampleId :
K580-B13


Manual Integrations
APPROVED

Ankita
7/21/2019 11:50:36 AM

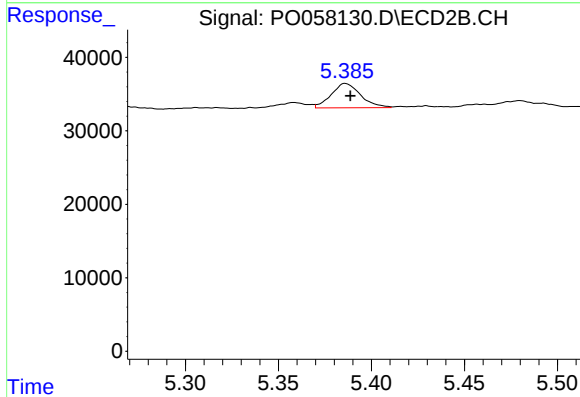


#26 AR-1254-1

R.T.: 5.385 min
Delta R.T.: -0.003 min
Response: 36224
Conc: 17.78 ng/ml m

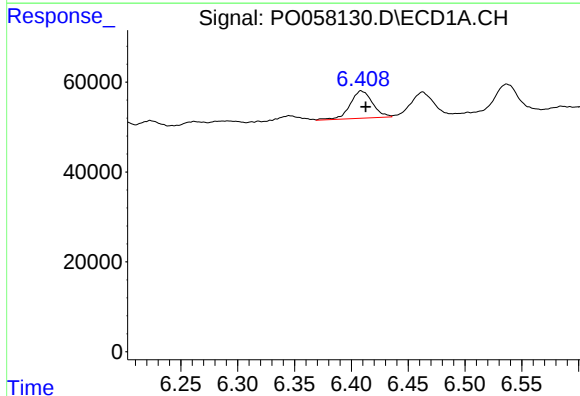


#27 AR-1254-2

R.T.: 6.409 min
Delta R.T.: -0.004 min
Response: 83242
Conc: 25.46 ng/ml

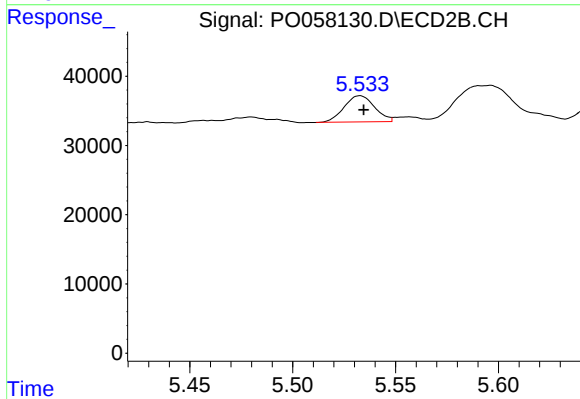

#27 AR-1254-2

R.T.: 5.533 min
Delta R.T.: -0.002 min
Response: 39297
Conc: 21.69 ng/ml m

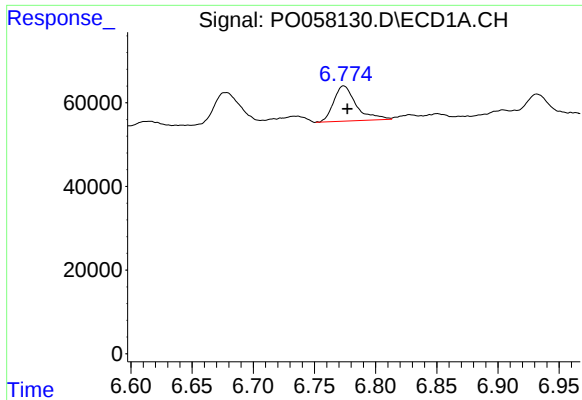


#28 AR-1254-3

R.T.: 6.774 min
Delta R.T.: -0.003 min
Response: 107671
Conc: 30.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
K580-B13


Manual Integrations
APPROVED

Ankita
7/21/2019 11:50:36 AM

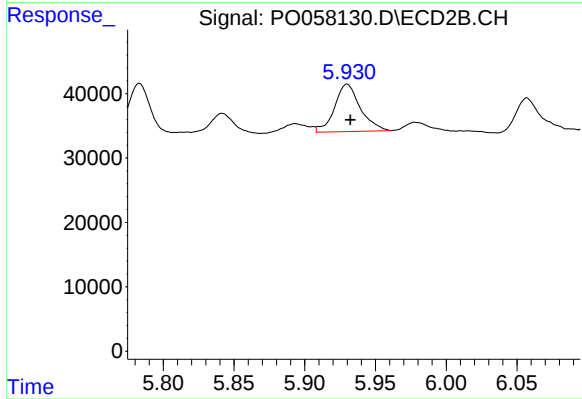


#28 AR-1254-3

R.T.: 5.930 min
Delta R.T.: -0.002 min
Response: 93374
Conc: 31.89 ng/ml

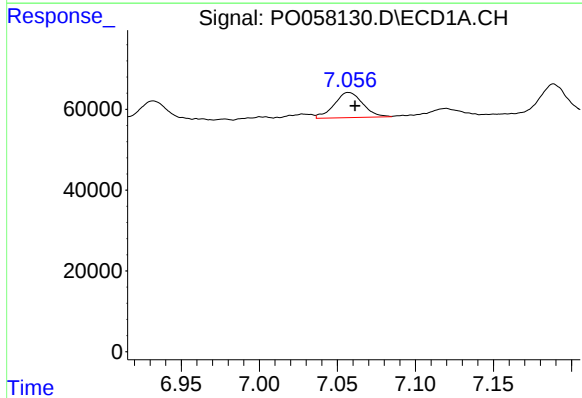


#29 AR-1254-4

R.T.: 7.057 min
Delta R.T.: -0.004 min
Response: 79278
Conc: 26.79 ng/ml

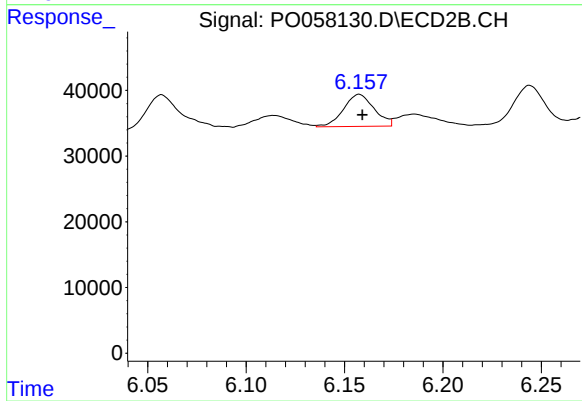

#29 AR-1254-4

R.T.: 6.157 min
Delta R.T.: -0.002 min
Response: 52867
Conc: 28.61 ng/ml

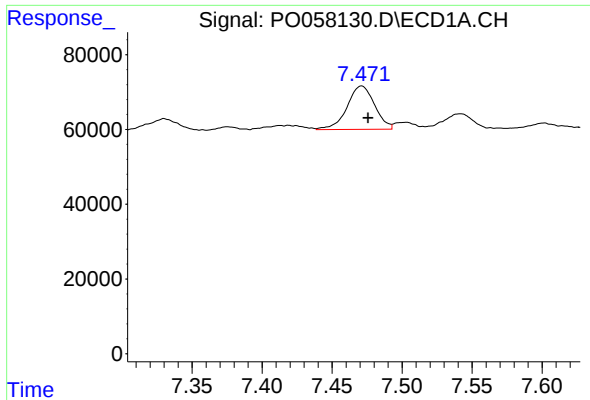


#30 AR-1254-5

R.T.: 7.471 min
Delta R.T.: -0.005 min
Response: 158802
Conc: 54.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
K580-B13

Manual Integrations
APPROVED

Ankita
7/21/2019 11:50:36 AM

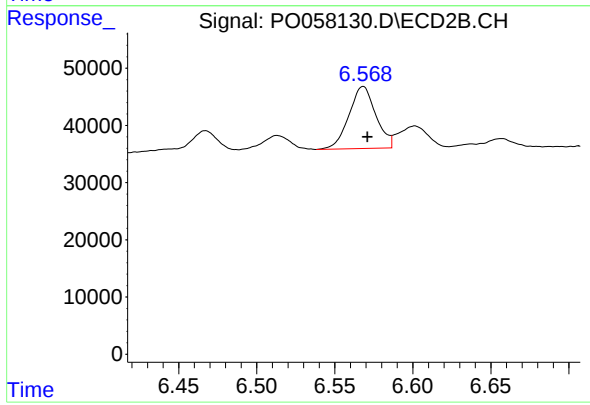

#30 AR-1254-5

R.T.: 6.568 min
Delta R.T.: -0.003 min
Response: 130243
Conc: 47.91 ng/ml