

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071919\
 Data File : P0058131.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jul 2019 1:59
 Operator : SM/AJ
 Sample : K3894-07
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 K580-B14

Manual Integrations
 APPROVED

Ankita
 7/21/2019 11:50:38 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 05:59:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.196	3.540	843923	705120	24.904	21.984
2) SA Decachlor...	9.707	8.440	736411	503313	14.394	14.684
Target Compounds						
26) L6 AR-1254-1	6.192	5.386	647071	532459	329.266m	261.336
27) L6 AR-1254-2	6.408	5.533	1090863	699979	333.695m	386.277
28) L6 AR-1254-3	6.772	5.930	2324911	2038594	659.027m	696.137
29) L6 AR-1254-4	7.055	6.157	815877	437146	275.744m	236.597
30) L6 AR-1254-5	7.470	6.568	2715673	2277791	925.194m	837.888

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071919\
Data File : P0058131.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jul 2019 1:59
Operator : SM/AJ
Sample : K3894-07
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
K580-B14


Manual Integrations
APPROVED

Ankita
7/21/2019 11:50:38 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 05:59:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

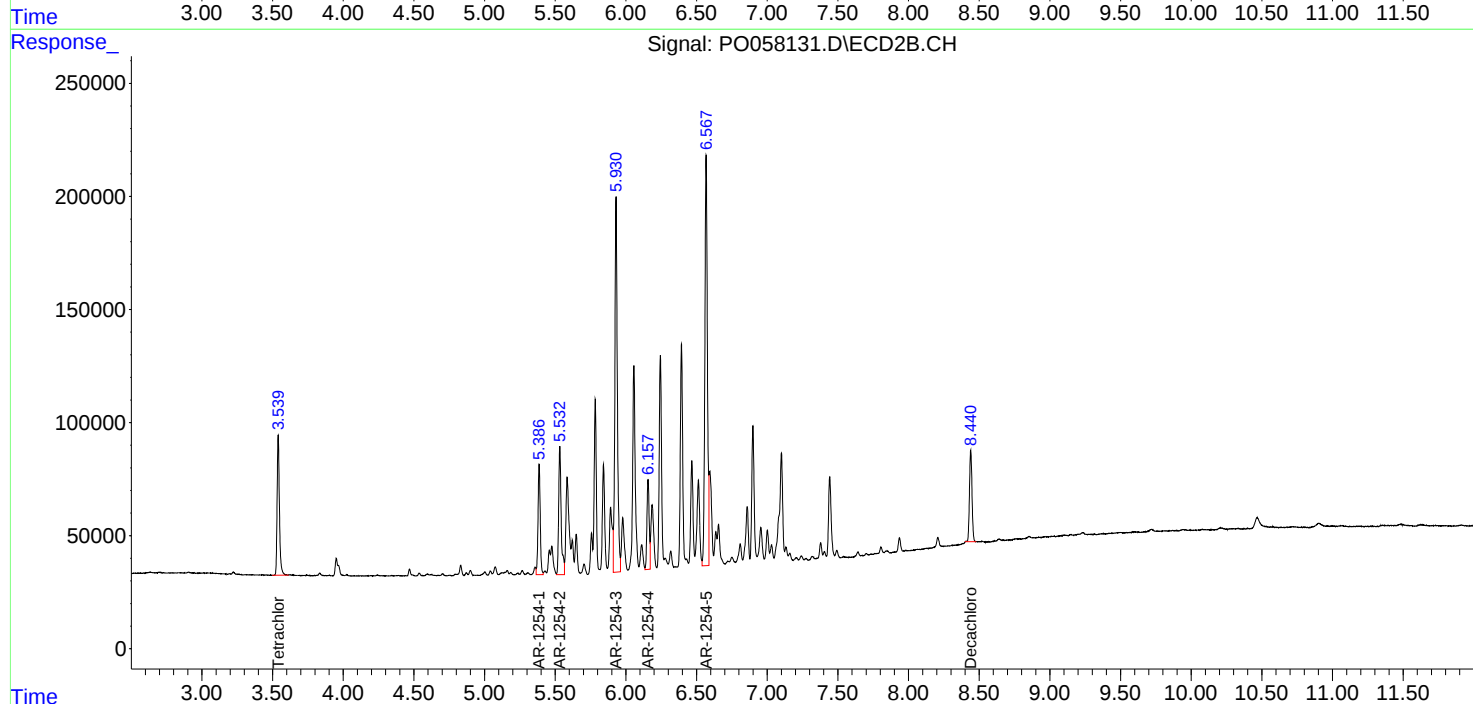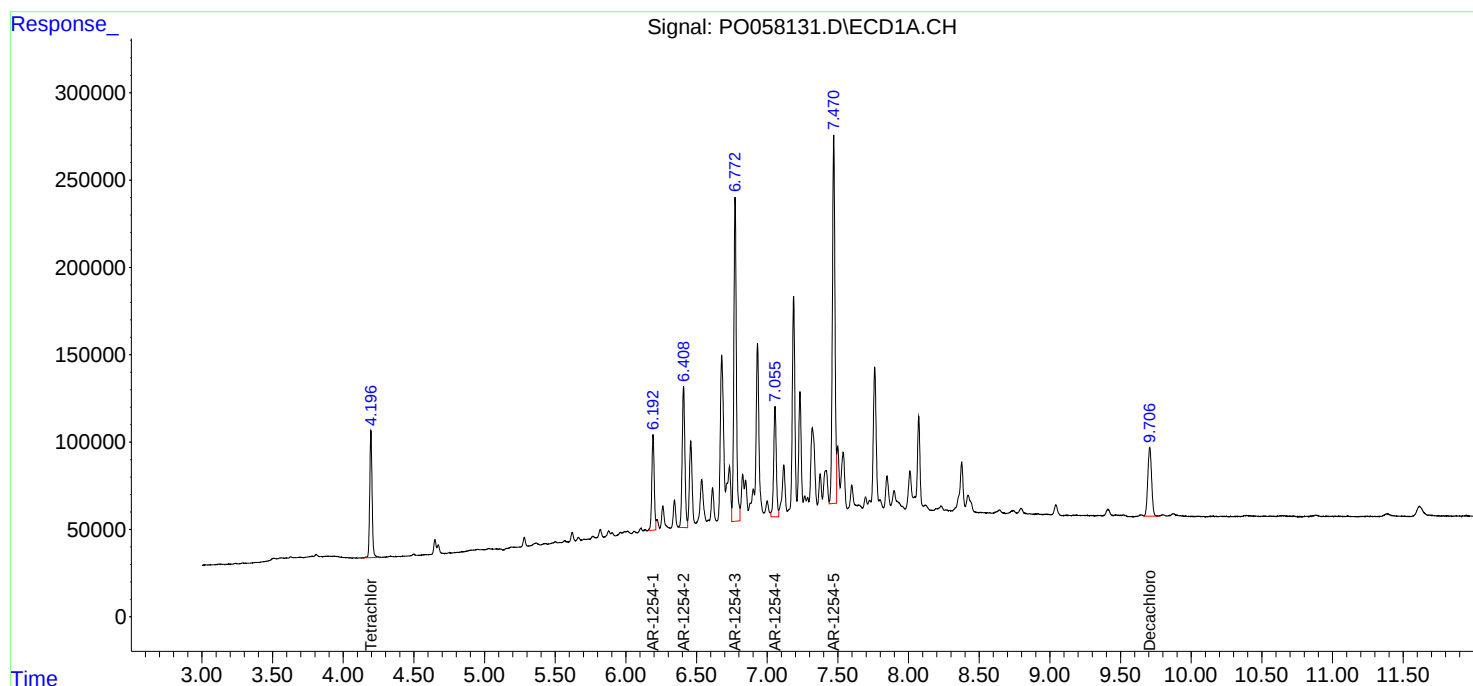

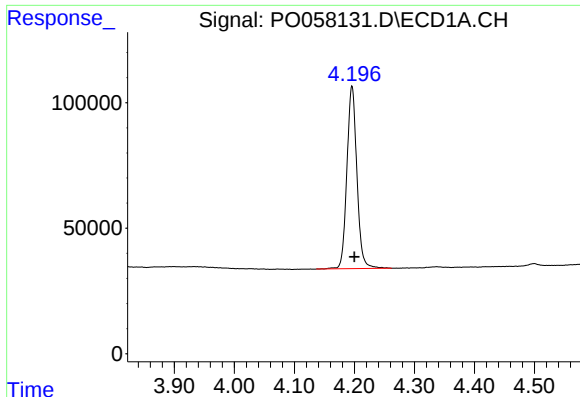


#1 Tetrachloro-m-xylene

R.T.: 4.196 min
Delta R.T.: -0.004 min
Response: 843923
Conc: 24.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
K580-B14


Manual Integrations
APPROVED

Ankita
7/21/2019 11:50:38 AM

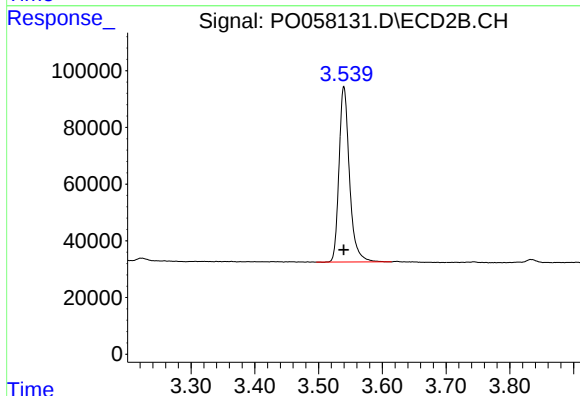


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: 0.000 min
Response: 705120
Conc: 21.98 ng/ml

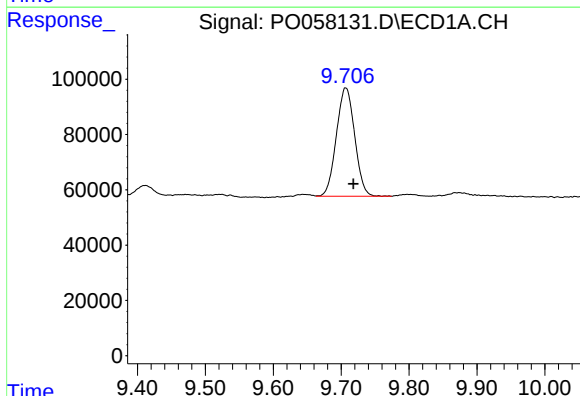


#2 Decachlorobiphenyl

R.T.: 9.707 min
Delta R.T.: -0.011 min
Response: 736411
Conc: 14.39 ng/ml

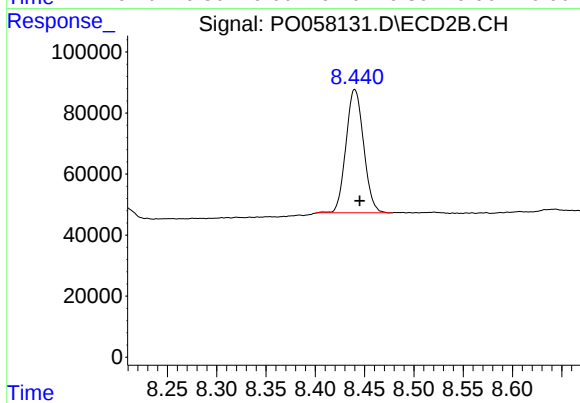

#2 Decachlorobiphenyl

R.T.: 8.440 min
Delta R.T.: -0.005 min
Response: 503313
Conc: 14.68 ng/ml

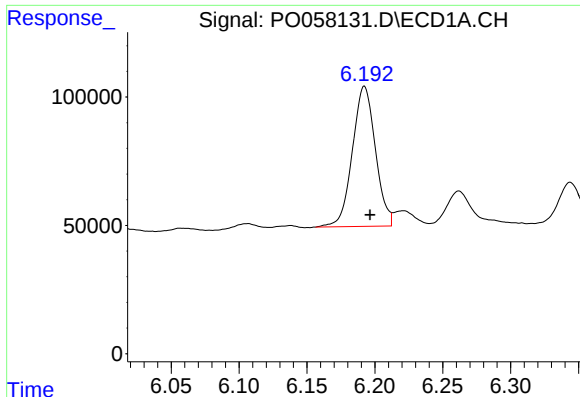


#26 AR-1254-1

R.T.: 6.192 min
Delta R.T.: -0.004 min
Response: 647071
Conc: 329.27 ng/ml m

Instrument :
ECD_O
ClientSampleId :
K580-B14


Manual Integrations
APPROVED

Ankita
7/21/2019 11:50:38 AM

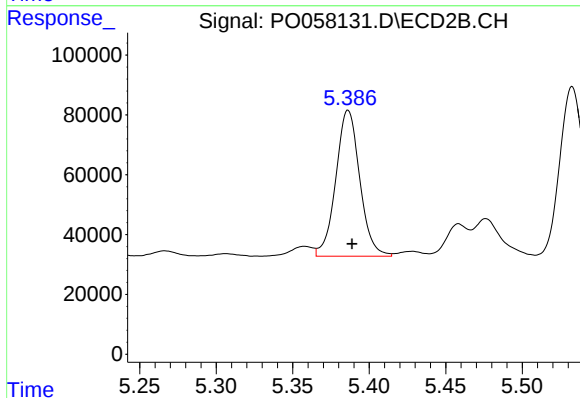


#26 AR-1254-1

R.T.: 5.386 min
Delta R.T.: -0.003 min
Response: 532459
Conc: 261.34 ng/ml

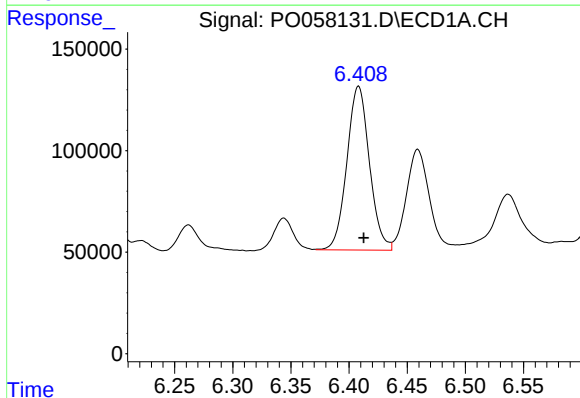


#27 AR-1254-2

R.T.: 6.408 min
Delta R.T.: -0.005 min
Response: 1090863
Conc: 333.70 ng/ml m

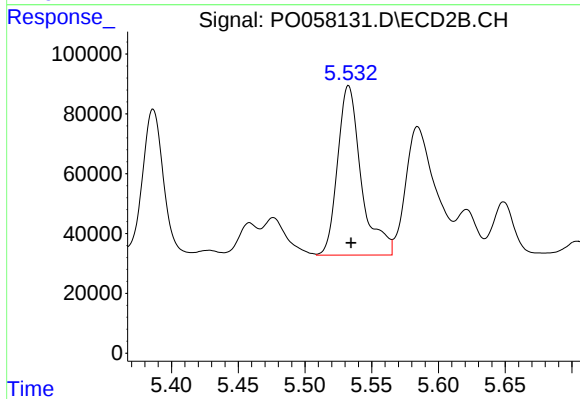

#27 AR-1254-2

R.T.: 5.533 min
Delta R.T.: -0.002 min
Response: 699979
Conc: 386.28 ng/ml

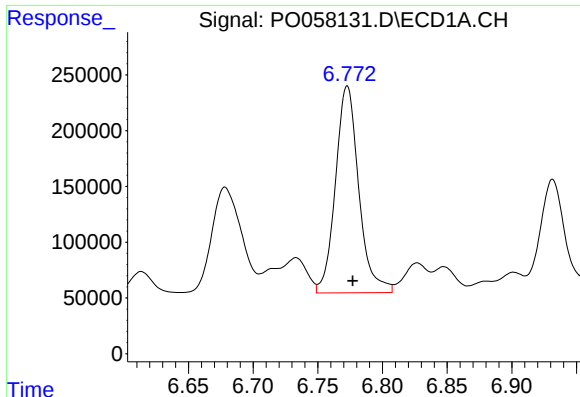


#28 AR-1254-3

R.T.: 6.772 min
Delta R.T.: -0.004 min
Response: 2324911
Conc: 659.03 ng/ml m

Instrument :
ECD_O
ClientSampleId :
K580-B14


Manual Integrations
APPROVED

Ankita
7/21/2019 11:50:38 AM

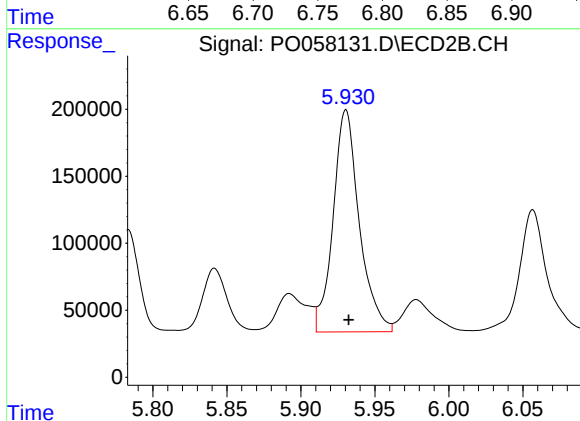


#28 AR-1254-3

R.T.: 5.930 min
Delta R.T.: -0.002 min
Response: 2038594
Conc: 696.14 ng/ml

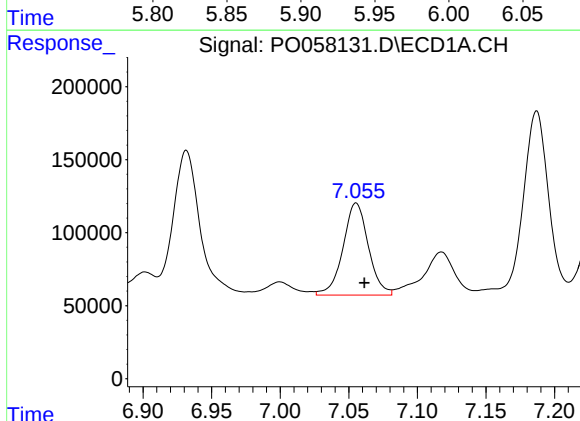


#29 AR-1254-4

R.T.: 7.055 min
Delta R.T.: -0.006 min
Response: 815877
Conc: 275.74 ng/ml m

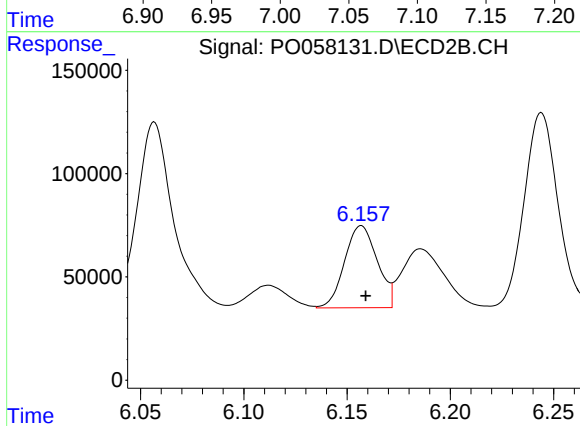

#29 AR-1254-4

R.T.: 6.157 min
Delta R.T.: -0.002 min
Response: 437146
Conc: 236.60 ng/ml

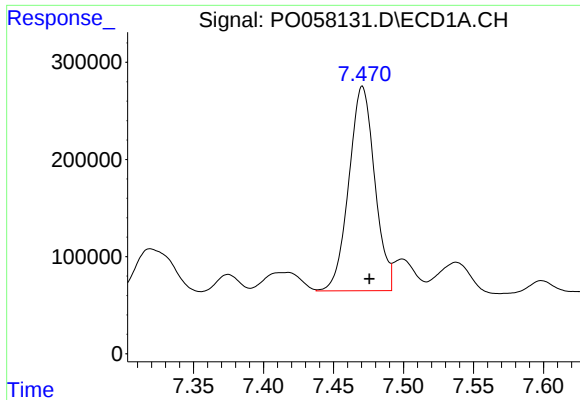


#30 AR-1254-5

R.T.: 7.470 min
Delta R.T.: -0.005 min
Response: 2715673
Conc: 925.19 ng/ml m

Instrument :
ECD_O
ClientSampleId :
K580-B14

Manual Integrations
APPROVED

Ankita
7/21/2019 11:50:38 AM

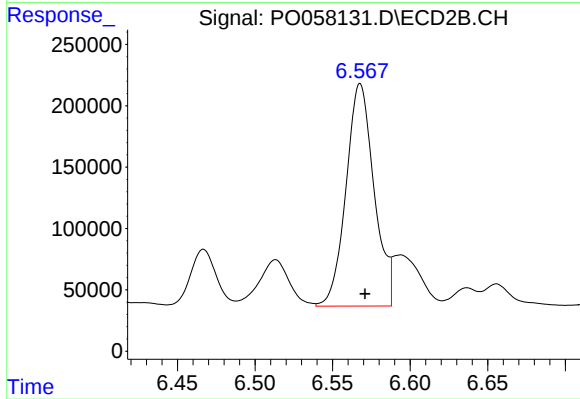

#30 AR-1254-5

R.T.: 6.568 min
Delta R.T.: -0.003 min
Response: 2277791
Conc: 837.89 ng/ml