

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071922\
 Data File : P0088182.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jul 2022 06:09
 Operator : YP/AJ
 Sample : N3763-01
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TRE-1279-SLUDGE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 06:25:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 15 03:57:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.446	3.604	31280996	12089540	12.261	12.814
2) SA Decachlor...	10.293	8.605	25416790	12784988	11.968	12.234
Target Compounds						
26) L6 AR-1254-1	6.486	5.485	4219673	1771195	44.505	30.721m#
27) L6 AR-1254-2	6.703	5.633	7718343	1762217	53.764	34.368 #
28) L6 AR-1254-3	7.071	6.038	6719197	4407838	45.872m	54.317
29) L6 AR-1254-4	7.357	6.264	9865623	2907557	91.156	58.298 #
30) L6 AR-1254-5	7.779	6.682	8621000	4847978	71.631	64.190



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071922\
Data File : P0088182.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jul 2022 06:09
Operator : YP/AJ
Sample : N3763-01
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TRE-1279-SLUDGE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 06:25:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071422.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 15 03:57:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

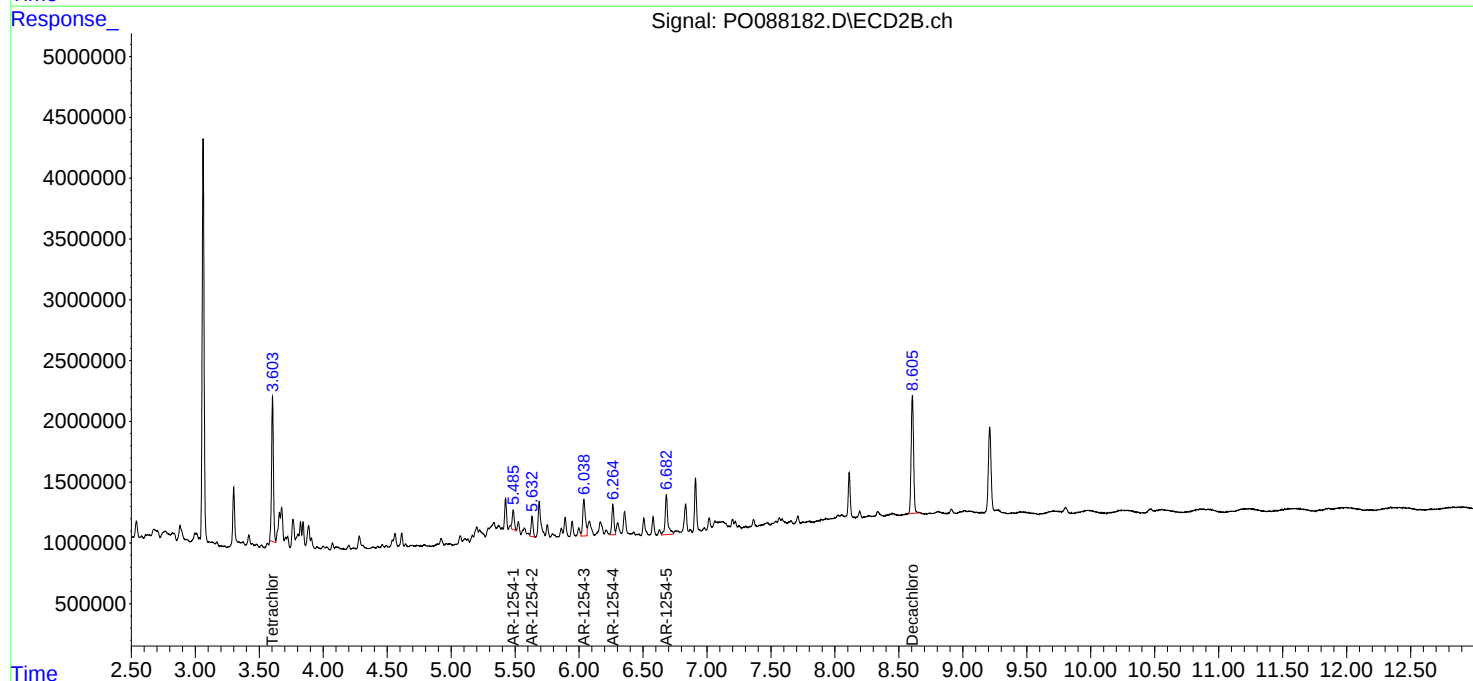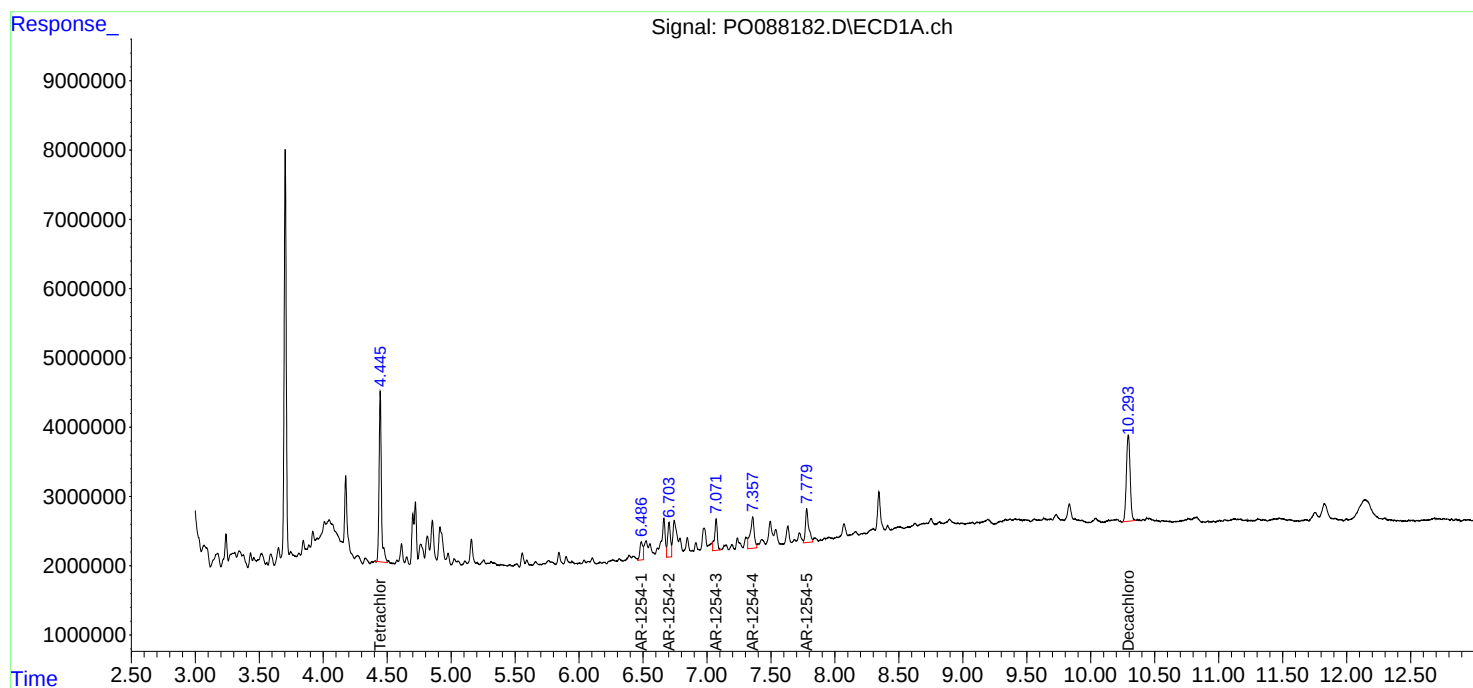


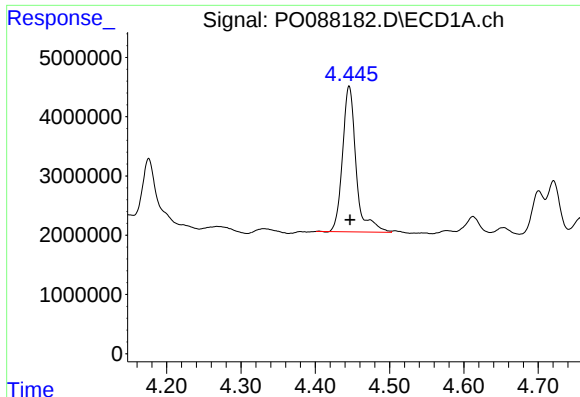

#1 Tetrachloro-m-xylene


R.T.: 4.446 min
Delta R.T.: -0.001 min
Response: 31280996
Conc: 12.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
TRE-1279-SLUDGE

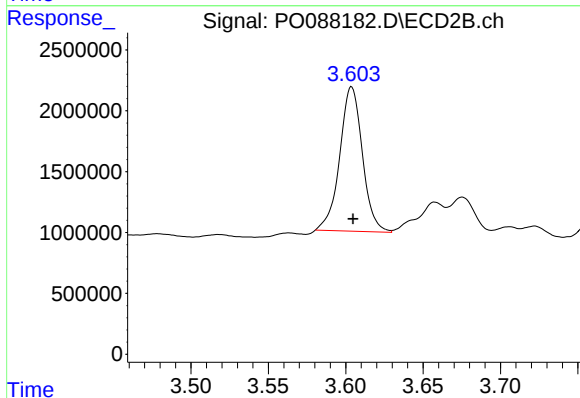


#1 Tetrachloro-m-xylene

R.T.: 3.604 min
Delta R.T.: 0.000 min
Response: 12089540
Conc: 12.81 ng/ml

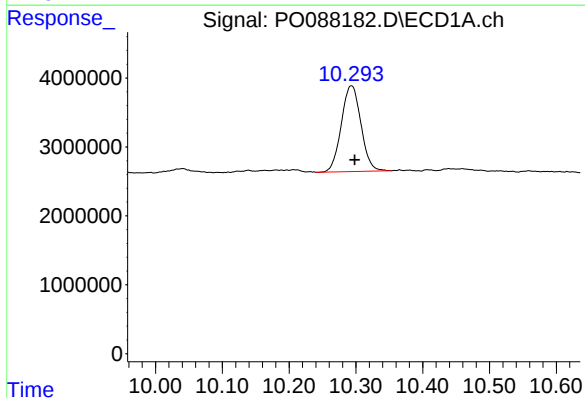


#2 Decachlorobiphenyl

R.T.: 10.293 min
Delta R.T.: -0.005 min
Response: 25416790
Conc: 11.97 ng/ml

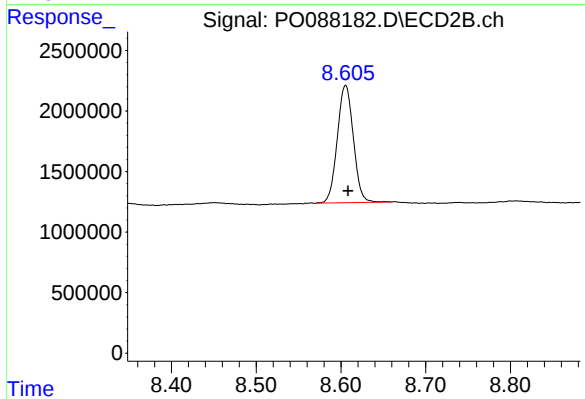

#2 Decachlorobiphenyl


R.T.: 8.605 min
Delta R.T.: -0.003 min
Response: 12784988
Conc: 12.23 ng/ml

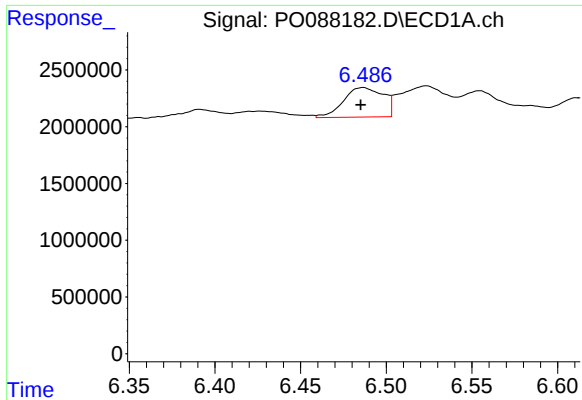

#26 AR-1254-1


R.T.: 6.486 min
Delta R.T.: 0.001 min
Response: 4219673
Conc: 44.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
TRE-1279-SLUDGE

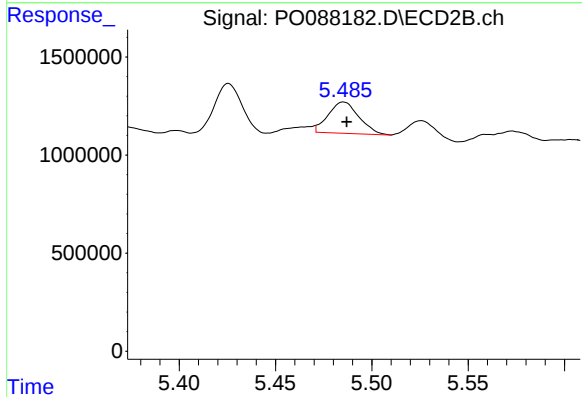


#26 AR-1254-1

R.T.: 5.485 min
Delta R.T.: -0.002 min
Response: 1771195
Conc: 30.72 ng/ml m

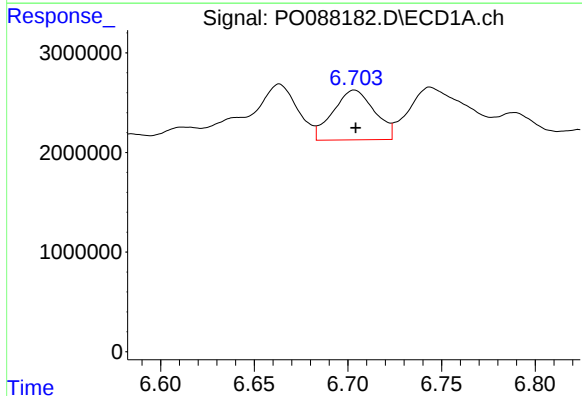


#27 AR-1254-2

R.T.: 6.703 min
Delta R.T.: 0.000 min
Response: 7718343
Conc: 53.76 ng/ml

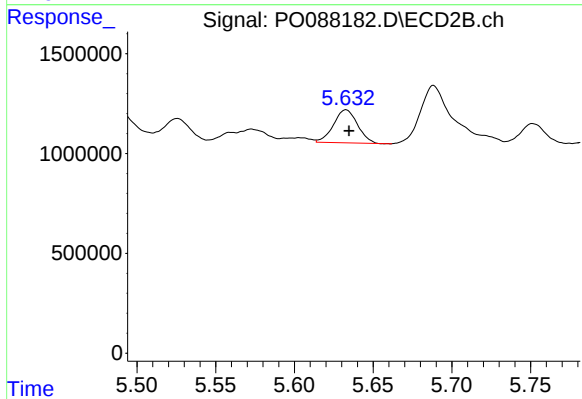

#27 AR-1254-2


R.T.: 5.633 min
Delta R.T.: -0.002 min
Response: 1762217
Conc: 34.37 ng/ml

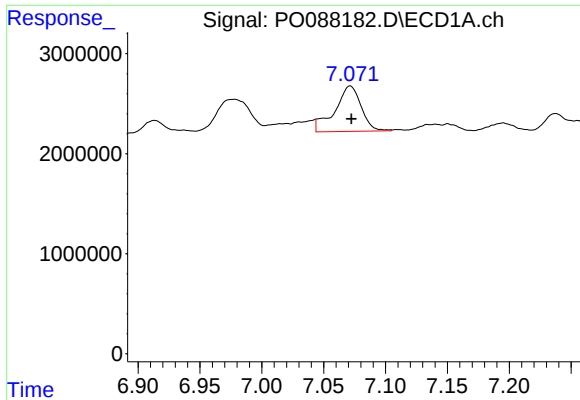

#28 AR-1254-3


R.T.: 7.071 min
Delta R.T.: -0.001 min
Response: 6719197
Conc: 45.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
TRE-1279-SLUDGE

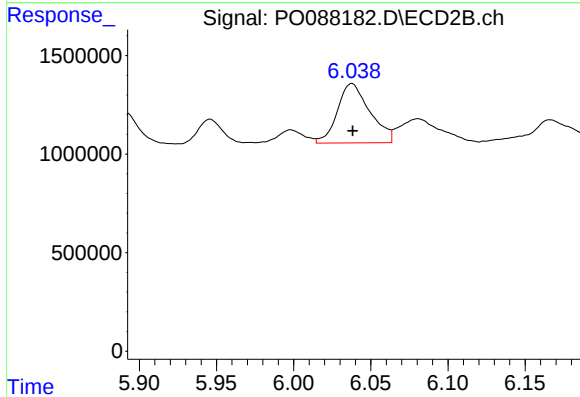


#28 AR-1254-3

R.T.: 6.038 min
Delta R.T.: 0.000 min
Response: 4407838
Conc: 54.32 ng/ml

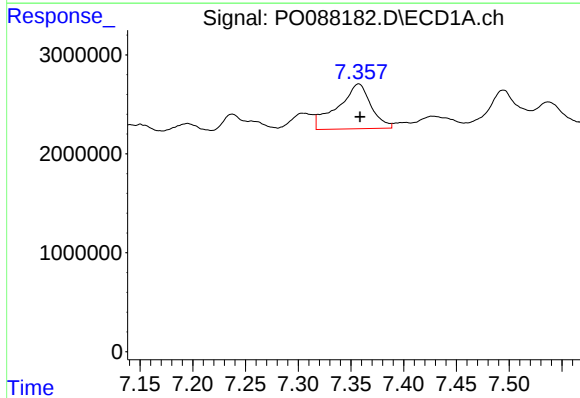


#29 AR-1254-4

R.T.: 7.357 min
Delta R.T.: -0.001 min
Response: 9865623
Conc: 91.16 ng/ml

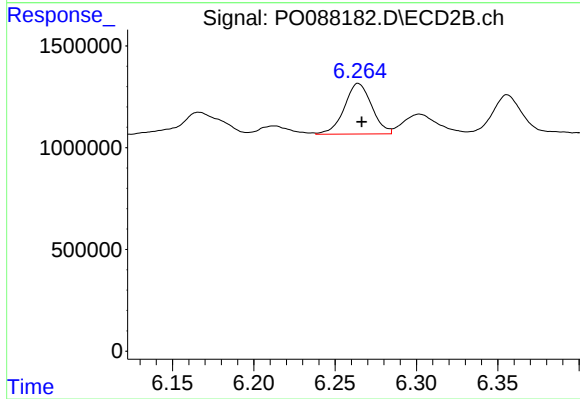

#29 AR-1254-4


R.T.: 6.264 min
Delta R.T.: -0.002 min
Response: 2907557
Conc: 58.30 ng/ml

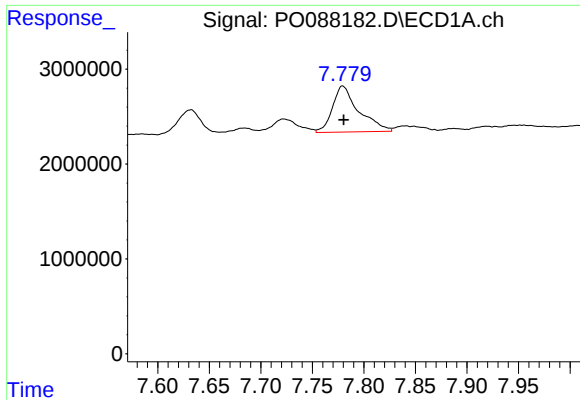

#30 AR-1254-5

R.T.: 7.779 min
Delta R.T.: 0.000 min
Response: 8621000
Conc: 71.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
TRE-1279-SLUDGE

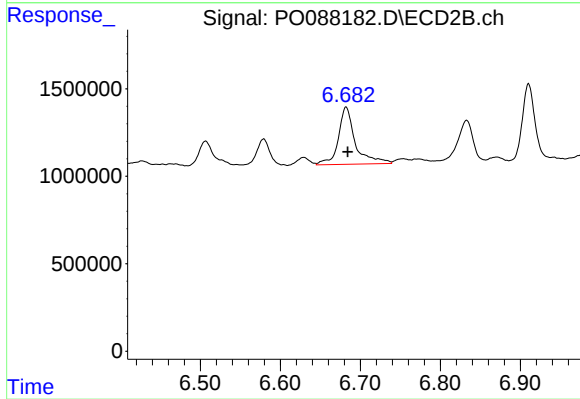

#30 AR-1254-5

R.T.: 6.682 min
Delta R.T.: -0.002 min
Response: 4847978
Conc: 64.19 ng/ml