

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072018\
 Data File : P0046947.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jul 2018 18:02
 Operator : SM/SJ
 Sample : PB111270BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB111270BL

Manual Integrations
 APPROVED

Sohil
 7/20/2018 11:24:41 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 03:13:30 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0071918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 19 01:07:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.199	3.522	599817	735386	2.087m	2.409
2) SA Decachlor...	9.725	8.447	709071	724591	3.224	2.959

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072018\
Data File : P0046947.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jul 2018 18:02
Operator : SM/SJ
Sample : PB111270BL
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB111270BL


Manual Integrations
APPROVED

Sohil
7/20/2018 11:24:41 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 03:13:30 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071918.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 19 01:07:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

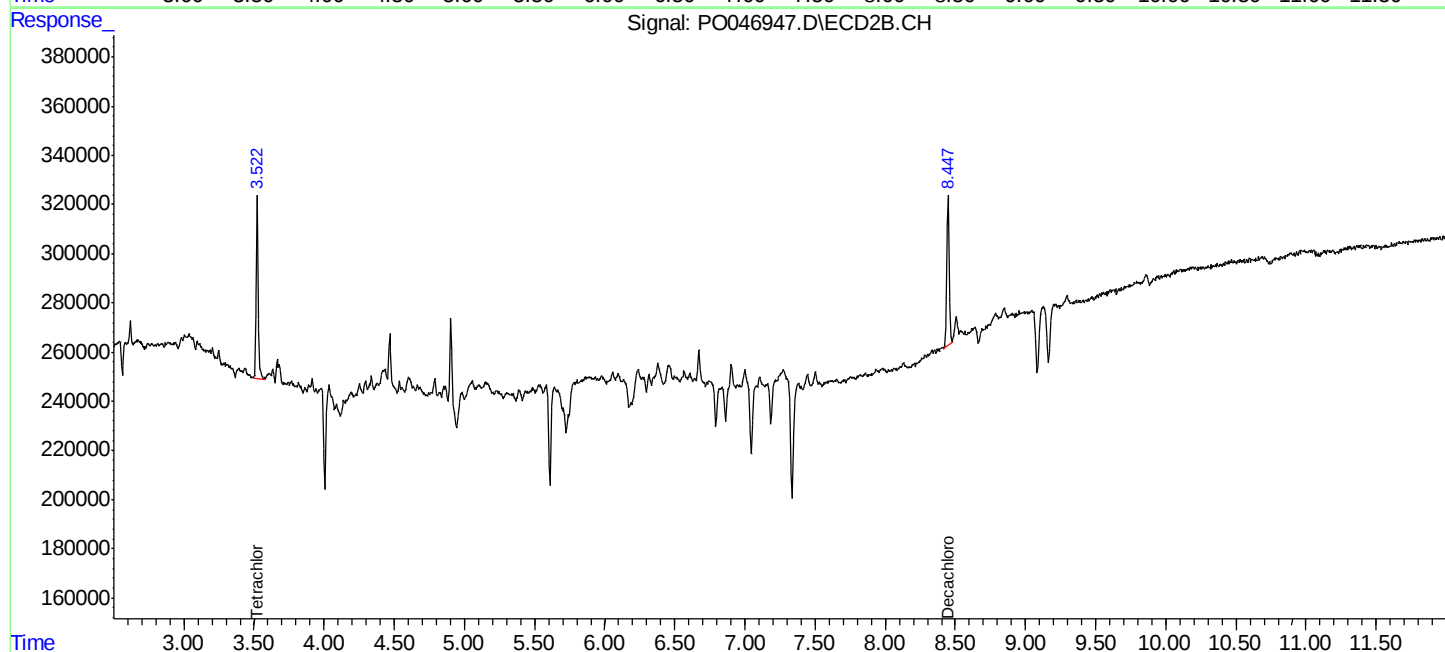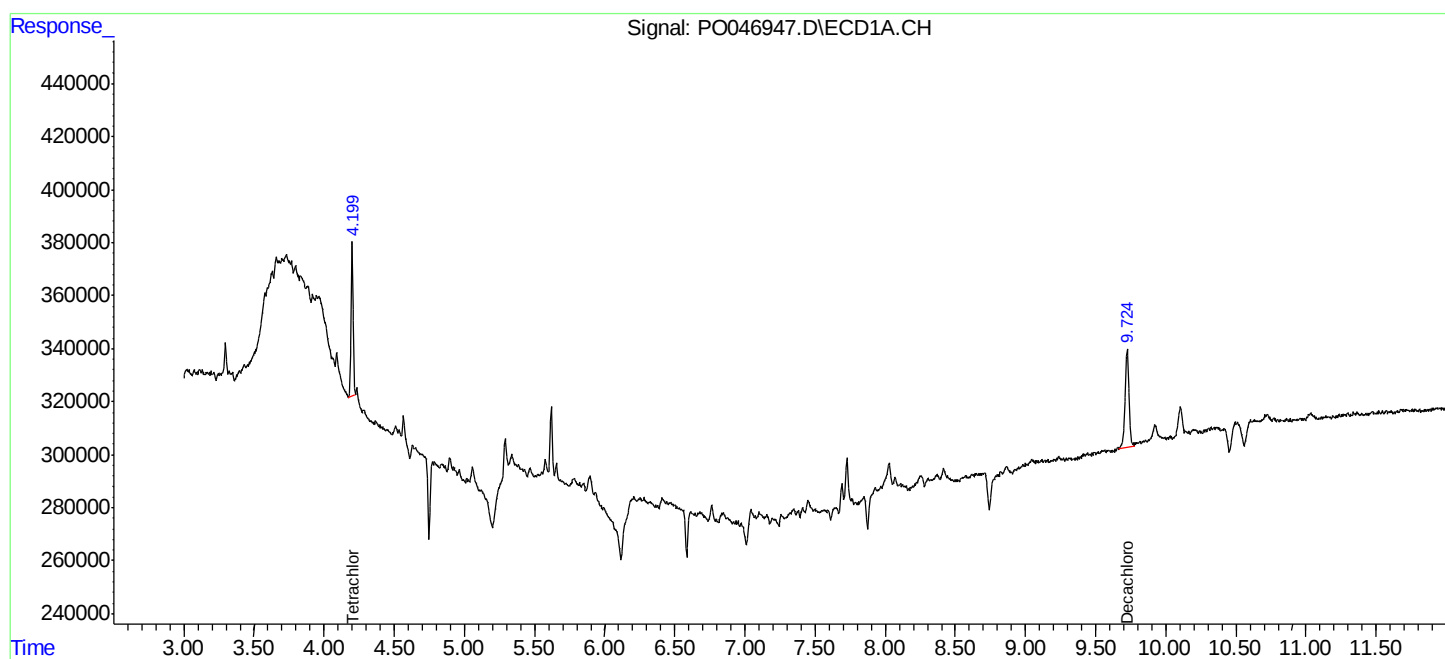

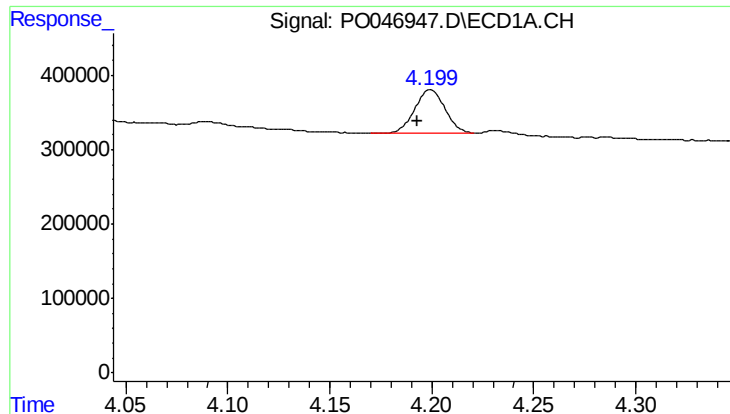


#1 Tetrachloro-m-xylene

R.T.: 4.199 min
Delta R.T.: 0.006 min
Response: 599817
Conc: 2.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB111270BL


Manual Integrations
APPROVED

Sohil
7/20/2018 11:24:41 AM

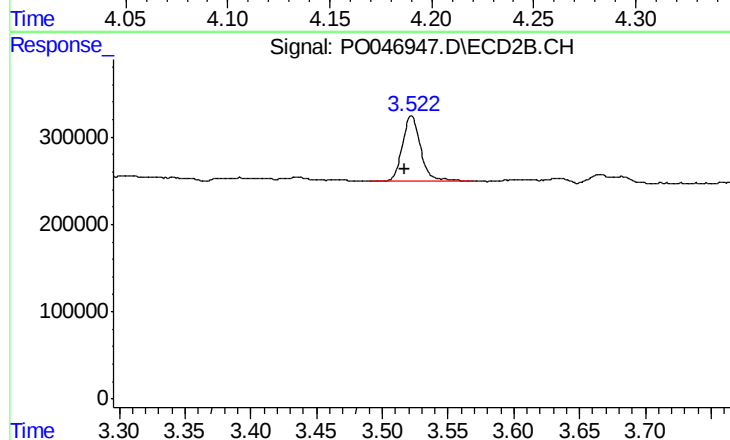


#1 Tetrachloro-m-xylene

R.T.: 3.522 min
Delta R.T.: 0.005 min
Response: 735386
Conc: 2.41 ng/ml

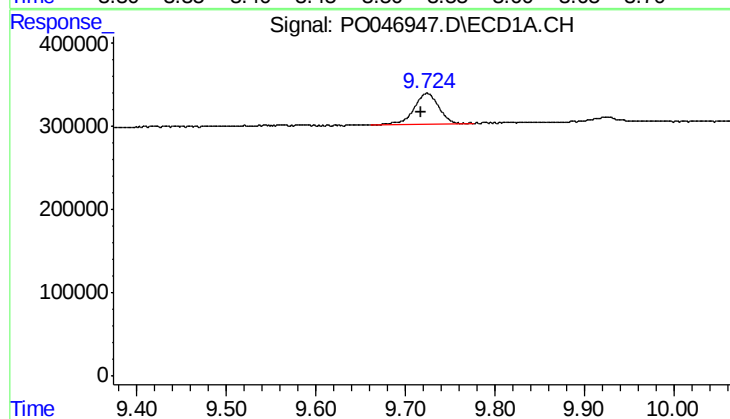

#2 Decachlorobiphenyl

R.T.: 9.725 min
Delta R.T.: 0.007 min
Response: 709071
Conc: 3.22 ng/ml

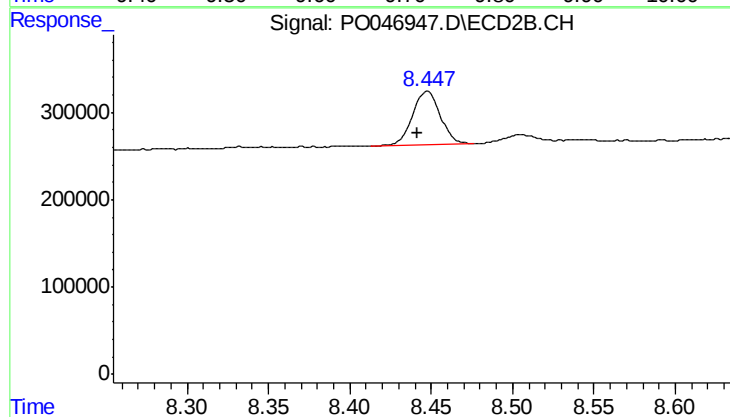

#2 Decachlorobiphenyl

R.T.: 8.447 min
Delta R.T.: 0.006 min
Response: 724591
Conc: 2.96 ng/ml