

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072018\
Data File : P0046965.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jul 2018 22:49
Operator : SM/SJ
Sample : J4061-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
071718-TIPC-F-D-S

Manual Integrations
APPROVED

Sohil
7/20/2018 11:25:09 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 01:55:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0071918.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 19 01:07:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.199	3.523	3757389	3805688	13.075m	12.468m
2) SA Decachlor...	9.723	8.446	3486991	3559324	15.854	14.536

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072018\
Data File : P0046965.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jul 2018 22:49
Operator : SM/SJ
Sample : J4061-08
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
071718-TIPC-F-D-S


Manual Integrations
APPROVED

Sohil
7/20/2018 11:25:09 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 01:55:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071918.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 19 01:07:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

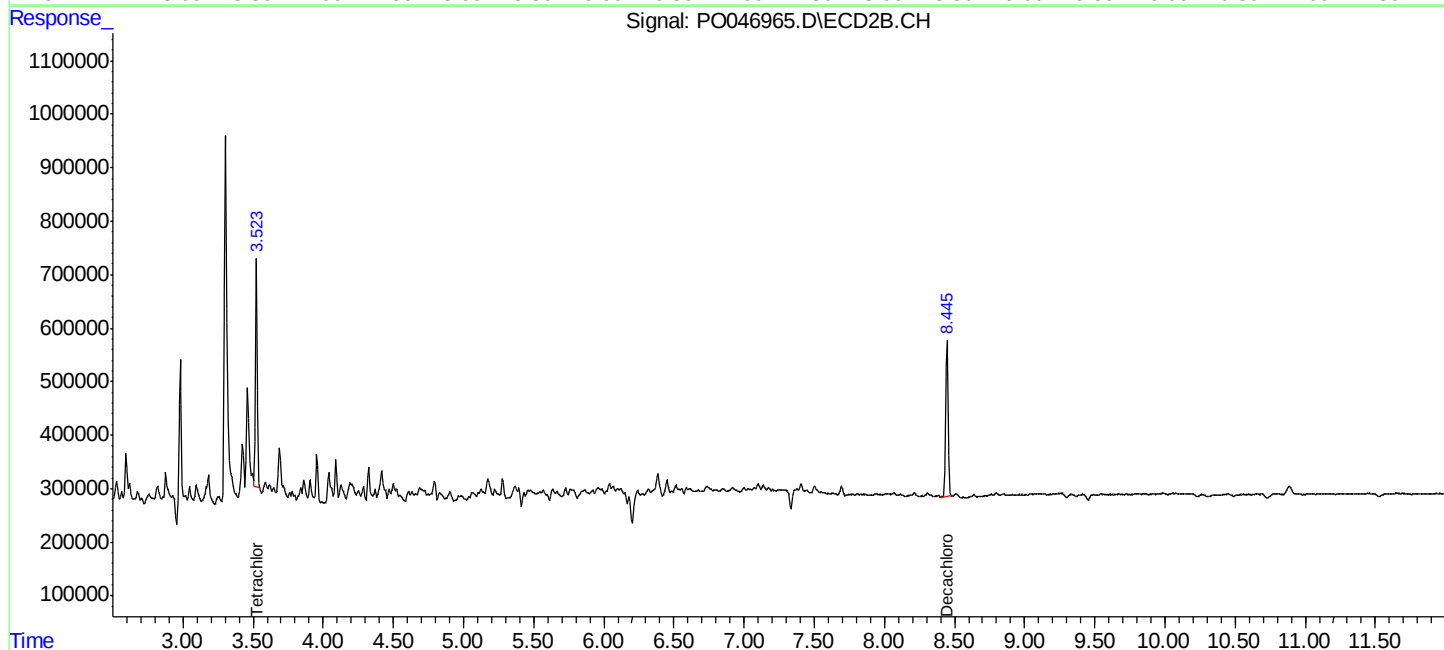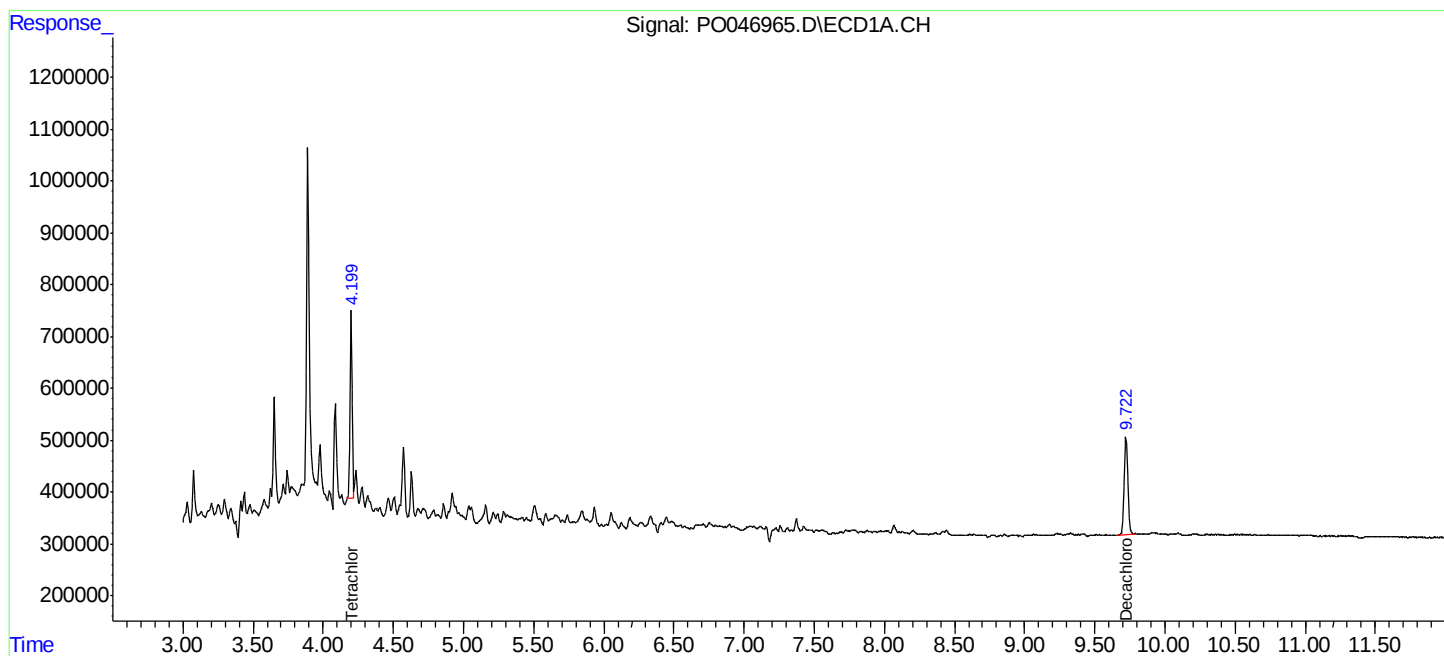

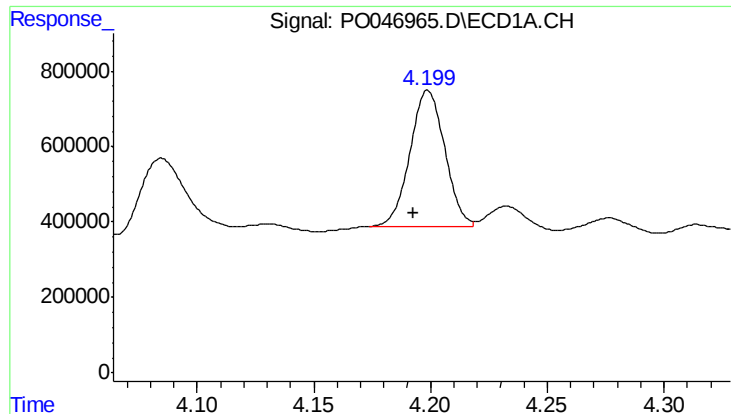


#1 Tetrachloro-m-xylene

R.T.: 4.199 min
Delta R.T.: 0.006 min
Response: 3757389
Conc: 13.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
071718-TIPC-F-D-S


Manual Integrations
APPROVED

Sohil
7/20/2018 11:25:09 AM

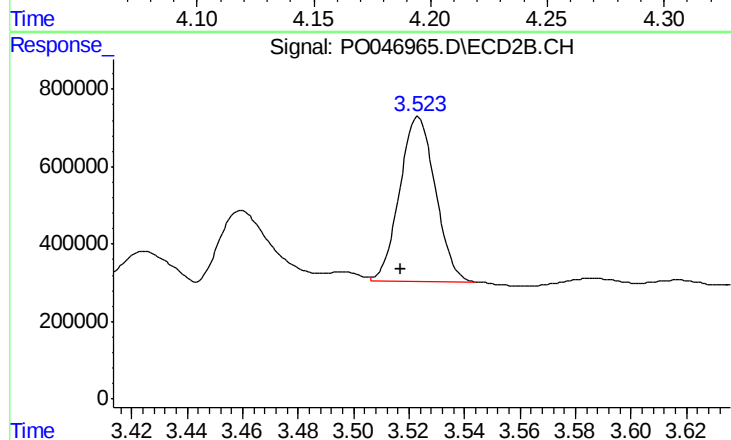


#1 Tetrachloro-m-xylene

R.T.: 3.523 min
Delta R.T.: 0.006 min
Response: 3805688
Conc: 12.47 ng/ml m

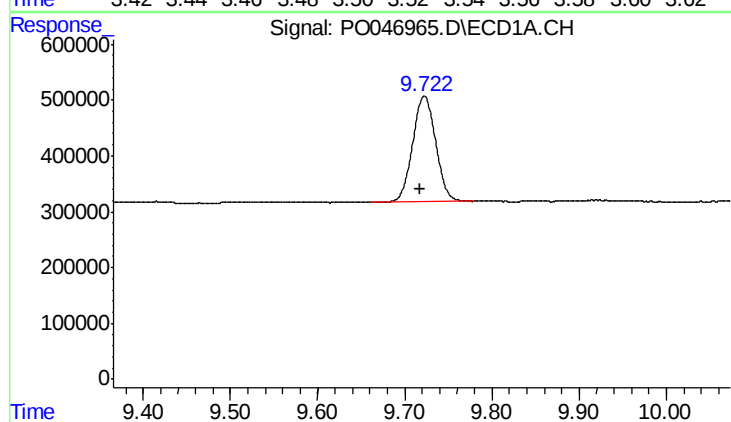

#2 Decachlorobiphenyl

R.T.: 9.723 min
Delta R.T.: 0.005 min
Response: 3486991
Conc: 15.85 ng/ml

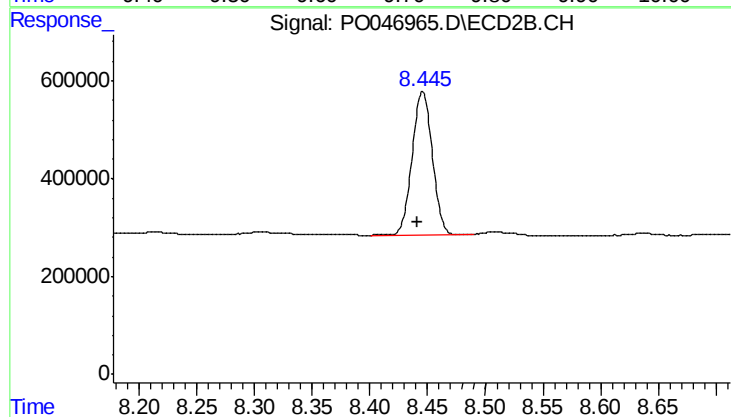

#2 Decachlorobiphenyl

R.T.: 8.446 min
Delta R.T.: 0.004 min
Response: 3559324
Conc: 14.54 ng/ml