

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072019\
 Data File : P0058146.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jul 2019 9:39
 Operator : SM/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 13:25:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.190	3.535	644833	652190	19.029	20.334
2)	SA Decachlor...	9.698	8.435	951020	623353	18.589	18.186
Target Compounds							
15)	L3 AR-1232-5	5.612	0.000	47100	0	124.911	N.D. #
20)	L4 AR-1242-5	6.197	0.000	325022	0	280.677	N.D. #
22)	L5 AR-1248-2	5.612	0.000	47100	0	34.955	N.D. #
24)	L5 AR-1248-4	6.197	0.000	325022	0	166.011	N.D. #
25)	L5 AR-1248-5	6.197	0.000	325022	0	170.540	N.D. #
26)	L6 AR-1254-1	6.197	0.000	325022	0	165.390	N.D. #
27)	L6 AR-1254-2	6.443	0.000	95263	0	29.141	N.D. #
32)	L7 AR-1260-2	7.178	0.000	291076	0	82.789	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO072019\
Data File : PO058146.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jul 2019 9:39
Operator : SM/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 13:25:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

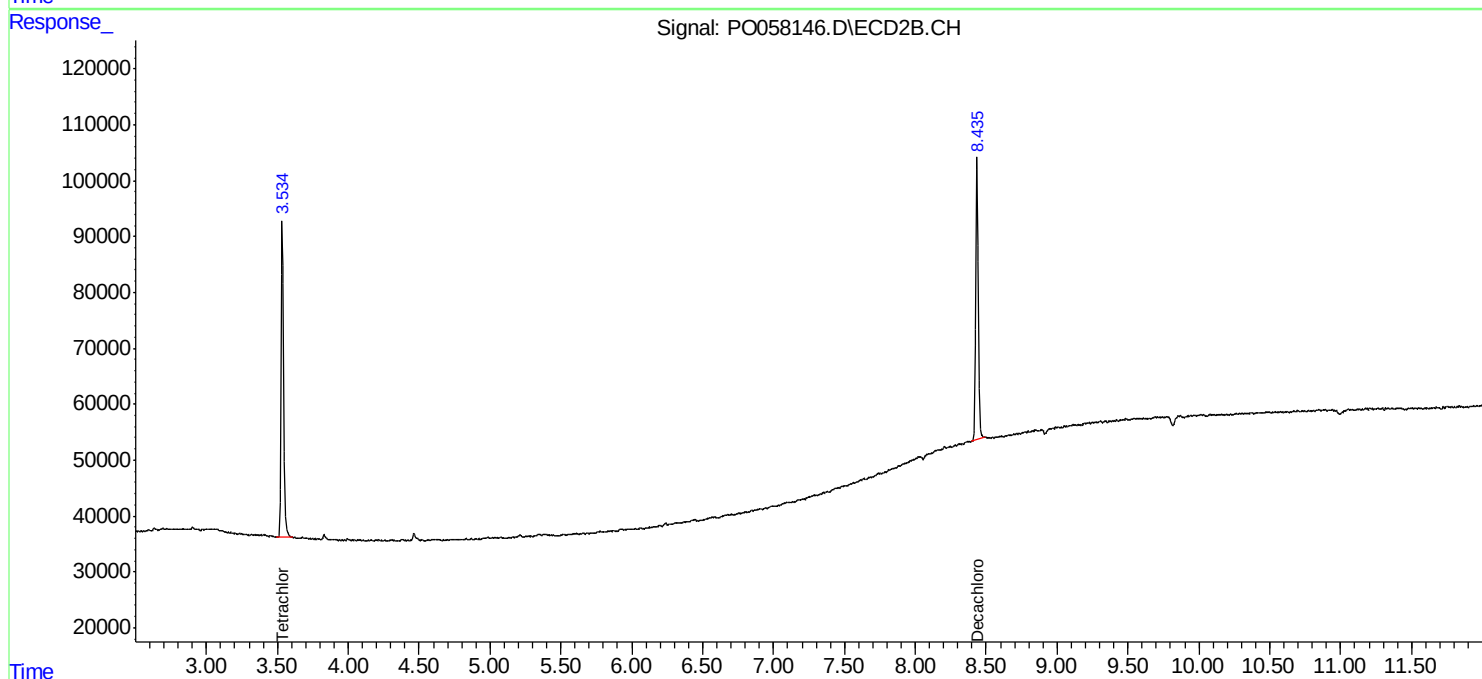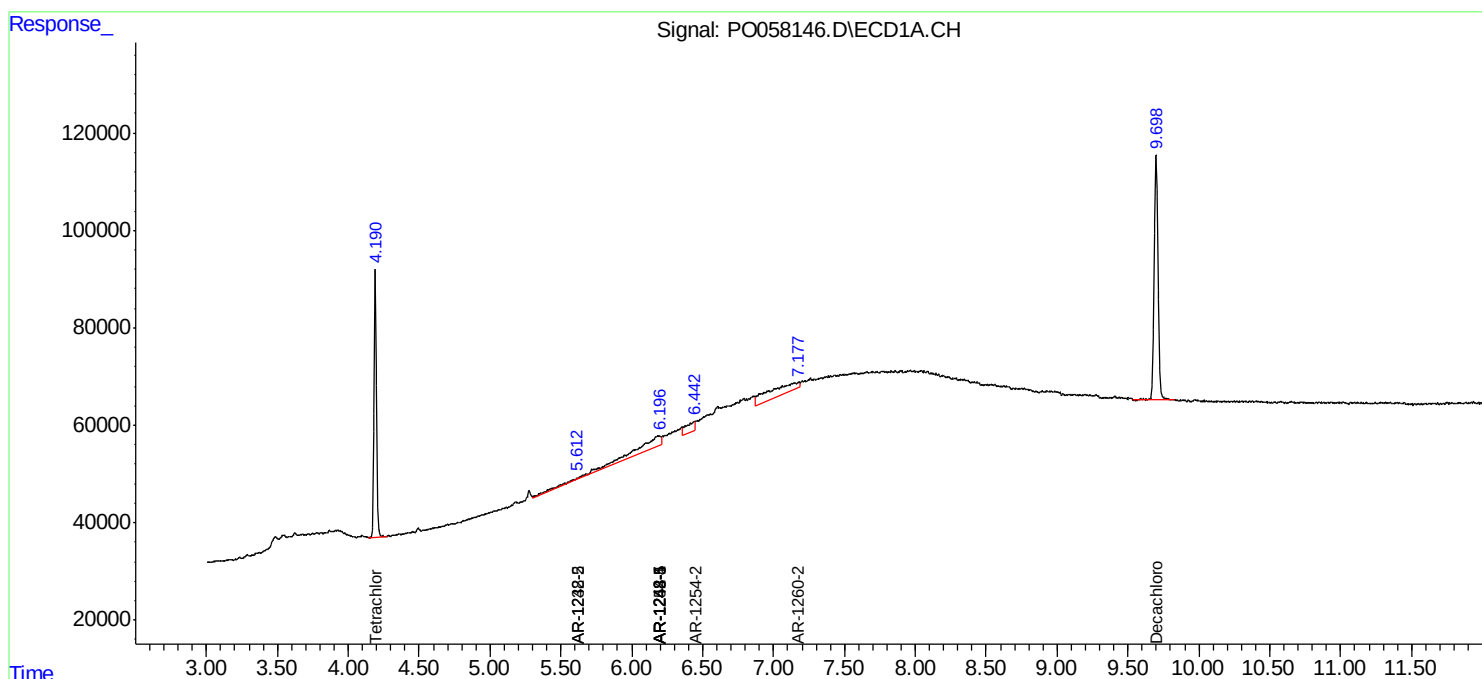


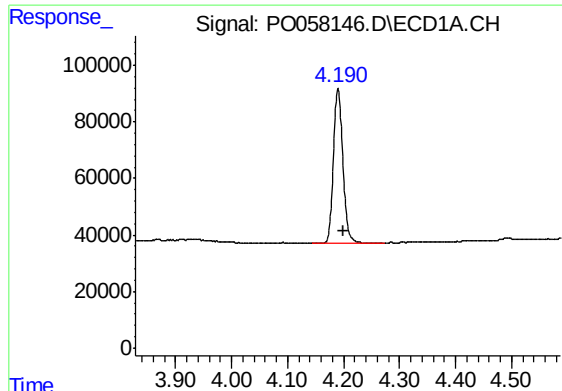

#1 Tetrachloro-m-xylene


R.T.: 4.190 min
Delta R.T.: -0.010 min
Response: 644833
Conc: 19.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

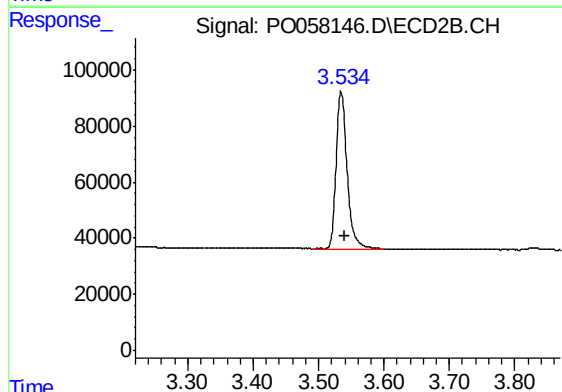


#1 Tetrachloro-m-xylene

R.T.: 3.535 min
Delta R.T.: -0.005 min
Response: 652190
Conc: 20.33 ng/ml

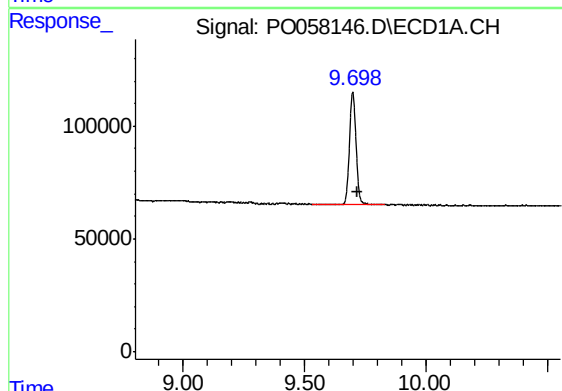


#2 Decachlorobiphenyl

R.T.: 9.698 min
Delta R.T.: -0.020 min
Response: 951020
Conc: 18.59 ng/ml

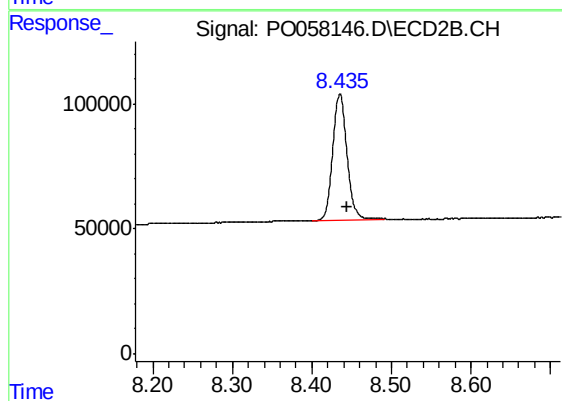

#2 Decachlorobiphenyl


R.T.: 8.435 min
Delta R.T.: -0.010 min
Response: 623353
Conc: 18.19 ng/ml

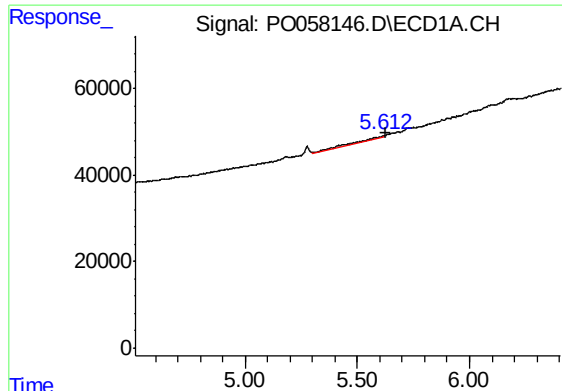

#15 AR-1232-5


R.T.: 5.612 min
Delta R.T.: -0.013 min
Response: 47100
Conc: 124.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

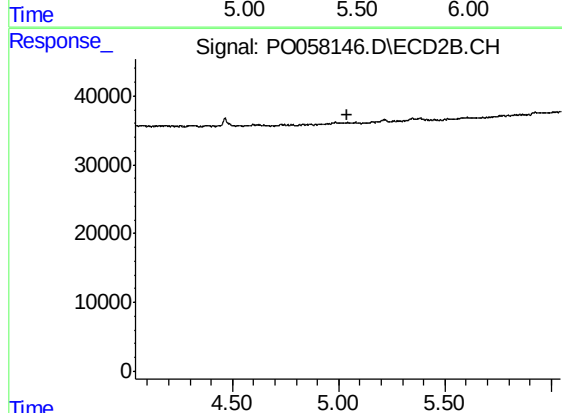


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 5.043 min
Response: 0
Conc: N.D.

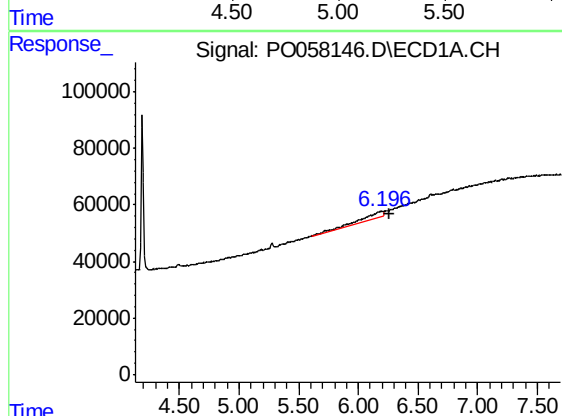


#20 AR-1242-5

R.T.: 6.197 min
Delta R.T.: -0.066 min
Response: 325022
Conc: 280.68 ng/ml

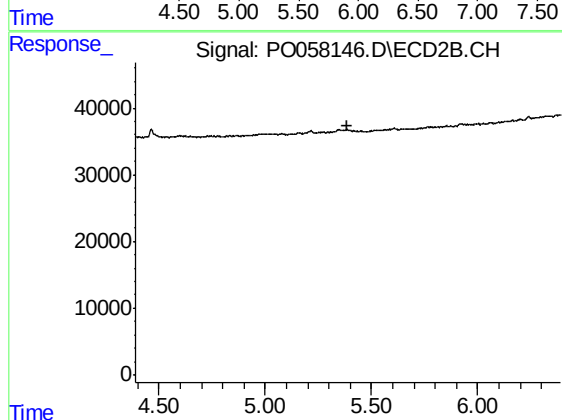

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 5.389 min
Response: 0
Conc: N.D.

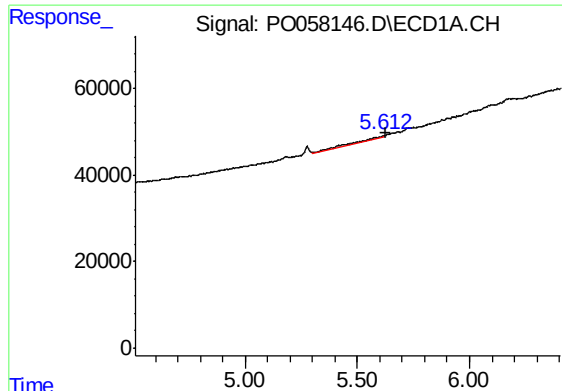

#22 AR-1248-2


R.T.: 5.612 min
Delta R.T.: -0.013 min
Response: 47100
Conc: 34.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

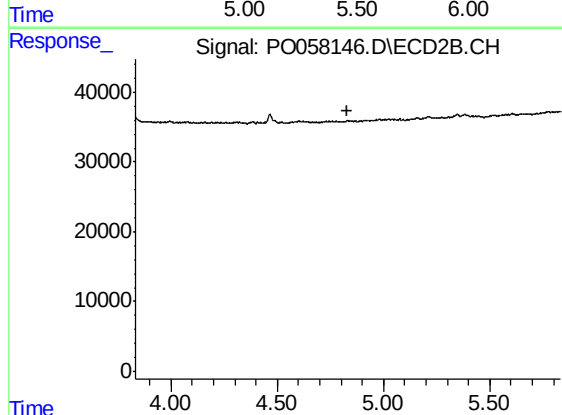


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T. : 4.833 min
Response: 0
Conc: N.D.

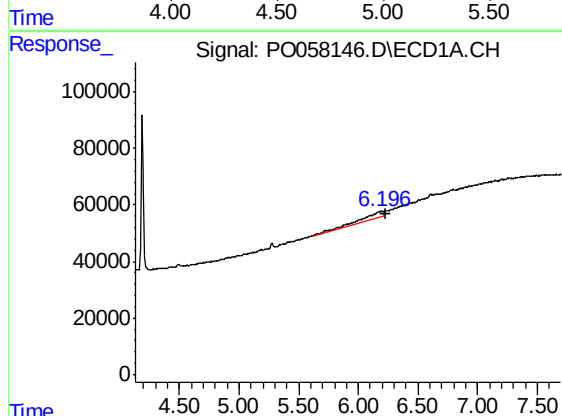


#24 AR-1248-4

R.T.: 6.197 min
Delta R.T.: -0.029 min
Response: 325022
Conc: 166.01 ng/ml

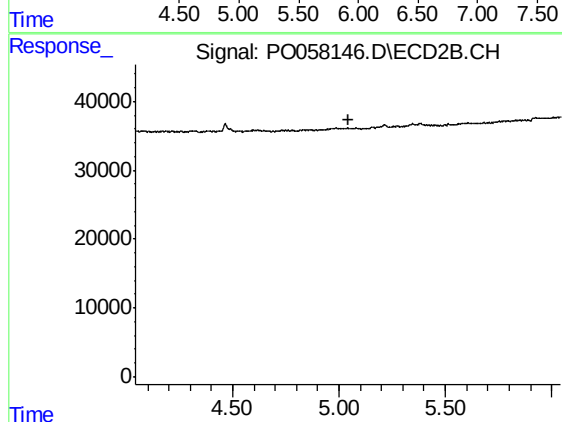

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.042 min
Response: 0
Conc: N.D.

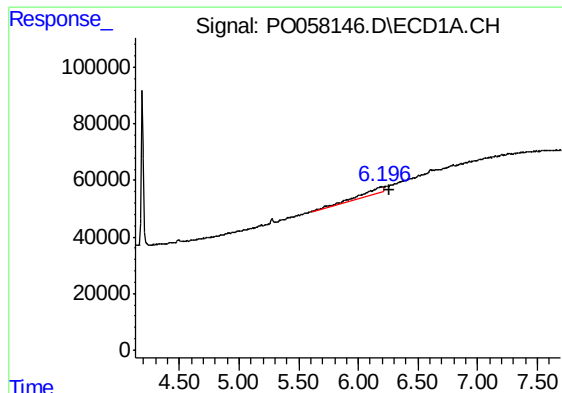

#25 AR-1248-5


R.T.: 6.197 min
Delta R.T.: -0.066 min
Response: 325022
Conc: 170.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

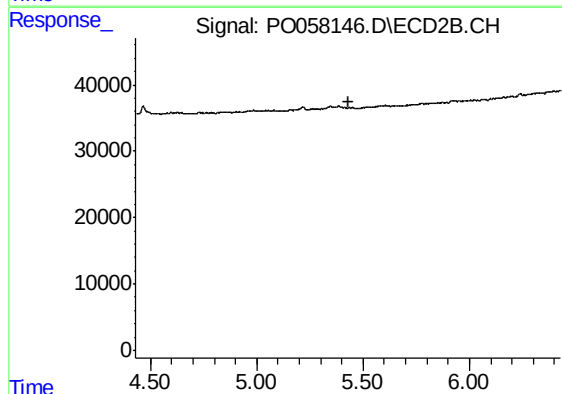


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.429 min
Response: 0
Conc: N.D.

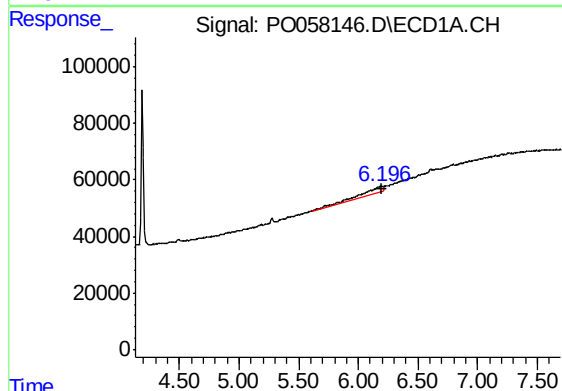


#26 AR-1254-1

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 325022
Conc: 165.39 ng/ml

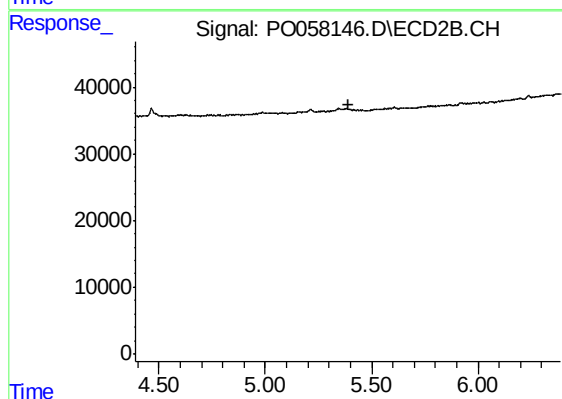

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.389 min
Response: 0
Conc: N.D.

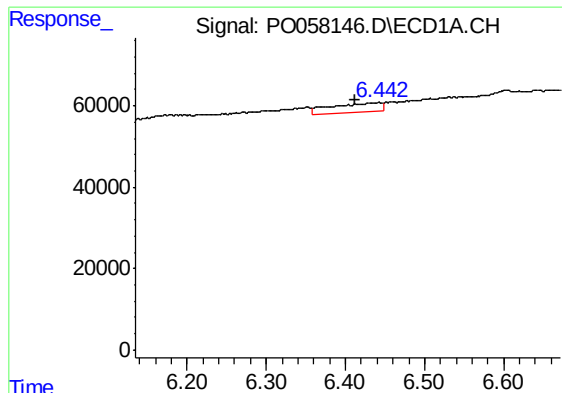

#27 AR-1254-2


R.T.: 6.443 min
Delta R.T.: 0.030 min
Response: 95263
Conc: 29.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

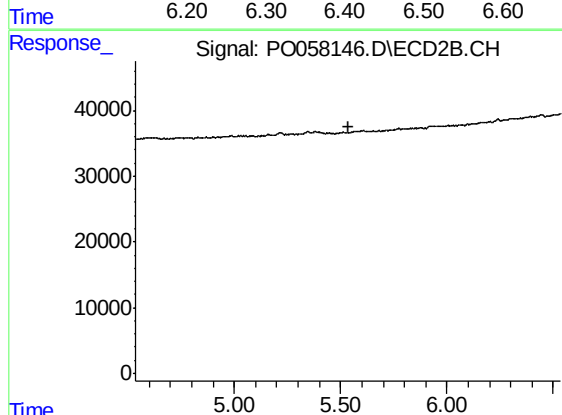


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 5.535 min
Response: 0
Conc: N.D.

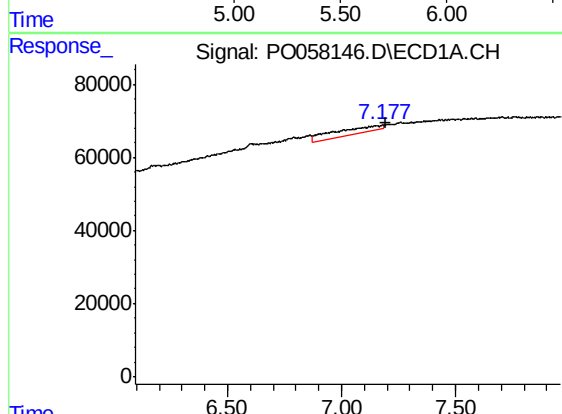

#32 AR-1260-2

R.T.: 7.178 min
Delta R.T.: -0.016 min
Response: 291076
Conc: 82.79 ng/ml

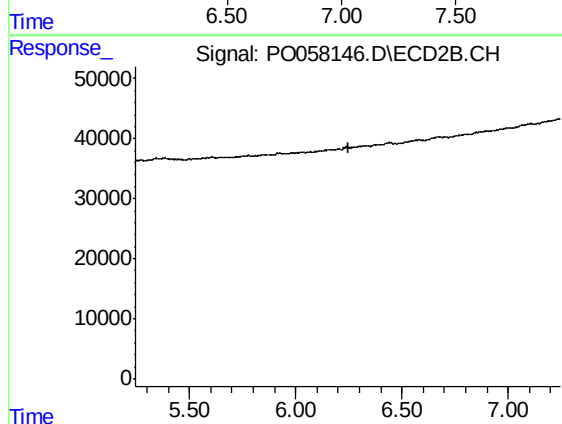

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.247 min
Response: 0
Conc: N.D.