

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072019\
 Data File : P0058196.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jul 2019 3:09
 Operator : SM/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 04:28:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.192	3.535	629114	616863	18.565	19.233
2)	SA Decachlor...	9.702	8.438	1035658	710992	20.244	20.743
Target Compounds							
20)	L4 AR-1242-5	6.195	0.000	119639	0	103.316	N.D. #
24)	L5 AR-1248-4	6.195	0.000	119639	0	61.108	N.D. #
25)	L5 AR-1248-5	6.195	0.000	119639	0	62.775	N.D. #
26)	L6 AR-1254-1	6.195	0.000	119639	0	60.879	N.D. #
28)	L6 AR-1254-3	6.789	0.000	442431	0	125.413	N.D. #
29)	L6 AR-1254-4	7.044	0.000	43729	0	14.779	N.D. #
31)	L7 AR-1260-1	6.970	0.000	32470	0	12.982	N.D. #
32)	L7 AR-1260-2	7.183	0.000	22964	0	6.532	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072019\
Data File : P0058196.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jul 2019 3:09
Operator : SM/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 04:28:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

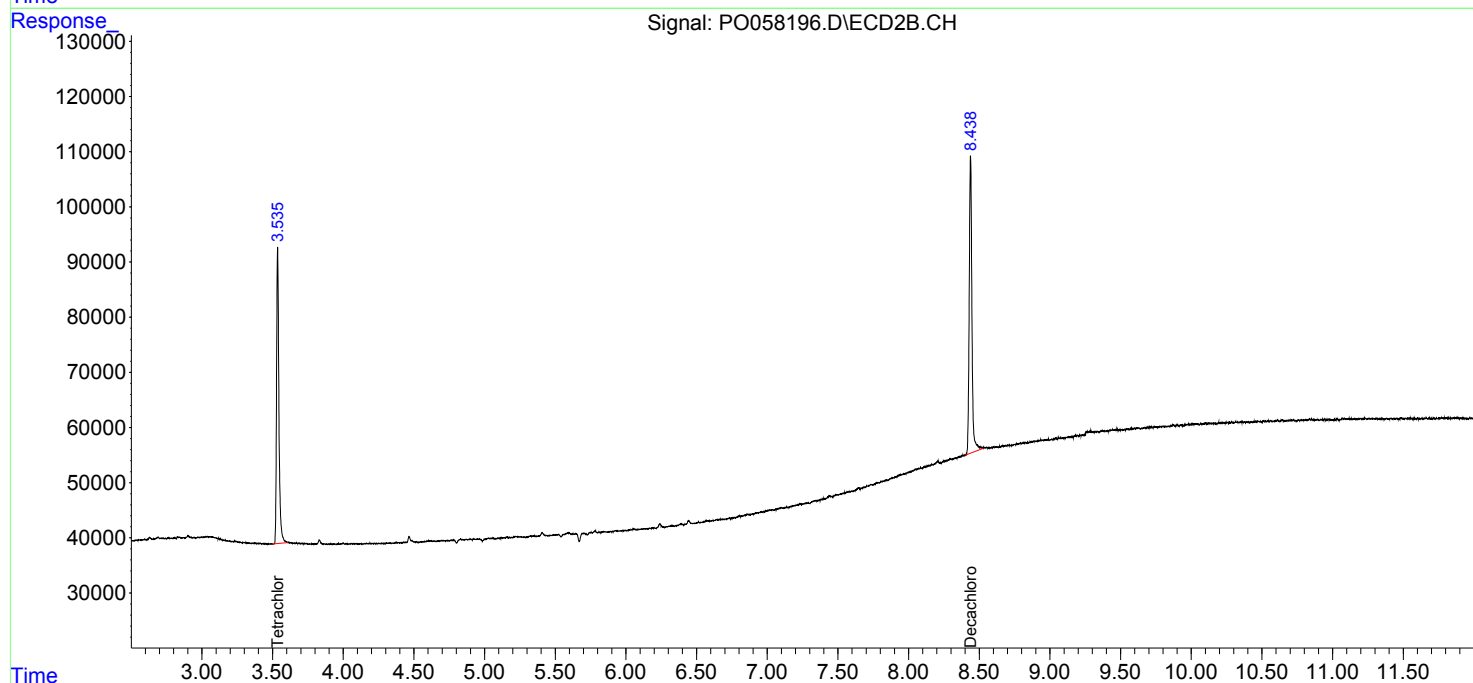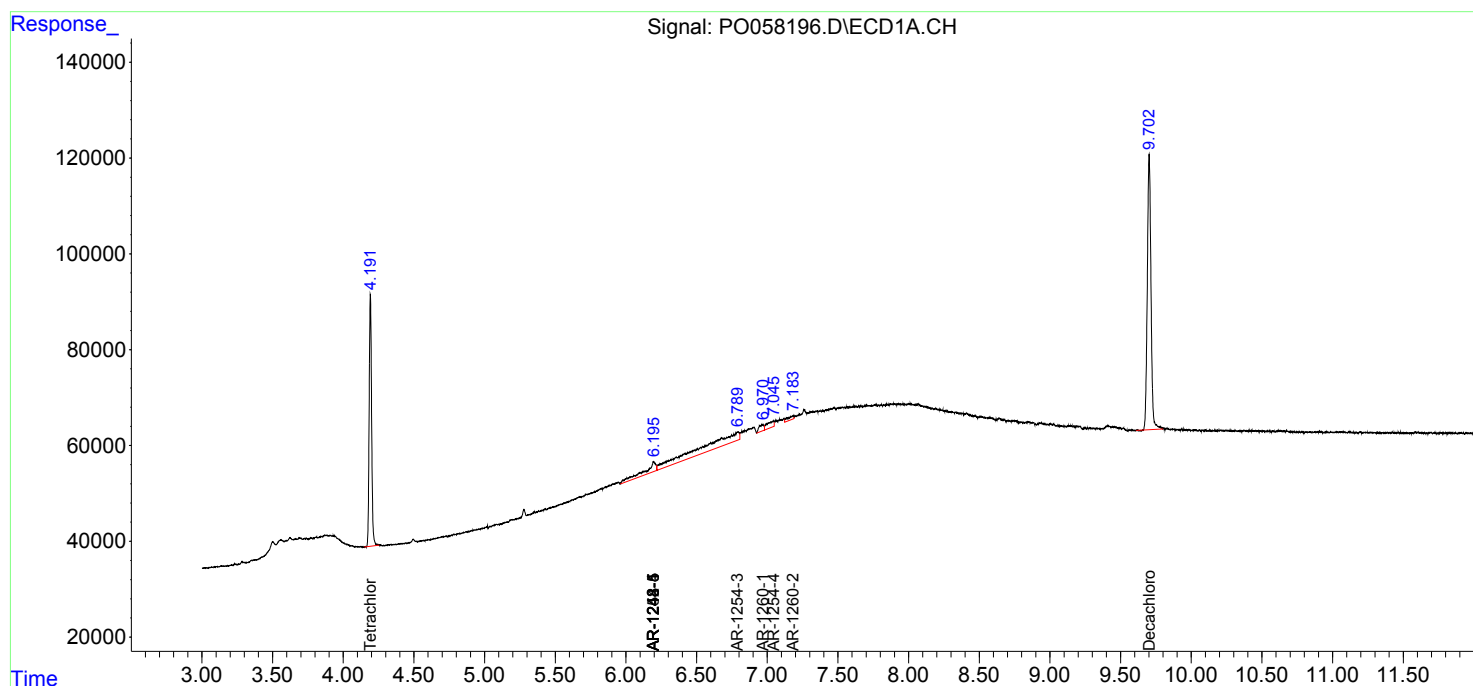


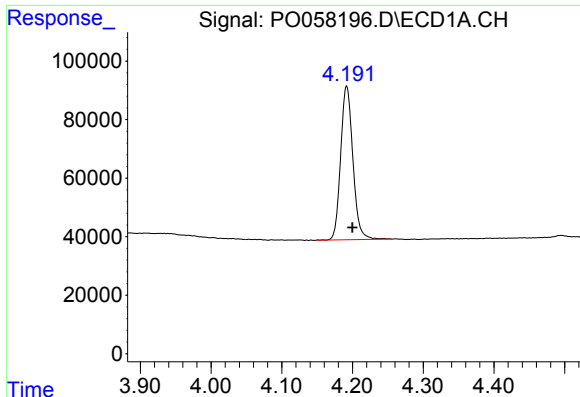

#1 Tetrachloro-m-xylene


R.T.: 4.192 min
Delta R.T.: -0.008 min
Response: 629114
Conc: 18.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

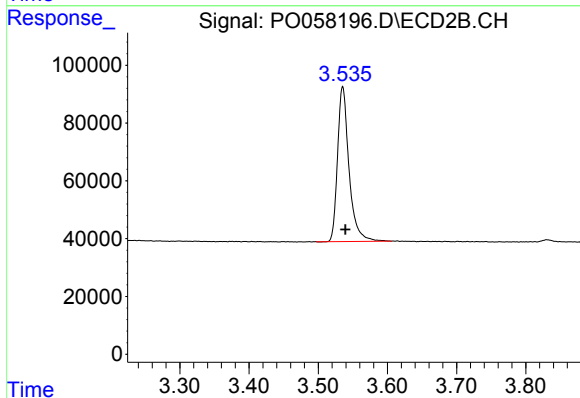


#1 Tetrachloro-m-xylene

R.T.: 3.535 min
Delta R.T.: -0.004 min
Response: 616863
Conc: 19.23 ng/ml

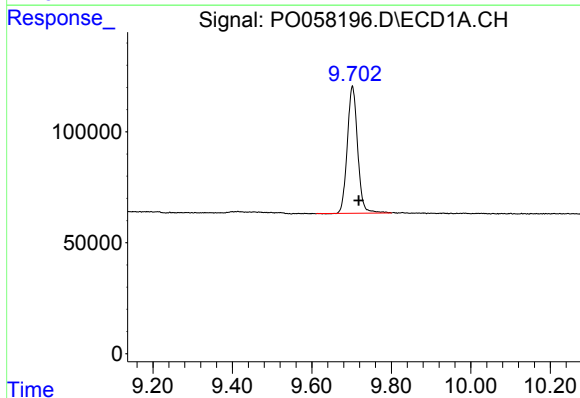


#2 Decachlorobiphenyl

R.T.: 9.702 min
Delta R.T.: -0.016 min
Response: 1035658
Conc: 20.24 ng/ml

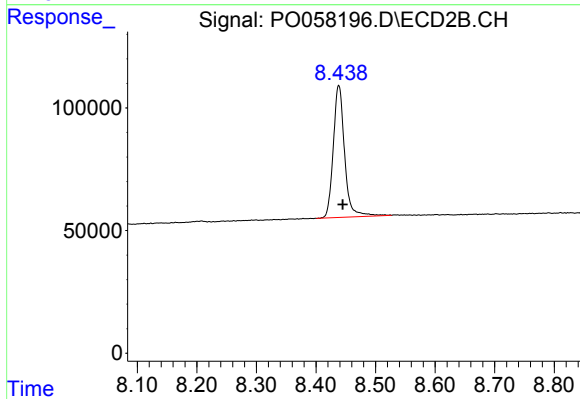

#2 Decachlorobiphenyl


R.T.: 8.438 min
Delta R.T.: -0.007 min
Response: 710992
Conc: 20.74 ng/ml

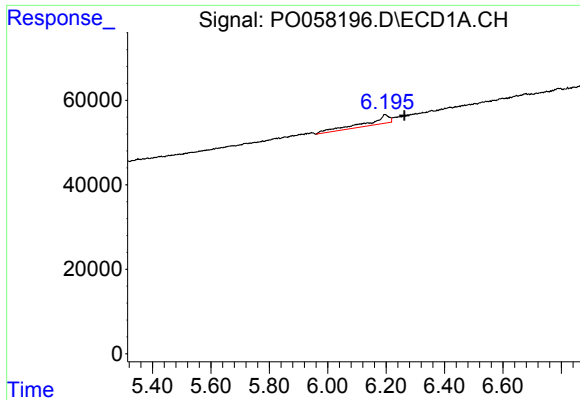

#20 AR-1242-5


R.T.: 6.195 min
Delta R.T.: -0.068 min
Response: 119639
Conc: 103.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

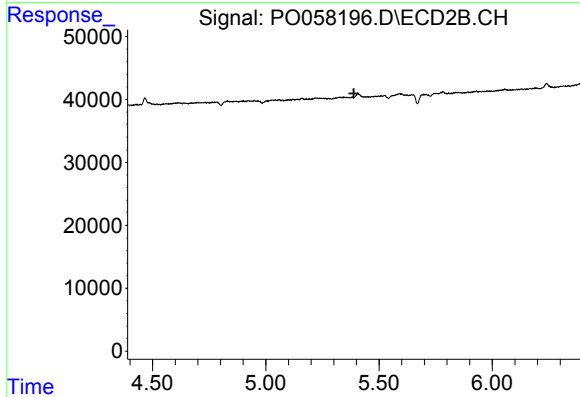


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 5.389 min
Response: 0
Conc: N.D.

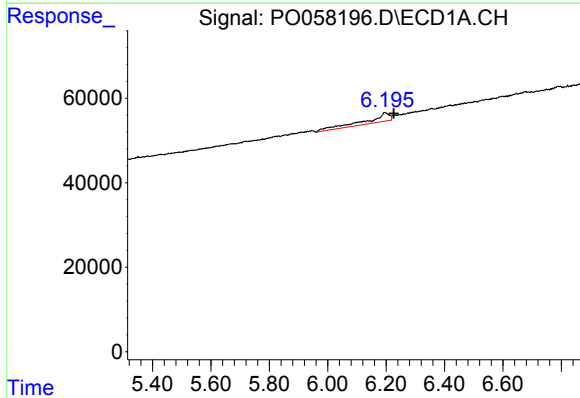


#24 AR-1248-4

R.T.: 6.195 min
Delta R.T.: -0.031 min
Response: 119639
Conc: 61.11 ng/ml

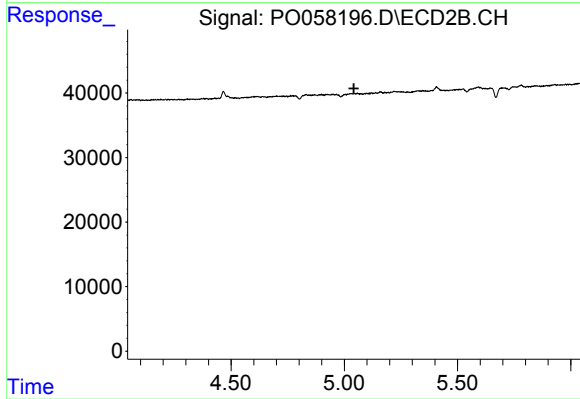

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.042 min
Response: 0
Conc: N.D.

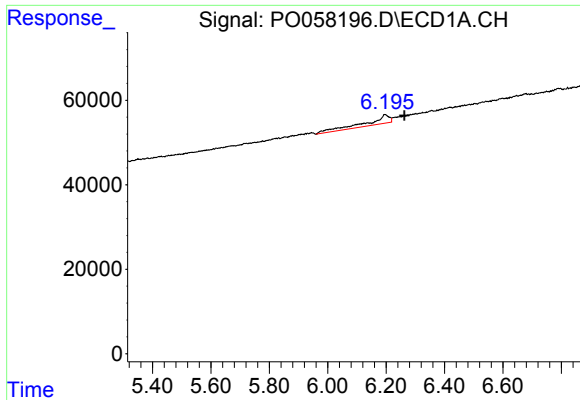

#25 AR-1248-5


R.T.: 6.195 min
Delta R.T.: -0.068 min
Response: 119639
Conc: 62.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

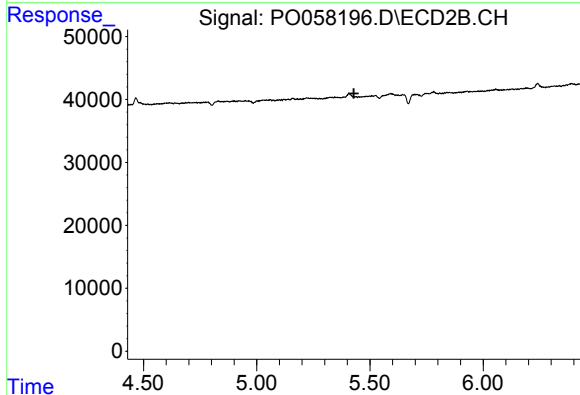


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.429 min
Response: 0
Conc: N.D.

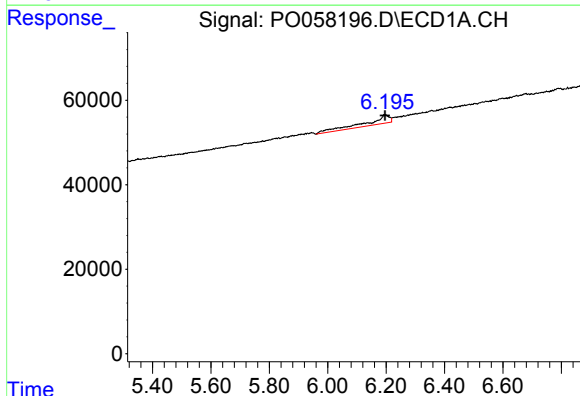


#26 AR-1254-1

R.T.: 6.195 min
Delta R.T.: -0.001 min
Response: 119639
Conc: 60.88 ng/ml

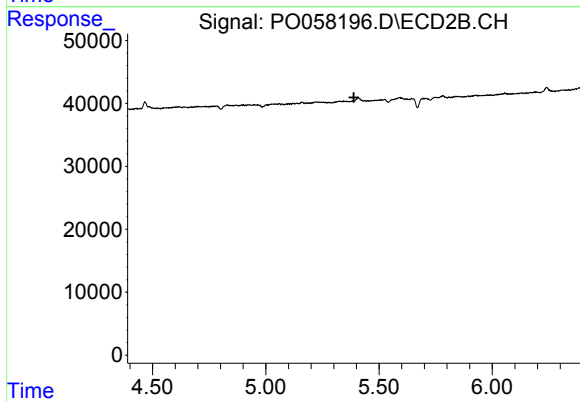

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.389 min
Response: 0
Conc: N.D.

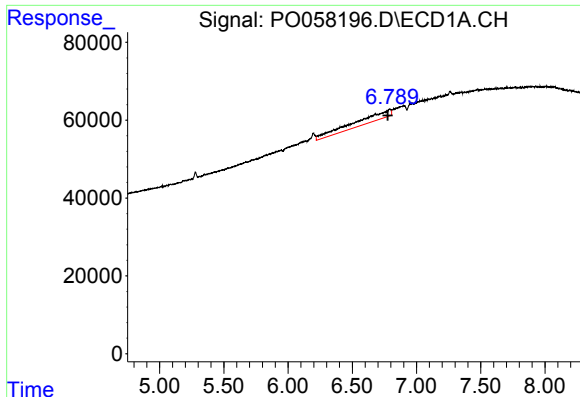

#28 AR-1254-3


R.T.: 6.789 min
Delta R.T.: 0.012 min
Response: 442431
Conc: 125.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

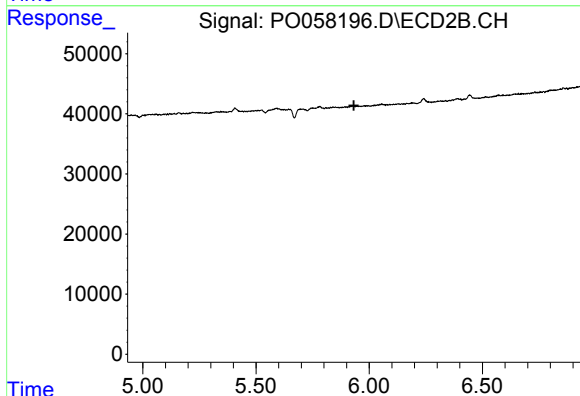


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 5.932 min
Response: 0
Conc: N.D.

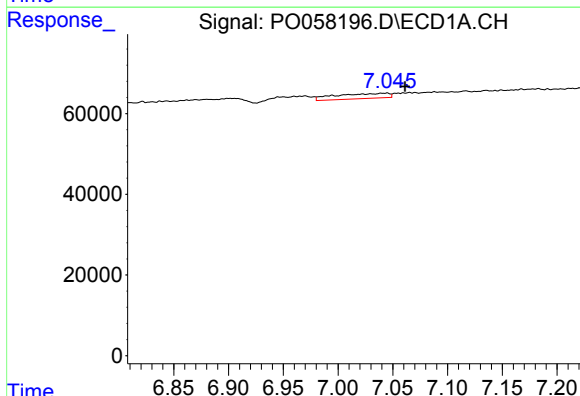


#29 AR-1254-4

R.T.: 7.044 min
Delta R.T.: -0.017 min
Response: 43729
Conc: 14.78 ng/ml

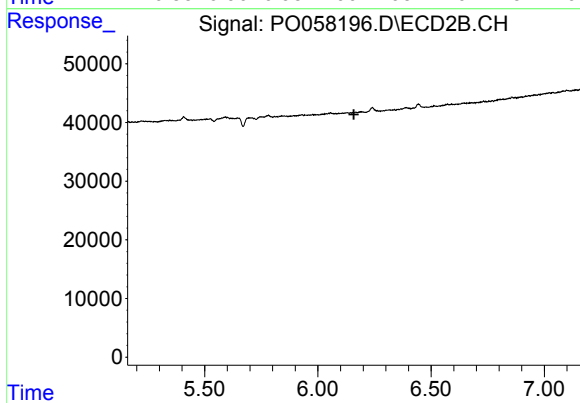

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.159 min
Response: 0
Conc: N.D.

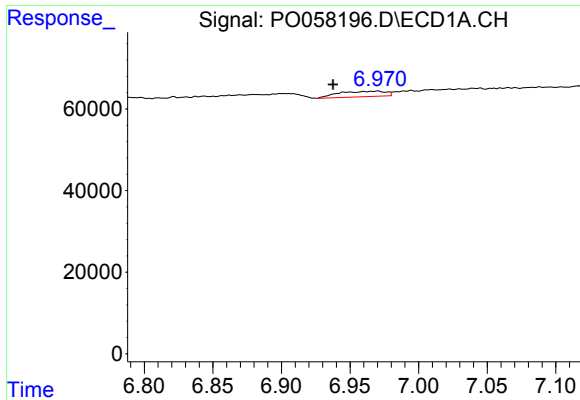

#31 AR-1260-1


R.T.: 6.970 min
Delta R.T.: 0.032 min
Response: 32470
Conc: 12.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

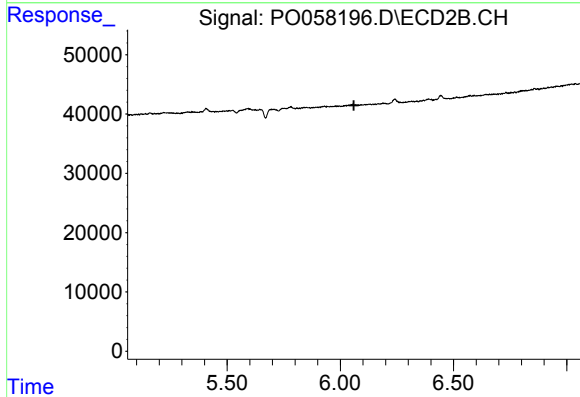


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.060 min
Response: 0
Conc: N.D.

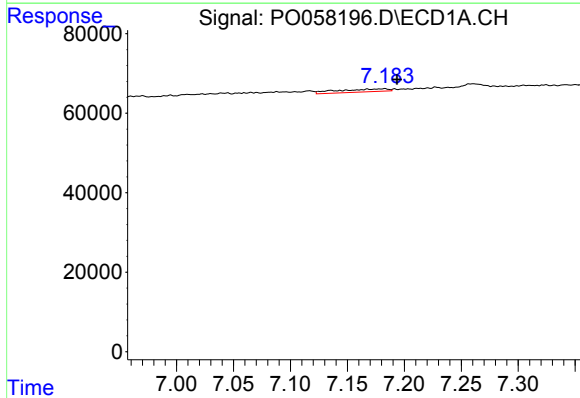

#32 AR-1260-2

R.T.: 7.183 min
Delta R.T.: -0.011 min
Response: 22964
Conc: 6.53 ng/ml

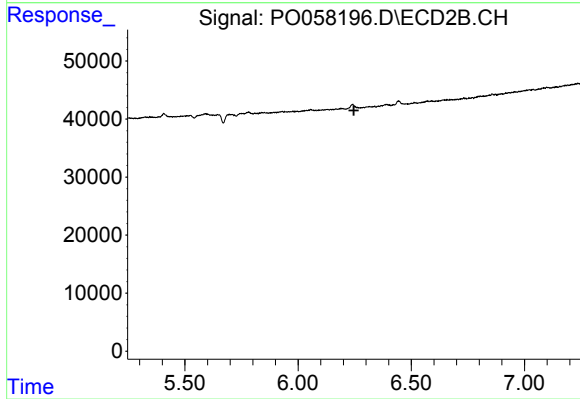

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.247 min
Response: 0
Conc: N.D.