

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072019\
 Data File : P0058157.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jul 2019 12:57
 Operator : SM/AJ
 Sample : K3807-01RE
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-PS-01-053RE

Manual Integrations
 APPROVED

Ankita
 7/21/2019 12:01:49 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 19 14:58:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.191	3.535	778955	628054	22.987	19.582
2) SA Decachlor...	9.698	8.436	552469	402307	10.799m	11.737

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO072019\
Data File : PO058157.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jul 2019 12:57
Operator : SM/AJ
Sample : K3807-01RE
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-PS-01-053RE


Manual Integrations
APPROVED

Ankita
7/21/2019 12:01:49 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 19 14:58:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

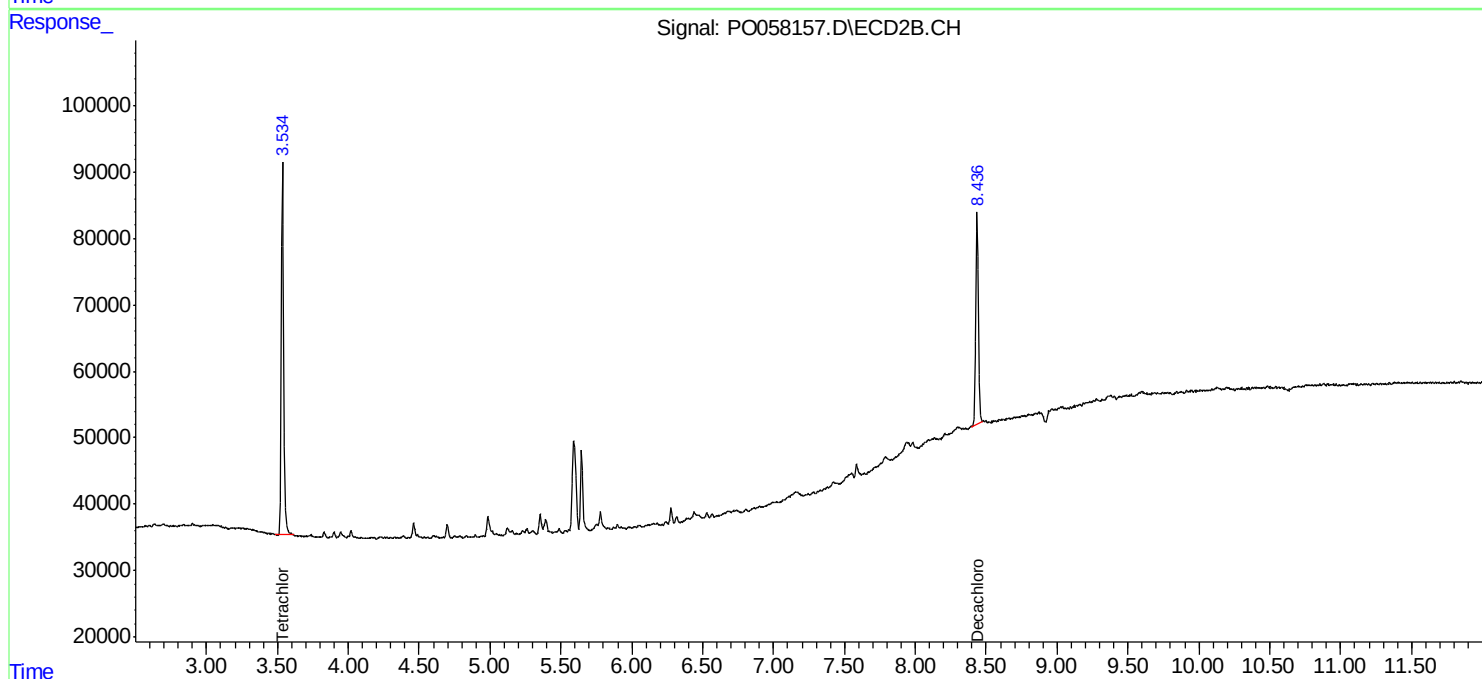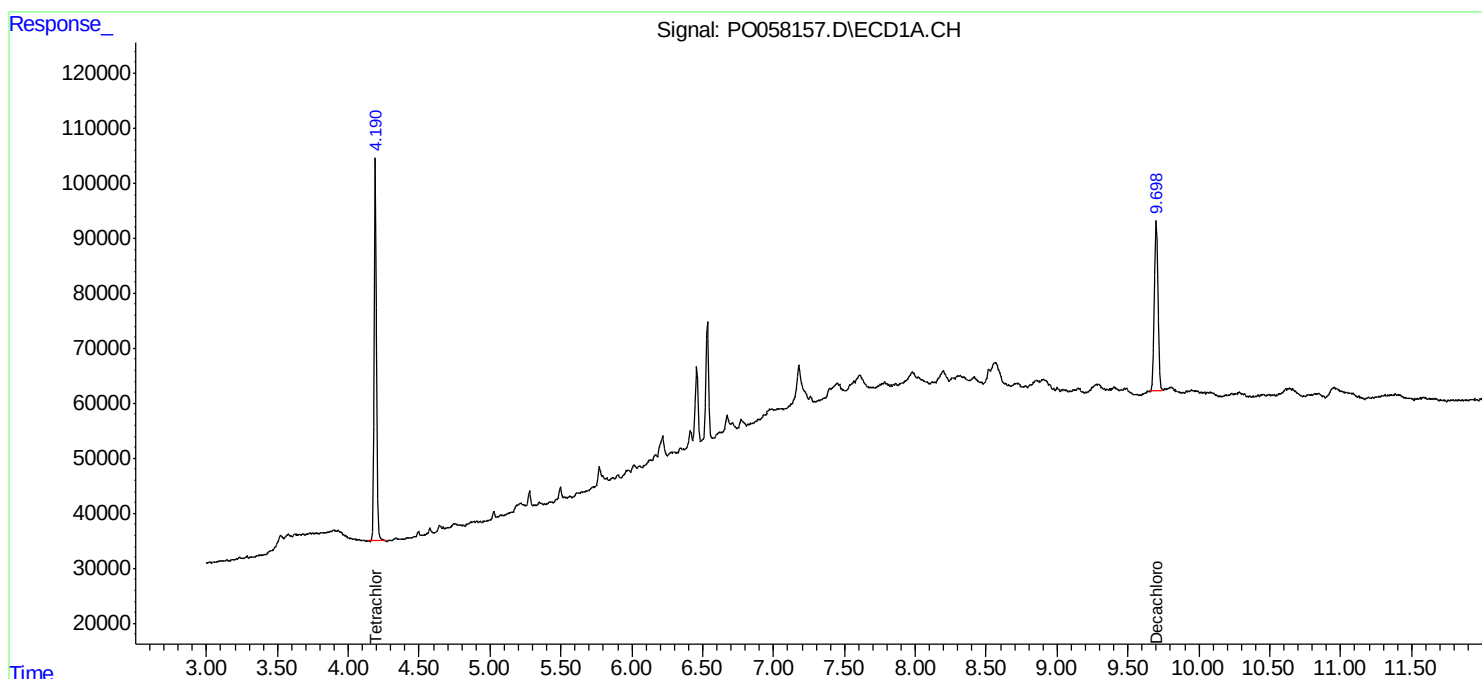

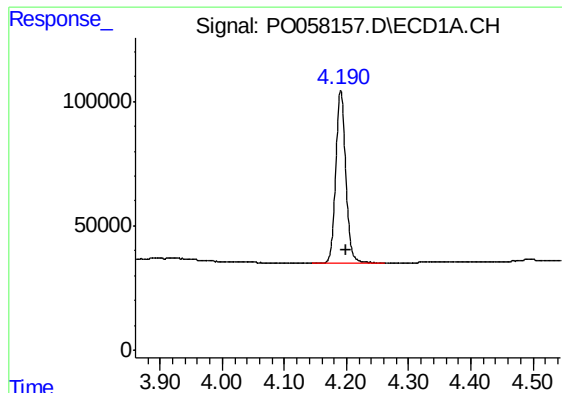


#1 Tetrachloro-m-xylene

R.T.: 4.191 min
Delta R.T.: -0.009 min
Response: 778955
Conc: 22.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-053RE


Manual Integrations
APPROVED

Ankita
7/21/2019 12:01:49 PM

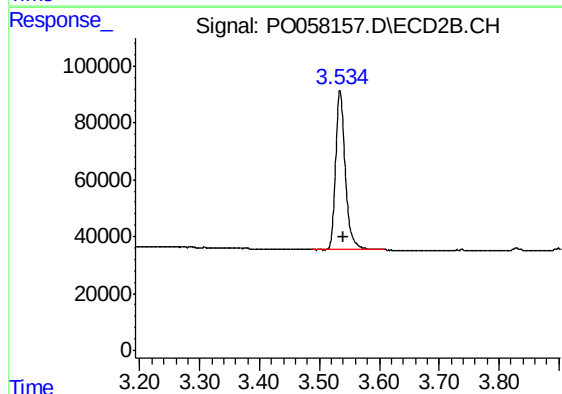


#1 Tetrachloro-m-xylene

R.T.: 3.535 min
Delta R.T.: -0.005 min
Response: 628054
Conc: 19.58 ng/ml

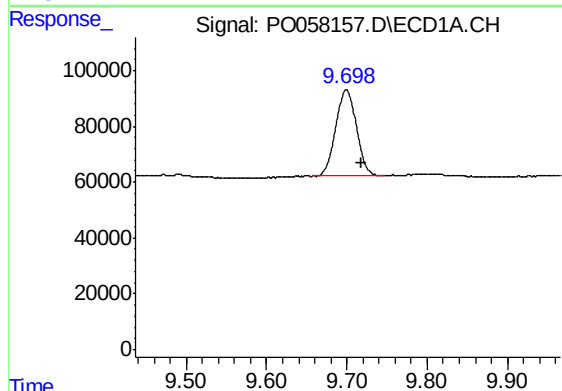

#2 Decachlorobiphenyl

R.T.: 9.698 min
Delta R.T.: -0.020 min
Response: 552469
Conc: 10.80 ng/ml m

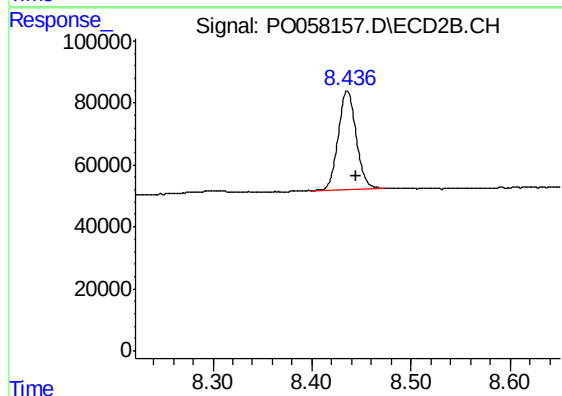

#2 Decachlorobiphenyl

R.T.: 8.436 min
Delta R.T.: -0.009 min
Response: 402307
Conc: 11.74 ng/ml