

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072019\
 Data File : P0058165.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Jul 2019 17:08
 Operator : SM/AJ
 Sample : K3783-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KY030LC018-SD-190711

Manual Integrations
 APPROVED

Ankita
 7/21/2019 12:01:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 01:32:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.193	3.536	627041	556538	18.504	17.352
2)	SA Decachlor...	9.706	8.439	405285	263784	7.922	7.696
Target Compounds							
26)	L6 AR-1254-1	6.191	5.385	157671	129744	80.232m	63.679
27)	L6 AR-1254-2	6.408	5.530	248737	123993	76.089m	68.424
28)	L6 AR-1254-3	6.772	5.928	242217	223995	68.660m	76.489
29)	L6 AR-1254-4	7.055	6.155	186464	115739	63.020m	62.642
30)	L6 AR-1254-5	7.468	6.566	185494	146184	63.195m	53.774

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO072019\
Data File : PO058165.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Jul 2019 17:08
Operator : SM/AJ
Sample : K3783-03
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KY030LC018-SD-190711


Manual Integrations
APPROVED

Ankita
7/21/2019 12:01:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 01:32:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

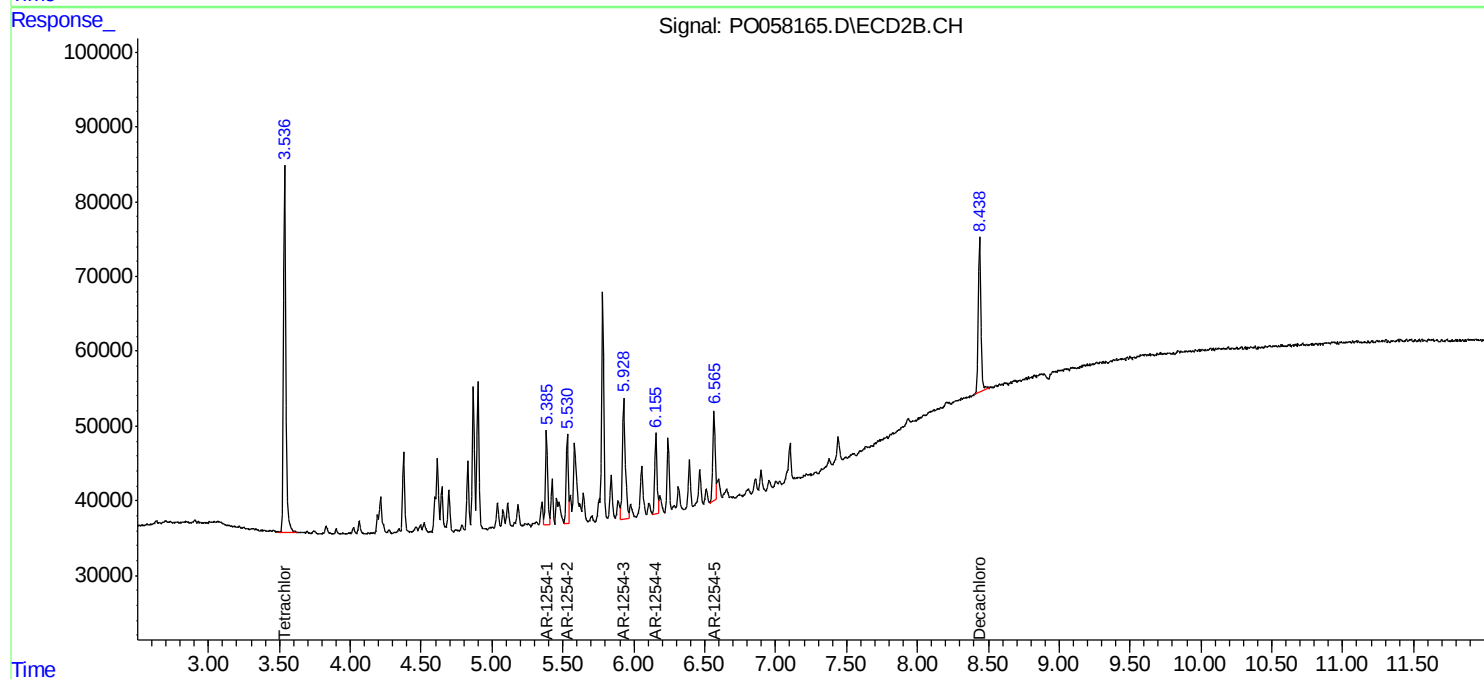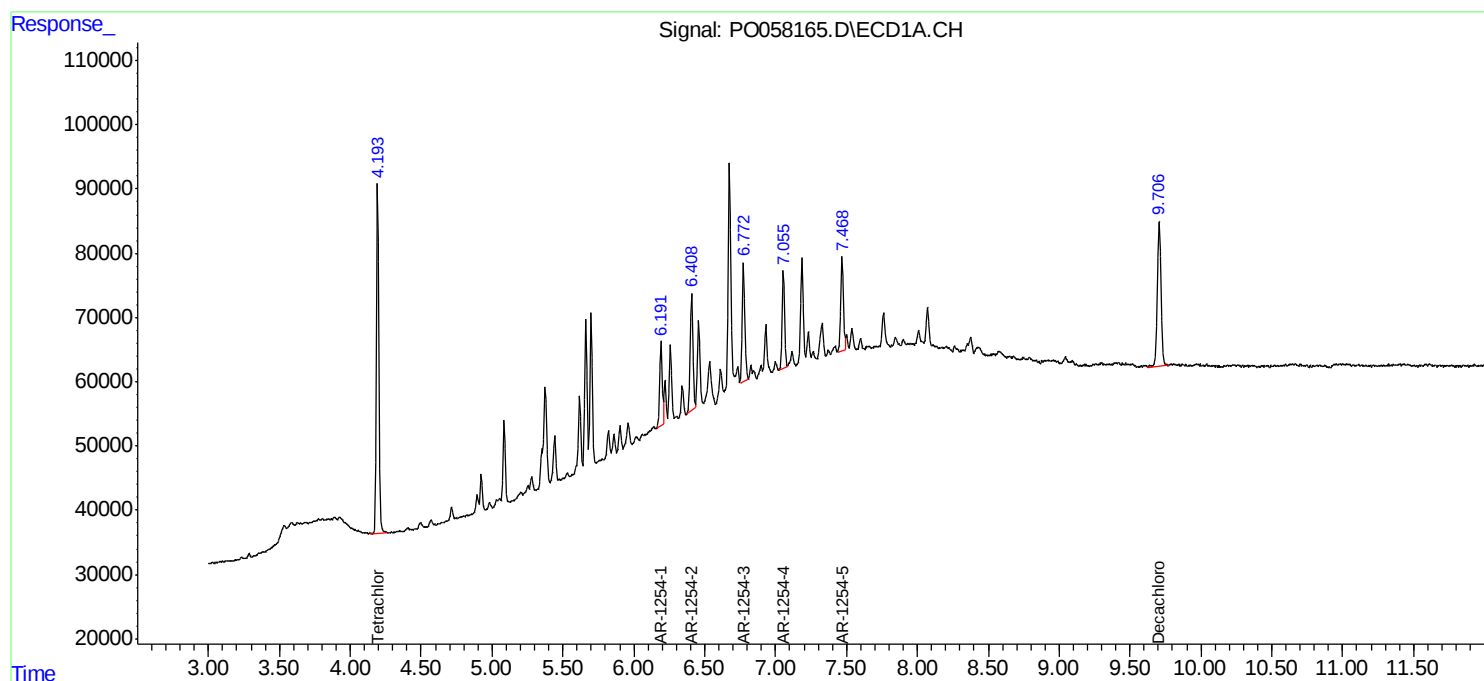

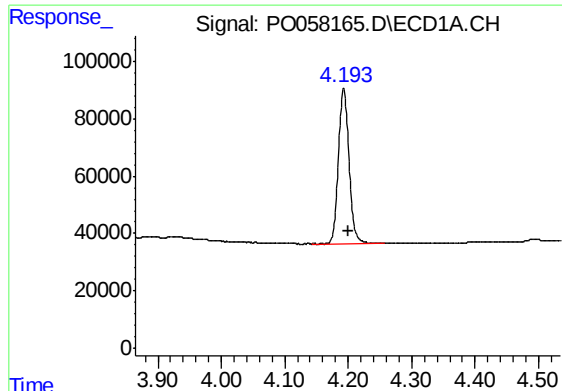


#1 Tetrachloro-m-xylene

R.T.: 4.193 min
Delta R.T.: -0.007 min
Response: 627041
Conc: 18.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
KY030LC018-SD-190711


Manual Integrations
APPROVED

Ankita
7/21/2019 12:01:58 PM

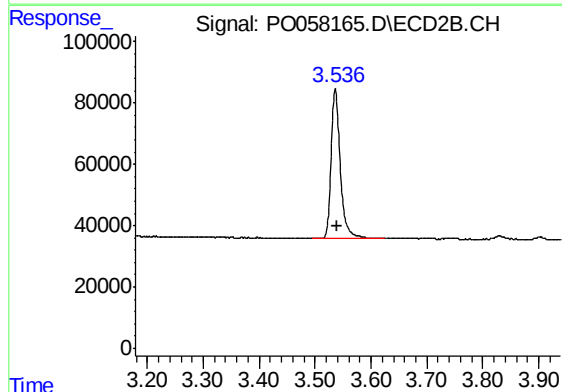


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: -0.003 min
Response: 556538
Conc: 17.35 ng/ml

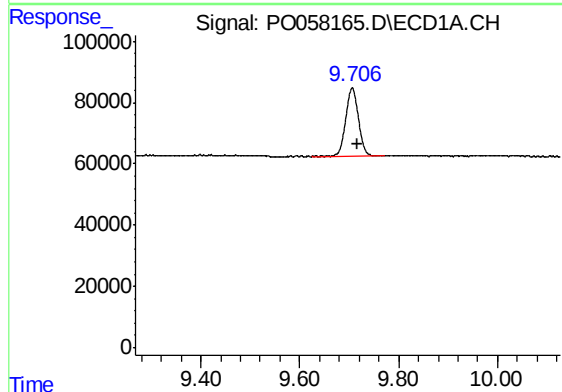


#2 Decachlorobiphenyl

R.T.: 9.706 min
Delta R.T.: -0.012 min
Response: 405285
Conc: 7.92 ng/ml

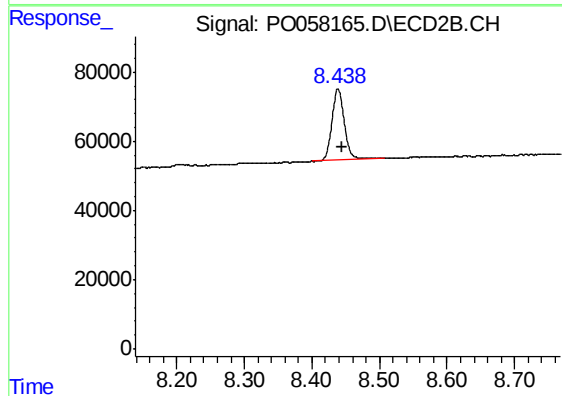

#2 Decachlorobiphenyl

R.T.: 8.439 min
Delta R.T.: -0.006 min
Response: 263784
Conc: 7.70 ng/ml

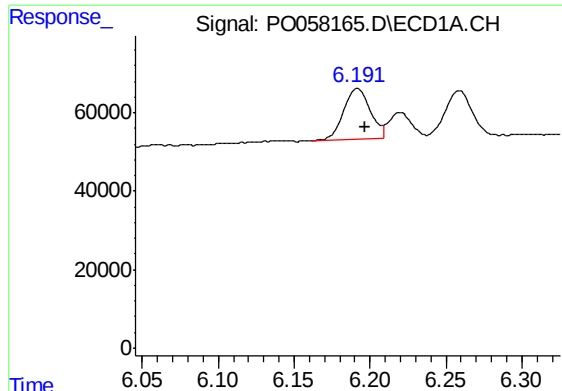


#26 AR-1254-1

R.T.: 6.191 min
Delta R.T.: -0.005 min
Response: 157671
Conc: 80.23 ng/ml m

Instrument :
ECD_O
ClientSampleId :
KY030LC018-SD-190711


Manual Integrations
APPROVED

Ankita
7/21/2019 12:01:58 PM

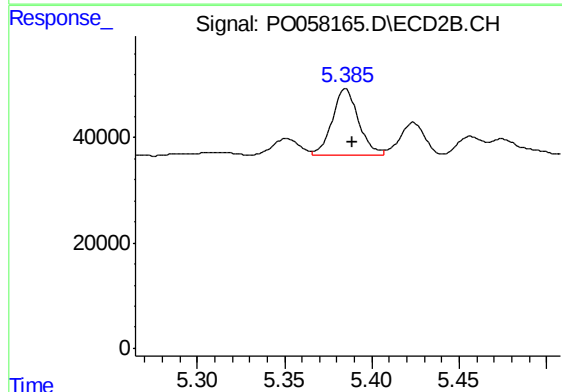


#26 AR-1254-1

R.T.: 5.385 min
Delta R.T.: -0.004 min
Response: 129744
Conc: 63.68 ng/ml

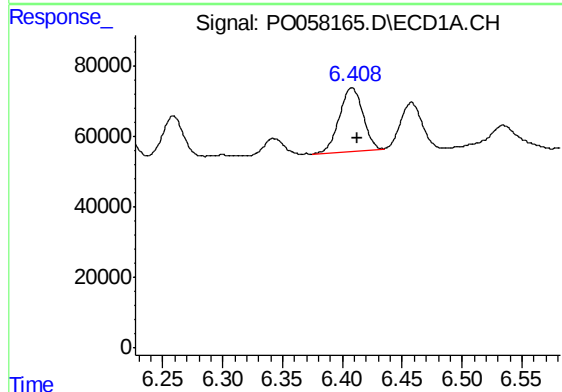


#27 AR-1254-2

R.T.: 6.408 min
Delta R.T.: -0.005 min
Response: 248737
Conc: 76.09 ng/ml m

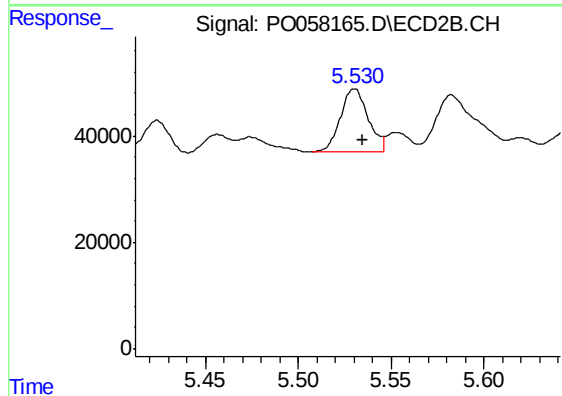

#27 AR-1254-2

R.T.: 5.530 min
Delta R.T.: -0.004 min
Response: 123993
Conc: 68.42 ng/ml

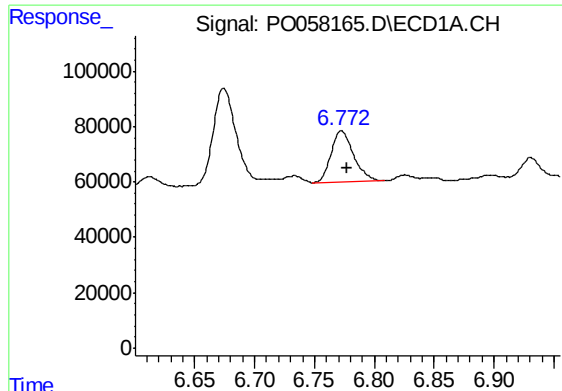


#28 AR-1254-3

R.T.: 6.772 min
Delta R.T.: -0.005 min
Response: 242217
Conc: 68.66 ng/ml m

Instrument :
ECD_O
ClientSampleId :
KY030LC018-SD-190711


Manual Integrations
APPROVED

Ankita
7/21/2019 12:01:58 PM

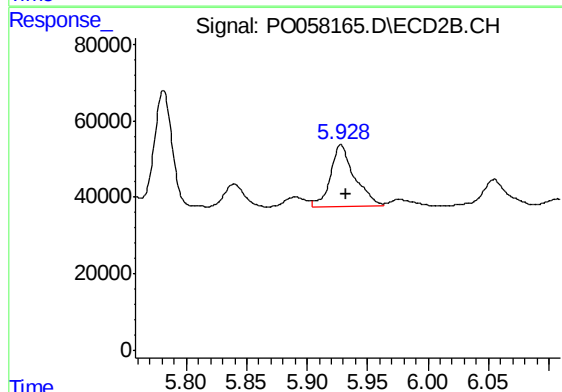


#28 AR-1254-3

R.T.: 5.928 min
Delta R.T.: -0.004 min
Response: 223995
Conc: 76.49 ng/ml

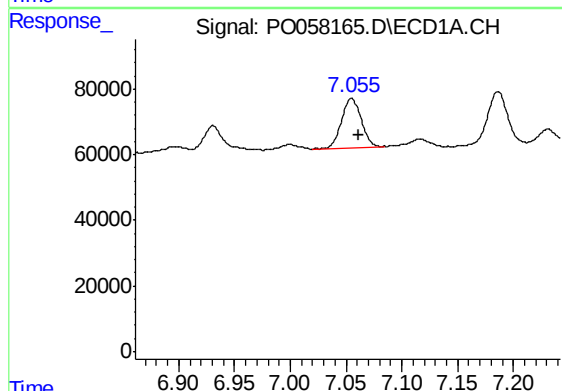


#29 AR-1254-4

R.T.: 7.055 min
Delta R.T.: -0.007 min
Response: 186464
Conc: 63.02 ng/ml m

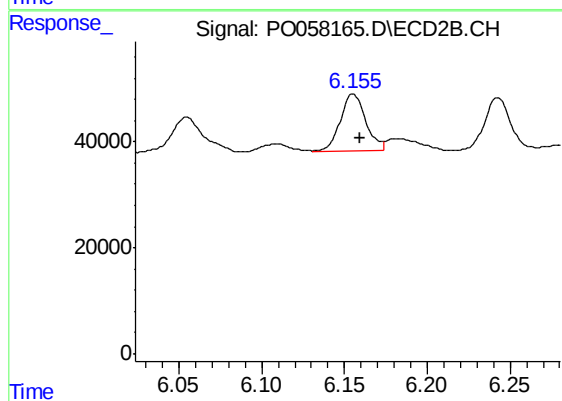

#29 AR-1254-4

R.T.: 6.155 min
Delta R.T.: -0.004 min
Response: 115739
Conc: 62.64 ng/ml

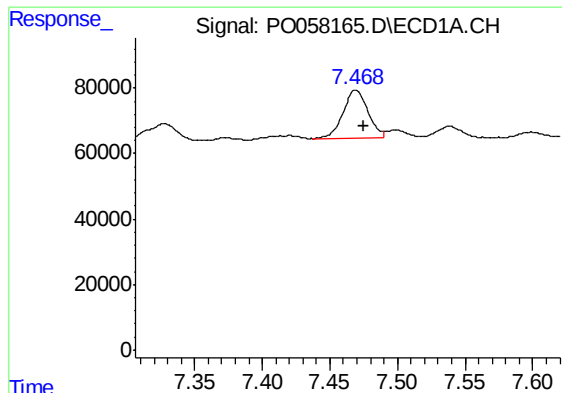


#30 AR-1254-5

R.T.: 7.468 min
Delta R.T.: -0.007 min
Response: 185494
Conc: 63.20 ng/ml m

Instrument :
ECD_O
ClientSampleId :
KY030LC018-SD-190711

Manual Integrations
APPROVED

Ankita
7/21/2019 12:01:58 PM

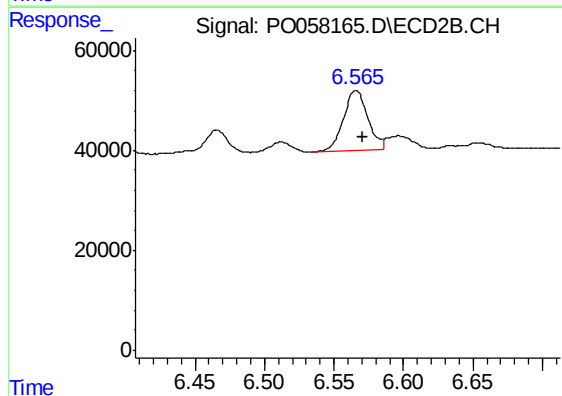

#30 AR-1254-5

R.T.: 6.566 min
Delta R.T.: -0.005 min
Response: 146184
Conc: 53.77 ng/ml