

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072019\
Data File : P0058191.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jul 2019 1:43
Operator : SM/AJ
Sample : K3866-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
RT-1488

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 03:29:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.193	3.536	699218	685119	20.634	21.361
2) SA Decachlor...	9.704	8.438	800729	556948	15.652	16.249

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072019\
Data File : P0058191.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jul 2019 1:43
Operator : SM/AJ
Sample : K3866-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
RT-1488

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 03:29:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

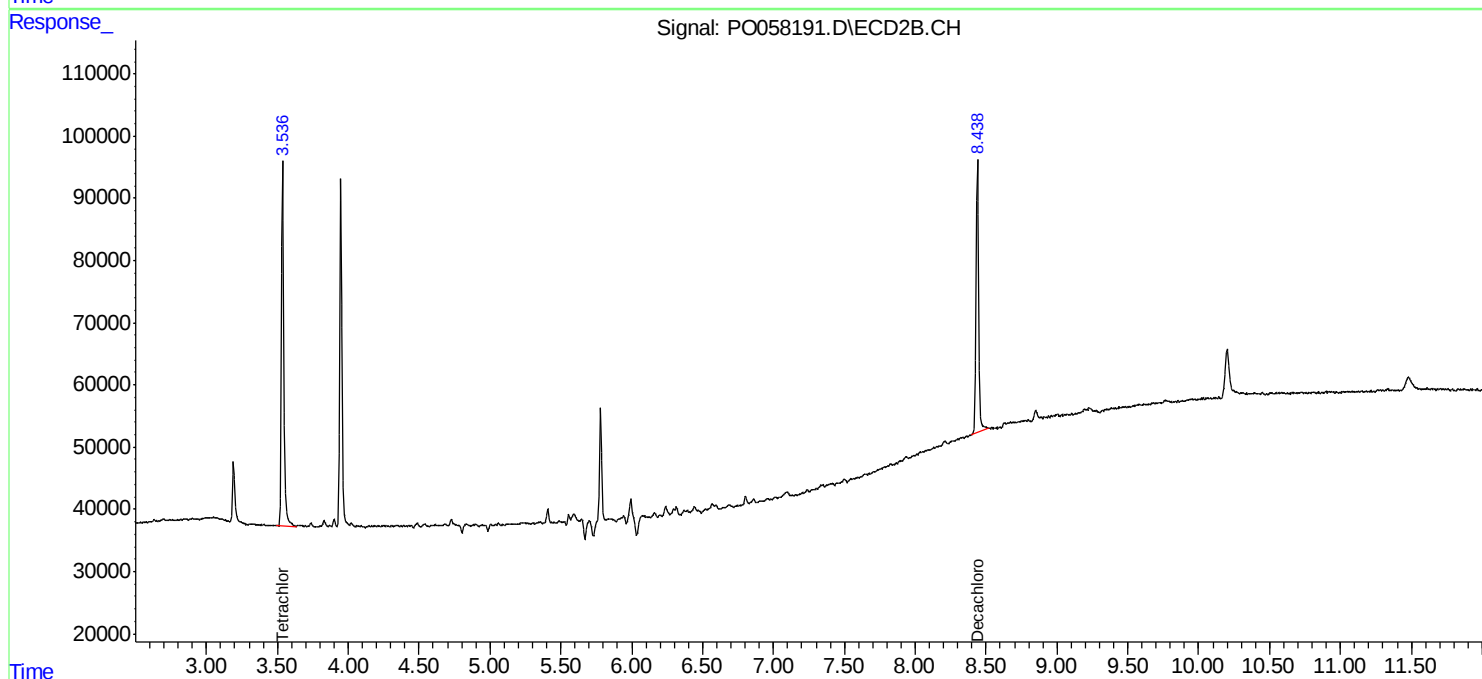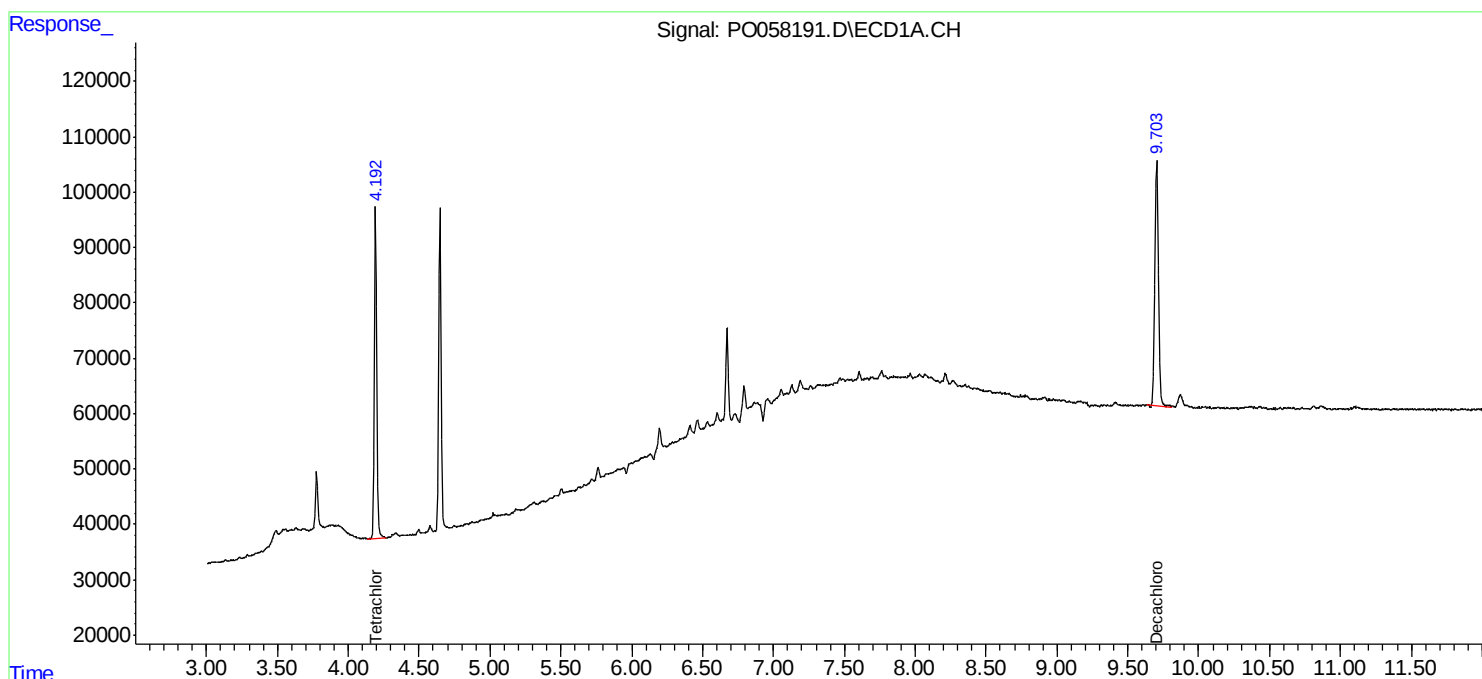


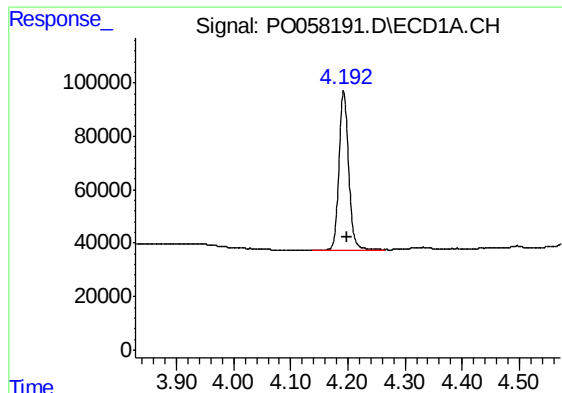

#1 Tetrachloro-m-xylene


R.T.: 4.193 min
Delta R.T.: -0.007 min
Response: 699218
Conc: 20.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
RT-1488

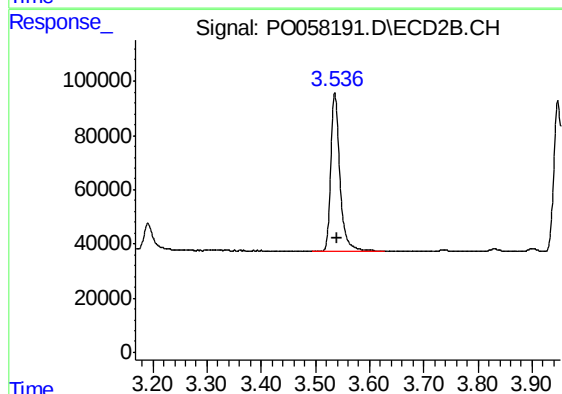


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: -0.004 min
Response: 685119
Conc: 21.36 ng/ml

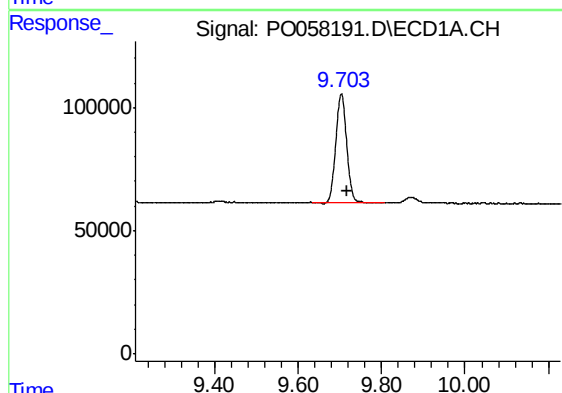

#2 Decachlorobiphenyl

R.T.: 9.704 min
Delta R.T.: -0.014 min
Response: 800729
Conc: 15.65 ng/ml

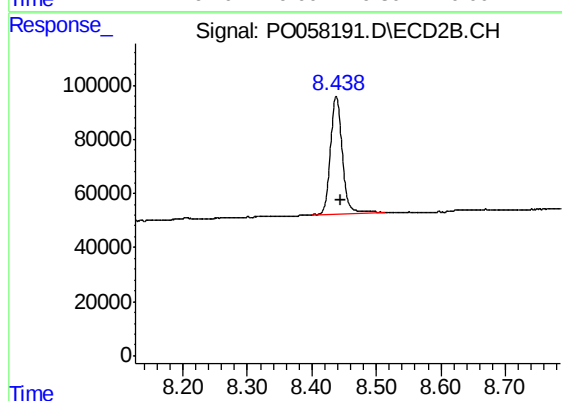

#2 Decachlorobiphenyl

R.T.: 8.438 min
Delta R.T.: -0.007 min
Response: 556948
Conc: 16.25 ng/ml