

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072019\
 Data File : P0058208.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jul 2019 7:08
 Operator : SM/AJ
 Sample : K3868-07
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-2

Manual Integrations
 APPROVED

Ankita
 7/25/2019 3:25:28 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 06:44:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 17 11:13:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.193	3.539	1099540	937236	32.447m	29.221
2)	SA Decachlor...	9.702	8.439	1099709	650296	21.496	18.973
Target Compounds							
26)	L6 AR-1254-1	6.190	5.385	37385	47598	19.023	23.361
27)	L6 AR-1254-2	6.413	5.530	142976	66180	43.736m	36.521
28)	L6 AR-1254-3	6.768	5.928	207951	100187	58.947m	34.212m#
29)	L6 AR-1254-4	7.053	6.155	103196	72953	34.877m	39.484m
30)	L6 AR-1254-5	7.468	6.566	253096	325250	86.227m	119.644 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO072019\
Data File : PO058208.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jul 2019 7:08
Operator : SM/AJ
Sample : K3868-07
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-2


Manual Integrations
APPROVED

Ankita
7/25/2019 3:25:28 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 06:44:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO071719.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 17 11:13:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

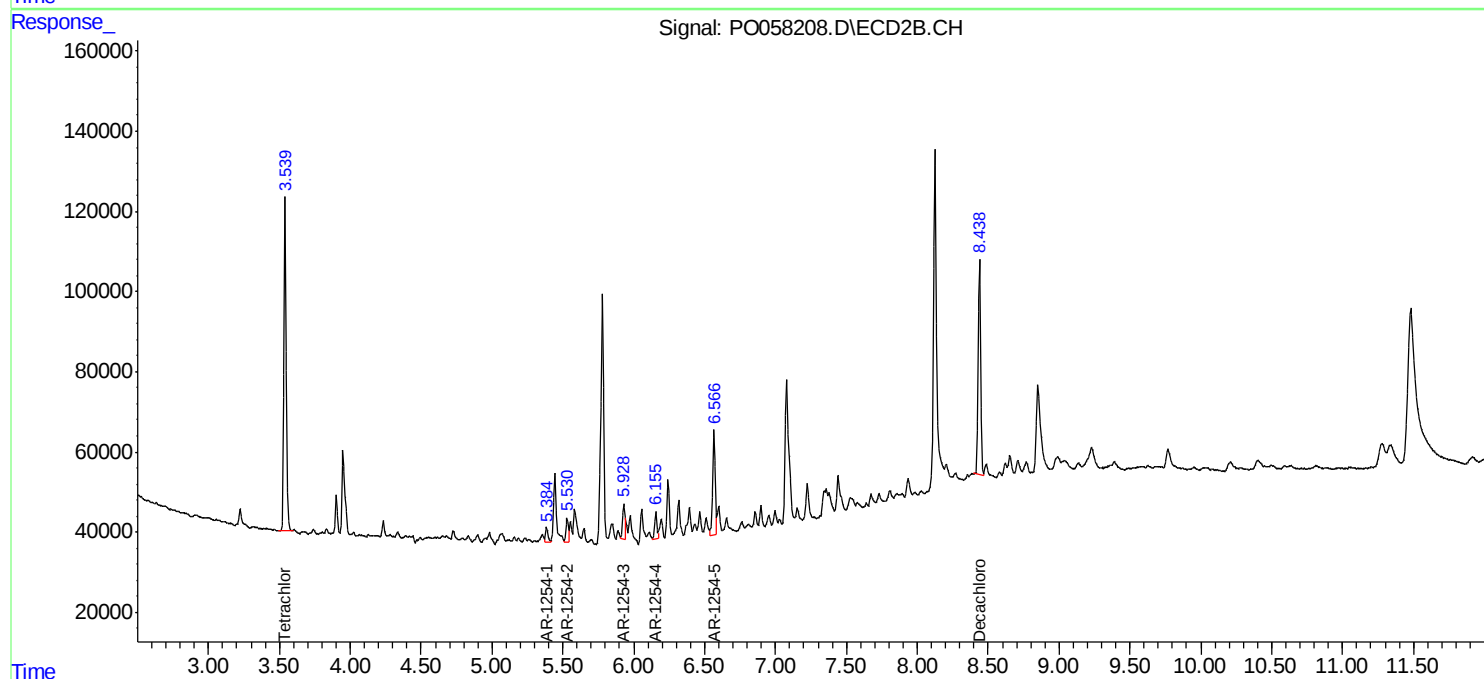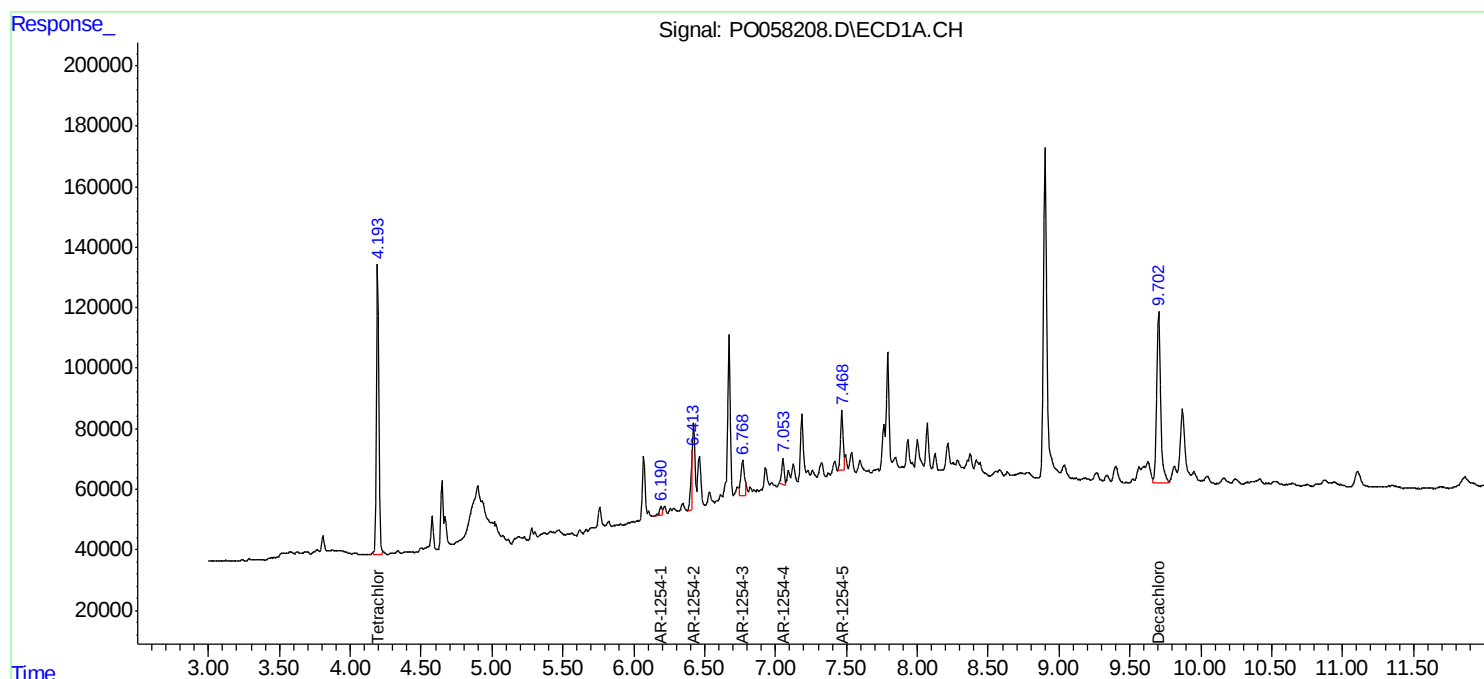

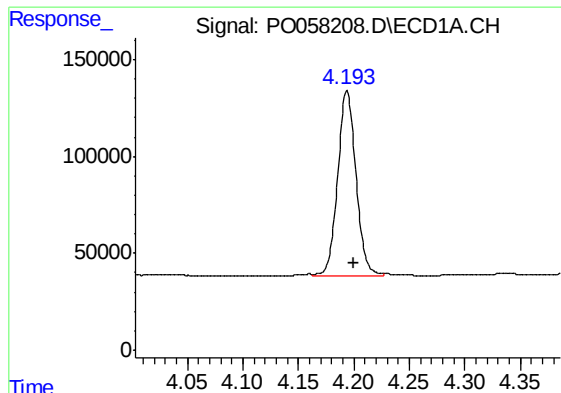


#1 Tetrachloro-m-xylene

R.T.: 4.193 min
Delta R.T.: -0.007 min
Response: 1099540
Conc: 32.45 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
7/25/2019 3:25:28 PM

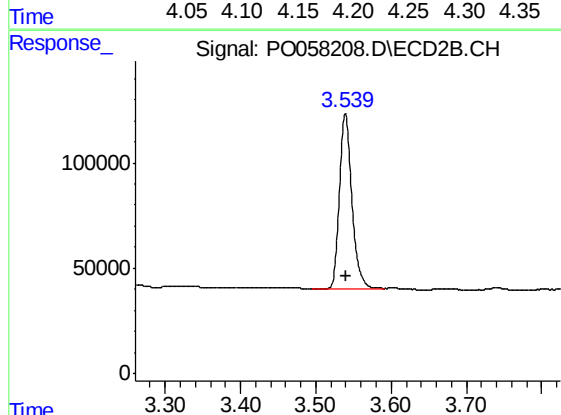


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 937236
Conc: 29.22 ng/ml

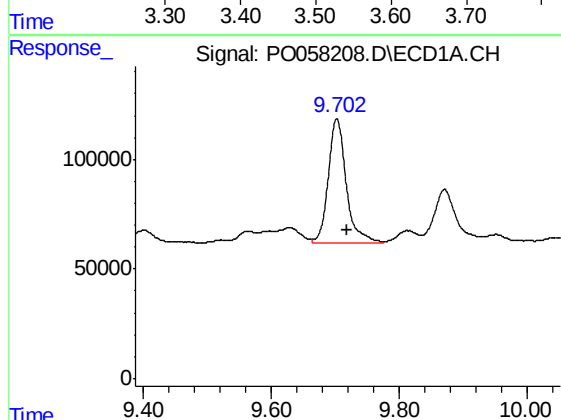


#2 Decachlorobiphenyl

R.T.: 9.702 min
Delta R.T.: -0.016 min
Response: 1099709
Conc: 21.50 ng/ml

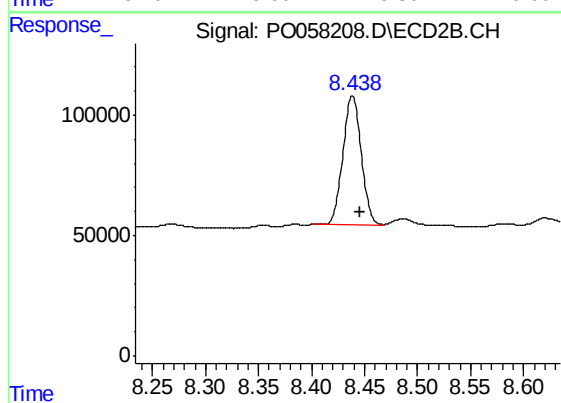

#2 Decachlorobiphenyl

R.T.: 8.439 min
Delta R.T.: -0.007 min
Response: 650296
Conc: 18.97 ng/ml

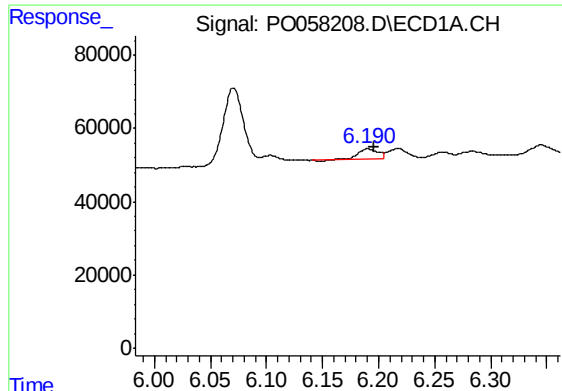


#26 AR-1254-1

R.T.: 6.190 min
Delta R.T.: -0.006 min
Response: 37385
Conc: 19.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
7/25/2019 3:25:28 PM

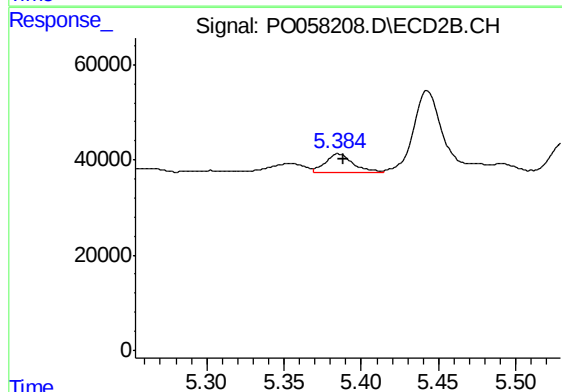


#26 AR-1254-1

R.T.: 5.385 min
Delta R.T.: -0.003 min
Response: 47598
Conc: 23.36 ng/ml

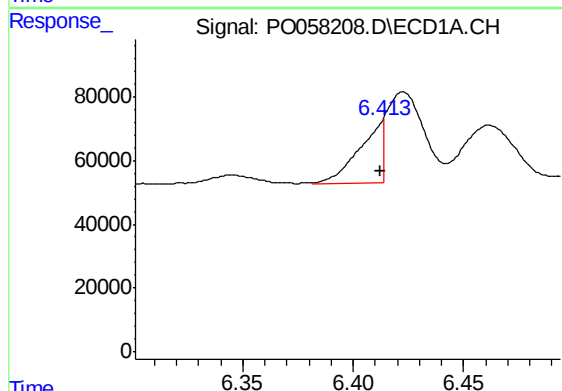


#27 AR-1254-2

R.T.: 6.413 min
Delta R.T.: 0.000 min
Response: 142976
Conc: 43.74 ng/ml m

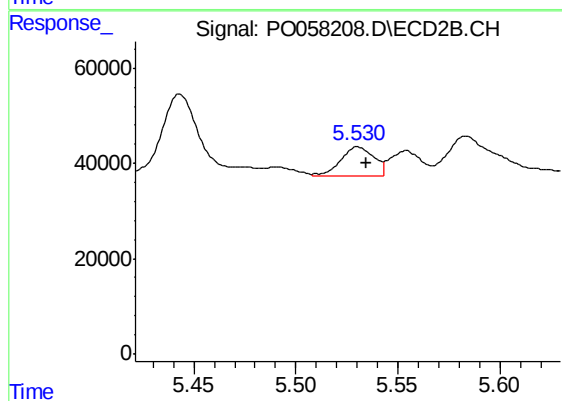

#27 AR-1254-2

R.T.: 5.530 min
Delta R.T.: -0.004 min
Response: 66180
Conc: 36.52 ng/ml

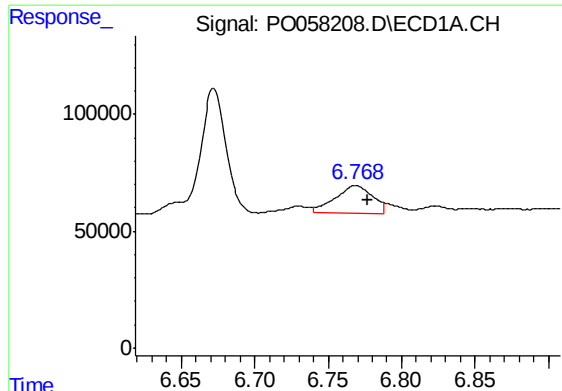


#28 AR-1254-3

R.T.: 6.768 min
Delta R.T.: -0.009 min
Response: 207951
Conc: 58.95 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
7/25/2019 3:25:28 PM

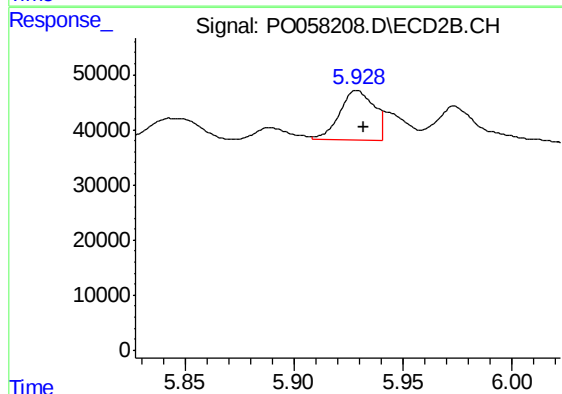


#28 AR-1254-3

R.T.: 5.928 min
Delta R.T.: -0.004 min
Response: 100187
Conc: 34.21 ng/ml m

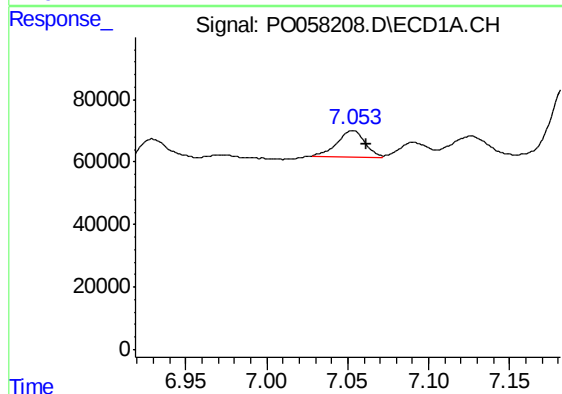


#29 AR-1254-4

R.T.: 7.053 min
Delta R.T.: -0.008 min
Response: 103196
Conc: 34.88 ng/ml m

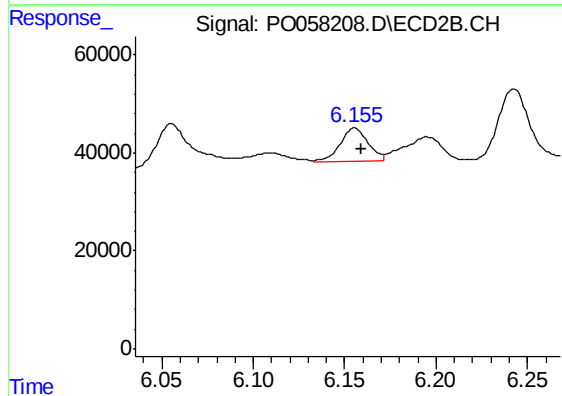

#29 AR-1254-4

R.T.: 6.155 min
Delta R.T.: -0.004 min
Response: 72953
Conc: 39.48 ng/ml m

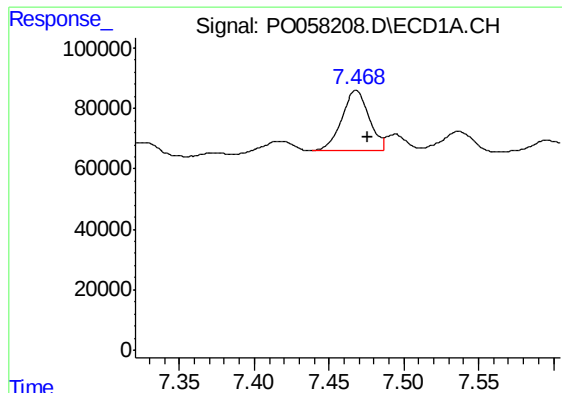


#30 AR-1254-5

R.T.: 7.468 min
Delta R.T.: -0.008 min
Response: 253096
Conc: 86.23 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-2

Manual Integrations
APPROVED

Ankita
7/25/2019 3:25:28 PM

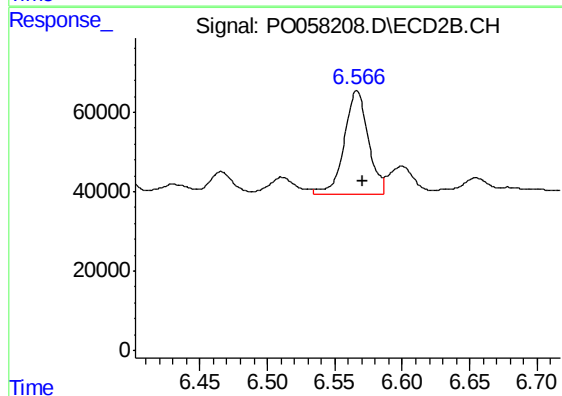

#30 AR-1254-5

R.T.: 6.566 min
Delta R.T.: -0.004 min
Response: 325250
Conc: 119.64 ng/ml