

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072020\
 Data File : P0069809.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jul 2020 10:57
 Operator : DD\AJ
 Sample : L3324-05RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TOTE-50-DIAZRE

Manual Integrations
 APPROVED

Ankita
 7/21/2020 10:38:54 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 15:52:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 08 16:12:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.388	3.561	237981	232976	6.374	5.854m
2) SA Decachlor...	10.044	8.768	241587	233383	4.015	4.112

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072020\
Data File : P0069809.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jul 2020 10:57
Operator : DD\AJ
Sample : L3324-05RE
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TOTE-50-DIAZRE


Manual Integrations
APPROVED

Ankita
7/21/2020 10:38:54 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 15:52:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 08 16:12:41 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

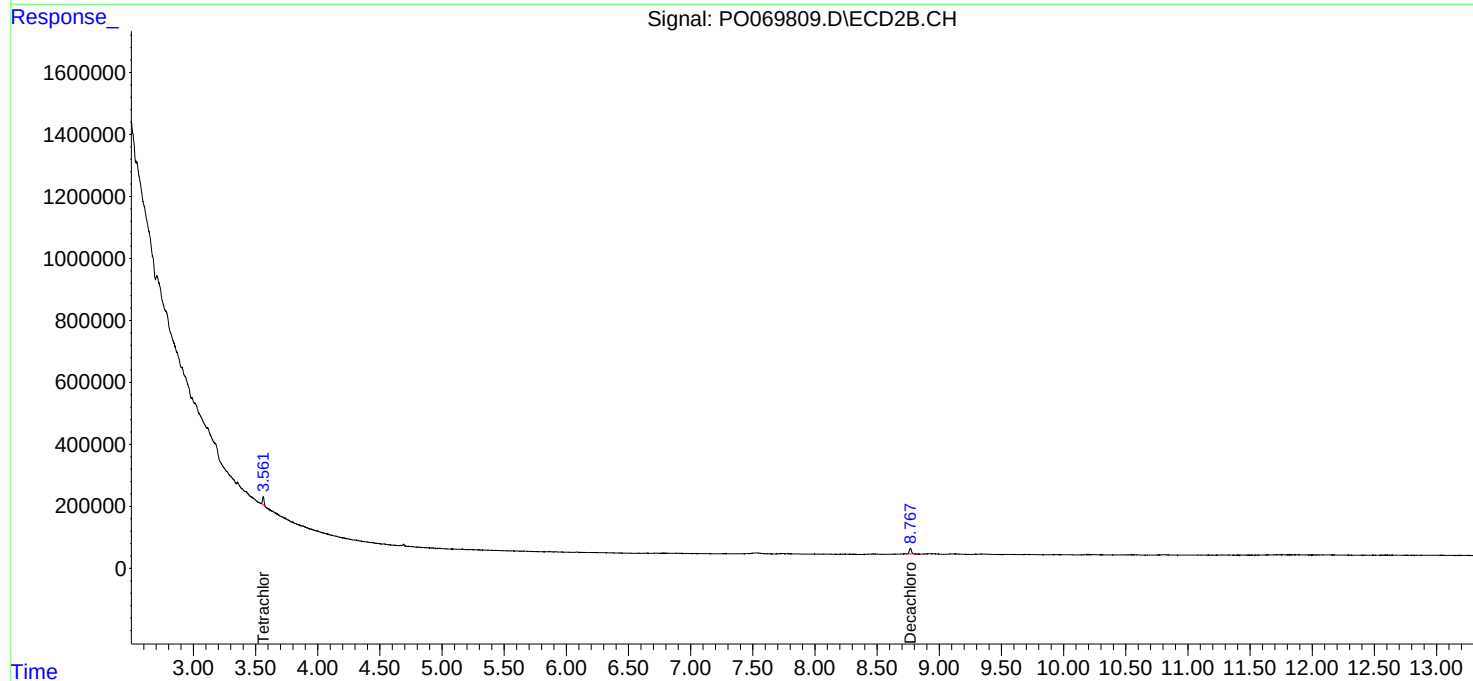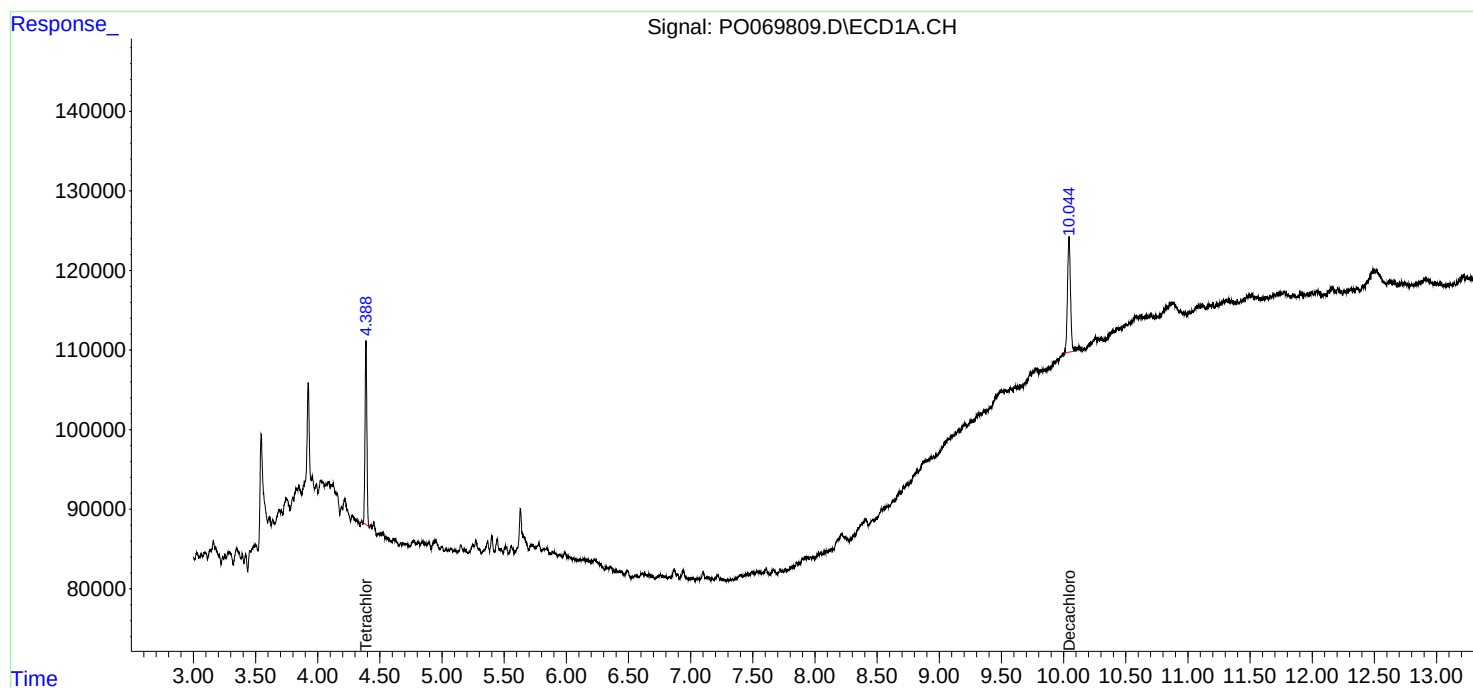

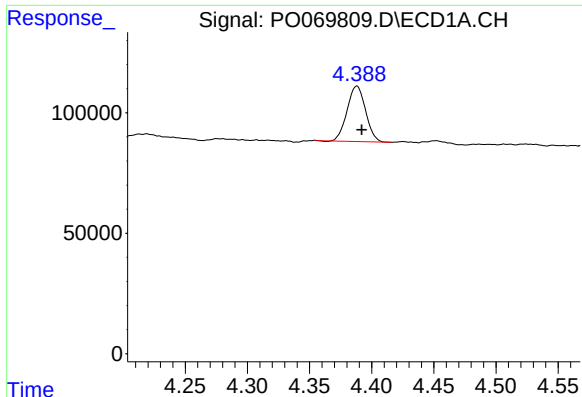


#1 Tetrachloro-m-xylene

R.T.: 4.388 min
Delta R.T.: -0.004 min
Response: 237981
Conc: 6.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
TOTE-50-DIAZRE


Manual Integrations
APPROVED

Ankita
7/21/2020 10:38:54 AM

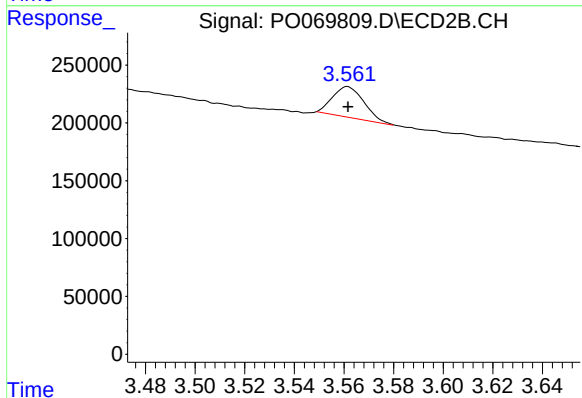


#1 Tetrachloro-m-xylene

R.T.: 3.561 min
Delta R.T.: 0.000 min
Response: 232976
Conc: 5.85 ng/ml m

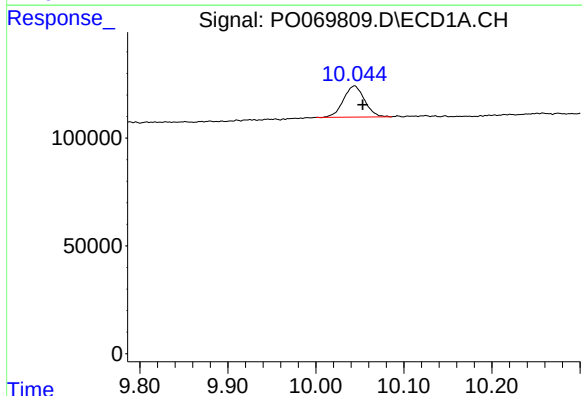

#2 Decachlorobiphenyl

R.T.: 10.044 min
Delta R.T.: -0.009 min
Response: 241587
Conc: 4.02 ng/ml

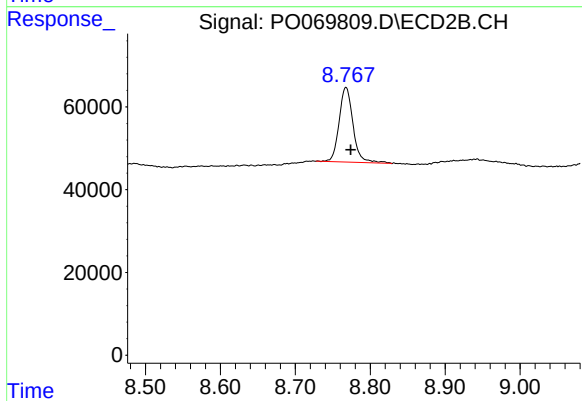

#2 Decachlorobiphenyl

R.T.: 8.768 min
Delta R.T.: -0.006 min
Response: 233383
Conc: 4.11 ng/ml