

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072021\
 Data File : P0079690.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jul 2021 12:01
 Operator : DD\AJ
 Sample : M3073-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 14:43:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 20 14:31:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.016	4.221f	1480167	521763	19.996	20.767
2)	SA Decachlor...	11.142	9.698	1186650	513531	22.069	22.592
Target Compounds							
9)	L2 AR-1221-2	5.371	0.000	12754	0	22.333	N.D. #
20)	L4 AR-1242-5	7.328	0.000	572	0	0.416	N.D. #
24)	L5 AR-1248-4	7.295	0.000	4276	0	1.648	N.D. #
25)	L5 AR-1248-5	7.328	0.000	572	0	0.231	N.D. #
26)	L6 AR-1254-1	7.263	0.000	39828	0	15.894	N.D. #
28)	L6 AR-1254-3	7.893f	0.000	28736	0	6.863	N.D. #
29)	L6 AR-1254-4	8.171	0.000	4118	0	1.387	N.D. #
32)	L7 AR-1260-2	8.314	0.000	14567	0	4.280	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072021\
Data File : P0079690.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jul 2021 12:01
Operator : DD\AJ
Sample : M3073-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 14:43:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071921.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 20 14:31:26 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

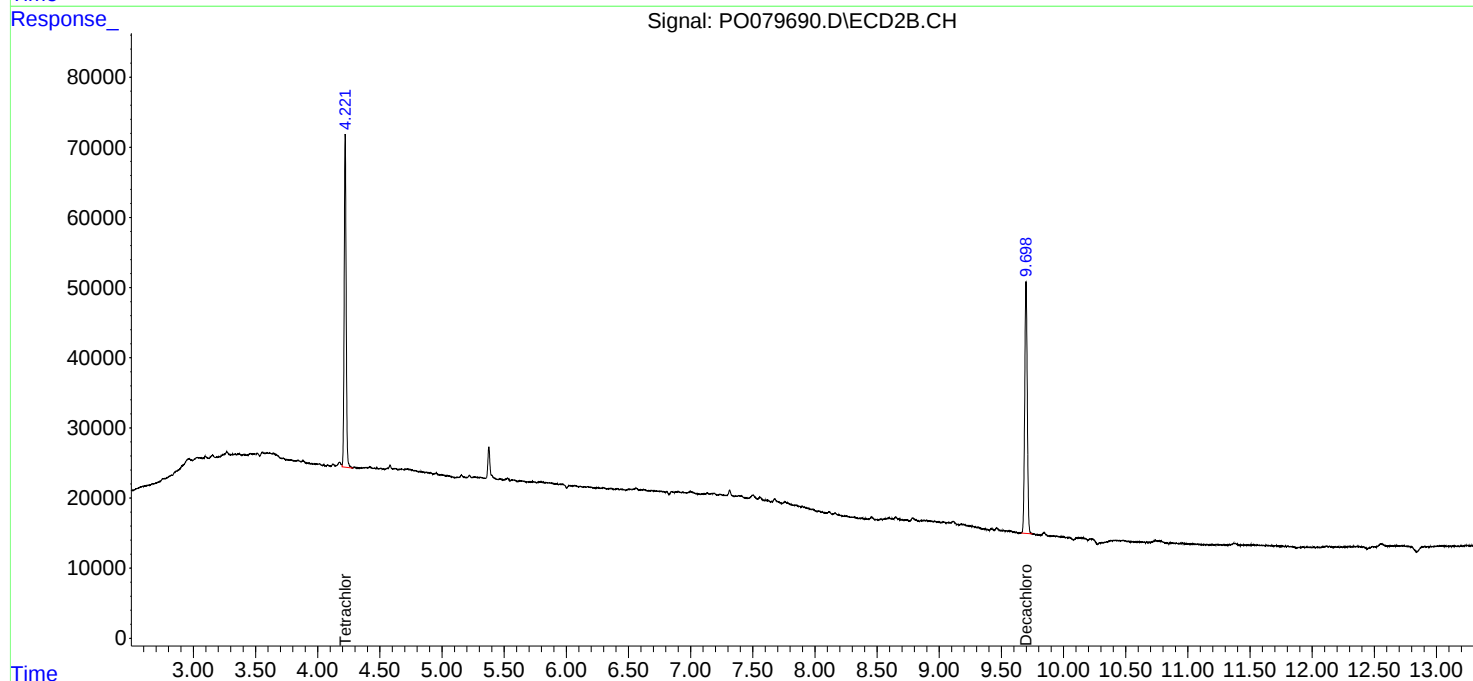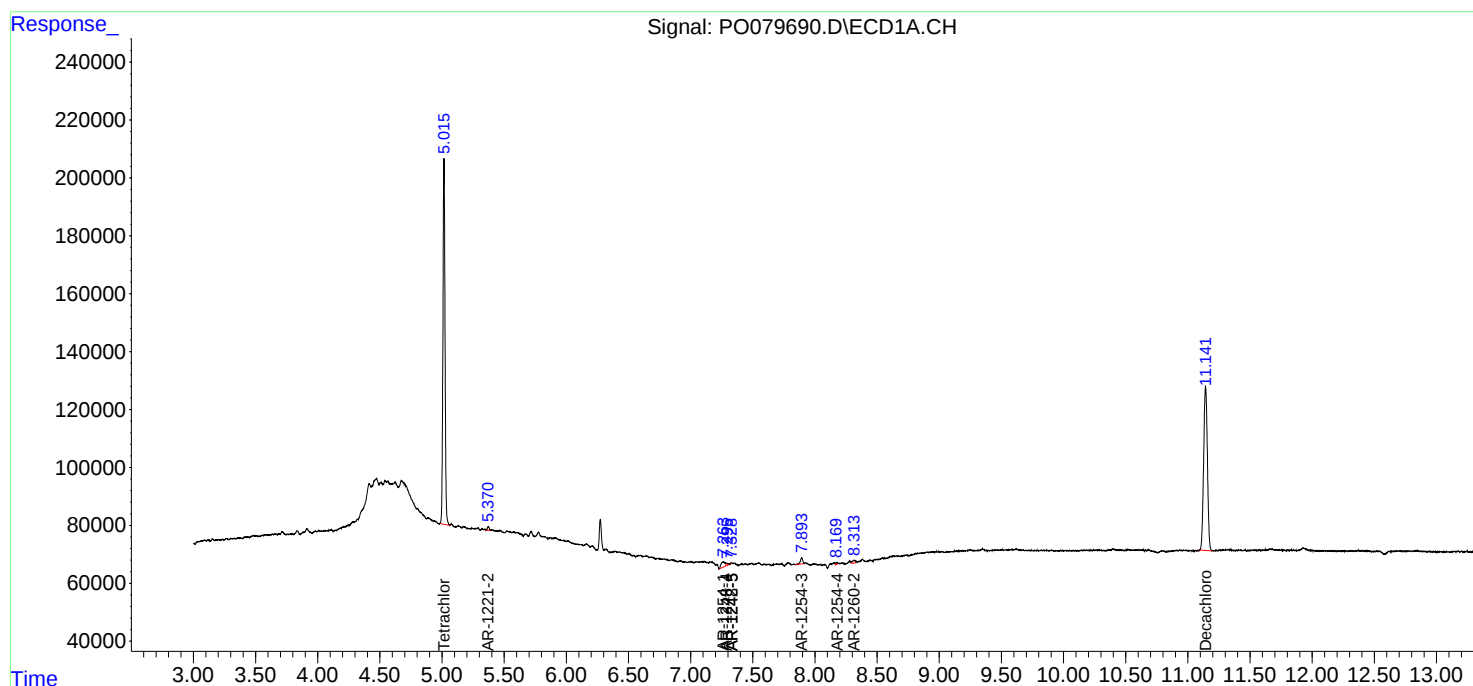


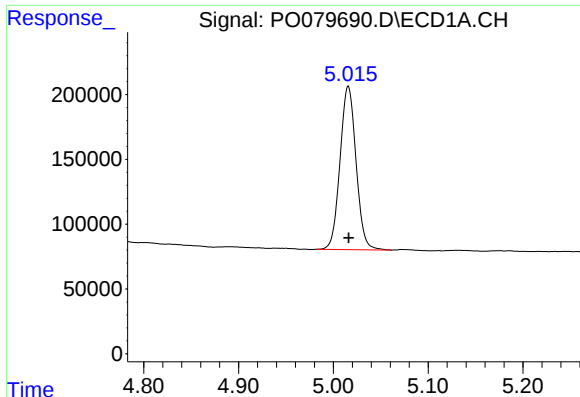

#1 Tetrachloro-m-xylene


R.T.: 5.016 min
Delta R.T.: 0.000 min
Response: 1480167
Conc: 20.00 ng/ml

Instrument :
ECD_O
ClientSampleId :

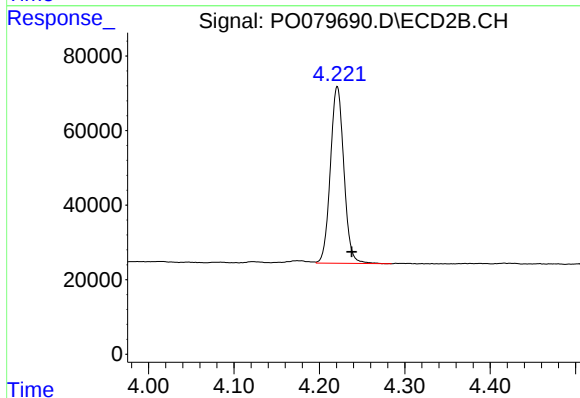


#1 Tetrachloro-m-xylene

R.T.: 4.221 min
Delta R.T.: -0.017 min
Response: 521763
Conc: 20.77 ng/ml

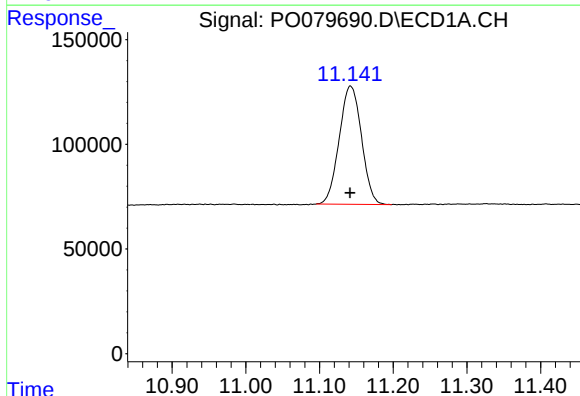


#2 Decachlorobiphenyl

R.T.: 11.142 min
Delta R.T.: 0.000 min
Response: 1186650
Conc: 22.07 ng/ml

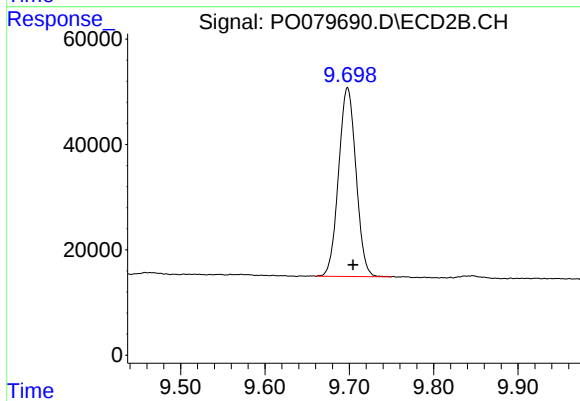

#2 Decachlorobiphenyl


R.T.: 9.698 min
Delta R.T.: -0.007 min
Response: 513531
Conc: 22.59 ng/ml

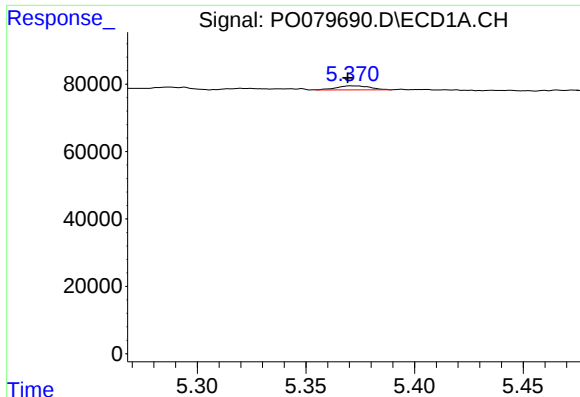

#9 AR-1221-2


R.T.: 5.371 min
Delta R.T.: 0.001 min
Response: 12754
Conc: 22.33 ng/ml

Instrument :
ECD_O
ClientSampleId :

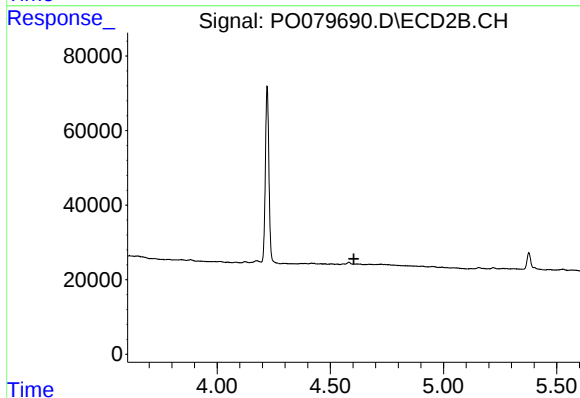


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.604 min
Response: 0
Conc: N.D.

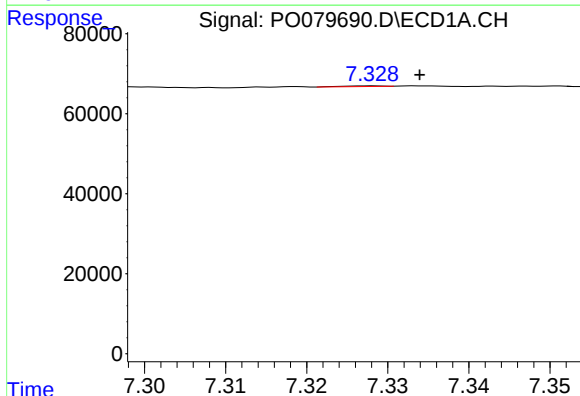


#20 AR-1242-5

R.T.: 7.328 min
Delta R.T.: -0.006 min
Response: 572
Conc: 0.42 ng/ml

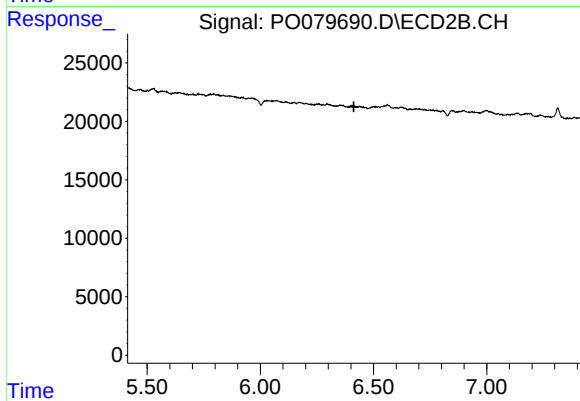

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 6.413 min
Response: 0
Conc: N.D.

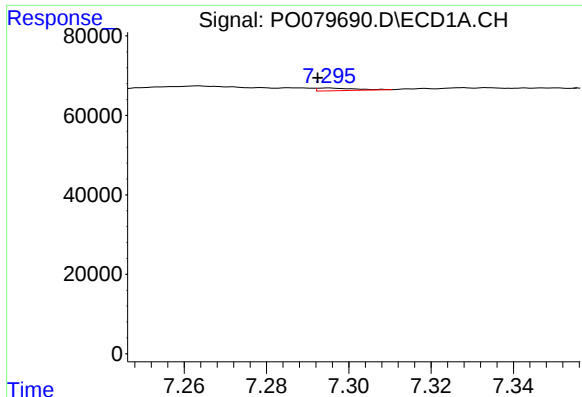

#24 AR-1248-4


R.T.: 7.295 min
Delta R.T.: 0.003 min
Response: 4276
Conc: 1.65 ng/ml

Instrument :
ECD_O
ClientSampleId :

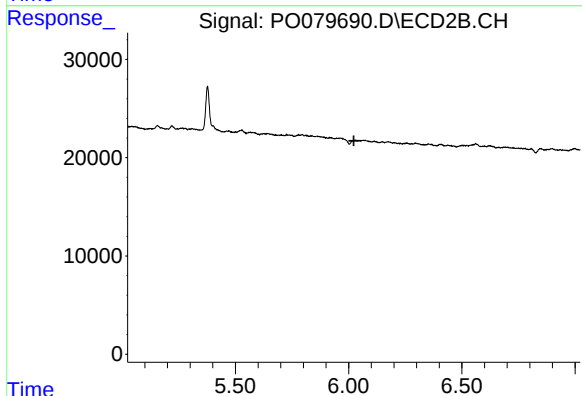


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

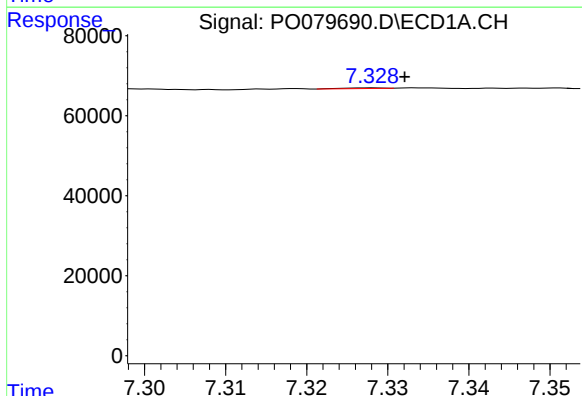


#25 AR-1248-5

R.T.: 7.328 min
Delta R.T.: -0.004 min
Response: 572
Conc: 0.23 ng/ml

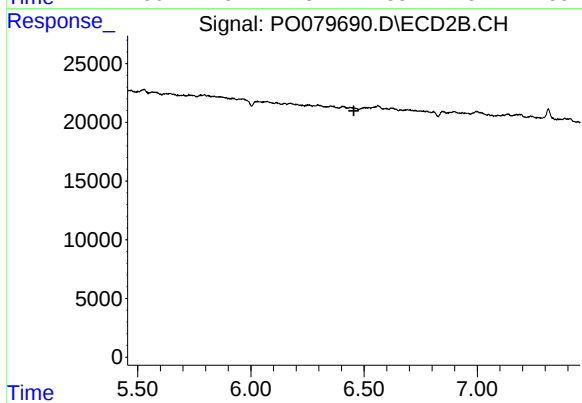

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 6.455 min
Response: 0
Conc: N.D.

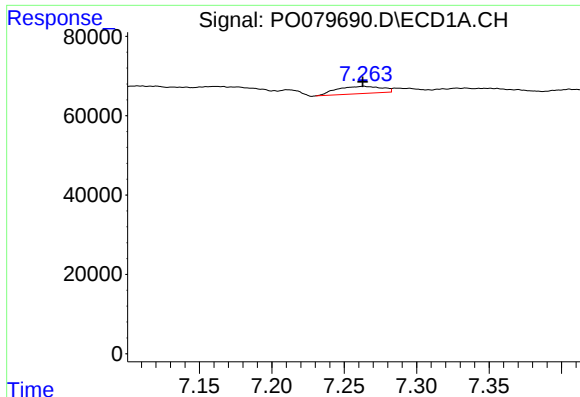

#26 AR-1254-1


R.T.: 7.263 min
Delta R.T.: 0.000 min
Response: 39828
Conc: 15.89 ng/ml

Instrument :
ECD_O
ClientSampleId :

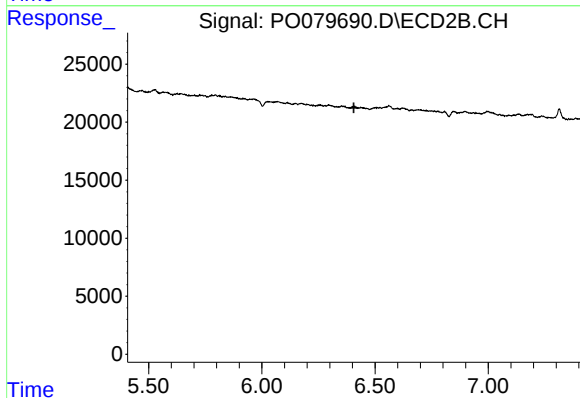


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.407 min
Response: 0
Conc: N.D.

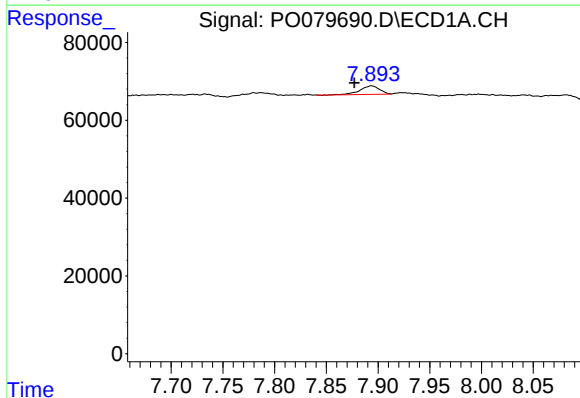


#28 AR-1254-3

R.T.: 7.893 min
Delta R.T.: 0.016 min
Response: 28736
Conc: 6.86 ng/ml

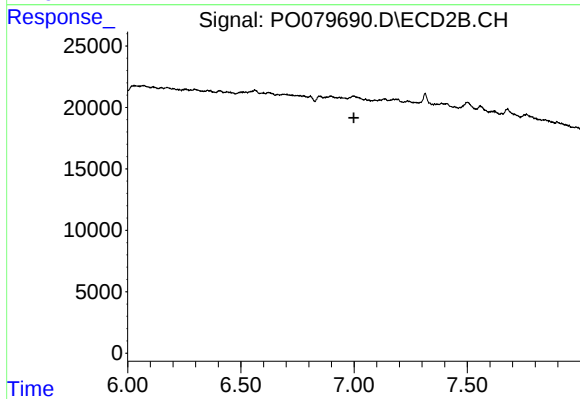

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.999 min
Response: 0
Conc: N.D.

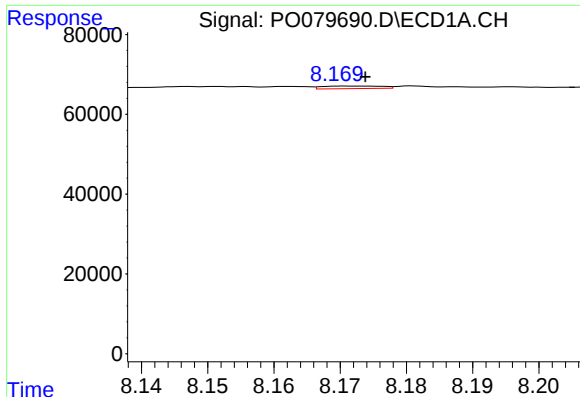

#29 AR-1254-4


R.T.: 8.171 min
Delta R.T.: -0.003 min
Response: 4118
Conc: 1.39 ng/ml

Instrument :
ECD_O
ClientSampleId :

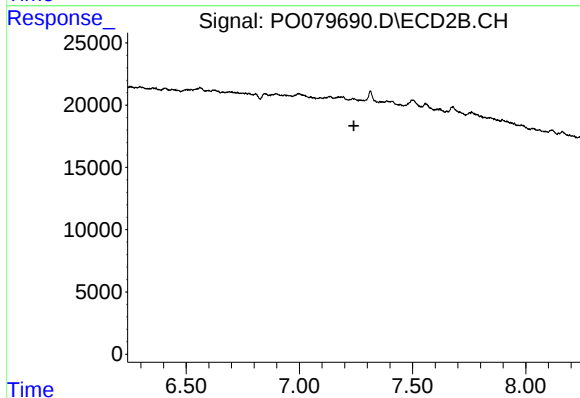


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.241 min
Response: 0
Conc: N.D.

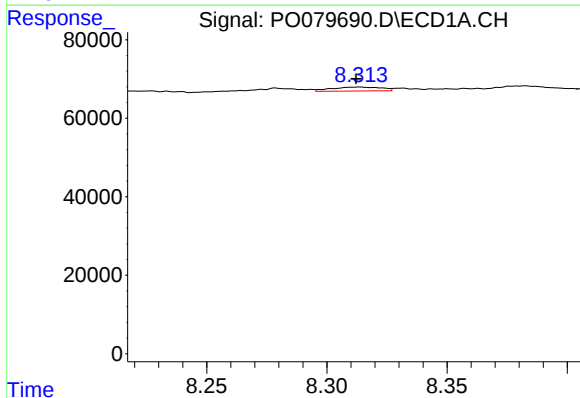

#32 AR-1260-2

R.T.: 8.314 min
Delta R.T.: 0.002 min
Response: 14567
Conc: 4.28 ng/ml

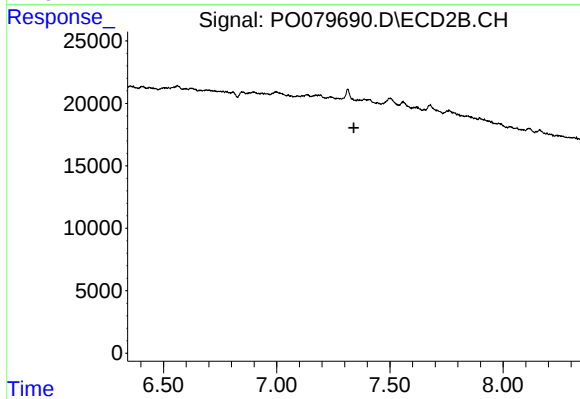

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.341 min
Response: 0
Conc: N.D.