

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072021\
 Data File : P0079701.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jul 2021 16:15
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 20 16:48:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 20 14:31:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.016	4.225	1590090	567390	21.481	22.583
2)	SA Decachlor...	11.144	9.701	1143170	507643	21.261	22.333
Target Compounds							
8)	L2 AR-1221-1	5.268	0.000	44039	0	56.334	N.D. #
9)	L2 AR-1221-2	5.371	0.000	18817	0	32.950	N.D. #
15)	L3 AR-1232-5	6.640	0.000	17418	0	31.278	N.D. #
22)	L5 AR-1248-2	6.640	0.000	17418	0	8.627	N.D. #
24)	L5 AR-1248-4	7.285	0.000	286	0	0.110	N.D. #
26)	L6 AR-1254-1	7.269	0.000	14124	0	5.637	N.D. #
28)	L6 AR-1254-3	7.893f	0.000	23755	0	5.673	N.D. #
32)	L7 AR-1260-2	8.313	7.316f	8230	18233	2.418	11.032 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072021\
Data File : P0079701.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jul 2021 16:15
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 20 16:48:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071921.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 20 14:31:26 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

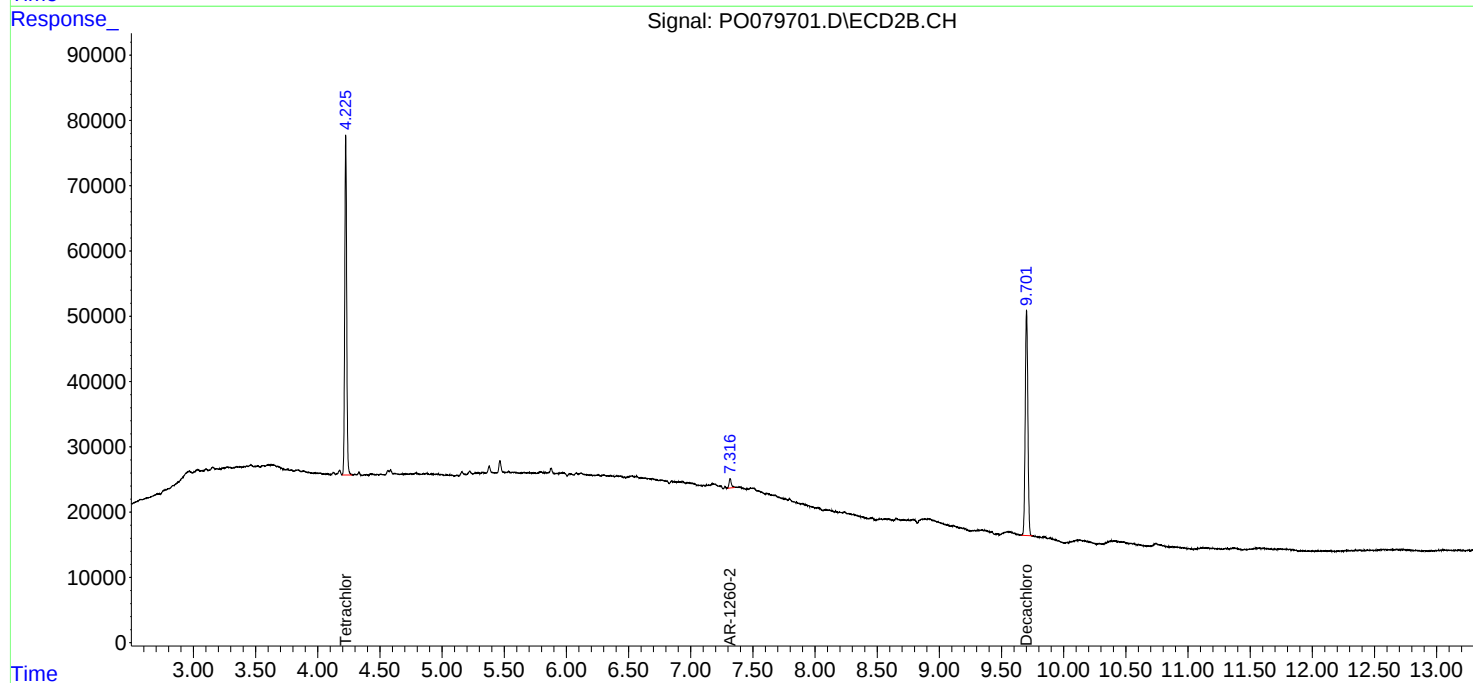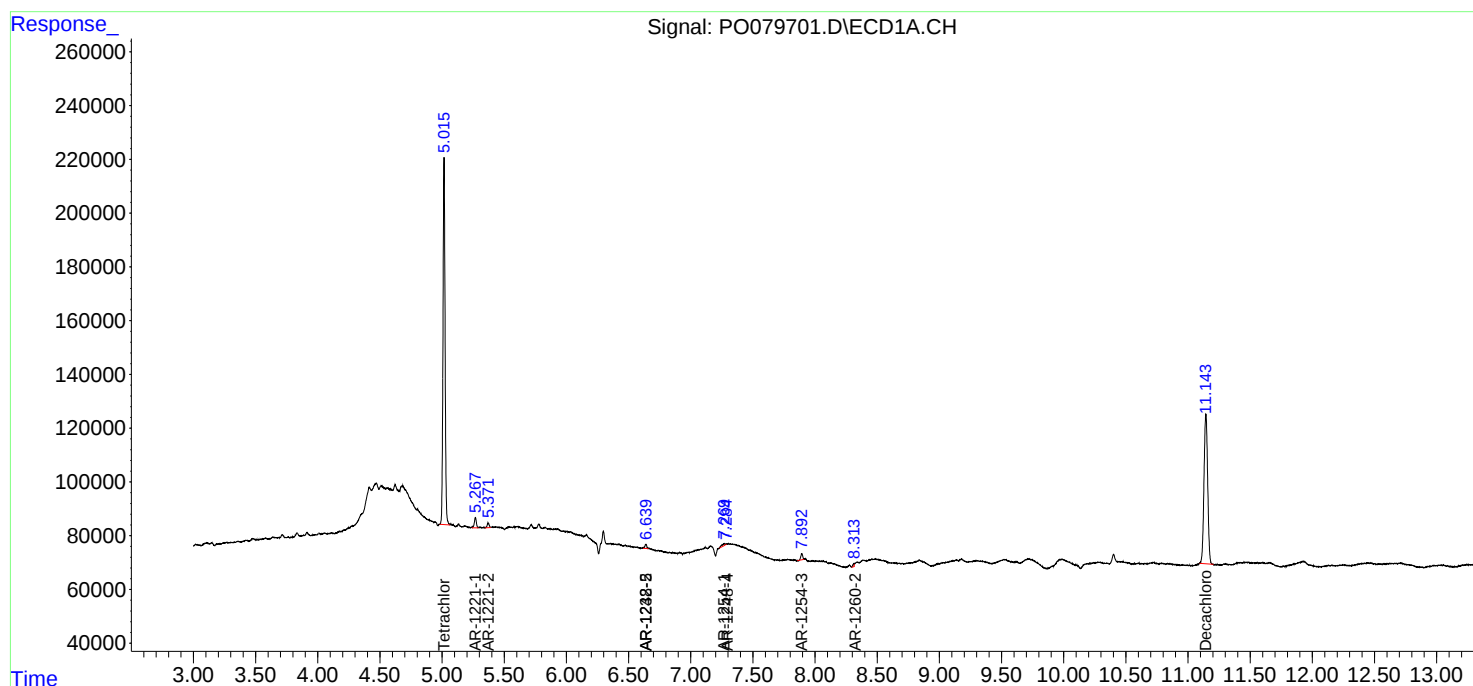


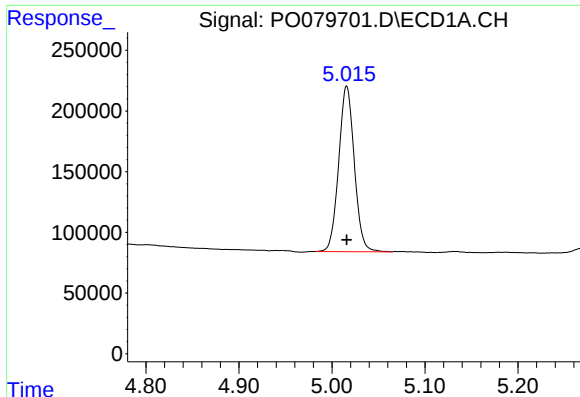

#1 Tetrachloro-m-xylene


R.T.: 5.016 min
Delta R.T.: 0.000 min
Response: 1590090
Conc: 21.48 ng/ml

Instrument :
ECD_O
ClientSampleId :

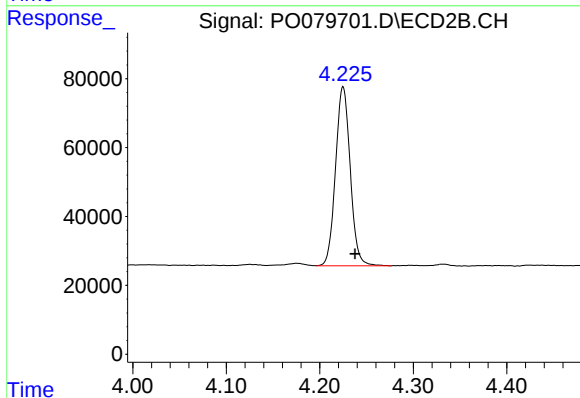


#1 Tetrachloro-m-xylene

R.T.: 4.225 min
Delta R.T.: -0.013 min
Response: 567390
Conc: 22.58 ng/ml

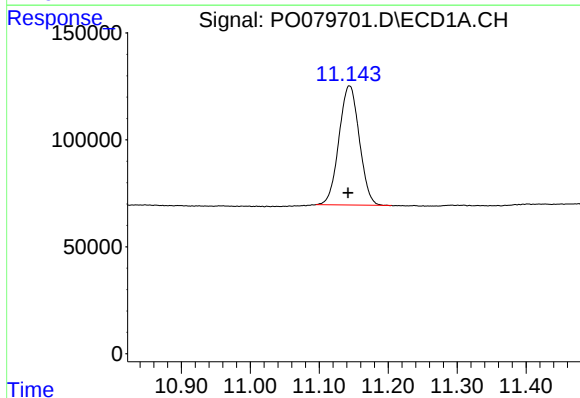


#2 Decachlorobiphenyl

R.T.: 11.144 min
Delta R.T.: 0.002 min
Response: 1143170
Conc: 21.26 ng/ml

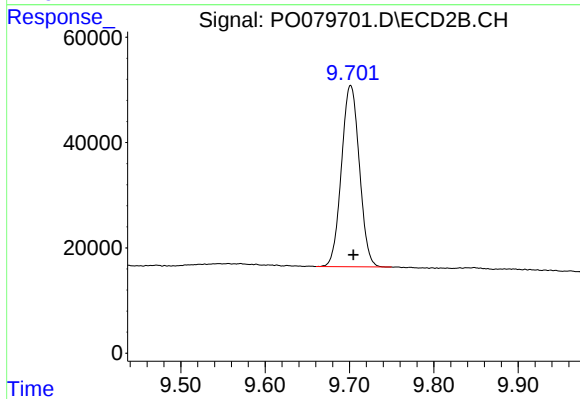

#2 Decachlorobiphenyl


R.T.: 9.701 min
Delta R.T.: -0.003 min
Response: 507643
Conc: 22.33 ng/ml

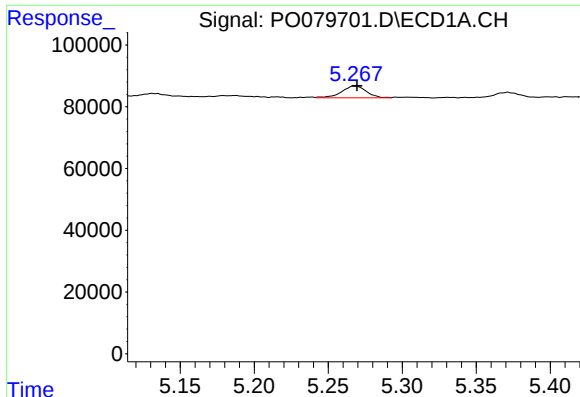

#8 AR-1221-1


R.T.: 5.268 min
Delta R.T.: -0.002 min
Response: 44039
Conc: 56.33 ng/ml

Instrument :
ECD_O
ClientSampleId :

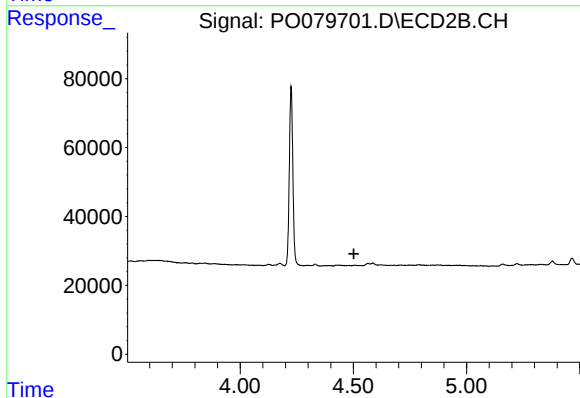


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.502 min
Response: 0
Conc: N.D.

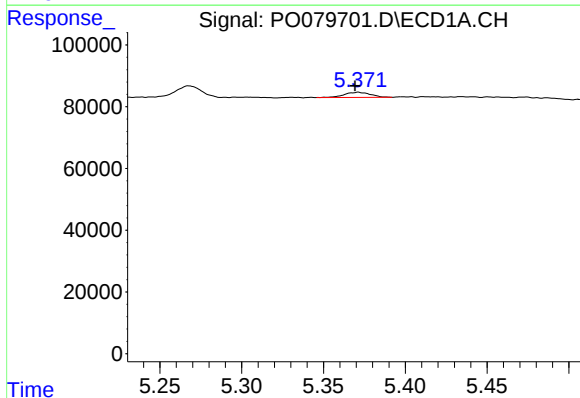


#9 AR-1221-2

R.T.: 5.371 min
Delta R.T.: 0.002 min
Response: 18817
Conc: 32.95 ng/ml

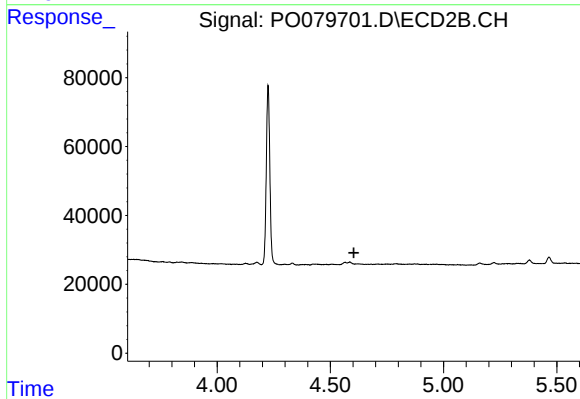

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.604 min
Response: 0
Conc: N.D.

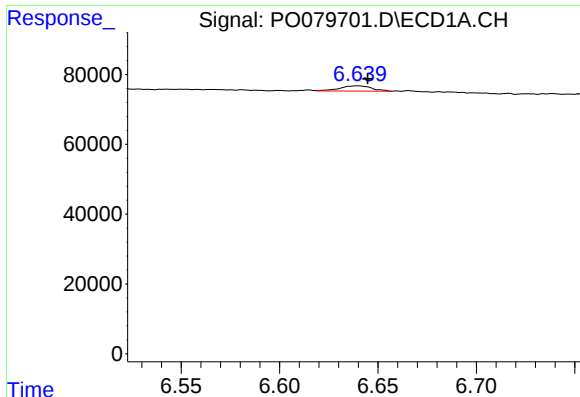

#15 AR-1232-5


R.T.: 6.640 min
Delta R.T.: -0.005 min
Response: 17418
Conc: 31.28 ng/ml

Instrument :
ECD_O
ClientSampleId :

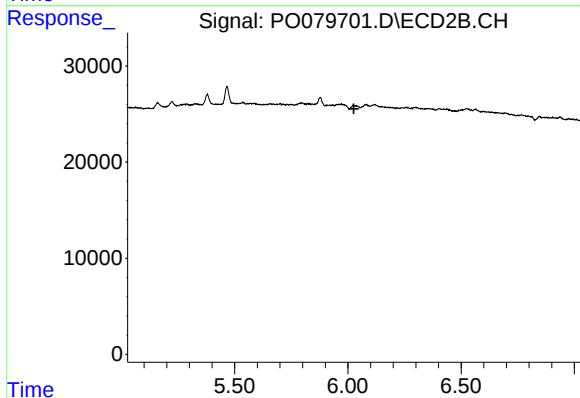


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

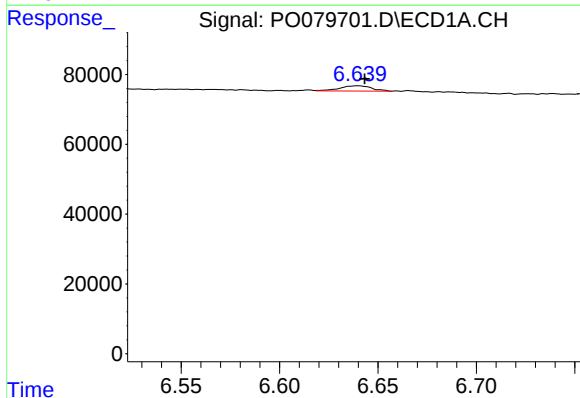


#22 AR-1248-2

R.T.: 6.640 min
Delta R.T.: -0.003 min
Response: 17418
Conc: 8.63 ng/ml

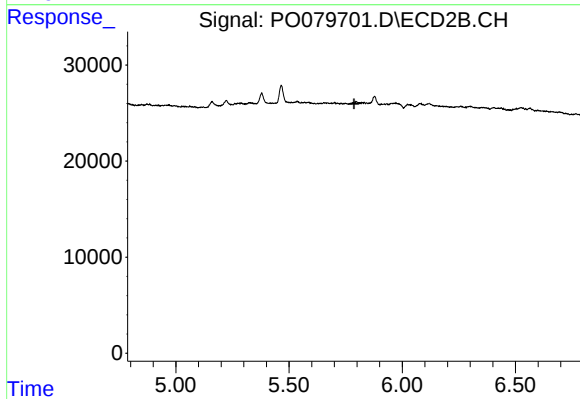

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T. : 5.787 min
Response: 0
Conc: N.D.

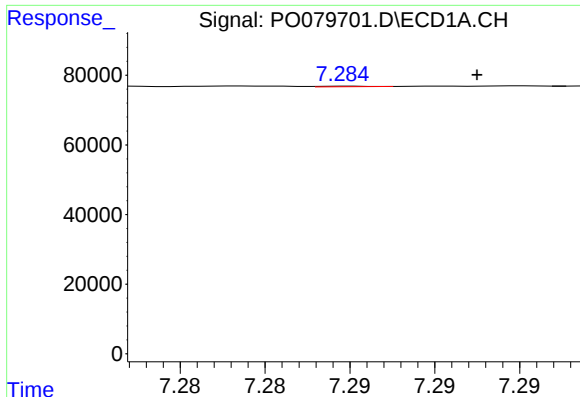

#24 AR-1248-4


R.T.: 7.285 min
Delta R.T.: -0.007 min
Response: 286
Conc: 0.11 ng/ml

Instrument :
ECD_O
ClientSampleId :

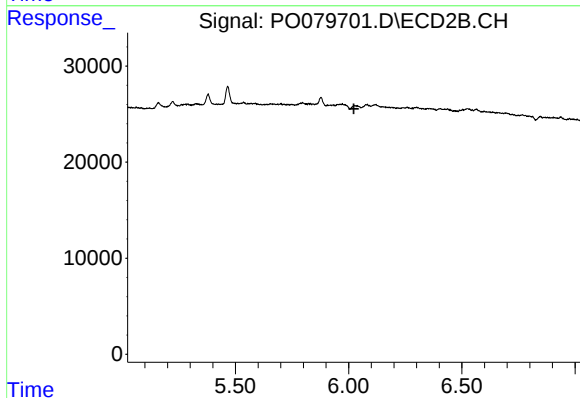


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

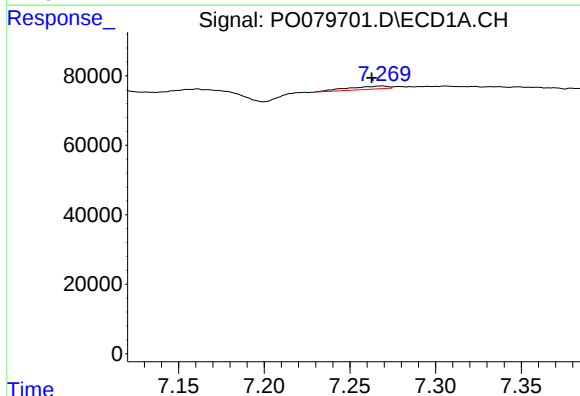


#26 AR-1254-1

R.T.: 7.269 min
Delta R.T.: 0.006 min
Response: 14124
Conc: 5.64 ng/ml

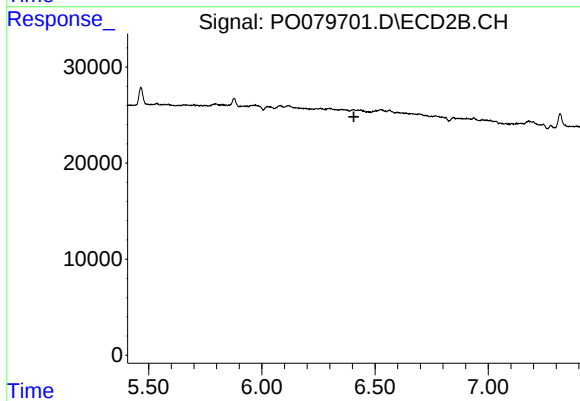

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.407 min
Response: 0
Conc: N.D.

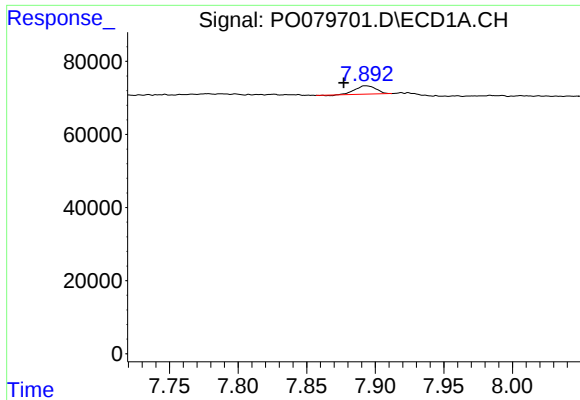

#28 AR-1254-3


R.T.: 7.893 min
Delta R.T.: 0.016 min
Response: 23755
Conc: 5.67 ng/ml

Instrument :
ECD_O
ClientSampleId :

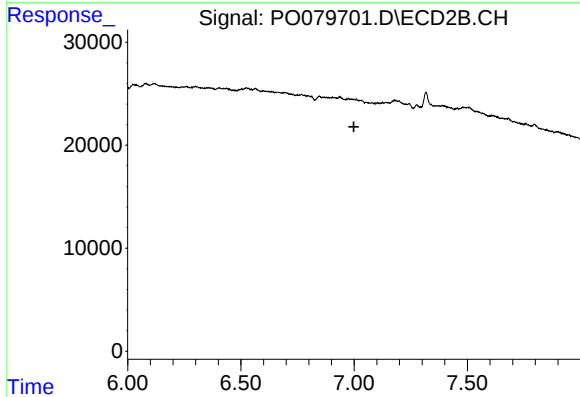


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.999 min
Response: 0
Conc: N.D.

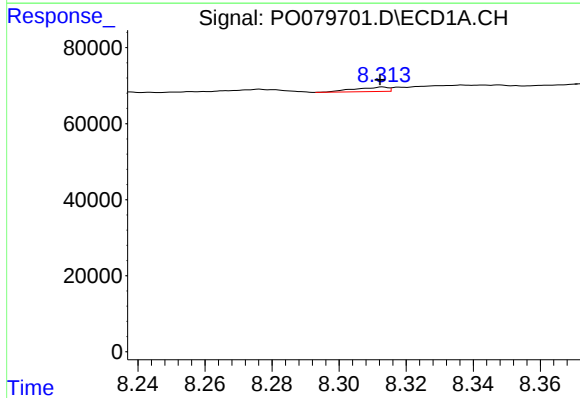

#32 AR-1260-2

R.T.: 8.313 min
Delta R.T.: 0.000 min
Response: 8230
Conc: 2.42 ng/ml

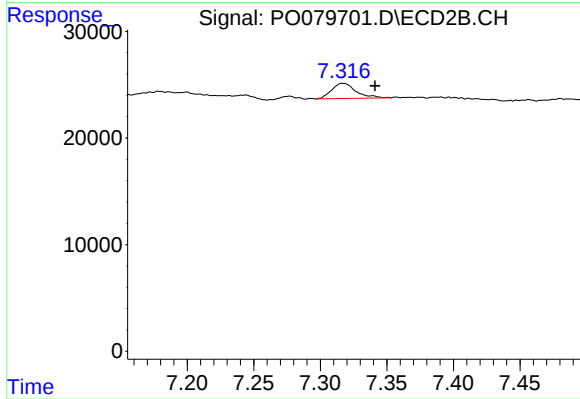

#32 AR-1260-2

R.T.: 7.316 min
Delta R.T.: -0.025 min
Response: 18233
Conc: 11.03 ng/ml