

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072021\
 Data File : P0079723.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jul 2021 22:53
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 02:00:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 20 14:31:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.015	4.232	1581732	563866	21.368	22.442
2)	SA Decachlor...	11.143	9.703	1218119	540690	22.655	23.787
Target Compounds							
8)	L2 AR-1221-1	5.268	0.000	40469	0	51.768	N.D. #
9)	L2 AR-1221-2	5.369	0.000	21010	0	36.790	N.D. #
15)	L3 AR-1232-5	6.639	0.000	22467	0	40.344	N.D. #
22)	L5 AR-1248-2	6.639	0.000	22467	0	11.127	N.D. #
24)	L5 AR-1248-4	7.289	0.000	1088	0	0.419	N.D. #
26)	L6 AR-1254-1	7.268	0.000	24441	0	9.754	N.D. #
28)	L6 AR-1254-3	7.896f	0.000	24275	0	5.797	N.D. #
32)	L7 AR-1260-2	8.321	7.319f	18625	15973	5.471	9.665 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072021\
Data File : P0079723.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jul 2021 22:53
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 02:00:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071921.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 20 14:31:26 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

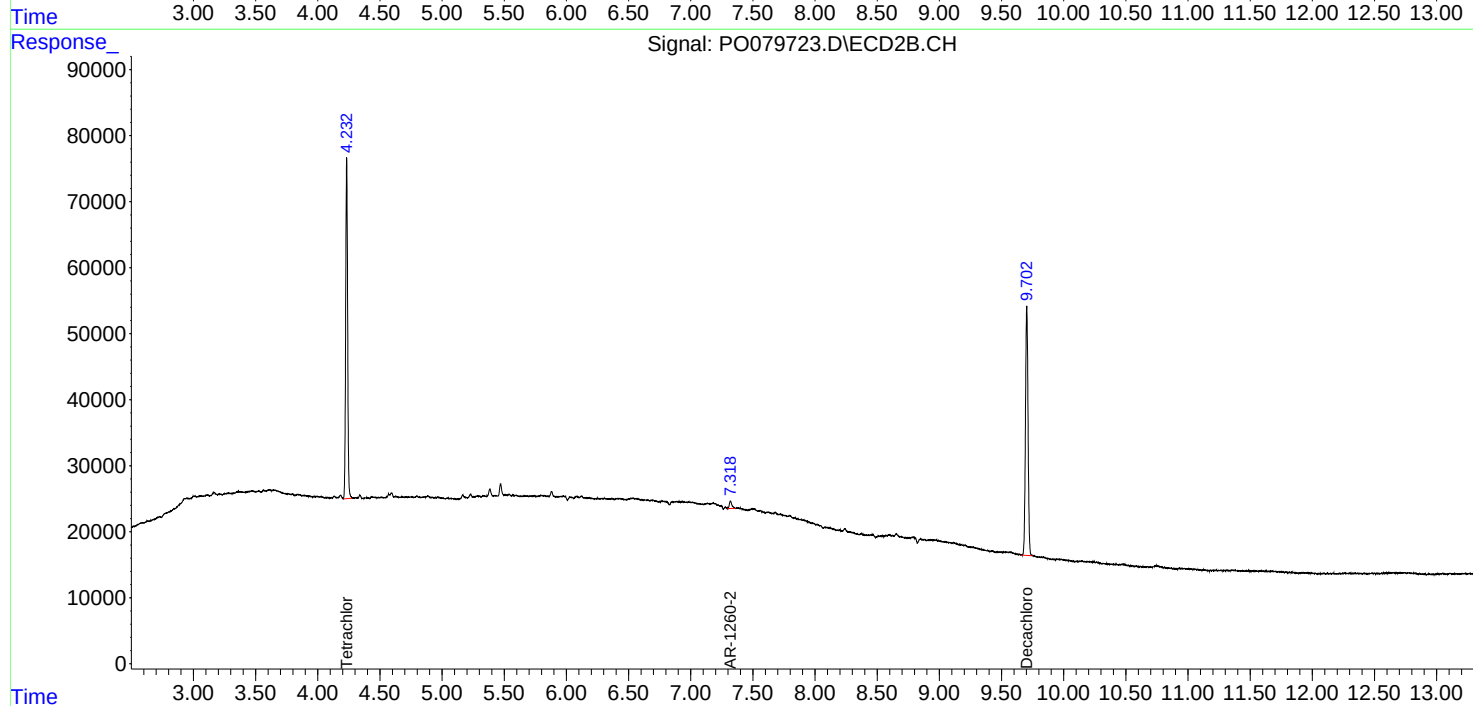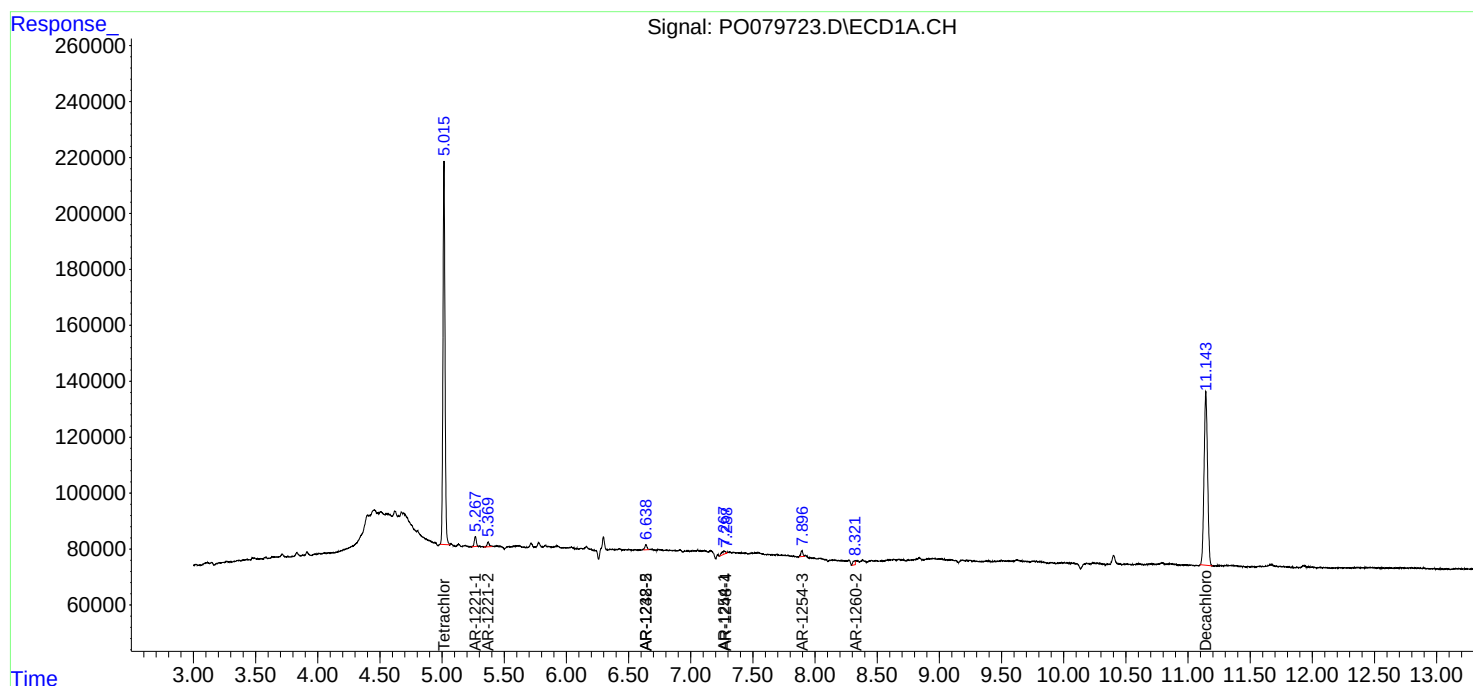


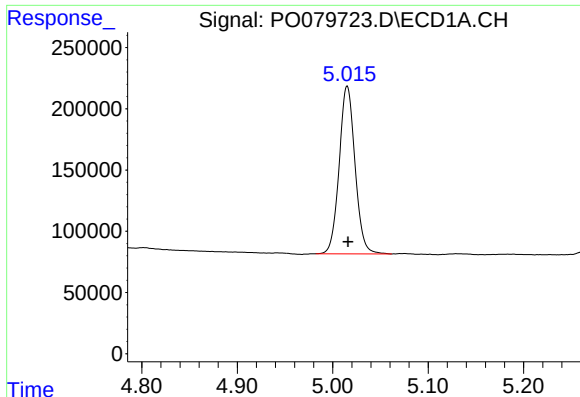

#1 Tetrachloro-m-xylene


R.T.: 5.015 min
Delta R.T.: 0.000 min
Response: 1581732
Conc: 21.37 ng/ml

Instrument :
ECD_O
ClientSampleId :

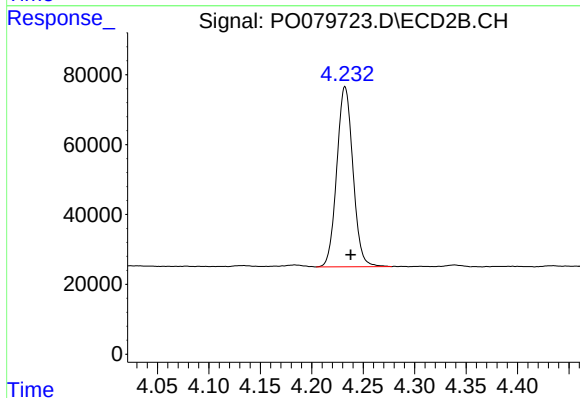


#1 Tetrachloro-m-xylene

R.T.: 4.232 min
Delta R.T.: -0.006 min
Response: 563866
Conc: 22.44 ng/ml

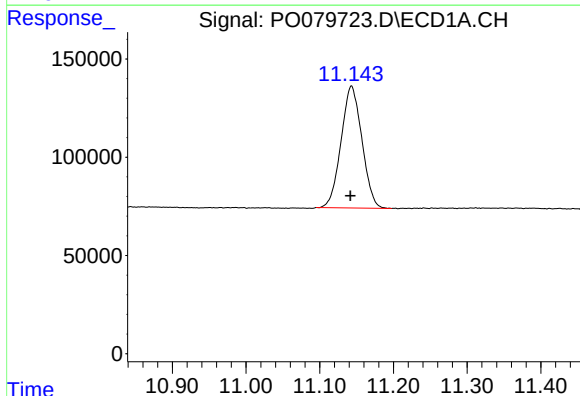


#2 Decachlorobiphenyl

R.T.: 11.143 min
Delta R.T.: 0.002 min
Response: 1218119
Conc: 22.65 ng/ml

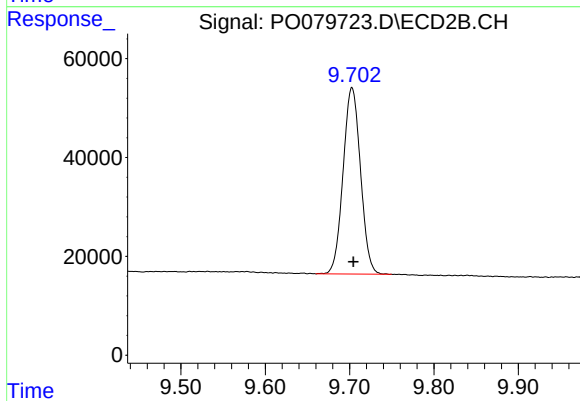

#2 Decachlorobiphenyl


R.T.: 9.703 min
Delta R.T.: -0.002 min
Response: 540690
Conc: 23.79 ng/ml

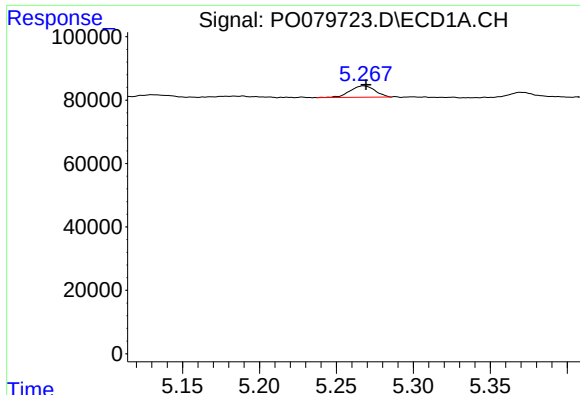

#8 AR-1221-1


R.T.: 5.268 min
Delta R.T.: -0.002 min
Response: 40469
Conc: 51.77 ng/ml

Instrument :
ECD_O
ClientSampleId :

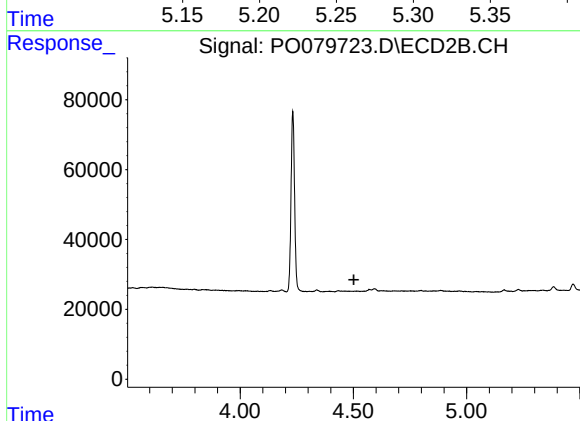


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.502 min
Response: 0
Conc: N.D.

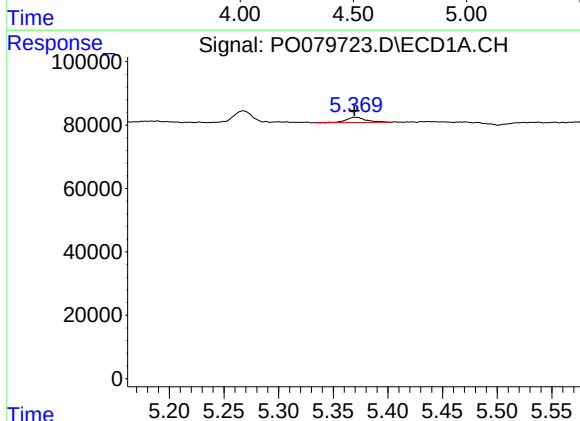


#9 AR-1221-2

R.T.: 5.369 min
Delta R.T.: 0.000 min
Response: 21010
Conc: 36.79 ng/ml

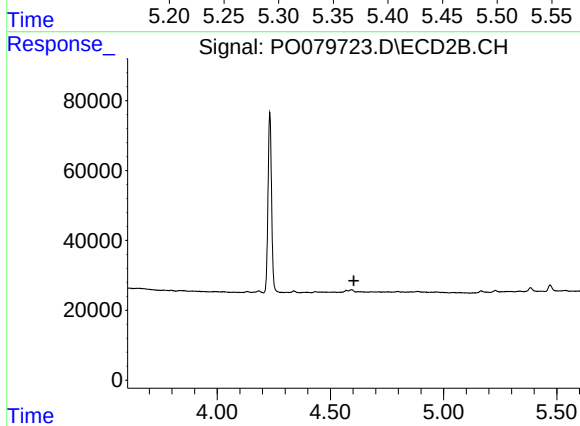

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.604 min
Response: 0
Conc: N.D.

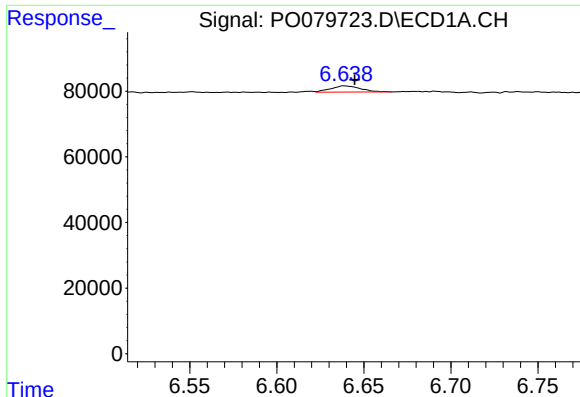

#15 AR-1232-5


R.T.: 6.639 min
Delta R.T.: -0.006 min
Response: 22467
Conc: 40.34 ng/ml

Instrument :
ECD_O
ClientSampleId :

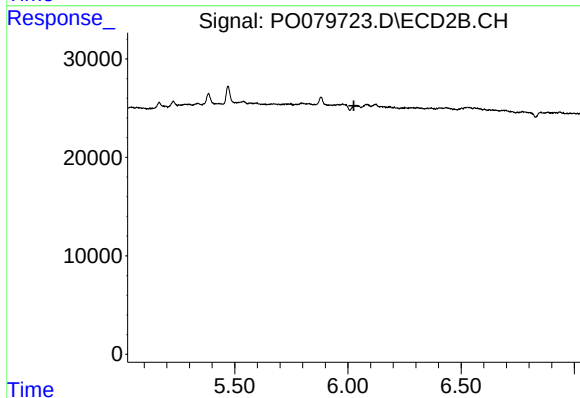


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 6.026 min
Response: 0
Conc: N.D.

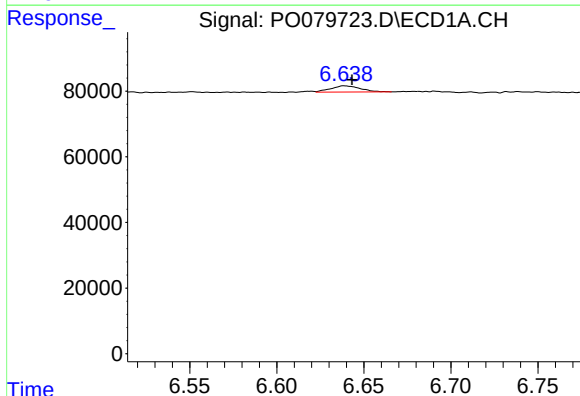


#22 AR-1248-2

R.T.: 6.639 min
Delta R.T.: -0.004 min
Response: 22467
Conc: 11.13 ng/ml

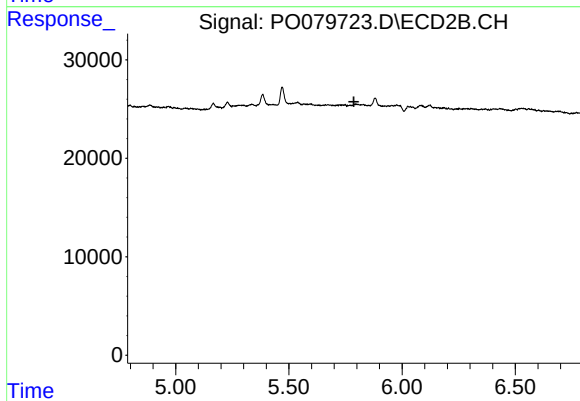

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T. : 5.787 min
Response: 0
Conc: N.D.

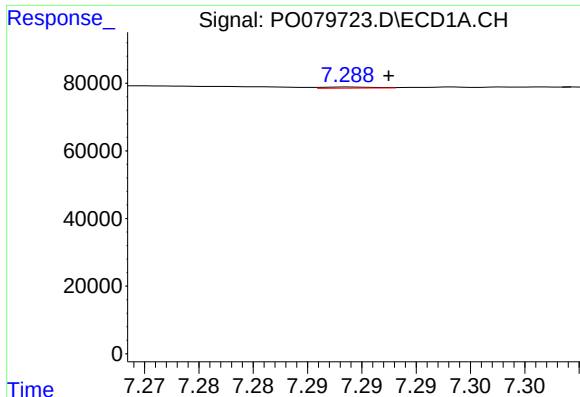

#24 AR-1248-4


R.T.: 7.289 min
Delta R.T.: -0.003 min
Response: 1088
Conc: 0.42 ng/ml

Instrument :
ECD_O
ClientSampleId :

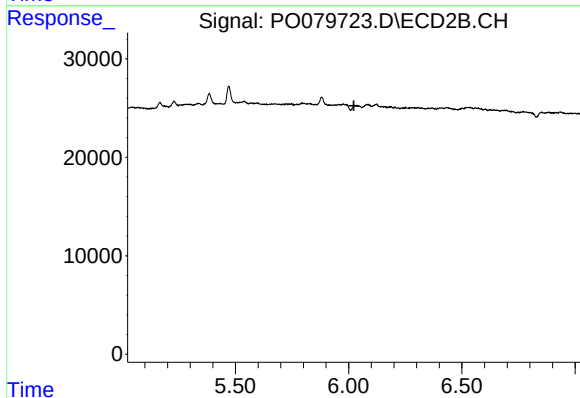


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 6.023 min
Response: 0
Conc: N.D.

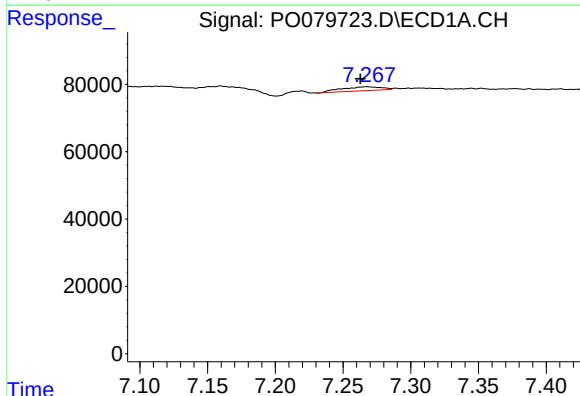


#26 AR-1254-1

R.T.: 7.268 min
Delta R.T.: 0.005 min
Response: 24441
Conc: 9.75 ng/ml

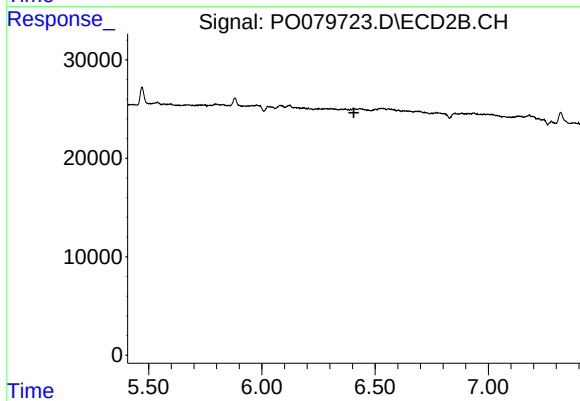

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.407 min
Response: 0
Conc: N.D.

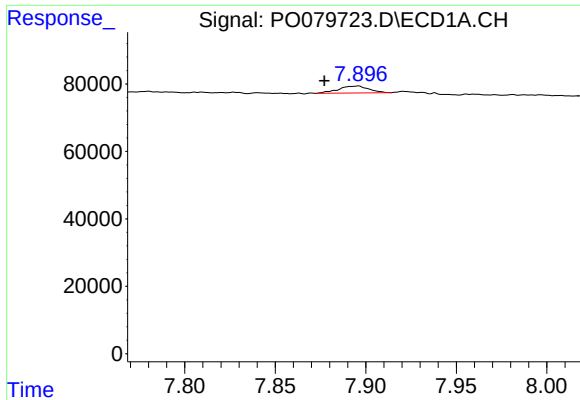

#28 AR-1254-3


R.T.: 7.896 min
Delta R.T.: 0.019 min
Response: 24275
Conc: 5.80 ng/ml

Instrument :
ECD_O
ClientSampleId :

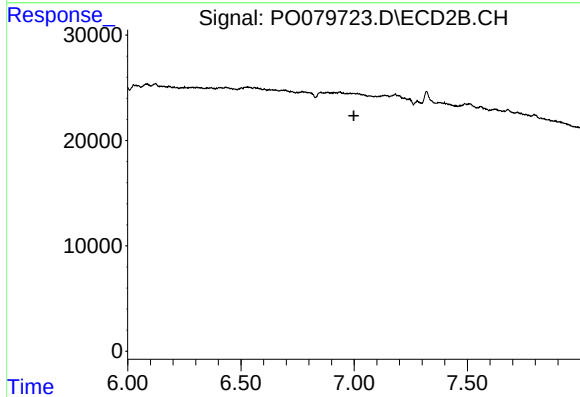


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.999 min
Response: 0
Conc: N.D.

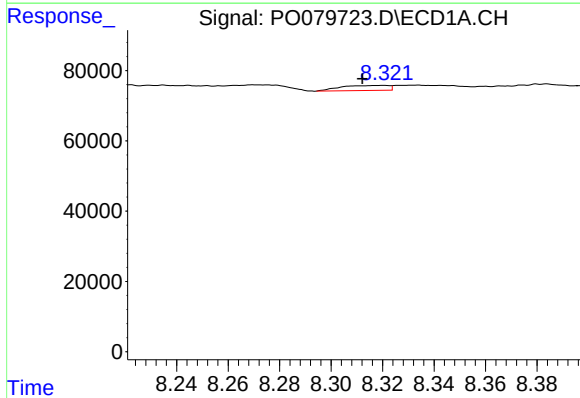

#32 AR-1260-2

R.T.: 8.321 min
Delta R.T.: 0.008 min
Response: 18625
Conc: 5.47 ng/ml

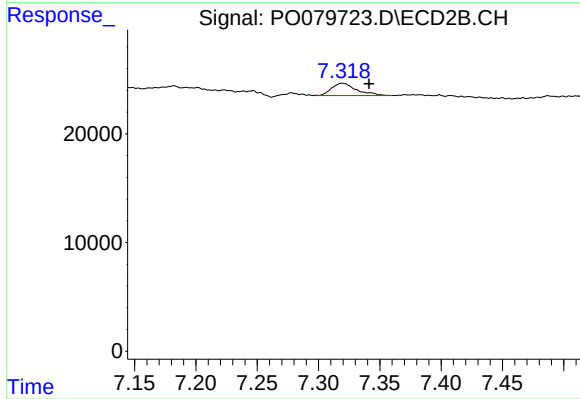

#32 AR-1260-2

R.T.: 7.319 min
Delta R.T.: -0.022 min
Response: 15973
Conc: 9.67 ng/ml