

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072021\
 Data File : PP037455.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jul 2021 23:12
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 02:17:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.957	3.947	871544	504346	19.176	18.431
2)	SA Decachlor...	10.989	9.240	847733	474421	18.415	17.044
Target Compounds							
8)	L2 AR-1221-1	5.208	0.000	11669	0	22.002	N.D. #
9)	L2 AR-1221-2	5.310	0.000	10886	0	26.870	N.D. #
20)	L4 AR-1242-5	0.000	6.091f	0	9463	N.D.	13.903 #
24)	L5 AR-1248-4	7.194f	0.000	16409	0	8.681	N.D. #
25)	L5 AR-1248-5	0.000	6.091f	0	9463	N.D.	8.922 #
26)	L6 AR-1254-1	7.194	6.091f	16409	9463	9.134	6.375 #
28)	L6 AR-1254-3	7.817f	0.000	11178	0	3.626	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072021\
Data File : PP037455.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jul 2021 23:12
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 02:17:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

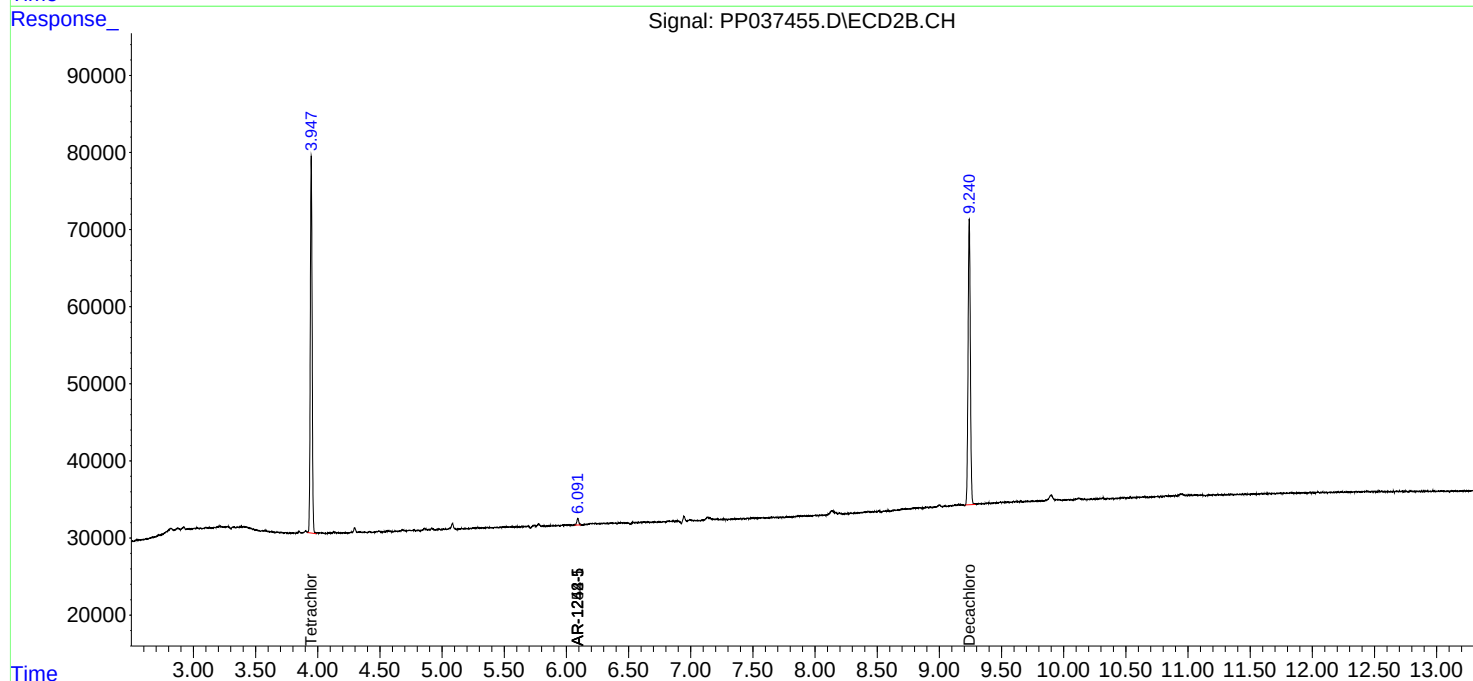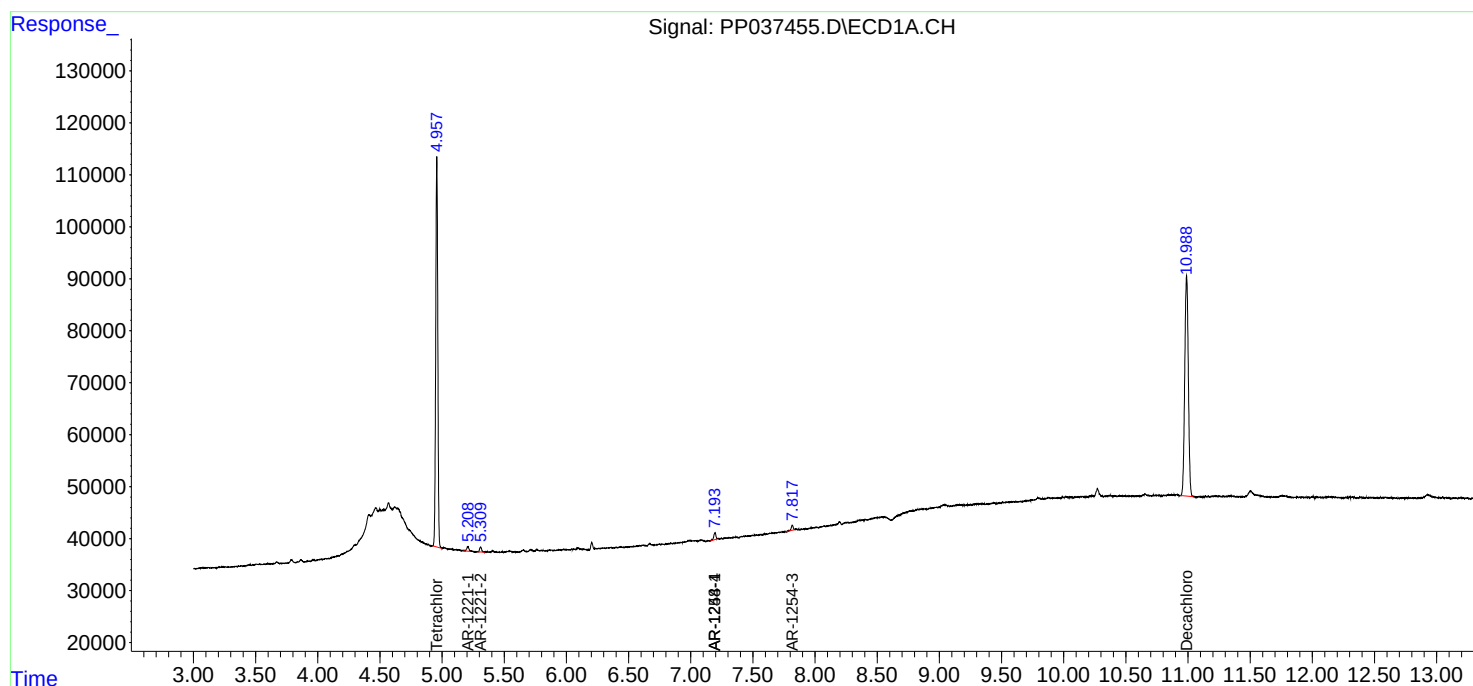


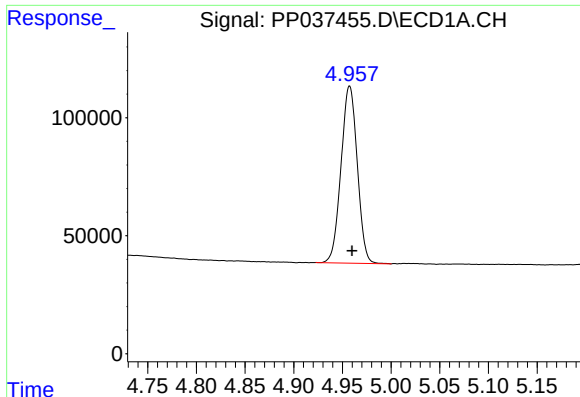

#1 Tetrachloro-m-xylene


R.T.: 4.957 min
Delta R.T.: -0.003 min
Response: 871544
Conc: 19.18 ng/ml

Instrument :
ECD_O
ClientSampleId :

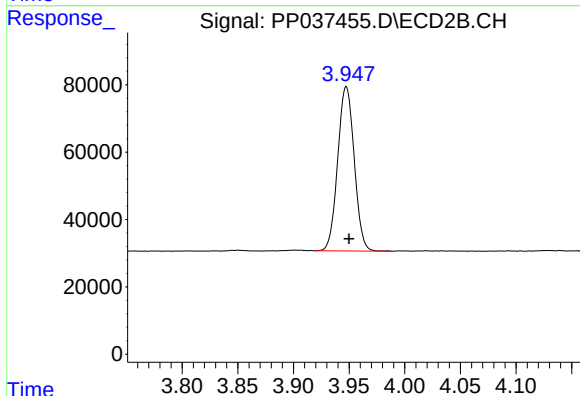


#1 Tetrachloro-m-xylene

R.T.: 3.947 min
Delta R.T.: -0.002 min
Response: 504346
Conc: 18.43 ng/ml

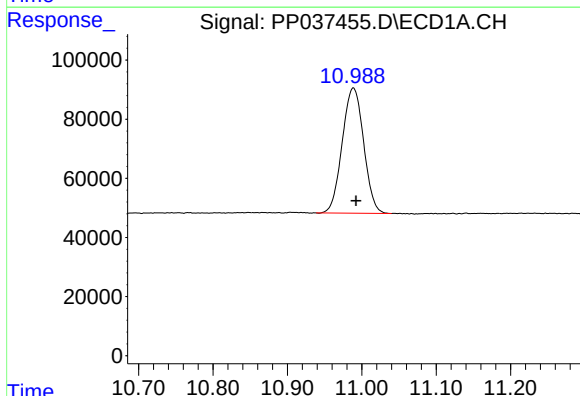


#2 Decachlorobiphenyl

R.T.: 10.989 min
Delta R.T.: -0.004 min
Response: 847733
Conc: 18.41 ng/ml

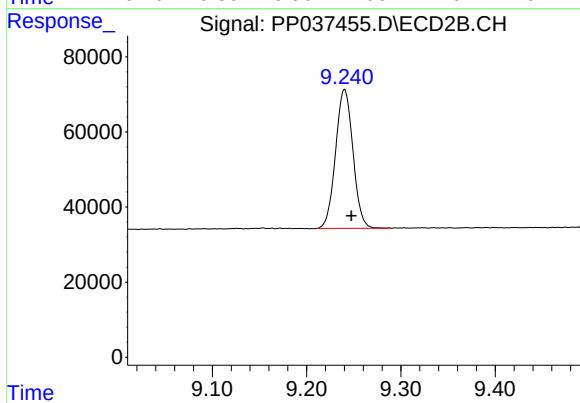

#2 Decachlorobiphenyl


R.T.: 9.240 min
Delta R.T.: -0.007 min
Response: 474421
Conc: 17.04 ng/ml

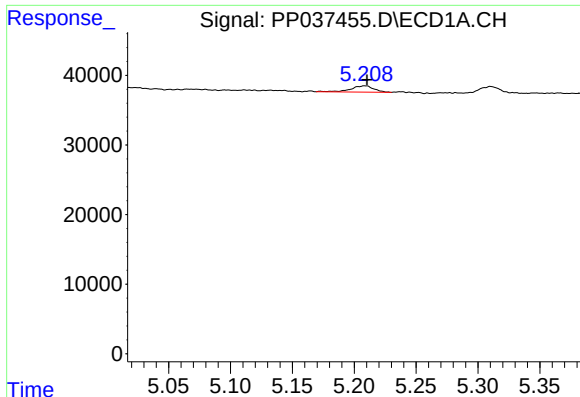

#8 AR-1221-1


R.T.: 5.208 min
Delta R.T.: -0.002 min
Response: 11669
Conc: 22.00 ng/ml

Instrument :
ECD_O
ClientSampleId :

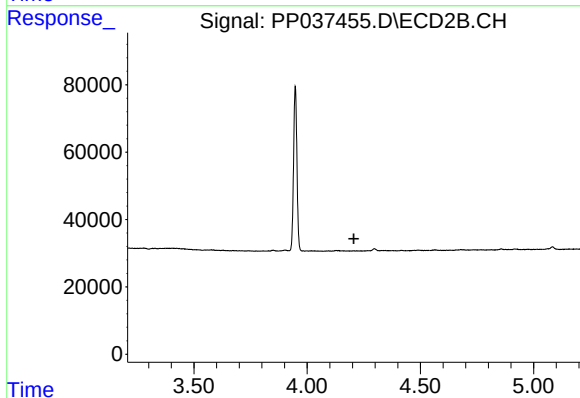


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.207 min
Response: 0
Conc: N.D.

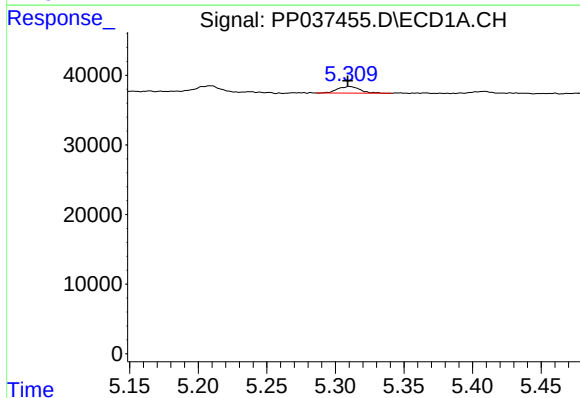


#9 AR-1221-2

R.T.: 5.310 min
Delta R.T.: 0.001 min
Response: 10886
Conc: 26.87 ng/ml

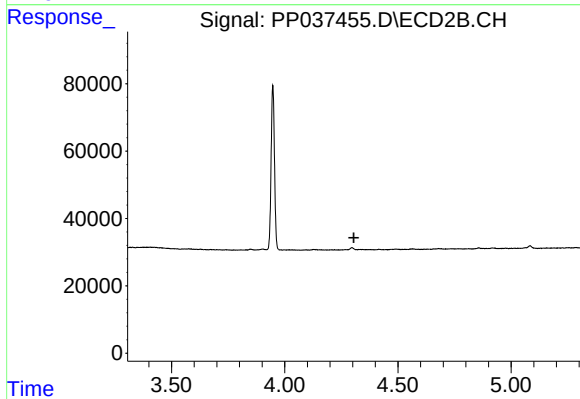

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.305 min
Response: 0
Conc: N.D.

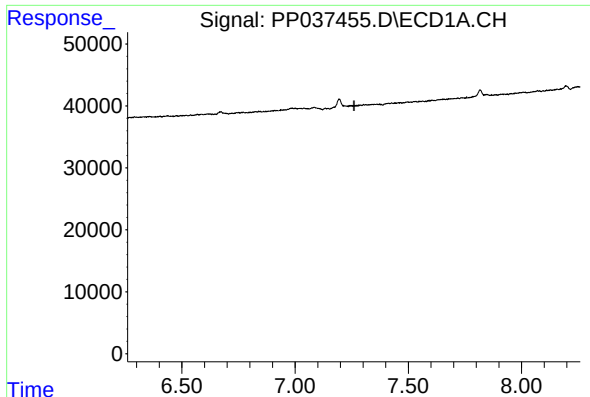

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.260 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

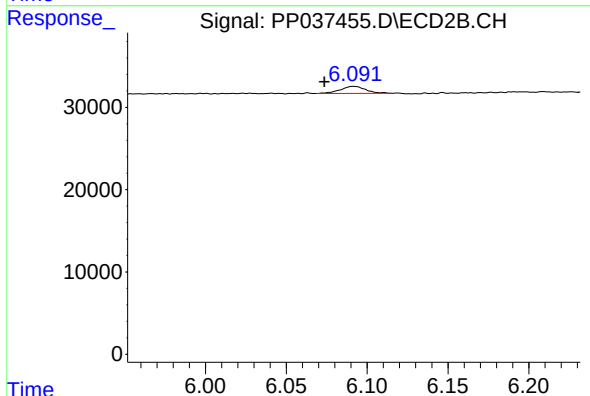


#20 AR-1242-5

R.T.: 6.091 min
Delta R.T.: 0.018 min
Response: 9463
Conc: 13.90 ng/ml

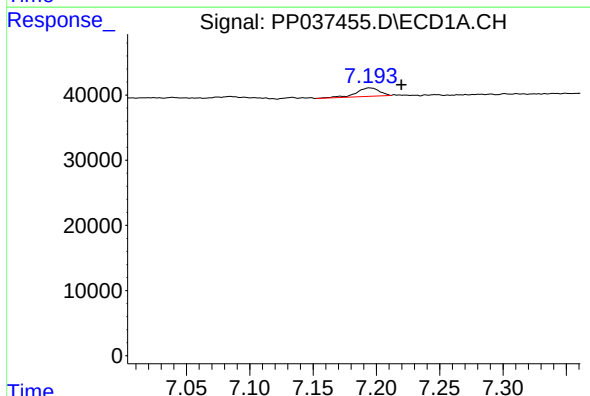


#24 AR-1248-4

R.T.: 7.194 min
Delta R.T.: -0.026 min
Response: 16409
Conc: 8.68 ng/ml

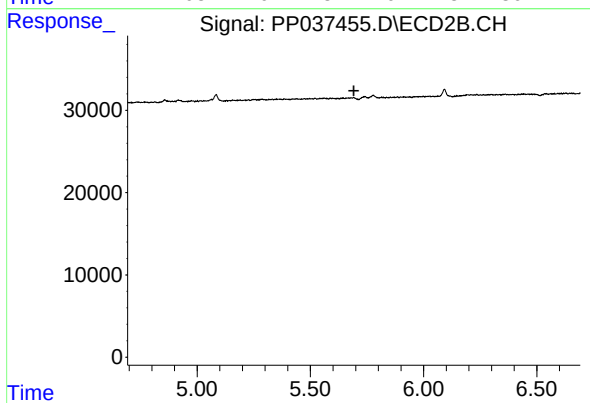

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.692 min
Response: 0
Conc: N.D.

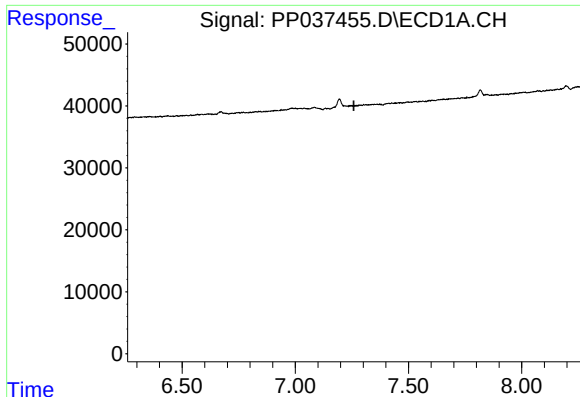

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 7.259 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

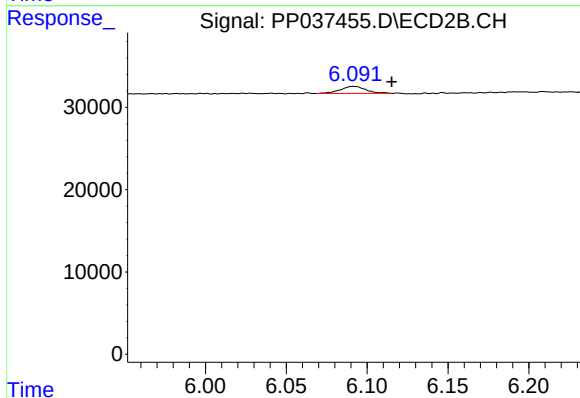


#25 AR-1248-5

R.T.: 6.091 min
Delta R.T.: -0.024 min
Response: 9463
Conc: 8.92 ng/ml

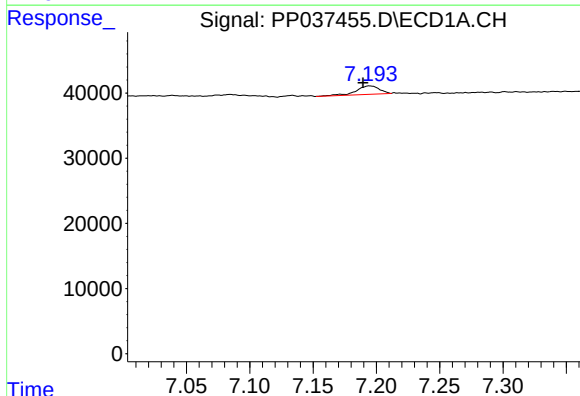


#26 AR-1254-1

R.T.: 7.194 min
Delta R.T.: 0.005 min
Response: 16409
Conc: 9.13 ng/ml

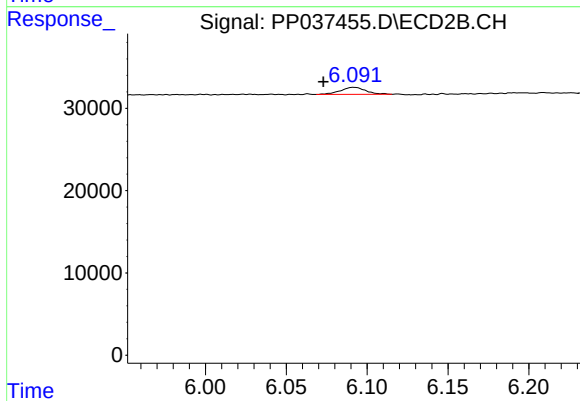

#26 AR-1254-1


R.T.: 6.091 min
Delta R.T.: 0.019 min
Response: 9463
Conc: 6.37 ng/ml

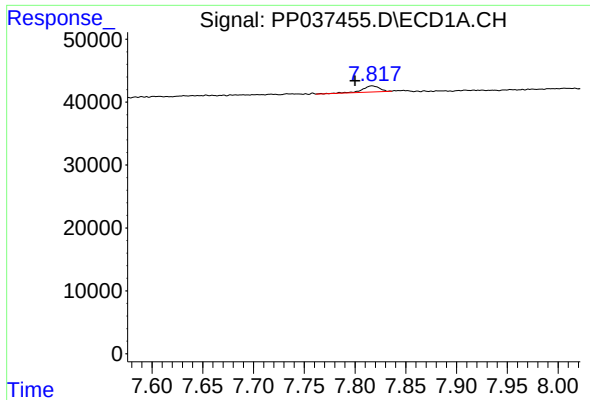

#28 AR-1254-3

R.T.: 7.817 min
Delta R.T.: 0.017 min
Response: 11178
Conc: 3.63 ng/ml

Instrument :
ECD_O
ClientSampleId :

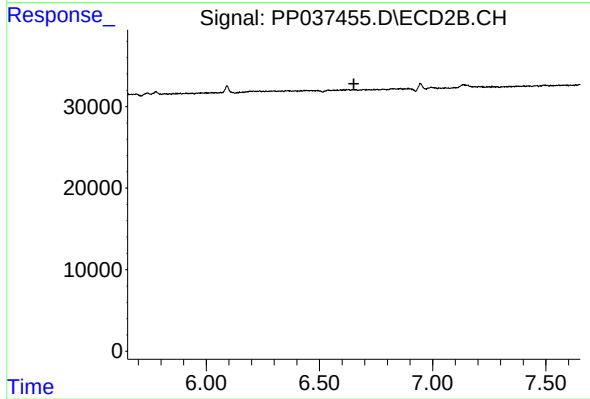

#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.652 min
Response: 0
Conc: N.D.