

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072021\
 Data File : PP037460.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jul 2021 00:37
 Operator : DD\AJ
 Sample : M3053-06RE
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 02:19:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 07 08:32:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.960	3.950	744969	434804	16.391	15.890
2)	SA Decachlor...	10.991	9.243	804824	360423	17.483	12.949 #
Target Compounds							
12)	L3 AR-1232-2	5.982	0.000	22905	0	38.414	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP072021\
Data File : PP037460.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jul 2021 00:37
Operator : DD\AJ
Sample : M3053-06RE
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 02:19:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP070621.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 07 08:32:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

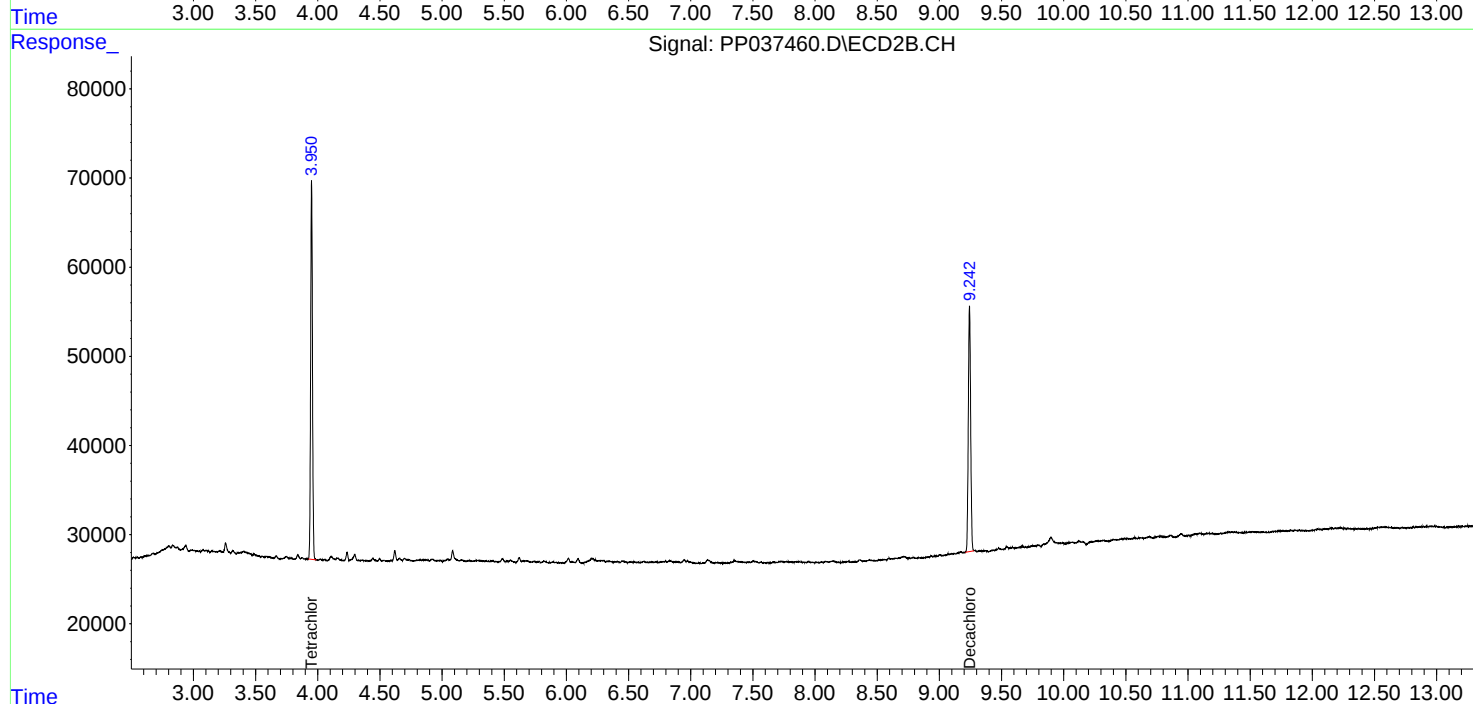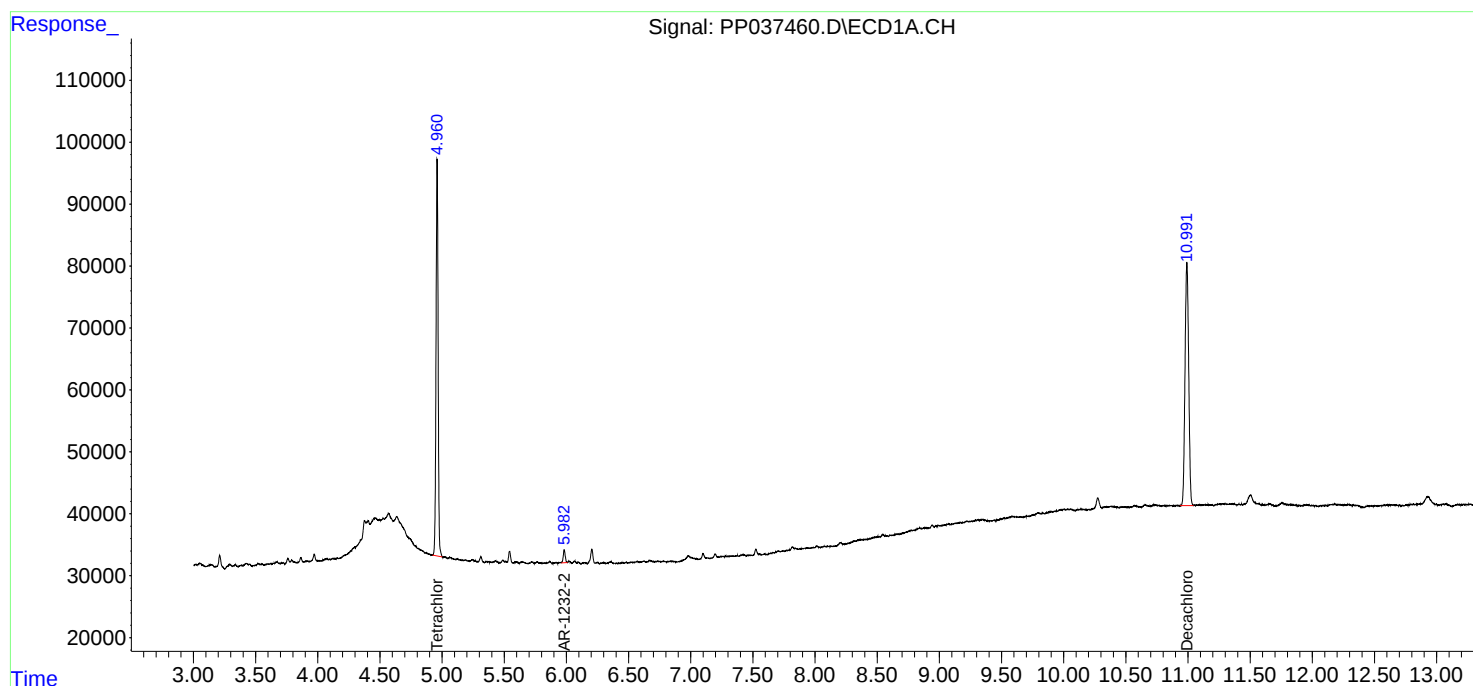


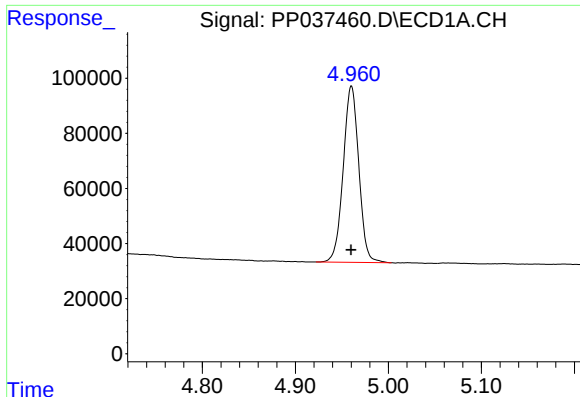

#1 Tetrachloro-m-xylene


R.T.: 4.960 min
Delta R.T.: 0.000 min
Response: 744969
Conc: 16.39 ng/ml

Instrument :
ECD_O
ClientSampleId :

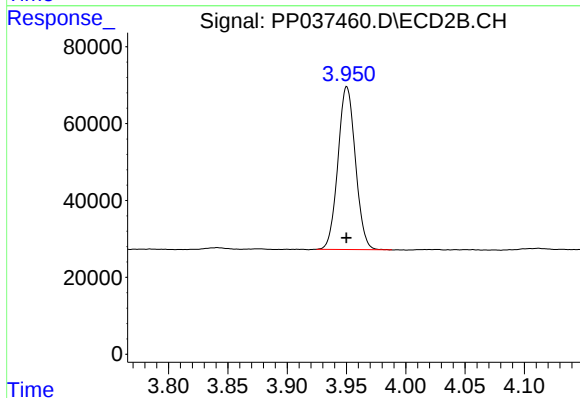


#1 Tetrachloro-m-xylene

R.T.: 3.950 min
Delta R.T.: 0.000 min
Response: 434804
Conc: 15.89 ng/ml

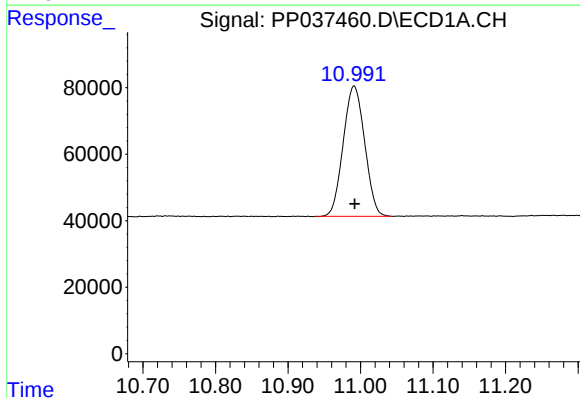


#2 Decachlorobiphenyl

R.T.: 10.991 min
Delta R.T.: -0.001 min
Response: 804824
Conc: 17.48 ng/ml

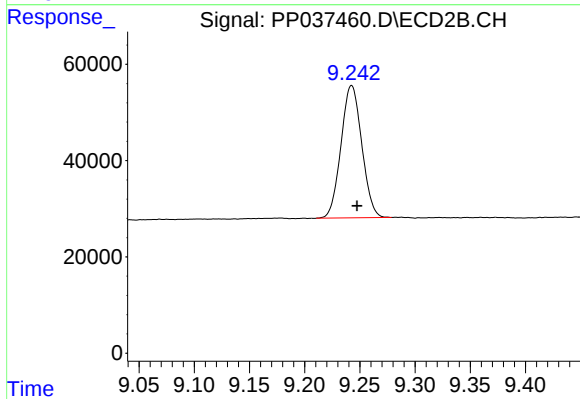

#2 Decachlorobiphenyl


R.T.: 9.243 min
Delta R.T.: -0.005 min
Response: 360423
Conc: 12.95 ng/ml

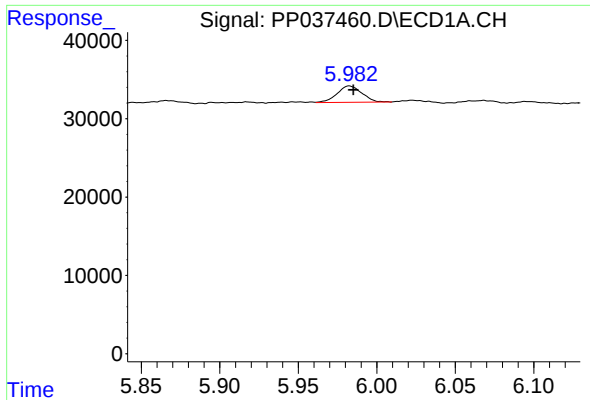

#12 AR-1232-2

R.T.: 5.982 min
Delta R.T.: -0.003 min
Response: 22905
Conc: 38.41 ng/ml

Instrument :
ECD_O
ClientSampleId :

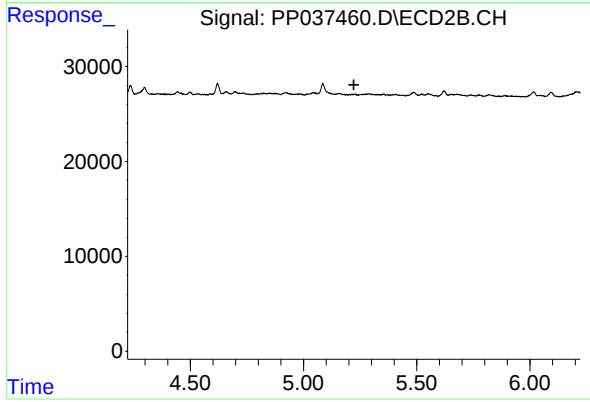

#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.222 min
Response: 0
Conc: N.D.