

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072021\
 Data File : P0079715.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jul 2021 20:17
 Operator : DD\AJ
 Sample : M3076-04
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20210587-AMENDED-COM-1-SPLP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 01:55:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 20 14:31:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.016	4.233	1476649	528247	19.948	21.025
2) SA Decachlor...	11.143	9.702	1210196	528418	22.507	23.247

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072021\
Data File : P0079715.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jul 2021 20:17
Operator : DD\AJ
Sample : M3076-04
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
20210587-AMENDED-COM-1-SPLP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 01:55:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071921.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 20 14:31:26 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

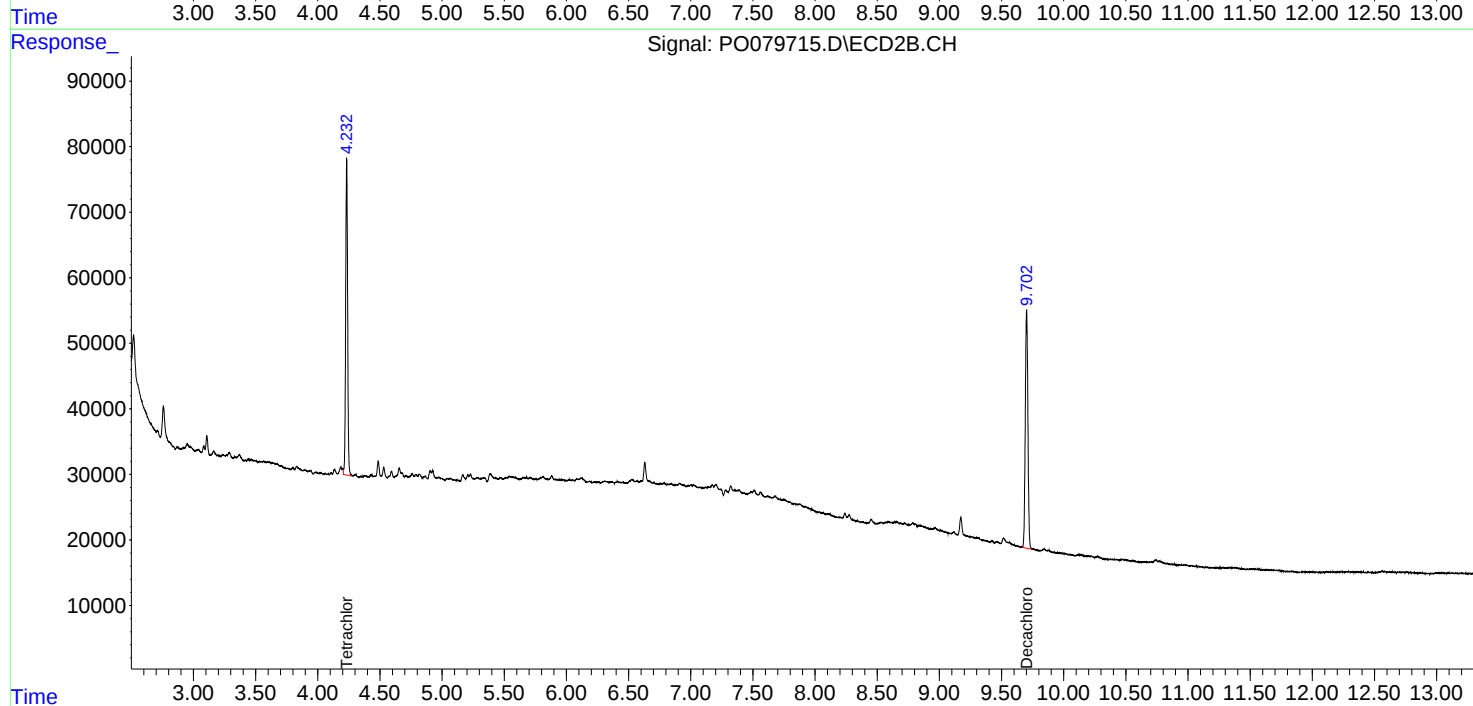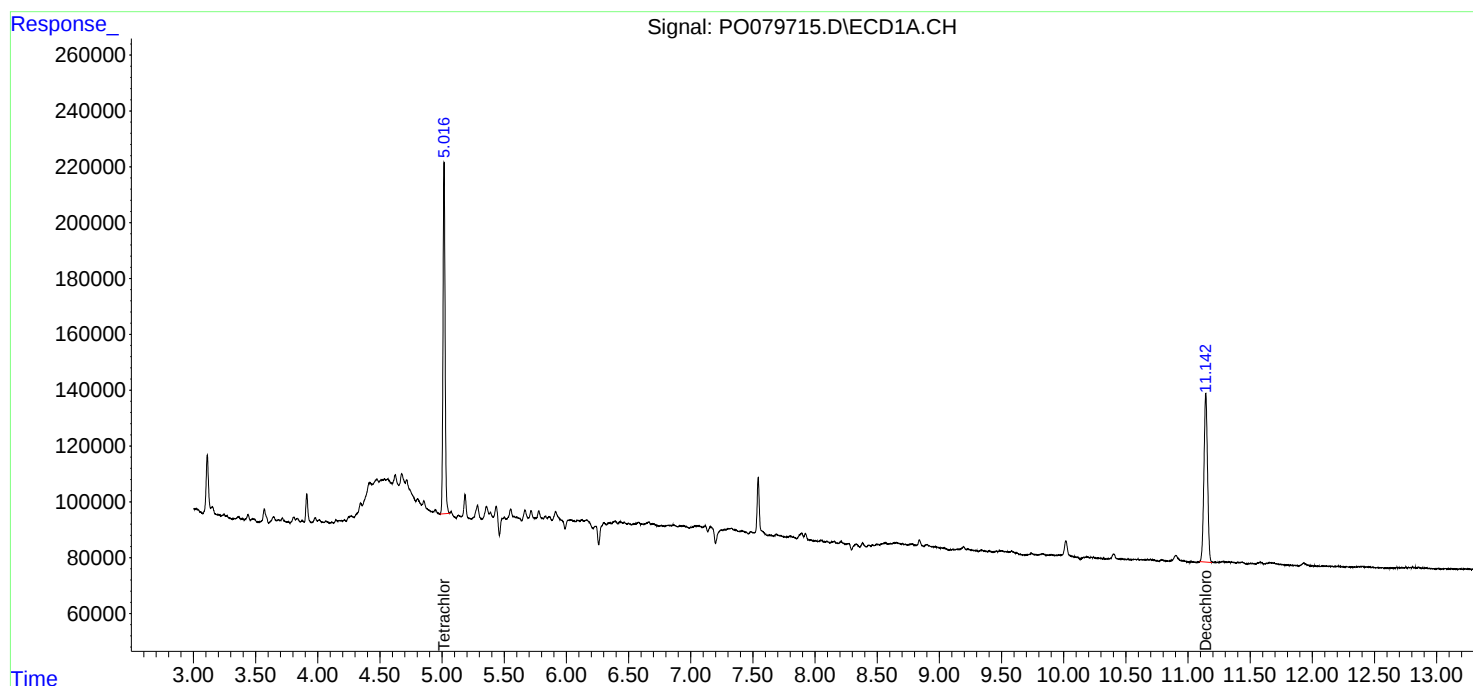


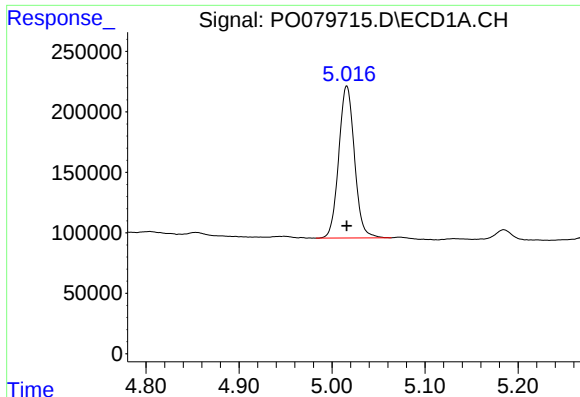

#1 Tetrachloro-m-xylene


R.T.: 5.016 min
Delta R.T.: 0.000 min
Response: 1476649
Conc: 19.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
20210587-AMENDED-COM-1-SPLP

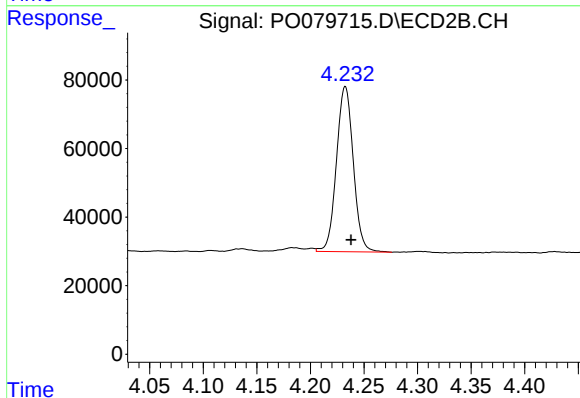


#1 Tetrachloro-m-xylene

R.T.: 4.233 min
Delta R.T.: -0.005 min
Response: 528247
Conc: 21.02 ng/ml

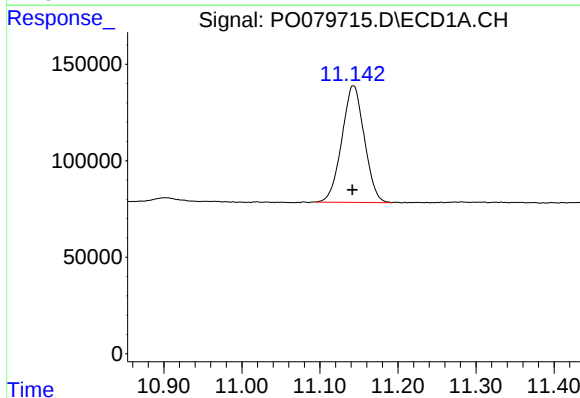

#2 Decachlorobiphenyl

R.T.: 11.143 min
Delta R.T.: 0.001 min
Response: 1210196
Conc: 22.51 ng/ml

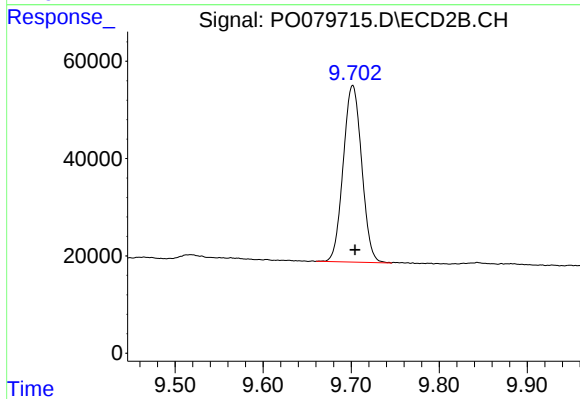

#2 Decachlorobiphenyl

R.T.: 9.702 min
Delta R.T.: -0.003 min
Response: 528418
Conc: 23.25 ng/ml