

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072021\
 Data File : P0079734.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jul 2021 2:38
 Operator : DD\AJ
 Sample : M3053-02 20X
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC204799LLK-END-1-2

Manual Integrations
 APPROVED

mohammad
 7/21/2021 3:42:48 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 04:33:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 20 14:31:26 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.015	4.231	34273	34108	0.463m	1.358m#
2) SA Decachlor...	11.138	9.705	85660	21042	1.593m	0.926 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072021\
Data File : P0079734.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jul 2021 2:38
Operator : DD\AJ
Sample : M3053-02 20X
Misc :
ALS Vial : 44 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
BC204799LLK-END-1-2


Manual Integrations
APPROVED

mohammad
7/21/2021 3:42:48 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 04:33:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071921.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 20 14:31:26 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

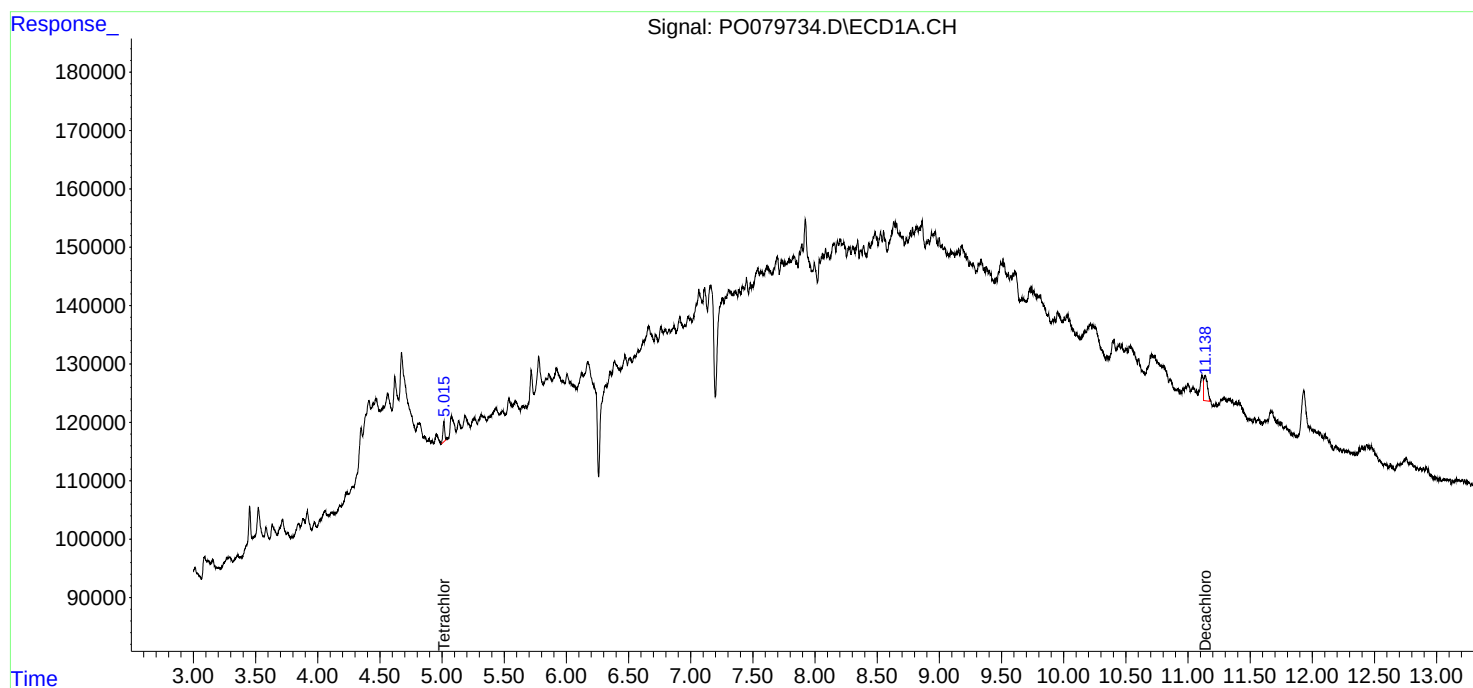

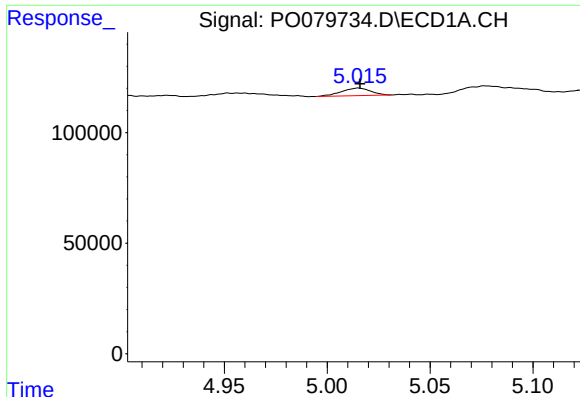


#1 Tetrachloro-m-xylene

R.T.: 5.015 min
Delta R.T.: -0.001 min
Response: 34273
Conc: 0.46 ng/ml m

Instrument :
ECD_O
ClientSampleId :
BC204799LLK-END-1-2


Manual Integrations
APPROVED

mohammad
7/21/2021 3:42:48 PM

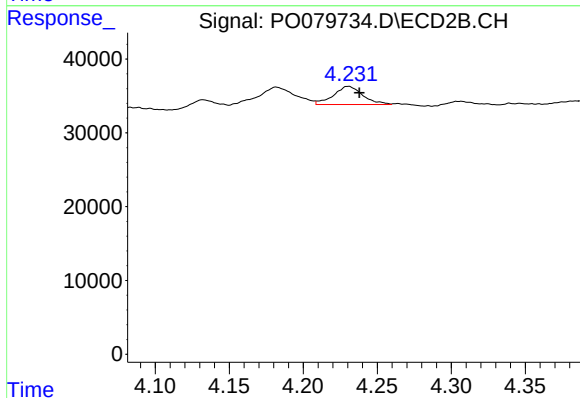


#1 Tetrachloro-m-xylene

R.T.: 4.231 min
Delta R.T.: -0.007 min
Response: 34108
Conc: 1.36 ng/ml m

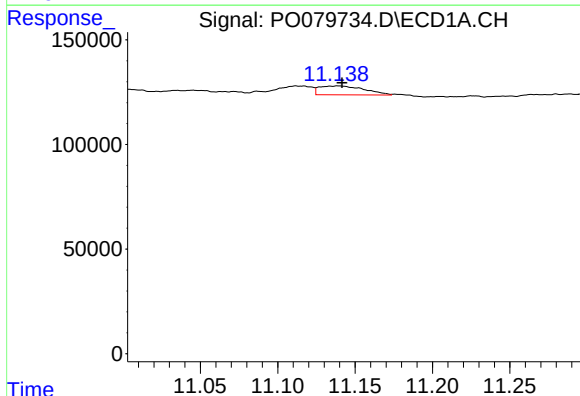

#2 Decachlorobiphenyl

R.T.: 11.138 min
Delta R.T.: -0.004 min
Response: 85660
Conc: 1.59 ng/ml m

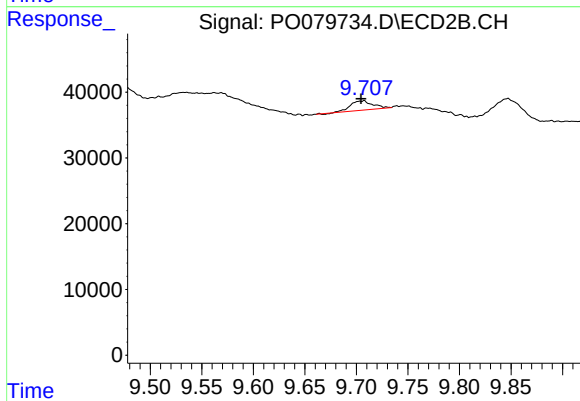

#2 Decachlorobiphenyl

R.T.: 9.705 min
Delta R.T.: 0.000 min
Response: 21042
Conc: 0.93 ng/ml