

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\P0072022\  
 Data File : P0088194.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 20 Jul 2022 11:31  
 Operator : YP/AJ  
 Sample : N3760-05  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 AUD-1645

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jul 20 12:26:52 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\P0071422.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Jul 15 03:57:23 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound        | RT#1   | RT#2  | Resp#1   | Resp#2  | ng/ml | ng/ml |
|-----------------------------|-----------------|--------|-------|----------|---------|-------|-------|
| -----                       |                 |        |       |          |         |       |       |
| System Monitoring Compounds |                 |        |       |          |         |       |       |
| 1)                          | SA Tetrachlo... | 4.449  | 3.607 | 20300360 | 7518428 | 7.957 | 7.969 |
| 2)                          | SA Decachlor... | 10.295 | 8.607 | 18420389 | 9061131 | 8.674 | 8.671 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\P0072022\  
Data File : P0088194.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 20 Jul 2022 11:31  
Operator : YP/AJ  
Sample : N3760-05  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
AUD-1645

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jul 20 12:26:52 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\P0071422.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Fri Jul 15 03:57:23 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

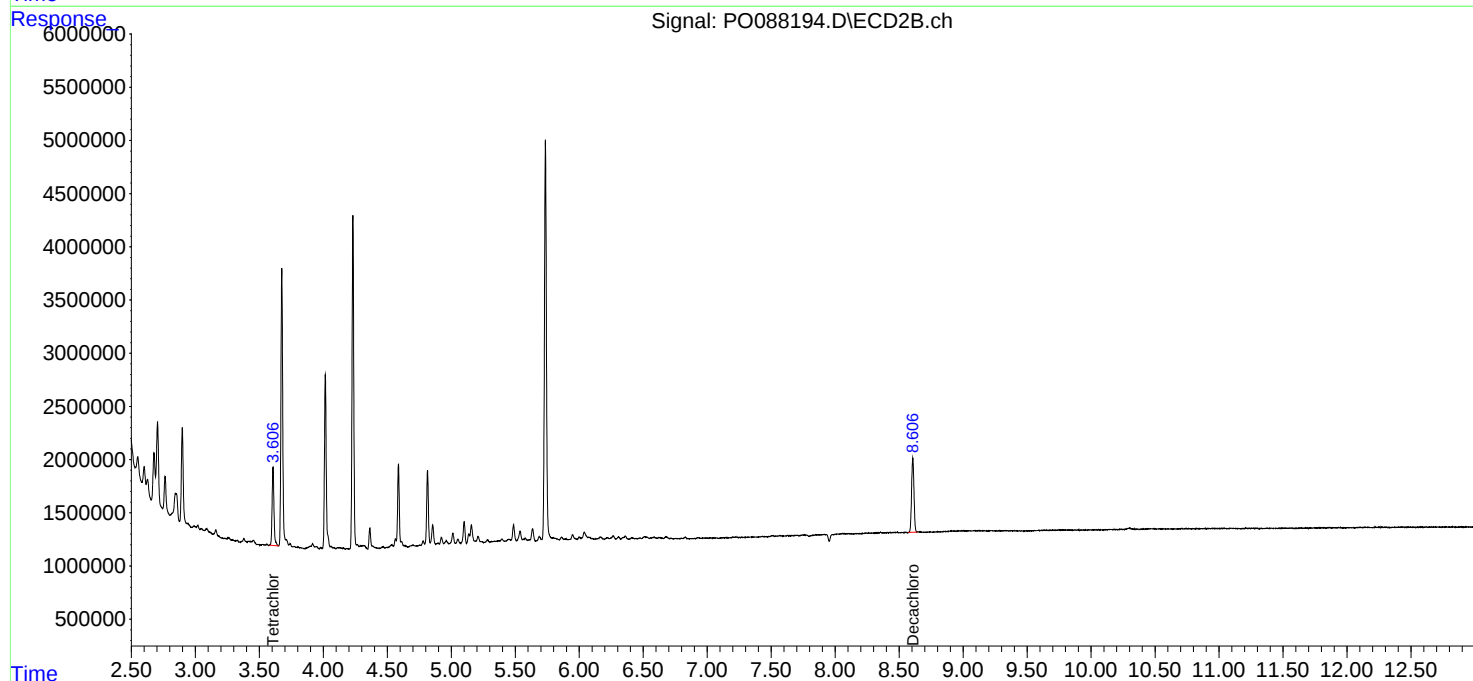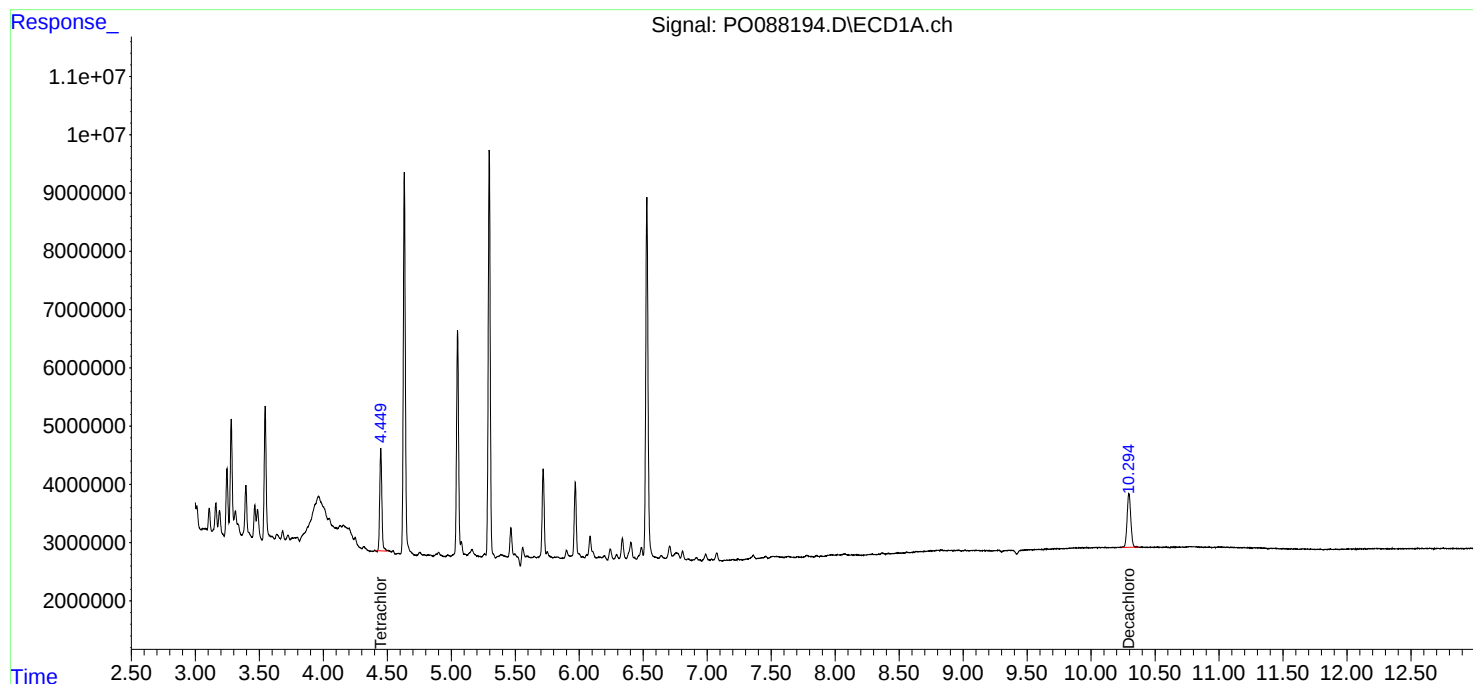


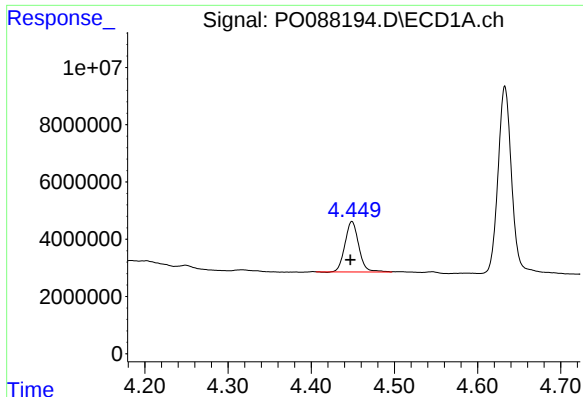

#1 Tetrachloro-m-xylene


R.T.: 4.449 min  
Delta R.T.: 0.002 min  
Response: 20300360  
Conc: 7.96 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
AUD-1645

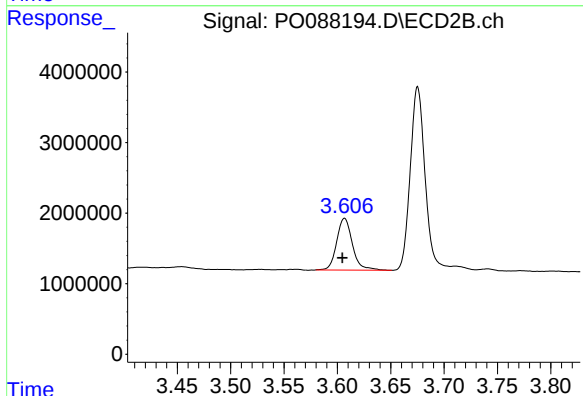


#1 Tetrachloro-m-xylene

R.T.: 3.607 min  
Delta R.T.: 0.002 min  
Response: 7518428  
Conc: 7.97 ng/ml

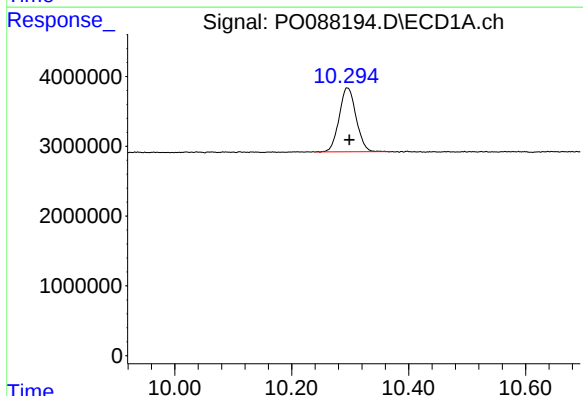

#2 Decachlorobiphenyl

R.T.: 10.295 min  
Delta R.T.: -0.003 min  
Response: 18420389  
Conc: 8.67 ng/ml

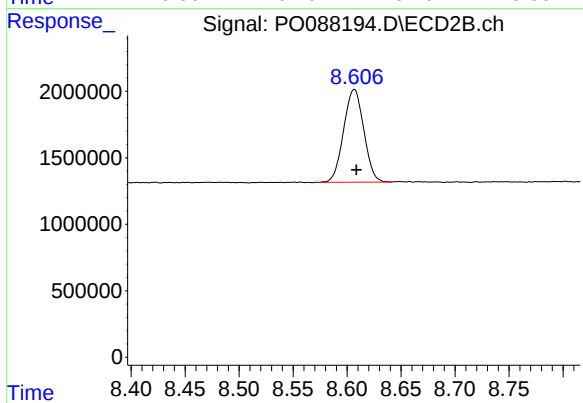

#2 Decachlorobiphenyl

R.T.: 8.607 min  
Delta R.T.: -0.002 min  
Response: 9061131  
Conc: 8.67 ng/ml