

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0072118\
 Data File : P0047001.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Jul 2018 17:18
 Operator : SM/SJ
 Sample : J4070-02
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KY030LC015-S-180718

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 04:17:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0071918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 19 01:07:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.200	3.524	3281434	4372372	11.419	14.324 #
2) SA Decachlor...	9.726	8.446	1836710	1736381	8.351	7.091

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0072118\
Data File : P0047001.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Jul 2018 17:18
Operator : SM/SJ
Sample : J4070-02
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
KY030LC015-S-180718

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 04:17:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0071918.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 19 01:07:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

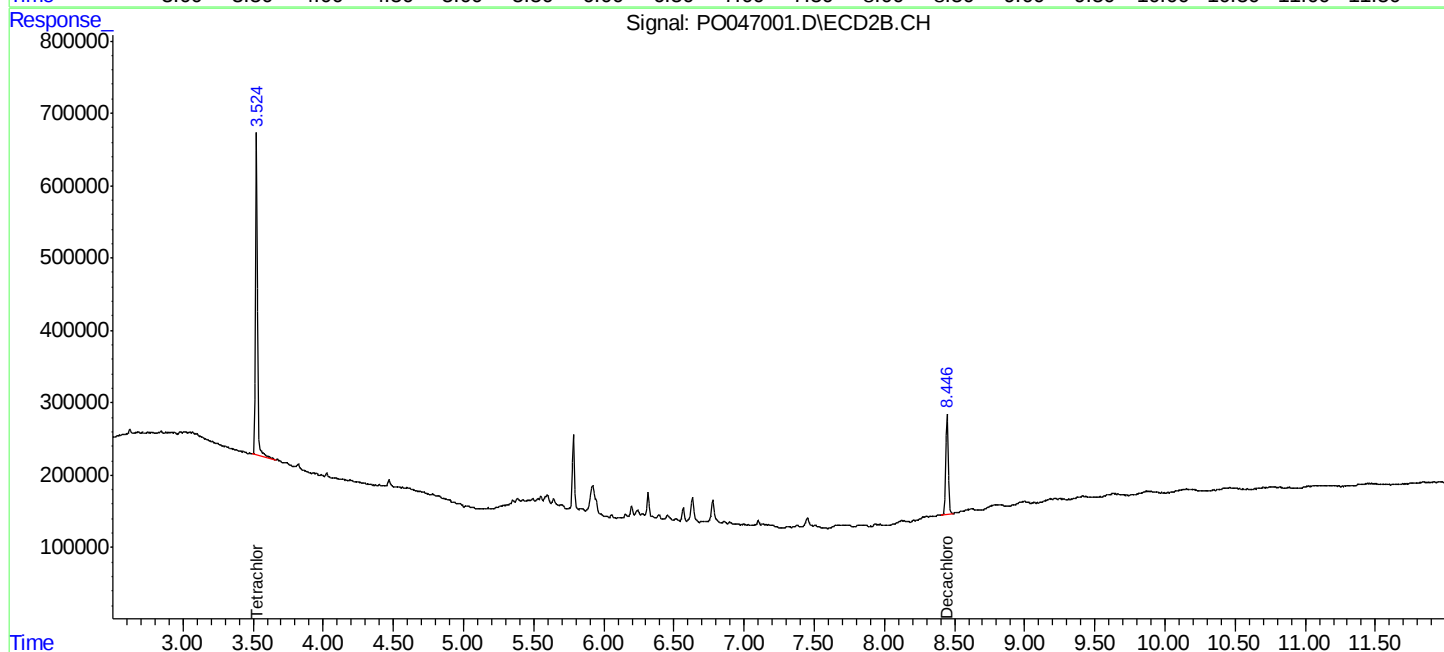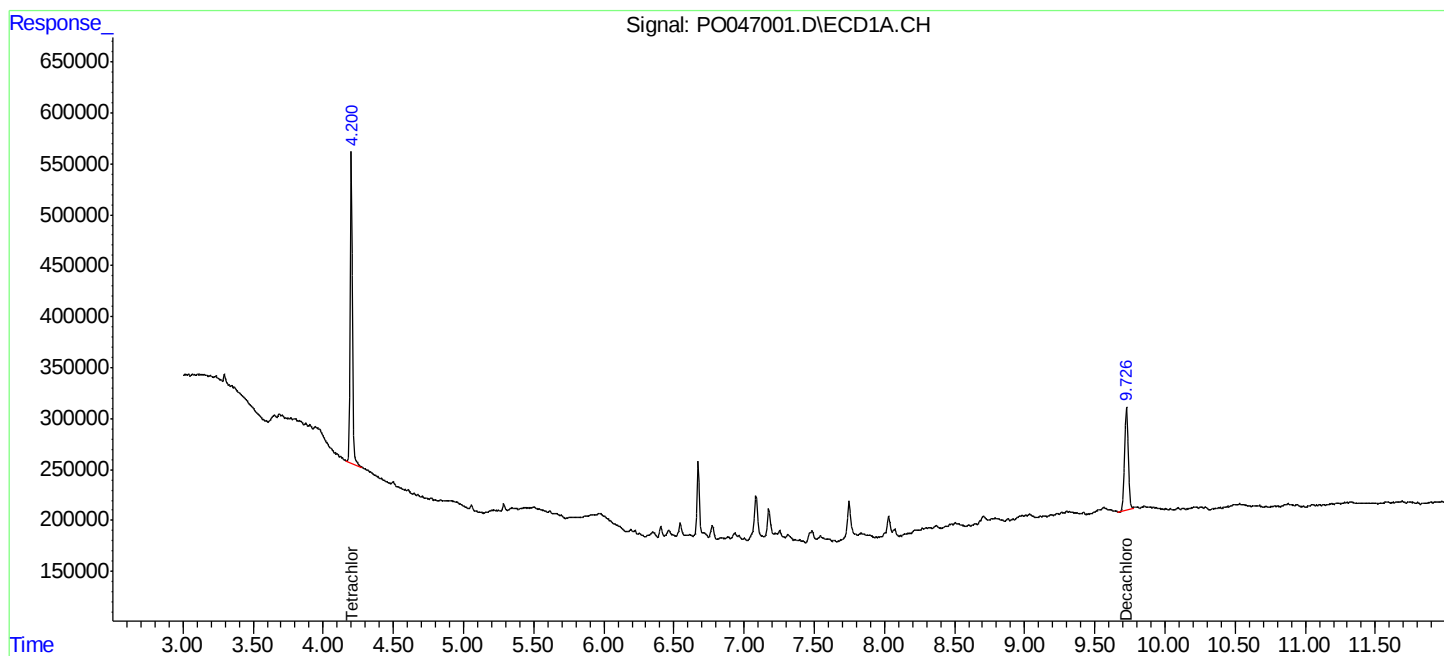


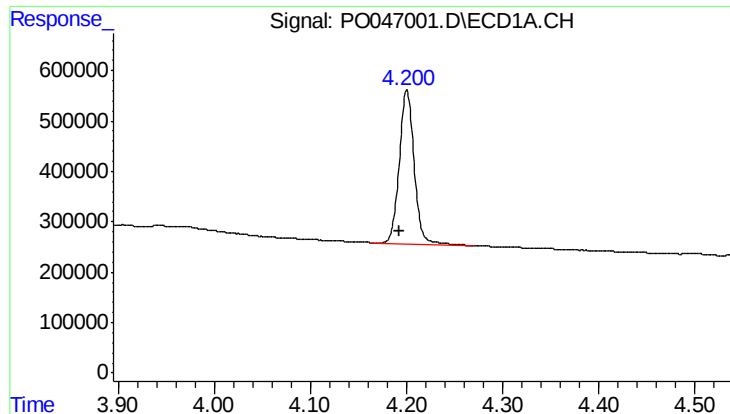

#1 Tetrachloro-m-xylene


R.T.: 4.200 min
Delta R.T.: 0.007 min
Response: 3281434
Conc: 11.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
KY030LC015-S-180718

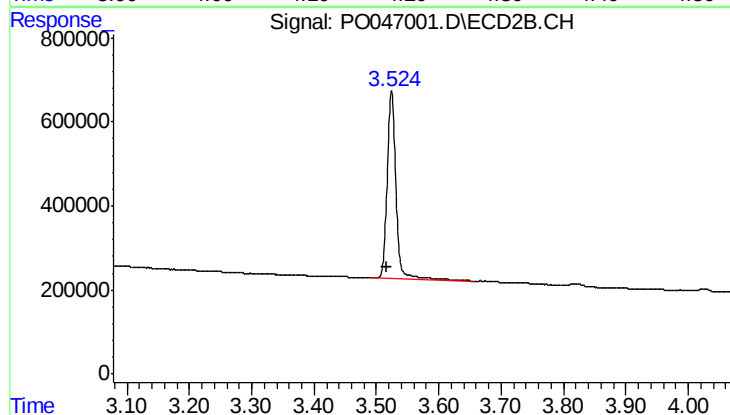


#1 Tetrachloro-m-xylene

R.T.: 3.524 min
Delta R.T.: 0.007 min
Response: 4372372
Conc: 14.32 ng/ml

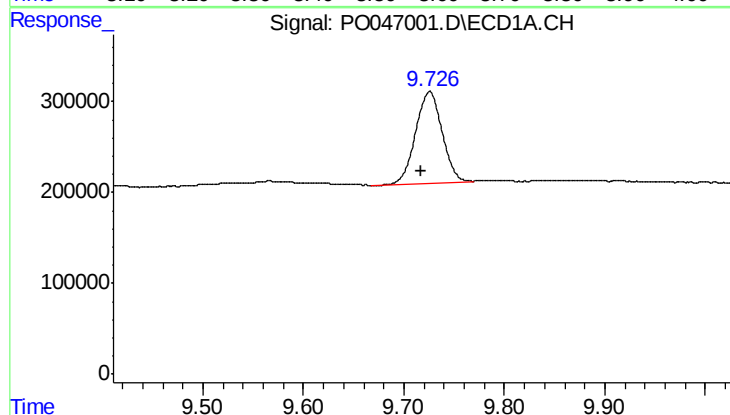

#2 Decachlorobiphenyl

R.T.: 9.726 min
Delta R.T.: 0.008 min
Response: 1836710
Conc: 8.35 ng/ml

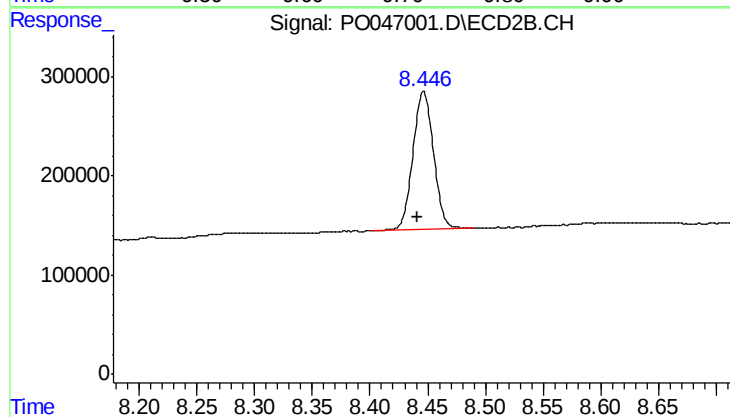

#2 Decachlorobiphenyl

R.T.: 8.446 min
Delta R.T.: 0.005 min
Response: 1736381
Conc: 7.09 ng/ml