

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072120\
Data File : P0069836.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jul 2020 12:31
Operator : DD\AJ
Sample : PB130336BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB130336BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 13:45:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 08 16:12:41 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.385	3.559	785313	724859	21.034	18.214
2) SA Decachlor...	10.037f	8.763	1128357	1064088	18.754	18.749

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072120\
Data File : P0069836.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jul 2020 12:31
Operator : DD\AJ
Sample : PB130336BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB130336BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 13:45:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 08 16:12:41 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

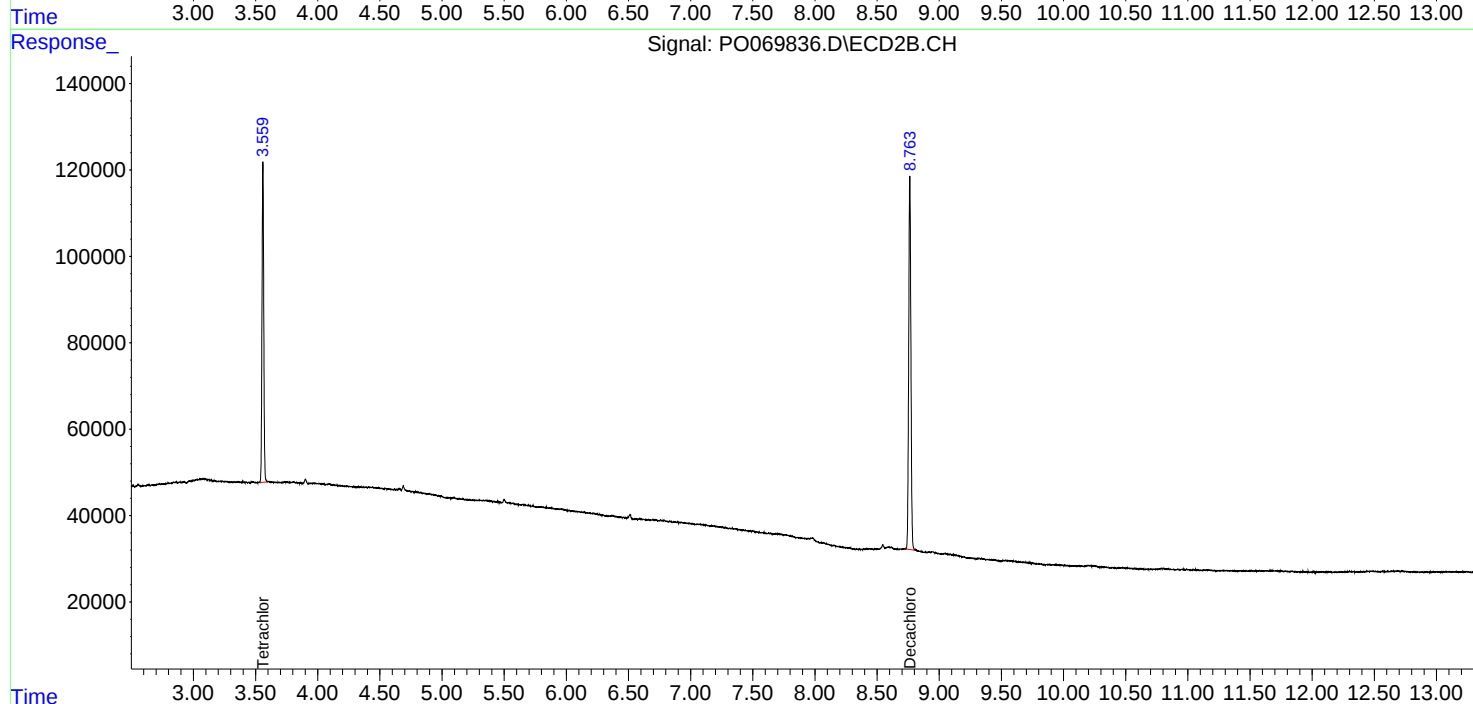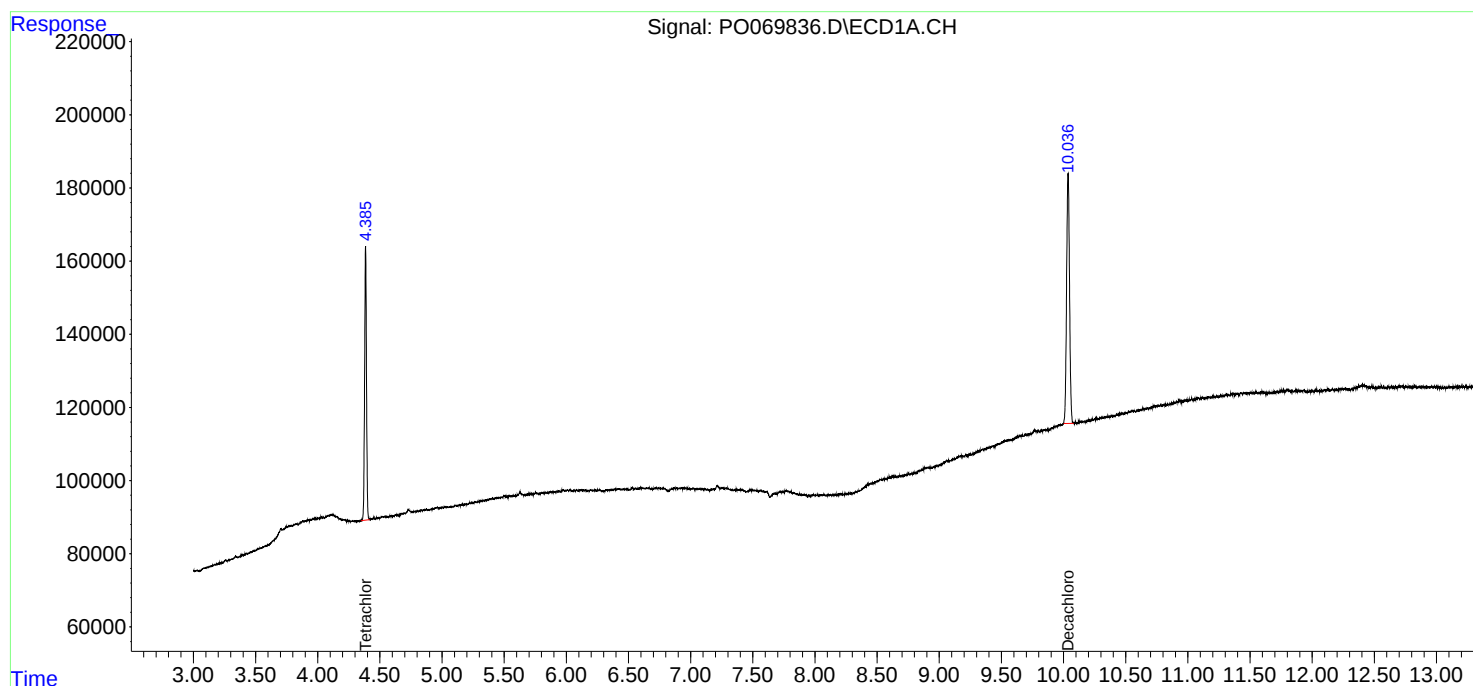


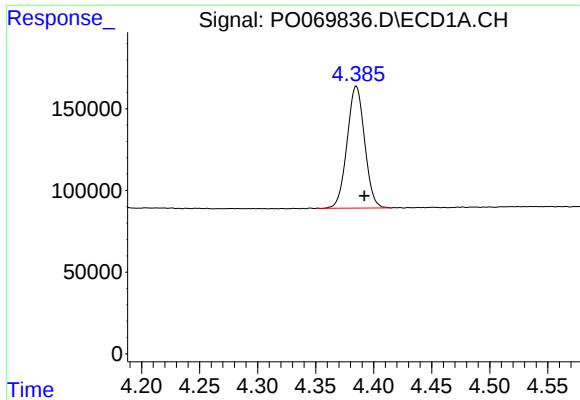

#1 Tetrachloro-m-xylene


R.T.: 4.385 min
Delta R.T.: -0.007 min
Response: 785313
Conc: 21.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB130336BL

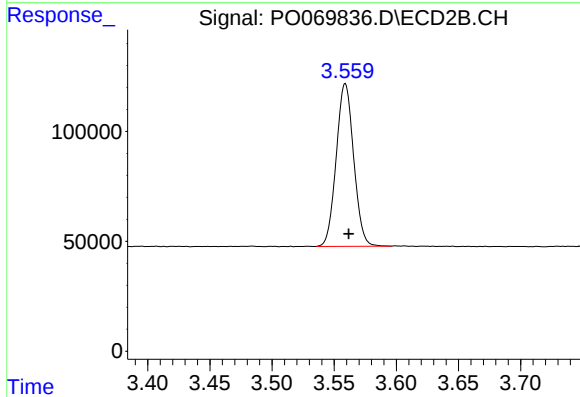


#1 Tetrachloro-m-xylene

R.T.: 3.559 min
Delta R.T.: -0.003 min
Response: 724859
Conc: 18.21 ng/ml

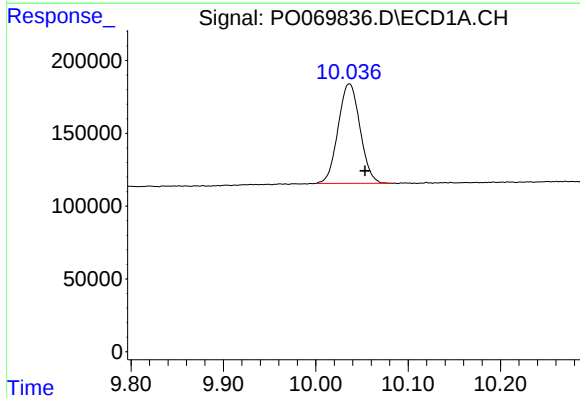

#2 Decachlorobiphenyl

R.T.: 10.037 min
Delta R.T.: -0.017 min
Response: 1128357
Conc: 18.75 ng/ml

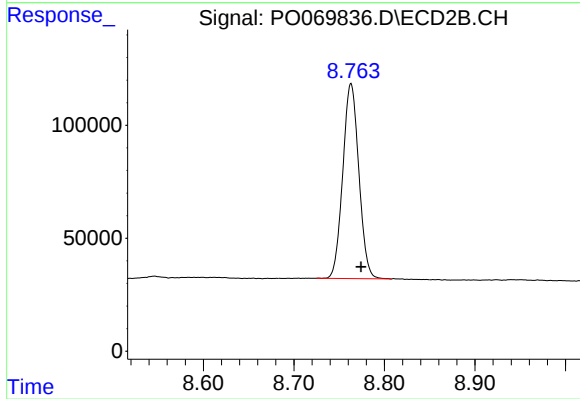

#2 Decachlorobiphenyl

R.T.: 8.763 min
Delta R.T.: -0.011 min
Response: 1064088
Conc: 18.75 ng/ml