

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072120\
 Data File : P0069829.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jul 2020 9:22
 Operator : DD\AJ
 Sample : L3324-05RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TOTE-50-DIAZRE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 08:28:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 08 16:12:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.385	3.560	290804	186881	7.789	4.696 #
2) SA Decachlor...	10.036	8.763	305861	317541	5.084	5.595

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072120\
Data File : P0069829.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jul 2020 9:22
Operator : DD\AJ
Sample : L3324-05RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TOTE-50-DIAZRE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 08:28:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 08 16:12:41 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

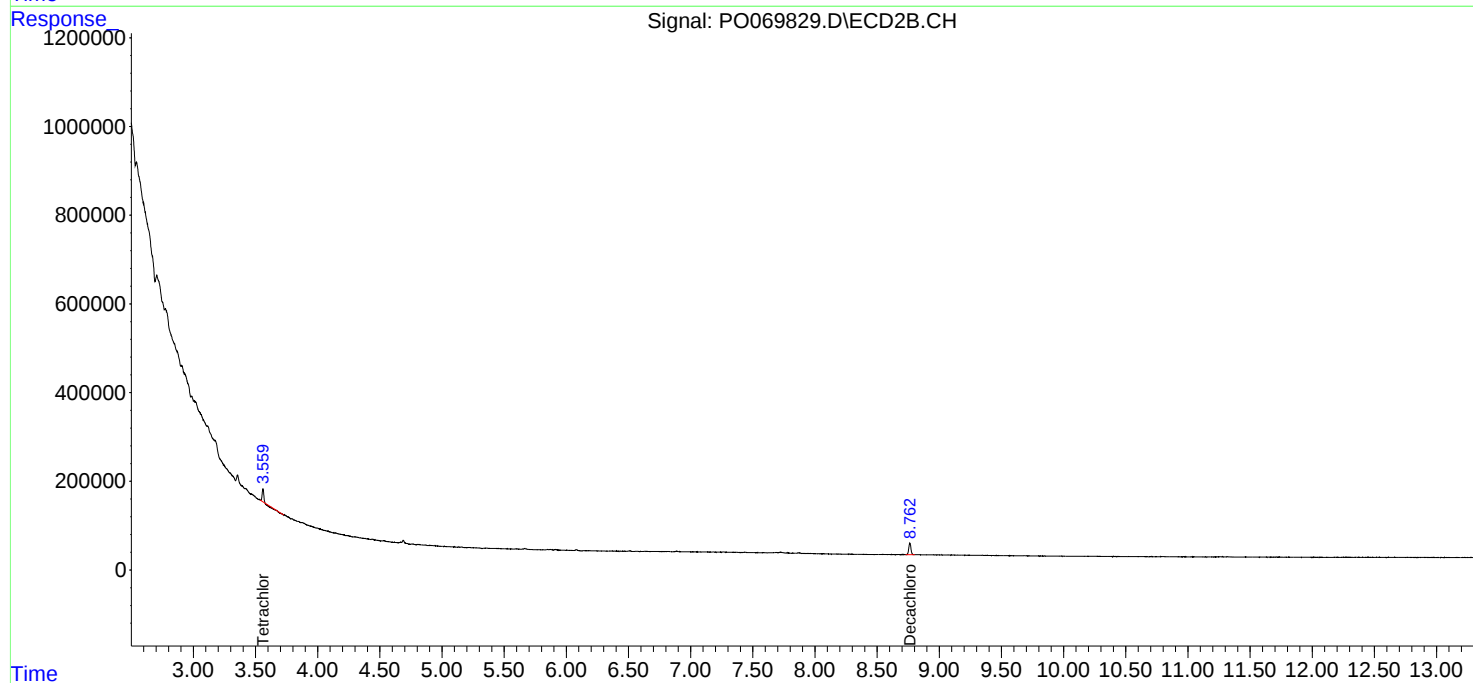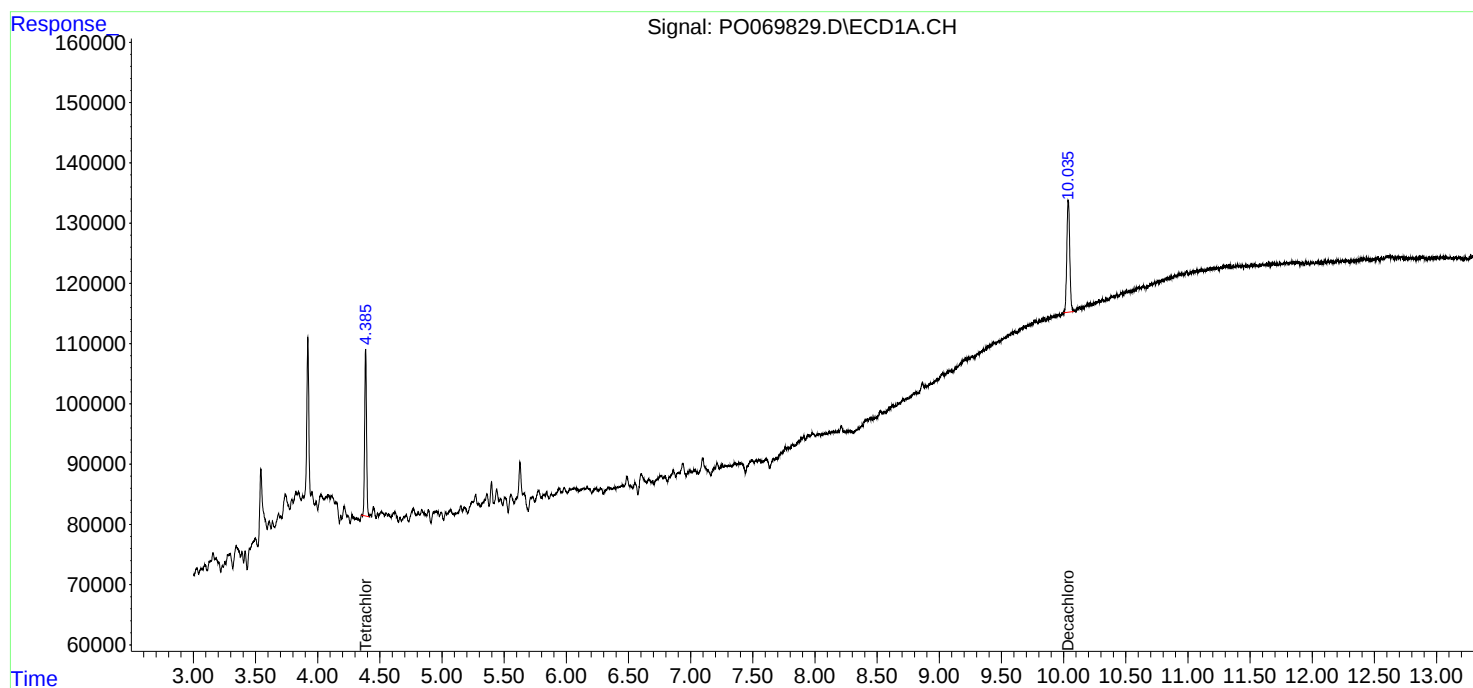


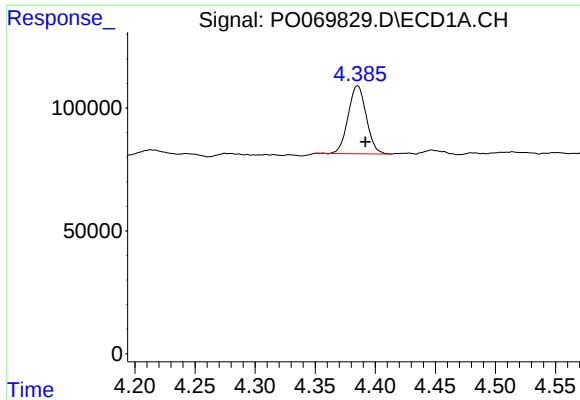

#1 Tetrachloro-m-xylene


R.T.: 4.385 min
Delta R.T.: -0.007 min
Response: 290804
Conc: 7.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
TOTE-50-DIAZRE

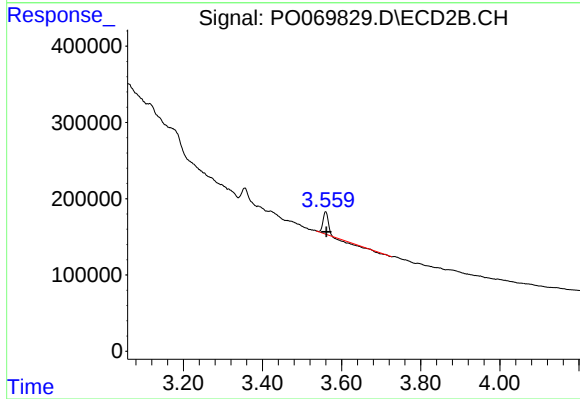


#1 Tetrachloro-m-xylene

R.T.: 3.560 min
Delta R.T.: -0.002 min
Response: 186881
Conc: 4.70 ng/ml

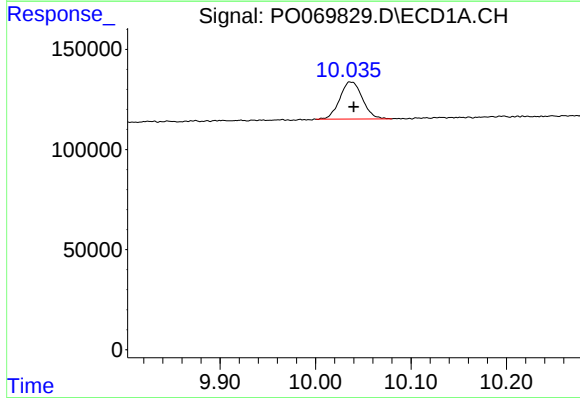

#2 Decachlorobiphenyl

R.T.: 10.036 min
Delta R.T.: -0.004 min
Response: 305861
Conc: 5.08 ng/ml

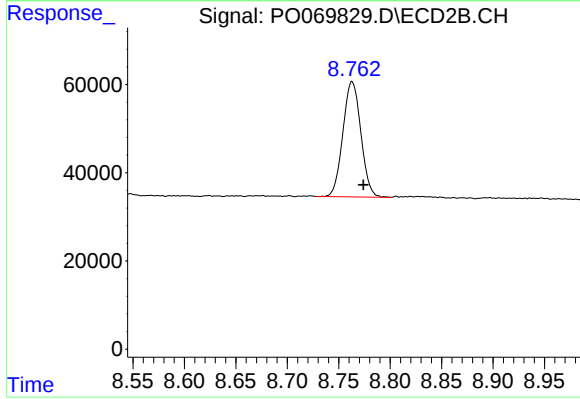

#2 Decachlorobiphenyl

R.T.: 8.763 min
Delta R.T.: -0.011 min
Response: 317541
Conc: 5.60 ng/ml