

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072120\
 Data File : P0069833.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jul 2020 11:38
 Operator : DD\AJ
 Sample : L3356-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S5-04-B-01

Manual Integrations
 APPROVED

Ankita
 7/29/2020 8:28:28 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 06:40:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 08 16:12:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.388	3.561	879861	862415	23.566m	21.671
2) SA Decachlor...	10.041	8.766	8445801	7078600	140.374	124.724
Target Compounds						
31) L7 AR-1260-1	7.358	6.360	333476	433999	126.825m	164.545 #
32) L7 AR-1260-2	7.626	6.561	926603	801092	261.206	244.746
33) L7 AR-1260-3	7.985	6.705	283016	376092	97.896	123.526 #
34) L7 AR-1260-4	8.209	7.186	529592	262254	178.799	96.887 #
35) L7 AR-1260-5	8.527	7.438	562791	467978	83.174	73.023

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072120\
Data File : P0069833.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jul 2020 11:38
Operator : DD\AJ
Sample : L3356-01
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S5-04-B-01


Manual Integrations
APPROVED

Ankita
7/29/2020 8:28:28 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 06:40:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 08 16:12:41 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

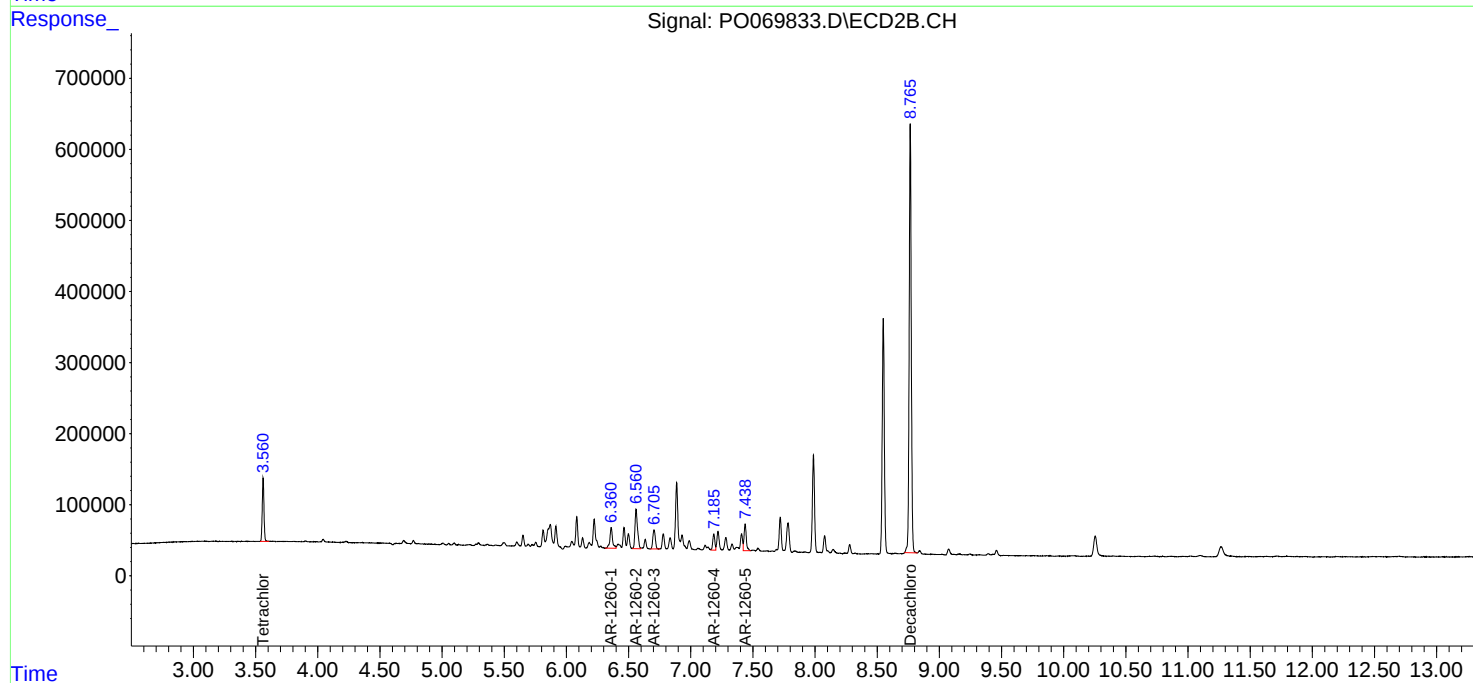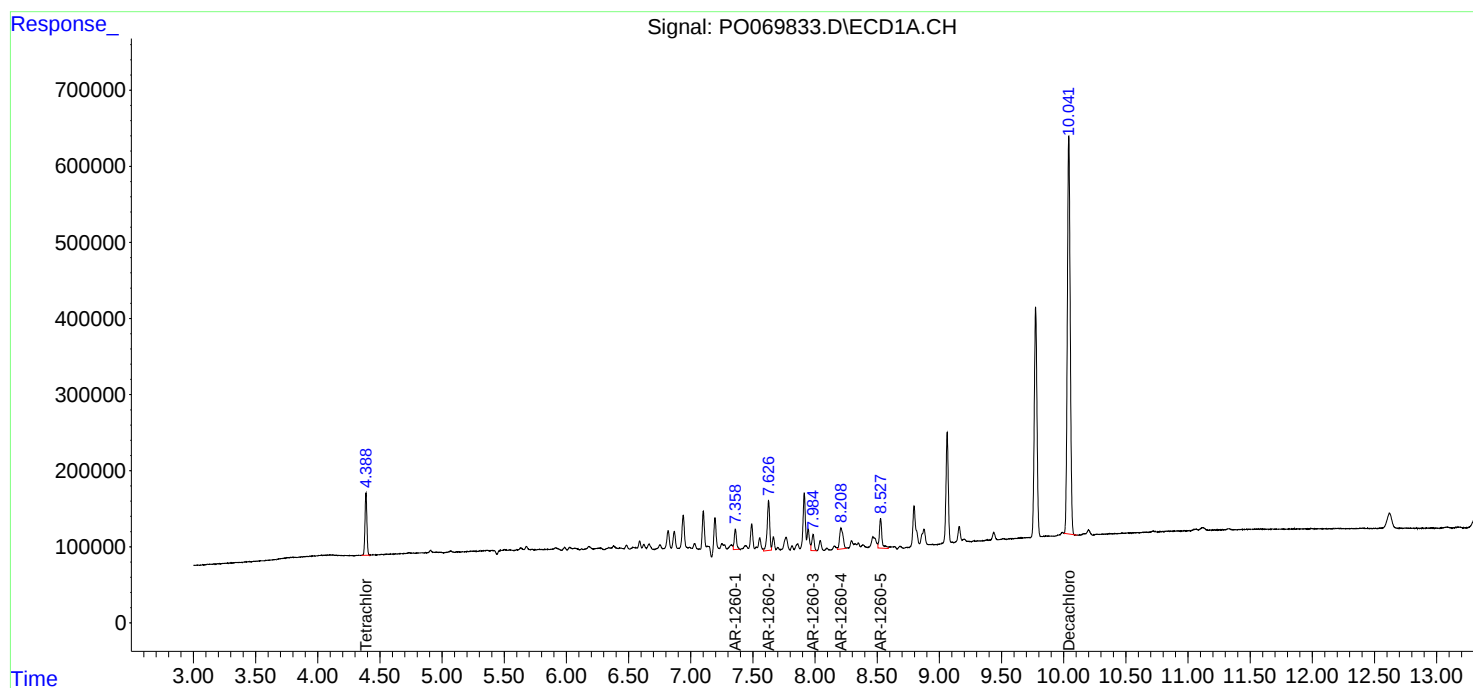

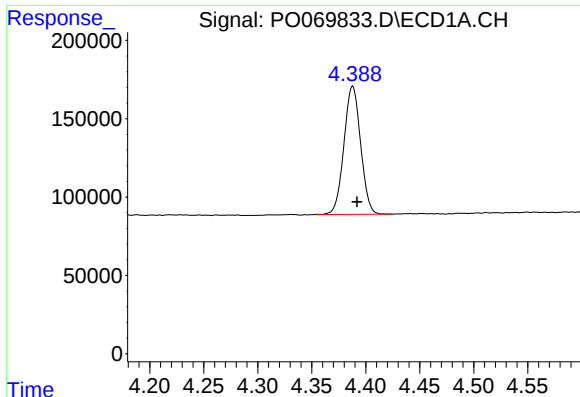


#1 Tetrachloro-m-xylene

R.T.: 4.388 min
Delta R.T.: -0.004 min
Response: 879861
Conc: 23.57 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S5-04-B-01


Manual Integrations
APPROVED

Ankita
7/29/2020 8:28:28 AM

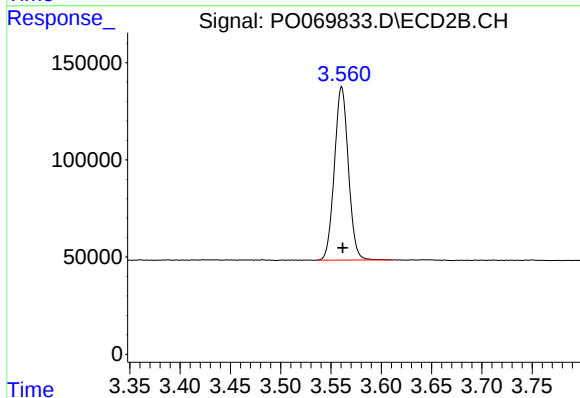


#1 Tetrachloro-m-xylene

R.T.: 3.561 min
Delta R.T.: 0.000 min
Response: 862415
Conc: 21.67 ng/ml

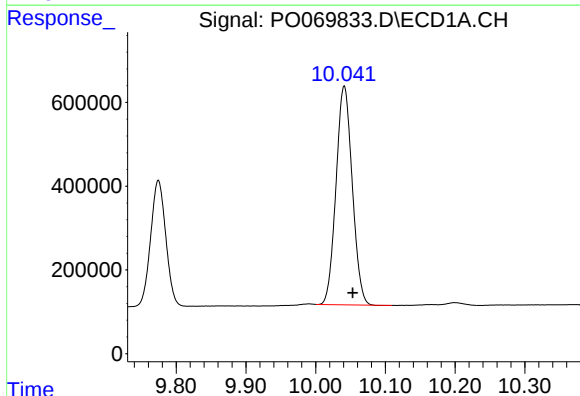


#2 Decachlorobiphenyl

R.T.: 10.041 min
Delta R.T.: -0.012 min
Response: 8445801
Conc: 140.37 ng/ml

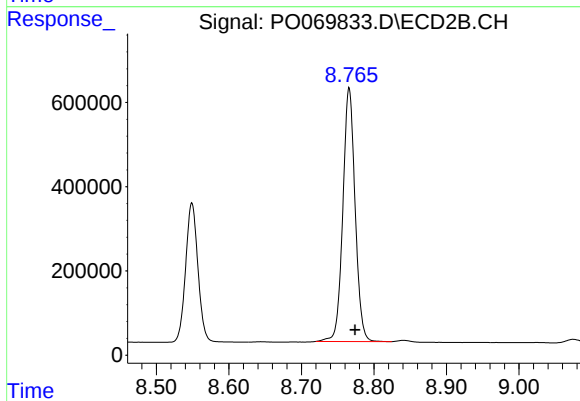

#2 Decachlorobiphenyl

R.T.: 8.766 min
Delta R.T.: -0.008 min
Response: 7078600
Conc: 124.72 ng/ml

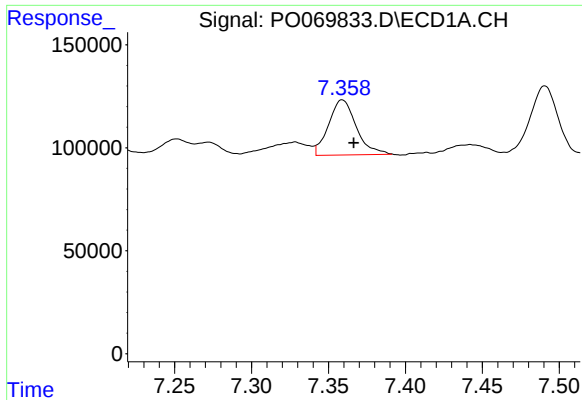


#31 AR-1260-1

R.T.: 7.358 min
Delta R.T.: -0.008 min
Response: 333476
Conc: 126.83 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S5-04-B-01


Manual Integrations
APPROVED

Ankita
7/29/2020 8:28:28 AM

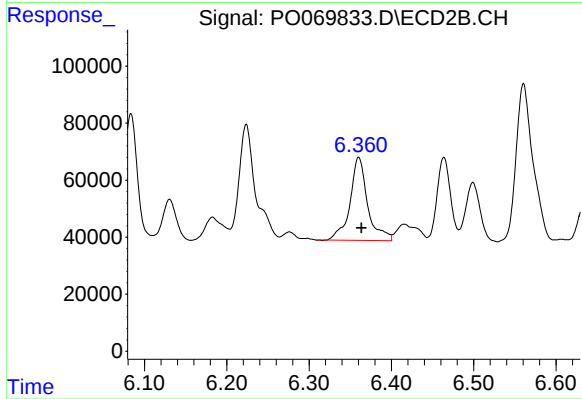


#31 AR-1260-1

R.T.: 6.360 min
Delta R.T.: -0.003 min
Response: 433999
Conc: 164.54 ng/ml

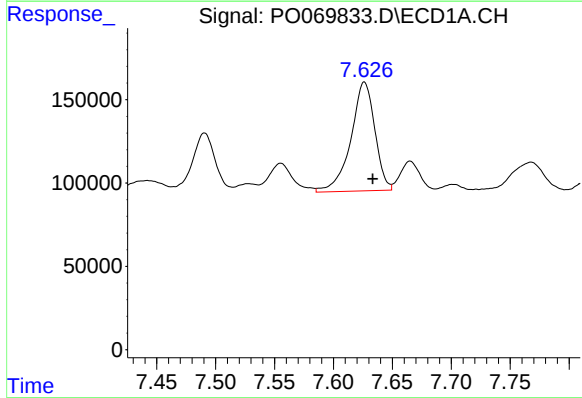


#32 AR-1260-2

R.T.: 7.626 min
Delta R.T.: -0.007 min
Response: 926603
Conc: 261.21 ng/ml

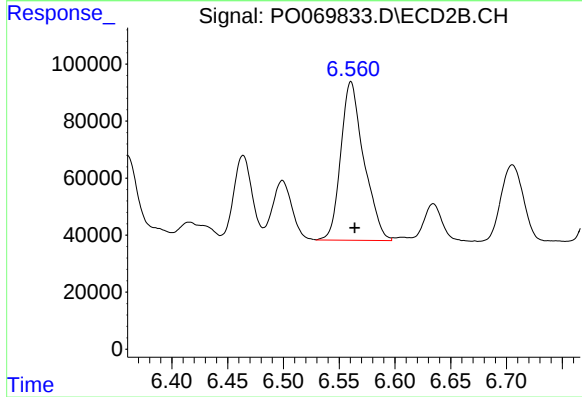

#32 AR-1260-2

R.T.: 6.561 min
Delta R.T.: -0.003 min
Response: 801092
Conc: 244.75 ng/ml

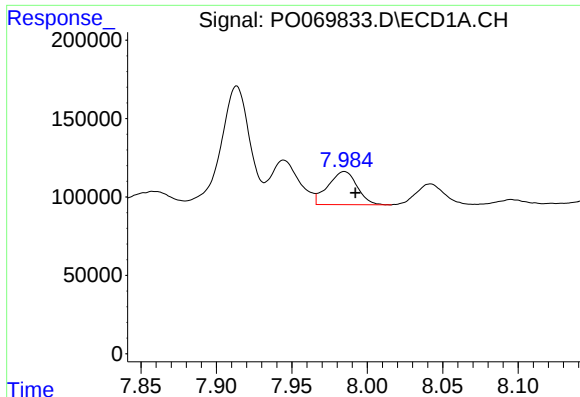


#33 AR-1260-3

R.T.: 7.985 min
Delta R.T.: -0.007 min
Response: 283016
Conc: 97.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-04-B-01


Manual Integrations
APPROVED

Ankita
7/29/2020 8:28:28 AM

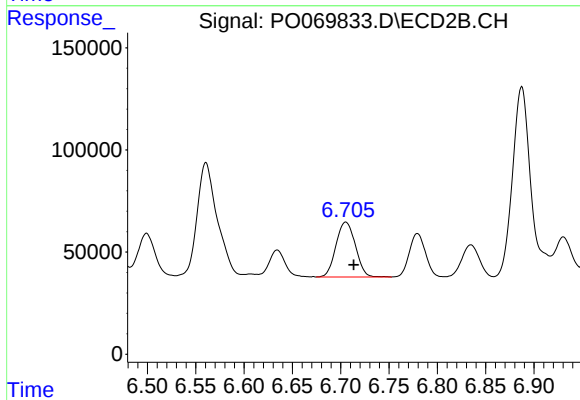


#33 AR-1260-3

R.T.: 6.705 min
Delta R.T.: -0.008 min
Response: 376092
Conc: 123.53 ng/ml

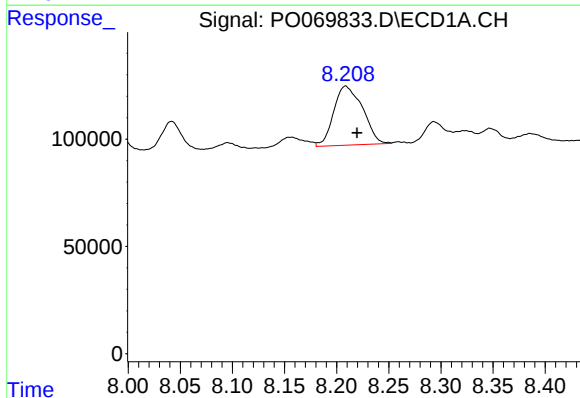


#34 AR-1260-4

R.T.: 8.209 min
Delta R.T.: -0.011 min
Response: 529592
Conc: 178.80 ng/ml

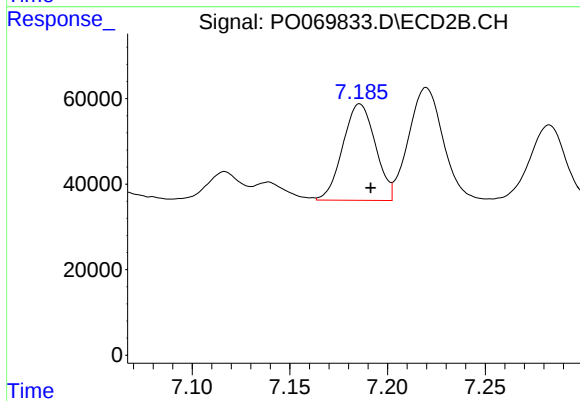

#34 AR-1260-4

R.T.: 7.186 min
Delta R.T.: -0.006 min
Response: 262254
Conc: 96.89 ng/ml

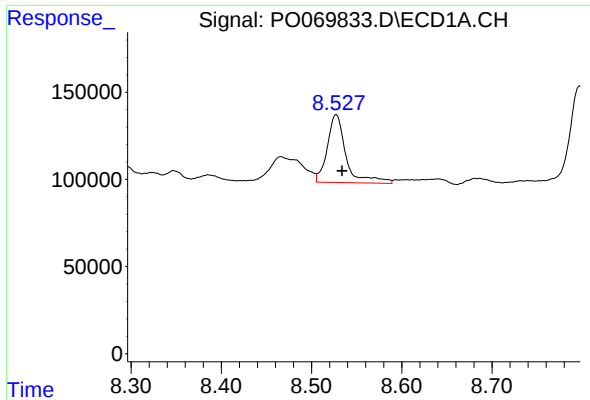


#35 AR-1260-5

R.T.: 8.527 min
Delta R.T.: -0.007 min
Response: 562791
Conc: 83.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-04-B-01

Manual Integrations
APPROVED

Ankita
7/29/2020 8:28:28 AM

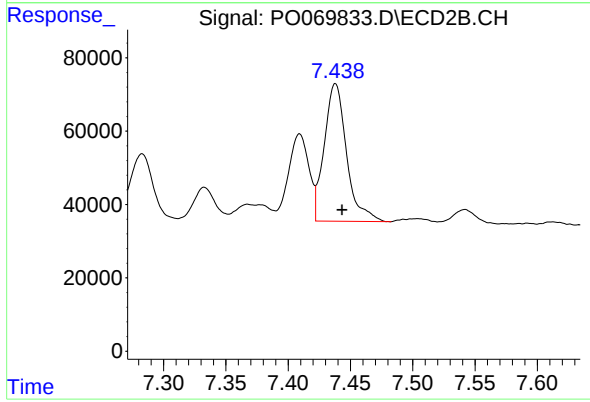

#35 AR-1260-5

R.T.: 7.438 min
Delta R.T.: -0.005 min
Response: 467978
Conc: 73.02 ng/ml