

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072120\
 Data File : P0069838.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jul 2020 13:05
 Operator : DD\AJ
 Sample : L3184-13
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 EO-03-072020

Manual Integrations
 APPROVED

Ankita
 7/22/2020 2:35:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 15:01:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 08 16:12:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.385	3.560	1024890	1117634	27.451m	28.084
2) SA Decachlor...	10.037f	8.764	1271786	1096003	21.138	19.311

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072120\
Data File : P0069838.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jul 2020 13:05
Operator : DD\AJ
Sample : L3184-13
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
EO-03-072020


Manual Integrations
APPROVED

Ankita
7/22/2020 2:35:10 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 15:01:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 08 16:12:41 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

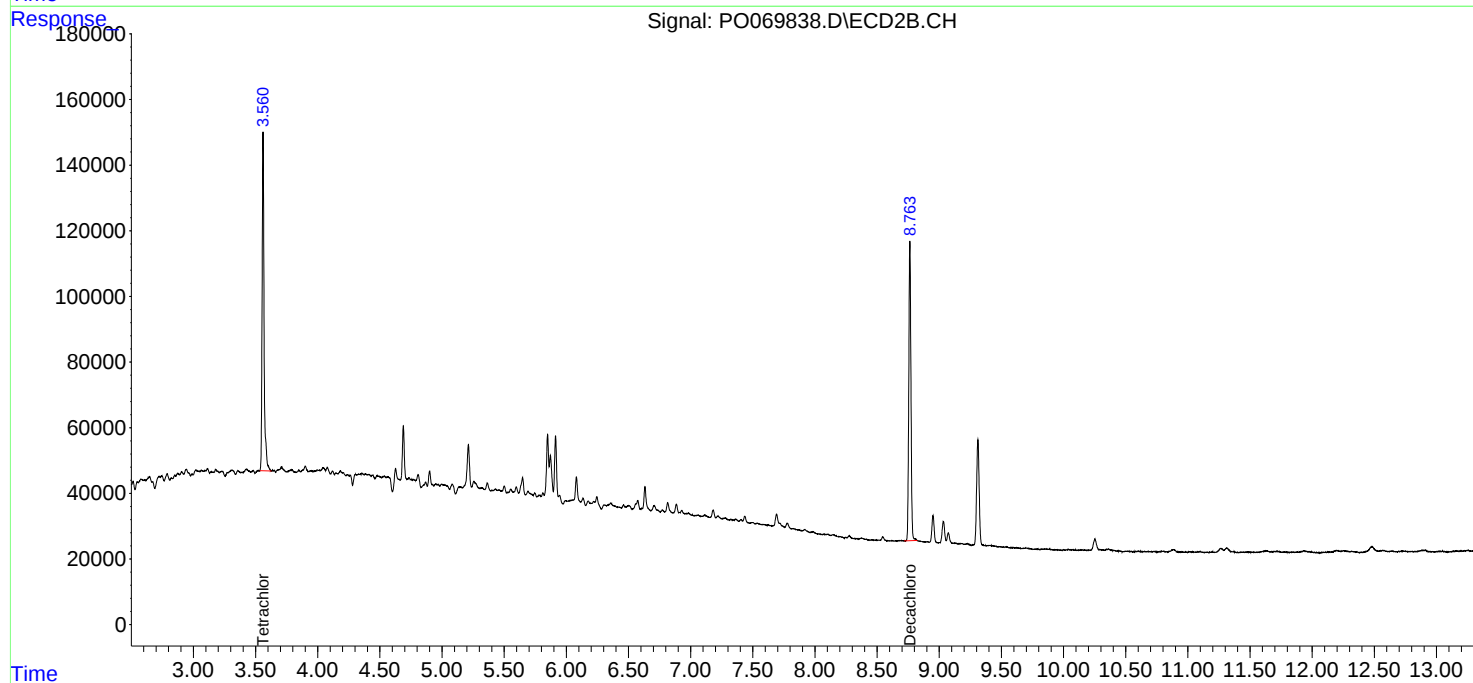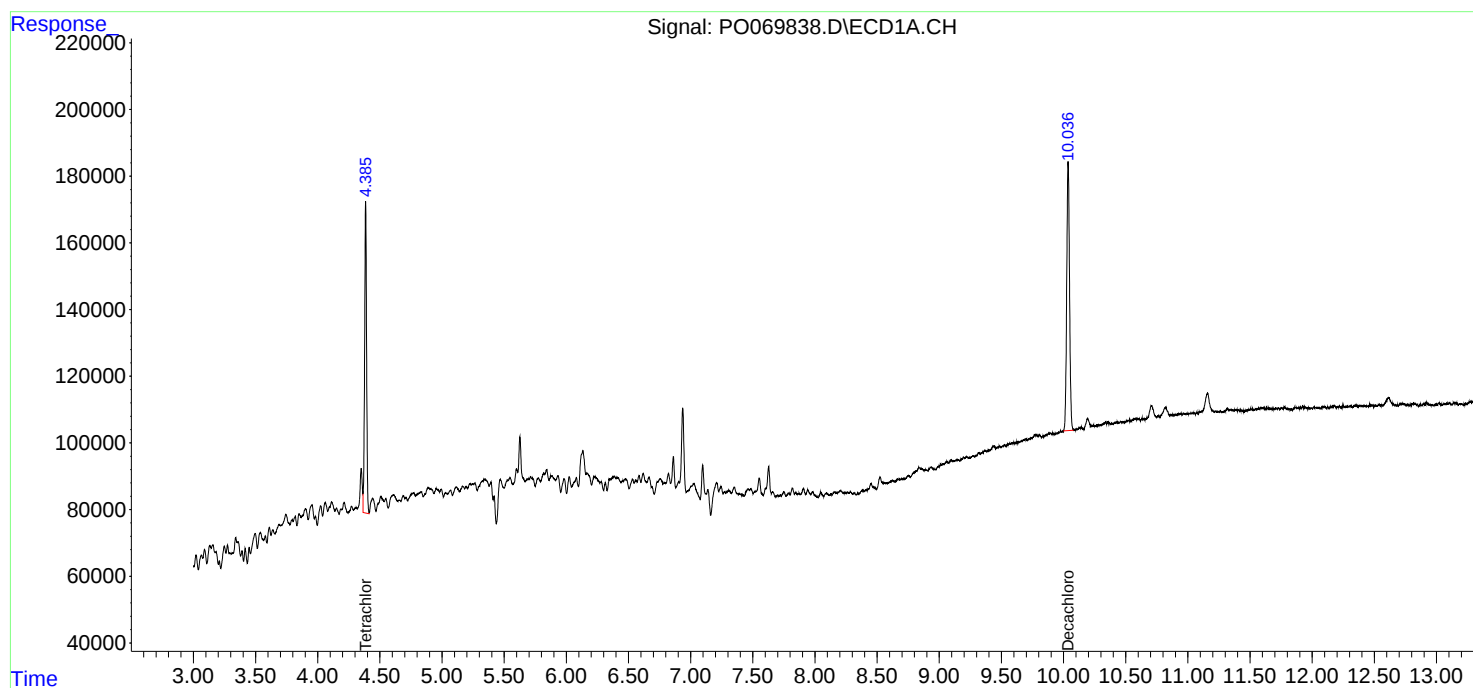

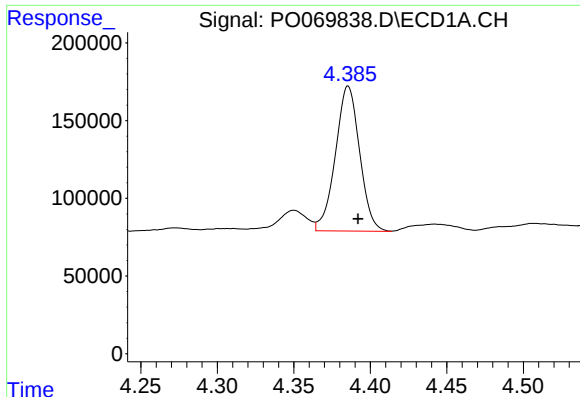


#1 Tetrachloro-m-xylene

R.T.: 4.385 min
Delta R.T.: -0.007 min
Response: 1024890
Conc: 27.45 ng/ml m

Instrument :
ECD_O
ClientSampleId :
EO-03-072020


Manual Integrations
APPROVED

Ankita
7/22/2020 2:35:10 PM

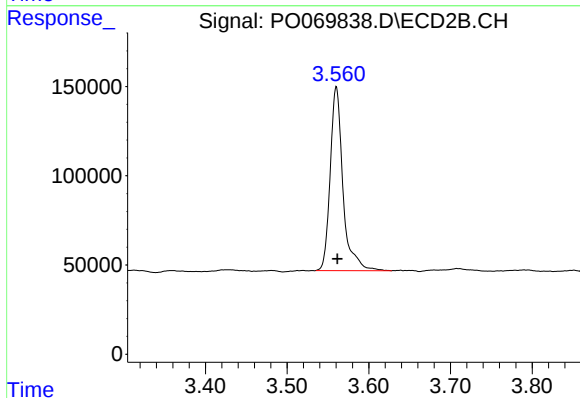


#1 Tetrachloro-m-xylene

R.T.: 3.560 min
Delta R.T.: -0.001 min
Response: 1117634
Conc: 28.08 ng/ml

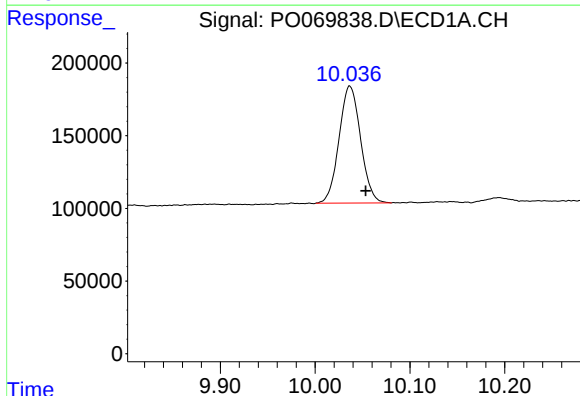

#2 Decachlorobiphenyl

R.T.: 10.037 min
Delta R.T.: -0.017 min
Response: 1271786
Conc: 21.14 ng/ml

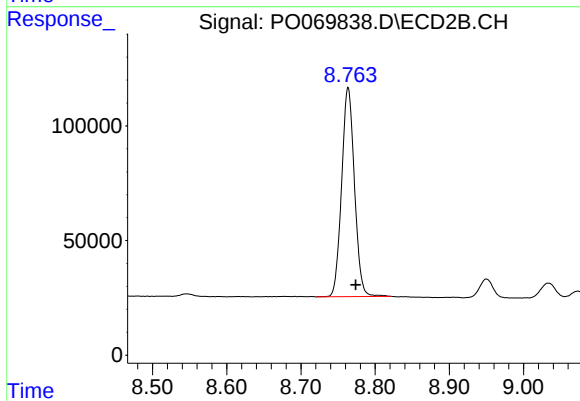

#2 Decachlorobiphenyl

R.T.: 8.764 min
Delta R.T.: -0.010 min
Response: 1096003
Conc: 19.31 ng/ml