

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072122\
 Data File : P0088247.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2022 17:43
 Operator : YP/AJ
 Sample : N3786-13
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 0718-WC-TP-WC5A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/22/2022
 Supervised By :Ankita Jodhani 07/22/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 21 23:40:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071422.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 15 03:57:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.447	3.606	63160904	23115428	24.757	24.500
2) SA Decachlor...	10.294	8.603	43014747	22973315	20.255	21.983m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072122\
Data File : P0088247.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2022 17:43
Operator : YP/AJ
Sample : N3786-13
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
0718-WC-TP-WC5A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2022
Supervised By :Ankita Jodhani 07/22/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 21 23:40:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0071422.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 15 03:57:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

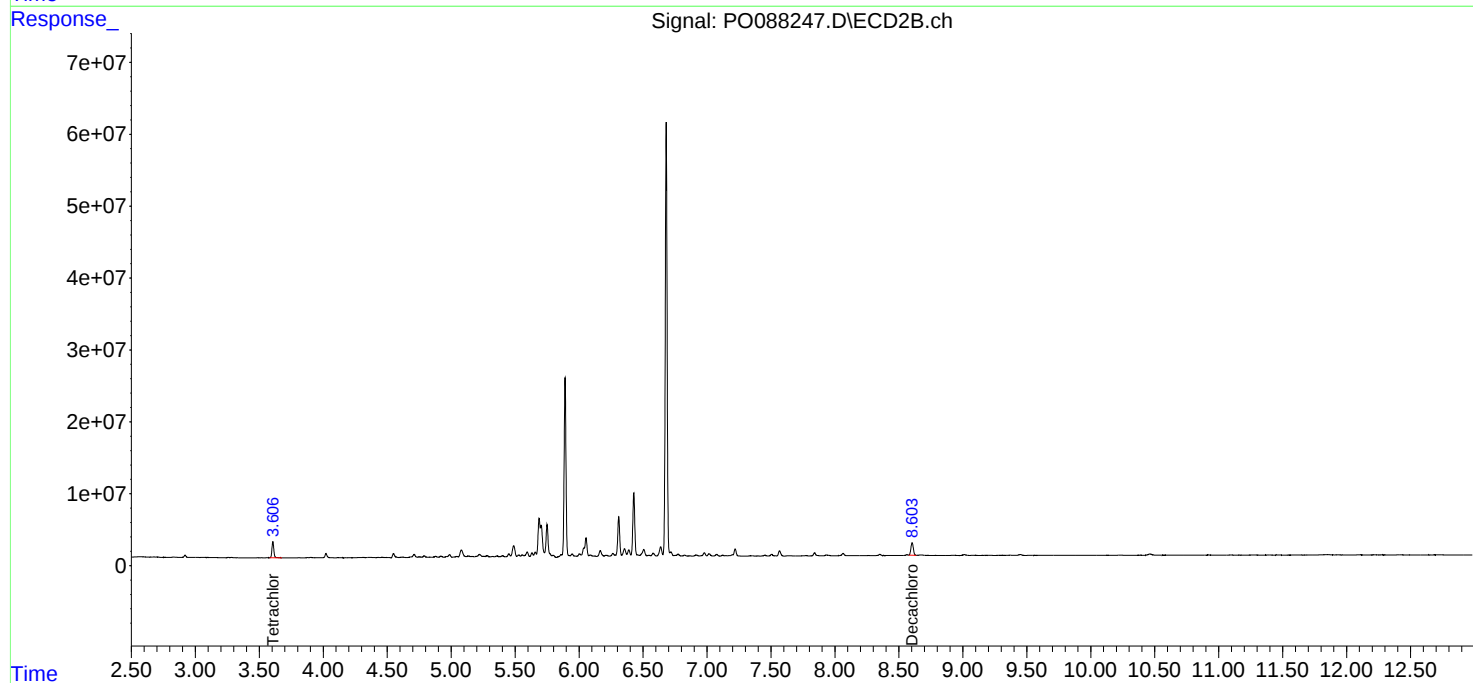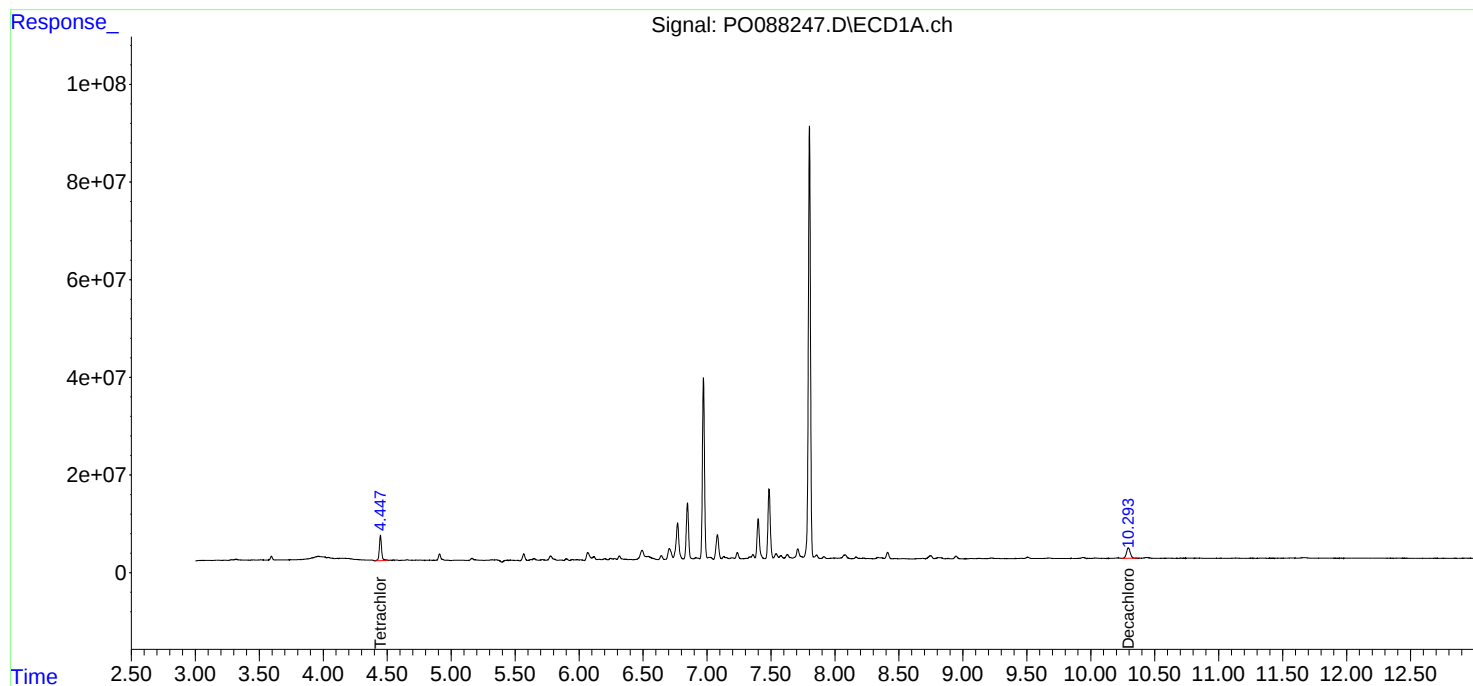

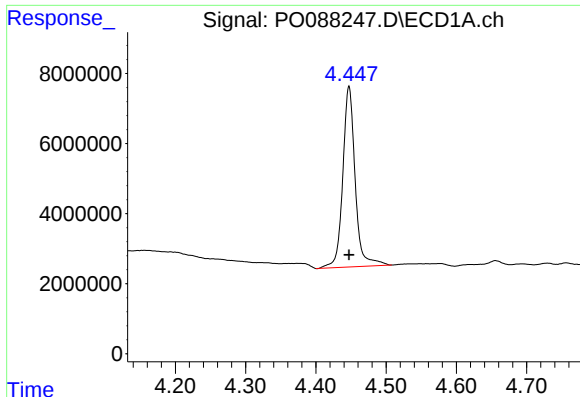


#1 Tetrachloro-m-xylene

R.T.: 4.447 min
Delta R.T.: 0.000 min
Response: 63160904
Conc: 24.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
0718-WC-TP-WC5A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/22/2022
Supervised By :Ankita Jodhani 07/22/2022

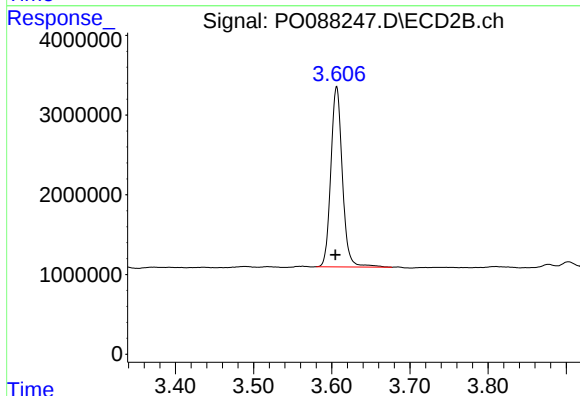


#1 Tetrachloro-m-xylene

R.T.: 3.606 min
Delta R.T.: 0.002 min
Response: 23115428
Conc: 24.50 ng/ml

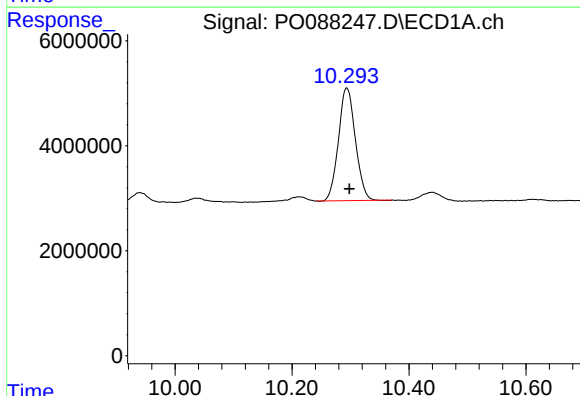

#2 Decachlorobiphenyl

R.T.: 10.294 min
Delta R.T.: -0.005 min
Response: 43014747
Conc: 20.25 ng/ml

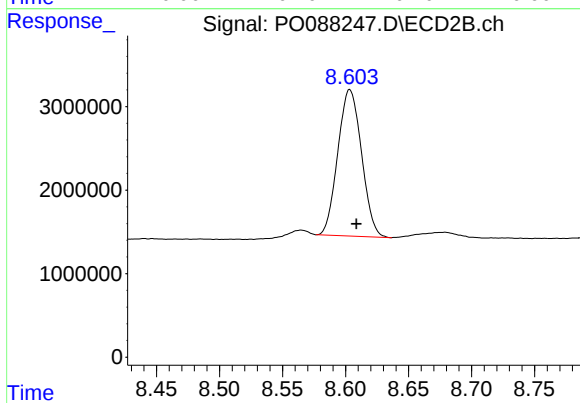

#2 Decachlorobiphenyl

R.T.: 8.603 min
Delta R.T.: -0.006 min
Response: 22973315
Conc: 21.98 ng/ml m