

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072125\
 Data File : P0112337.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jul 2025 12:53
 Operator : YP/AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 01:47:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 21 10:54:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.665	3.663	460367	110770	0.047	0.017 #
2)	SA Decachlor...	8.706	8.642	529205	104098	0.077	0.060
Target Compounds							
3)	L1 AR-1016-1	4.754	4.734	173892	216762	0.511	0.973 #
4)	L1 AR-1016-2	4.772	4.755	490663	76632	0.987	0.233 #
5)	L1 AR-1016-3	4.829	4.982	852209	3587326	2.633	21.118 #
6)	L1 AR-1016-4	4.952	4.982	7704496	3587326	30.002	26.141
7)	L1 AR-1016-5	5.228	5.196	28964951	5370574	105.842	31.143 #
8)	L2 AR-1221-1	3.879	3.870	171155	63331	1.468	0.770 #
9)	L2 AR-1221-2	3.902f	3.957	627149	77978	7.955	1.314 #
12)	L3 AR-1232-2	4.535	4.755	472089	76632	4.154	0.501 #
13)	L3 AR-1232-3	4.772	4.935	490663	1007265	2.143	13.340 #
14)	L3 AR-1232-4	4.952	4.982	7704496	3587326	67.408	54.363
15)	L3 AR-1232-5	5.008	5.196	4971544	5370574	67.732	72.321
16)	L4 AR-1242-1	4.754	4.734	173892	216762	0.600	1.118 #
17)	L4 AR-1242-2	4.772	4.755	490663	76632	1.152	0.270 #
18)	L4 AR-1242-3	4.829	4.935	852209	1007265	3.114	6.914 #
19)	L4 AR-1242-4	4.952	4.982	7704496	3587326	34.194	25.291 #
20)	L4 AR-1242-5	5.586	5.528	38937051	5056942	183.951	27.826 #
21)	L5 AR-1248-1	4.754	4.734	173892	216762	0.766	1.404 #
22)	L5 AR-1248-2	5.008	4.982	4971544	3587326	16.124	17.434
23)	L5 AR-1248-3	5.228	4.982	28964951	3587326	71.111	16.701 #
24)	L5 AR-1248-4	5.586	5.196	38937051	5370574	67.465	20.758 #
25)	L5 AR-1248-5	5.586	5.592	38937051	3445220	99.761	13.751 #
26)	L6 AR-1254-1	5.586	5.528	38937051	5056942	63.301	13.267 #
27)	L6 AR-1254-2	5.735	5.707	44308870	15956035	82.714	48.088 #
28)	L6 AR-1254-3	6.135	6.103	11583843	17461996	13.797	36.225 #
29)	L6 AR-1254-4	6.327	6.330	3818976	2391280	7.939	9.173
30)	L6 AR-1254-5	6.764	6.729	4652.6E6	2218.8E6	6011.472	6226.392
31)	L7 AR-1260-1	6.236	6.198	357849	5879942	0.714	20.958 #
32)	L7 AR-1260-2	6.442	6.407	8796070	5639735	11.917	16.588 #
33)	L7 AR-1260-3	6.764f	0.000	4652.6E6	0	7097.931	N.D. #
34)	L7 AR-1260-4	7.059	0.000	2614469	0	6.007	N.D. #
35)	L7 AR-1260-5	7.300	7.246	3461684	346512	2.742	0.774 #
36)	L8 AR-1262-1	6.764f	6.729f	4652.6E6	2218.8E6	4553.807	5447.336
37)	L8 AR-1262-2	7.300	7.246	3461684	346512	2.112	0.676 #
38)	L8 AR-1262-3	7.591	7.563	3801135	9037742	5.921	50.343 #
39)	L8 AR-1262-4	7.659	7.563f	555217	9037742	0.518	31.066 #
41)	L9 AR-1268-1	7.591	7.563	3801135	9037742	2.069	18.390 #
42)	L9 AR-1268-2	7.659	7.563f	555217	9037742	0.356	21.664 #
43)	L9 AR-1268-3	7.850	7.841	1531906	846	1.179	0.003 #
45)	L9 AR-1268-5	8.437	8.398	412086	199153	0.126	0.274 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072125\
Data File : P0112337.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2025 12:53
Operator : YP/AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 01:47:47 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 21 10:54:00 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO072125\
Data File : PO112337.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jul 2025 12:53
Operator : YP/AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 01:47:47 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 21 10:54:00 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

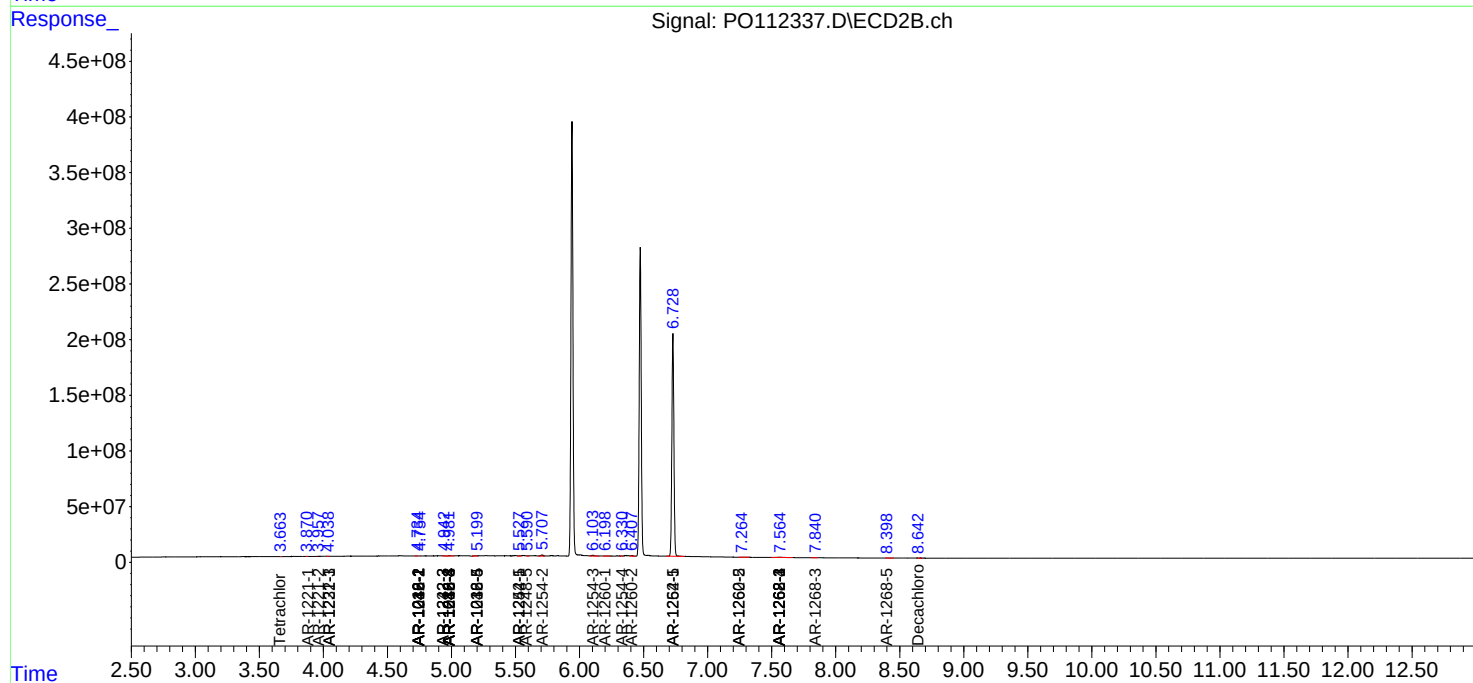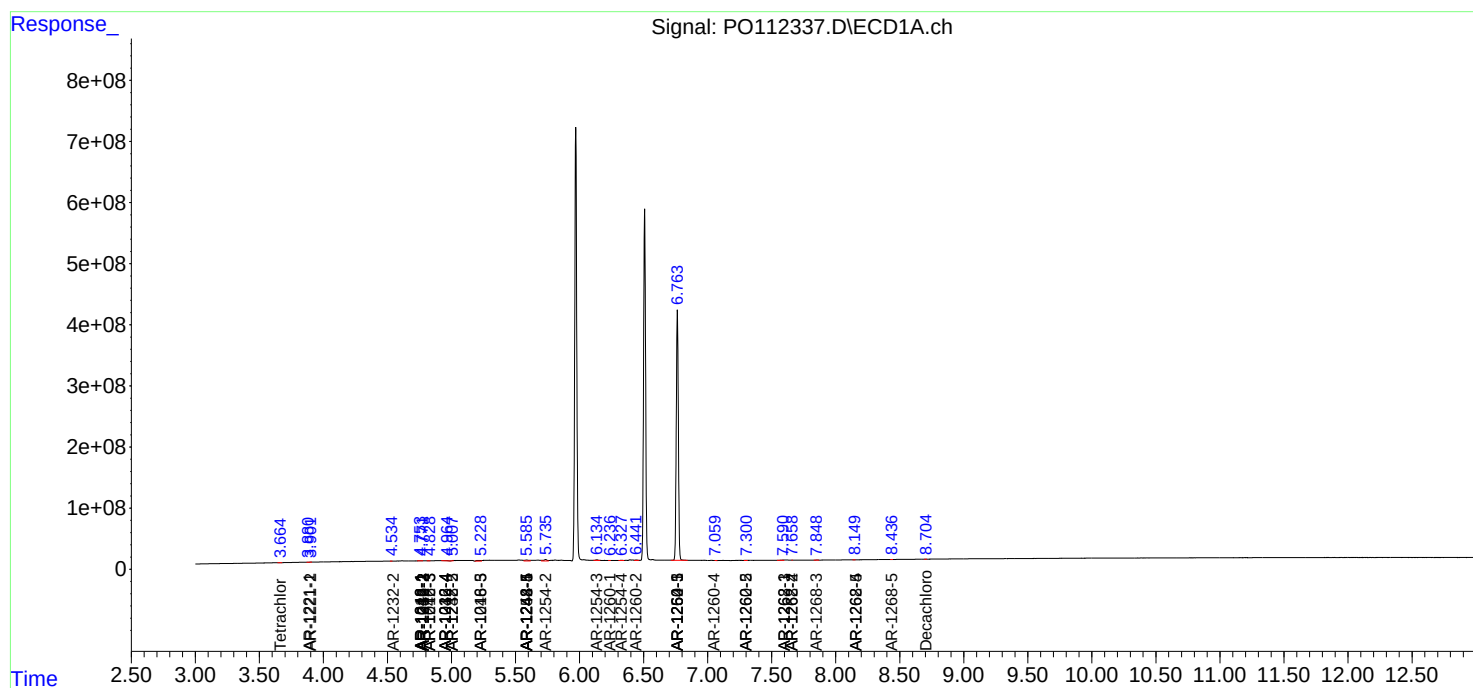


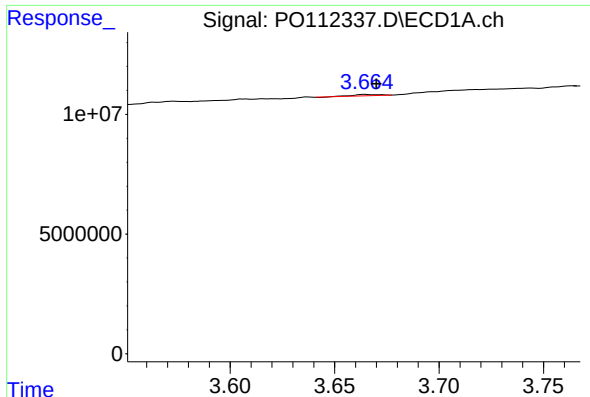

#1 Tetrachloro-m-xylene


R.T.: 3.665 min
Delta R.T.: -0.005 min
Response: 460367
Conc: 0.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

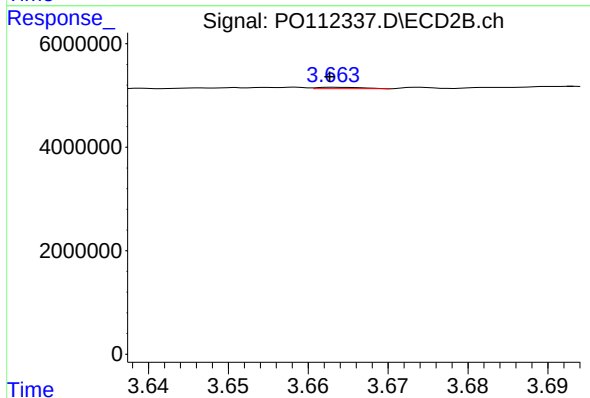


#1 Tetrachloro-m-xylene

R.T.: 3.663 min
Delta R.T.: 0.000 min
Response: 110770
Conc: 0.02 ng/ml

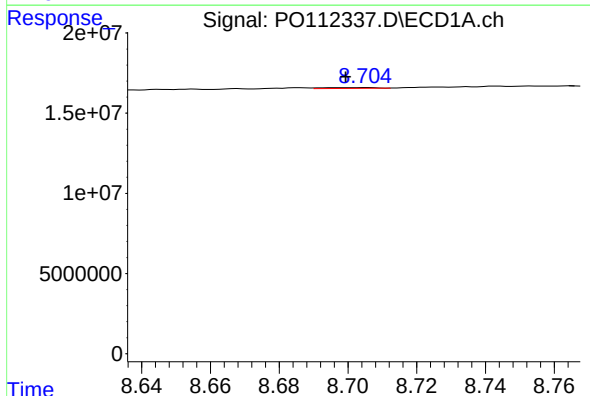


#2 Decachlorobiphenyl

R.T.: 8.706 min
Delta R.T.: 0.006 min
Response: 529205
Conc: 0.08 ng/ml

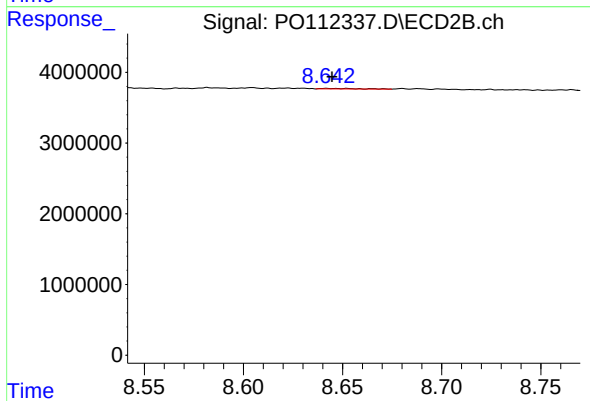

#2 Decachlorobiphenyl


R.T.: 8.642 min
Delta R.T.: -0.003 min
Response: 104098
Conc: 0.06 ng/ml

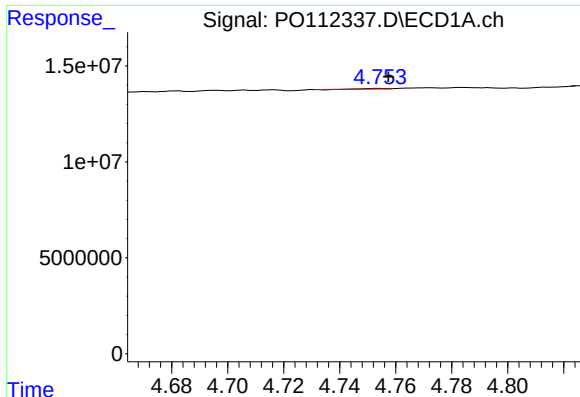

#3 AR-1016-1


R.T.: 4.754 min
Delta R.T.: -0.003 min
Response: 173892
Conc: 0.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

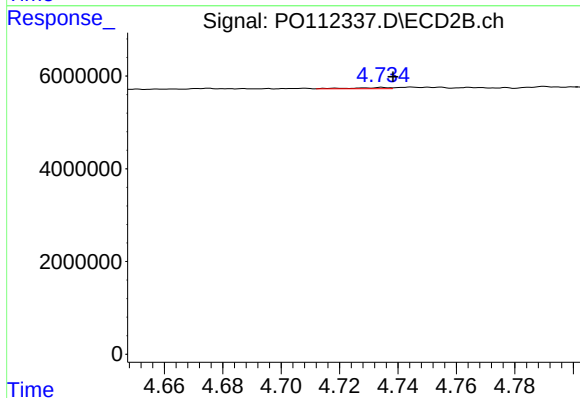


#3 AR-1016-1

R.T.: 4.734 min
Delta R.T.: -0.004 min
Response: 216762
Conc: 0.97 ng/ml

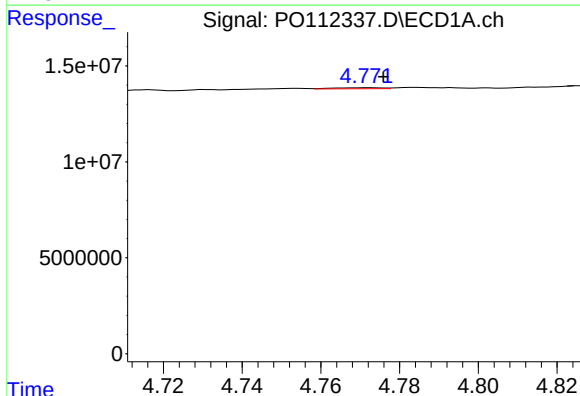


#4 AR-1016-2

R.T.: 4.772 min
Delta R.T.: -0.004 min
Response: 490663
Conc: 0.99 ng/ml

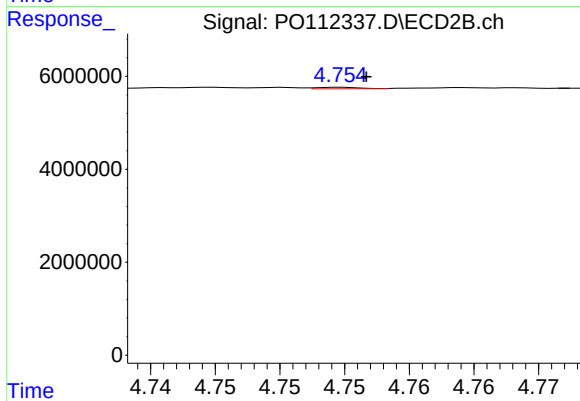

#4 AR-1016-2


R.T.: 4.755 min
Delta R.T.: -0.002 min
Response: 76632
Conc: 0.23 ng/ml

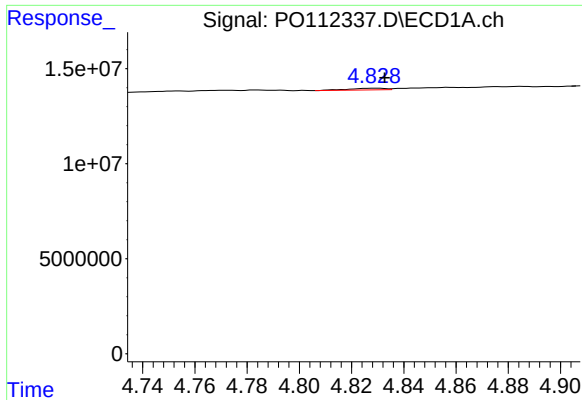

#5 AR-1016-3


R.T.: 4.829 min
Delta R.T.: -0.004 min
Response: 852209
Conc: 2.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

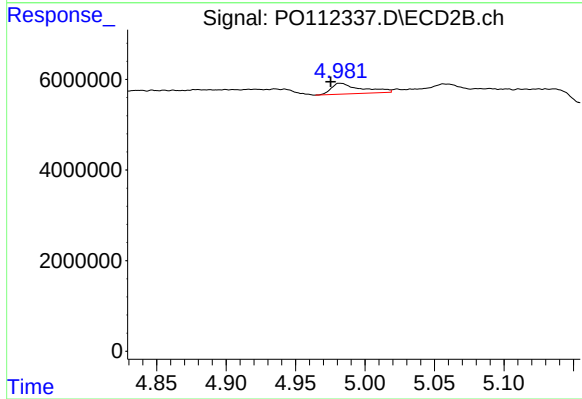


#5 AR-1016-3

R.T.: 4.982 min
Delta R.T.: 0.007 min
Response: 3587326
Conc: 21.12 ng/ml

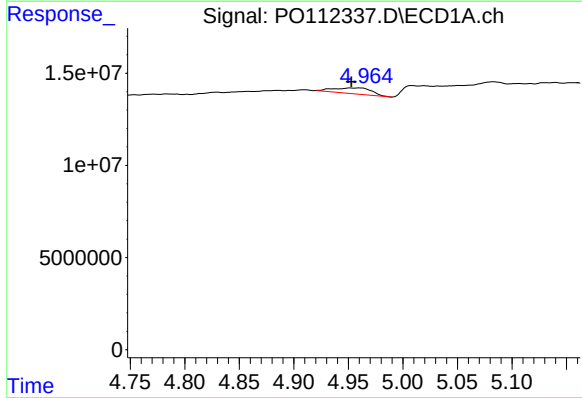


#6 AR-1016-4

R.T.: 4.952 min
Delta R.T.: 0.000 min
Response: 7704496
Conc: 30.00 ng/ml

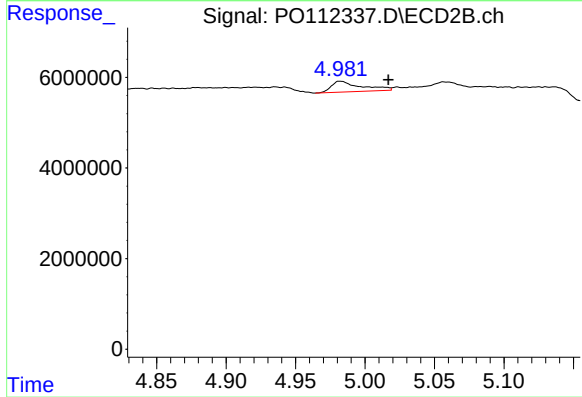

#6 AR-1016-4


R.T.: 4.982 min
Delta R.T.: -0.034 min
Response: 3587326
Conc: 26.14 ng/ml

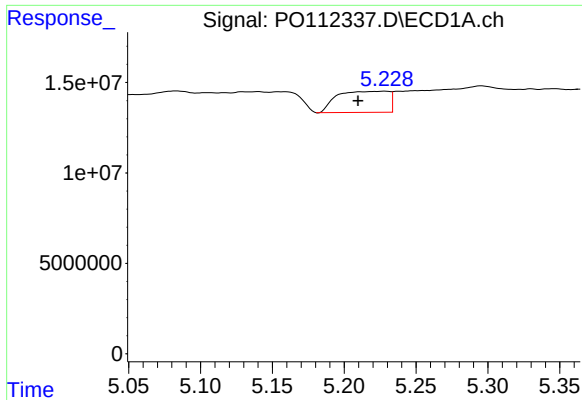

#7 AR-1016-5


R.T.: 5.228 min
Delta R.T.: 0.019 min
Response: 28964951
Conc: 105.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

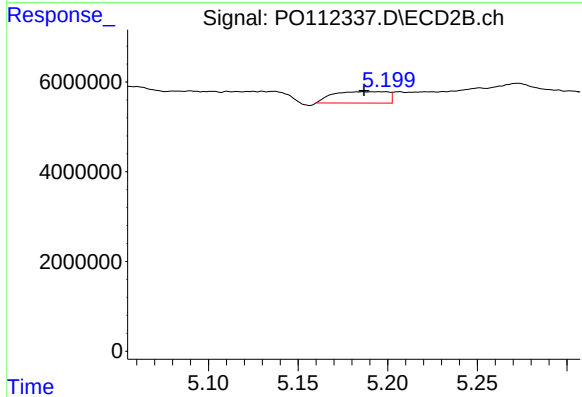


#7 AR-1016-5

R.T.: 5.196 min
Delta R.T.: 0.009 min
Response: 5370574
Conc: 31.14 ng/ml

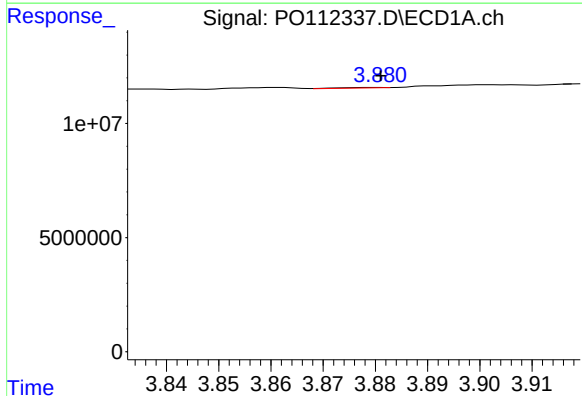


#8 AR-1221-1

R.T.: 3.879 min
Delta R.T.: -0.002 min
Response: 171155
Conc: 1.47 ng/ml

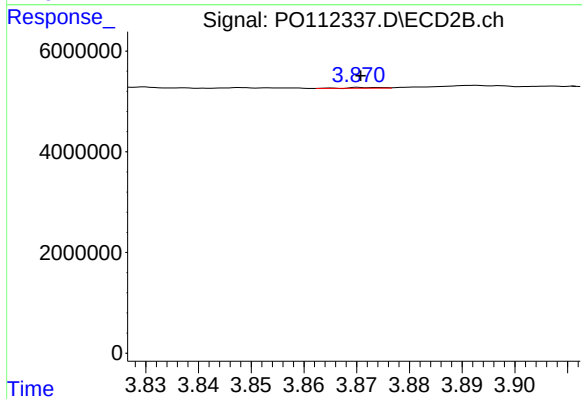

#8 AR-1221-1


R.T.: 3.870 min
Delta R.T.: 0.000 min
Response: 63331
Conc: 0.77 ng/ml

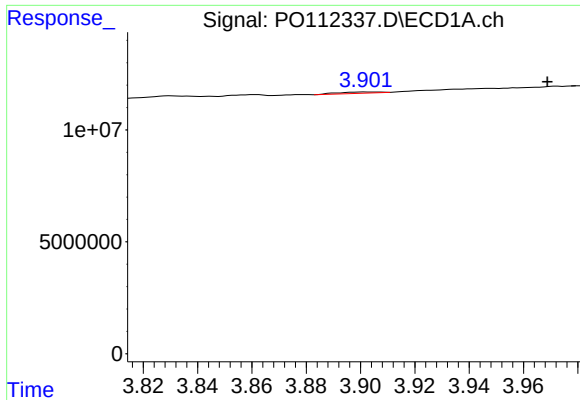

#9 AR-1221-2


R.T.: 3.902 min
Delta R.T.: -0.067 min
Response: 627149
Conc: 7.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

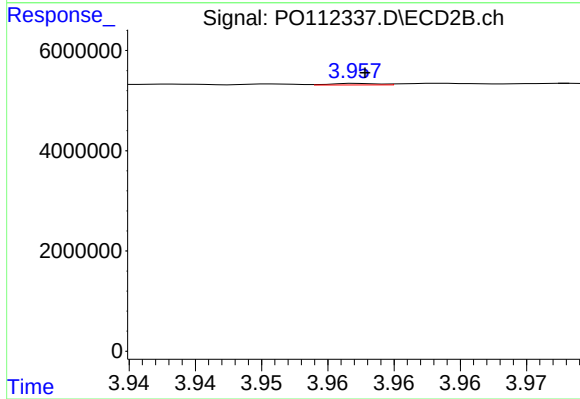


#9 AR-1221-2

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 77978
Conc: 1.31 ng/ml

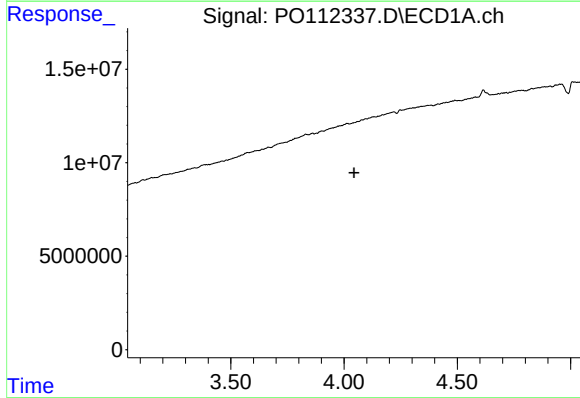


#10 AR-1221-3

R.T.: 4.078 min
Delta R.T.: 0.034 min
Response: -1275148
Conc: N.D.

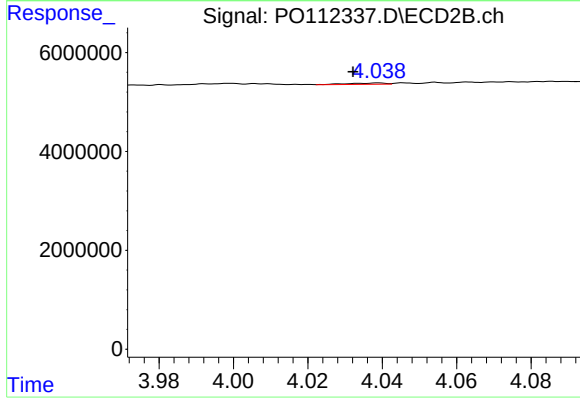

#10 AR-1221-3


R.T.: 4.039 min
Delta R.T.: 0.007 min
Response: 180134
Conc: 0.95 ng/ml

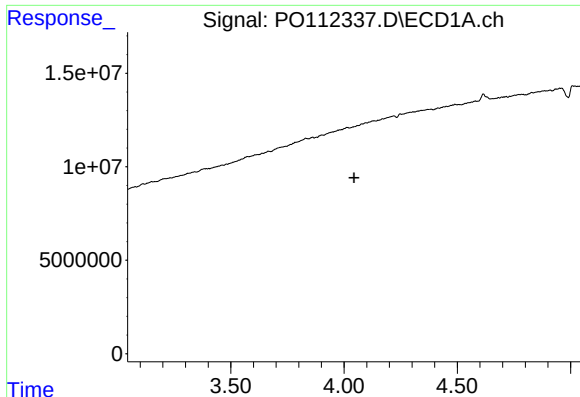

#11 AR-1232-1


R.T.: 4.078 min
Delta R.T.: 0.034 min
Response: -1275148
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

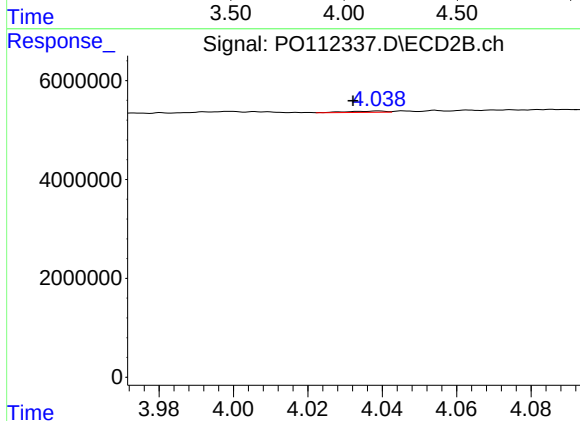


#11 AR-1232-1

R.T.: 4.039 min
Delta R.T.: 0.007 min
Response: 180134
Conc: 1.20 ng/ml

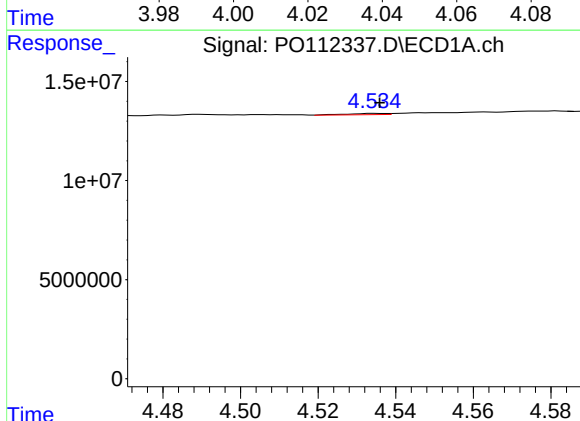


#12 AR-1232-2

R.T.: 4.535 min
Delta R.T.: 0.000 min
Response: 472089
Conc: 4.15 ng/ml

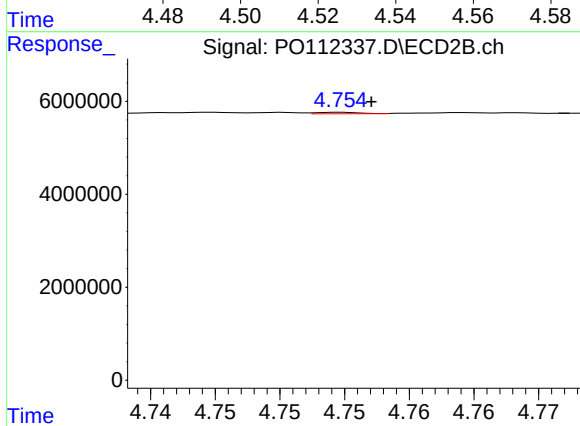

#12 AR-1232-2


R.T.: 4.755 min
Delta R.T.: -0.002 min
Response: 76632
Conc: 0.50 ng/ml

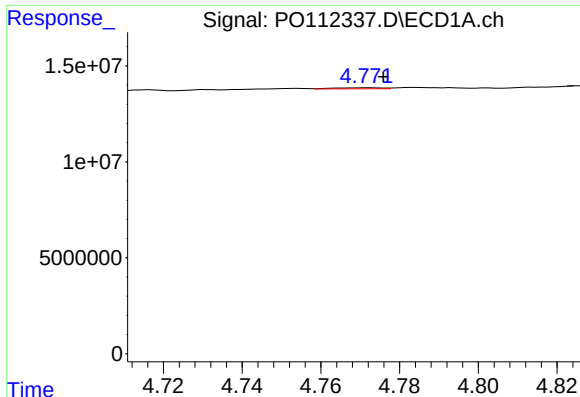

#13 AR-1232-3


R.T.: 4.772 min
Delta R.T.: -0.004 min
Response: 490663
Conc: 2.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

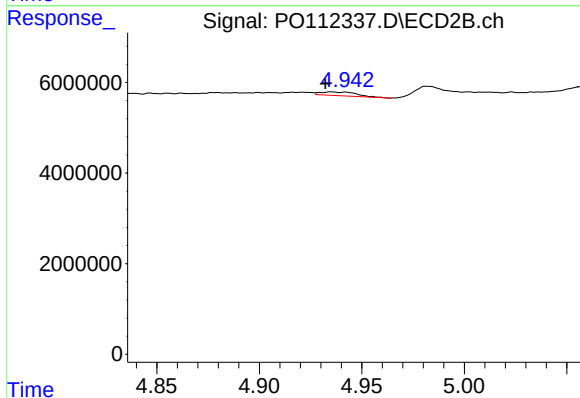


#13 AR-1232-3

R.T.: 4.935 min
Delta R.T.: 0.003 min
Response: 1007265
Conc: 13.34 ng/ml

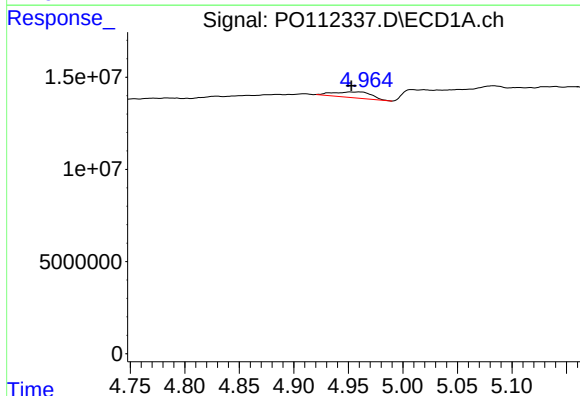


#14 AR-1232-4

R.T.: 4.952 min
Delta R.T.: 0.000 min
Response: 7704496
Conc: 67.41 ng/ml

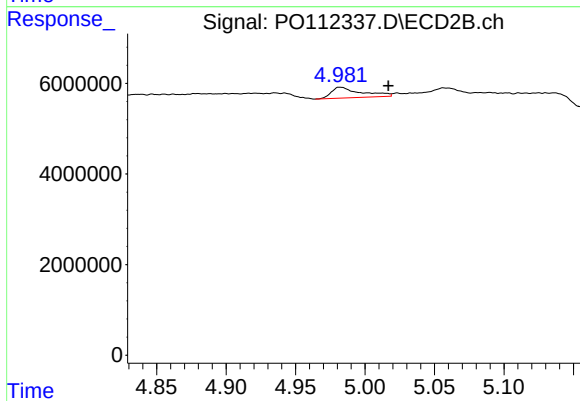

#14 AR-1232-4


R.T.: 4.982 min
Delta R.T.: -0.034 min
Response: 3587326
Conc: 54.36 ng/ml

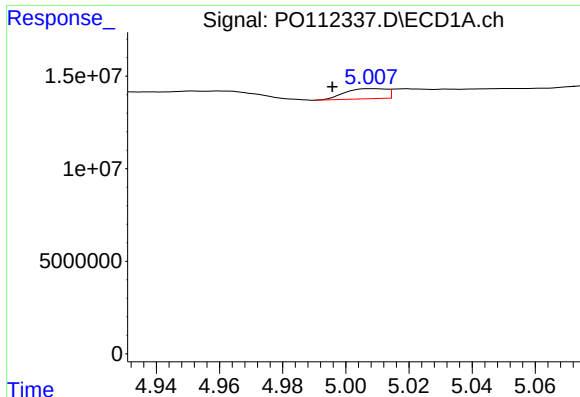

#15 AR-1232-5


R.T.: 5.008 min
Delta R.T.: 0.013 min
Response: 4971544
Conc: 67.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

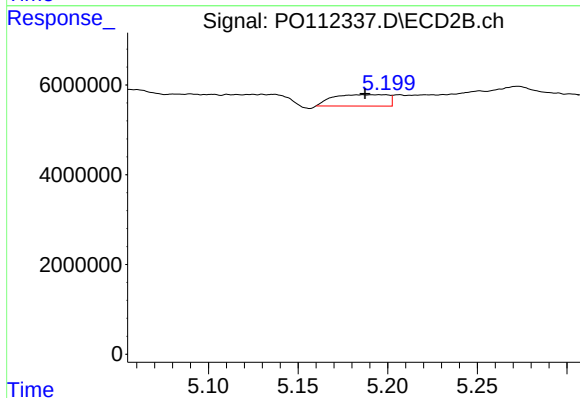


#15 AR-1232-5

R.T.: 5.196 min
Delta R.T.: 0.008 min
Response: 5370574
Conc: 72.32 ng/ml

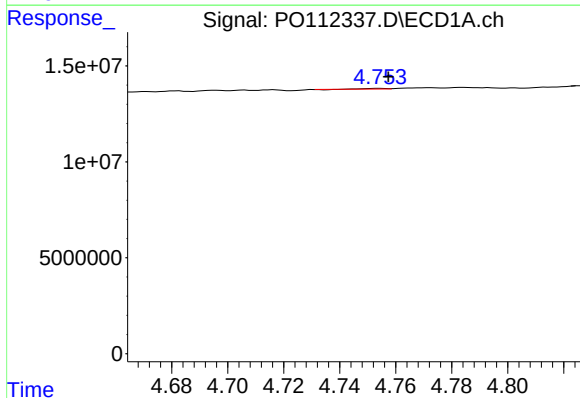


#16 AR-1242-1

R.T.: 4.754 min
Delta R.T.: -0.003 min
Response: 173892
Conc: 0.60 ng/ml

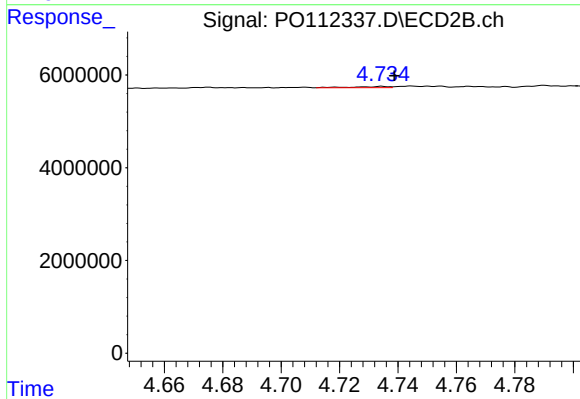

#16 AR-1242-1


R.T.: 4.734 min
Delta R.T.: -0.004 min
Response: 216762
Conc: 1.12 ng/ml

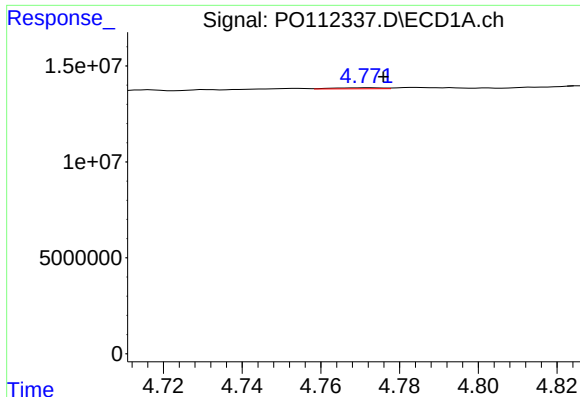

#17 AR-1242-2


R.T.: 4.772 min
Delta R.T.: -0.004 min
Response: 490663
Conc: 1.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

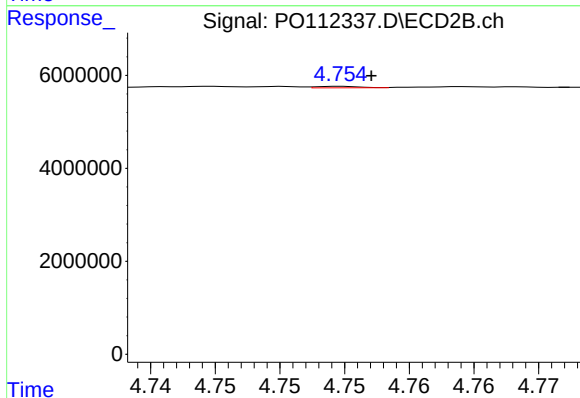


#17 AR-1242-2

R.T.: 4.755 min
Delta R.T.: -0.002 min
Response: 76632
Conc: 0.27 ng/ml

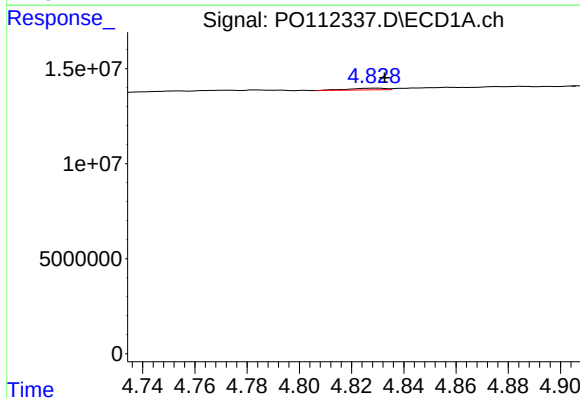


#18 AR-1242-3

R.T.: 4.829 min
Delta R.T.: -0.004 min
Response: 852209
Conc: 3.11 ng/ml

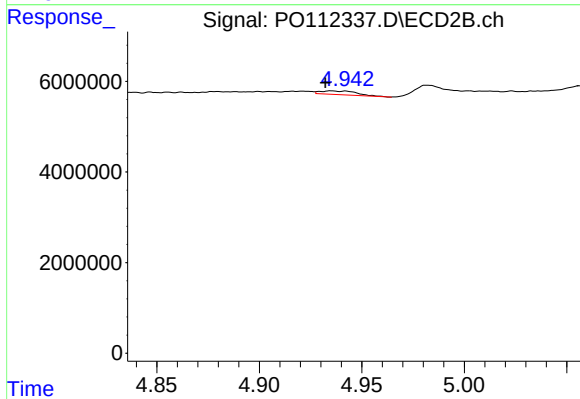

#18 AR-1242-3


R.T.: 4.935 min
Delta R.T.: 0.003 min
Response: 1007265
Conc: 6.91 ng/ml

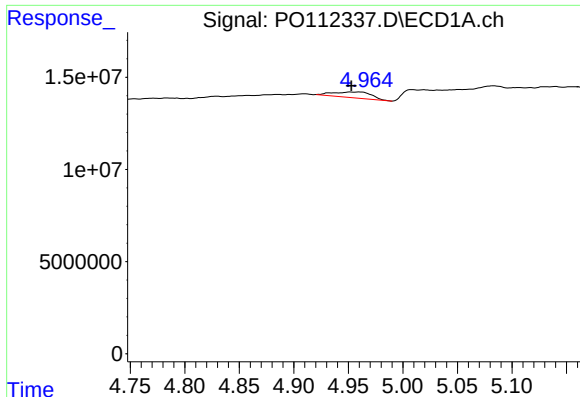

#19 AR-1242-4


R.T.: 4.952 min
Delta R.T.: 0.000 min
Response: 7704496
Conc: 34.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

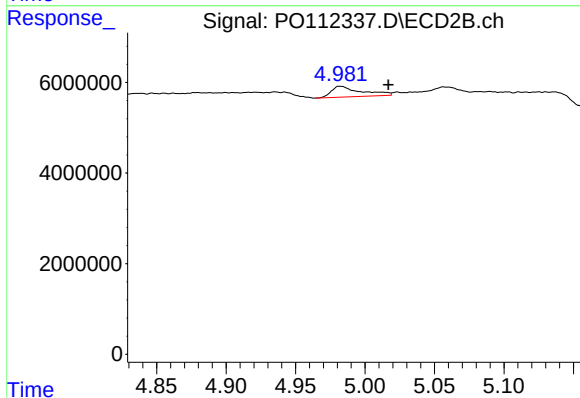


#19 AR-1242-4

R.T.: 4.982 min
Delta R.T.: -0.034 min
Response: 3587326
Conc: 25.29 ng/ml

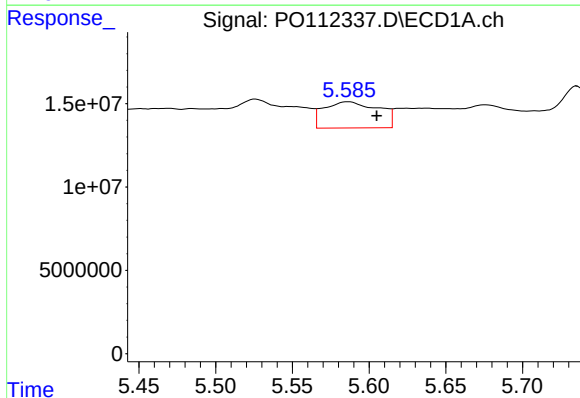


#20 AR-1242-5

R.T.: 5.586 min
Delta R.T.: -0.019 min
Response: 38937051
Conc: 183.95 ng/ml

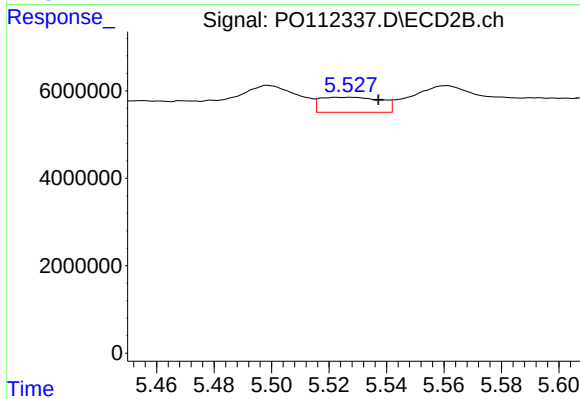

#20 AR-1242-5


R.T.: 5.528 min
Delta R.T.: -0.009 min
Response: 5056942
Conc: 27.83 ng/ml

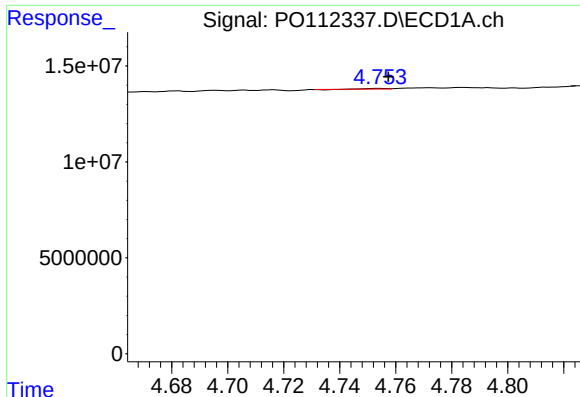

#21 AR-1248-1


R.T.: 4.754 min
Delta R.T.: -0.003 min
Response: 173892
Conc: 0.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

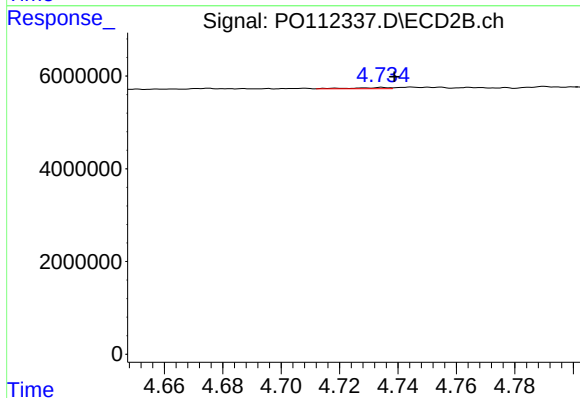


#21 AR-1248-1

R.T.: 4.734 min
Delta R.T.: -0.004 min
Response: 216762
Conc: 1.40 ng/ml

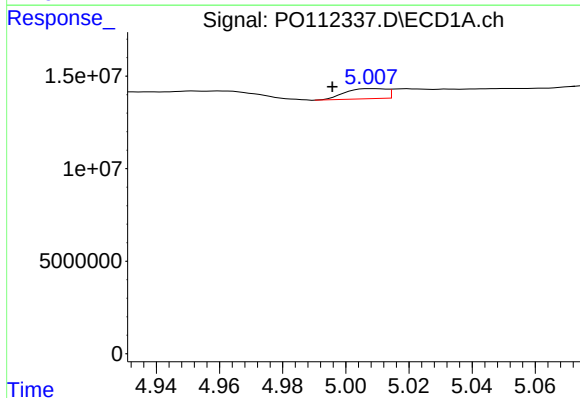


#22 AR-1248-2

R.T.: 5.008 min
Delta R.T.: 0.013 min
Response: 4971544
Conc: 16.12 ng/ml

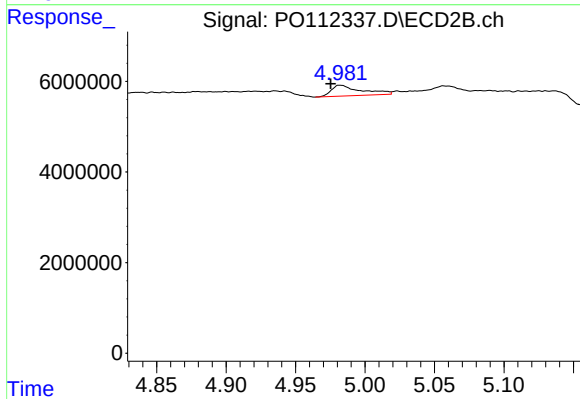

#22 AR-1248-2


R.T.: 4.982 min
Delta R.T.: 0.007 min
Response: 3587326
Conc: 17.43 ng/ml

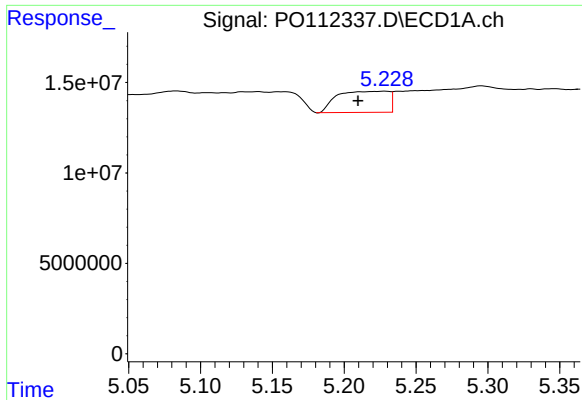

#23 AR-1248-3


R.T.: 5.228 min
Delta R.T.: 0.019 min
Response: 28964951
Conc: 71.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

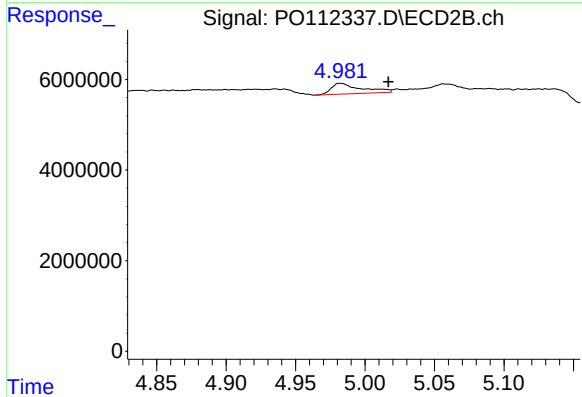


#23 AR-1248-3

R.T.: 4.982 min
Delta R.T.: -0.034 min
Response: 3587326
Conc: 16.70 ng/ml

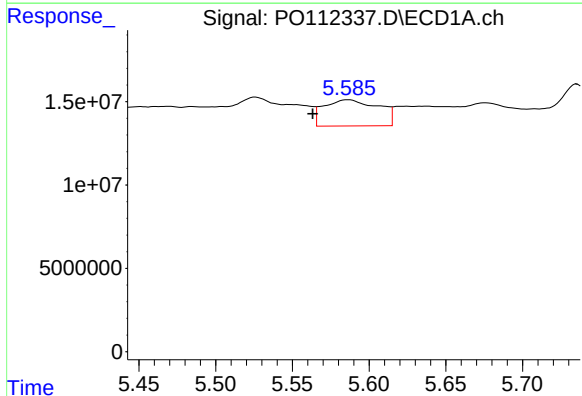


#24 AR-1248-4

R.T.: 5.586 min
Delta R.T.: 0.023 min
Response: 38937051
Conc: 67.46 ng/ml

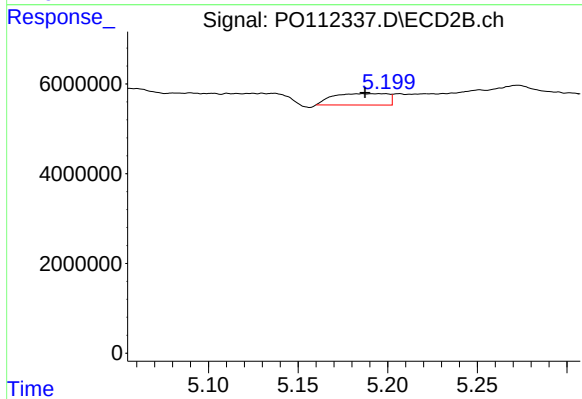

#24 AR-1248-4


R.T.: 5.196 min
Delta R.T.: 0.008 min
Response: 5370574
Conc: 20.76 ng/ml

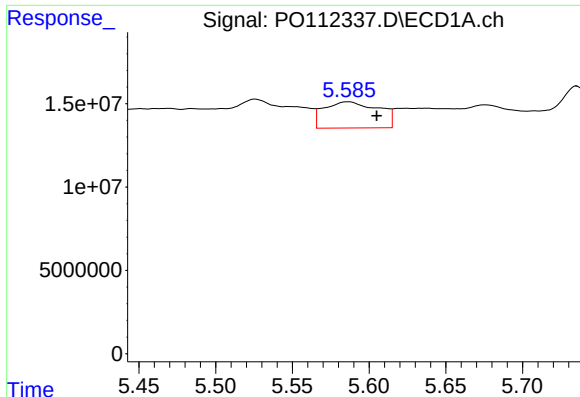

#25 AR-1248-5


R.T.: 5.586 min
Delta R.T.: -0.019 min
Response: 38937051
Conc: 99.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

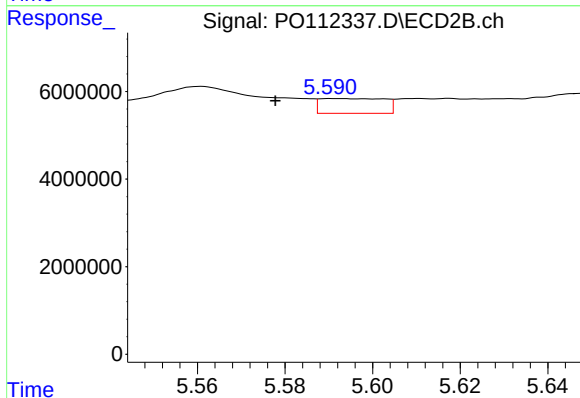


#25 AR-1248-5

R.T.: 5.592 min
Delta R.T.: 0.014 min
Response: 3445220
Conc: 13.75 ng/ml

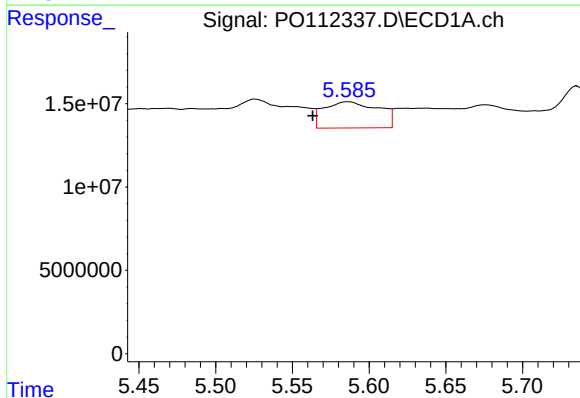


#26 AR-1254-1

R.T.: 5.586 min
Delta R.T.: 0.023 min
Response: 38937051
Conc: 63.30 ng/ml

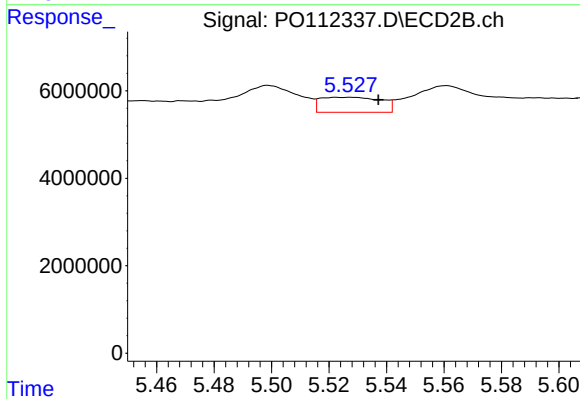

#26 AR-1254-1


R.T.: 5.528 min
Delta R.T.: -0.009 min
Response: 5056942
Conc: 13.27 ng/ml

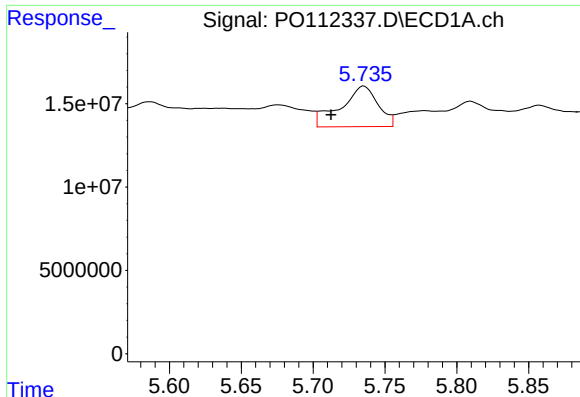

#27 AR-1254-2


R.T.: 5.735 min
Delta R.T.: 0.023 min
Response: 44308870
Conc: 82.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

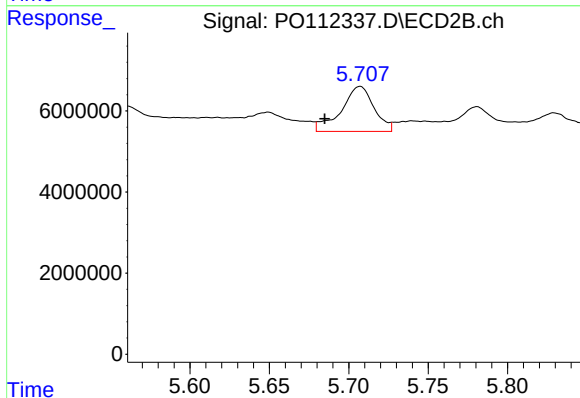


#27 AR-1254-2

R.T.: 5.707 min
Delta R.T.: 0.022 min
Response: 15956035
Conc: 48.09 ng/ml

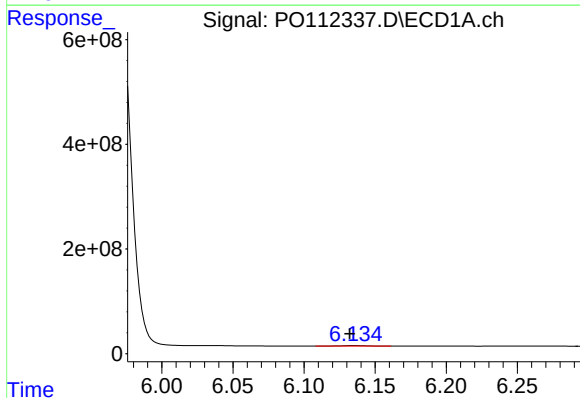


#28 AR-1254-3

R.T.: 6.135 min
Delta R.T.: 0.003 min
Response: 11583843
Conc: 13.80 ng/ml

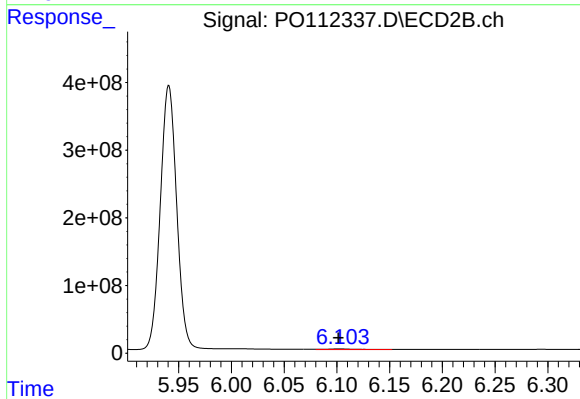

#28 AR-1254-3


R.T.: 6.103 min
Delta R.T.: 0.001 min
Response: 17461996
Conc: 36.22 ng/ml

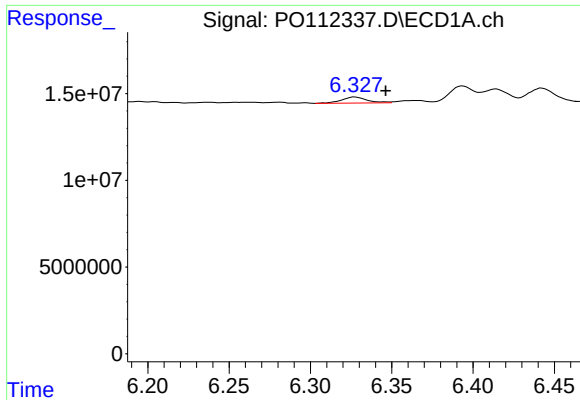

#29 AR-1254-4


R.T.: 6.327 min
Delta R.T.: -0.019 min
Response: 3818976
Conc: 7.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

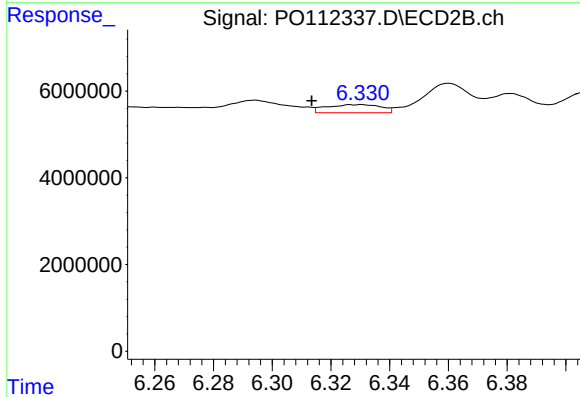


#29 AR-1254-4

R.T.: 6.330 min
Delta R.T.: 0.016 min
Response: 2391280
Conc: 9.17 ng/ml

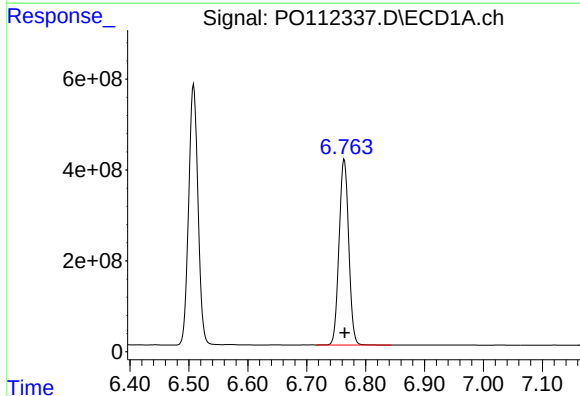


#30 AR-1254-5

R.T.: 6.764 min
Delta R.T.: 0.000 min
Response: 4652565593
Conc: 6011.47 ng/ml

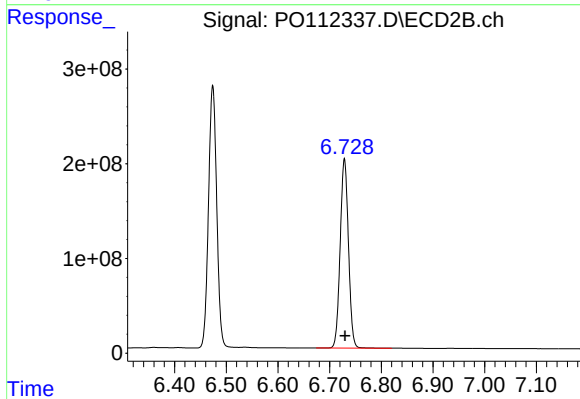

#30 AR-1254-5


R.T.: 6.729 min
Delta R.T.: 0.000 min
Response: 2218813524
Conc: 6226.39 ng/ml

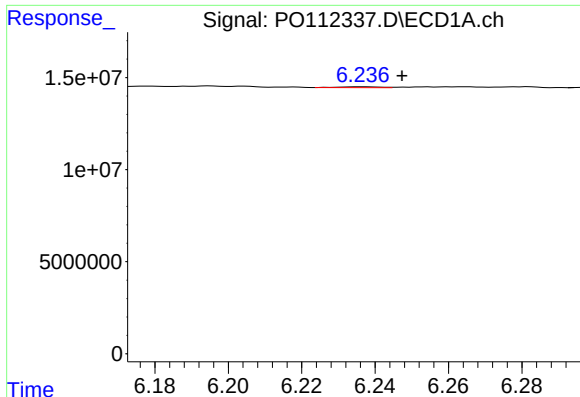

#31 AR-1260-1


R.T.: 6.236 min
Delta R.T.: -0.011 min
Response: 357849
Conc: 0.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

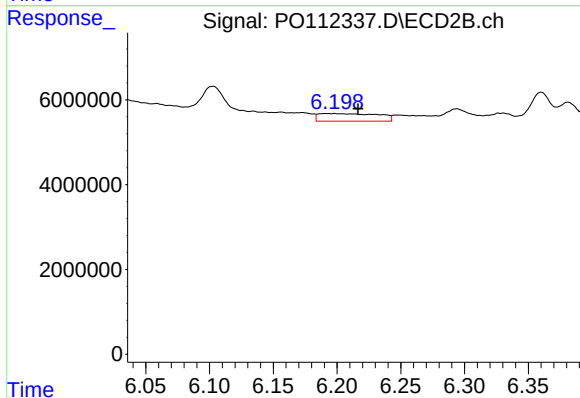


#31 AR-1260-1

R.T.: 6.198 min
Delta R.T.: -0.018 min
Response: 5879942
Conc: 20.96 ng/ml

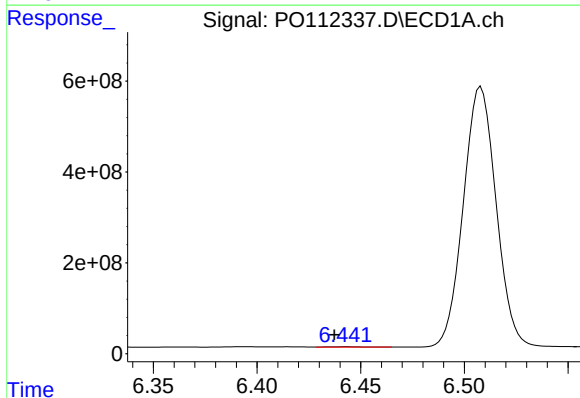


#32 AR-1260-2

R.T.: 6.442 min
Delta R.T.: 0.005 min
Response: 8796070
Conc: 11.92 ng/ml

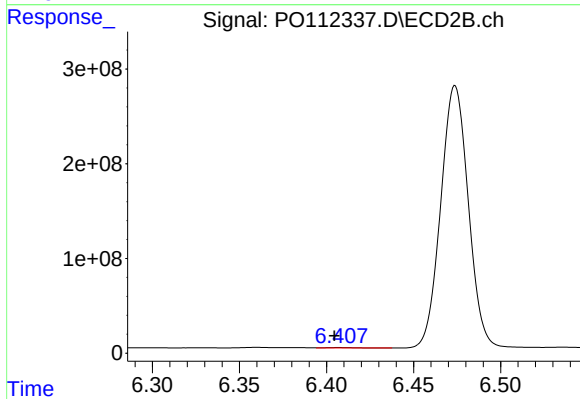

#32 AR-1260-2


R.T.: 6.407 min
Delta R.T.: 0.003 min
Response: 5639735
Conc: 16.59 ng/ml

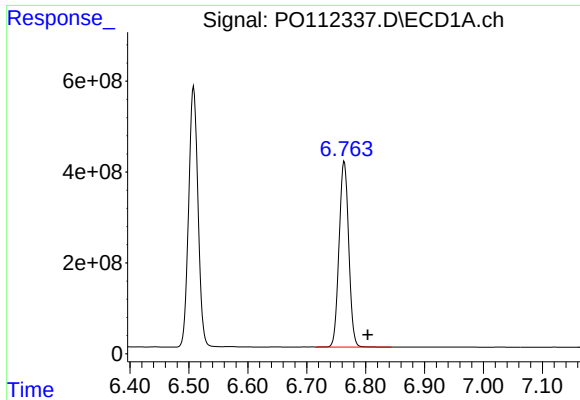

#33 AR-1260-3


R.T.: 6.764 min
Delta R.T.: -0.040 min
Response: 4652565593
Conc: 7097.93 ng/m

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

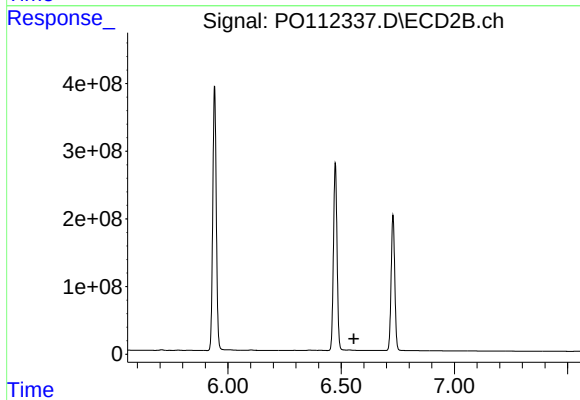


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.556 min
Response: 0
Conc: N.D.

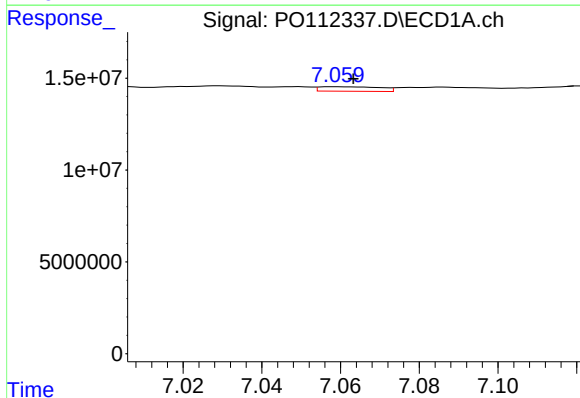


#34 AR-1260-4

R.T.: 7.059 min
Delta R.T.: -0.004 min
Response: 2614469
Conc: 6.01 ng/ml

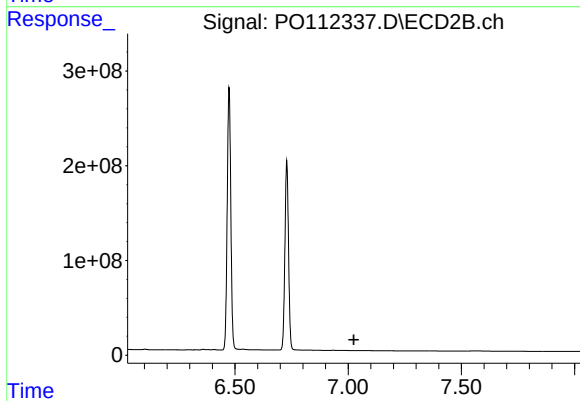

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.026 min
Response: 0
Conc: N.D.

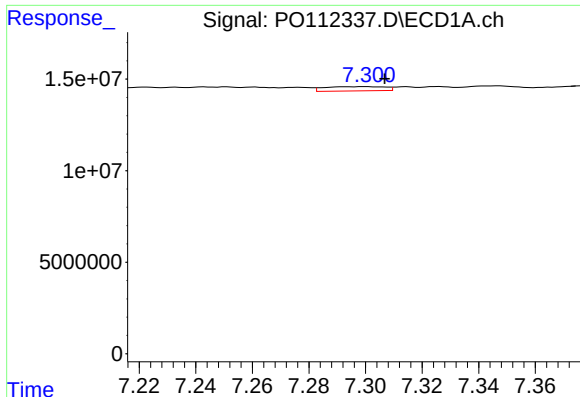

#35 AR-1260-5


R.T.: 7.300 min
Delta R.T.: -0.007 min
Response: 3461684
Conc: 2.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

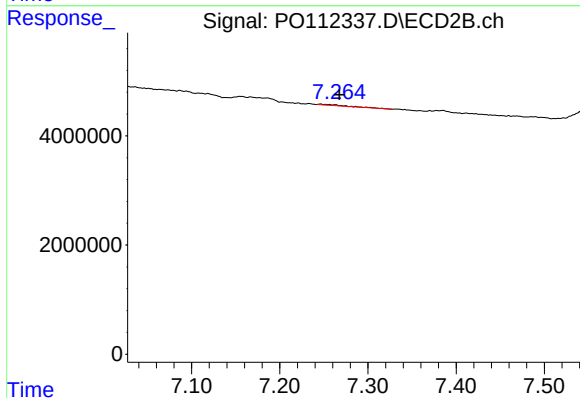


#35 AR-1260-5

R.T.: 7.246 min
Delta R.T.: -0.021 min
Response: 346512
Conc: 0.77 ng/ml

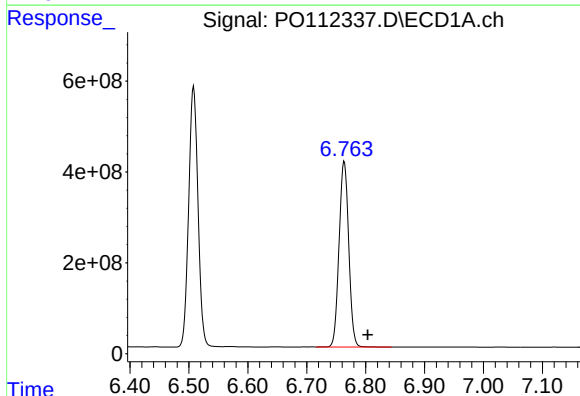


#36 AR-1262-1

R.T.: 6.764 min
Delta R.T.: -0.040 min
Response: 4652565593
Conc: 4553.81 ng/ml

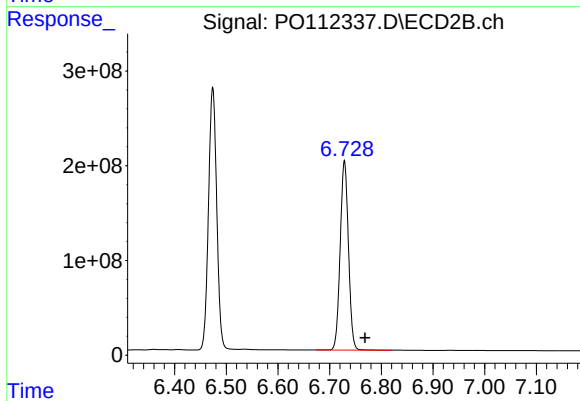

#36 AR-1262-1


R.T.: 6.729 min
Delta R.T.: -0.040 min
Response: 2218813524
Conc: 5447.34 ng/ml

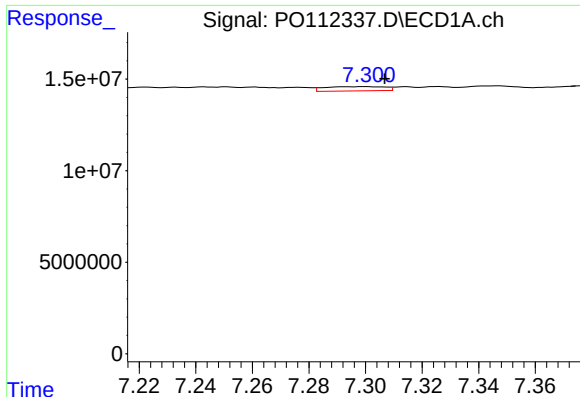

#37 AR-1262-2


R.T.: 7.300 min
Delta R.T.: -0.007 min
Response: 3461684
Conc: 2.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

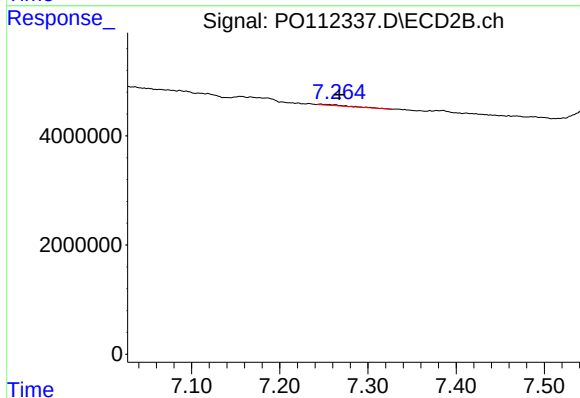


#37 AR-1262-2

R.T.: 7.246 min
Delta R.T.: -0.021 min
Response: 346512
Conc: 0.68 ng/ml

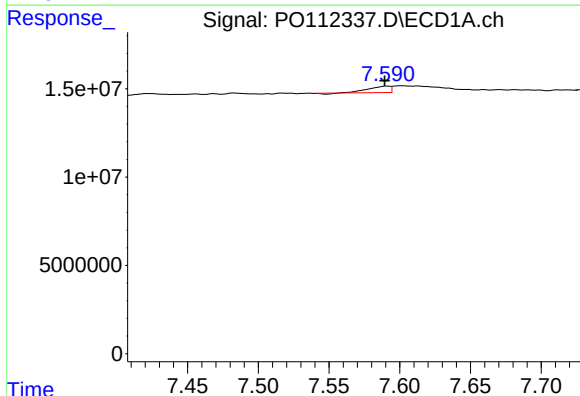


#38 AR-1262-3

R.T.: 7.591 min
Delta R.T.: 0.002 min
Response: 3801135
Conc: 5.92 ng/ml

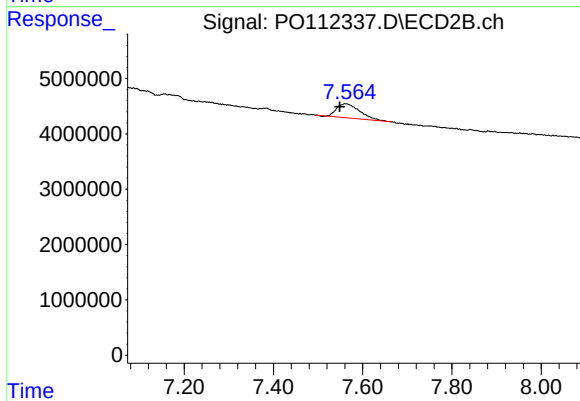

#38 AR-1262-3


R.T.: 7.563 min
Delta R.T.: 0.014 min
Response: 9037742
Conc: 50.34 ng/ml

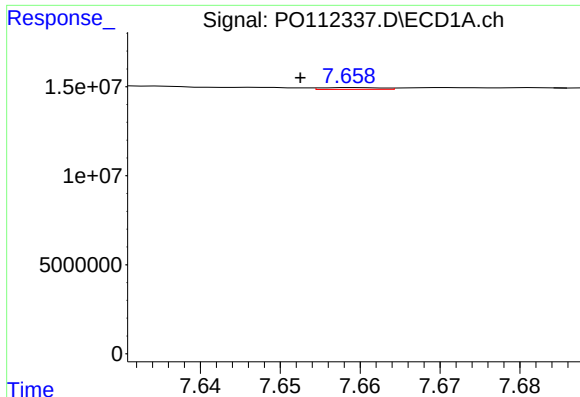

#39 AR-1262-4


R.T.: 7.659 min
Delta R.T.: 0.007 min
Response: 555217
Conc: 0.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

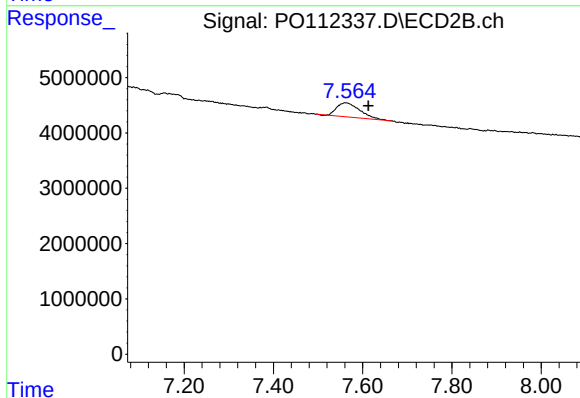


#39 AR-1262-4

R.T.: 7.563 min
Delta R.T.: -0.050 min
Response: 9037742
Conc: 31.07 ng/ml

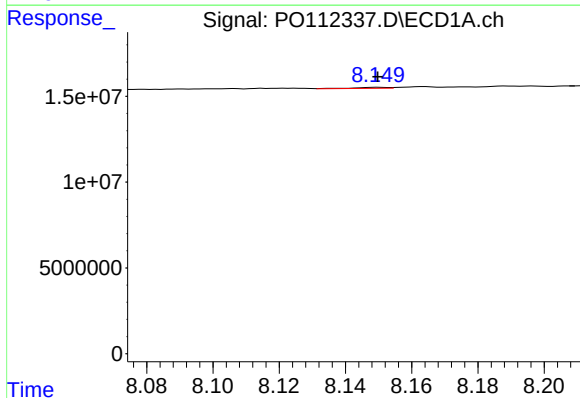


#40 AR-1262-5

R.T.: 8.150 min
Delta R.T.: 0.000 min
Response: 428310
Conc: 0.96 ng/ml

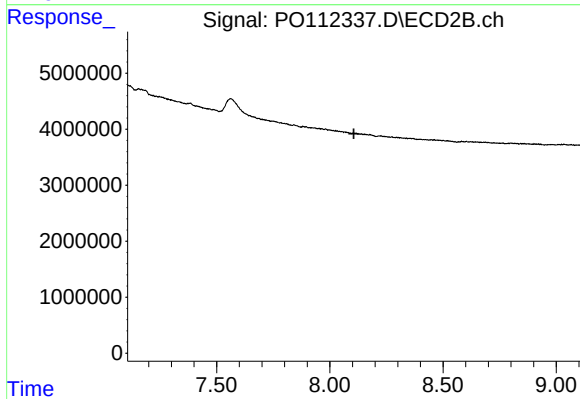

#40 AR-1262-5


R.T.: 8.116 min
Delta R.T.: 0.010 min
Response: -124746
Conc: N.D.

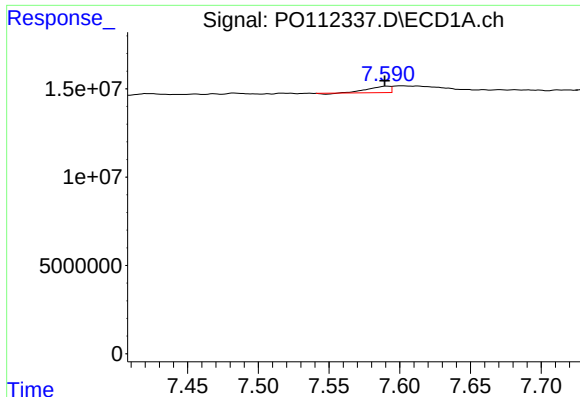

#41 AR-1268-1


R.T.: 7.591 min
Delta R.T.: 0.002 min
Response: 3801135
Conc: 2.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

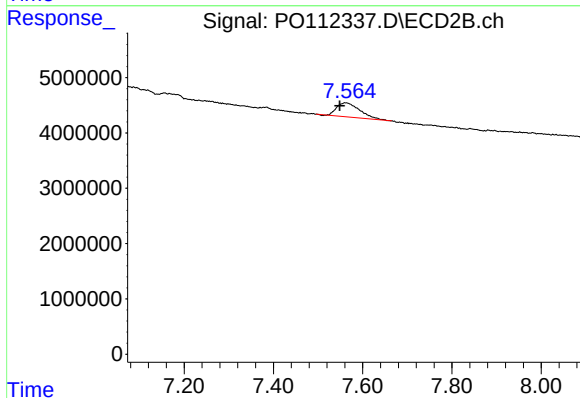


#41 AR-1268-1

R.T.: 7.563 min
Delta R.T.: 0.014 min
Response: 9037742
Conc: 18.39 ng/ml

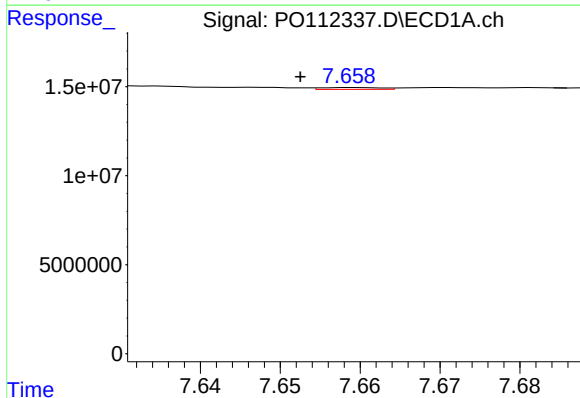


#42 AR-1268-2

R.T.: 7.659 min
Delta R.T.: 0.007 min
Response: 555217
Conc: 0.36 ng/ml

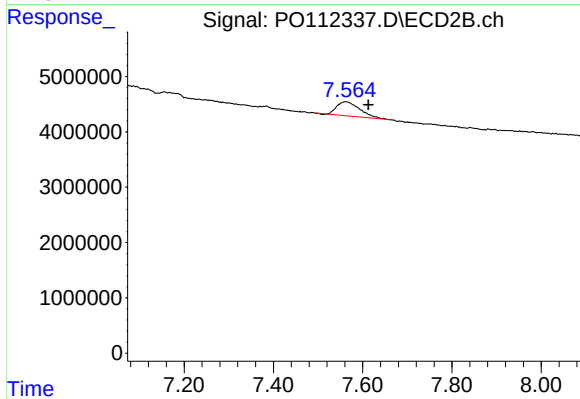

#42 AR-1268-2


R.T.: 7.563 min
Delta R.T.: -0.050 min
Response: 9037742
Conc: 21.66 ng/ml

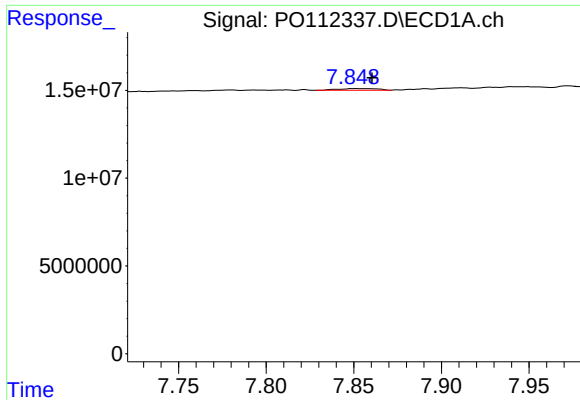

#43 AR-1268-3


R.T.: 7.850 min
Delta R.T.: -0.010 min
Response: 1531906
Conc: 1.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

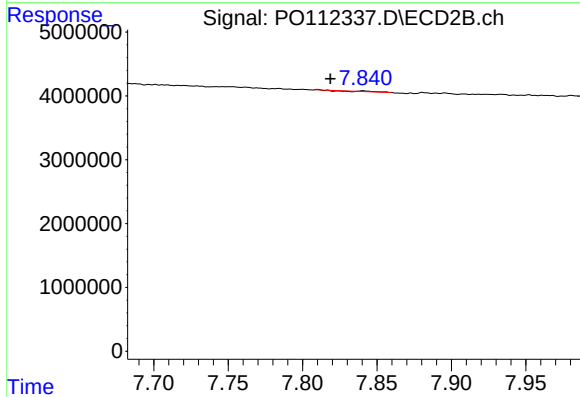


#43 AR-1268-3

R.T.: 7.841 min
Delta R.T.: 0.022 min
Response: 846
Conc: 0.00 ng/ml

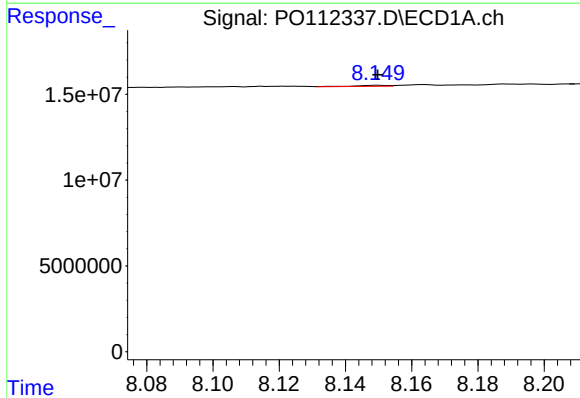


#44 AR-1268-4

R.T.: 8.150 min
Delta R.T.: 0.000 min
Response: 428310
Conc: 0.89 ng/ml

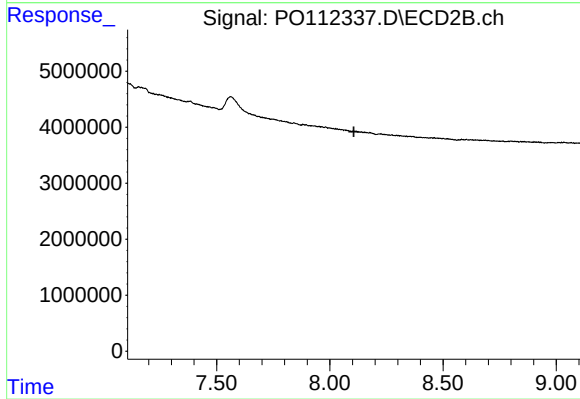

#44 AR-1268-4


R.T.: 8.116 min
Delta R.T.: 0.010 min
Response: -124746
Conc: N.D.

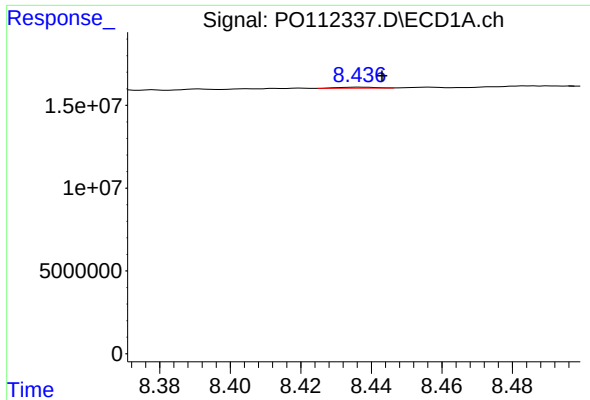

#45 AR-1268-5

R.T.: 8.437 min
Delta R.T.: -0.006 min
Response: 412086
Conc: 0.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

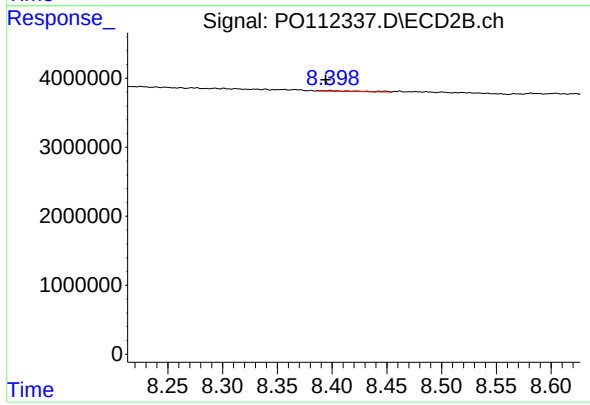

#45 AR-1268-5

R.T.: 8.398 min
Delta R.T.: 0.004 min
Response: 199153
Conc: 0.27 ng/ml