

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072220\
 Data File : P0069866.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jul 2020 10:20
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 22 10:41:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 08 16:12:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.395	3.562	683593	710748	18.309	17.860
2)	SA Decachlor...	10.041	8.765	1299304	1138813	21.595	20.066
Target Compounds							
20)	L4 AR-1242-5	0.000	5.675f	0	46308	N.D.	36.536 #
24)	L5 AR-1248-4	6.606f	0.000	71239	0	35.109	N.D. #
25)	L5 AR-1248-5	0.000	5.675f	0	46308	N.D.	28.062 #
26)	L6 AR-1254-1	6.606	5.675f	71239	46308	35.788	17.790 #
38)	L8 AR-1262-3	8.830f	0.000	46955	0	9.806	N.D. #
39)	L8 AR-1262-4	8.889	0.000	44614	0	23.016	N.D. #
41)	L9 AR-1268-1	8.830f	0.000	46955	0	5.123	N.D. #
42)	L9 AR-1268-2	8.889	0.000	44614	0	5.383	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072220\
Data File : P0069866.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jul 2020 10:20
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 22 10:41:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 08 16:12:41 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

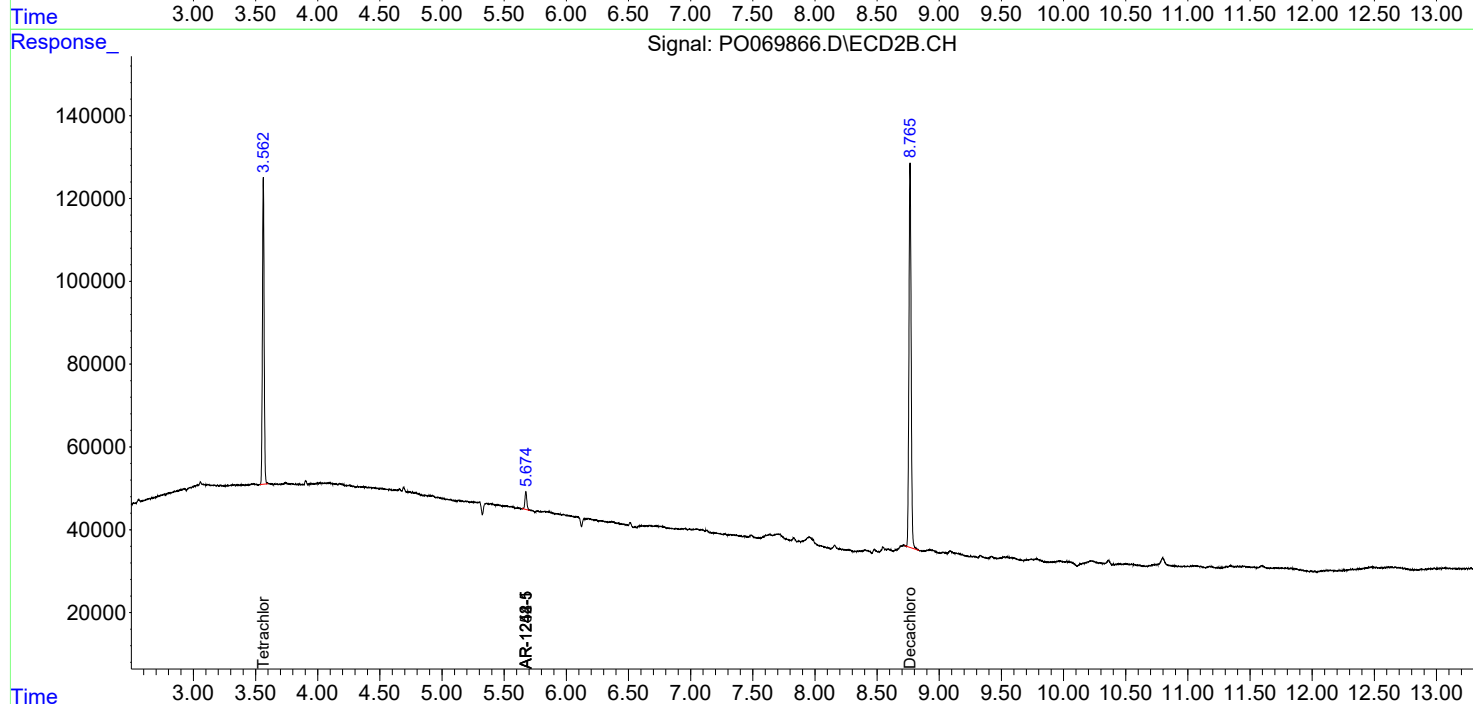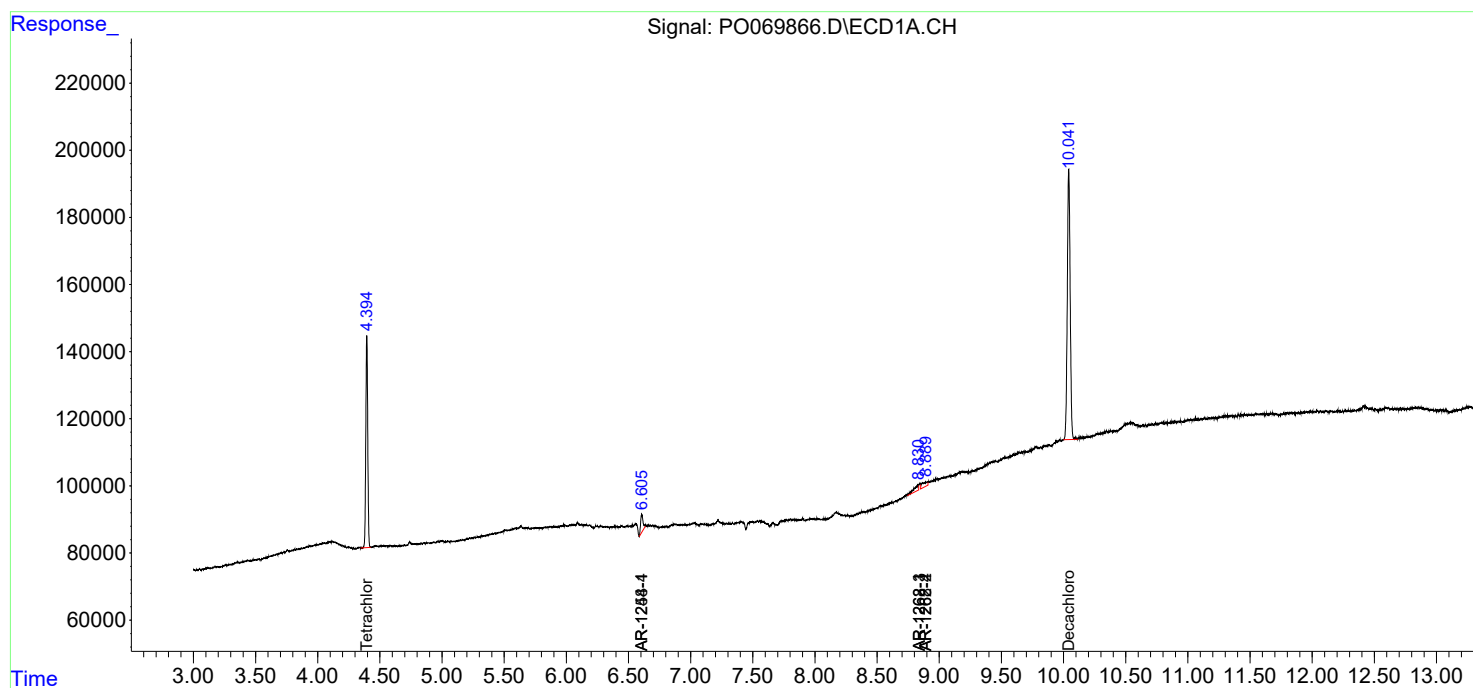


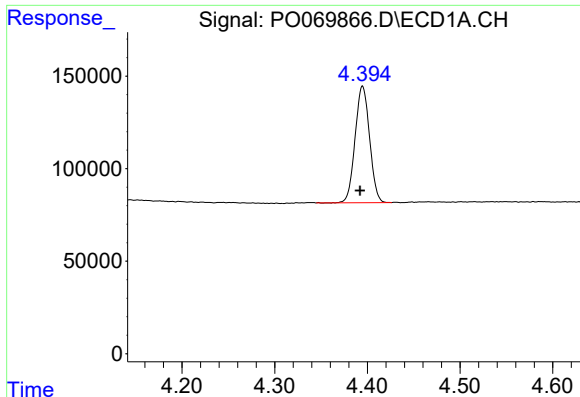

#1 Tetrachloro-m-xylene


R.T.: 4.395 min
Delta R.T.: 0.003 min
Response: 683593
Conc: 18.31 ng/ml

Instrument :
ECD_O
ClientSampleId :

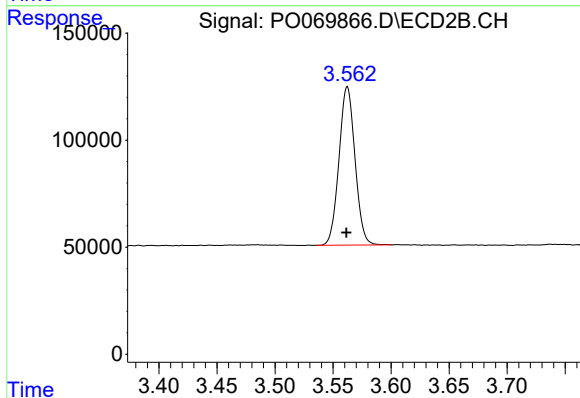


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: 0.000 min
Response: 710748
Conc: 17.86 ng/ml

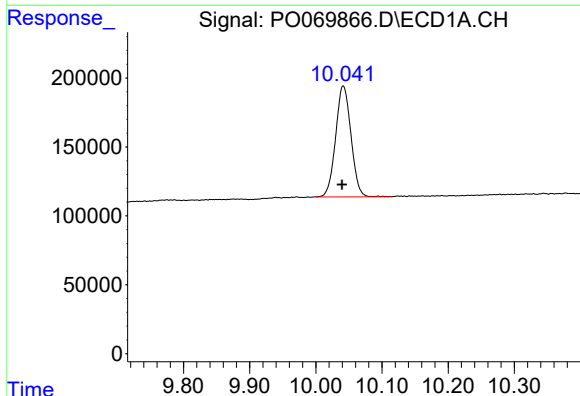


#2 Decachlorobiphenyl

R.T.: 10.041 min
Delta R.T.: 0.001 min
Response: 1299304
Conc: 21.60 ng/ml

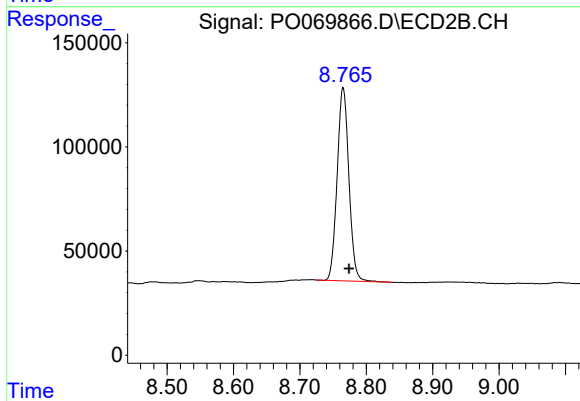

#2 Decachlorobiphenyl


R.T.: 8.765 min
Delta R.T.: -0.009 min
Response: 1138813
Conc: 20.07 ng/ml

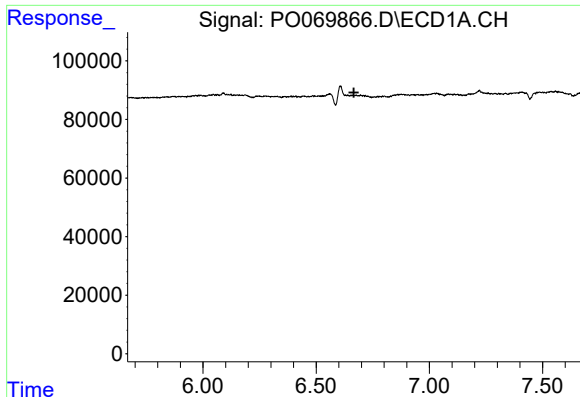

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.667 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

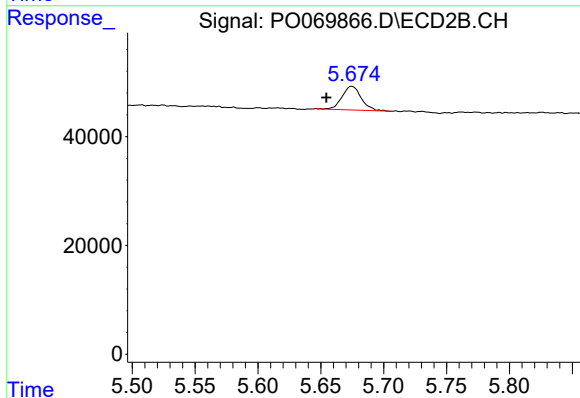


#20 AR-1242-5

R.T.: 5.675 min
Delta R.T.: 0.020 min
Response: 46308
Conc: 36.54 ng/ml

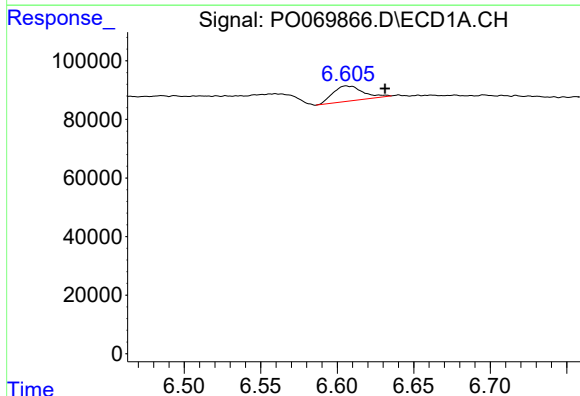


#24 AR-1248-4

R.T.: 6.606 min
Delta R.T.: -0.025 min
Response: 71239
Conc: 35.11 ng/ml

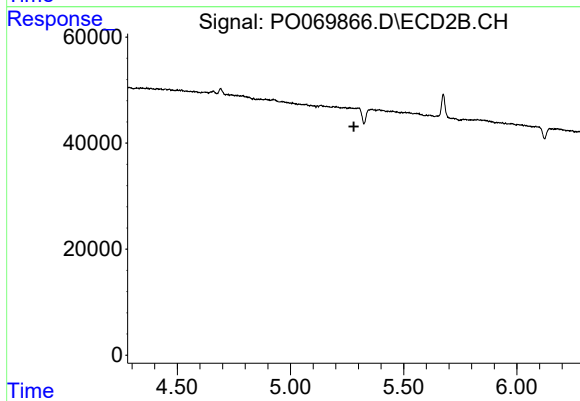

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.280 min
Response: 0
Conc: N.D.

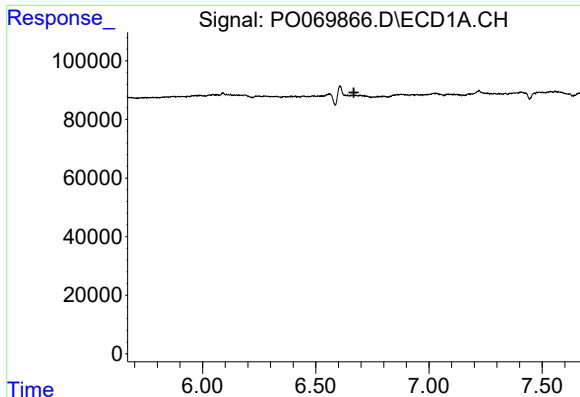

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.668 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

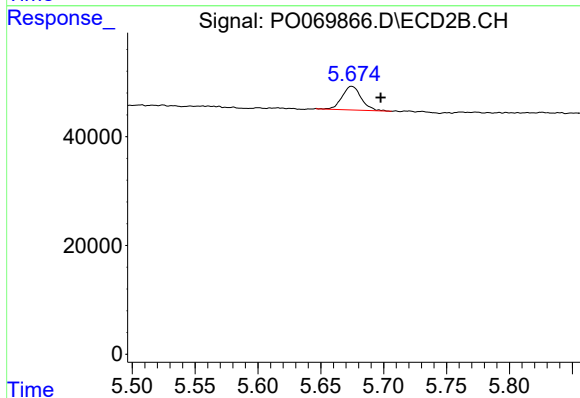


#25 AR-1248-5

R.T.: 5.675 min
Delta R.T.: -0.023 min
Response: 46308
Conc: 28.06 ng/ml

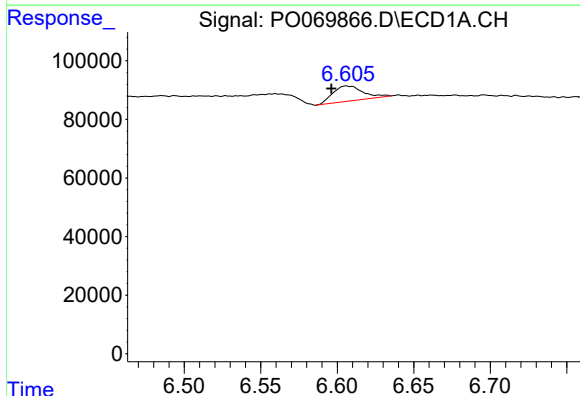


#26 AR-1254-1

R.T.: 6.606 min
Delta R.T.: 0.010 min
Response: 71239
Conc: 35.79 ng/ml

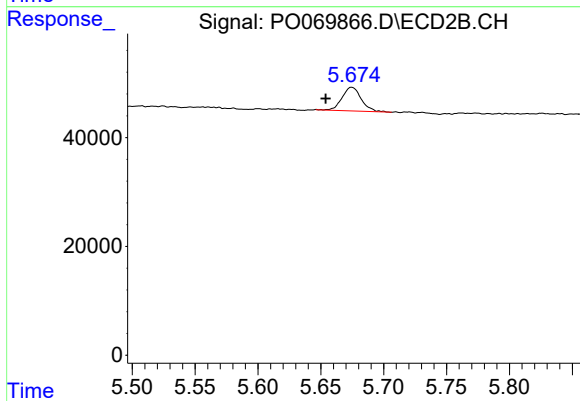

#26 AR-1254-1


R.T.: 5.675 min
Delta R.T.: 0.021 min
Response: 46308
Conc: 17.79 ng/ml

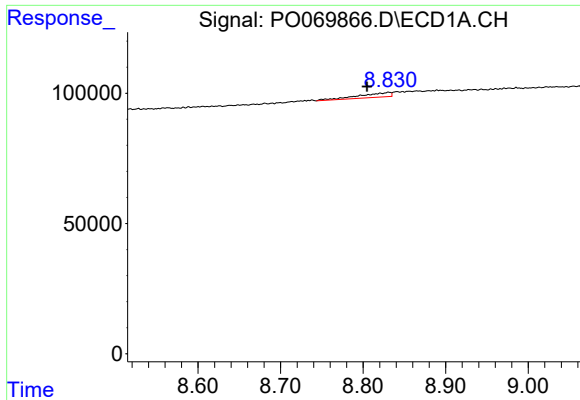

#38 AR-1262-3


R.T.: 8.830 min
Delta R.T.: 0.026 min
Response: 46955
Conc: 9.81 ng/ml

Instrument :
ECD_O
ClientSampleId :

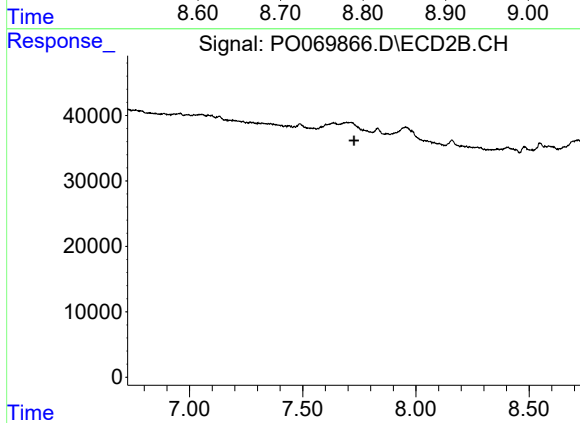


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 7.726 min
Response: 0
Conc: N.D.

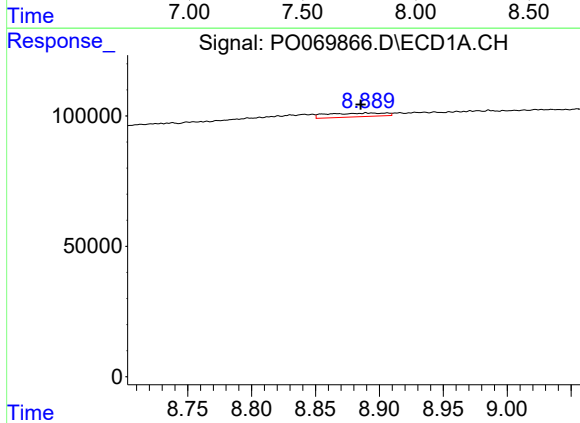


#39 AR-1262-4

R.T.: 8.889 min
Delta R.T.: 0.004 min
Response: 44614
Conc: 23.02 ng/ml

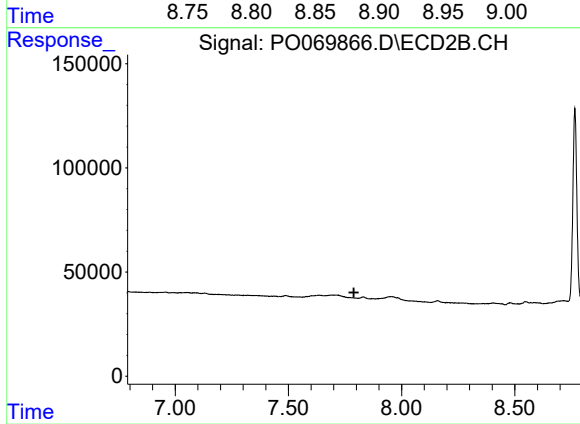

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 7.789 min
Response: 0
Conc: N.D.

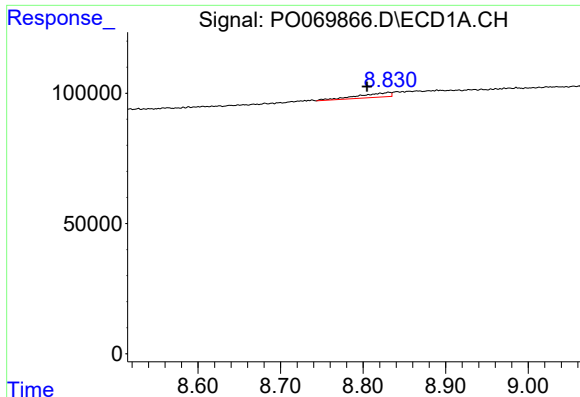

#41 AR-1268-1


R.T.: 8.830 min
Delta R.T.: 0.026 min
Response: 46955
Conc: 5.12 ng/ml

Instrument :
ECD_O
ClientSampleId :

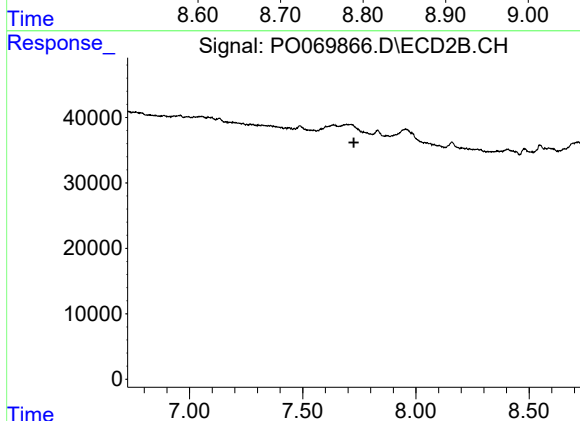


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 7.726 min
Response: 0
Conc: N.D.

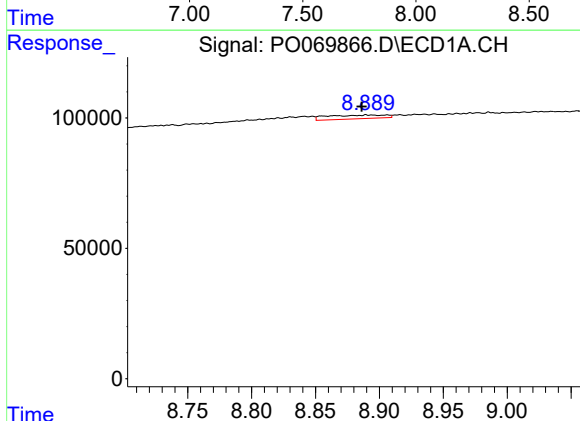

#42 AR-1268-2

R.T.: 8.889 min
Delta R.T.: 0.003 min
Response: 44614
Conc: 5.38 ng/ml

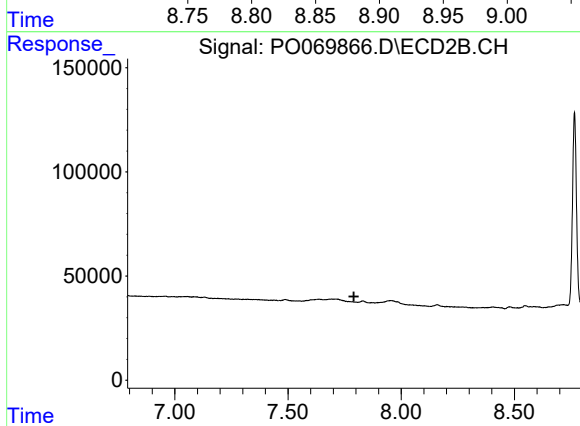

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 7.791 min
Response: 0
Conc: N.D.