

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072225\
 Data File : P0112371.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2025 10:26
 Operator : YP/AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 01:47:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 22 09:14:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.656	3.683	110226	66514	0.011	0.010
2)	SA Decachlor...	8.702	8.670	52160	36170	0.008	0.021 #
Target Compounds							
3)	L1 AR-1016-1	4.762	4.766	536175	52679	1.576	0.236 #
4)	L1 AR-1016-2	4.770	4.771	745374	43402	1.499	0.132 #
5)	L1 AR-1016-3	4.823	4.936	2998056	1693050	9.261	9.967
6)	L1 AR-1016-4	4.961	5.004	8747221	896489	34.062	6.533 #
7)	L1 AR-1016-5	5.222	5.205	47967182	1519698	175.279	8.812 #
8)	L2 AR-1221-1	3.845f	3.867	183522	120108	1.574	1.459
9)	L2 AR-1221-2	3.954	3.957	135925	359262	1.724	6.053 #
10)	L2 AR-1221-3	4.004f	4.032	838765	252503	3.111	1.338 #
11)	L3 AR-1232-1	4.004f	4.032	838765	252503	3.907	1.682 #
12)	L3 AR-1232-2	4.537	4.749	842043	174092	7.410	1.137 #
13)	L3 AR-1232-3	4.770	4.936	745374	1693050	3.255	22.423 #
14)	L3 AR-1232-4	4.961	5.020	8747221	1243543	76.531	18.845 #
15)	L3 AR-1232-5	5.013	5.195	10502076	4134628	143.080	55.678 #
16)	L4 AR-1242-1	4.762	4.737	536175	311337	1.851	1.606
17)	L4 AR-1242-2	4.770	4.749	745374	174092	1.750	0.614 #
18)	L4 AR-1242-3	4.823	4.936	2998056	1693050	10.954	11.622
19)	L4 AR-1242-4	4.961	5.020	8747221	1243543	38.822	8.767 #
20)	L4 AR-1242-5	5.584	5.524	60955878	5952436	287.975	32.754 #
21)	L5 AR-1248-1	4.762	4.737	536175	311337	2.363	2.017
22)	L5 AR-1248-2	5.013	4.982	10502076	3883568	34.062	18.874 #
23)	L5 AR-1248-3	5.222	5.020	47967182	1243543	117.763	5.789 #
24)	L5 AR-1248-4	5.550	5.195	20546571	4134628	35.600	15.981 #
25)	L5 AR-1248-5	5.584	5.559	60955878	17044693	156.175	68.029 #
26)	L6 AR-1254-1	5.550	5.524	20546571	5952436	33.403	15.616 #
27)	L6 AR-1254-2	5.733	5.678	51911881	2338823	96.907	7.049 #
28)	L6 AR-1254-3	6.132	6.101	12157102	20987916	14.480	43.540 #
29)	L6 AR-1254-4	6.367	6.328	1178740	1235750	2.451	4.740 #
30)	L6 AR-1254-5	6.761	6.726	4557.0E6	2264.0E6	5887.975	6353.066
31)	L7 AR-1260-1	6.246	6.243	3041322	1295180	6.068	4.616
32)	L7 AR-1260-2	6.439	6.405	11095202	5702796	15.031	16.773
33)	L7 AR-1260-3	6.832	6.584	4722163	-220948	7.204	N.D. #
34)	L7 AR-1260-4	7.062	7.046	2828500	603843	6.499	3.010 #
35)	L7 AR-1260-5	7.296	7.287	9152317	104033	7.249	0.232 #
36)	L8 AR-1262-1	6.832	6.726f	4722163	2264.0E6	4.622	5558.160 #
37)	L8 AR-1262-2	7.296	7.270	9152317	163308	5.583	0.319 #
38)	L8 AR-1262-3	7.591	7.560	10873815	20023808	16.938	111.538 #
39)	L8 AR-1262-4	7.662	7.633	1546265	403392	1.443	1.387
40)	L8 AR-1262-5	8.150	8.108	888281	29872	1.982	0.282 #
41)	L9 AR-1268-1	7.591	7.560	10873815	20023808	5.918	40.744 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072225\
Data File : P0112371.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jul 2025 10:26
Operator : YP/AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 01:47:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 22 09:14:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	7.662	7.633	1546265	403392	0.993	0.967
43)	L9 AR-1268-3	7.846	7.796	5844338	221096	4.497	0.699 #
44)	L9 AR-1268-4	8.150	8.108	888281	29872	1.849	0.268 #
45)	L9 AR-1268-5	8.431	8.392	251729	35543	0.077	0.049 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO072225\
Data File : PO112371.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jul 2025 10:26
Operator : YP/AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 01:47:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 22 09:14:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

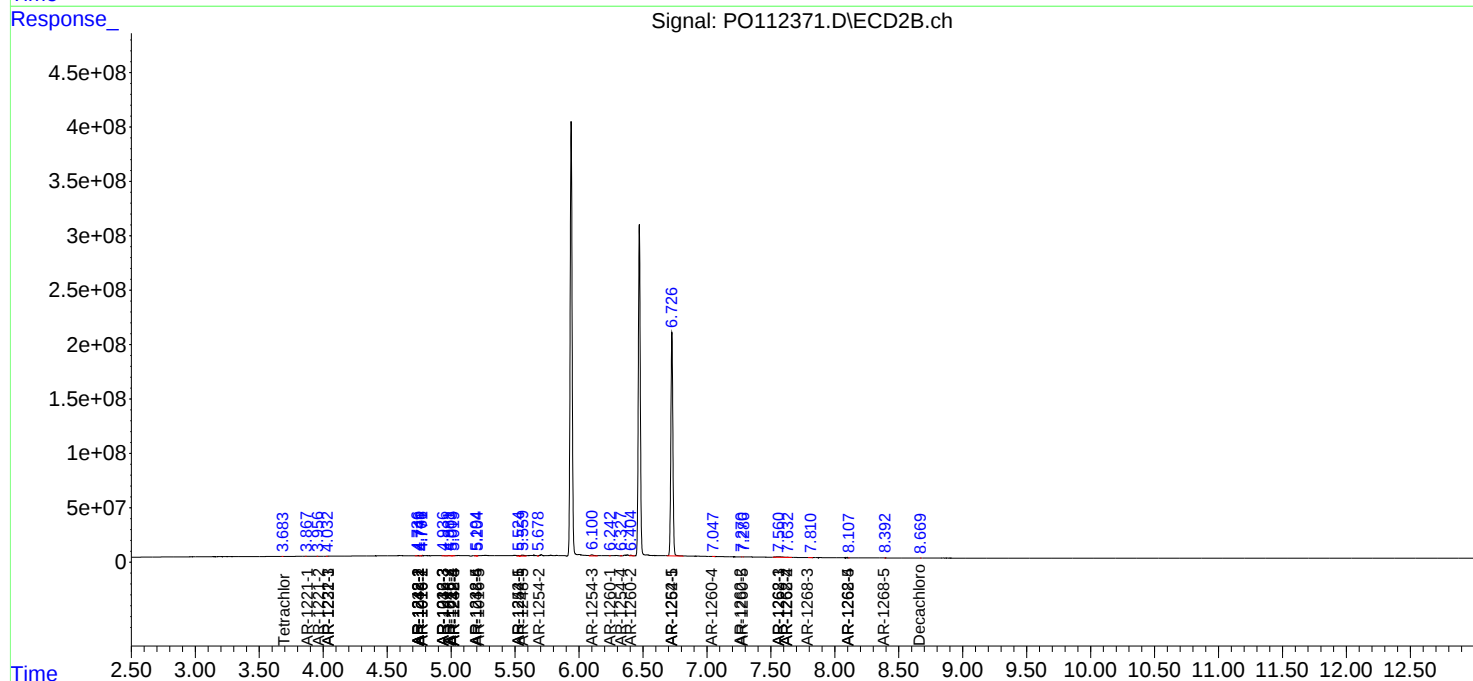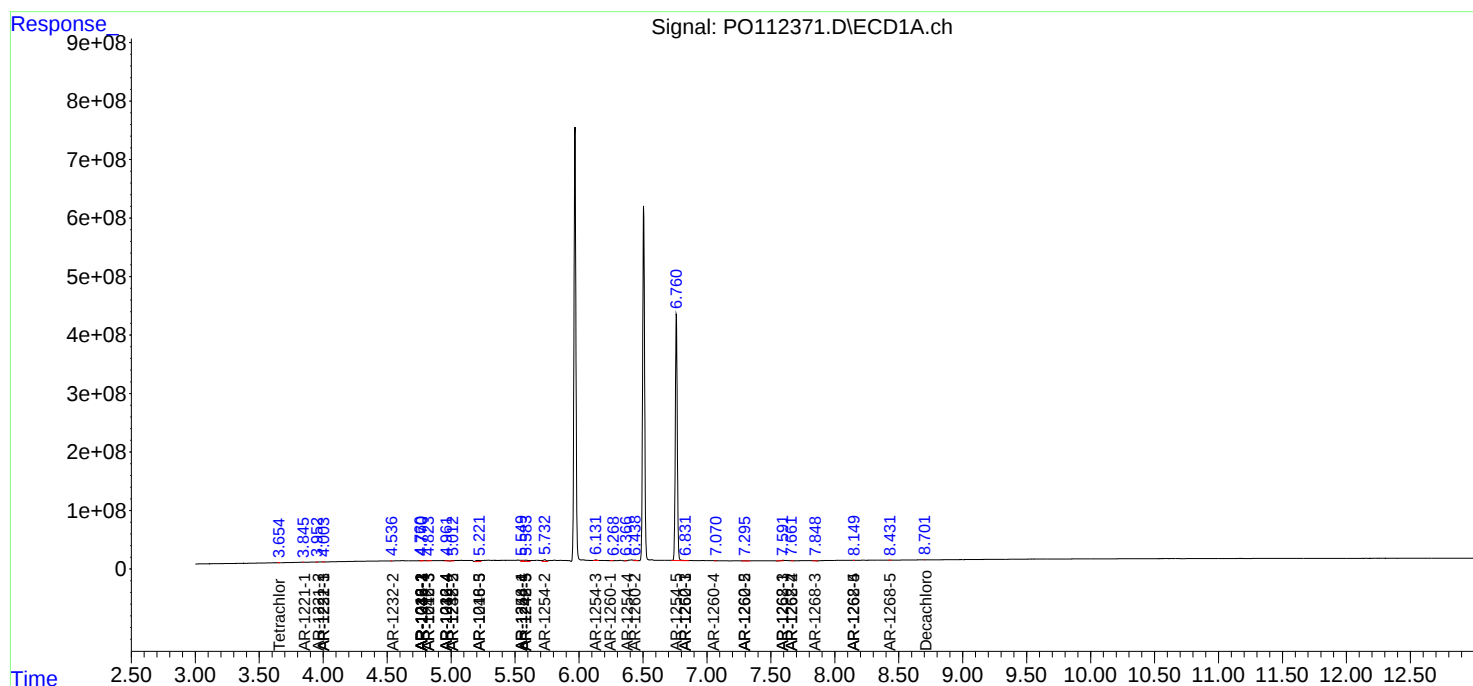


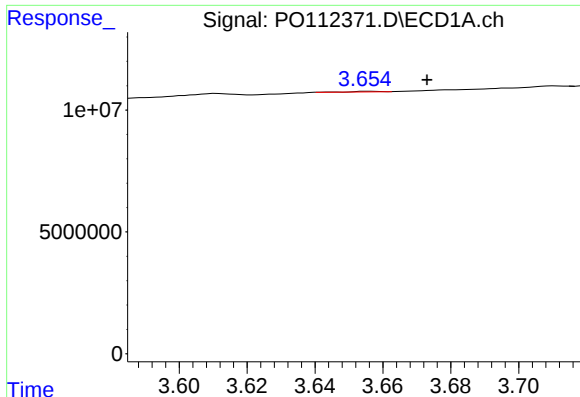

#1 Tetrachloro-m-xylene


R.T.: 3.656 min
Delta R.T.: -0.017 min
Response: 110226
Conc: 0.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

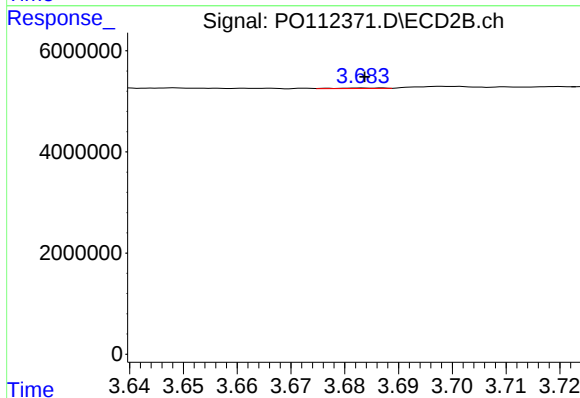


#1 Tetrachloro-m-xylene

R.T.: 3.683 min
Delta R.T.: 0.000 min
Response: 66514
Conc: 0.01 ng/ml

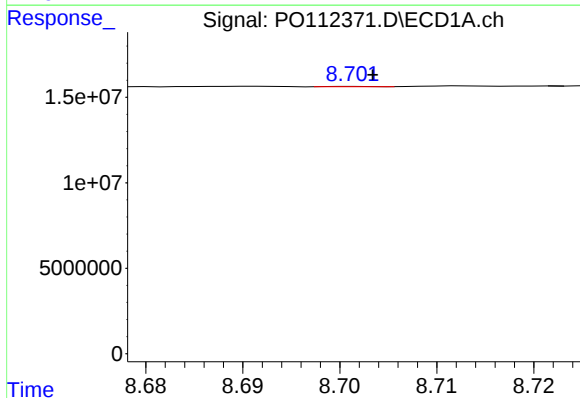


#2 Decachlorobiphenyl

R.T.: 8.702 min
Delta R.T.: -0.002 min
Response: 52160
Conc: 0.01 ng/ml

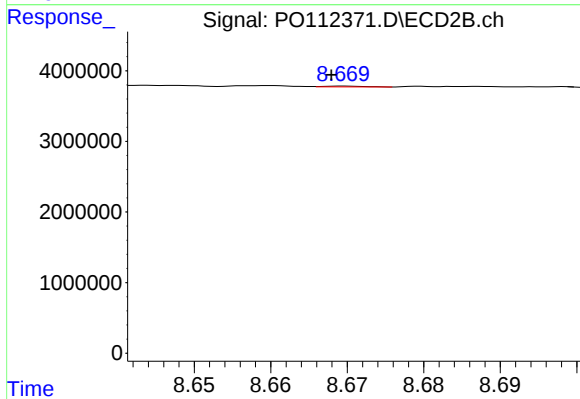

#2 Decachlorobiphenyl


R.T.: 8.670 min
Delta R.T.: 0.002 min
Response: 36170
Conc: 0.02 ng/ml

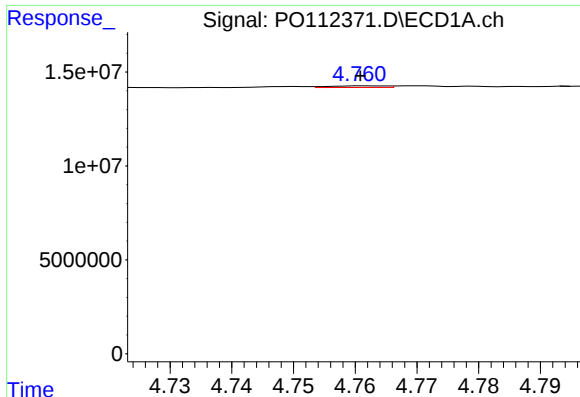

#3 AR-1016-1


R.T.: 4.762 min
Delta R.T.: 0.000 min
Response: 536175
Conc: 1.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

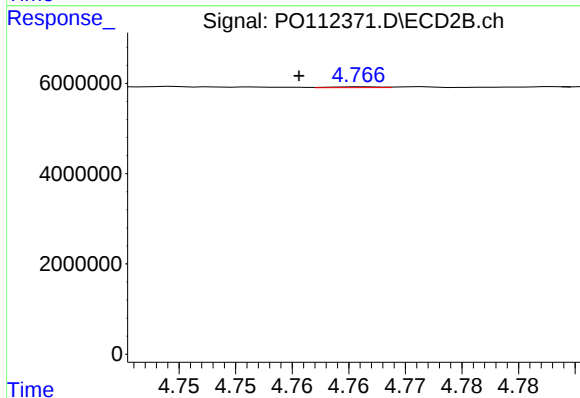


#3 AR-1016-1

R.T.: 4.766 min
Delta R.T.: 0.006 min
Response: 52679
Conc: 0.24 ng/ml

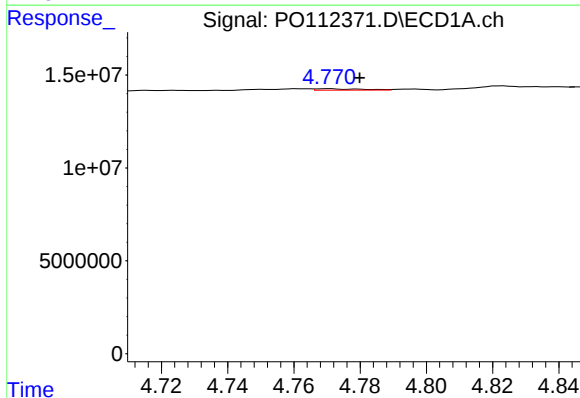


#4 AR-1016-2

R.T.: 4.770 min
Delta R.T.: -0.010 min
Response: 745374
Conc: 1.50 ng/ml

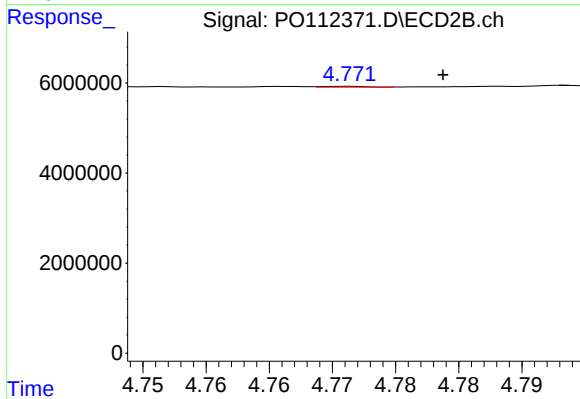

#4 AR-1016-2


R.T.: 4.771 min
Delta R.T.: -0.007 min
Response: 43402
Conc: 0.13 ng/ml

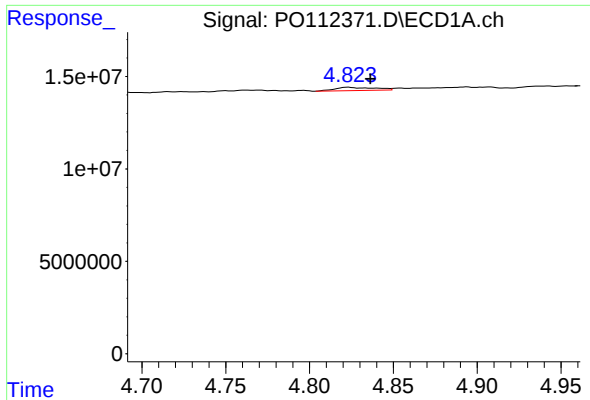

#5 AR-1016-3


R.T.: 4.823 min
Delta R.T.: -0.014 min
Response: 2998056
Conc: 9.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

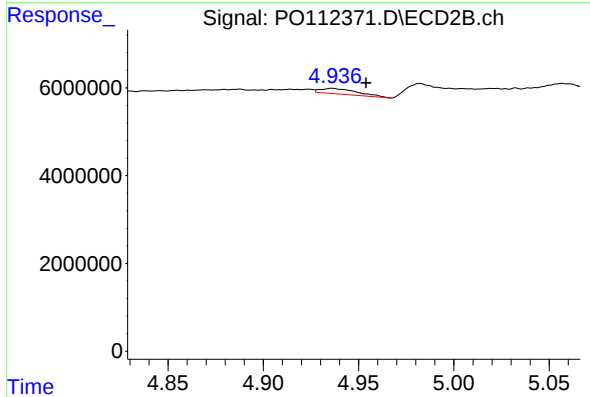


#5 AR-1016-3

R.T.: 4.936 min
Delta R.T.: -0.018 min
Response: 1693050
Conc: 9.97 ng/ml

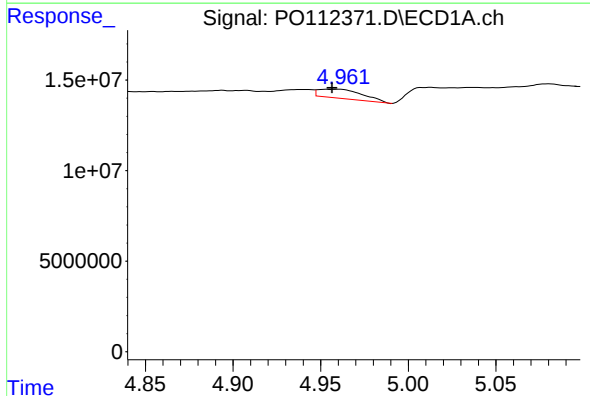


#6 AR-1016-4

R.T.: 4.961 min
Delta R.T.: 0.004 min
Response: 8747221
Conc: 34.06 ng/ml

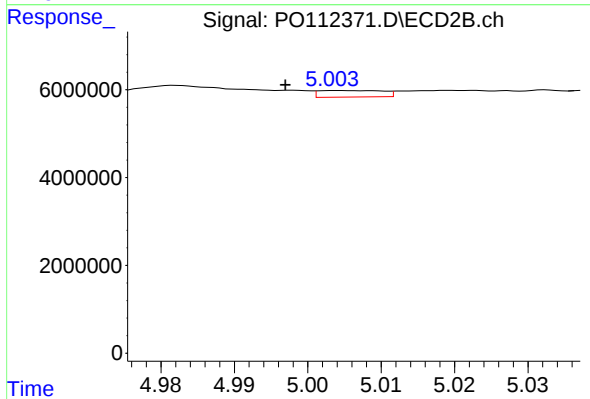

#6 AR-1016-4


R.T.: 5.004 min
Delta R.T.: 0.007 min
Response: 896489
Conc: 6.53 ng/ml

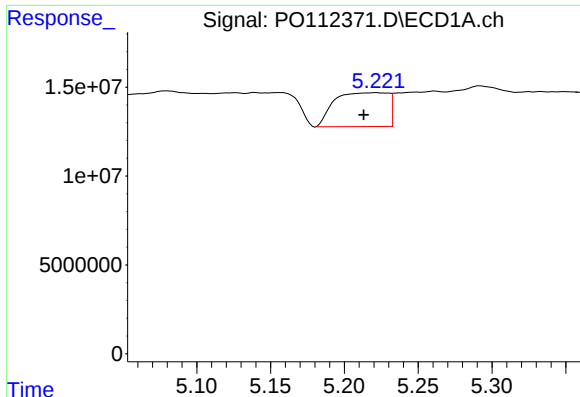

#7 AR-1016-5


R.T.: 5.222 min
Delta R.T.: 0.008 min
Response: 47967182
Conc: 175.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

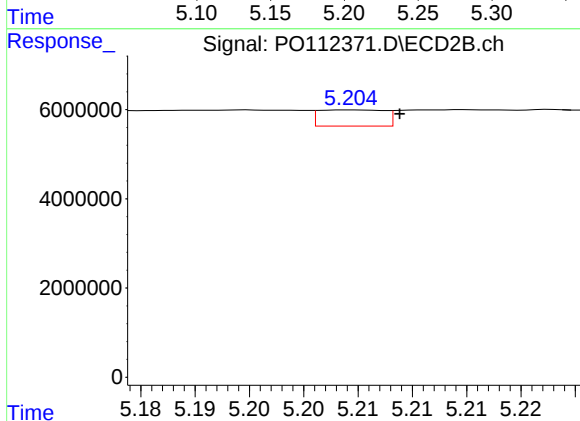


#7 AR-1016-5

R.T.: 5.205 min
Delta R.T.: -0.004 min
Response: 1519698
Conc: 8.81 ng/ml

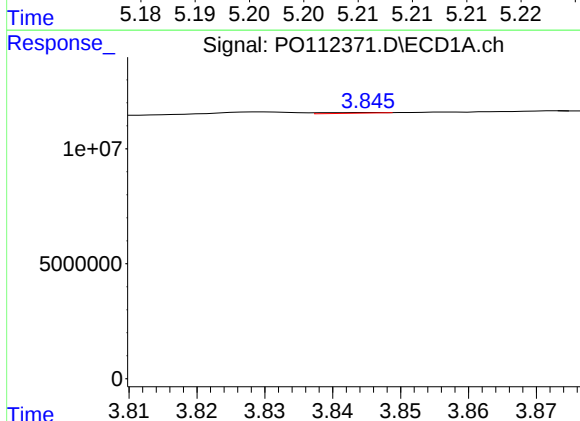


#8 AR-1221-1

R.T.: 3.845 min
Delta R.T.: -0.036 min
Response: 183522
Conc: 1.57 ng/ml

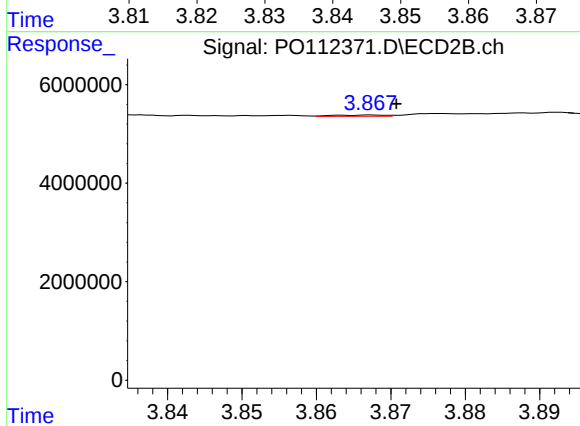

#8 AR-1221-1


R.T.: 3.867 min
Delta R.T.: -0.003 min
Response: 120108
Conc: 1.46 ng/ml

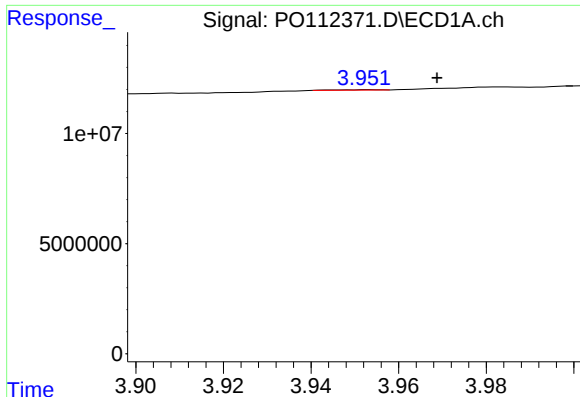

#9 AR-1221-2


R.T.: 3.954 min
Delta R.T.: -0.015 min
Response: 135925
Conc: 1.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

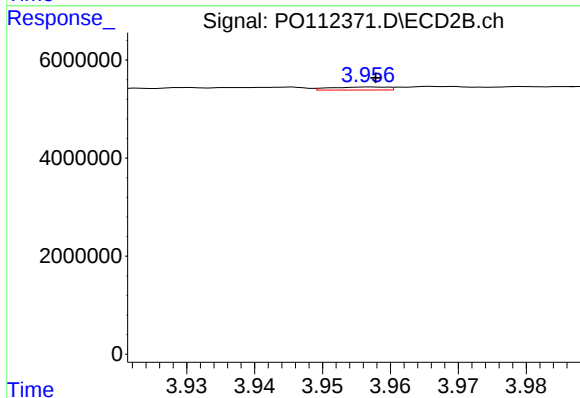


#9 AR-1221-2

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 359262
Conc: 6.05 ng/ml

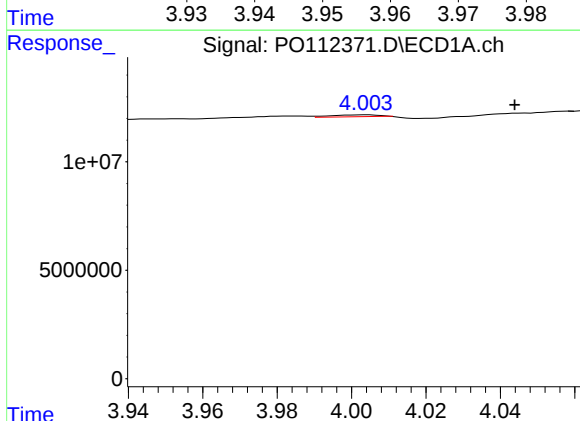


#10 AR-1221-3

R.T.: 4.004 min
Delta R.T.: -0.040 min
Response: 838765
Conc: 3.11 ng/ml

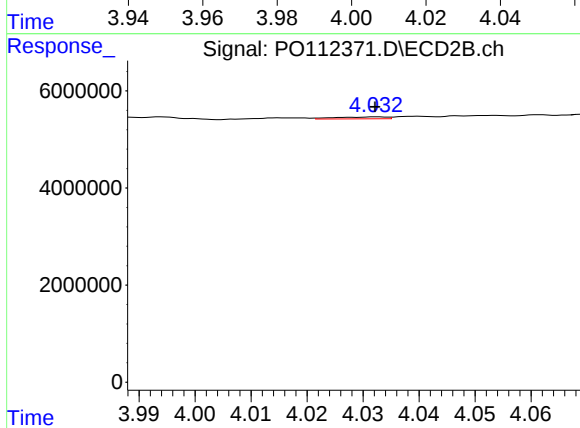

#10 AR-1221-3


R.T.: 4.032 min
Delta R.T.: 0.000 min
Response: 252503
Conc: 1.34 ng/ml

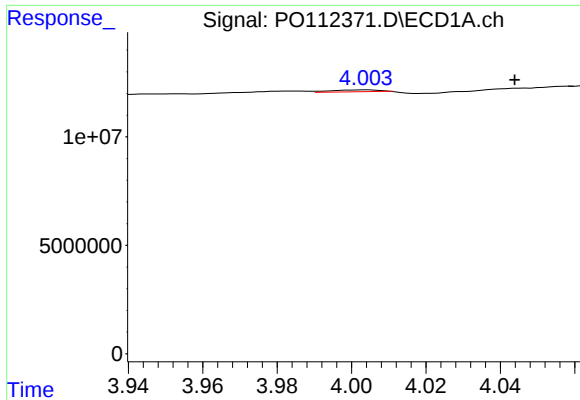

#11 AR-1232-1


R.T.: 4.004 min
Delta R.T.: -0.040 min
Response: 838765
Conc: 3.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

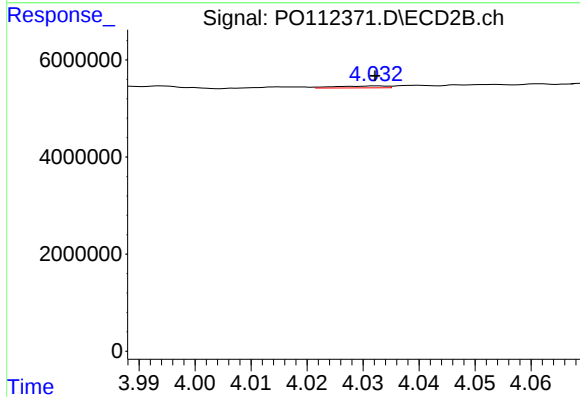


#11 AR-1232-1

R.T.: 4.032 min
Delta R.T.: 0.000 min
Response: 252503
Conc: 1.68 ng/ml

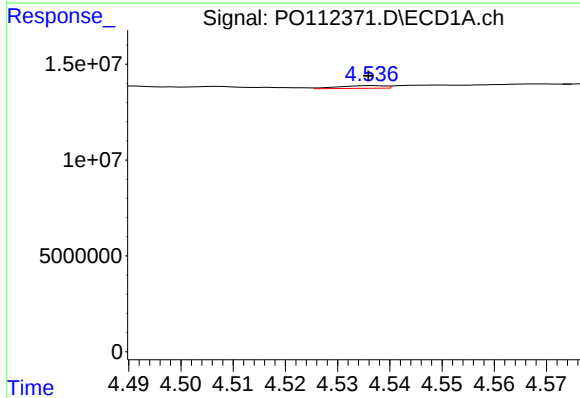


#12 AR-1232-2

R.T.: 4.537 min
Delta R.T.: 0.000 min
Response: 842043
Conc: 7.41 ng/ml

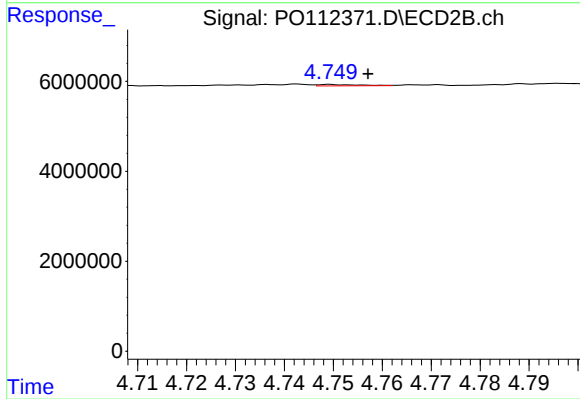

#12 AR-1232-2


R.T.: 4.749 min
Delta R.T.: -0.008 min
Response: 174092
Conc: 1.14 ng/ml

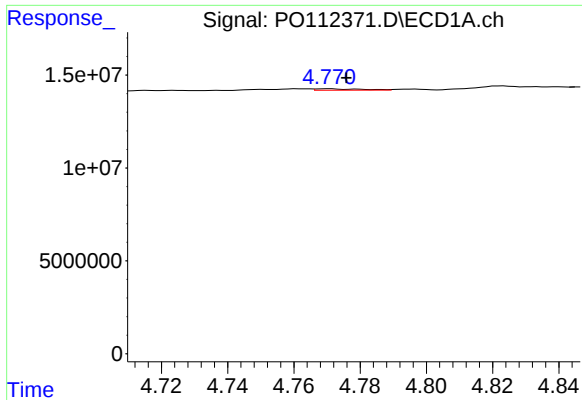

#13 AR-1232-3


R.T.: 4.770 min
Delta R.T.: -0.005 min
Response: 745374
Conc: 3.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

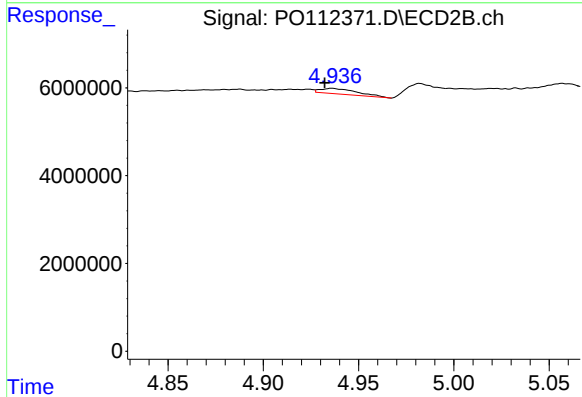


#13 AR-1232-3

R.T.: 4.936 min
Delta R.T.: 0.004 min
Response: 1693050
Conc: 22.42 ng/ml

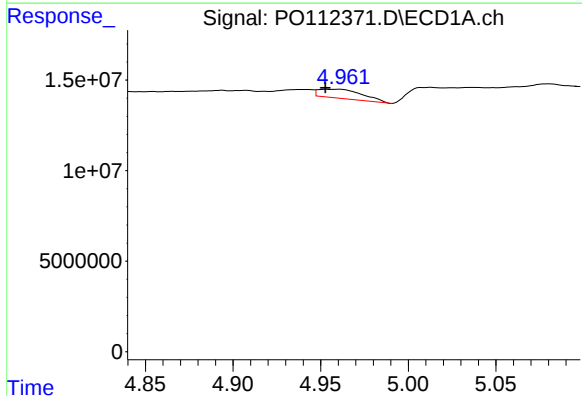


#14 AR-1232-4

R.T.: 4.961 min
Delta R.T.: 0.008 min
Response: 8747221
Conc: 76.53 ng/ml

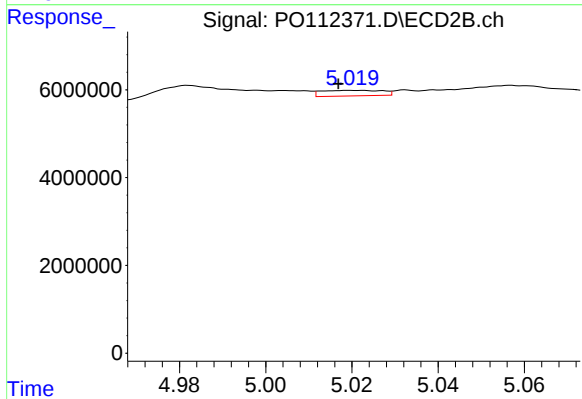

#14 AR-1232-4


R.T.: 5.020 min
Delta R.T.: 0.003 min
Response: 1243543
Conc: 18.84 ng/ml

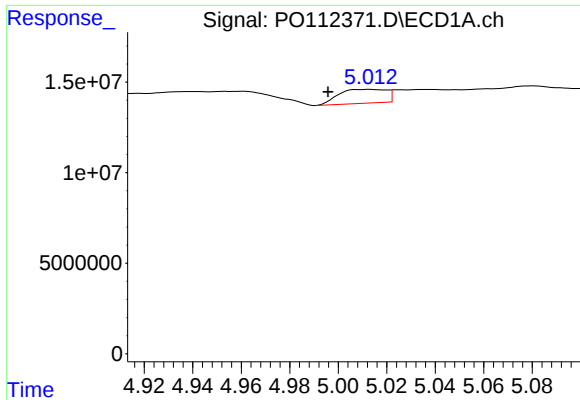

#15 AR-1232-5


R.T.: 5.013 min
Delta R.T.: 0.017 min
Response: 10502076
Conc: 143.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

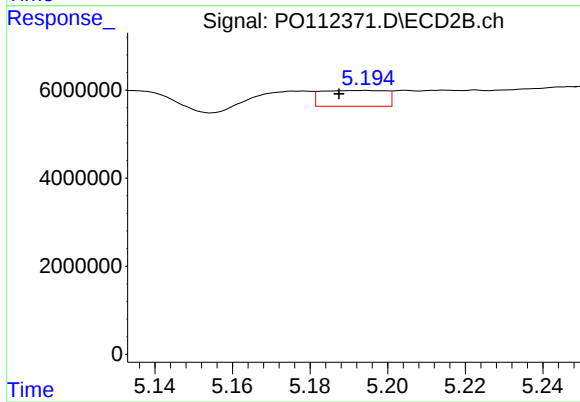


#15 AR-1232-5

R.T.: 5.195 min
Delta R.T.: 0.007 min
Response: 4134628
Conc: 55.68 ng/ml

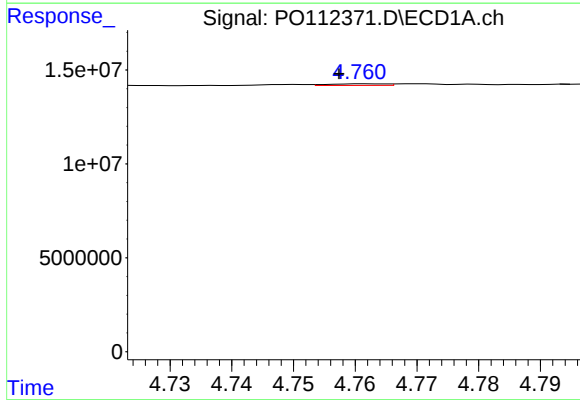


#16 AR-1242-1

R.T.: 4.762 min
Delta R.T.: 0.004 min
Response: 536175
Conc: 1.85 ng/ml

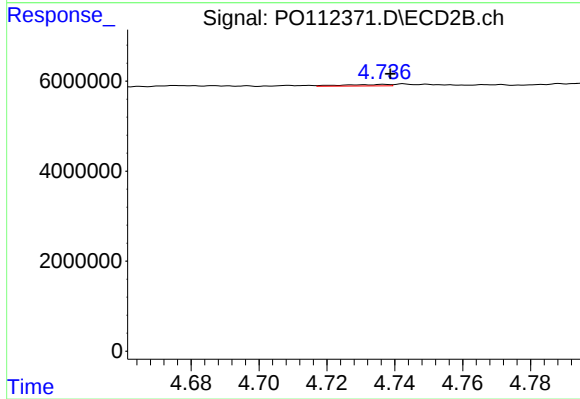

#16 AR-1242-1


R.T.: 4.737 min
Delta R.T.: -0.002 min
Response: 311337
Conc: 1.61 ng/ml

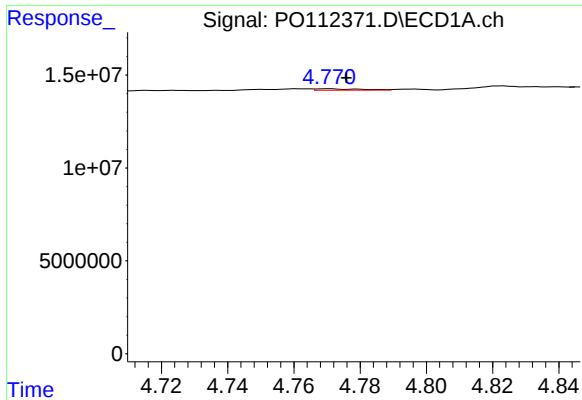

#17 AR-1242-2


R.T.: 4.770 min
Delta R.T.: -0.005 min
Response: 745374
Conc: 1.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

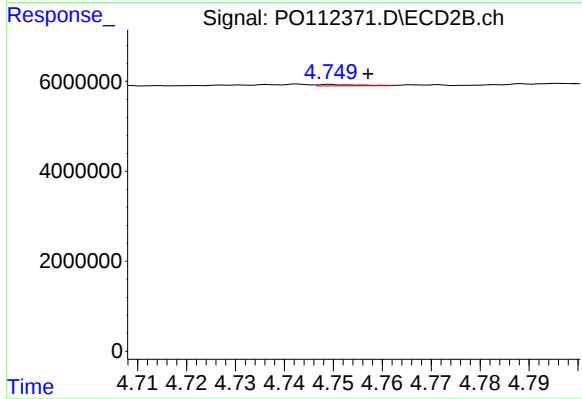


#17 AR-1242-2

R.T.: 4.749 min
Delta R.T.: -0.008 min
Response: 174092
Conc: 0.61 ng/ml

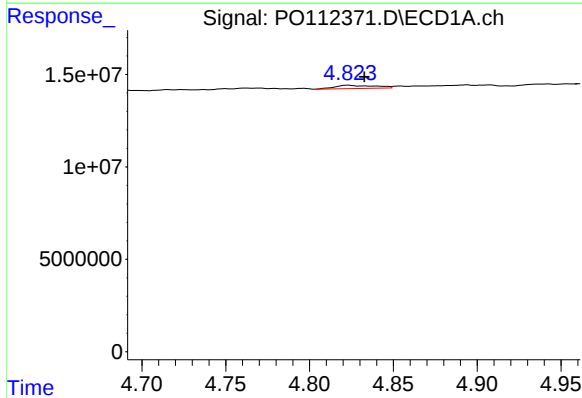


#18 AR-1242-3

R.T.: 4.823 min
Delta R.T.: -0.010 min
Response: 2998056
Conc: 10.95 ng/ml

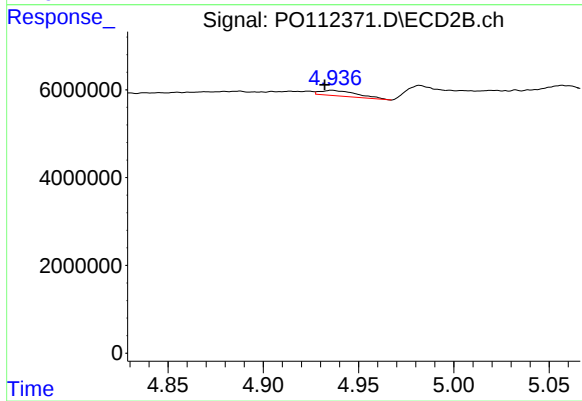

#18 AR-1242-3


R.T.: 4.936 min
Delta R.T.: 0.004 min
Response: 1693050
Conc: 11.62 ng/ml

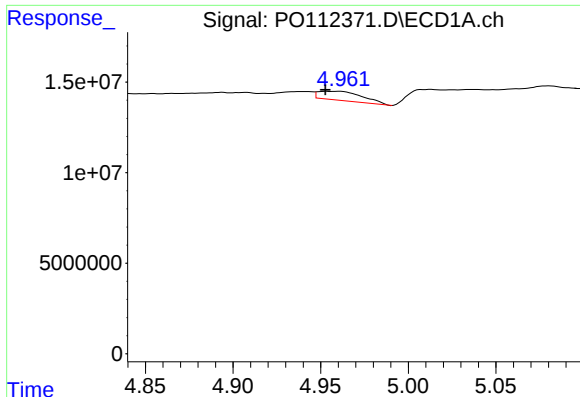

#19 AR-1242-4


R.T.: 4.961 min
Delta R.T.: 0.008 min
Response: 8747221
Conc: 38.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

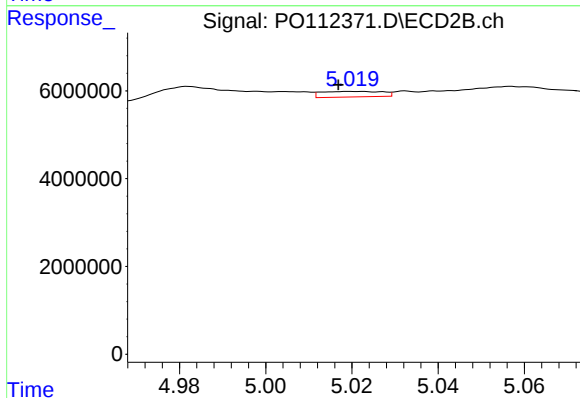


#19 AR-1242-4

R.T.: 5.020 min
Delta R.T.: 0.003 min
Response: 1243543
Conc: 8.77 ng/ml

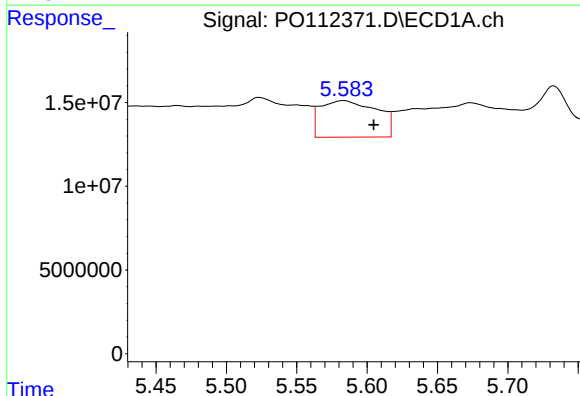


#20 AR-1242-5

R.T.: 5.584 min
Delta R.T.: -0.021 min
Response: 60955878
Conc: 287.97 ng/ml

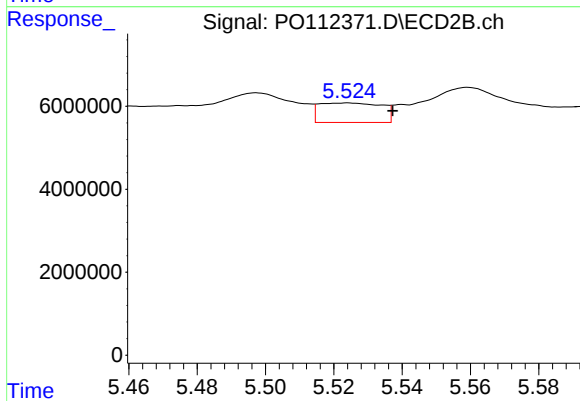

#20 AR-1242-5


R.T.: 5.524 min
Delta R.T.: -0.013 min
Response: 5952436
Conc: 32.75 ng/ml

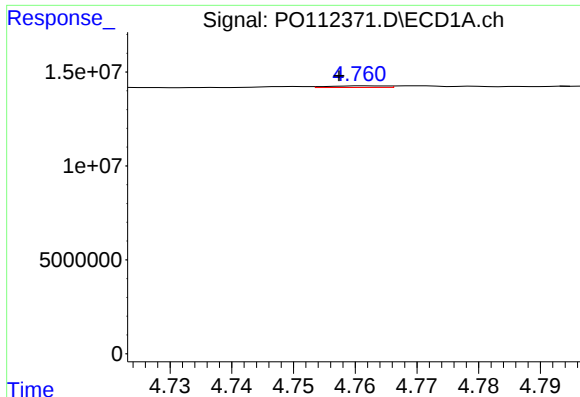

#21 AR-1248-1


R.T.: 4.762 min
Delta R.T.: 0.004 min
Response: 536175
Conc: 2.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

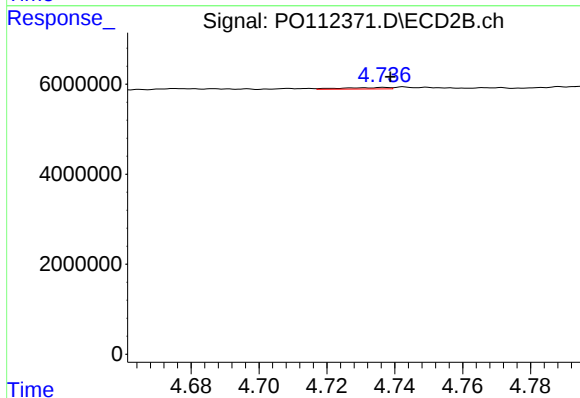


#21 AR-1248-1

R.T.: 4.737 min
Delta R.T.: -0.002 min
Response: 311337
Conc: 2.02 ng/ml

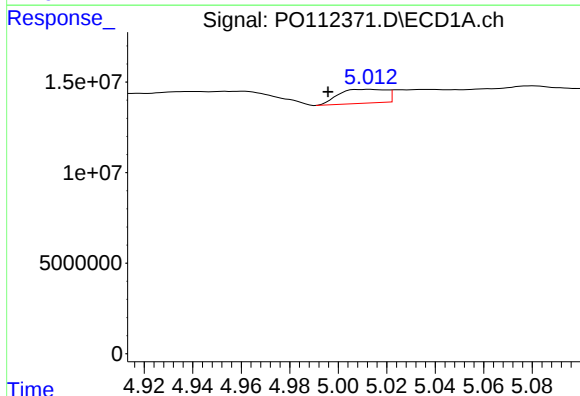


#22 AR-1248-2

R.T.: 5.013 min
Delta R.T.: 0.017 min
Response: 10502076
Conc: 34.06 ng/ml

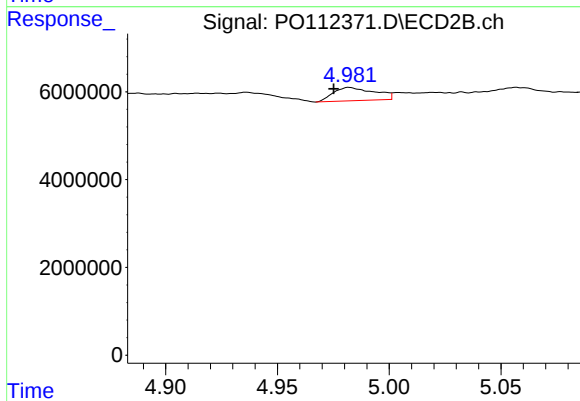

#22 AR-1248-2


R.T.: 4.982 min
Delta R.T.: 0.007 min
Response: 3883568
Conc: 18.87 ng/ml

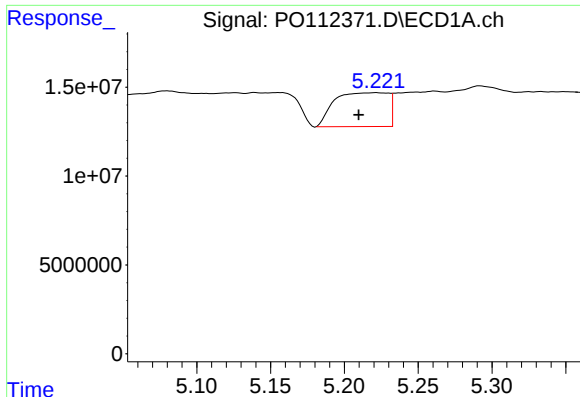

#23 AR-1248-3


R.T.: 5.222 min
Delta R.T.: 0.012 min
Response: 47967182
Conc: 117.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

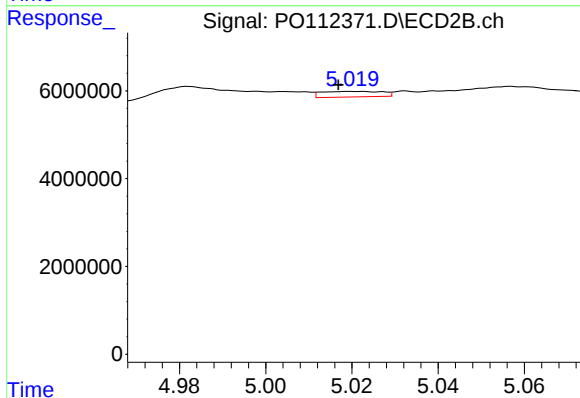


#23 AR-1248-3

R.T.: 5.020 min
Delta R.T.: 0.003 min
Response: 1243543
Conc: 5.79 ng/ml

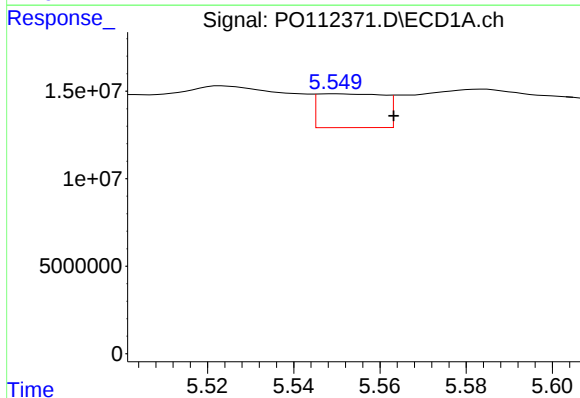


#24 AR-1248-4

R.T.: 5.550 min
Delta R.T.: -0.013 min
Response: 20546571
Conc: 35.60 ng/ml

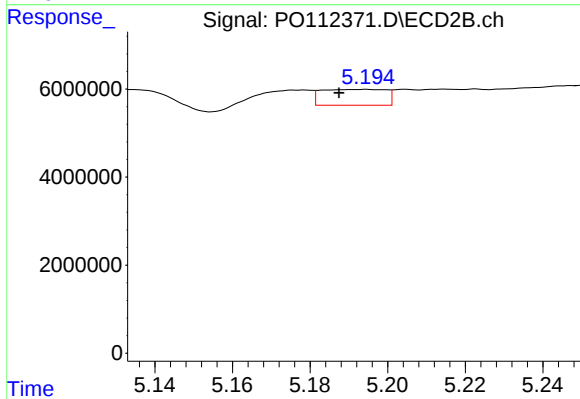

#24 AR-1248-4


R.T.: 5.195 min
Delta R.T.: 0.007 min
Response: 4134628
Conc: 15.98 ng/ml

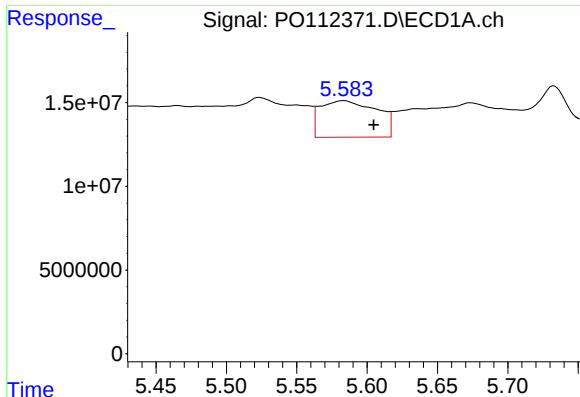

#25 AR-1248-5


R.T.: 5.584 min
Delta R.T.: -0.021 min
Response: 60955878
Conc: 156.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

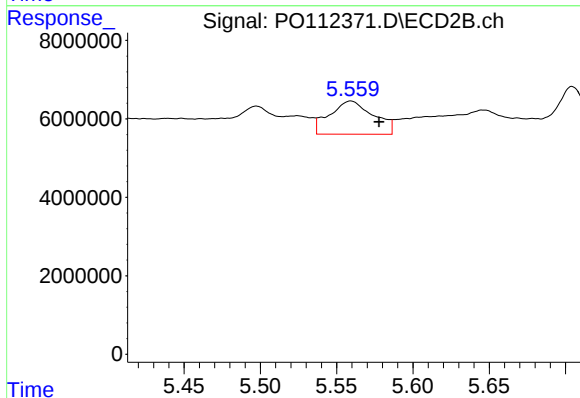


#25 AR-1248-5

R.T.: 5.559 min
Delta R.T.: -0.019 min
Response: 17044693
Conc: 68.03 ng/ml

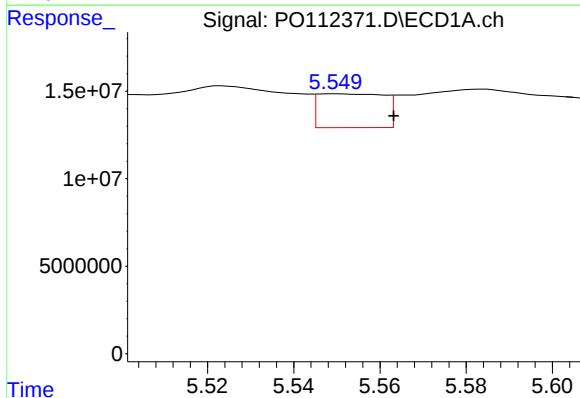


#26 AR-1254-1

R.T.: 5.550 min
Delta R.T.: -0.013 min
Response: 20546571
Conc: 33.40 ng/ml

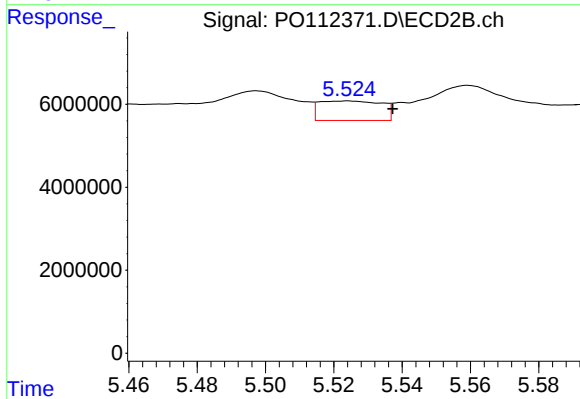

#26 AR-1254-1


R.T.: 5.524 min
Delta R.T.: -0.013 min
Response: 5952436
Conc: 15.62 ng/ml

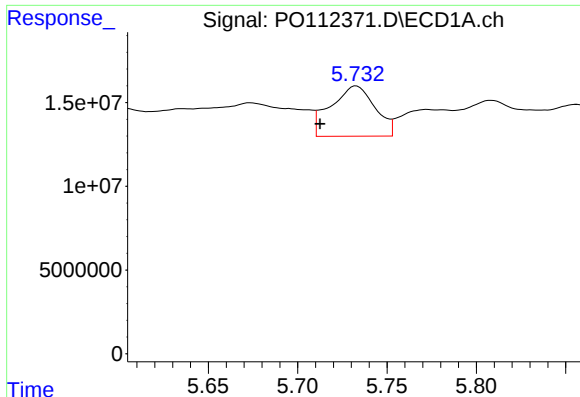

#27 AR-1254-2


R.T.: 5.733 min
Delta R.T.: 0.020 min
Response: 51911881
Conc: 96.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

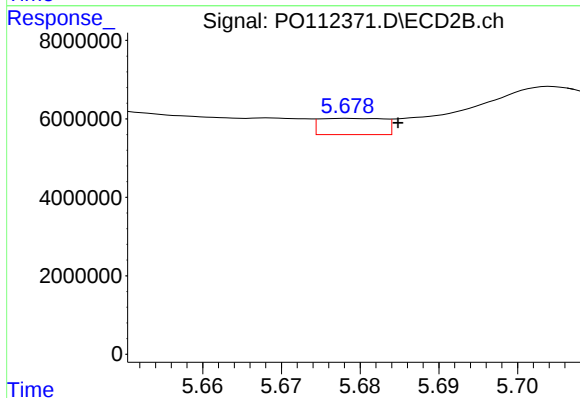


#27 AR-1254-2

R.T.: 5.678 min
Delta R.T.: -0.006 min
Response: 2338823
Conc: 7.05 ng/ml

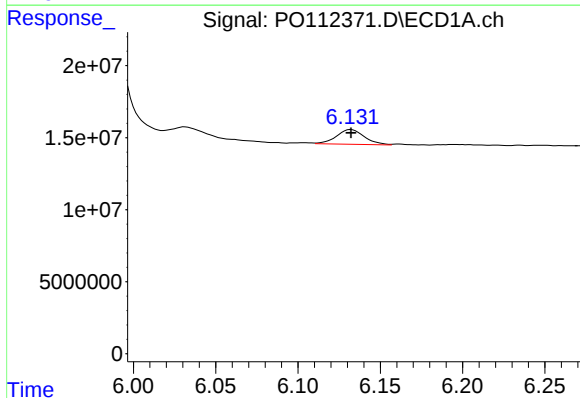


#28 AR-1254-3

R.T.: 6.132 min
Delta R.T.: 0.000 min
Response: 12157102
Conc: 14.48 ng/ml

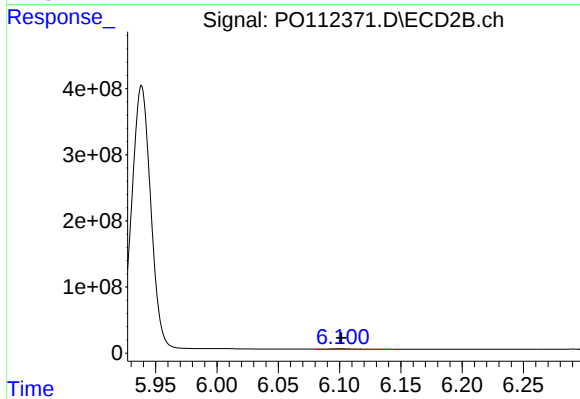

#28 AR-1254-3


R.T.: 6.101 min
Delta R.T.: 0.000 min
Response: 20987916
Conc: 43.54 ng/ml

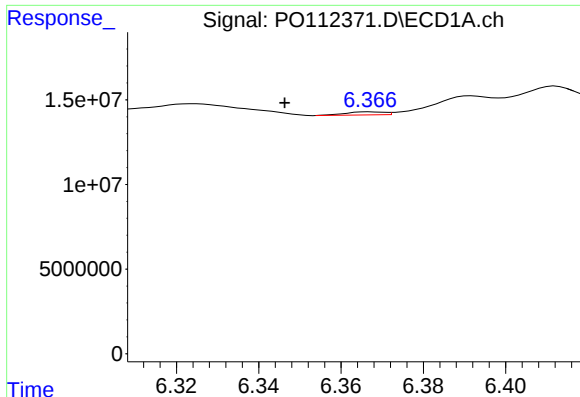

#29 AR-1254-4


R.T.: 6.367 min
Delta R.T.: 0.021 min
Response: 1178740
Conc: 2.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

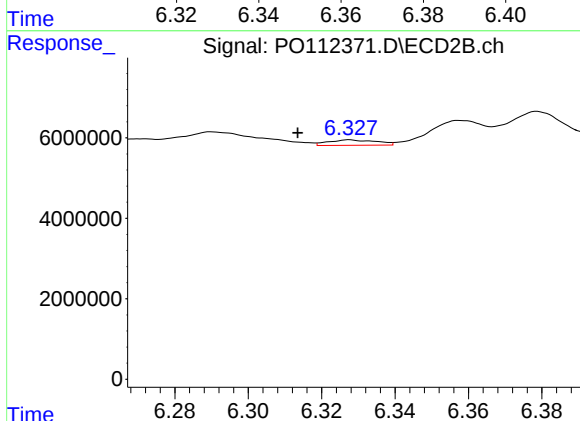


#29 AR-1254-4

R.T.: 6.328 min
Delta R.T.: 0.014 min
Response: 1235750
Conc: 4.74 ng/ml

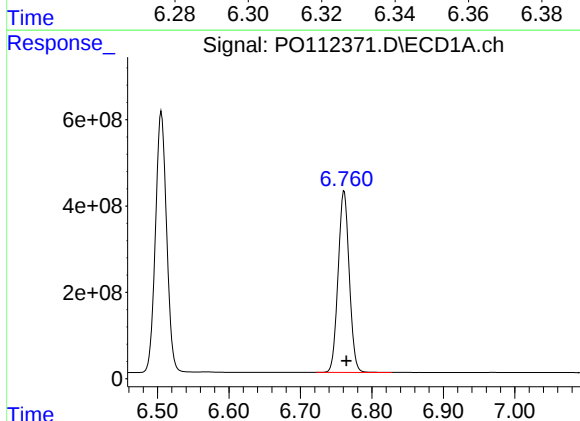


#30 AR-1254-5

R.T.: 6.761 min
Delta R.T.: -0.003 min
Response: 4556985748
Conc: 5887.98 ng/ml

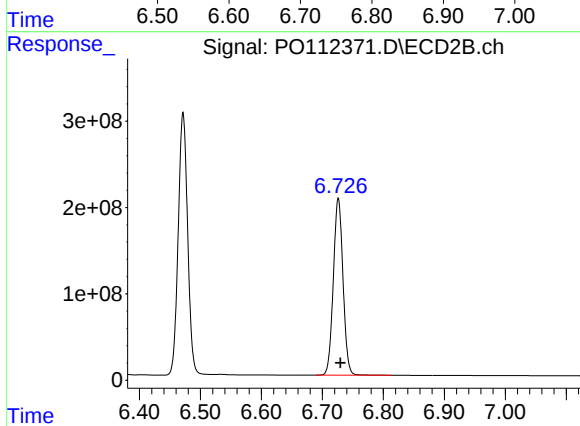

#30 AR-1254-5


R.T.: 6.726 min
Delta R.T.: -0.003 min
Response: 2263954405
Conc: 6353.07 ng/ml

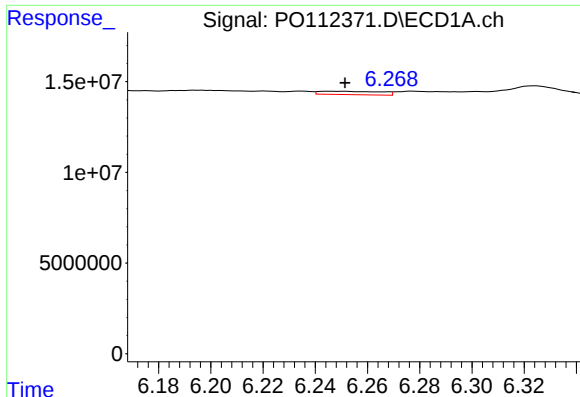

#31 AR-1260-1


R.T.: 6.246 min
Delta R.T.: -0.006 min
Response: 3041322
Conc: 6.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

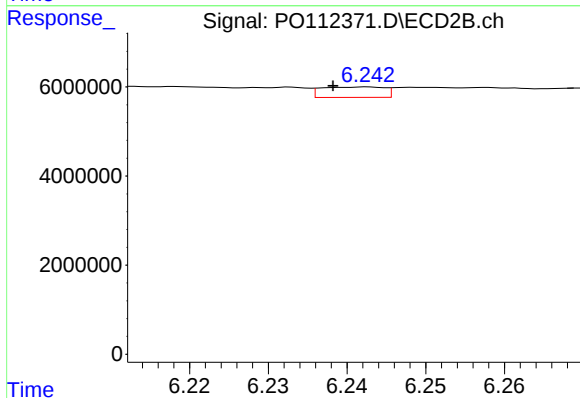


#31 AR-1260-1

R.T.: 6.243 min
Delta R.T.: 0.004 min
Response: 1295180
Conc: 4.62 ng/ml

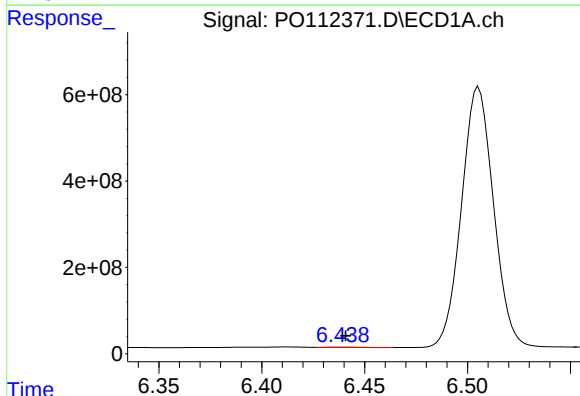


#32 AR-1260-2

R.T.: 6.439 min
Delta R.T.: -0.002 min
Response: 11095202
Conc: 15.03 ng/ml

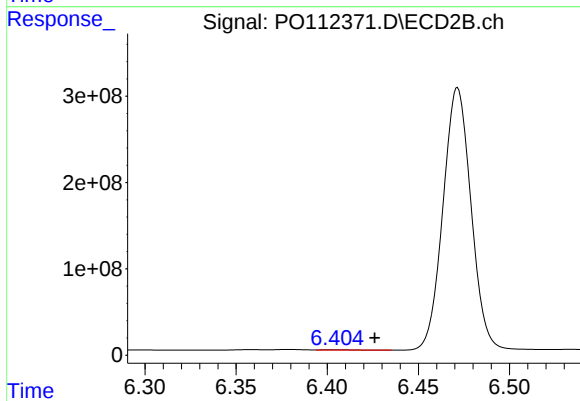

#32 AR-1260-2


R.T.: 6.405 min
Delta R.T.: -0.021 min
Response: 5702796
Conc: 16.77 ng/ml

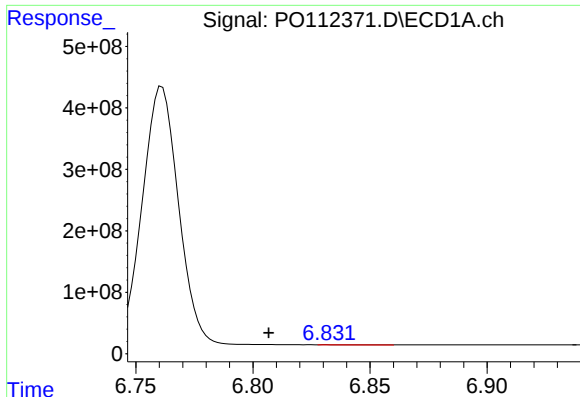

#33 AR-1260-3


R.T.: 6.832 min
Delta R.T.: 0.025 min
Response: 4722163
Conc: 7.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

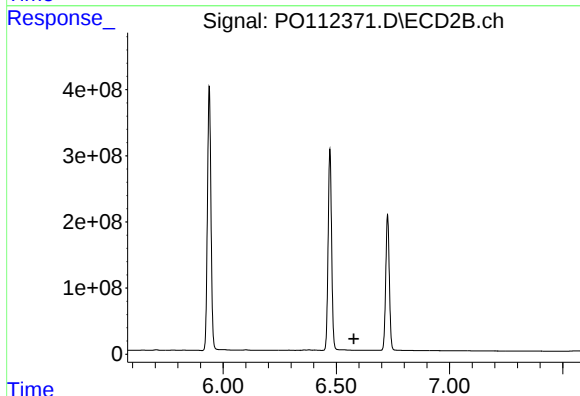


#33 AR-1260-3

R.T.: 6.584 min
Delta R.T.: 0.006 min
Response: -220948
Conc: N.D.

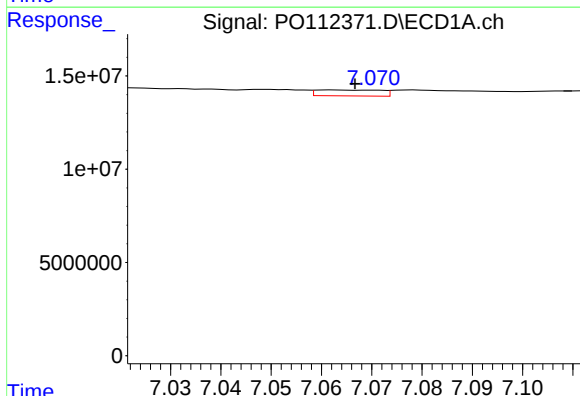


#34 AR-1260-4

R.T.: 7.062 min
Delta R.T.: -0.005 min
Response: 2828500
Conc: 6.50 ng/ml

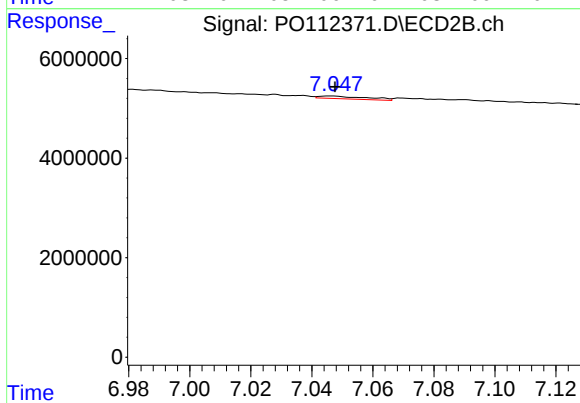

#34 AR-1260-4


R.T.: 7.046 min
Delta R.T.: -0.002 min
Response: 603843
Conc: 3.01 ng/ml

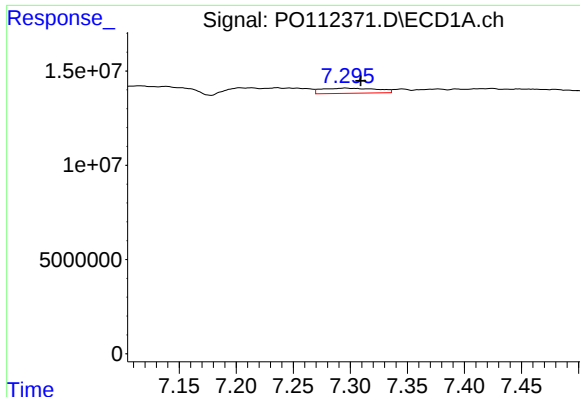

#35 AR-1260-5


R.T.: 7.296 min
Delta R.T.: -0.013 min
Response: 9152317
Conc: 7.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

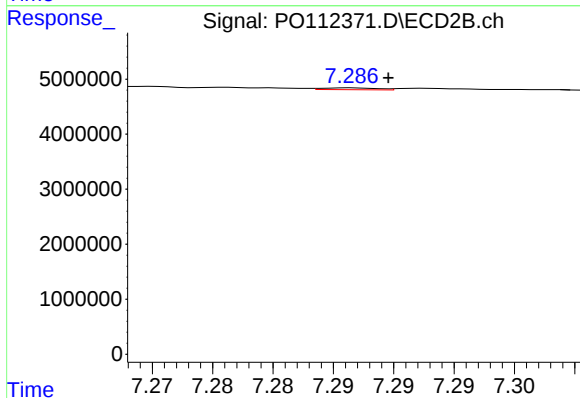


#35 AR-1260-5

R.T.: 7.287 min
Delta R.T.: -0.003 min
Response: 104033
Conc: 0.23 ng/ml

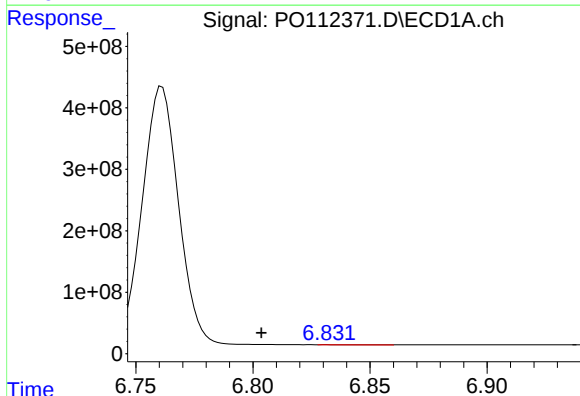


#36 AR-1262-1

R.T.: 6.832 min
Delta R.T.: 0.028 min
Response: 4722163
Conc: 4.62 ng/ml

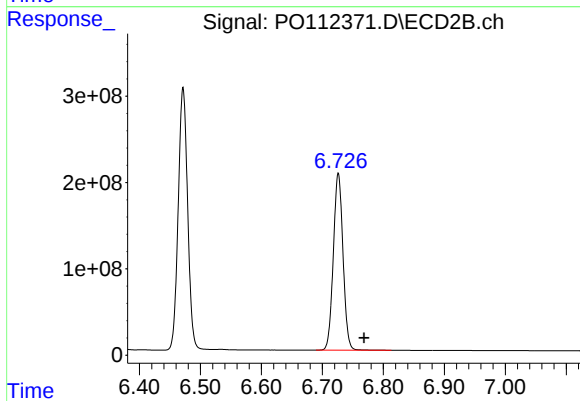

#36 AR-1262-1


R.T.: 6.726 min
Delta R.T.: -0.042 min
Response: 2263954405
Conc: 5558.16 ng/ml

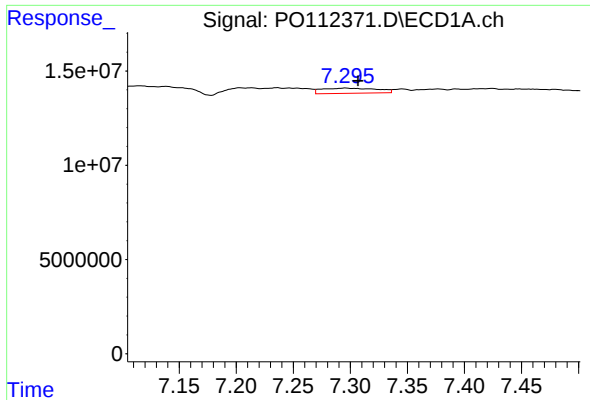

#37 AR-1262-2


R.T.: 7.296 min
Delta R.T.: -0.011 min
Response: 9152317
Conc: 5.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

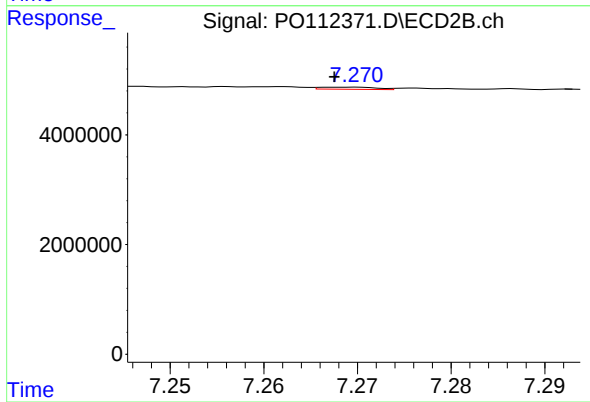


#37 AR-1262-2

R.T.: 7.270 min
Delta R.T.: 0.002 min
Response: 163308
Conc: 0.32 ng/ml

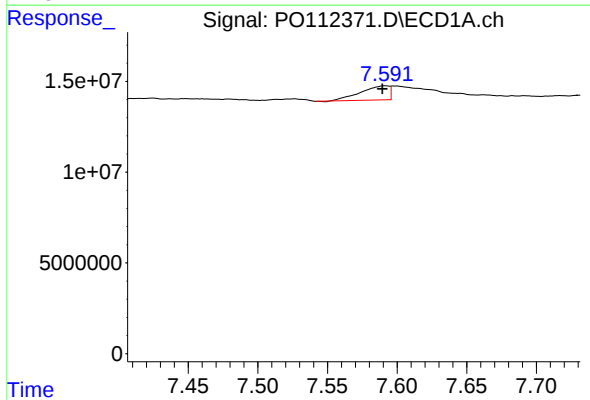


#38 AR-1262-3

R.T.: 7.591 min
Delta R.T.: 0.002 min
Response: 10873815
Conc: 16.94 ng/ml

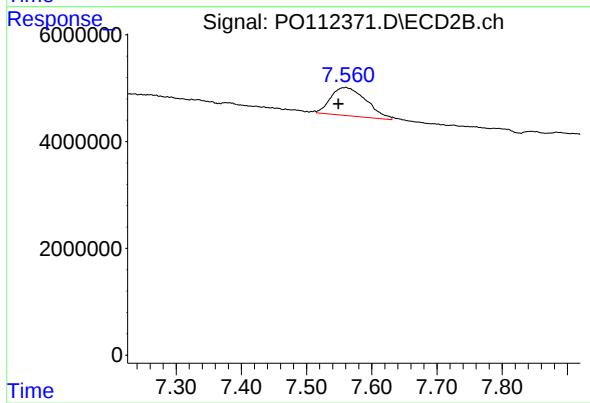

#38 AR-1262-3


R.T.: 7.560 min
Delta R.T.: 0.012 min
Response: 20023808
Conc: 111.54 ng/ml

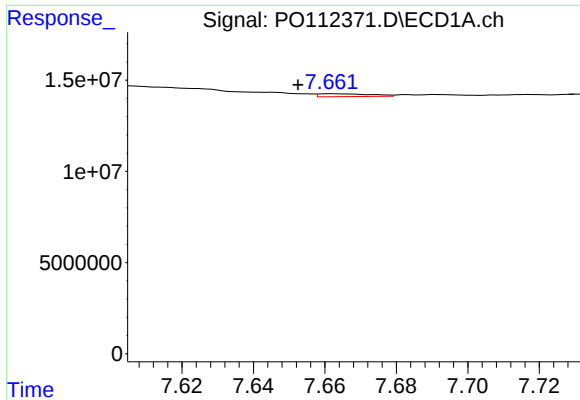

#39 AR-1262-4


R.T.: 7.662 min
Delta R.T.: 0.009 min
Response: 1546265
Conc: 1.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

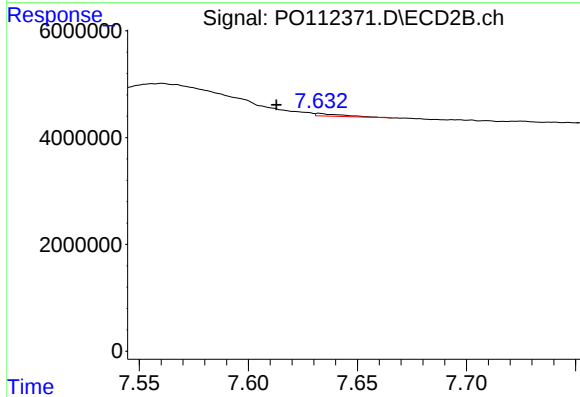


#39 AR-1262-4

R.T.: 7.633 min
Delta R.T.: 0.020 min
Response: 403392
Conc: 1.39 ng/ml

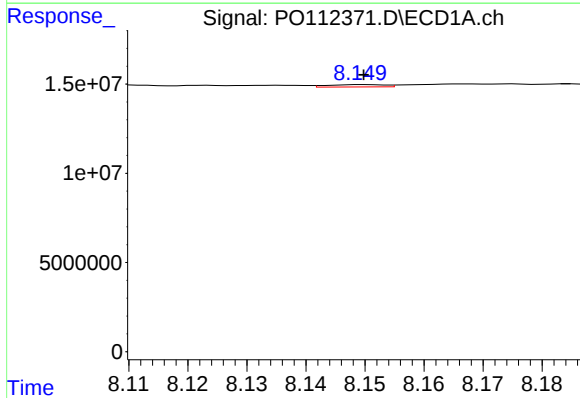


#40 AR-1262-5

R.T.: 8.150 min
Delta R.T.: 0.000 min
Response: 888281
Conc: 1.98 ng/ml

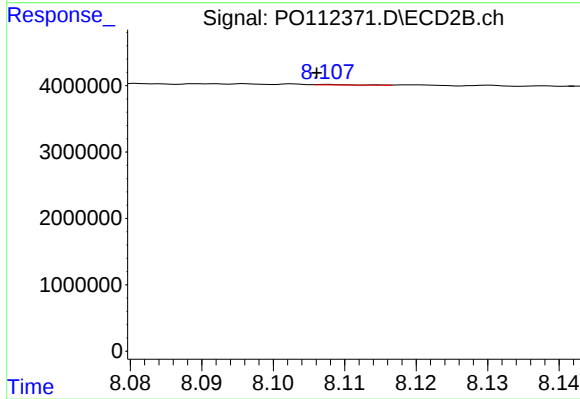

#40 AR-1262-5


R.T.: 8.108 min
Delta R.T.: 0.002 min
Response: 29872
Conc: 0.28 ng/ml

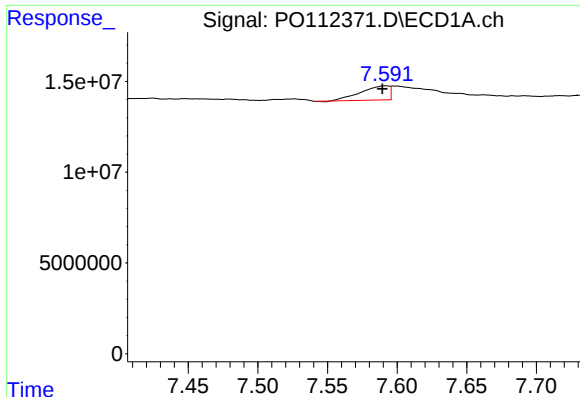

#41 AR-1268-1


R.T.: 7.591 min
Delta R.T.: 0.002 min
Response: 10873815
Conc: 5.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

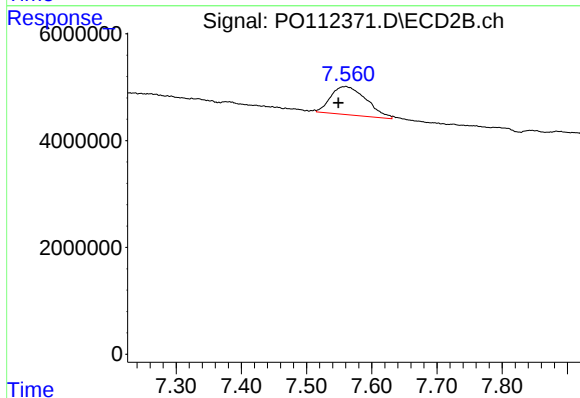


#41 AR-1268-1

R.T.: 7.560 min
Delta R.T.: 0.012 min
Response: 20023808
Conc: 40.74 ng/ml

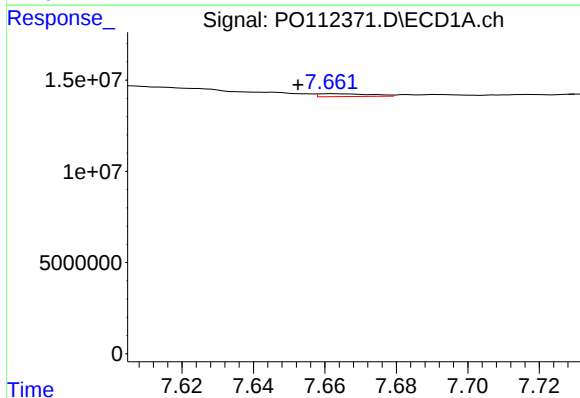


#42 AR-1268-2

R.T.: 7.662 min
Delta R.T.: 0.009 min
Response: 1546265
Conc: 0.99 ng/ml

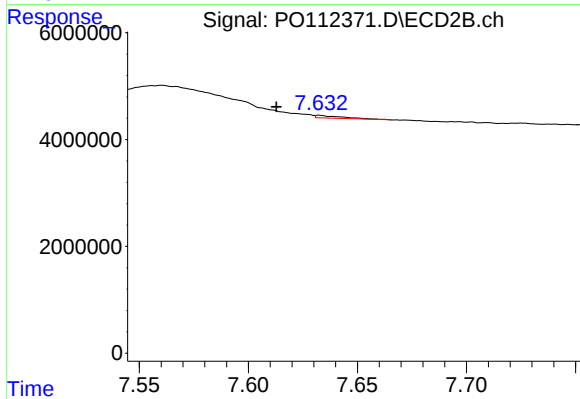

#42 AR-1268-2


R.T.: 7.633 min
Delta R.T.: 0.020 min
Response: 403392
Conc: 0.97 ng/ml

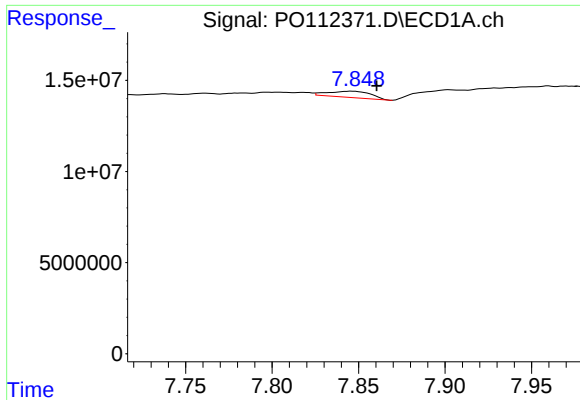

#43 AR-1268-3


R.T.: 7.846 min
Delta R.T.: -0.014 min
Response: 5844338
Conc: 4.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

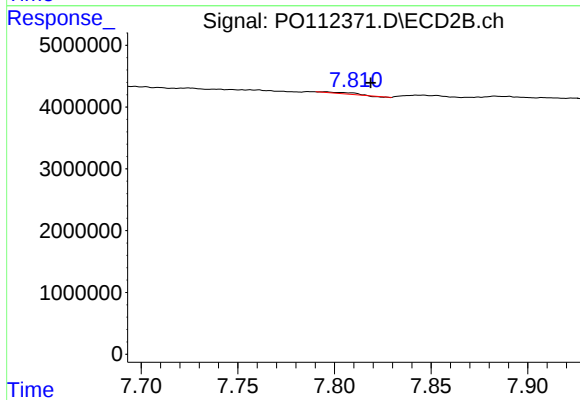


#43 AR-1268-3

R.T.: 7.796 min
Delta R.T.: -0.023 min
Response: 221096
Conc: 0.70 ng/ml

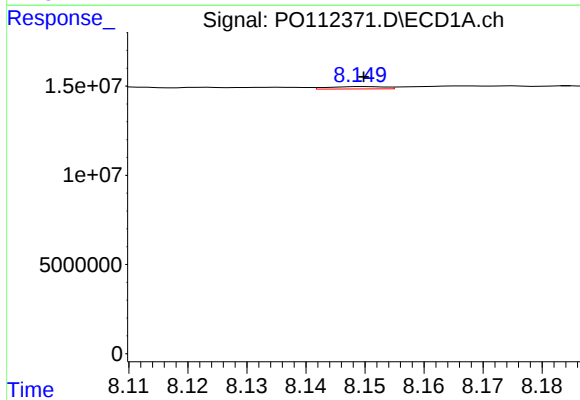


#44 AR-1268-4

R.T.: 8.150 min
Delta R.T.: 0.000 min
Response: 888281
Conc: 1.85 ng/ml

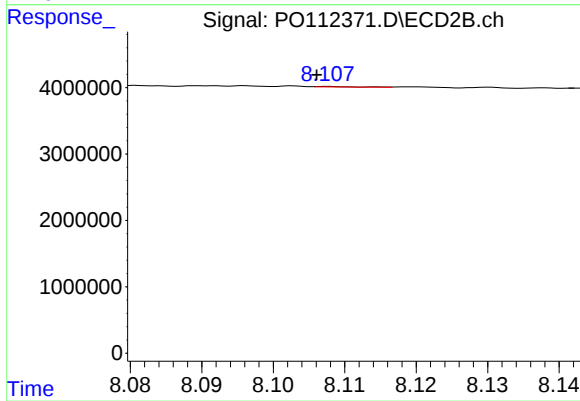

#44 AR-1268-4


R.T.: 8.108 min
Delta R.T.: 0.002 min
Response: 29872
Conc: 0.27 ng/ml

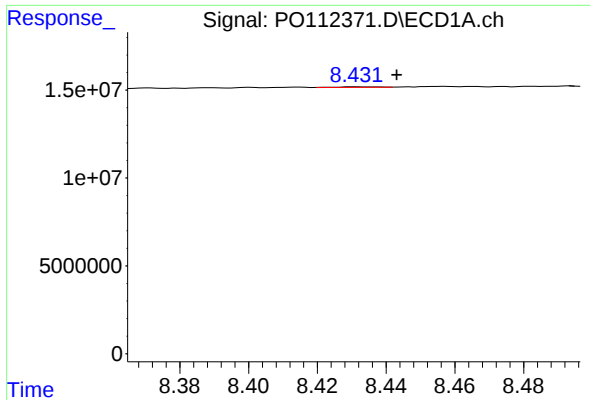

#45 AR-1268-5

R.T.: 8.431 min
Delta R.T.: -0.012 min
Response: 251729
Conc: 0.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
DDT ANALOG

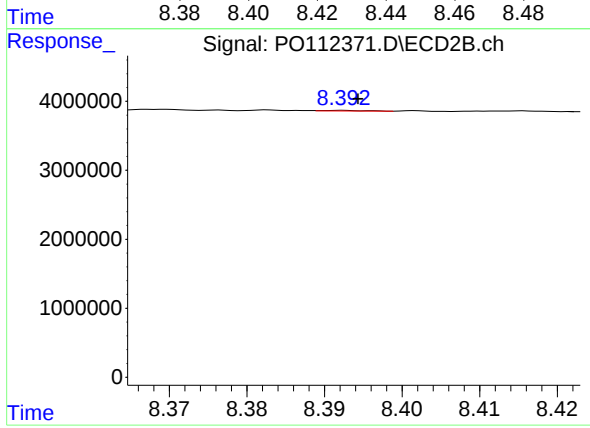

#45 AR-1268-5

R.T.: 8.392 min
Delta R.T.: -0.002 min
Response: 35543
Conc: 0.05 ng/ml