

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072225\
 Data File : P0112394.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Jul 2025 20:34
 Operator : YP/AJ
 Sample : PB168958BL
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB168958BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/23/2025
 Supervised By :mohammad ahmed 07/24/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 01:57:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 22 09:14:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.671	3.663	261.6E6	154.4E6	26.436	24.231
2) SA Decachlor...	8.696	8.642	147.2E6	36262380	21.535	21.040m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072225\
Data File : P0112394.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Jul 2025 20:34
Operator : YP/AJ
Sample : PB168958BL
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB168958BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/23/2025
Supervised By :mohammad ahmed 07/24/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 01:57:34 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 22 09:14:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

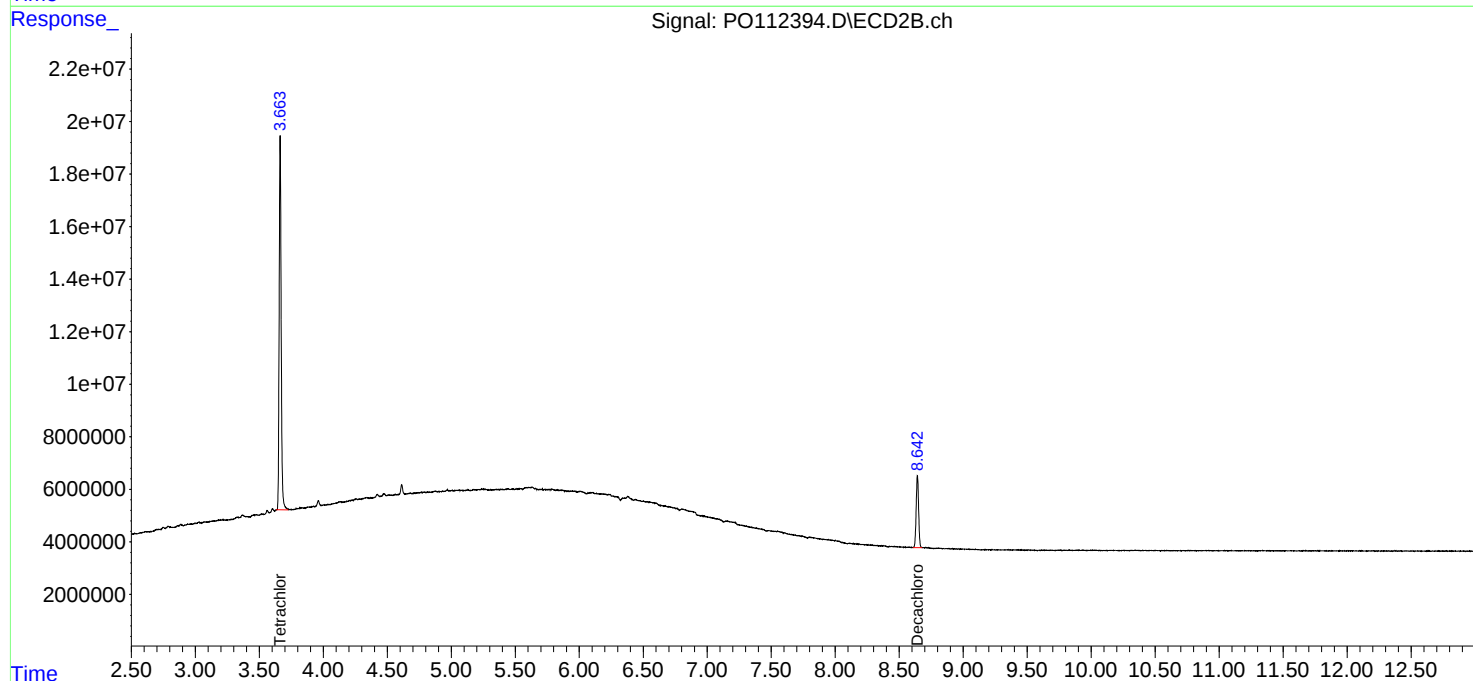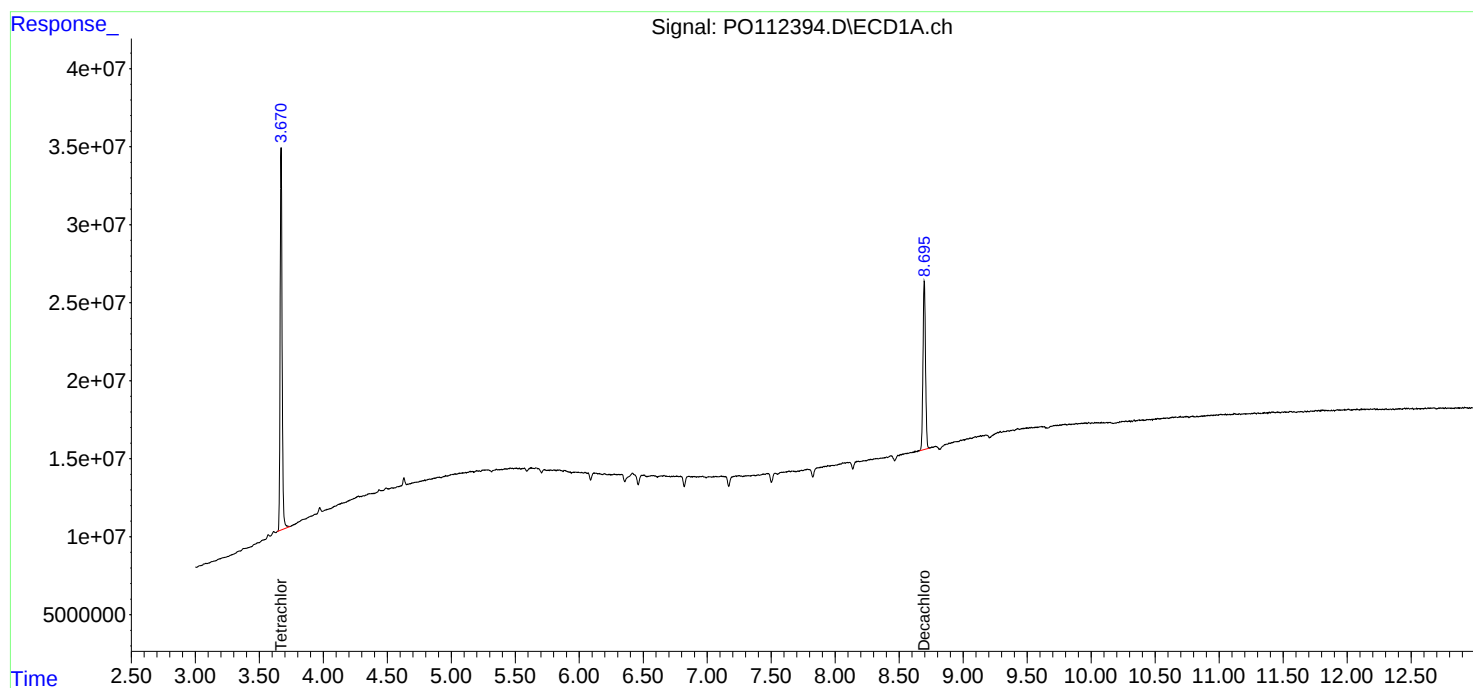

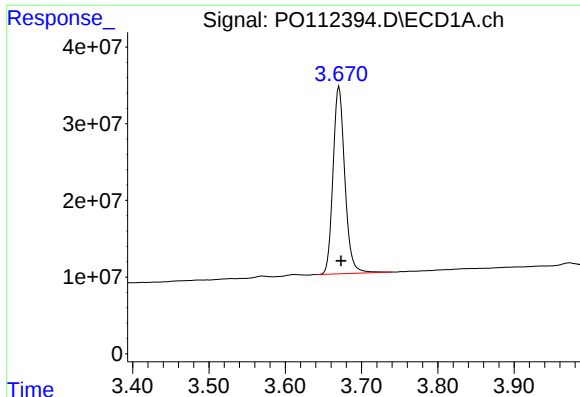

#1 Tetrachloro-m-xylene

R.T.: 3.671 min
Delta R.T.: -0.002 min
Response: 261578483
Conc: 26.44 ng/ml

Instrument :

ECD_O

ClientSampleId :


PB168958BL

Manual Integrations

APPROVED


Reviewed By :Yogesh Patel 07/23/2025

Supervised By :mohammad ahmed 07/24/2025

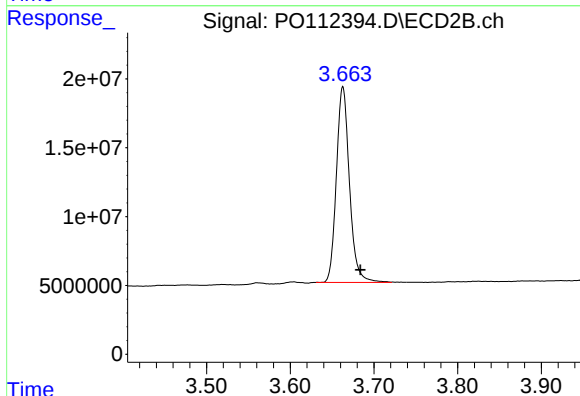


#1 Tetrachloro-m-xylene

R.T.: 3.663 min
Delta R.T.: -0.021 min
Response: 154374187
Conc: 24.23 ng/ml

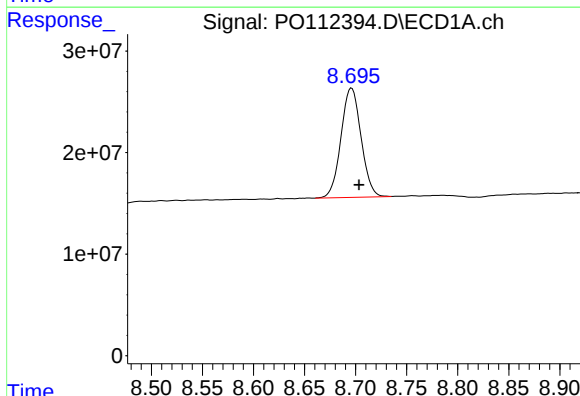

#2 Decachlorobiphenyl

R.T.: 8.696 min
Delta R.T.: -0.007 min
Response: 147237064
Conc: 21.54 ng/ml

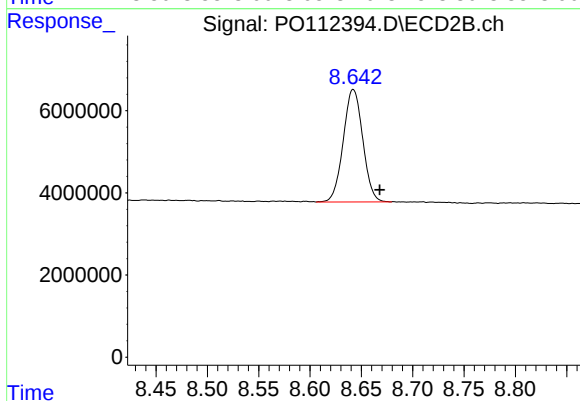

#2 Decachlorobiphenyl

R.T.: 8.642 min
Delta R.T.: -0.026 min
Response: 36262380
Conc: 21.04 ng/ml m