

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072225\
 Data File : P0112409.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 02:41
 Operator : YP/AJ
 Sample : Q2660-05 10X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MOO-25-0220

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/23/2025
 Supervised By :mohammad ahmed 07/24/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 04:32:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 22 09:14:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.670	3.661	7802123	6957281	0.789m	1.092m#
2) SA Decachlor...	8.696	8.642	4538816	1167765	0.664	0.678m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO072225\
Data File : PO112409.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2025 02:41
Operator : YP/AJ
Sample : Q2660-05 10X
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MOO-25-0220


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/23/2025
Supervised By :mohammad ahmed 07/24/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 23 04:32:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 22 09:14:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

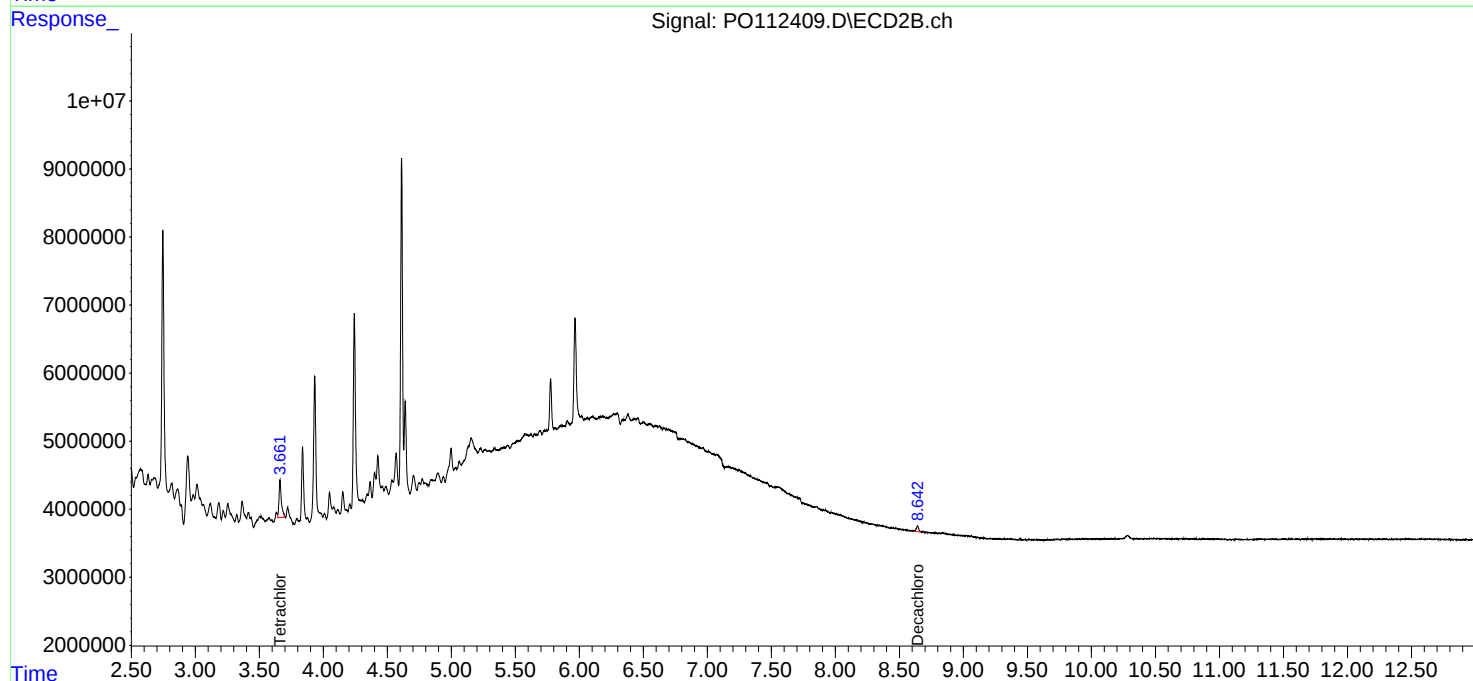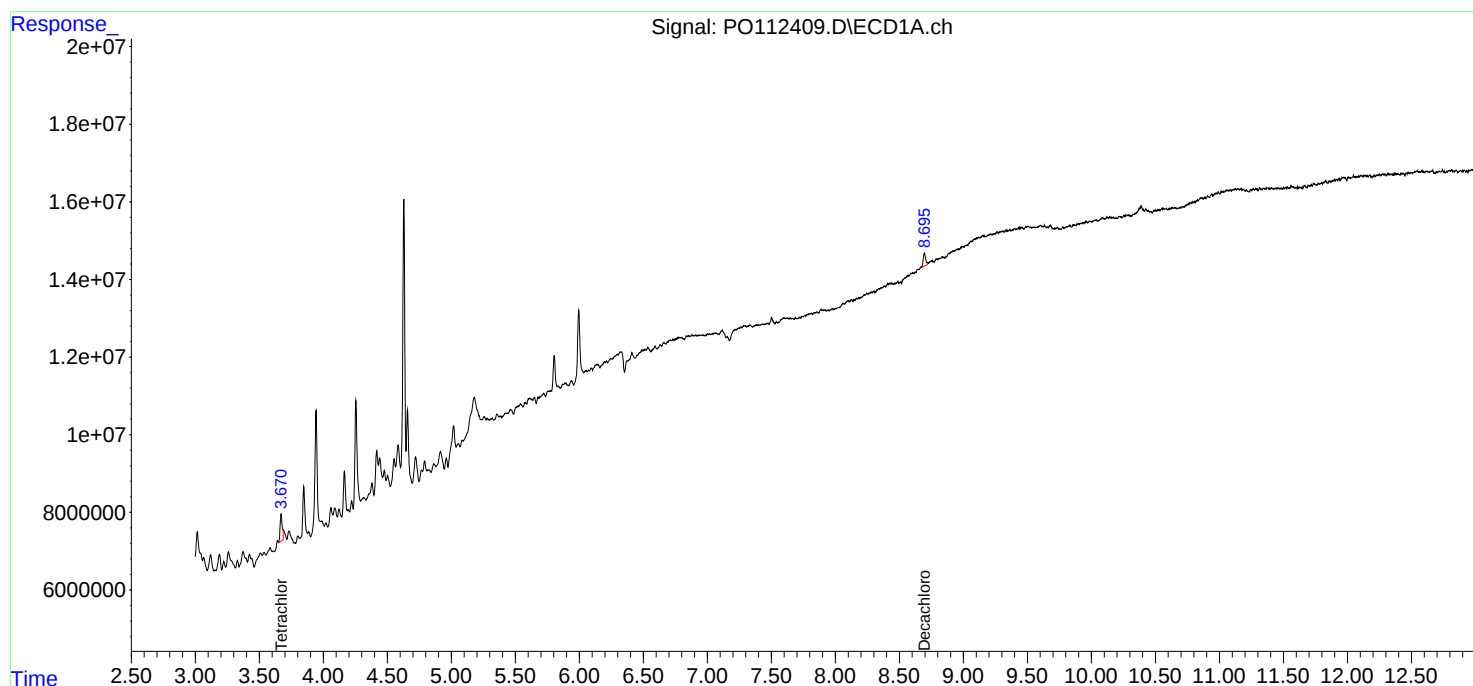

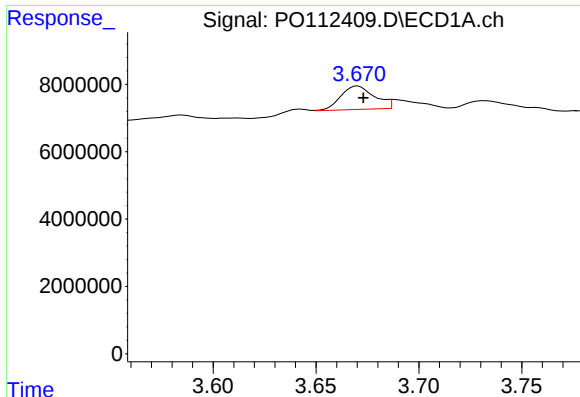


#1 Tetrachloro-m-xylene

R.T.: 3.670 min
Delta R.T.: -0.003 min
Response: 7802123
Conc: 0.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
MOO-25-0220


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/23/2025
Supervised By :mohammad ahmed 07/24/2025

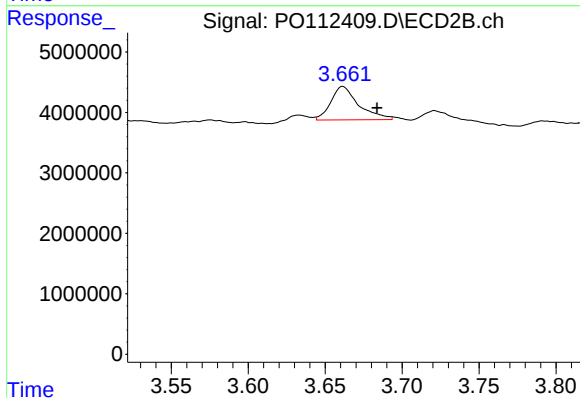


#1 Tetrachloro-m-xylene

R.T.: 3.661 min
Delta R.T.: -0.023 min
Response: 6957281
Conc: 1.09 ng/ml m

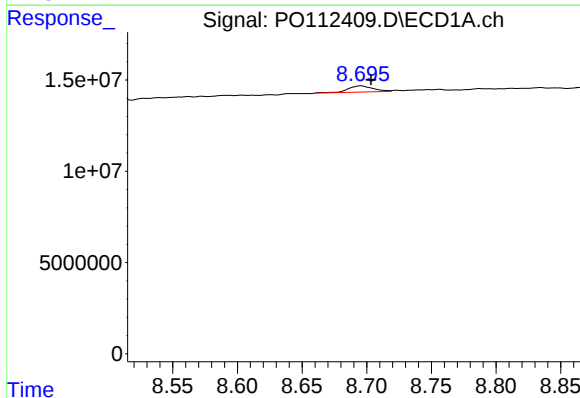

#2 Decachlorobiphenyl

R.T.: 8.696 min
Delta R.T.: -0.008 min
Response: 4538816
Conc: 0.66 ng/ml

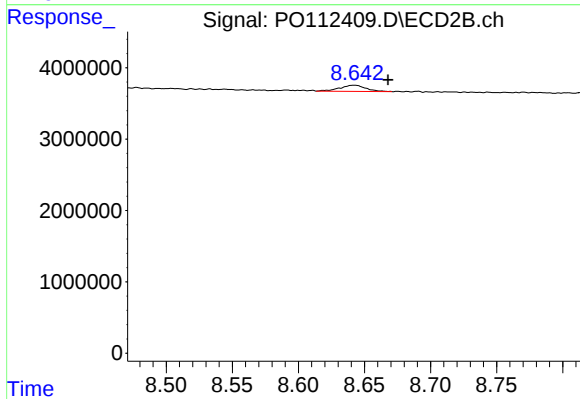

#2 Decachlorobiphenyl

R.T.: 8.642 min
Delta R.T.: -0.026 min
Response: 1167765
Conc: 0.68 ng/ml m