

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072318\
 Data File : P0047049.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jul 2018 00:59
 Operator : SM/SJ
 Sample : J3762-07
 Misc : ECD_0 LOD WATER 25 PPB
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2018

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 06:01:32 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 24 03:04:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.398	3.649	3360165	3666295	20.041	19.116
2) SA Decachlor...	10.086	8.656	2445553	2133305	22.339	23.228
Target Compounds						
3) L1 AR-1016-1	5.298	4.517	117953	104925	36.263	30.884
4) L1 AR-1016-2	5.650	4.933	143618	96440	36.714	29.977
5) L1 AR-1016-3	5.748	4.973	107462	87364	33.378	33.278
6) L1 AR-1016-4	6.041	5.015	119184	86944	37.772	27.949 #
7) L1 AR-1016-5	6.180	5.187	117550	142402	35.591	41.237
9) L2 AR-1221-2	4.703	3.950	64602	49985	54.372	41.717
10) L2 AR-1221-3	4.770	4.027	88648	72069	23.912	18.257
11) L3 AR-1232-1	5.105	4.325	112714	226332	75.258	143.997 #
12) L3 AR-1232-2	5.565	4.737	169884	171481	83.375	85.998
13) L3 AR-1232-3	5.587	4.756	233341	253787	80.239	82.100
14) L3 AR-1232-4	5.650	4.812	143618	130605	80.491	71.636
15) L3 AR-1232-5	5.748	4.973	107462	87364	75.852	86.922
16) L4 AR-1242-1	5.587	4.756	233341	253787	40.257	44.111
17) L4 AR-1242-2	5.650	4.933	143618	96440	40.485	33.522
18) L4 AR-1242-3	5.748	5.015	107462	86944	37.871	30.435
19) L4 AR-1242-4	6.041	5.187	119184	142402	41.443	46.608
20) L4 AR-1242-5	6.180	5.335	117550	135555	37.947	41.960
21) L5 AR-1248-1	6.041	5.187	119184	142402	25.489	28.407
22) L5 AR-1248-2	6.180	5.335	117550	135555	29.659	32.346
23) L5 AR-1248-3	6.442	5.539	36235	129841	7.137	20.254 #
24) L5 AR-1248-4	6.442	5.579	36235	45819	7.586	10.237 #
25) L5 AR-1248-5	6.633	6.103	109813	232503	34.289	84.021 #
26) L6 AR-1254-1	6.633	5.539	109813	129841	13.355	18.176 #
27) L6 AR-1254-2	6.944	5.684	45552	106650	9.277	17.607 #
28) L6 AR-1254-3	6.999	6.103	77856	232503	9.059	24.694 #
29) L6 AR-1254-4	7.282	6.344	58223	63115	9.117	10.943
30) L6 AR-1254-5	7.546	6.680	115057	68461	24.230	17.244 #
31) L7 AR-1260-1	7.161	6.218	262249	236153	43.668	39.839
32) L7 AR-1260-2	7.418	6.404	278232	288699	38.072	41.105
33) L7 AR-1260-3	7.700	6.732	326386	326734	38.063	43.520
34) L7 AR-1260-4	8.315	7.269	399332	406981	32.987	34.899
35) L7 AR-1260-5	8.638	7.617	228055	354045	30.915	42.696 #
36) L8 AR-1262-1	7.161	6.404	262249	288699	48.726	46.781
37) L8 AR-1262-2	7.418	6.559	278232	260427	43.224	42.547
38) L8 AR-1262-3	7.774	6.771	159763	195935	19.360	24.075
39) L8 AR-1262-4	8.000	7.031	229173	176731	28.687	24.900

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072318\
 Data File : P0047049.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jul 2018 00:59
 Operator : SM/SJ
 Sample : J3762-07
 Misc : ECD_0 LOD WATER 25 PPB
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2018

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 06:01:32 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 24 03:04:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
40) L8	AR-1262-5	8.315	7.269	399332	406981	26.804	29.077
41) L9	AR-1268-1	8.638	7.555	228055	103890	14.561	7.625 #
42) L9	AR-1268-2	8.691	7.617	119889	354045	8.555	28.209 #
44) L9	AR-1268-4	9.354	8.110	82233	82703	16.273	18.881
45) L9	AR-1268-5	0.000	8.402	0	30940	N.D.	1.031 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO072318\
Data File : PO047049.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jul 2018 00:59
Operator : SM/SJ
Sample : J3762-07
Misc : ECD_0 LOD WATER 25 PPB
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 06:01:32 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO072318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 24 03:04:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

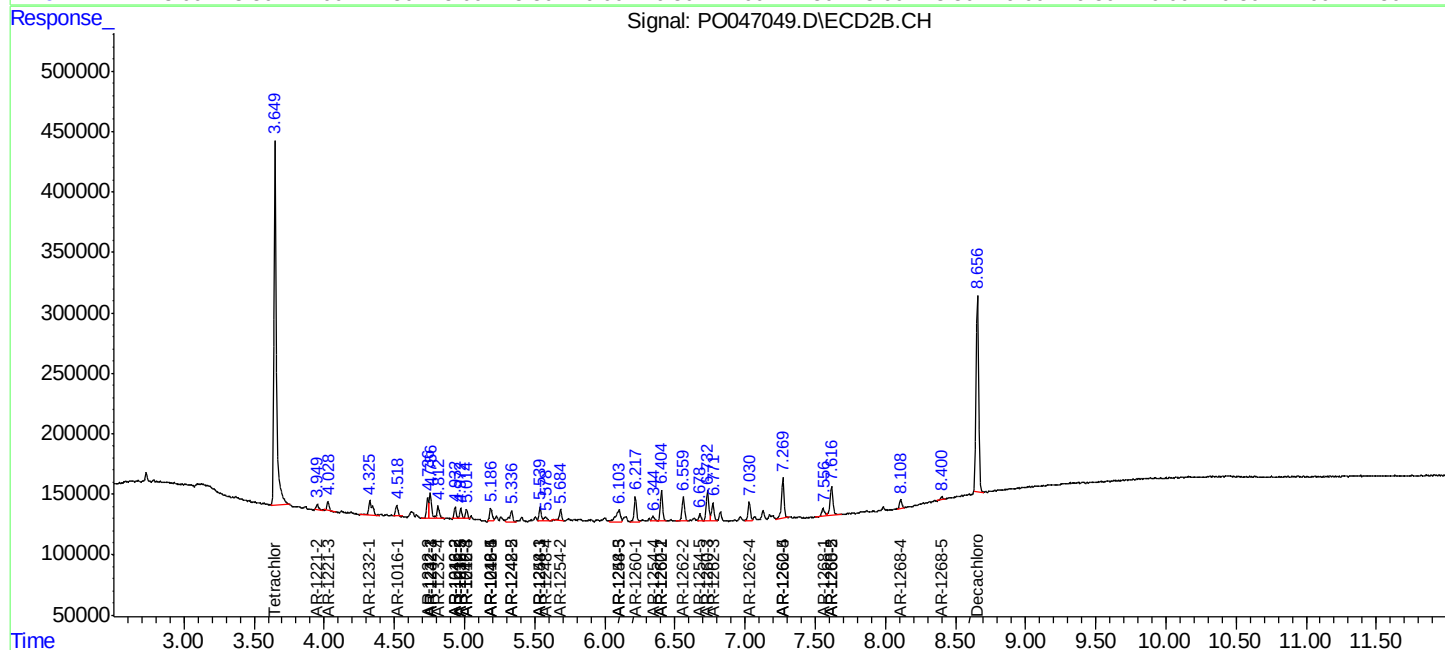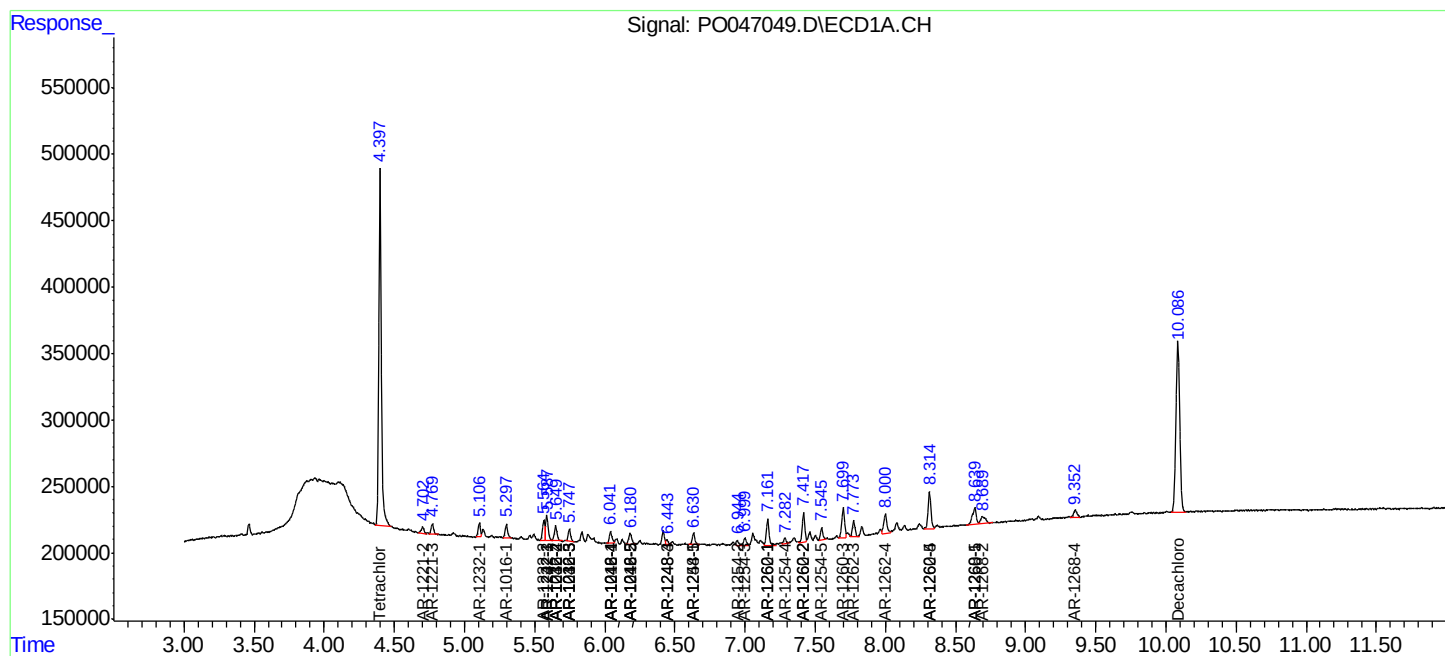


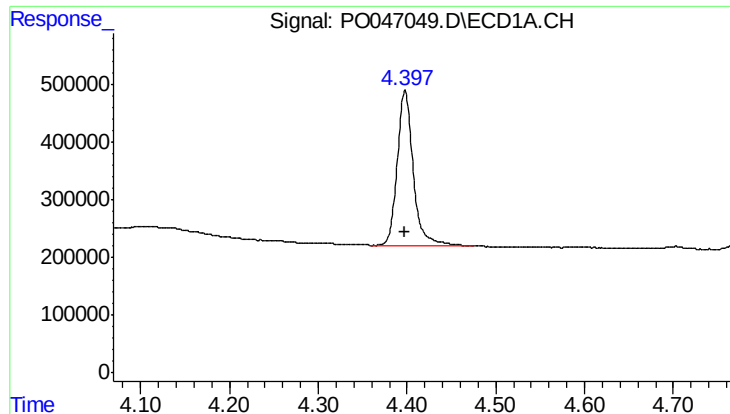

#1 Tetrachloro-m-xylene


R.T.: 4.398 min
Delta R.T.: 0.000 min
Response: 3360165
Conc: 20.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

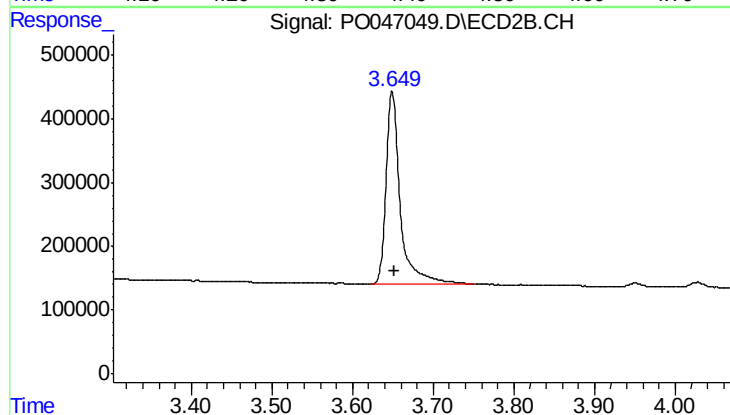


#1 Tetrachloro-m-xylene

R.T.: 3.649 min
Delta R.T.: -0.002 min
Response: 3666295
Conc: 19.12 ng/ml

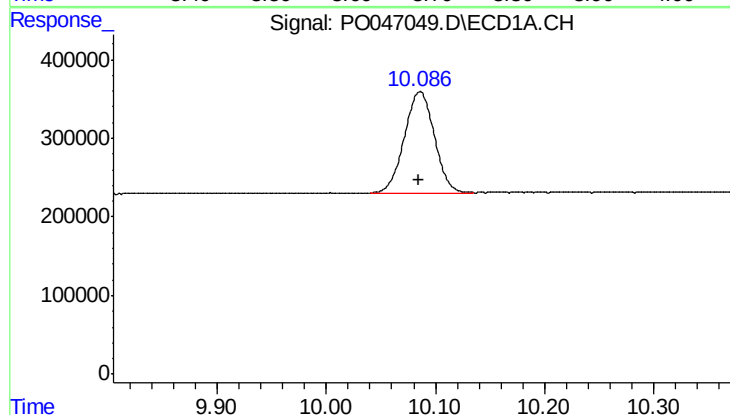


#2 Decachlorobiphenyl

R.T.: 10.086 min
Delta R.T.: 0.002 min
Response: 2445553
Conc: 22.34 ng/ml

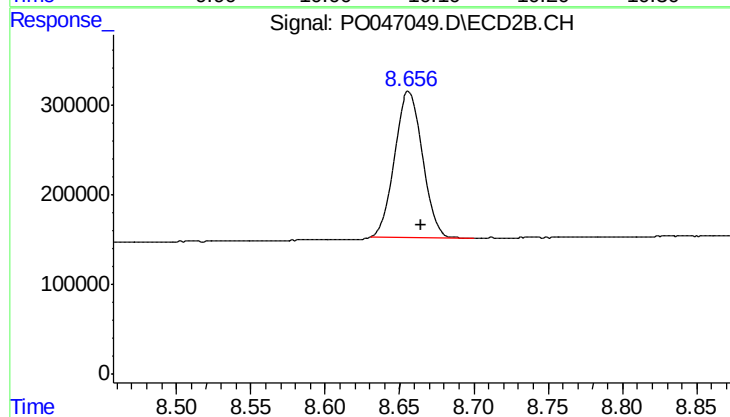

#2 Decachlorobiphenyl


R.T.: 8.656 min
Delta R.T.: -0.008 min
Response: 2133305
Conc: 23.23 ng/ml

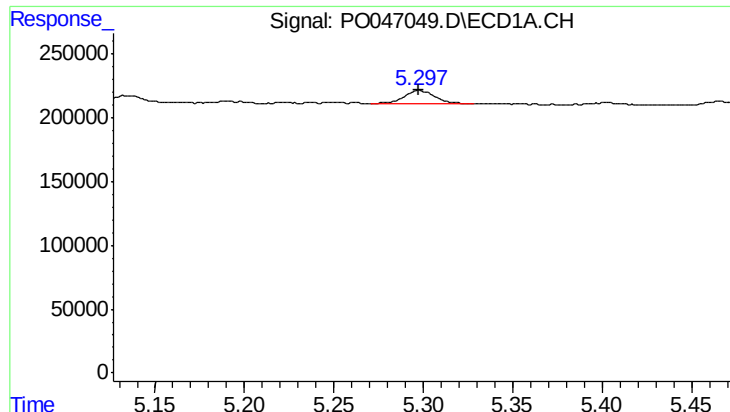

#3 AR-1016-1


R.T.: 5.298 min
Delta R.T.: 0.000 min
Response: 117953
Conc: 36.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

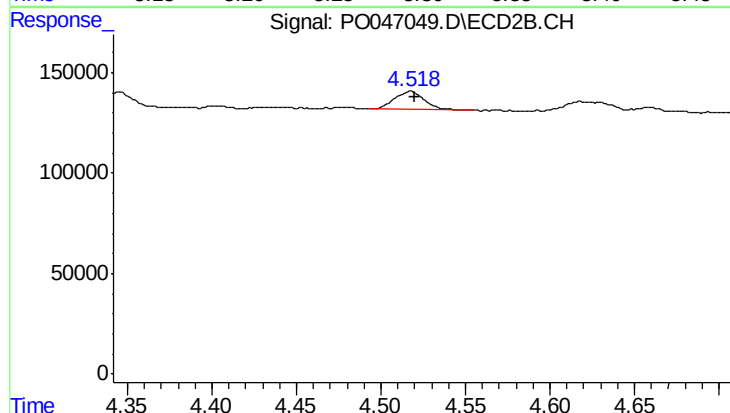


#3 AR-1016-1

R.T.: 4.517 min
Delta R.T.: -0.003 min
Response: 104925
Conc: 30.88 ng/ml

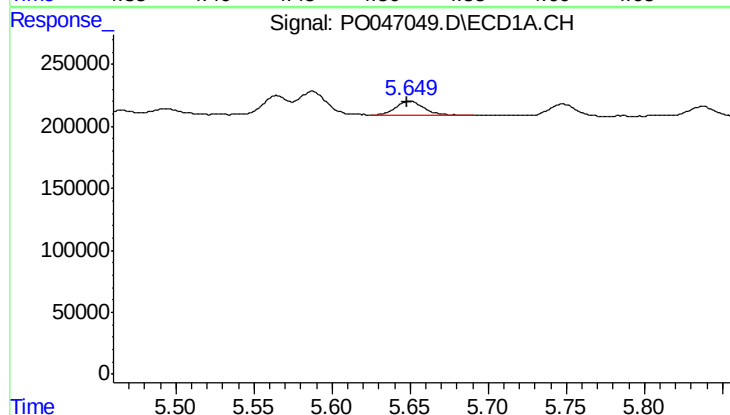


#4 AR-1016-2

R.T.: 5.650 min
Delta R.T.: 0.002 min
Response: 143618
Conc: 36.71 ng/ml

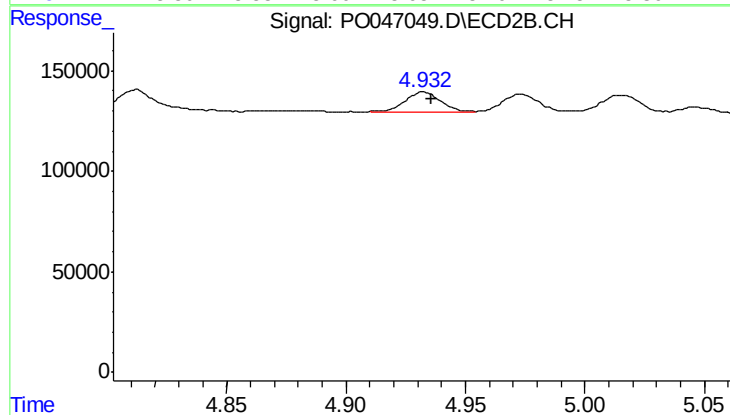

#4 AR-1016-2


R.T.: 4.933 min
Delta R.T.: -0.003 min
Response: 96440
Conc: 29.98 ng/ml

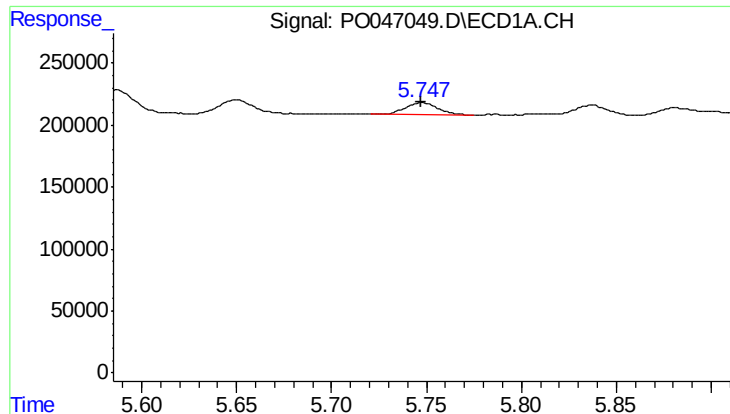

#5 AR-1016-3


R.T.: 5.748 min
Delta R.T.: 0.000 min
Response: 107462
Conc: 33.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

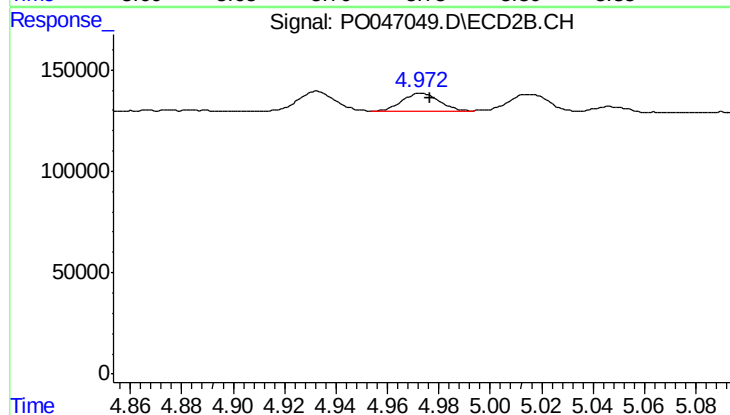


#5 AR-1016-3

R.T.: 4.973 min
Delta R.T.: -0.004 min
Response: 87364
Conc: 33.28 ng/ml

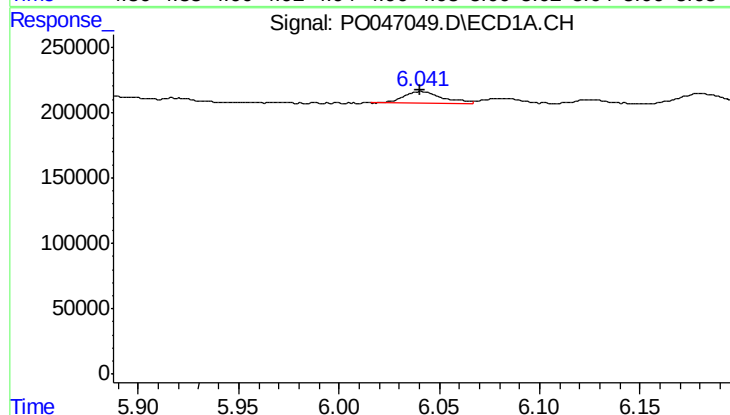


#6 AR-1016-4

R.T.: 6.041 min
Delta R.T.: 0.000 min
Response: 119184
Conc: 37.77 ng/ml

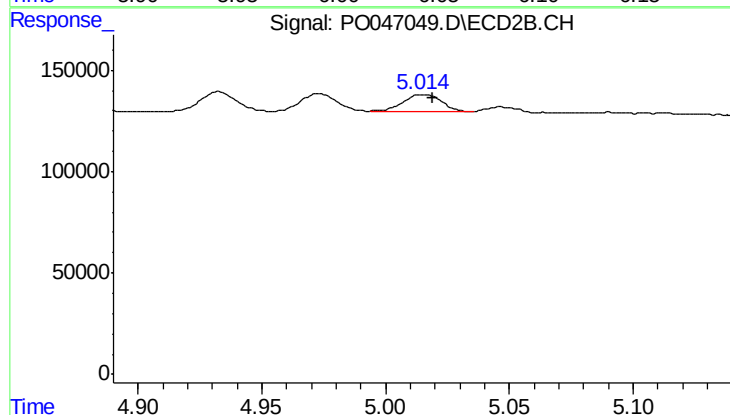

#6 AR-1016-4


R.T.: 5.015 min
Delta R.T.: -0.004 min
Response: 86944
Conc: 27.95 ng/ml

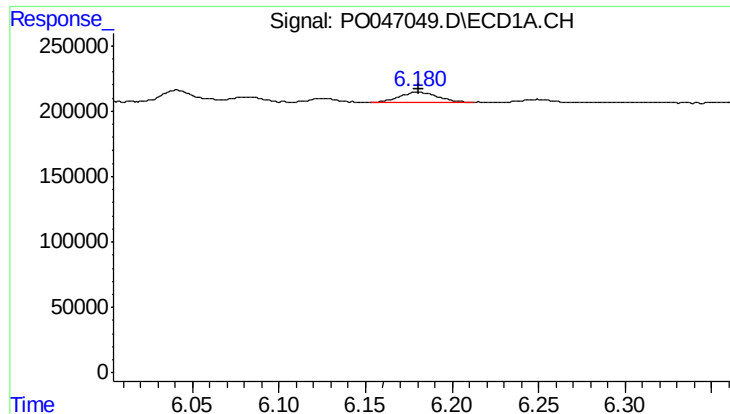

#7 AR-1016-5


R.T.: 6.180 min
Delta R.T.: 0.000 min
Response: 117550
Conc: 35.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

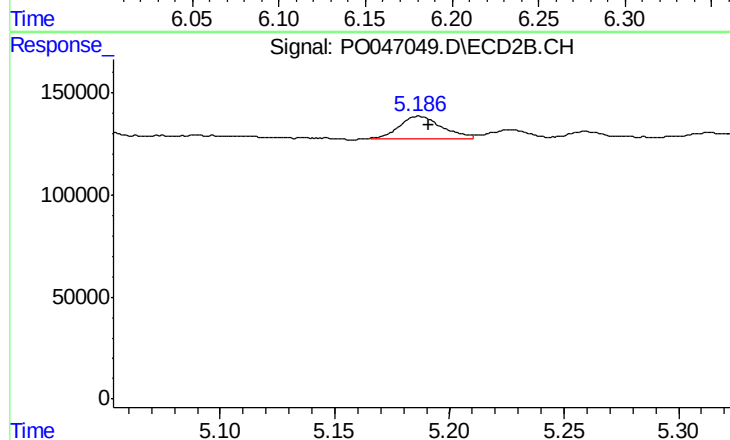


#7 AR-1016-5

R.T.: 5.187 min
Delta R.T.: -0.004 min
Response: 142402
Conc: 41.24 ng/ml

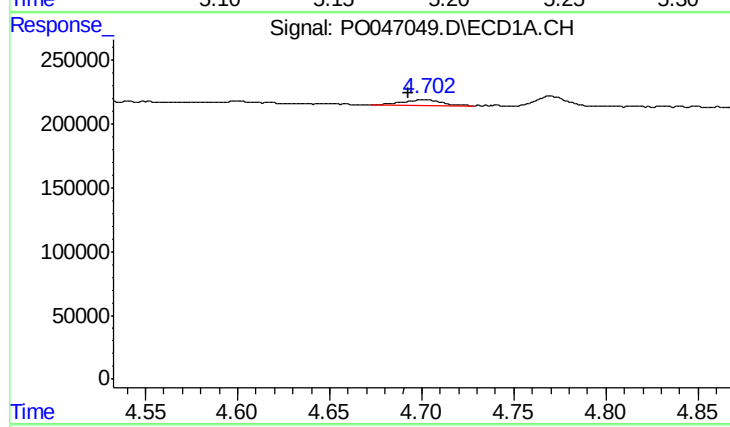


#9 AR-1221-2

R.T.: 4.703 min
Delta R.T.: 0.010 min
Response: 64602
Conc: 54.37 ng/ml

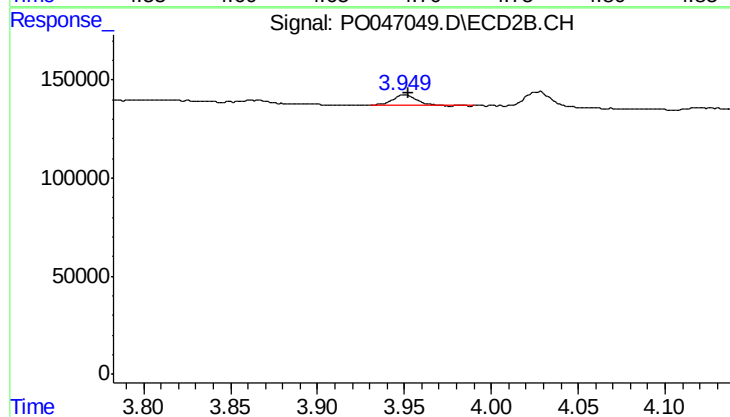

#9 AR-1221-2


R.T.: 3.950 min
Delta R.T.: -0.002 min
Response: 49985
Conc: 41.72 ng/ml

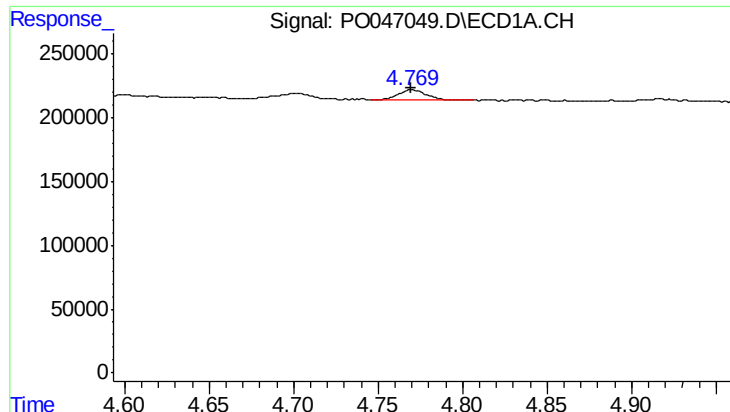

#10 AR-1221-3


R.T.: 4.770 min
Delta R.T.: 0.000 min
Response: 88648
Conc: 23.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

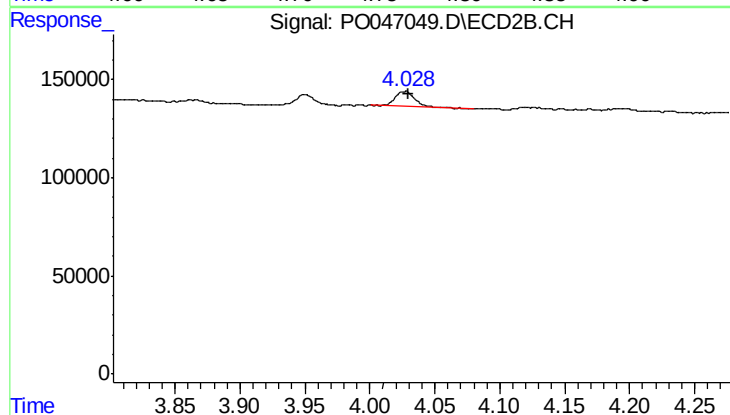


#10 AR-1221-3

R.T.: 4.027 min
Delta R.T.: -0.003 min
Response: 72069
Conc: 18.26 ng/ml

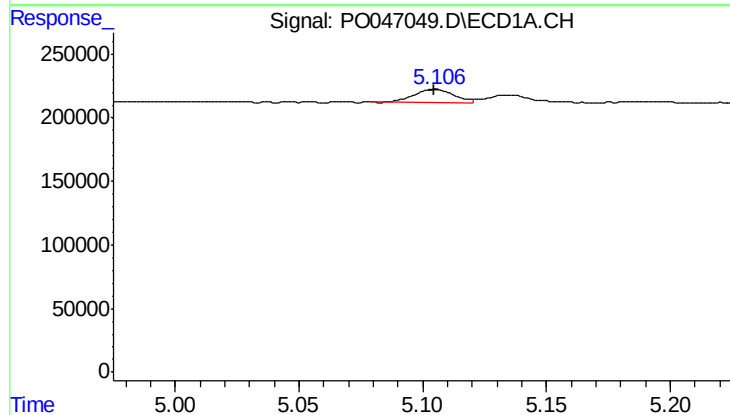


#11 AR-1232-1

R.T.: 5.105 min
Delta R.T.: 0.000 min
Response: 112714
Conc: 75.26 ng/ml

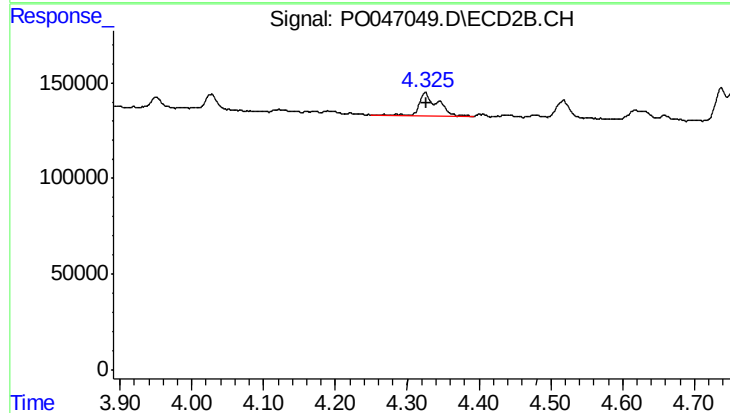

#11 AR-1232-1


R.T.: 4.325 min
Delta R.T.: -0.002 min
Response: 226332
Conc: 144.00 ng/ml

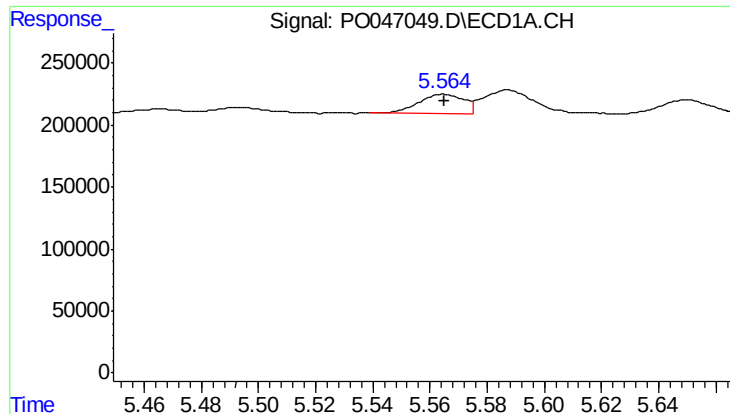

#12 AR-1232-2


R.T.: 5.565 min
Delta R.T.: 0.000 min
Response: 169884
Conc: 83.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

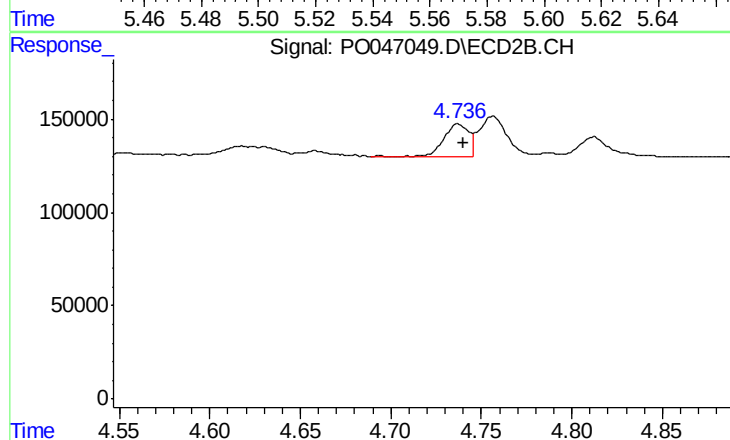


#12 AR-1232-2

R.T.: 4.737 min
Delta R.T.: -0.003 min
Response: 171481
Conc: 86.00 ng/ml

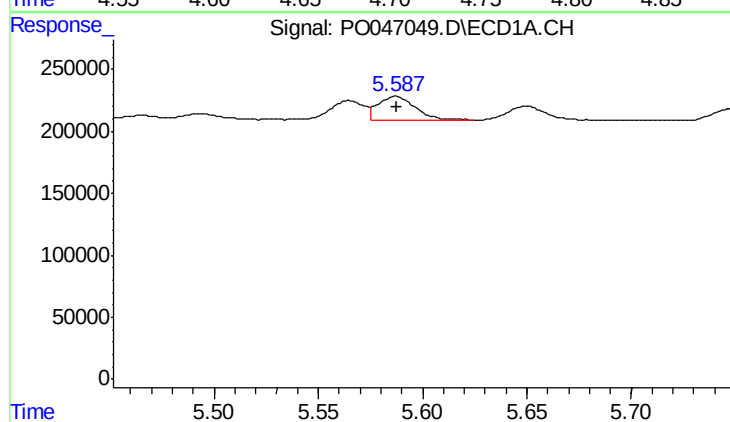


#13 AR-1232-3

R.T.: 5.587 min
Delta R.T.: 0.000 min
Response: 233341
Conc: 80.24 ng/ml

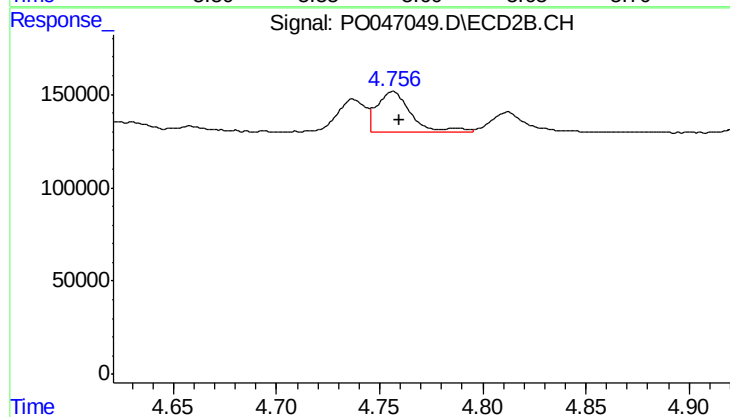

#13 AR-1232-3


R.T.: 4.756 min
Delta R.T.: -0.003 min
Response: 253787
Conc: 82.10 ng/ml

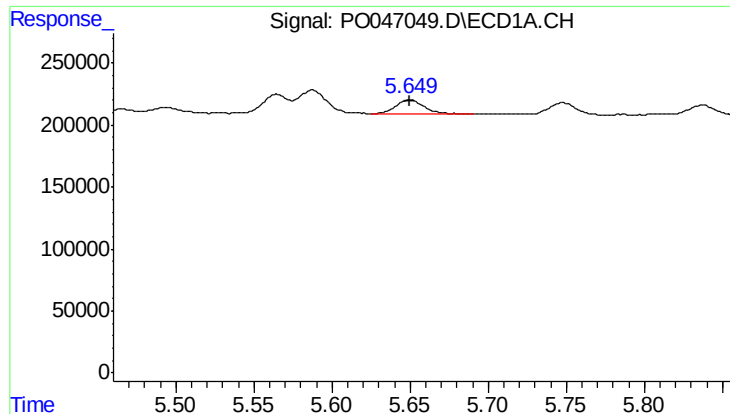

#14 AR-1232-4


R.T.: 5.650 min
Delta R.T.: 0.000 min
Response: 143618
Conc: 80.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

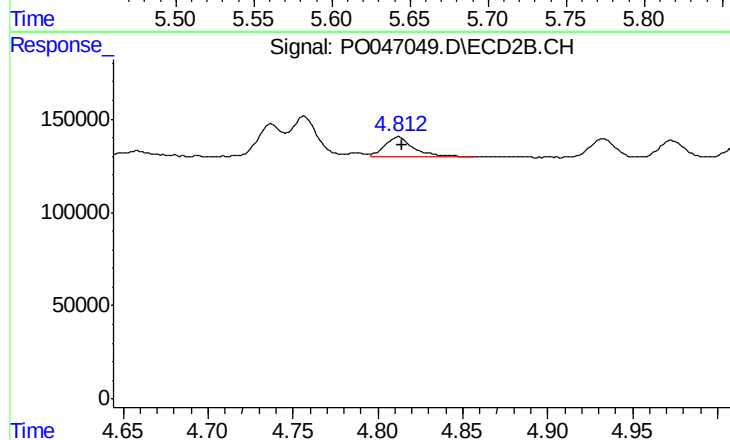


#14 AR-1232-4

R.T.: 4.812 min
Delta R.T.: -0.003 min
Response: 130605
Conc: 71.64 ng/ml

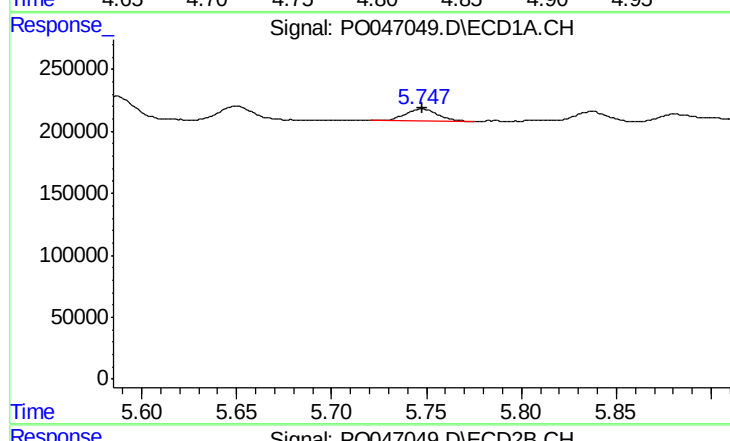


#15 AR-1232-5

R.T.: 5.748 min
Delta R.T.: 0.000 min
Response: 107462
Conc: 75.85 ng/ml

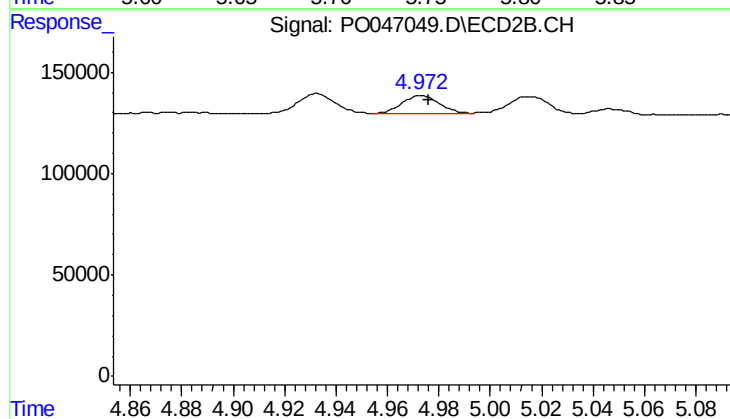

#15 AR-1232-5


R.T.: 4.973 min
Delta R.T.: -0.003 min
Response: 87364
Conc: 86.92 ng/ml

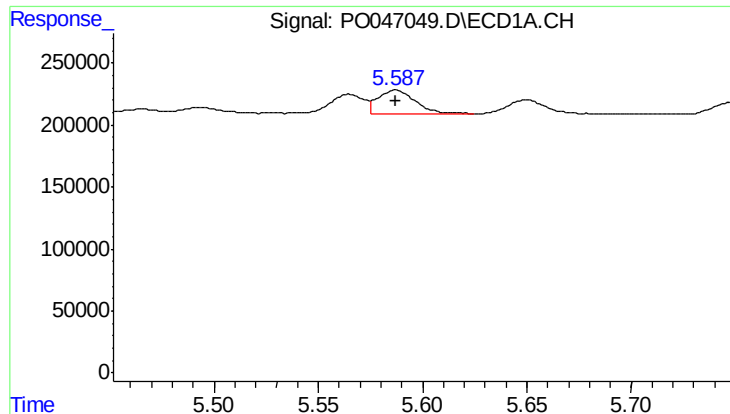

#16 AR-1242-1


R.T.: 5.587 min
Delta R.T.: 0.000 min
Response: 233341
Conc: 40.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

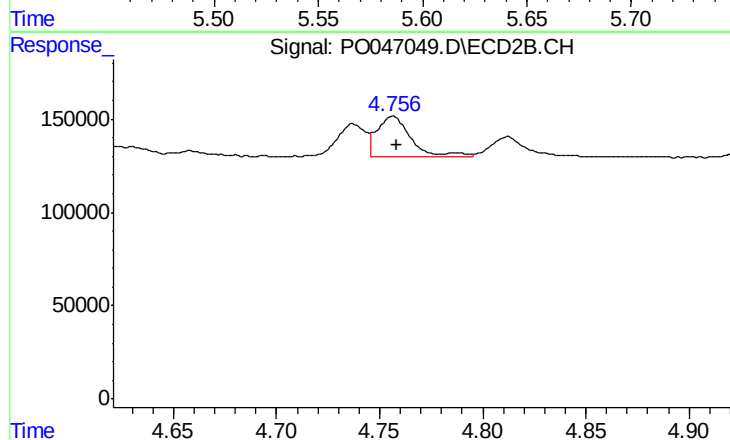


#16 AR-1242-1

R.T.: 4.756 min
Delta R.T.: -0.002 min
Response: 253787
Conc: 44.11 ng/ml

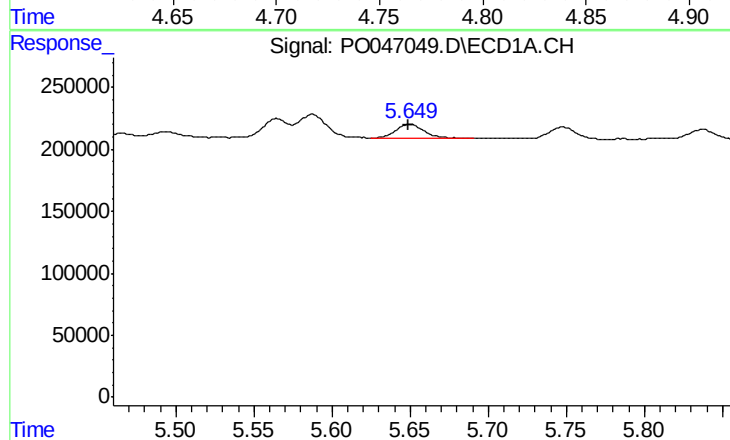


#17 AR-1242-2

R.T.: 5.650 min
Delta R.T.: 0.000 min
Response: 143618
Conc: 40.48 ng/ml

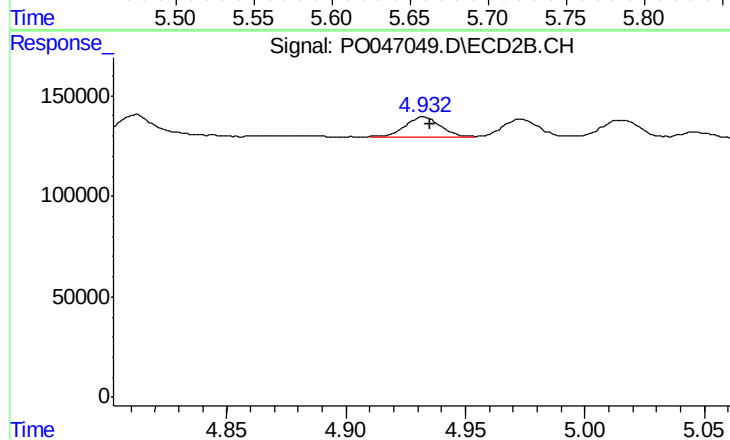

#17 AR-1242-2


R.T.: 4.933 min
Delta R.T.: -0.003 min
Response: 96440
Conc: 33.52 ng/ml

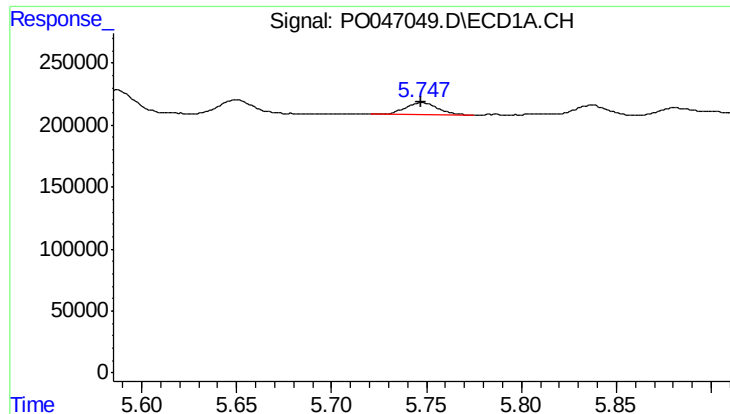

#18 AR-1242-3


R.T.: 5.748 min
Delta R.T.: 0.000 min
Response: 107462
Conc: 37.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

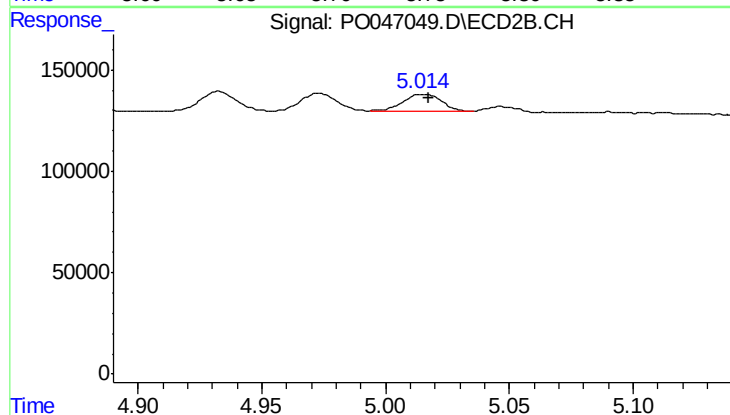


#18 AR-1242-3

R.T.: 5.015 min
Delta R.T.: -0.002 min
Response: 86944
Conc: 30.44 ng/ml

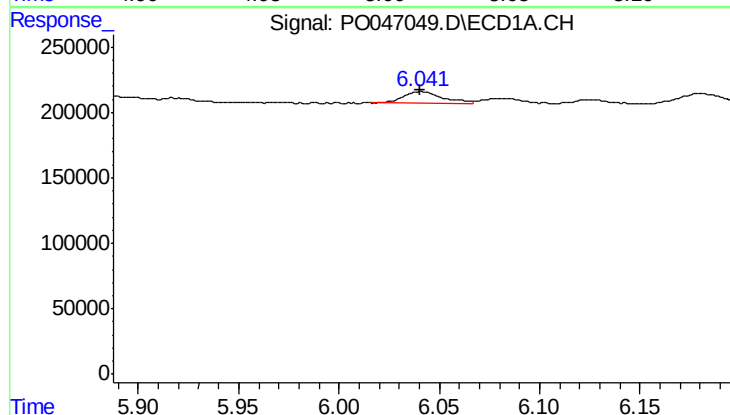


#19 AR-1242-4

R.T.: 6.041 min
Delta R.T.: 0.000 min
Response: 119184
Conc: 41.44 ng/ml

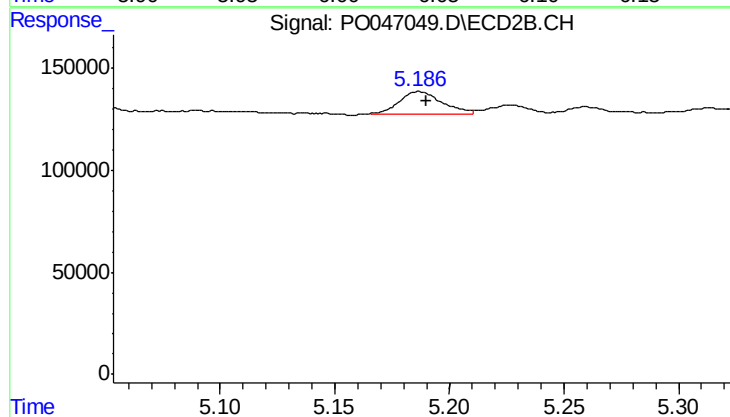

#19 AR-1242-4


R.T.: 5.187 min
Delta R.T.: -0.003 min
Response: 142402
Conc: 46.61 ng/ml

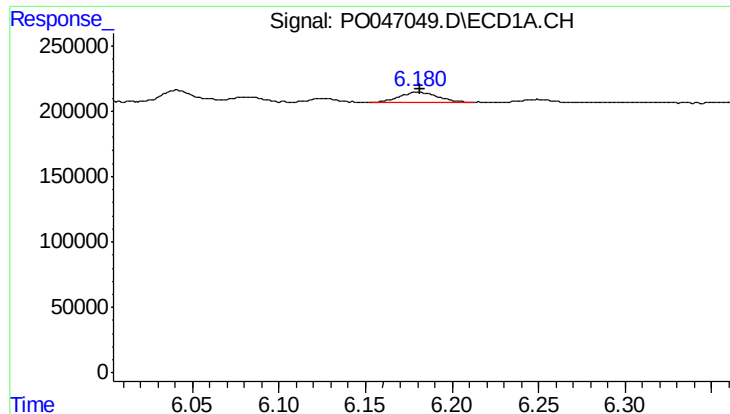

#20 AR-1242-5


R.T.: 6.180 min
Delta R.T.: -0.001 min
Response: 117550
Conc: 37.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

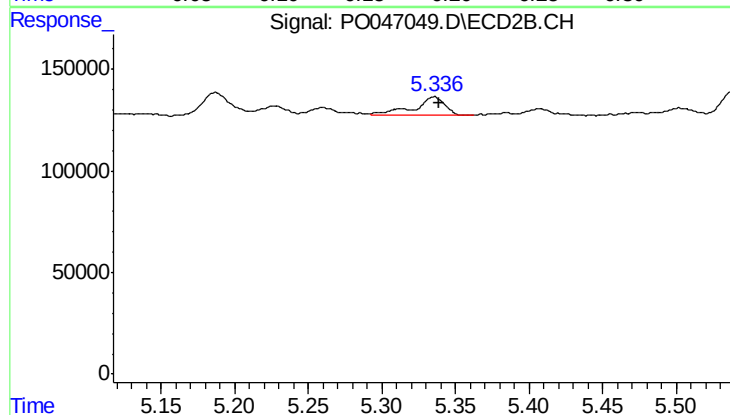


#20 AR-1242-5

R.T.: 5.335 min
Delta R.T.: -0.003 min
Response: 135555
Conc: 41.96 ng/ml

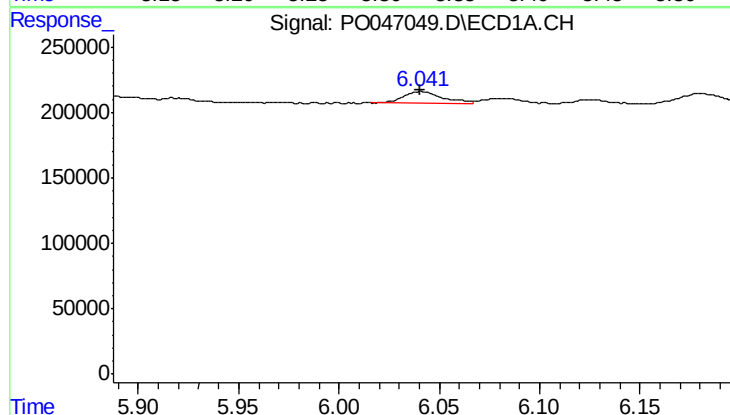


#21 AR-1248-1

R.T.: 6.041 min
Delta R.T.: 0.000 min
Response: 119184
Conc: 25.49 ng/ml

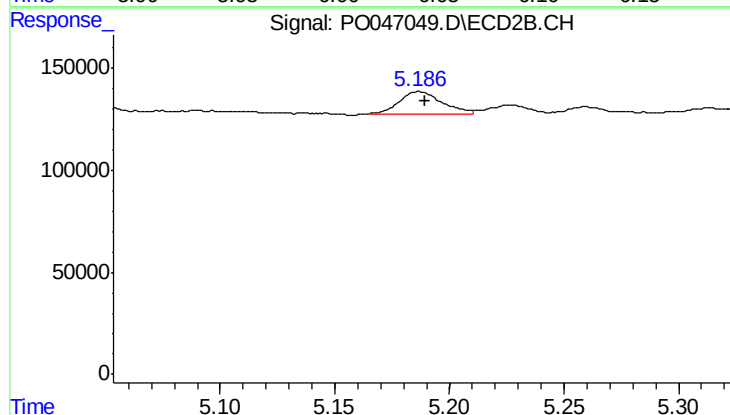

#21 AR-1248-1


R.T.: 5.187 min
Delta R.T.: -0.002 min
Response: 142402
Conc: 28.41 ng/ml

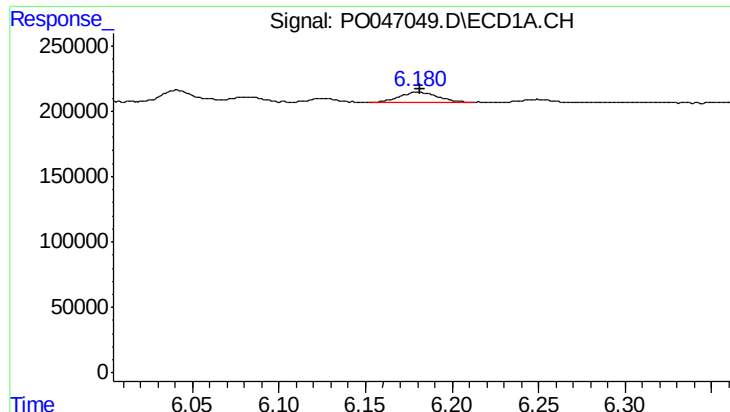

#22 AR-1248-2


R.T.: 6.180 min
Delta R.T.: -0.001 min
Response: 117550
Conc: 29.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

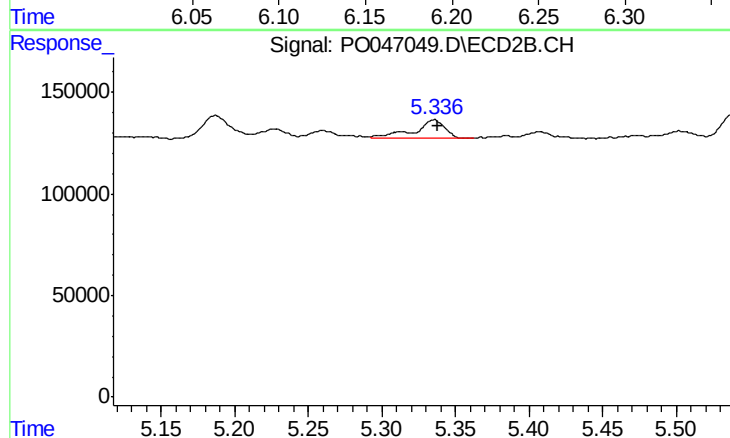


#22 AR-1248-2

R.T.: 5.335 min
Delta R.T.: -0.002 min
Response: 135555
Conc: 32.35 ng/ml

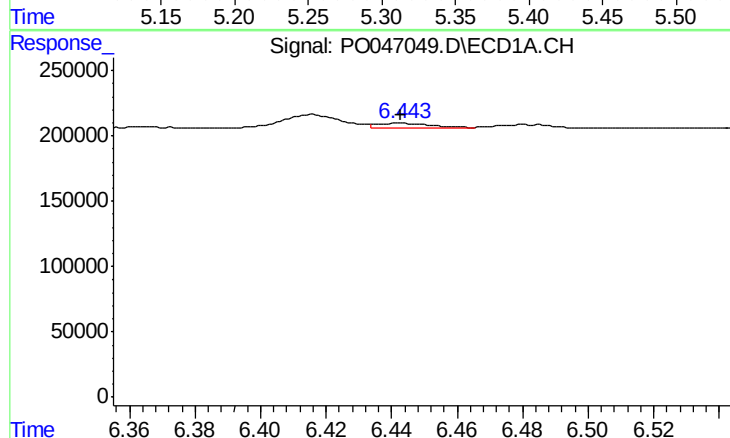


#23 AR-1248-3

R.T.: 6.442 min
Delta R.T.: 0.000 min
Response: 36235
Conc: 7.14 ng/ml

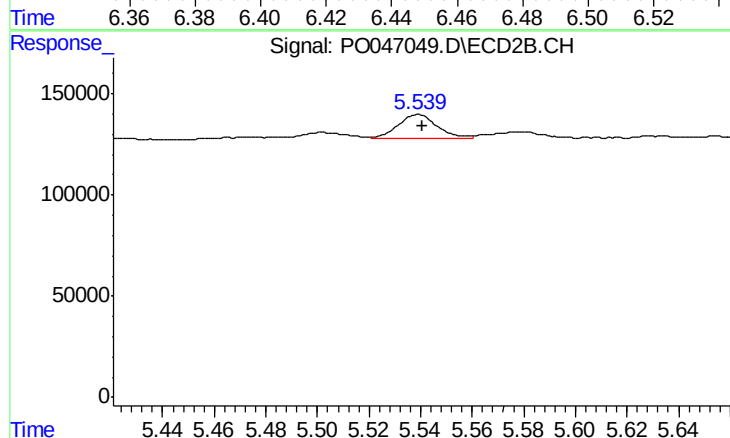

#23 AR-1248-3


R.T.: 5.539 min
Delta R.T.: -0.002 min
Response: 129841
Conc: 20.25 ng/ml

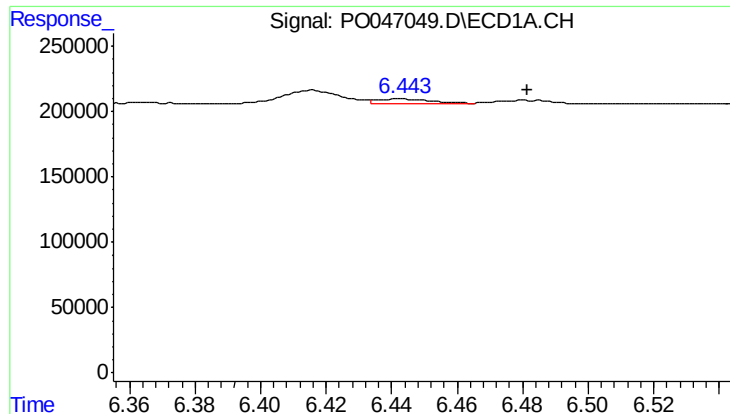

#24 AR-1248-4


R.T.: 6.442 min
Delta R.T.: -0.039 min
Response: 36235
Conc: 7.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

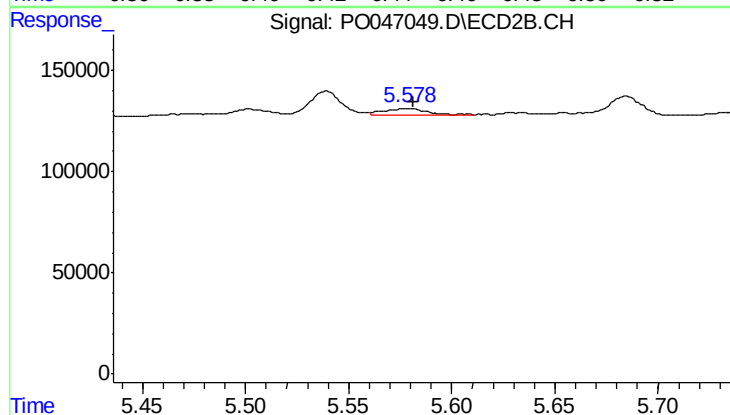


#24 AR-1248-4

R.T.: 5.579 min
Delta R.T.: -0.003 min
Response: 45819
Conc: 10.24 ng/ml

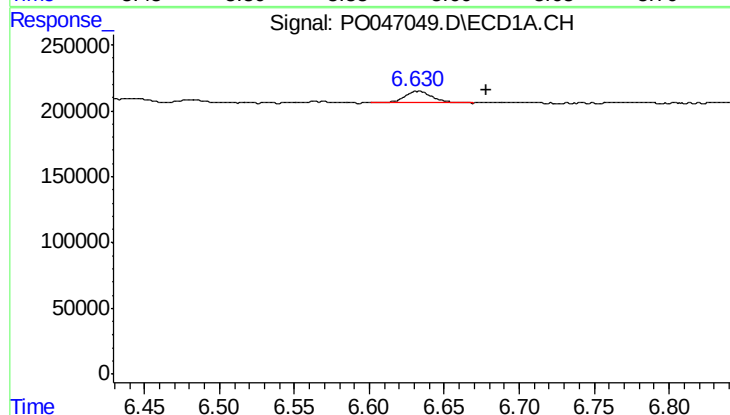


#25 AR-1248-5

R.T.: 6.633 min
Delta R.T.: -0.046 min
Response: 109813
Conc: 34.29 ng/ml

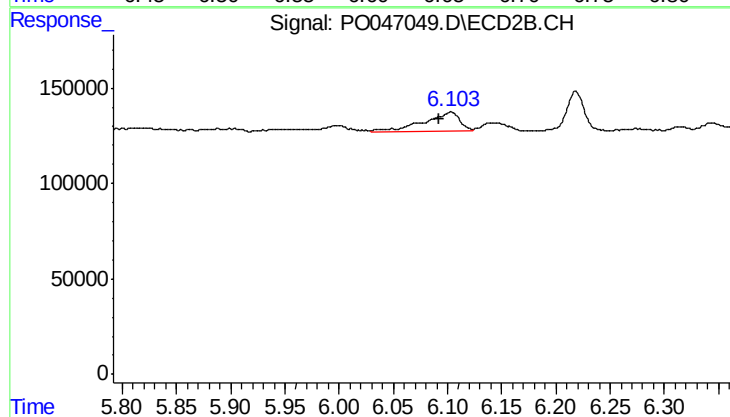

#25 AR-1248-5


R.T.: 6.103 min
Delta R.T.: 0.011 min
Response: 232503
Conc: 84.02 ng/ml

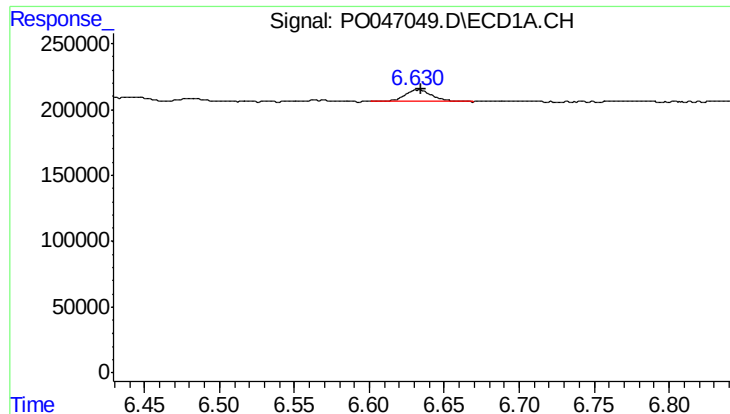

#26 AR-1254-1


R.T.: 6.633 min
Delta R.T.: -0.002 min
Response: 109813
Conc: 13.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

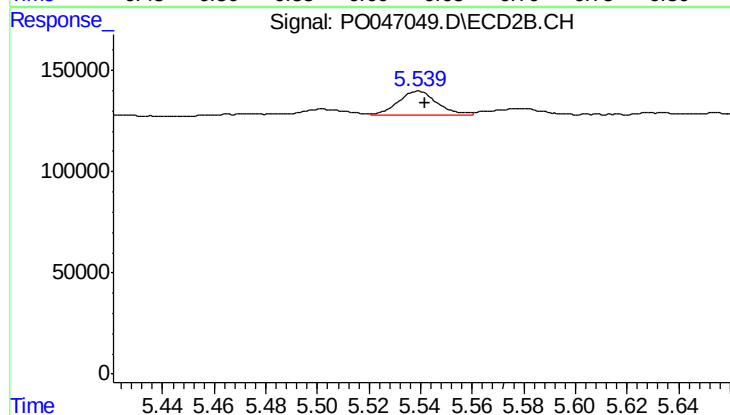


#26 AR-1254-1

R.T.: 5.539 min
Delta R.T.: -0.003 min
Response: 129841
Conc: 18.18 ng/ml

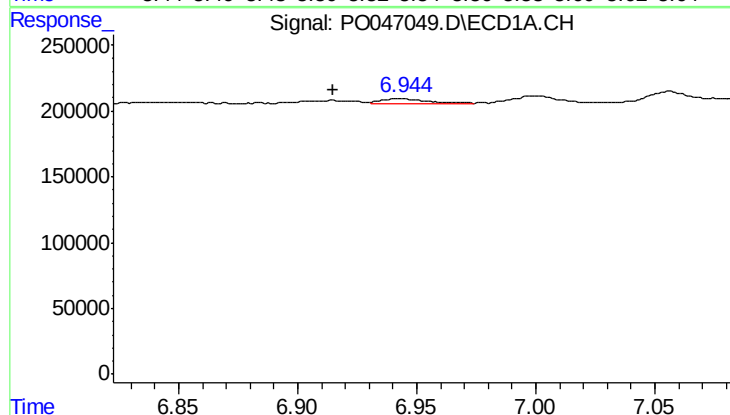


#27 AR-1254-2

R.T.: 6.944 min
Delta R.T.: 0.029 min
Response: 45552
Conc: 9.28 ng/ml

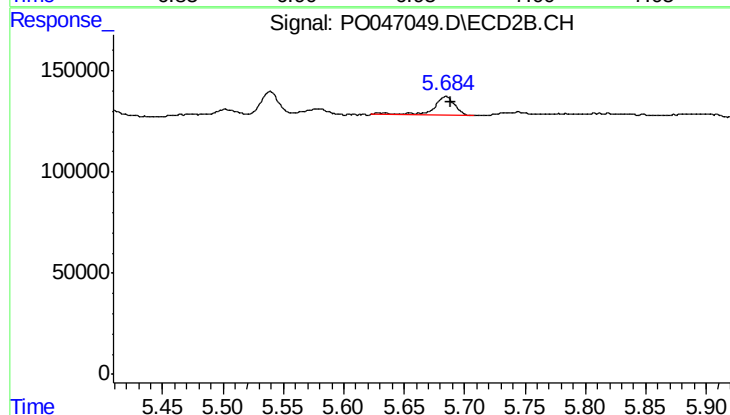

#27 AR-1254-2


R.T.: 5.684 min
Delta R.T.: -0.004 min
Response: 106650
Conc: 17.61 ng/ml

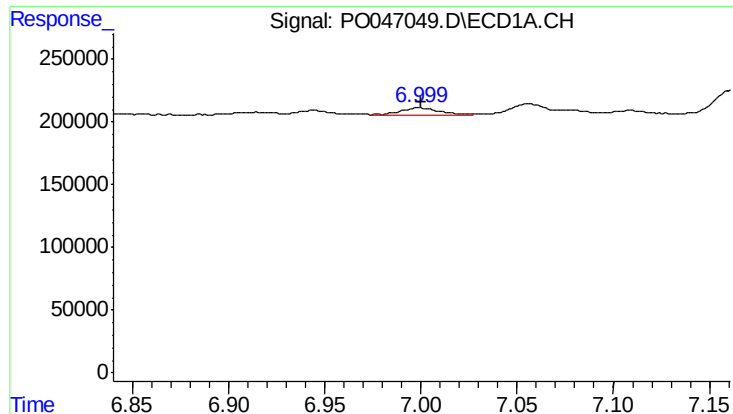

#28 AR-1254-3


R.T.: 6.999 min
Delta R.T.: 0.000 min
Response: 77856
Conc: 9.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

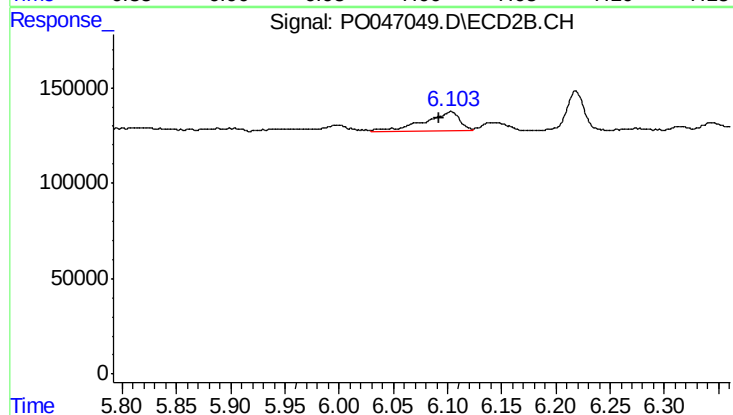


#28 AR-1254-3

R.T.: 6.103 min
Delta R.T.: 0.010 min
Response: 232503
Conc: 24.69 ng/ml

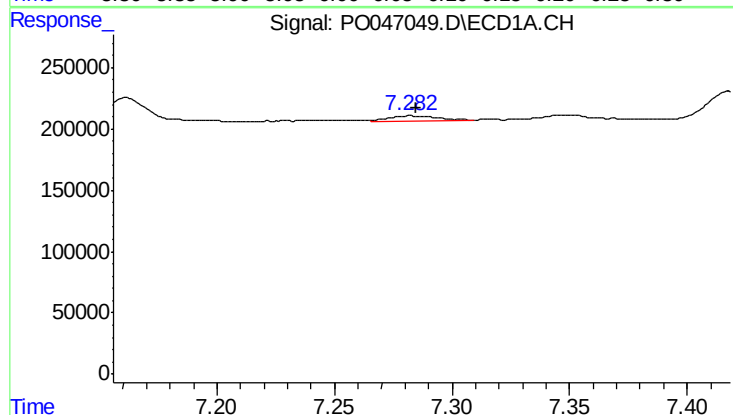


#29 AR-1254-4

R.T.: 7.282 min
Delta R.T.: -0.003 min
Response: 58223
Conc: 9.12 ng/ml

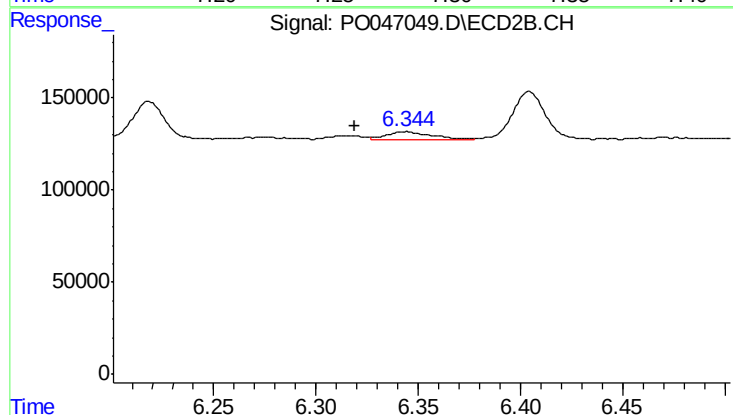

#29 AR-1254-4


R.T.: 6.344 min
Delta R.T.: 0.025 min
Response: 63115
Conc: 10.94 ng/ml

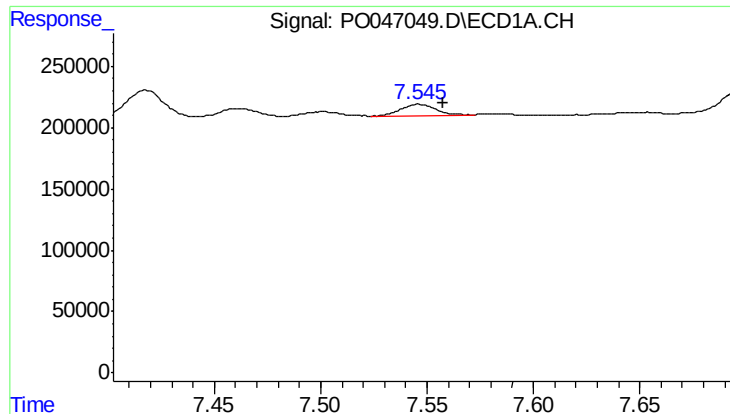

#30 AR-1254-5


R.T.: 7.546 min
Delta R.T.: -0.011 min
Response: 115057
Conc: 24.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

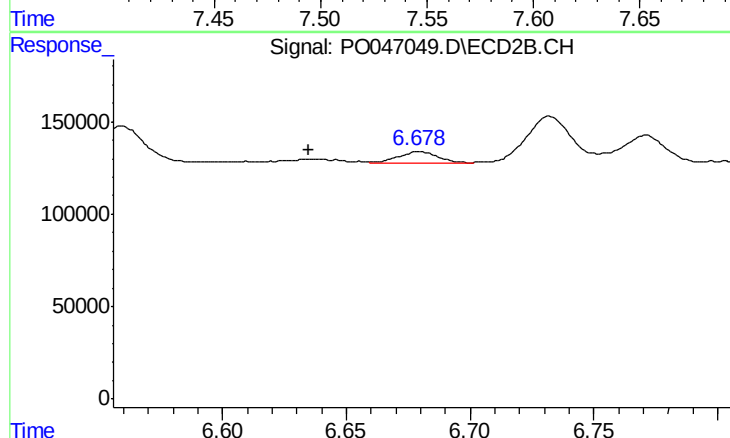


#30 AR-1254-5

R.T.: 6.680 min
Delta R.T.: 0.045 min
Response: 68461
Conc: 17.24 ng/ml

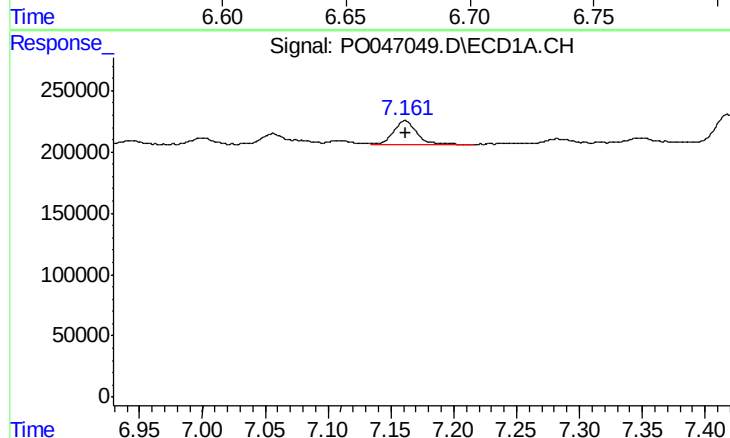


#31 AR-1260-1

R.T.: 7.161 min
Delta R.T.: 0.000 min
Response: 262249
Conc: 43.67 ng/ml

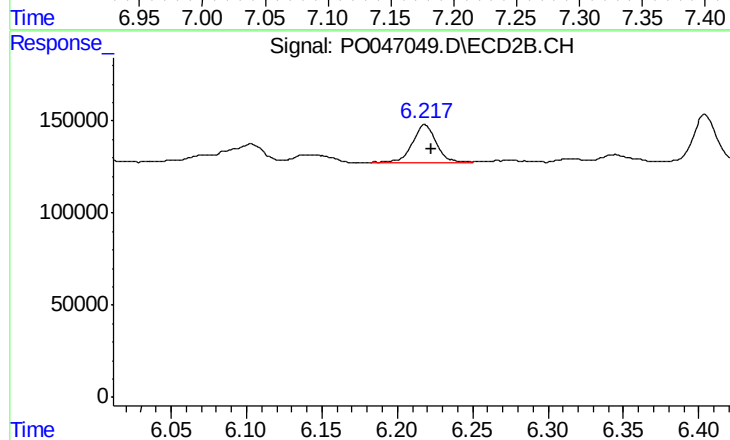

#31 AR-1260-1


R.T.: 6.218 min
Delta R.T.: -0.005 min
Response: 236153
Conc: 39.84 ng/ml

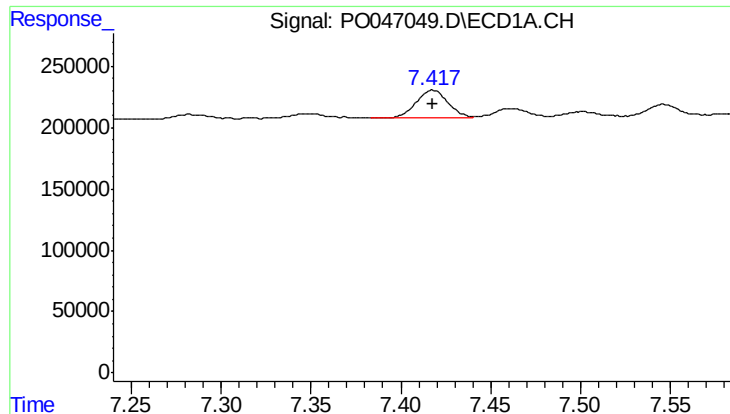

#32 AR-1260-2


R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 278232
Conc: 38.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

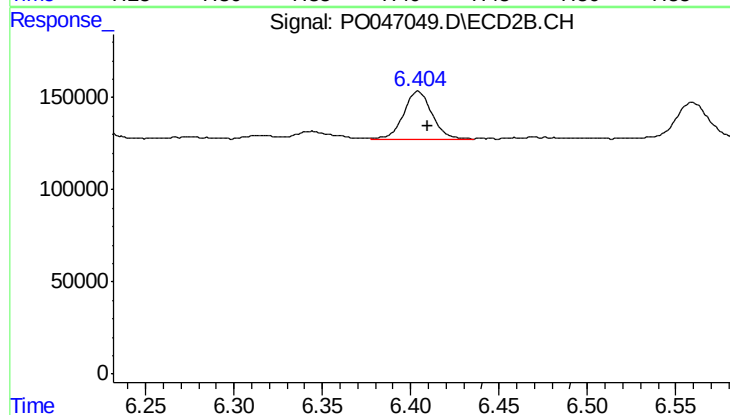


#32 AR-1260-2

R.T.: 6.404 min
Delta R.T.: -0.006 min
Response: 288699
Conc: 41.10 ng/ml

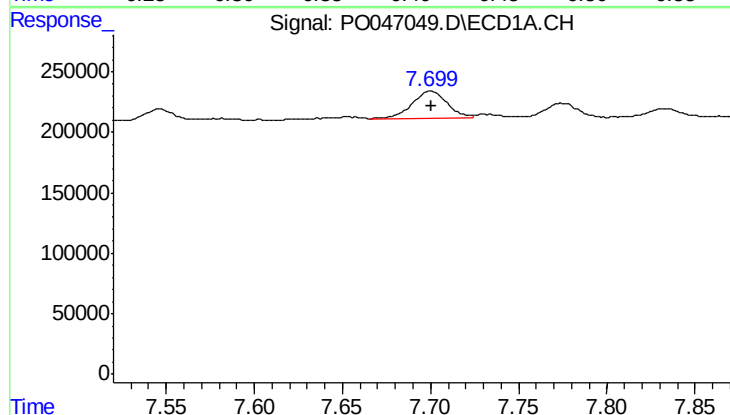


#33 AR-1260-3

R.T.: 7.700 min
Delta R.T.: 0.000 min
Response: 326386
Conc: 38.06 ng/ml

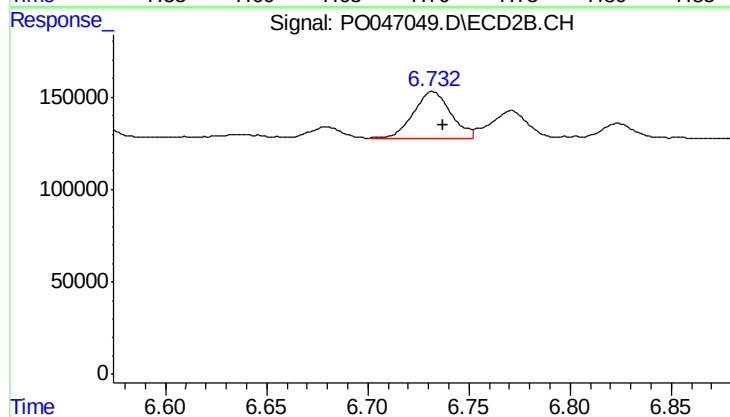

#33 AR-1260-3


R.T.: 6.732 min
Delta R.T.: -0.005 min
Response: 326734
Conc: 43.52 ng/ml

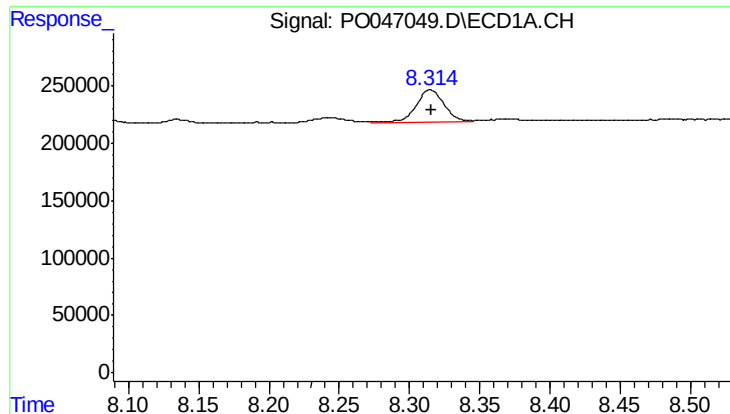

#34 AR-1260-4


R.T.: 8.315 min
Delta R.T.: 0.000 min
Response: 399332
Conc: 32.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

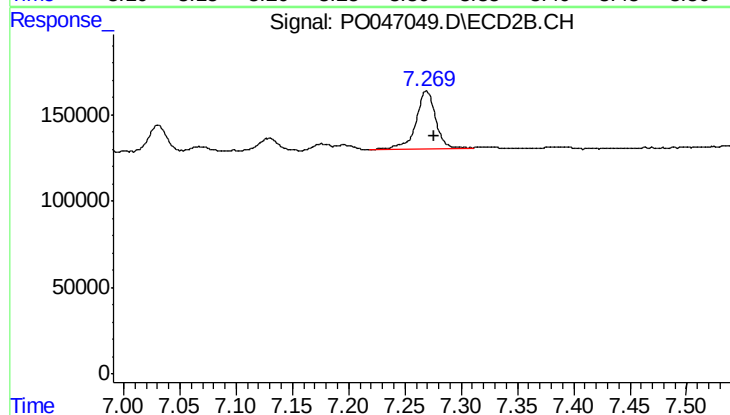


#34 AR-1260-4

R.T.: 7.269 min
Delta R.T.: -0.006 min
Response: 406981
Conc: 34.90 ng/ml

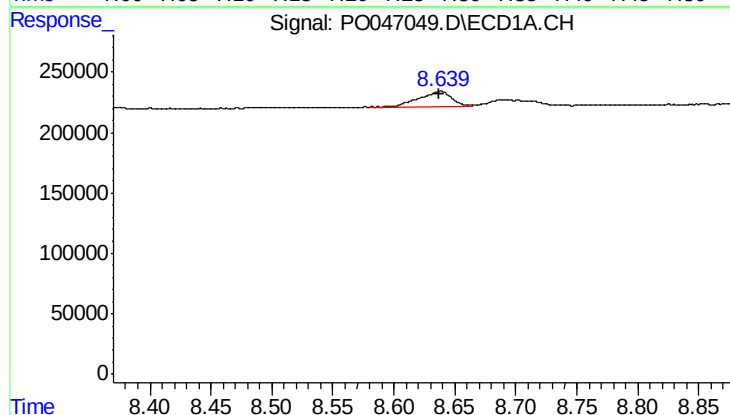


#35 AR-1260-5

R.T.: 8.638 min
Delta R.T.: 0.001 min
Response: 228055
Conc: 30.91 ng/ml

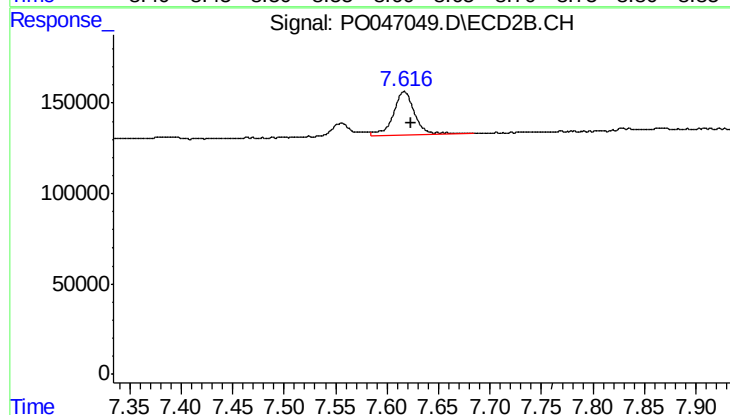

#35 AR-1260-5


R.T.: 7.617 min
Delta R.T.: -0.007 min
Response: 354045
Conc: 42.70 ng/ml

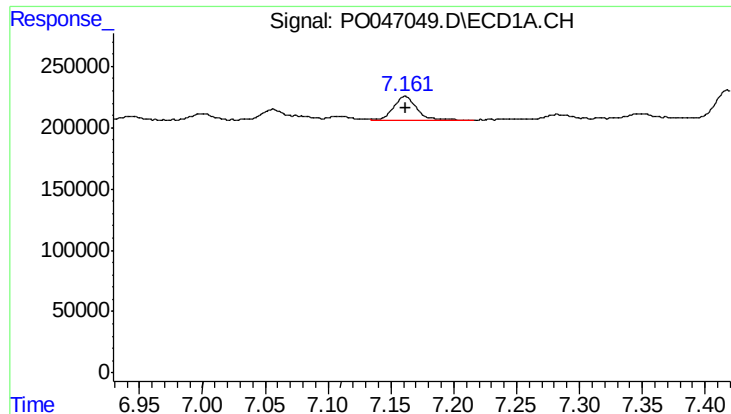

#36 AR-1262-1


R.T.: 7.161 min
Delta R.T.: 0.000 min
Response: 262249
Conc: 48.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

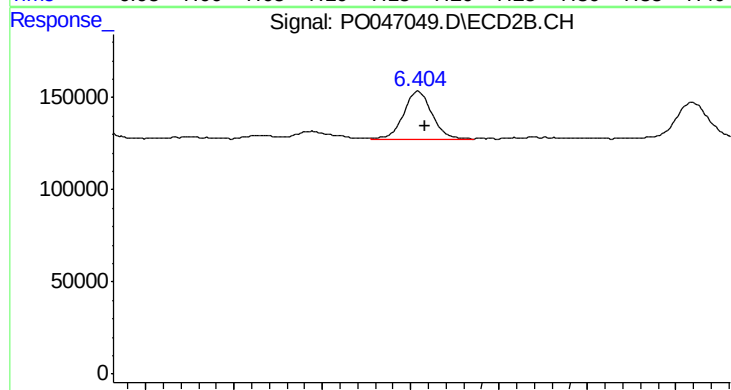


#36 AR-1262-1

R.T.: 6.404 min
Delta R.T.: -0.004 min
Response: 288699
Conc: 46.78 ng/ml

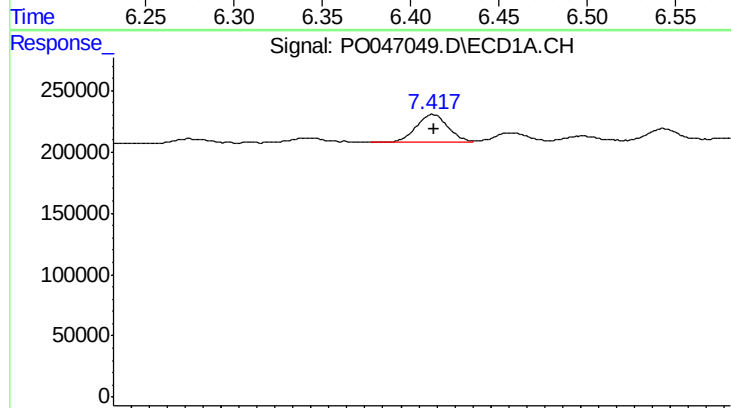


#37 AR-1262-2

R.T.: 7.418 min
Delta R.T.: -0.001 min
Response: 278232
Conc: 43.22 ng/ml

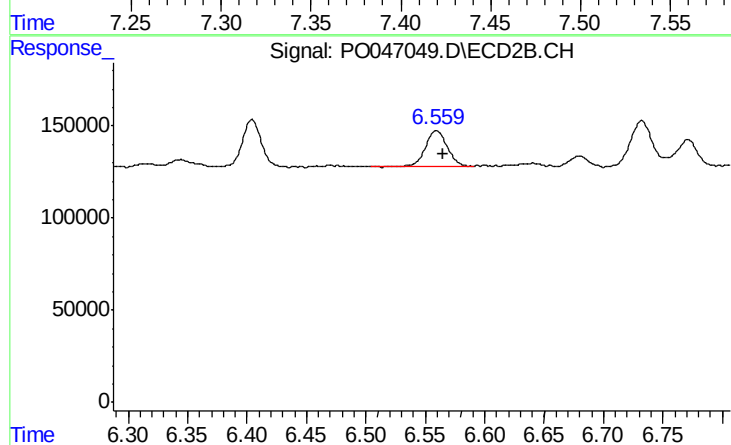

#37 AR-1262-2


R.T.: 6.559 min
Delta R.T.: -0.006 min
Response: 260427
Conc: 42.55 ng/ml

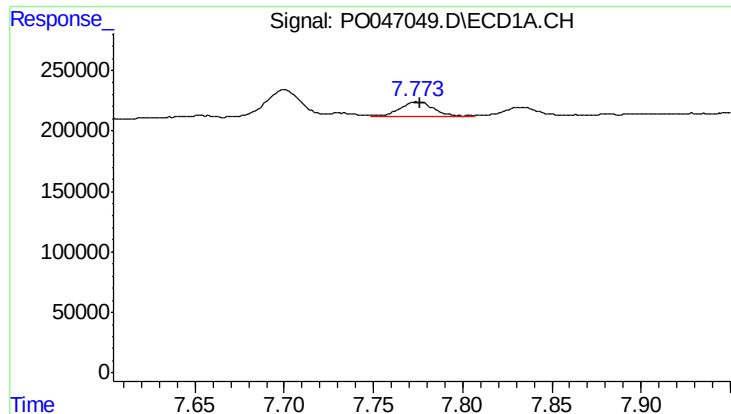

#38 AR-1262-3


R.T.: 7.774 min
Delta R.T.: -0.002 min
Response: 159763
Conc: 19.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

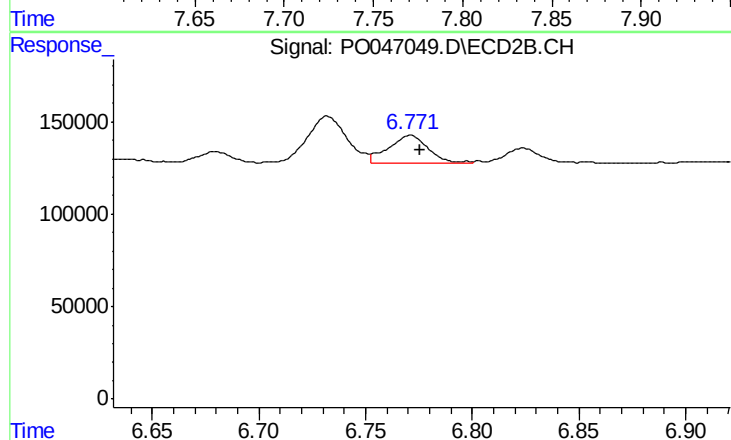


#38 AR-1262-3

R.T.: 6.771 min
Delta R.T.: -0.004 min
Response: 195935
Conc: 24.07 ng/ml

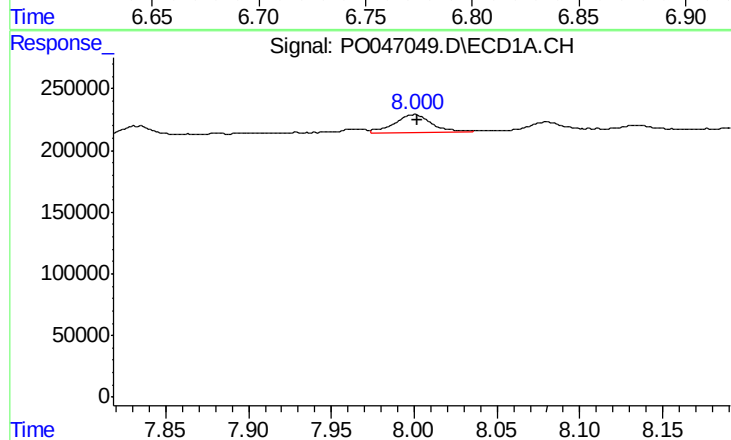


#39 AR-1262-4

R.T.: 8.000 min
Delta R.T.: -0.001 min
Response: 229173
Conc: 28.69 ng/ml

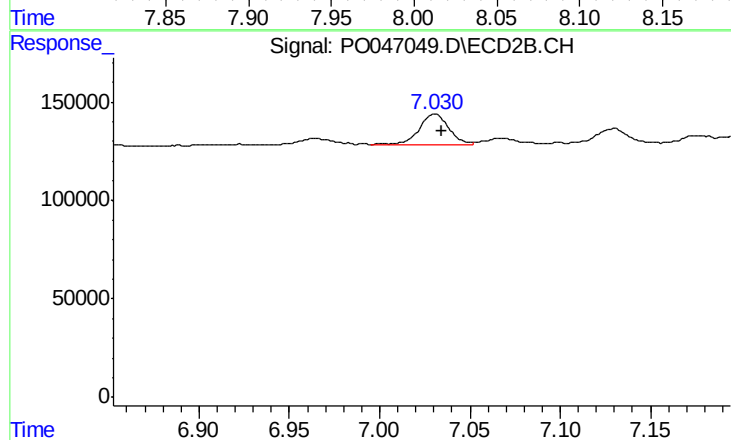

#39 AR-1262-4


R.T.: 7.031 min
Delta R.T.: -0.004 min
Response: 176731
Conc: 24.90 ng/ml

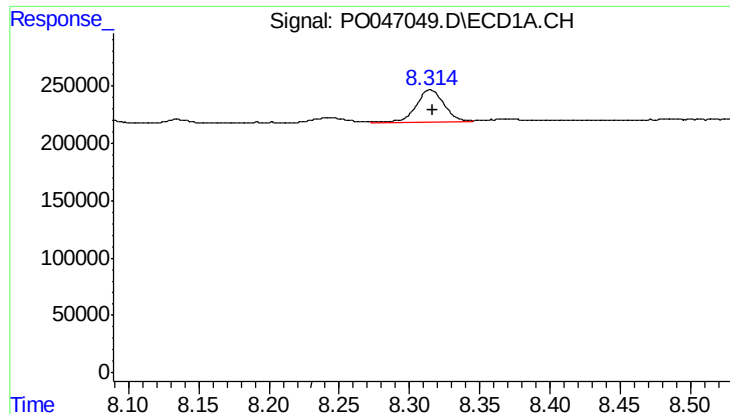

#40 AR-1262-5


R.T.: 8.315 min
Delta R.T.: -0.002 min
Response: 399332
Conc: 26.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

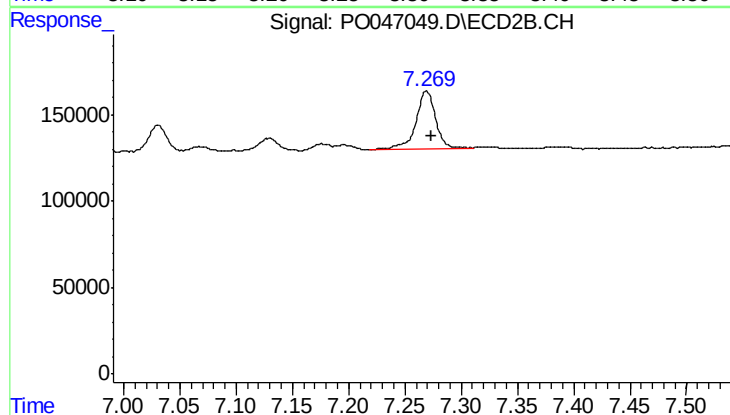


#40 AR-1262-5

R.T.: 7.269 min
Delta R.T.: -0.004 min
Response: 406981
Conc: 29.08 ng/ml

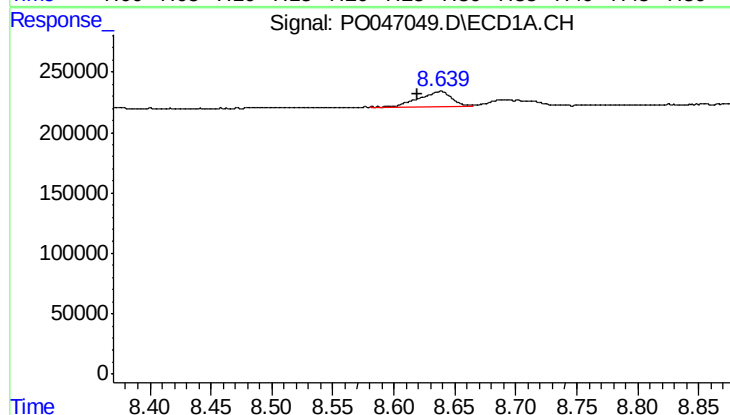


#41 AR-1268-1

R.T.: 8.638 min
Delta R.T.: 0.019 min
Response: 228055
Conc: 14.56 ng/ml

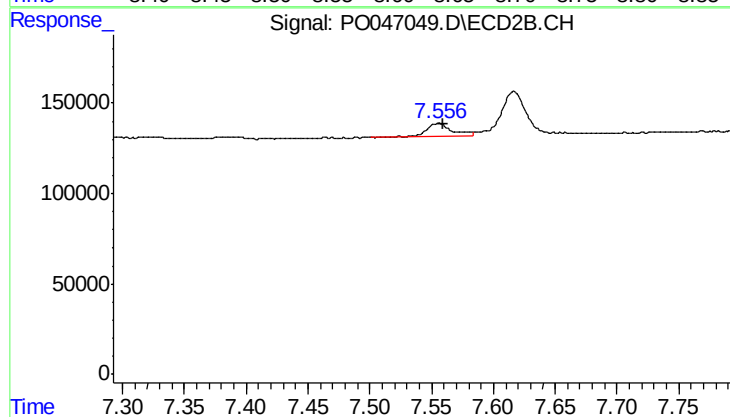

#41 AR-1268-1


R.T.: 7.555 min
Delta R.T.: -0.003 min
Response: 103890
Conc: 7.62 ng/ml

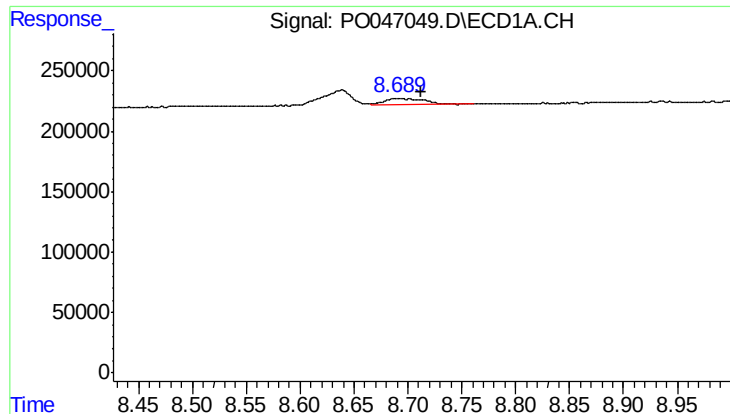

#42 AR-1268-2


R.T.: 8.691 min
Delta R.T.: -0.022 min
Response: 119889
Conc: 8.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

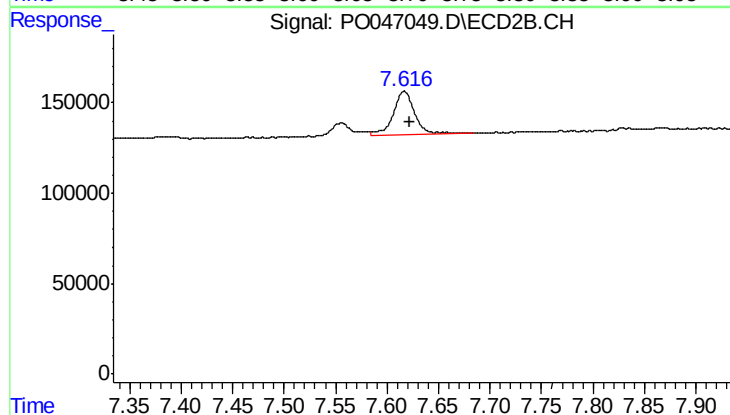


#42 AR-1268-2

R.T.: 7.617 min
Delta R.T.: -0.006 min
Response: 354045
Conc: 28.21 ng/ml

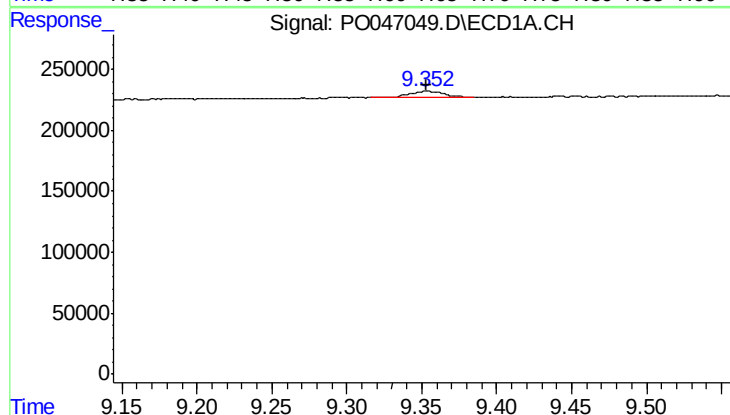


#44 AR-1268-4

R.T.: 9.354 min
Delta R.T.: 0.000 min
Response: 82233
Conc: 16.27 ng/ml

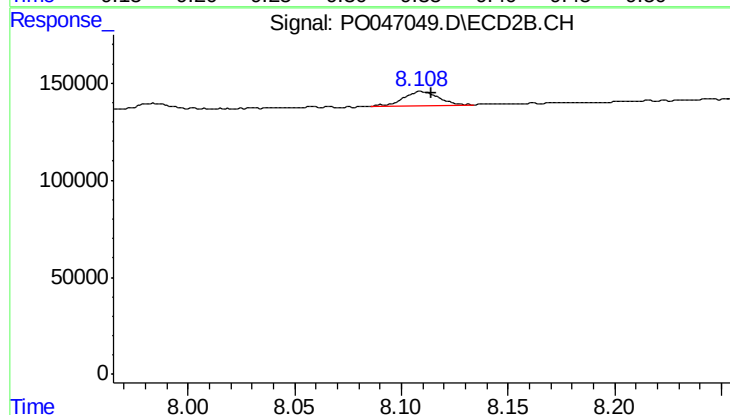

#44 AR-1268-4


R.T.: 8.110 min
Delta R.T.: -0.004 min
Response: 82703
Conc: 18.88 ng/ml

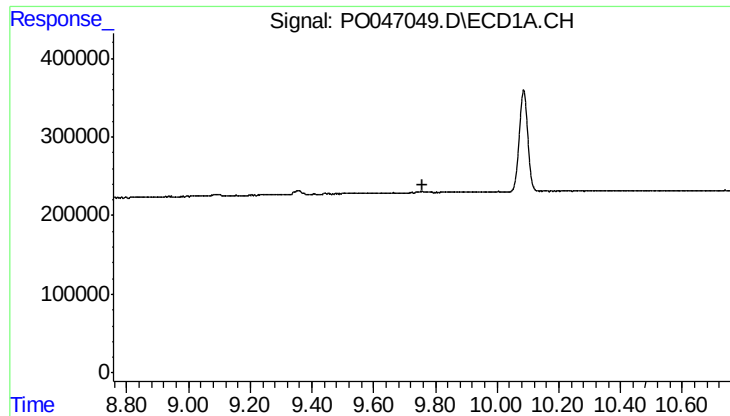

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.756 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT3-2018

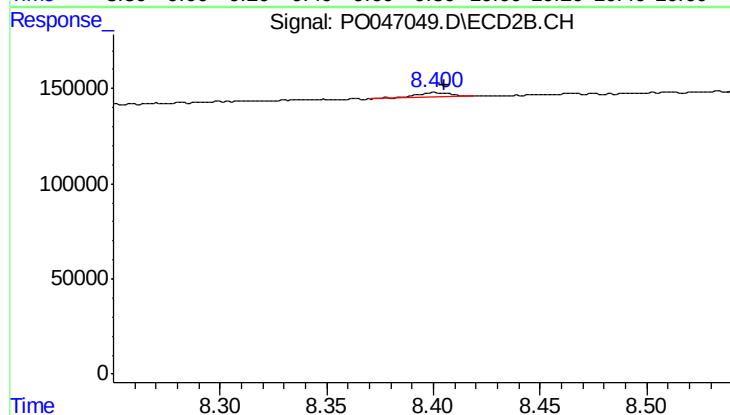

#45 AR-1268-5

R.T.: 8.402 min
Delta R.T.: -0.004 min
Response: 30940
Conc: 1.03 ng/ml