

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072318\
 Data File : P0047051.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jul 2018 1:31
 Operator : SM/SJ
 Sample : J3762-09
 Misc : ECD_0 MDL WATER 25 PPB
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 MDL-WATER-03-QT3-2018

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 06:02:43 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 24 03:04:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.397	3.649	3269634	3652668	19.501	19.044
2) SA Decachlor...	10.086	8.656	2428813	2103406	22.186	22.903
Target Compounds						
3) L1 AR-1016-1	5.298	4.517	114020	110267	35.054	32.457
4) L1 AR-1016-2	5.649	4.932	142655	96772	36.468	30.080
5) L1 AR-1016-3	5.747	4.972	106757	94024	33.160	35.815
6) L1 AR-1016-4	6.041	5.014	129016	104028	40.888	33.441
7) L1 AR-1016-5	6.180	5.186	108588	132366	32.877	38.331
9) L2 AR-1221-2	4.702	3.950	61898	56235	52.096	46.934
10) L2 AR-1221-3	4.769	4.027	84335	77571	22.749	19.650
11) L3 AR-1232-1	5.104	4.325	116551	196698	77.820	125.143 #
12) L3 AR-1232-2	5.564	4.737	165675	163315	81.309	81.903
13) L3 AR-1232-3	5.586	4.755	224527	260895	77.209	84.399
14) L3 AR-1232-4	5.649	4.811	142655	139600	79.951	76.570
15) L3 AR-1232-5	5.747	4.972	106757	94024	75.354	93.549
16) L4 AR-1242-1	5.586	4.755	224527	260895	38.736	45.346
17) L4 AR-1242-2	5.649	4.932	142655	96772	40.213	33.638
18) L4 AR-1242-3	5.747	5.014	106757	104028	37.623	36.416
19) L4 AR-1242-4	6.041	5.186	129016	132366	44.862	43.324
20) L4 AR-1242-5	6.180	5.335	108588	138610	35.054	42.905
21) L5 AR-1248-1	6.041	5.186	129016	132366	27.592	26.405
22) L5 AR-1248-2	6.180	5.335	108588	138610	27.398	33.075
23) L5 AR-1248-3	6.444	5.537	39236	131356	7.728	20.491 #
24) L5 AR-1248-4	6.444	5.578	39236	56269	8.214	12.572 #
25) L5 AR-1248-5	6.633	6.102	101983	250706	31.845	90.599 #
26) L6 AR-1254-1	6.633	5.537	101983	131356	12.403	18.388 #
27) L6 AR-1254-2	6.913	5.684	37307	131137	7.598	21.650 #
28) L6 AR-1254-3	7.000	6.102	75301	250706	8.762	26.628 #
29) L6 AR-1254-4	7.284	6.313	91237	26304	14.286	4.561 #
30) L6 AR-1254-5	7.546	6.680	126009	71279	26.537	17.954 #
31) L7 AR-1260-1	7.162	6.217	250743	249384	41.752	42.071
32) L7 AR-1260-2	7.418	6.403	284079	285763	38.872	40.687
33) L7 AR-1260-3	7.700	6.731	334742	336987	39.038	44.886
34) L7 AR-1260-4	8.315	7.269	377869	409146	31.214	35.084
35) L7 AR-1260-5	8.636	7.616	241301	312816	32.710	37.724
36) L8 AR-1262-1	7.162	6.403	250743	285763	46.588	46.306
37) L8 AR-1262-2	7.418	6.558	284079	259431	44.132	42.384
38) L8 AR-1262-3	7.775	6.769	166628	193884	20.192	23.823
39) L8 AR-1262-4	8.000	7.030	233196	184836	29.191	26.041

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072318\
Data File : P0047051.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jul 2018 1:31
Operator : SM/SJ
Sample : J3762-09
Misc : ECD_0 MDL WATER 25 PPB
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_0
ClientSampleId :
MDL-WATER-03-QT3-2018

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 06:02:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 24 03:04:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
40)	L8 AR-1262-5	8.315	7.269	377869	409146	25.363	29.231
41)	L9 AR-1268-1	8.636	7.554	241301	75823	15.406	5.565 #
42)	L9 AR-1268-2	8.688	7.616	136578	312816	9.746	24.924 #
44)	L9 AR-1268-4	9.355	8.109	66076	75827	13.076	17.312 #
45)	L9 AR-1268-5	0.000	8.400	0	33222	N.D.	1.107 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072318\
Data File : P0047051.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jul 2018 1:31
Operator : SM/SJ
Sample : J3762-09
Misc : ECD_O MDL WATER 25 PPB
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 06:02:43 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 24 03:04:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

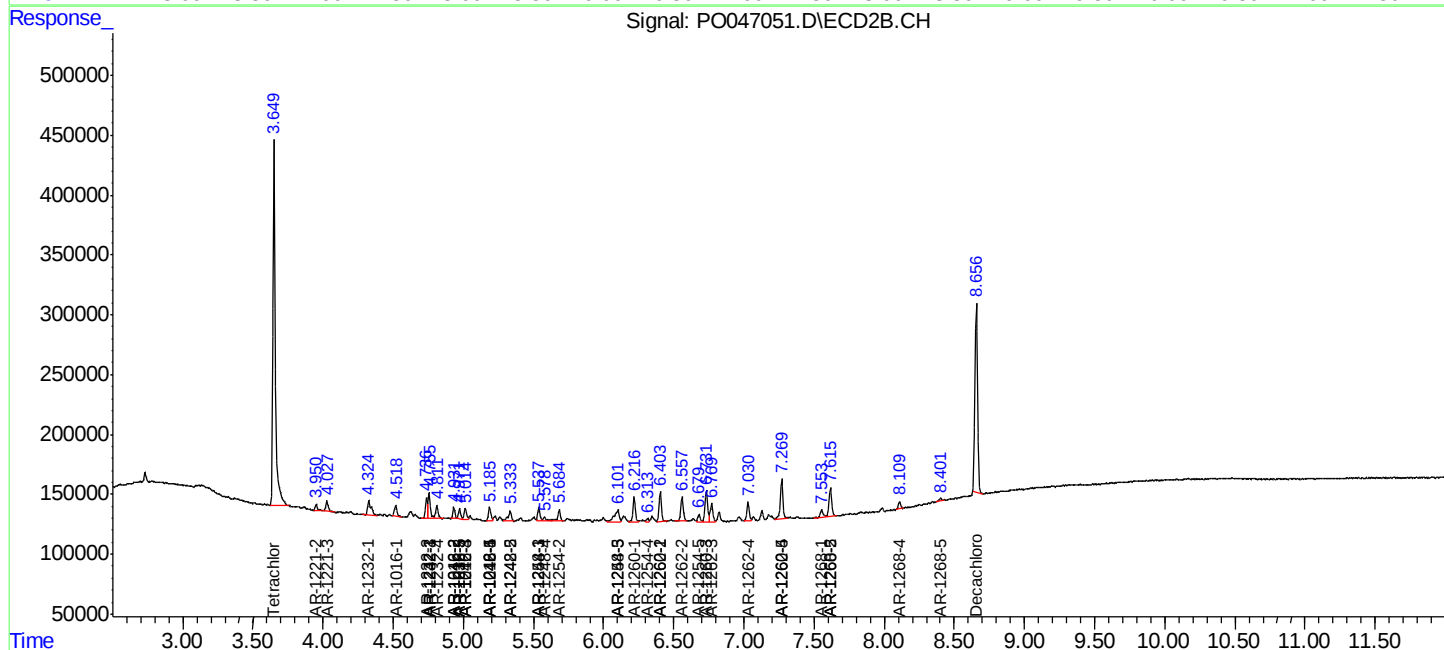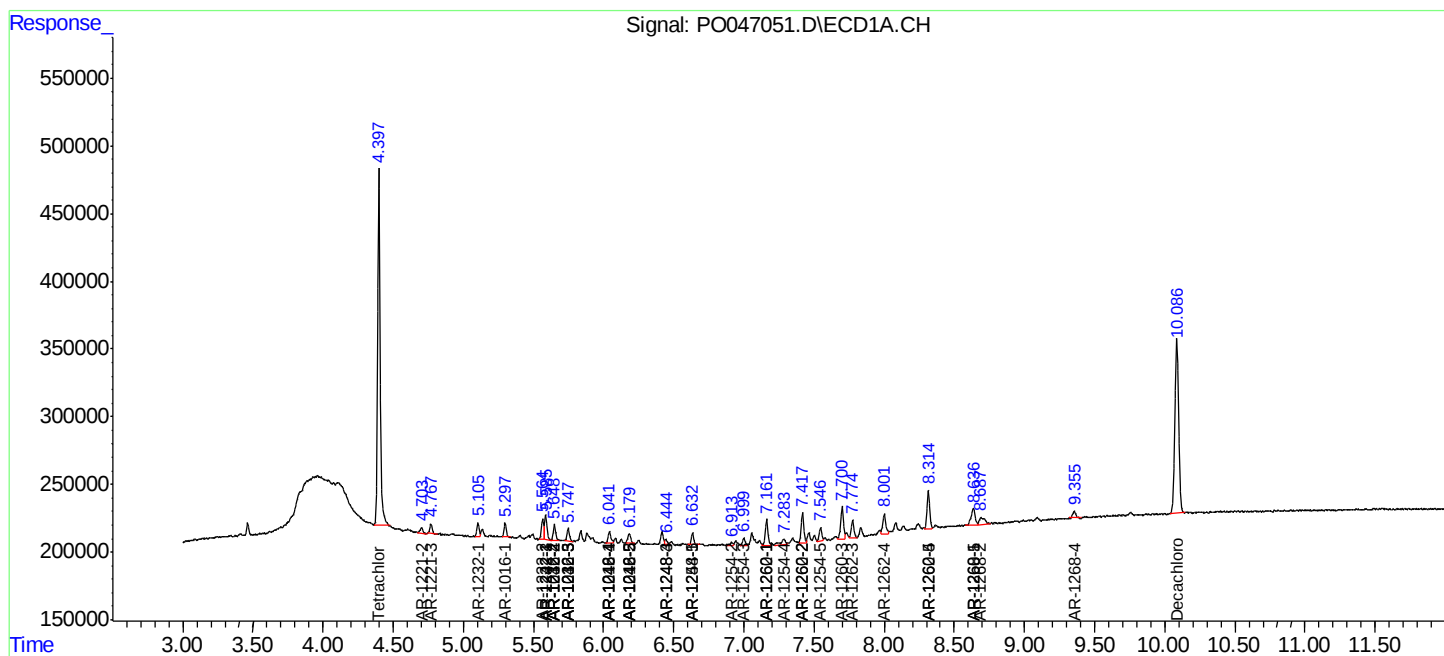


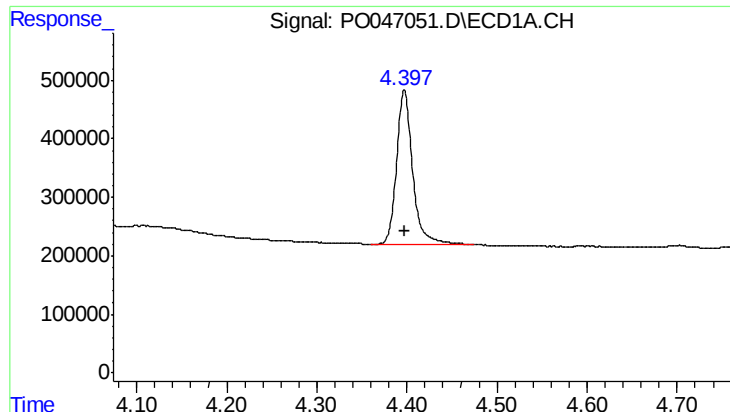

#1 Tetrachloro-m-xylene


R.T.: 4.397 min
Delta R.T.: 0.000 min
Response: 3269634
Conc: 19.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

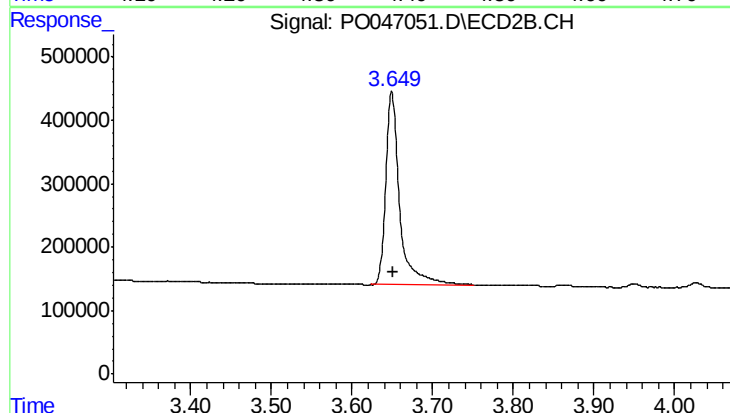


#1 Tetrachloro-m-xylene

R.T.: 3.649 min
Delta R.T.: -0.002 min
Response: 3652668
Conc: 19.04 ng/ml

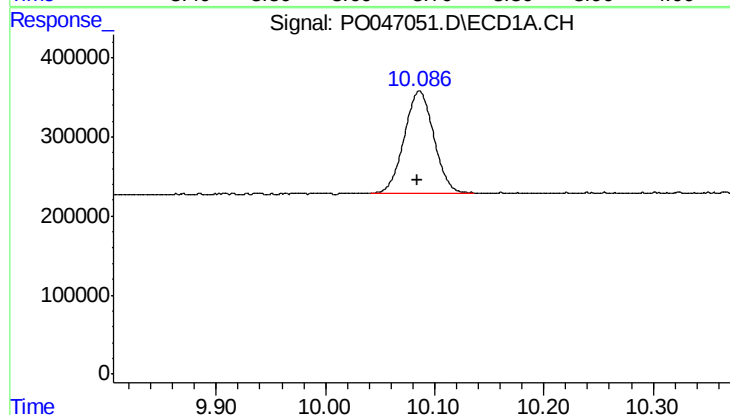


#2 Decachlorobiphenyl

R.T.: 10.086 min
Delta R.T.: 0.002 min
Response: 2428813
Conc: 22.19 ng/ml

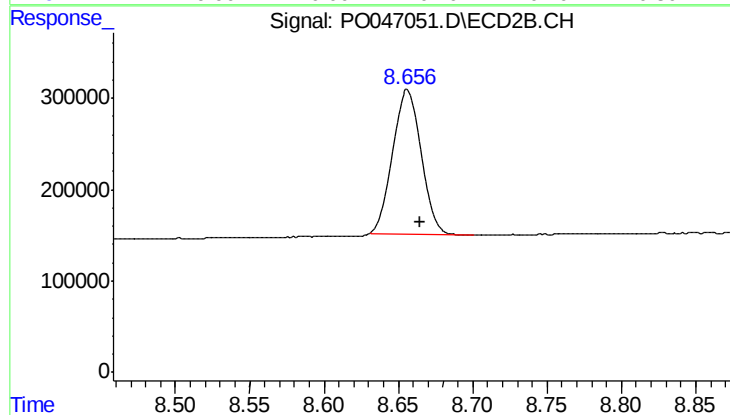

#2 Decachlorobiphenyl


R.T.: 8.656 min
Delta R.T.: -0.008 min
Response: 2103406
Conc: 22.90 ng/ml

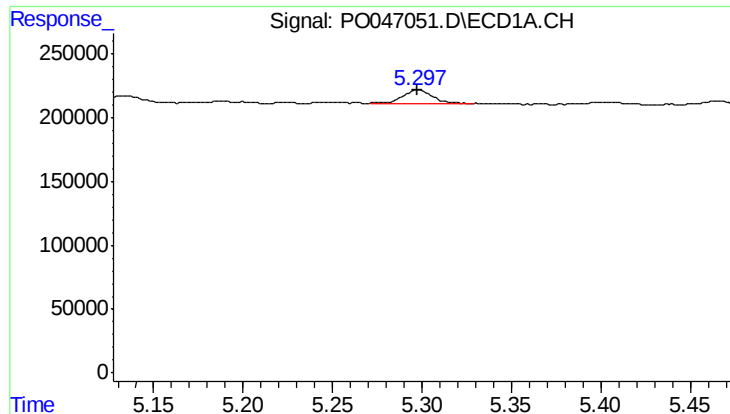

#3 AR-1016-1


R.T.: 5.298 min
Delta R.T.: 0.000 min
Response: 114020
Conc: 35.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

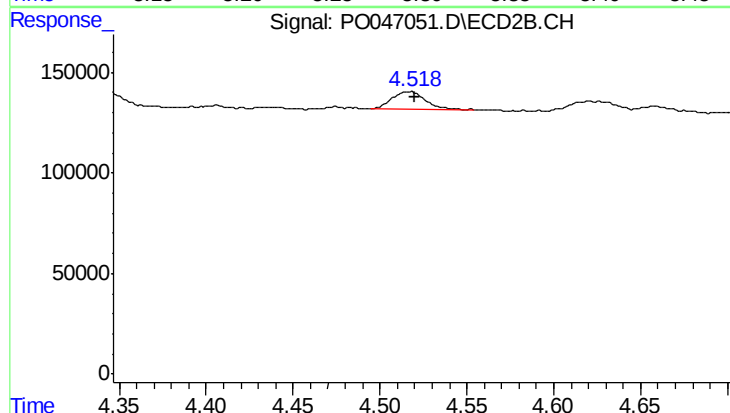


#3 AR-1016-1

R.T.: 4.517 min
Delta R.T.: -0.003 min
Response: 110267
Conc: 32.46 ng/ml

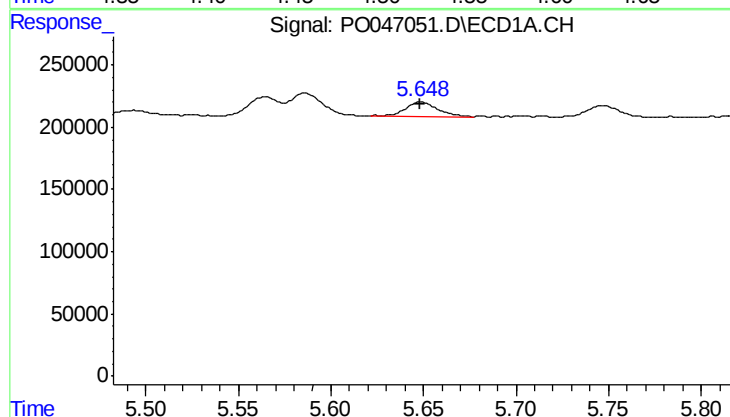


#4 AR-1016-2

R.T.: 5.649 min
Delta R.T.: 0.000 min
Response: 142655
Conc: 36.47 ng/ml

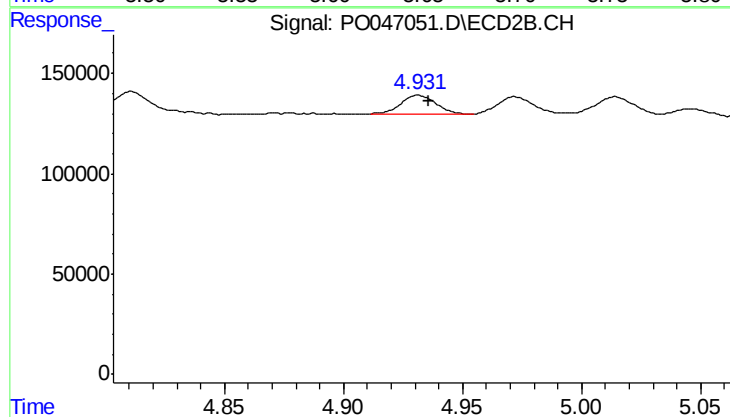

#4 AR-1016-2


R.T.: 4.932 min
Delta R.T.: -0.004 min
Response: 96772
Conc: 30.08 ng/ml

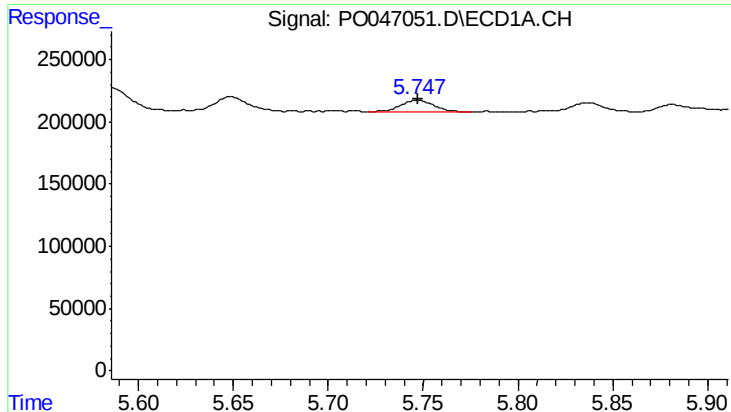

#5 AR-1016-3


R.T.: 5.747 min
Delta R.T.: 0.000 min
Response: 106757
Conc: 33.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

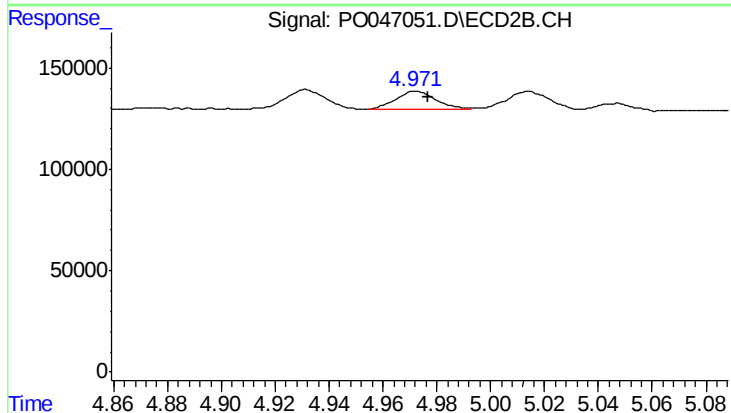


#5 AR-1016-3

R.T.: 4.972 min
Delta R.T.: -0.004 min
Response: 94024
Conc: 35.81 ng/ml

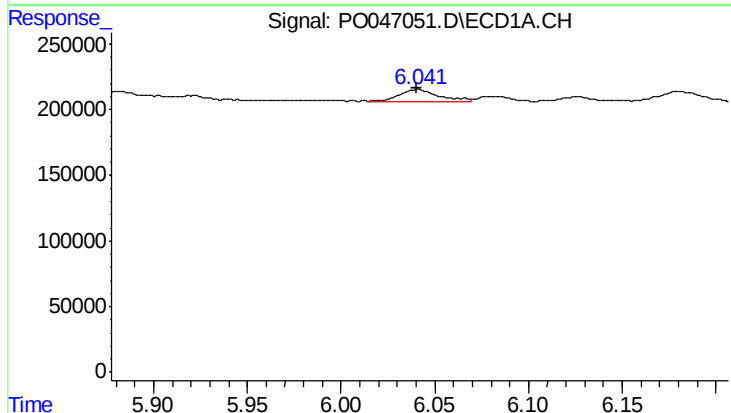


#6 AR-1016-4

R.T.: 6.041 min
Delta R.T.: 0.000 min
Response: 129016
Conc: 40.89 ng/ml

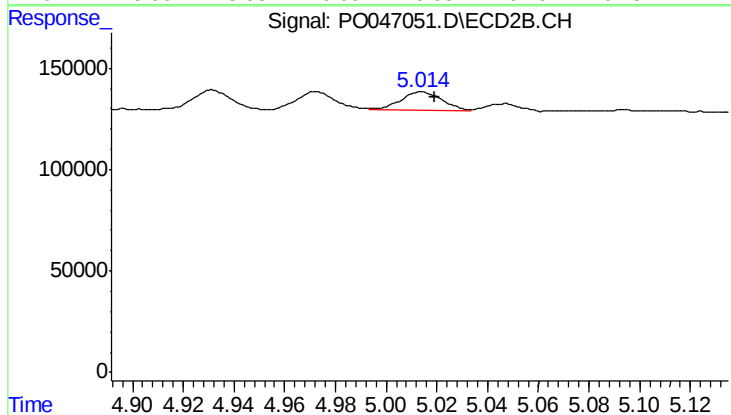

#6 AR-1016-4


R.T.: 5.014 min
Delta R.T.: -0.005 min
Response: 104028
Conc: 33.44 ng/ml

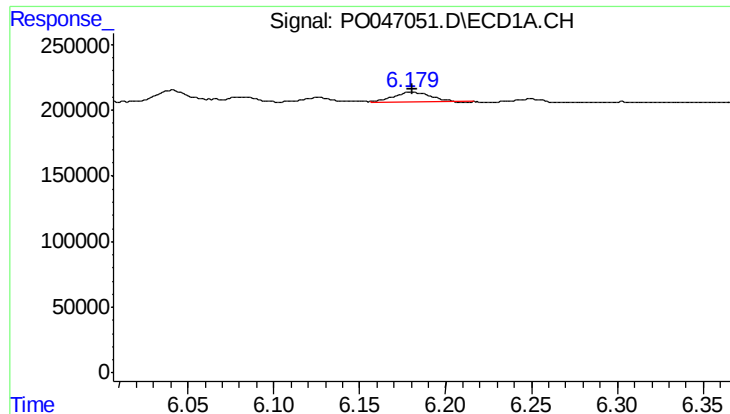

#7 AR-1016-5


R.T.: 6.180 min
Delta R.T.: 0.000 min
Response: 108588
Conc: 32.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

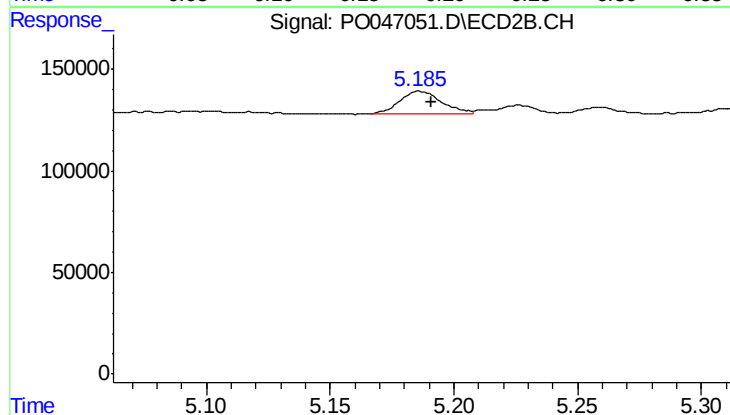


#7 AR-1016-5

R.T.: 5.186 min
Delta R.T.: -0.005 min
Response: 132366
Conc: 38.33 ng/ml

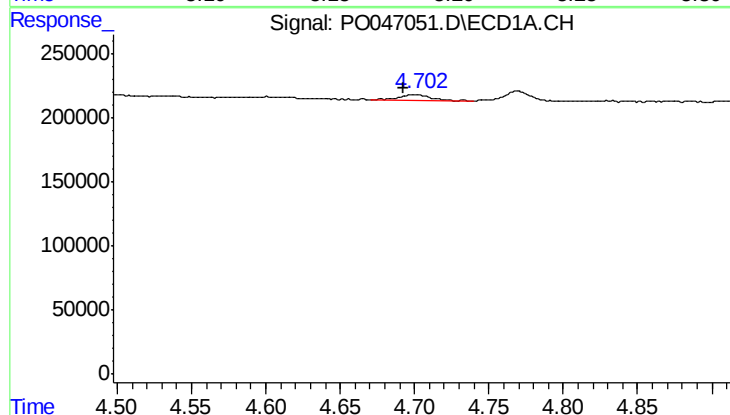


#9 AR-1221-2

R.T.: 4.702 min
Delta R.T.: 0.010 min
Response: 61898
Conc: 52.10 ng/ml

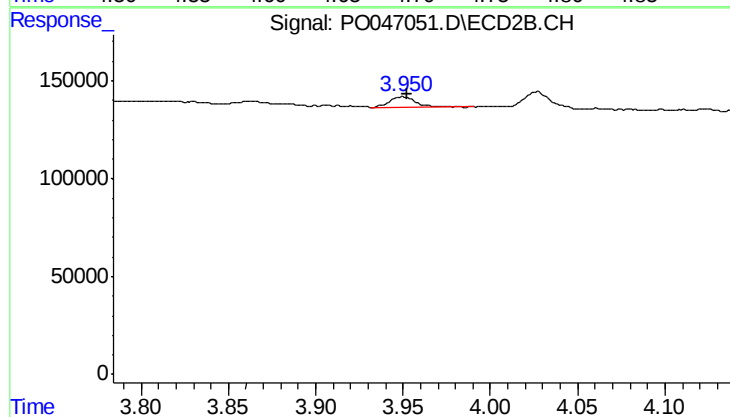

#9 AR-1221-2


R.T.: 3.950 min
Delta R.T.: -0.003 min
Response: 56235
Conc: 46.93 ng/ml

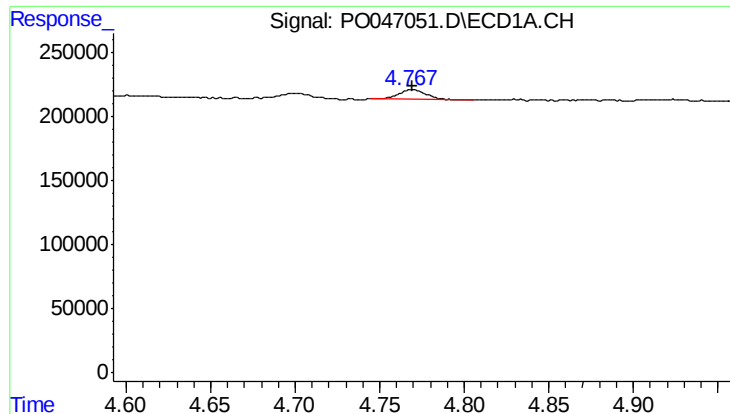

#10 AR-1221-3


R.T.: 4.769 min
Delta R.T.: 0.000 min
Response: 84335
Conc: 22.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

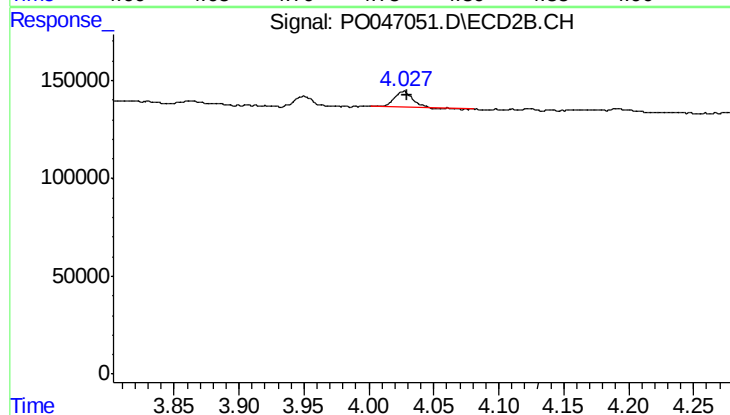


#10 AR-1221-3

R.T.: 4.027 min
Delta R.T.: -0.003 min
Response: 77571
Conc: 19.65 ng/ml

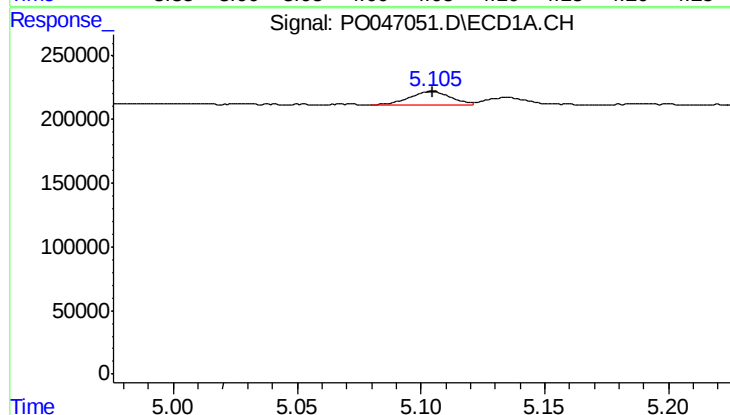


#11 AR-1232-1

R.T.: 5.104 min
Delta R.T.: 0.000 min
Response: 116551
Conc: 77.82 ng/ml

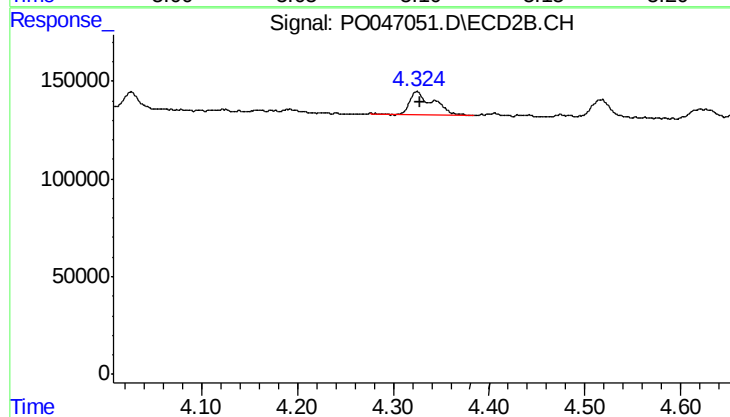

#11 AR-1232-1


R.T.: 4.325 min
Delta R.T.: -0.003 min
Response: 196698
Conc: 125.14 ng/ml

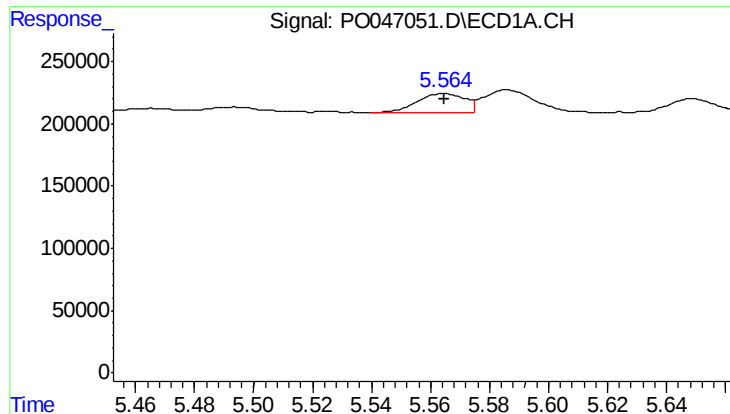

#12 AR-1232-2


R.T.: 5.564 min
Delta R.T.: 0.000 min
Response: 165675
Conc: 81.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

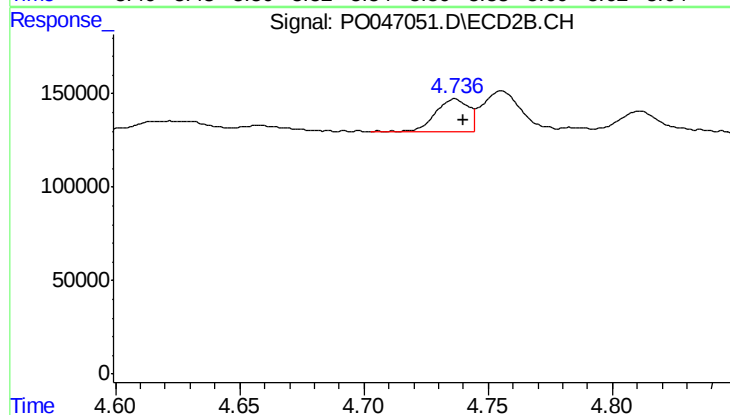


#12 AR-1232-2

R.T.: 4.737 min
Delta R.T.: -0.003 min
Response: 163315
Conc: 81.90 ng/ml

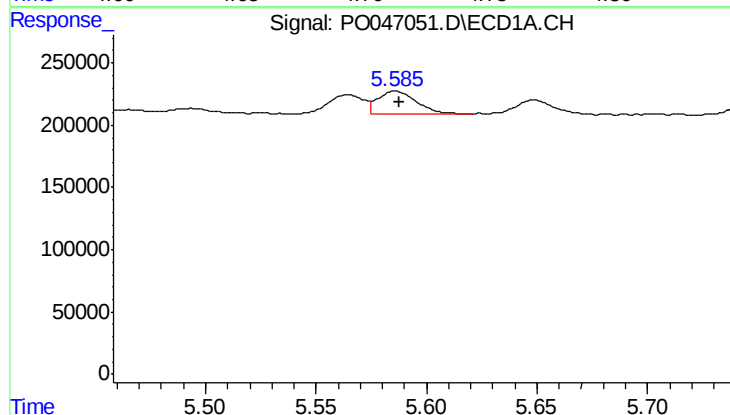


#13 AR-1232-3

R.T.: 5.586 min
Delta R.T.: -0.002 min
Response: 224527
Conc: 77.21 ng/ml

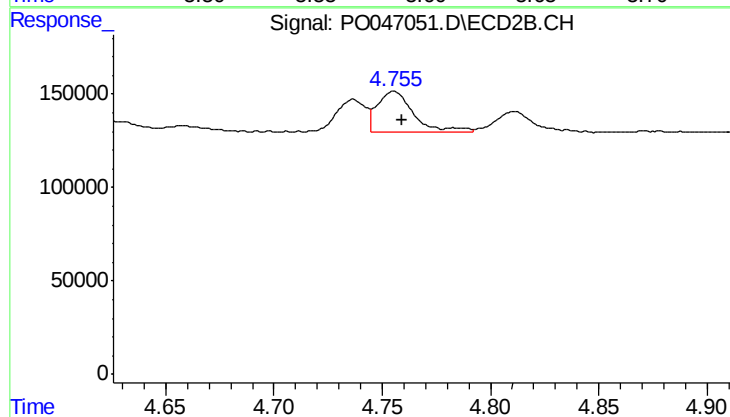

#13 AR-1232-3


R.T.: 4.755 min
Delta R.T.: -0.004 min
Response: 260895
Conc: 84.40 ng/ml

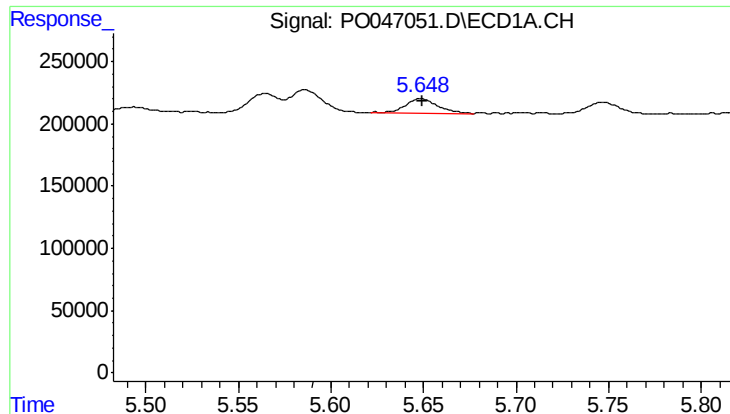

#14 AR-1232-4


R.T.: 5.649 min
Delta R.T.: -0.001 min
Response: 142655
Conc: 79.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

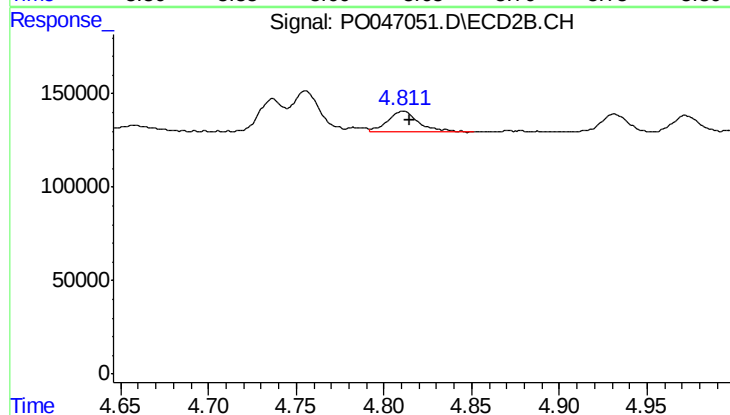


#14 AR-1232-4

R.T.: 4.811 min
Delta R.T.: -0.004 min
Response: 139600
Conc: 76.57 ng/ml

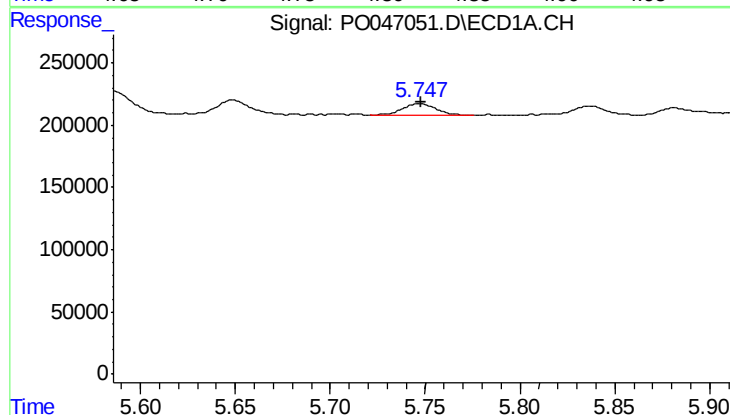


#15 AR-1232-5

R.T.: 5.747 min
Delta R.T.: 0.000 min
Response: 106757
Conc: 75.35 ng/ml

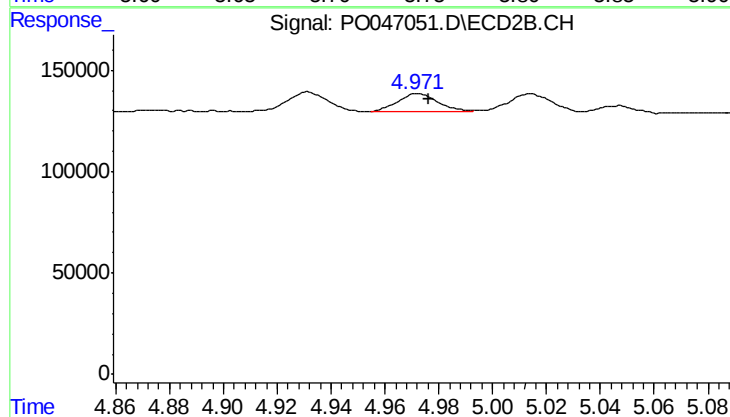

#15 AR-1232-5


R.T.: 4.972 min
Delta R.T.: -0.004 min
Response: 94024
Conc: 93.55 ng/ml

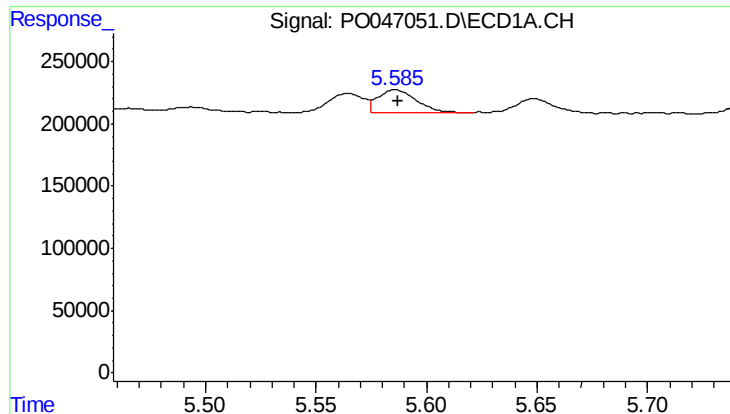

#16 AR-1242-1


R.T.: 5.586 min
Delta R.T.: -0.001 min
Response: 224527
Conc: 38.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

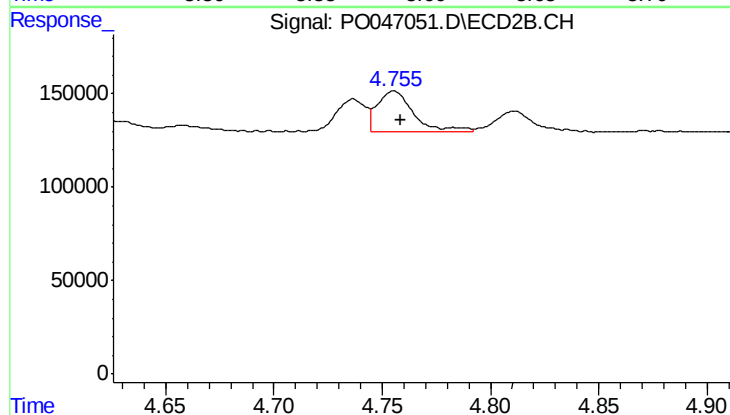


#16 AR-1242-1

R.T.: 4.755 min
Delta R.T.: -0.003 min
Response: 260895
Conc: 45.35 ng/ml

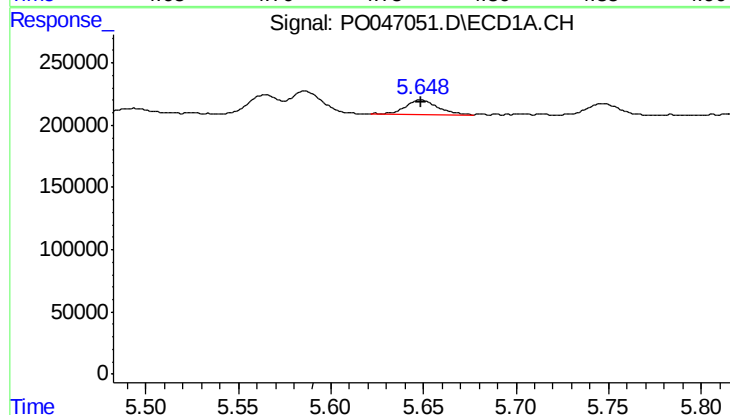


#17 AR-1242-2

R.T.: 5.649 min
Delta R.T.: 0.000 min
Response: 142655
Conc: 40.21 ng/ml

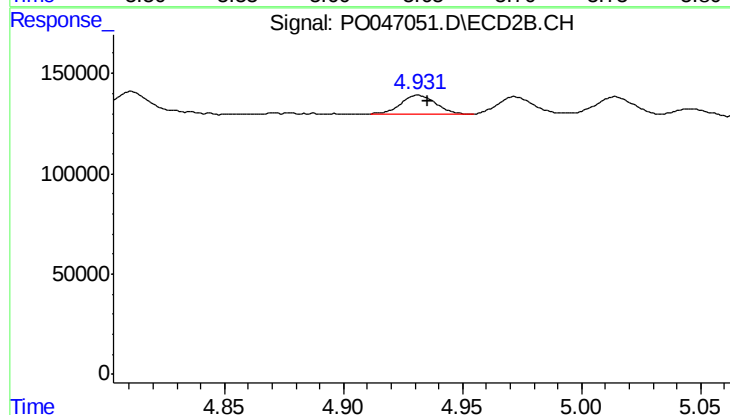

#17 AR-1242-2


R.T.: 4.932 min
Delta R.T.: -0.004 min
Response: 96772
Conc: 33.64 ng/ml

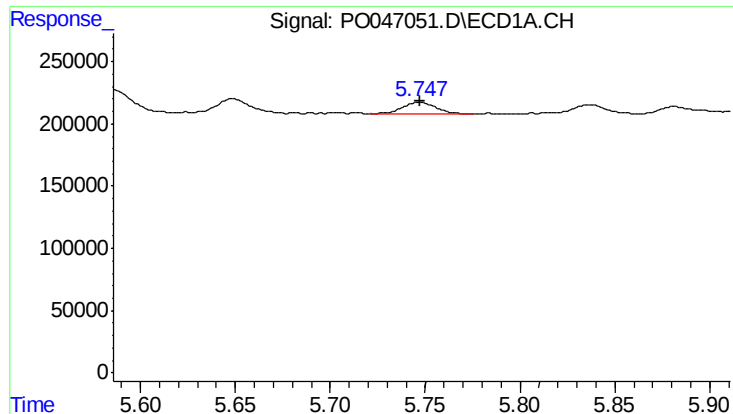

#18 AR-1242-3


R.T.: 5.747 min
Delta R.T.: 0.000 min
Response: 106757
Conc: 37.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

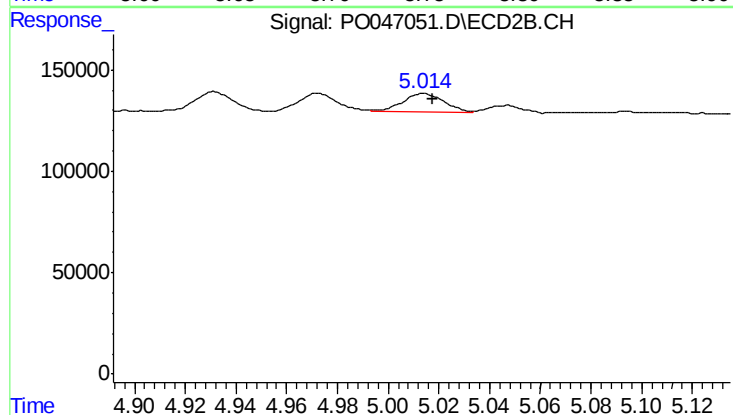


#18 AR-1242-3

R.T.: 5.014 min
Delta R.T.: -0.003 min
Response: 104028
Conc: 36.42 ng/ml

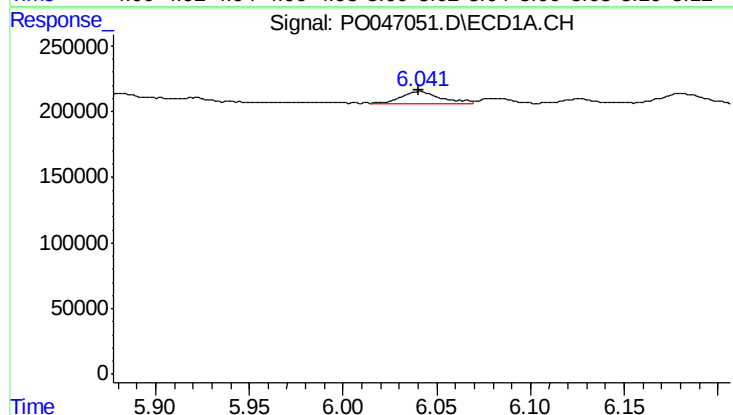


#19 AR-1242-4

R.T.: 6.041 min
Delta R.T.: 0.000 min
Response: 129016
Conc: 44.86 ng/ml

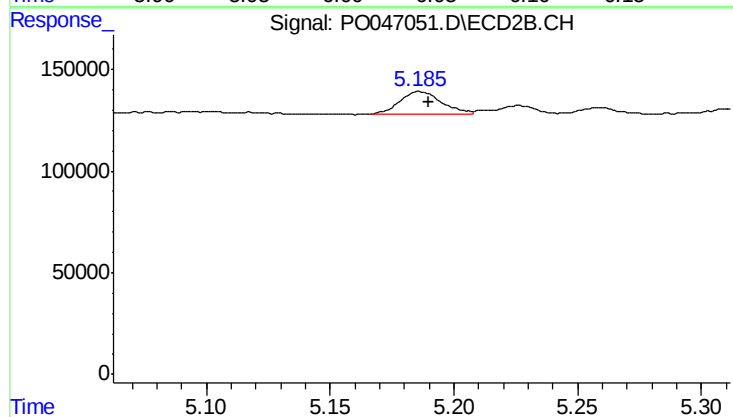

#19 AR-1242-4


R.T.: 5.186 min
Delta R.T.: -0.004 min
Response: 132366
Conc: 43.32 ng/ml

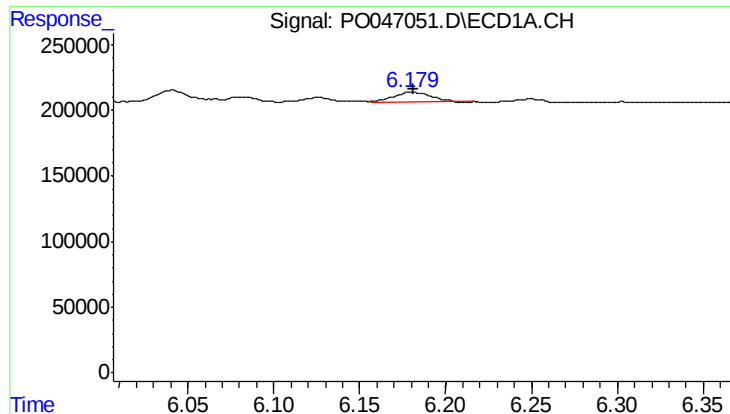

#20 AR-1242-5


R.T.: 6.180 min
Delta R.T.: -0.001 min
Response: 108588
Conc: 35.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

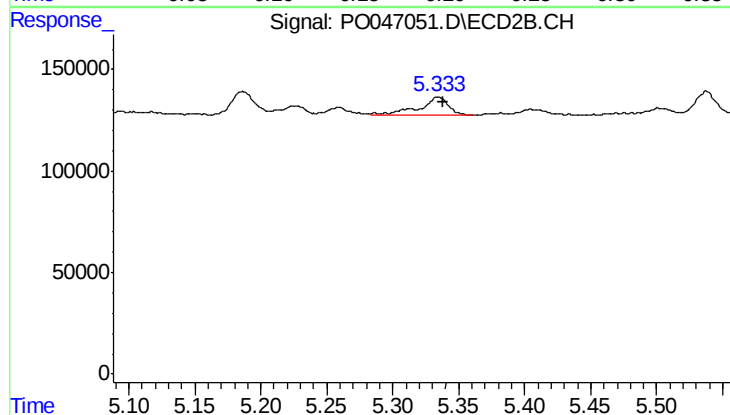


#20 AR-1242-5

R.T.: 5.335 min
Delta R.T.: -0.004 min
Response: 138610
Conc: 42.91 ng/ml

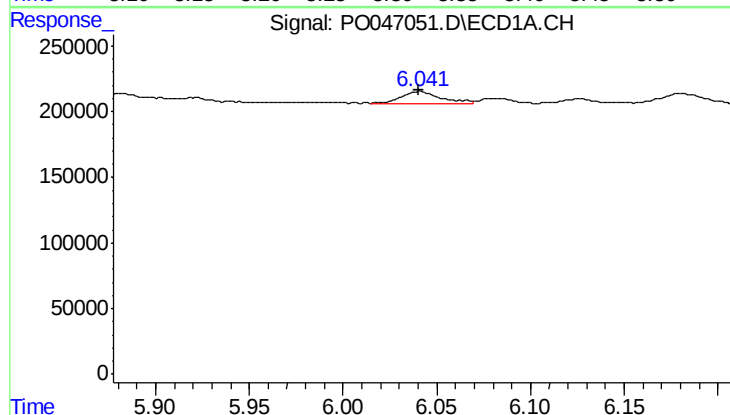


#21 AR-1248-1

R.T.: 6.041 min
Delta R.T.: 0.000 min
Response: 129016
Conc: 27.59 ng/ml

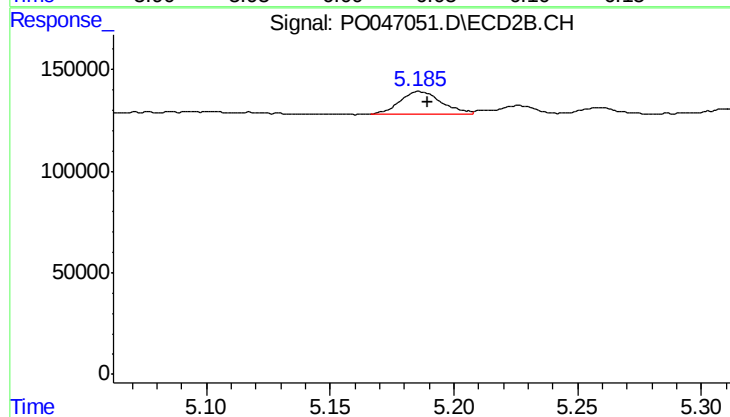

#21 AR-1248-1


R.T.: 5.186 min
Delta R.T.: -0.003 min
Response: 132366
Conc: 26.40 ng/ml

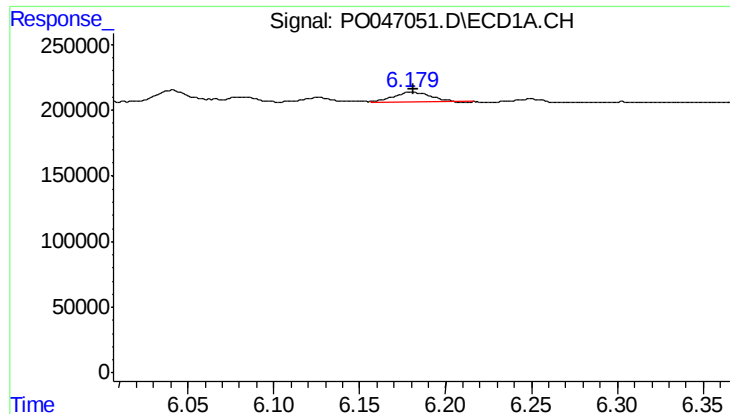

#22 AR-1248-2


R.T.: 6.180 min
Delta R.T.: -0.001 min
Response: 108588
Conc: 27.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

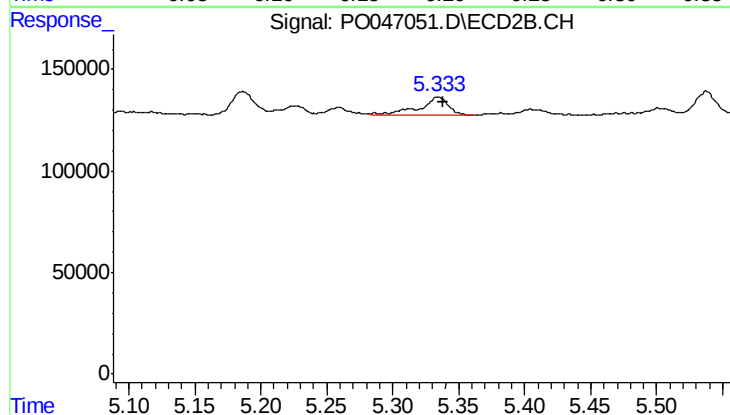


#22 AR-1248-2

R.T.: 5.335 min
Delta R.T.: -0.003 min
Response: 138610
Conc: 33.08 ng/ml

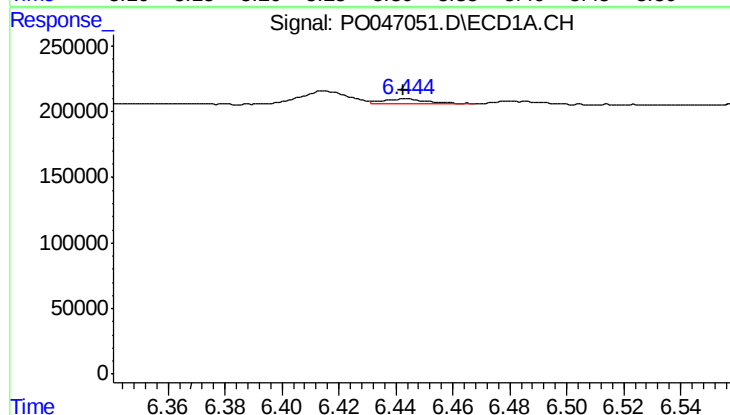


#23 AR-1248-3

R.T.: 6.444 min
Delta R.T.: 0.001 min
Response: 39236
Conc: 7.73 ng/ml

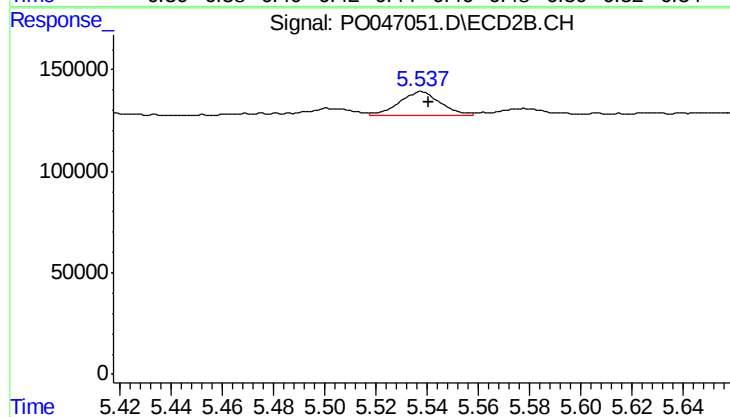

#23 AR-1248-3


R.T.: 5.537 min
Delta R.T.: -0.003 min
Response: 131356
Conc: 20.49 ng/ml

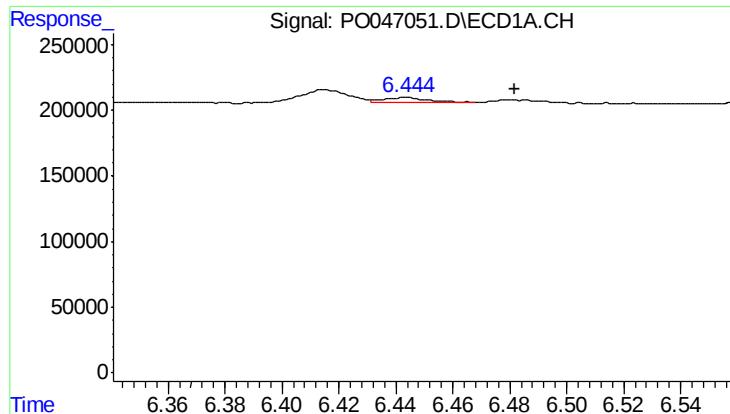

#24 AR-1248-4


R.T.: 6.444 min
Delta R.T.: -0.038 min
Response: 39236
Conc: 8.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

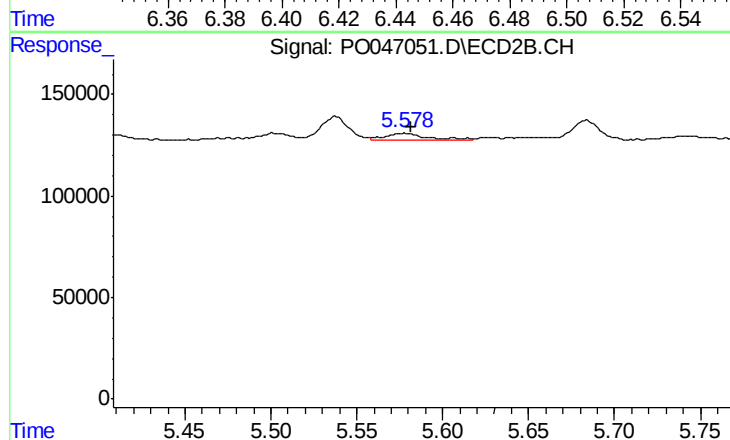


#24 AR-1248-4

R.T.: 5.578 min
Delta R.T.: -0.004 min
Response: 56269
Conc: 12.57 ng/ml

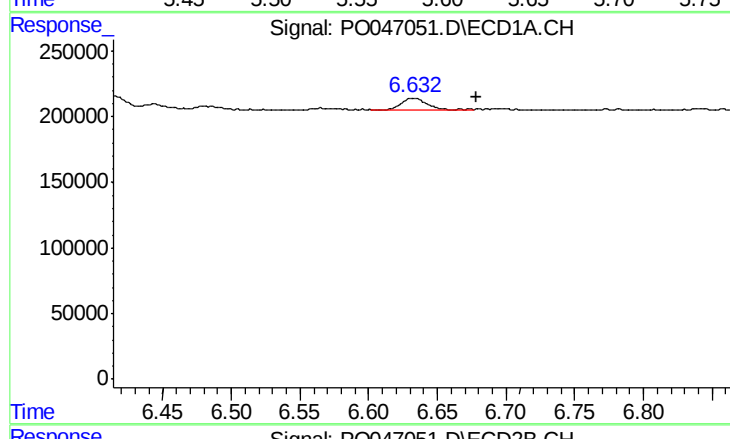


#25 AR-1248-5

R.T.: 6.633 min
Delta R.T.: -0.046 min
Response: 101983
Conc: 31.84 ng/ml

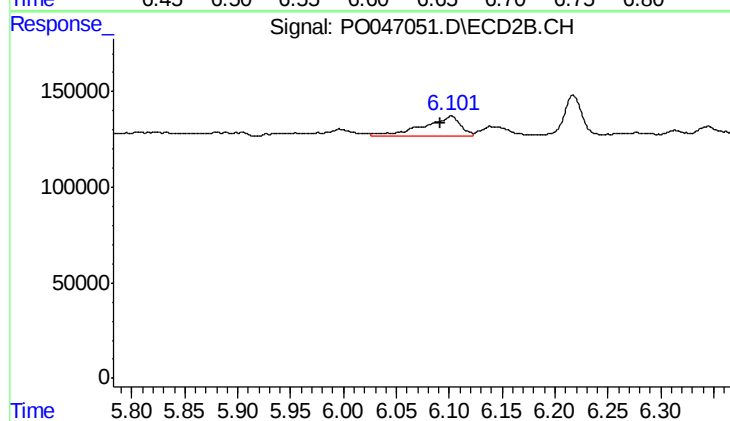

#25 AR-1248-5


R.T.: 6.102 min
Delta R.T.: 0.010 min
Response: 250706
Conc: 90.60 ng/ml

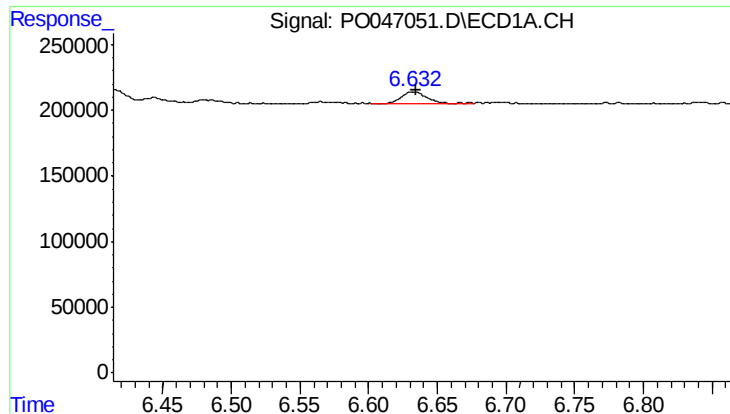

#26 AR-1254-1


R.T.: 6.633 min
Delta R.T.: -0.002 min
Response: 101983
Conc: 12.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

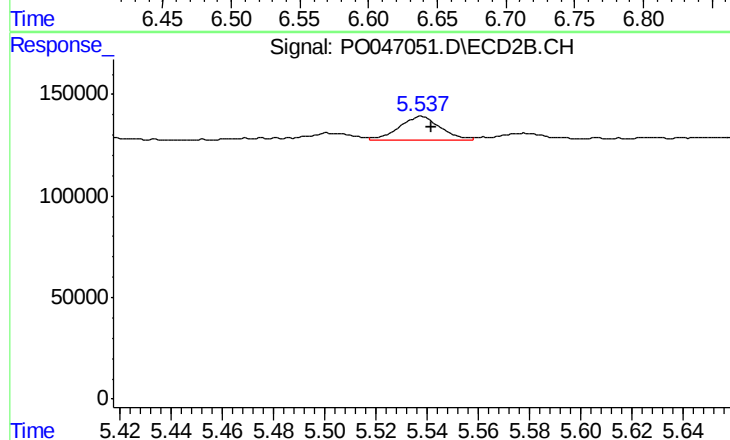


#26 AR-1254-1

R.T.: 5.537 min
Delta R.T.: -0.004 min
Response: 131356
Conc: 18.39 ng/ml

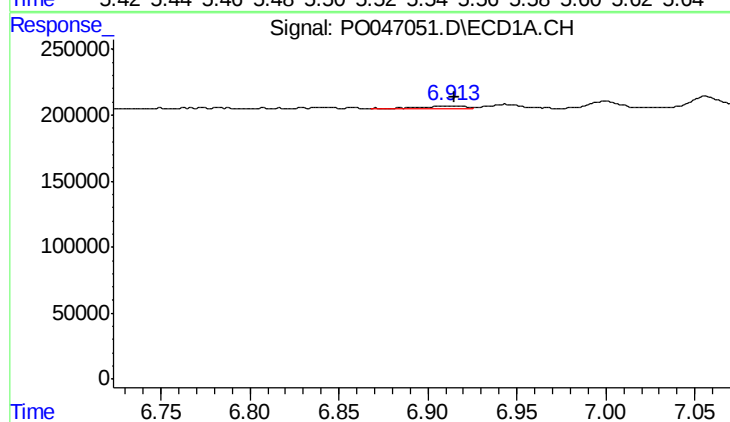


#27 AR-1254-2

R.T.: 6.913 min
Delta R.T.: -0.001 min
Response: 37307
Conc: 7.60 ng/ml

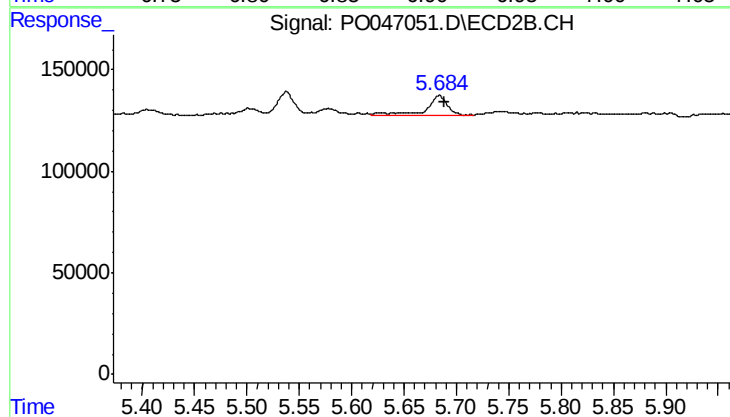

#27 AR-1254-2


R.T.: 5.684 min
Delta R.T.: -0.005 min
Response: 131137
Conc: 21.65 ng/ml

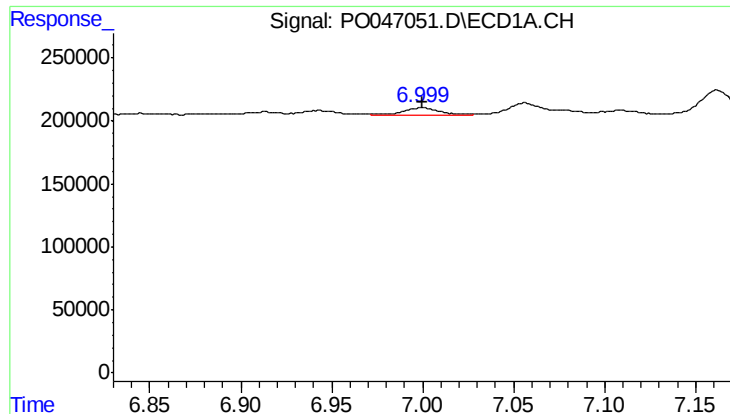

#28 AR-1254-3


R.T.: 7.000 min
Delta R.T.: 0.000 min
Response: 75301
Conc: 8.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

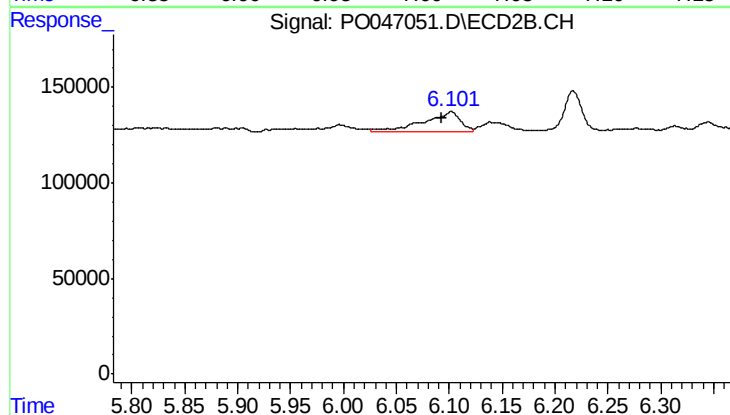


#28 AR-1254-3

R.T.: 6.102 min
Delta R.T.: 0.009 min
Response: 250706
Conc: 26.63 ng/ml

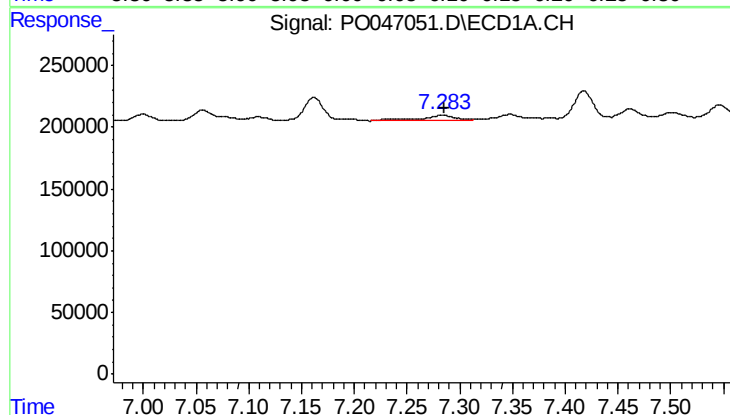


#29 AR-1254-4

R.T.: 7.284 min
Delta R.T.: 0.000 min
Response: 91237
Conc: 14.29 ng/ml

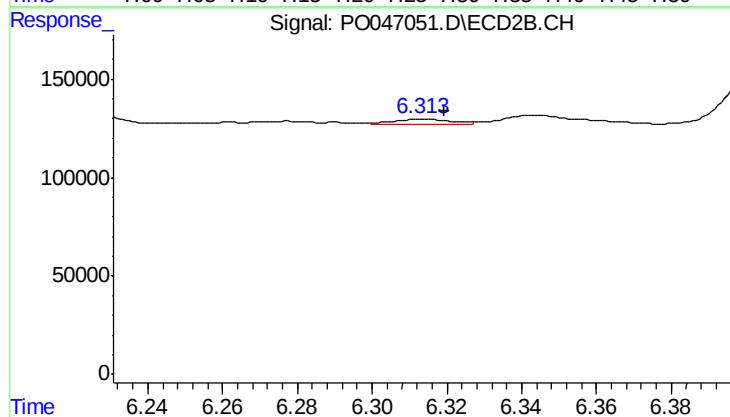

#29 AR-1254-4


R.T.: 6.313 min
Delta R.T.: -0.006 min
Response: 26304
Conc: 4.56 ng/ml

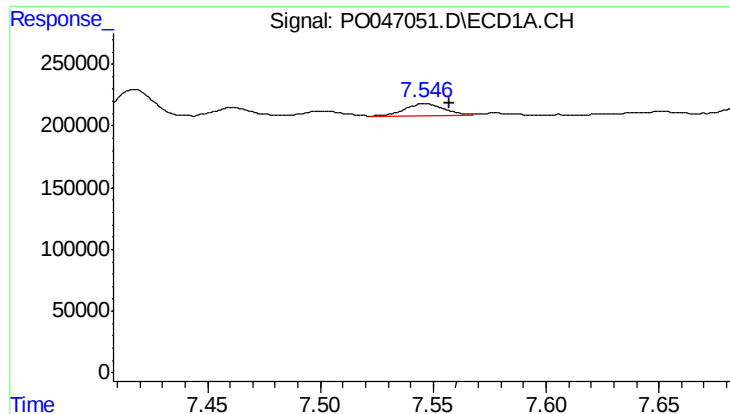

#30 AR-1254-5


R.T.: 7.546 min
Delta R.T.: -0.011 min
Response: 126009
Conc: 26.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

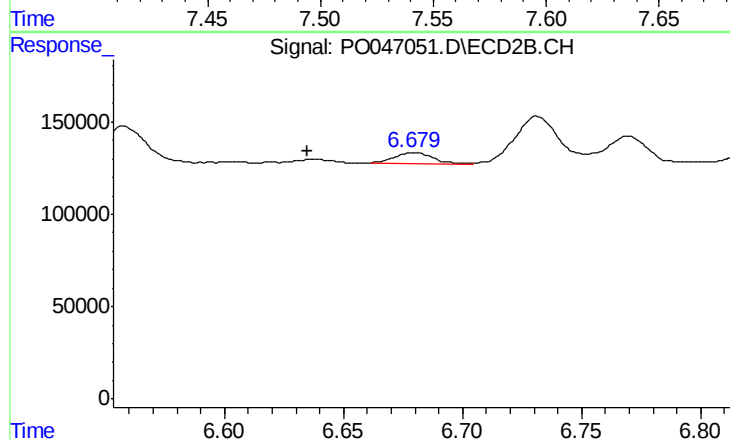


#30 AR-1254-5

R.T.: 6.680 min
Delta R.T.: 0.045 min
Response: 71279
Conc: 17.95 ng/ml

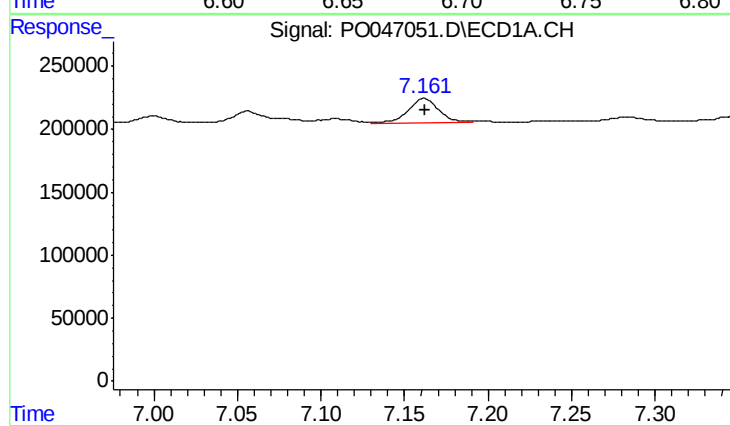


#31 AR-1260-1

R.T.: 7.162 min
Delta R.T.: 0.000 min
Response: 250743
Conc: 41.75 ng/ml

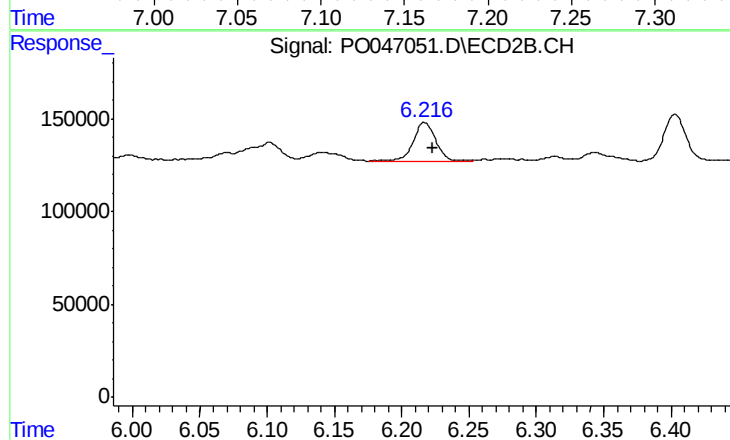

#31 AR-1260-1


R.T.: 6.217 min
Delta R.T.: -0.006 min
Response: 249384
Conc: 42.07 ng/ml

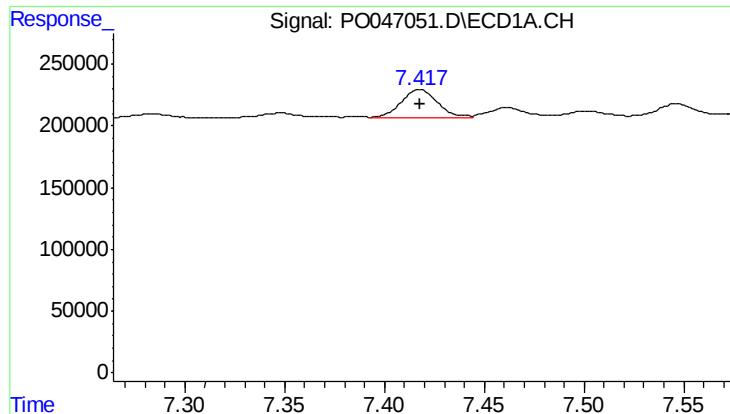

#32 AR-1260-2


R.T.: 7.418 min
Delta R.T.: 0.000 min
Response: 284079
Conc: 38.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

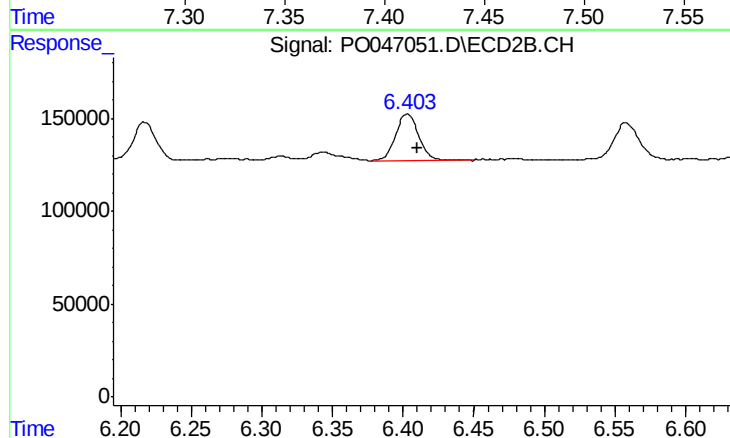


#32 AR-1260-2

R.T.: 6.403 min
Delta R.T.: -0.007 min
Response: 285763
Conc: 40.69 ng/ml

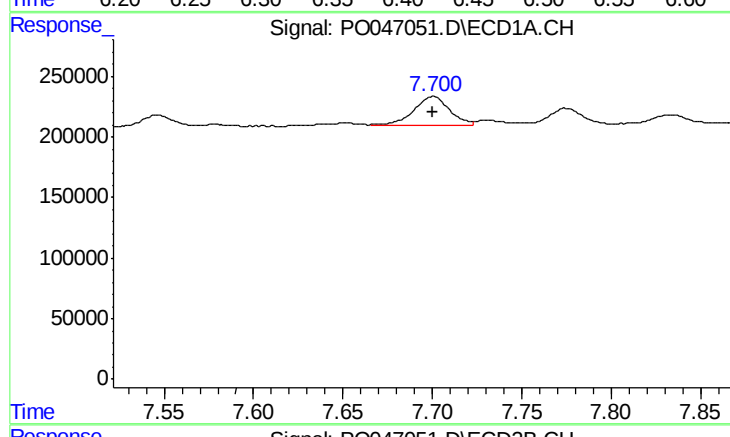


#33 AR-1260-3

R.T.: 7.700 min
Delta R.T.: 0.000 min
Response: 334742
Conc: 39.04 ng/ml

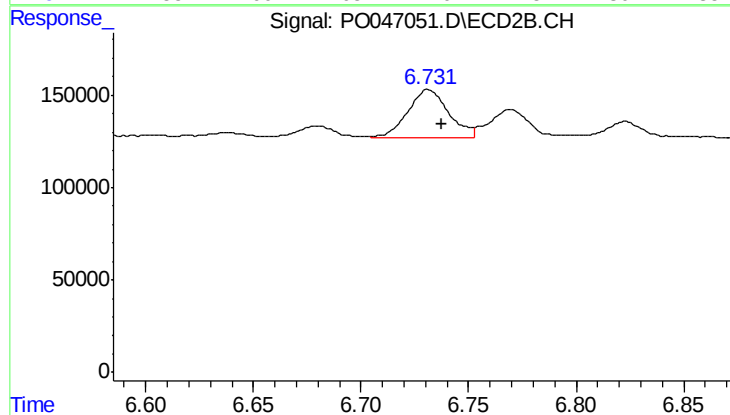

#33 AR-1260-3


R.T.: 6.731 min
Delta R.T.: -0.006 min
Response: 336987
Conc: 44.89 ng/ml

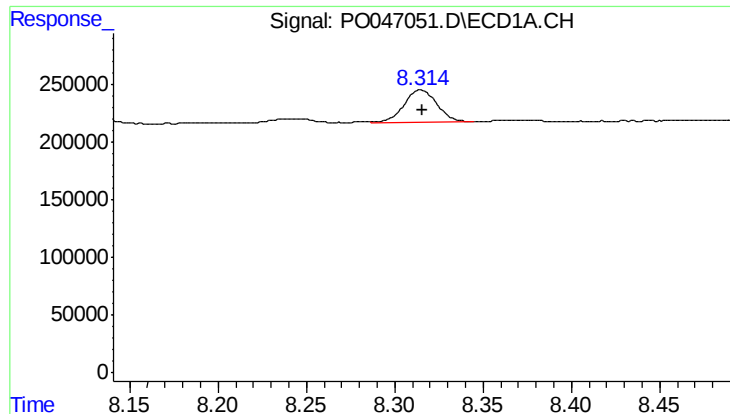

#34 AR-1260-4


R.T.: 8.315 min
Delta R.T.: -0.001 min
Response: 377869
Conc: 31.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

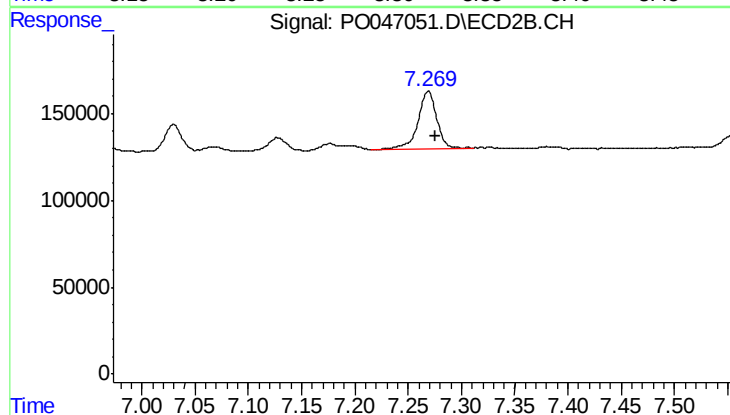


#34 AR-1260-4

R.T.: 7.269 min
Delta R.T.: -0.007 min
Response: 409146
Conc: 35.08 ng/ml

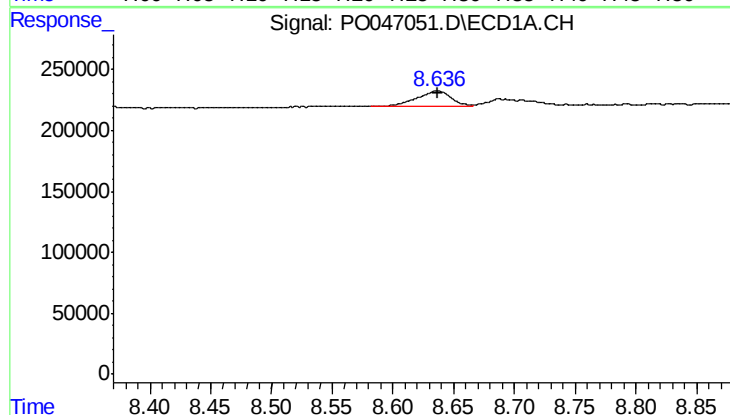


#35 AR-1260-5

R.T.: 8.636 min
Delta R.T.: 0.000 min
Response: 241301
Conc: 32.71 ng/ml

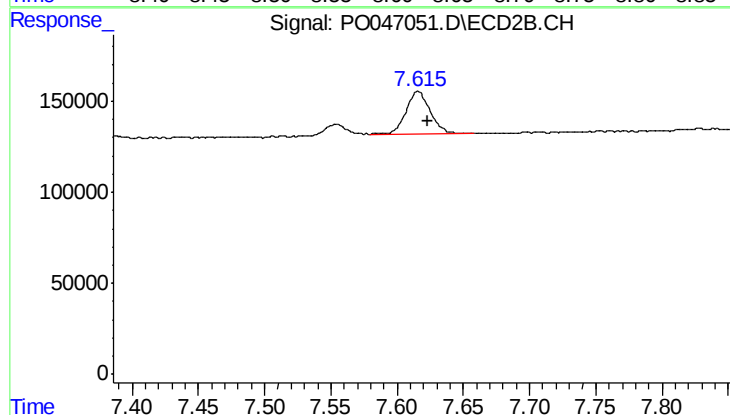

#35 AR-1260-5


R.T.: 7.616 min
Delta R.T.: -0.007 min
Response: 312816
Conc: 37.72 ng/ml

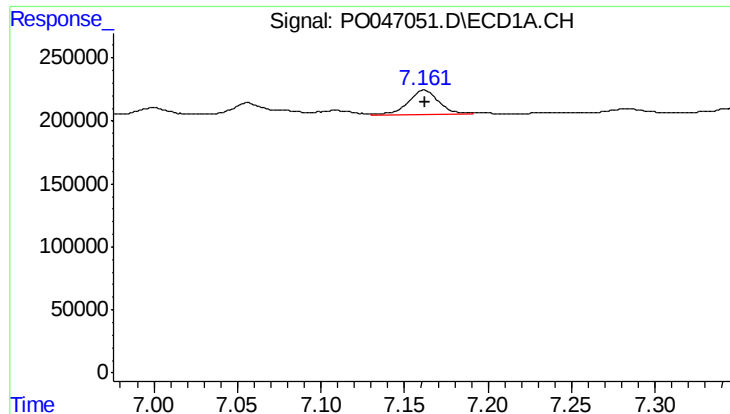

#36 AR-1262-1


R.T.: 7.162 min
Delta R.T.: 0.000 min
Response: 250743
Conc: 46.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

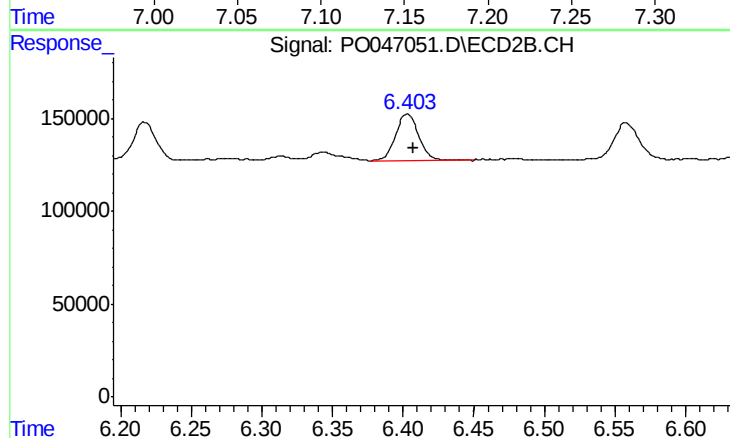


#36 AR-1262-1

R.T.: 6.403 min
Delta R.T.: -0.005 min
Response: 285763
Conc: 46.31 ng/ml

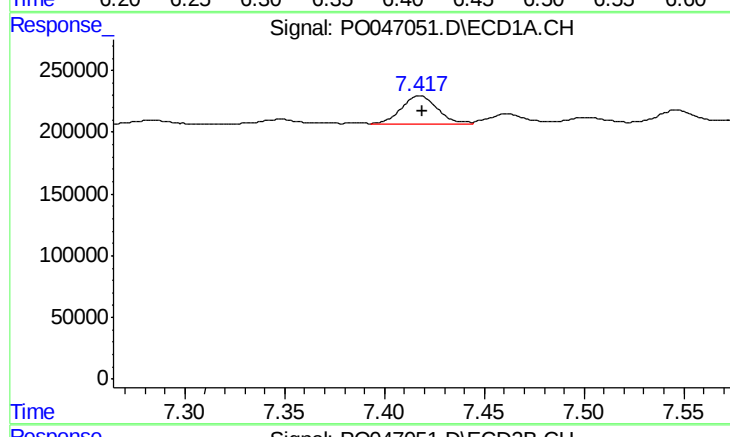


#37 AR-1262-2

R.T.: 7.418 min
Delta R.T.: -0.001 min
Response: 284079
Conc: 44.13 ng/ml

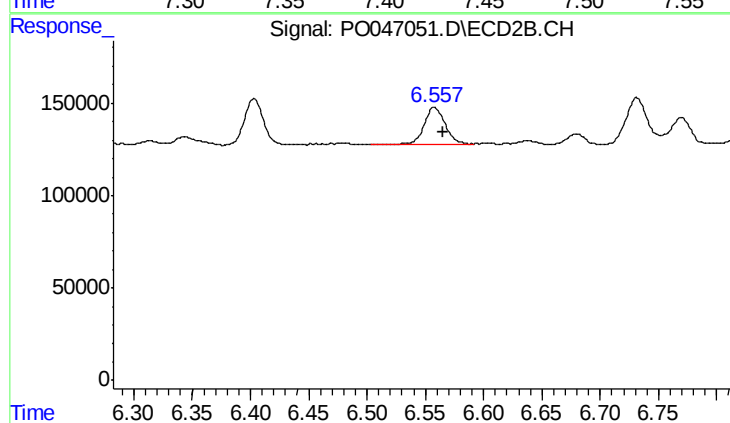

#37 AR-1262-2


R.T.: 6.558 min
Delta R.T.: -0.007 min
Response: 259431
Conc: 42.38 ng/ml

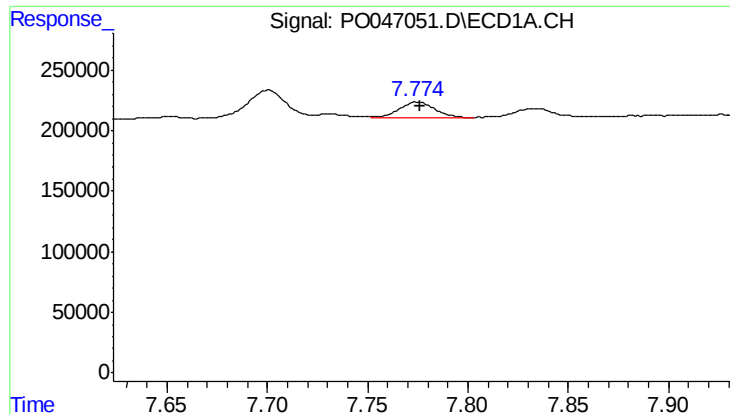

#38 AR-1262-3


R.T.: 7.775 min
Delta R.T.: -0.002 min
Response: 166628
Conc: 20.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

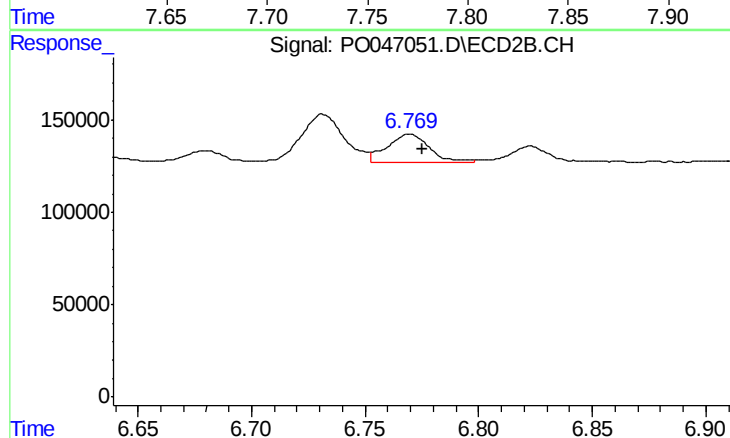


#38 AR-1262-3

R.T.: 6.769 min
Delta R.T.: -0.006 min
Response: 193884
Conc: 23.82 ng/ml

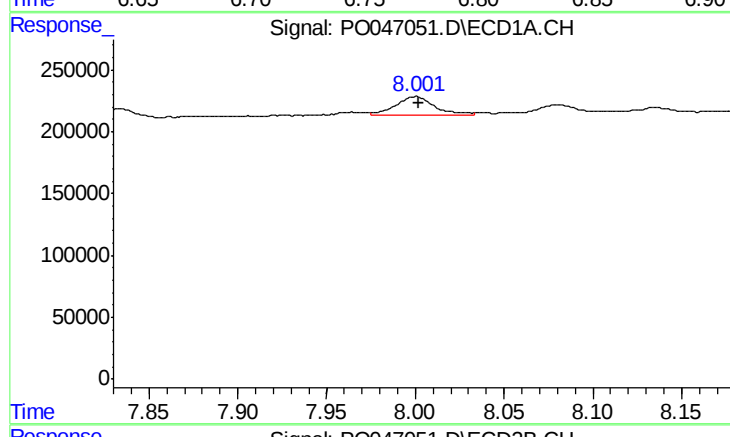


#39 AR-1262-4

R.T.: 8.000 min
Delta R.T.: -0.001 min
Response: 233196
Conc: 29.19 ng/ml

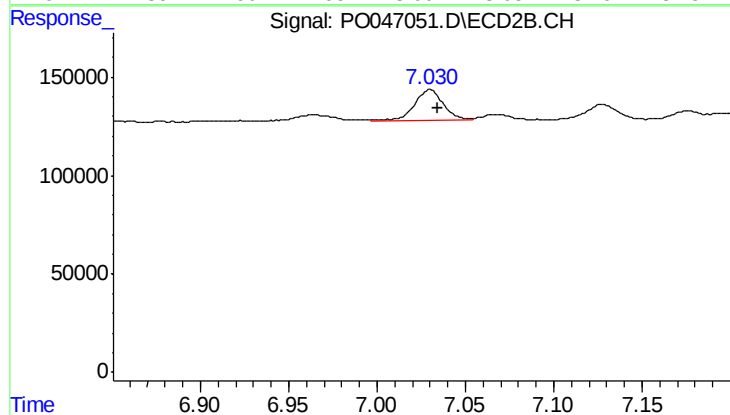

#39 AR-1262-4


R.T.: 7.030 min
Delta R.T.: -0.005 min
Response: 184836
Conc: 26.04 ng/ml

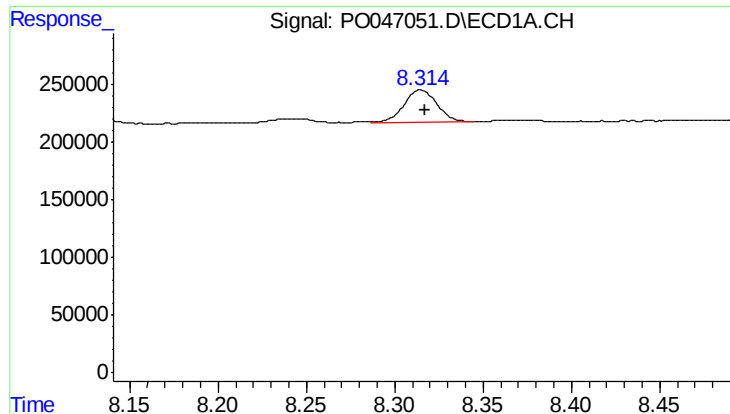

#40 AR-1262-5


R.T.: 8.315 min
Delta R.T.: -0.002 min
Response: 377869
Conc: 25.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

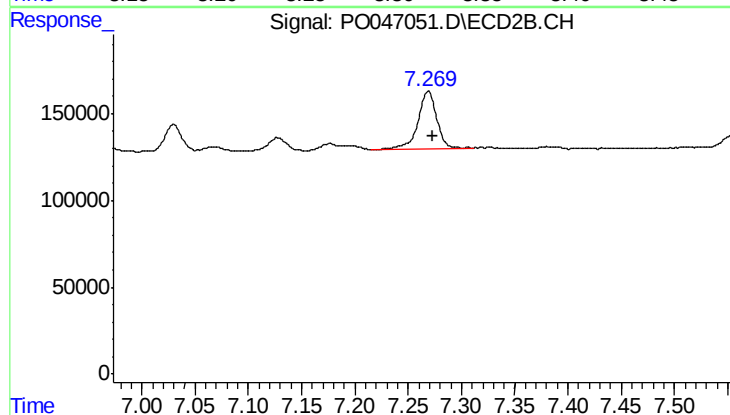


#40 AR-1262-5

R.T.: 7.269 min
Delta R.T.: -0.005 min
Response: 409146
Conc: 29.23 ng/ml

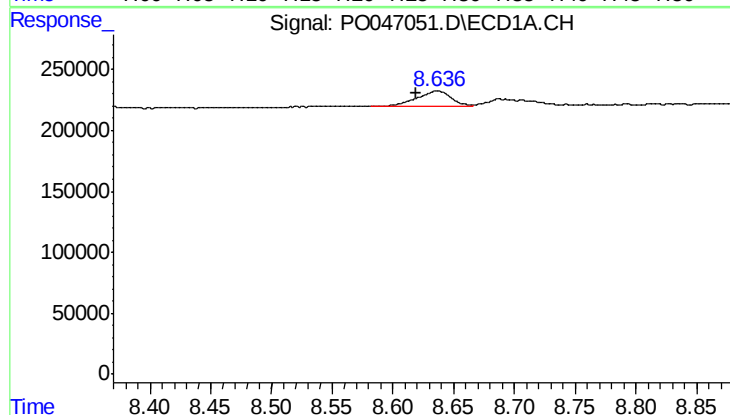


#41 AR-1268-1

R.T.: 8.636 min
Delta R.T.: 0.017 min
Response: 241301
Conc: 15.41 ng/ml

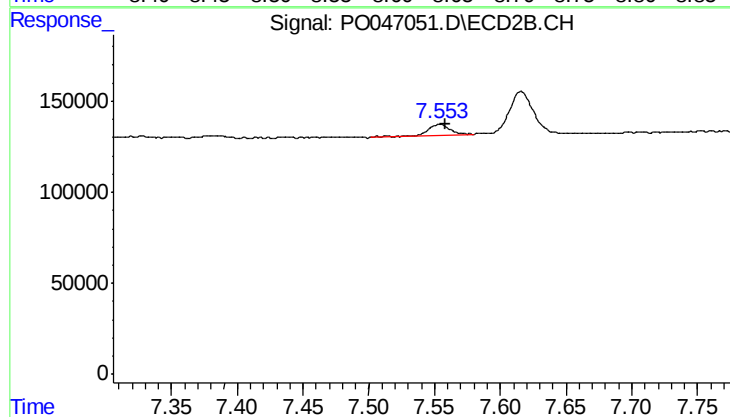

#41 AR-1268-1


R.T.: 7.554 min
Delta R.T.: -0.005 min
Response: 75823
Conc: 5.56 ng/ml

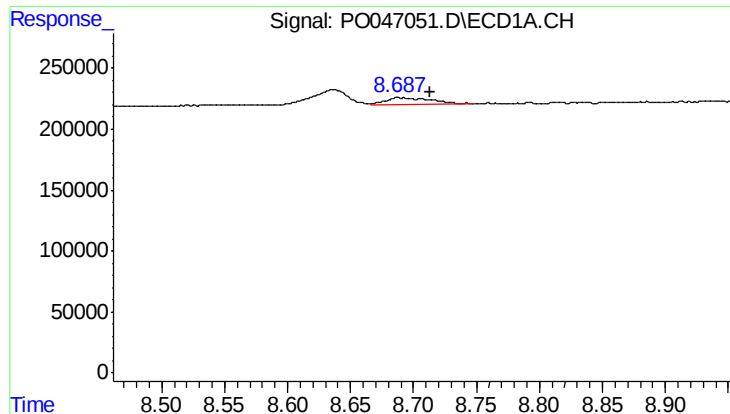

#42 AR-1268-2


R.T.: 8.688 min
Delta R.T.: -0.025 min
Response: 136578
Conc: 9.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

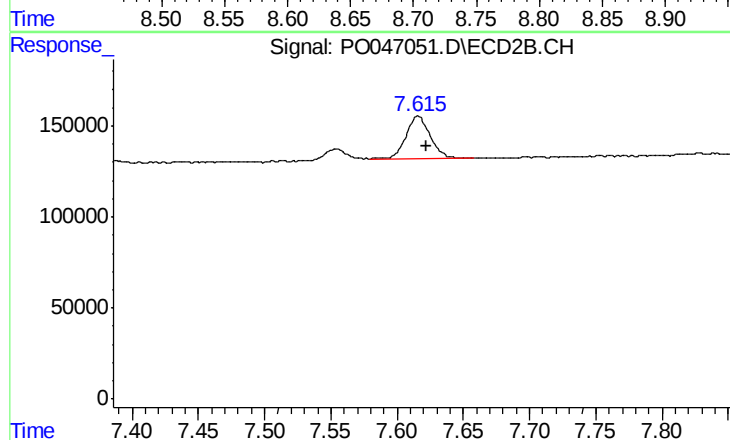


#42 AR-1268-2

R.T.: 7.616 min
Delta R.T.: -0.006 min
Response: 312816
Conc: 24.92 ng/ml

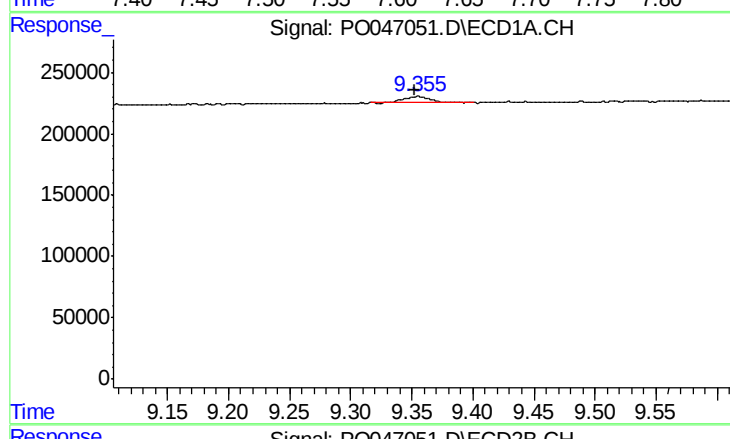


#44 AR-1268-4

R.T.: 9.355 min
Delta R.T.: 0.002 min
Response: 66076
Conc: 13.08 ng/ml

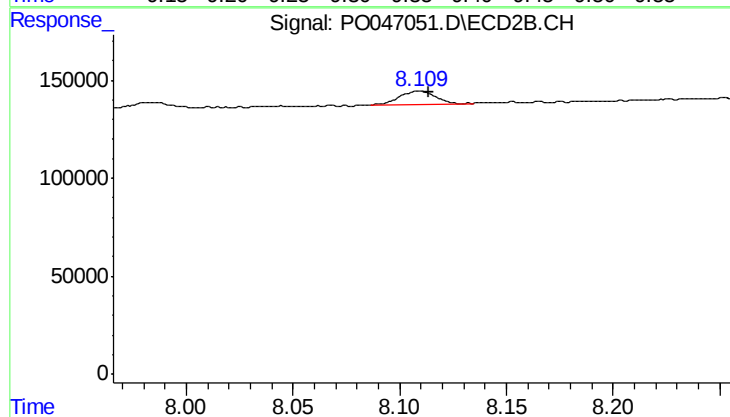

#44 AR-1268-4


R.T.: 8.109 min
Delta R.T.: -0.005 min
Response: 75827
Conc: 17.31 ng/ml

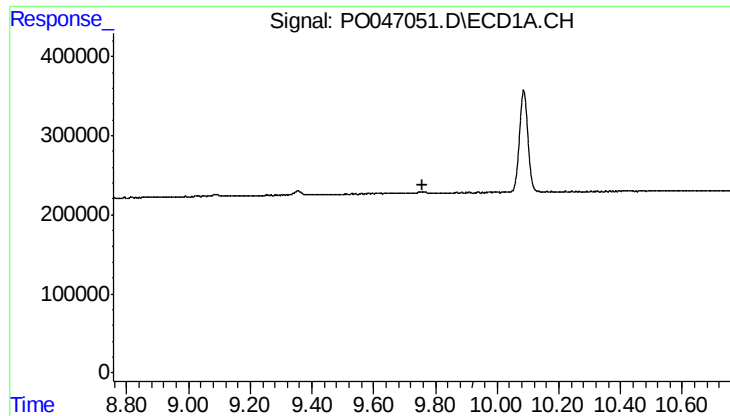

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.756 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT3-2018

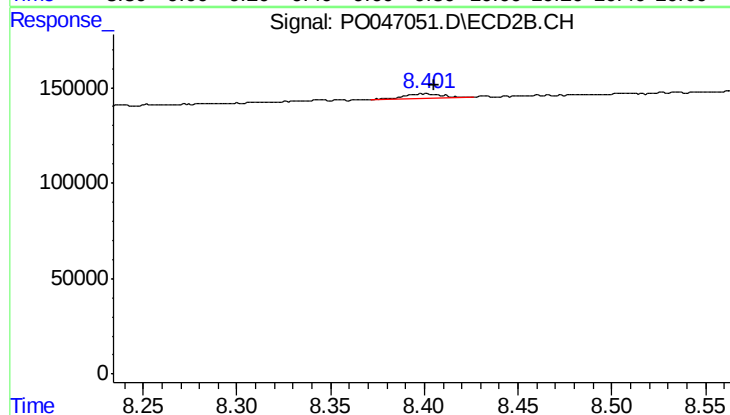

#45 AR-1268-5

R.T.: 8.400 min
Delta R.T.: -0.006 min
Response: 33222
Conc: 1.11 ng/ml