

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072318\
 Data File : P0047063.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jul 2018 4:43
 Operator : SM/SJ
 Sample : AR1248 MDL WATER
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 AR1248 MDL WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 06:08:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 24 03:04:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.397	3.648	3303534	3637564	19.703	18.966
2) SA Decachlor...	10.085	8.655	2445481	2097336	22.339	22.837
Target Compounds						
3) L1 AR-1016-1	5.298	4.520	62032	5393	19.071	1.587 #
4) L1 AR-1016-2	5.649	4.932	109114	90312	27.894	28.072
5) L1 AR-1016-3	5.746	4.972	83209	179308	25.845	68.300 #
6) L1 AR-1016-4	6.040	5.013	193395	154589	61.292	49.694
7) L1 AR-1016-5	6.180	5.185	177044	205372	53.604	59.472
8) L2 AR-1221-1	4.645	3.815	80859	35873	49.833	21.533 #
9) L2 AR-1221-2	4.702	3.948	72320	38677	60.868	32.280 #
10) L2 AR-1221-3	4.702	0.000	72320	0	19.508	N.D. #
11) L3 AR-1232-1	5.103	4.324	78049	143576	52.113	91.346 #
12) L3 AR-1232-2	5.564	4.736	127397	123311	62.523	61.841
13) L3 AR-1232-3	5.587	4.754	176346	160269	60.641	51.847
14) L3 AR-1232-4	5.649	4.810	109114	59780	61.153	32.789 #
15) L3 AR-1232-5	5.746	4.972	83209	179308	58.733	178.401 #
16) L4 AR-1242-1	5.587	4.754	176346	160269	30.424	27.857
17) L4 AR-1242-2	5.649	4.932	109114	90312	30.758	31.392
18) L4 AR-1242-3	5.746	5.013	83209	154589	29.324	54.115 #
19) L4 AR-1242-4	6.040	5.185	193395	205372	67.249	67.219
20) L4 AR-1242-5	6.180	5.335	177044	317154	57.153	98.172 #
21) L5 AR-1248-1	6.040	5.185	193395	205372	41.361	40.968
22) L5 AR-1248-2	6.180	5.335	177044	317154	44.670	75.680 #
23) L5 AR-1248-3	6.443	5.536	197607	392027	38.923	61.153 #
24) L5 AR-1248-4	6.481	5.577	183311	349101	38.377	78.000 #
25) L5 AR-1248-5	6.678	6.088	134002	309503	41.843	111.848 #
26) L6 AR-1254-1	6.637	5.536	204539	392027	24.876	54.878 #
27) L6 AR-1254-2	6.914	5.750	84731	429908	17.256	70.976 #
28) L6 AR-1254-3	7.001	6.088	168341	309503	19.587	32.873 #
29) L6 AR-1254-4	7.284	6.315	210030	280143	32.886	48.572 #
30) L6 AR-1254-5	7.557	6.629	155746	473677	32.799	119.310 #
31) L7 AR-1260-1	7.162	6.219	99921	463276	16.638	78.154 #
32) L7 AR-1260-2	7.419	6.399	129249	418960	17.686	59.651 #
33) L7 AR-1260-3	7.701	6.732	140689	384318	16.407	51.190 #
34) L7 AR-1260-4	8.316	7.268	95346	346915	7.876	29.748 #
35) L7 AR-1260-5	8.637	7.614	42489	728293	5.760	87.828 #
36) L8 AR-1262-1	7.162	6.399	99921	418960	18.565	67.889 #
37) L8 AR-1262-2	7.419	6.556	129249	530420	20.079	86.656 #
38) L8 AR-1262-3	7.778	6.769	66492	242940	8.058	29.850 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072318\
 Data File : P0047063.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jul 2018 4:43
 Operator : SM/SJ
 Sample : AR1248 MDL WATER
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248 MDL WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 06:08:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 24 03:04:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
39) L8	AR-1262-4	7.998	7.029	236136	277769	29.559	39.135 #
40) L8	AR-1262-5	8.316	7.268	95346	346915	6.400	24.785 #
41) L9	AR-1268-1	8.637	7.614	42489	728293	2.713	53.451 #
42) L9	AR-1268-2	0.000	7.614	0	728293	N.D.	58.028 #
43) L9	AR-1268-3	0.000	7.780	0	37735	N.D.	3.751 #
45) L9	AR-1268-5	0.000	8.398	0	18534	N.D.	0.617 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072318\
Data File : P0047063.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jul 2018 4:43
Operator : SM/SJ
Sample : AR1248 MDL WATER
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248 MDL WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 06:08:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 24 03:04:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

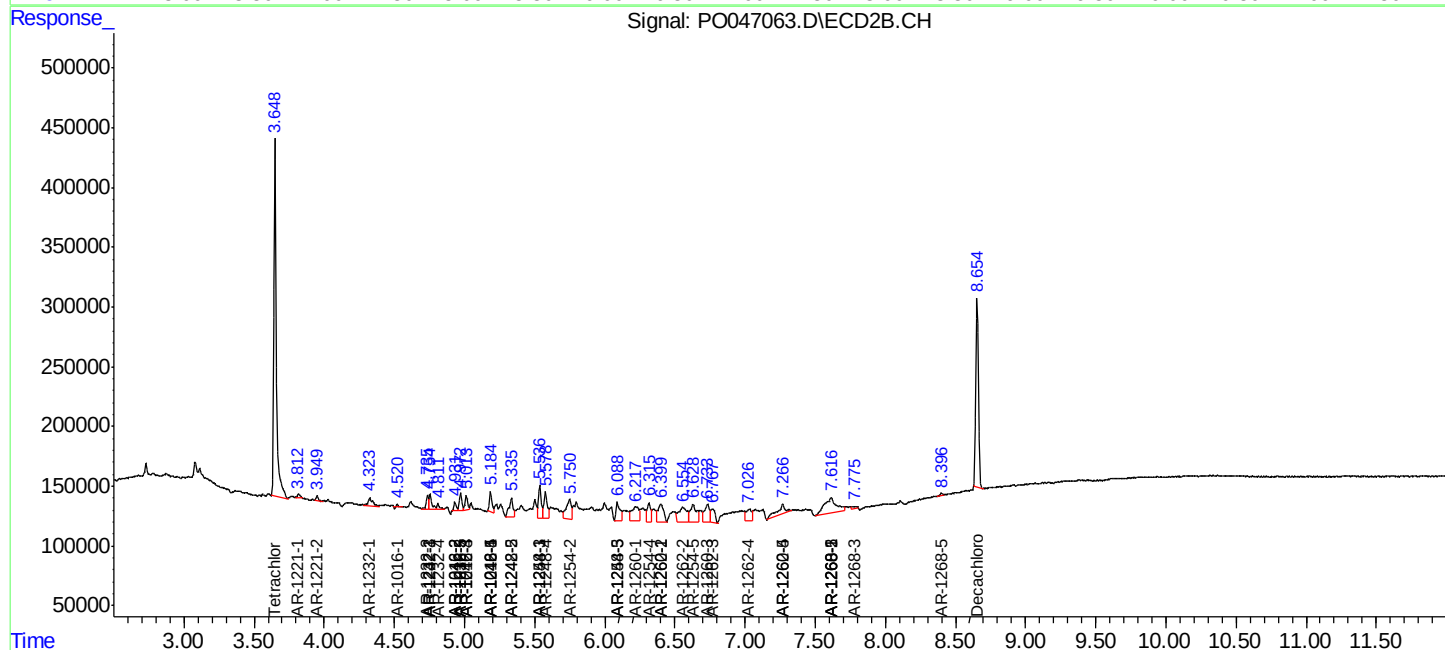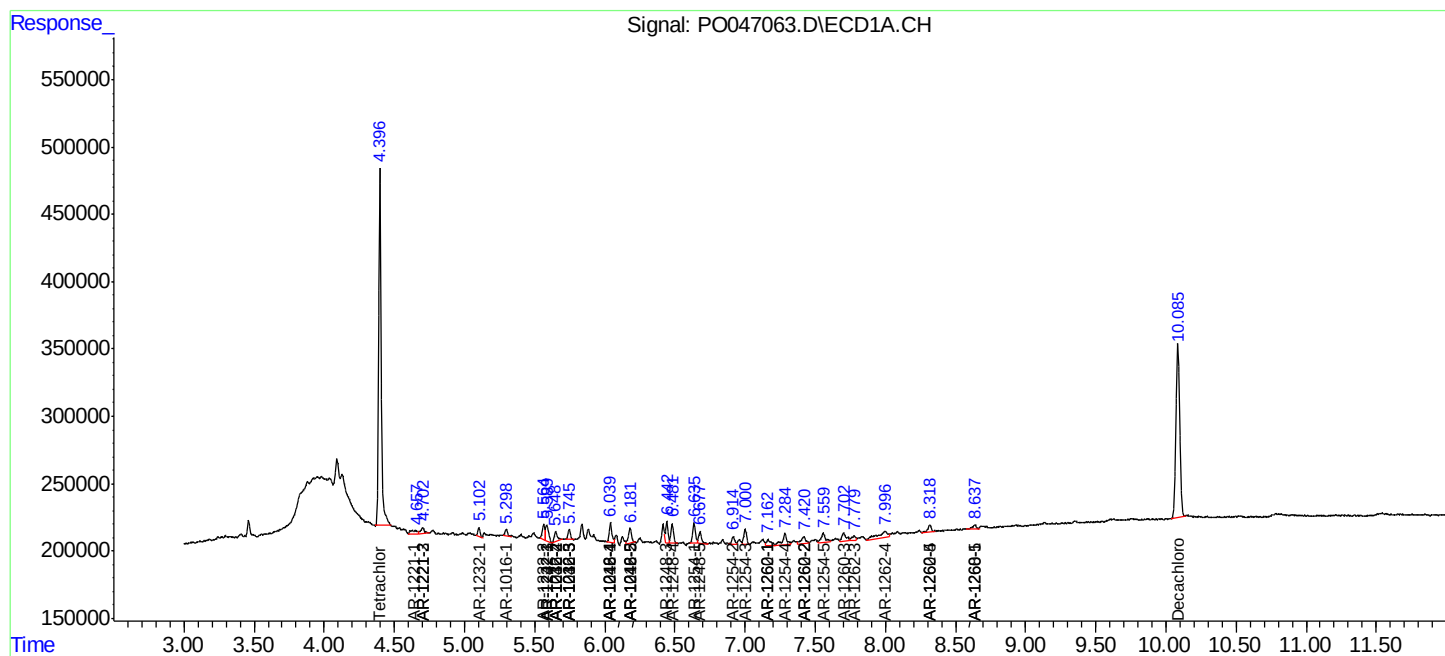


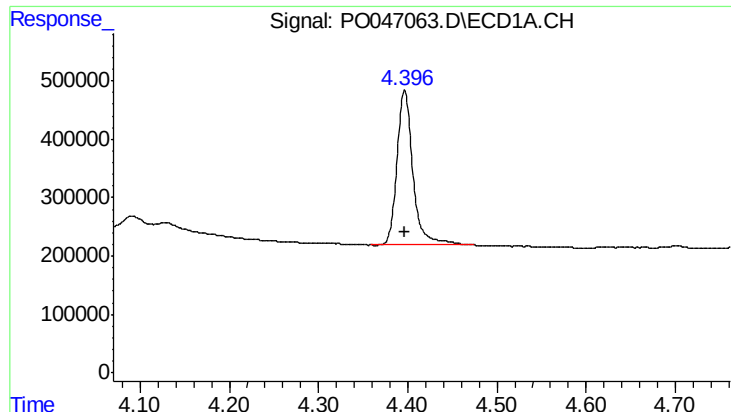

#1 Tetrachloro-m-xylene


R.T.: 4.397 min
Delta R.T.: 0.000 min
Response: 3303534
Conc: 19.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248 MDL WATER

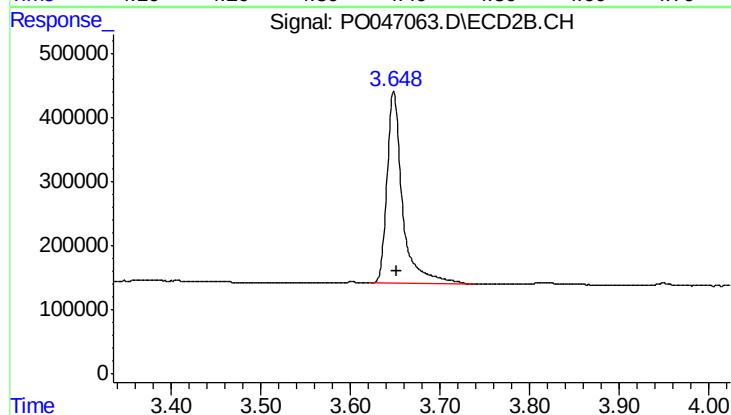


#1 Tetrachloro-m-xylene

R.T.: 3.648 min
Delta R.T.: -0.003 min
Response: 3637564
Conc: 18.97 ng/ml

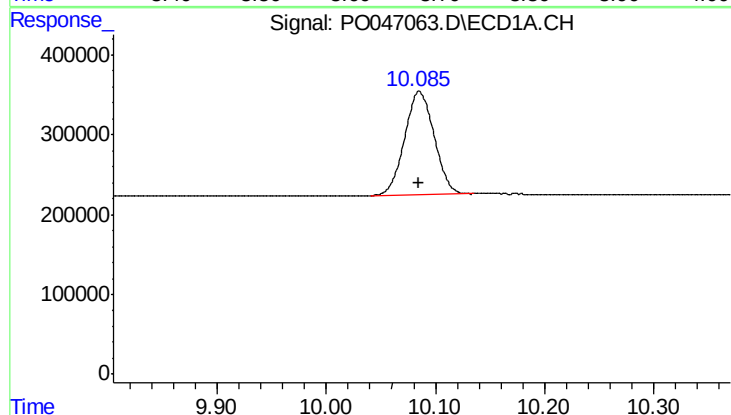


#2 Decachlorobiphenyl

R.T.: 10.085 min
Delta R.T.: 0.000 min
Response: 2445481
Conc: 22.34 ng/ml

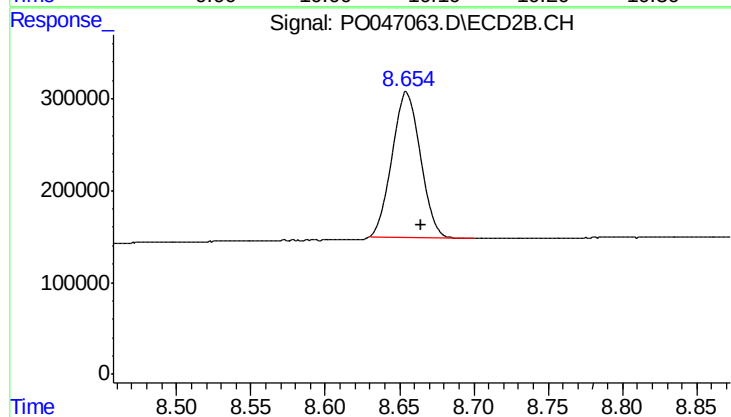

#2 Decachlorobiphenyl


R.T.: 8.655 min
Delta R.T.: -0.010 min
Response: 2097336
Conc: 22.84 ng/ml

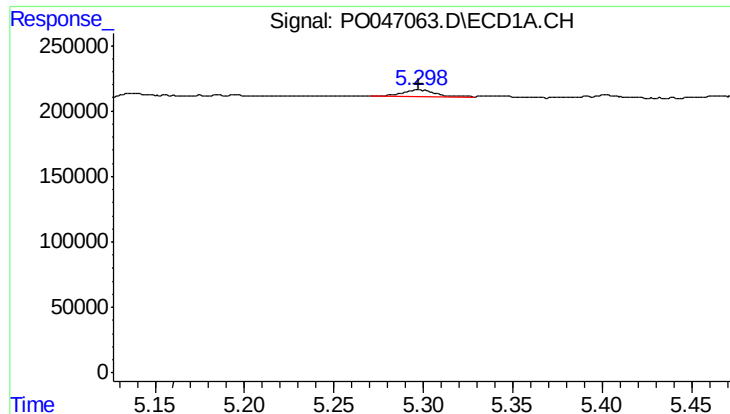

#3 AR-1016-1


R.T.: 5.298 min
Delta R.T.: 0.000 min
Response: 62032
Conc: 19.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248 MDL WATER

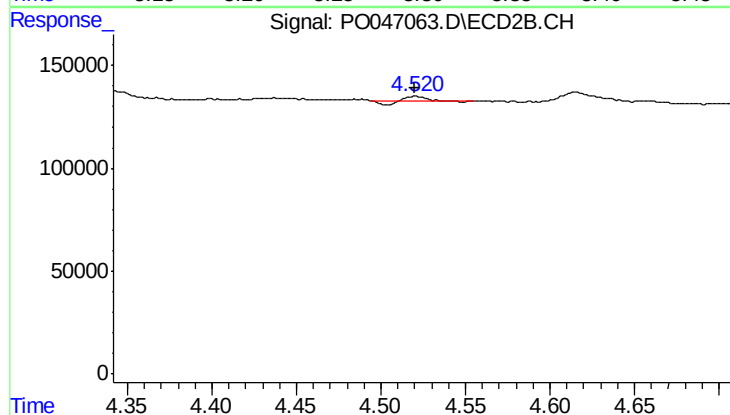


#3 AR-1016-1

R.T.: 4.520 min
Delta R.T.: 0.000 min
Response: 5393
Conc: 1.59 ng/ml

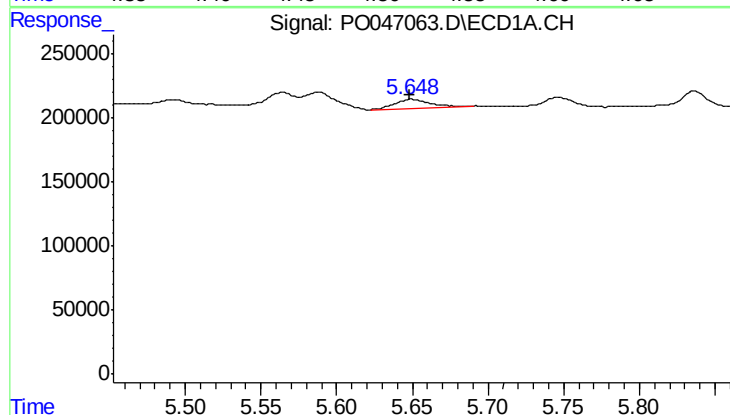


#4 AR-1016-2

R.T.: 5.649 min
Delta R.T.: 0.000 min
Response: 109114
Conc: 27.89 ng/ml

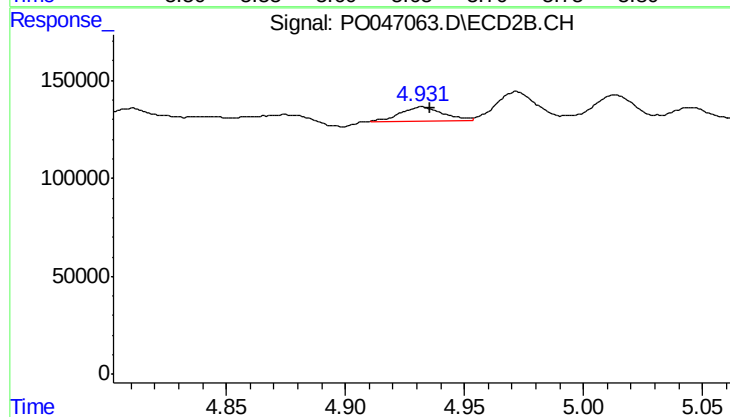

#4 AR-1016-2


R.T.: 4.932 min
Delta R.T.: -0.003 min
Response: 90312
Conc: 28.07 ng/ml

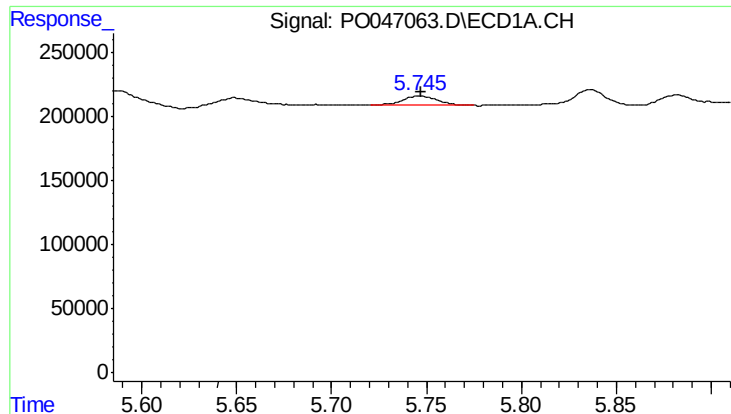

#5 AR-1016-3


R.T.: 5.746 min
Delta R.T.: -0.001 min
Response: 83209
Conc: 25.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248 MDL WATER

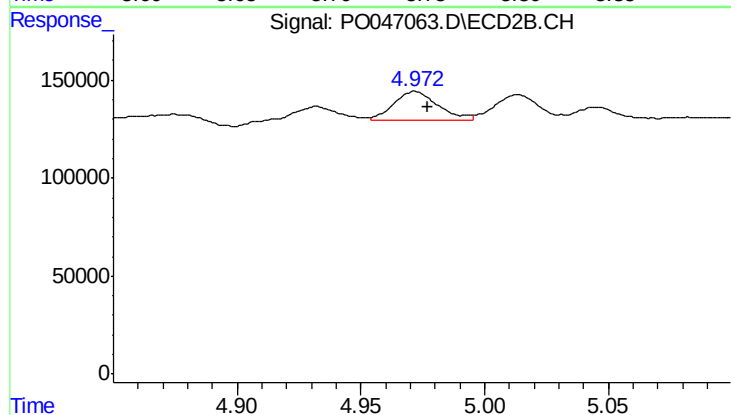


#5 AR-1016-3

R.T.: 4.972 min
Delta R.T.: -0.005 min
Response: 179308
Conc: 68.30 ng/ml

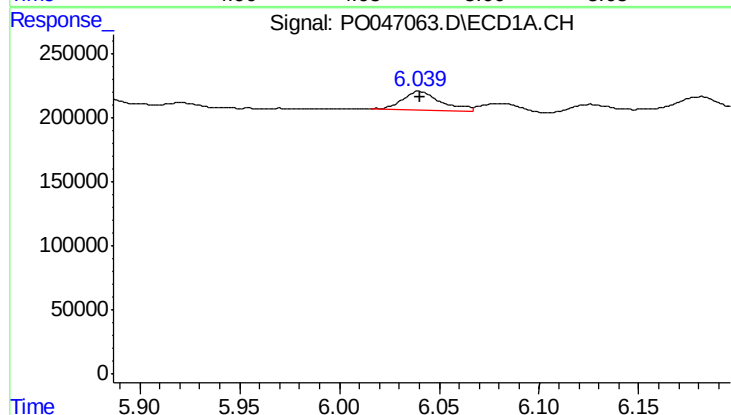


#6 AR-1016-4

R.T.: 6.040 min
Delta R.T.: 0.000 min
Response: 193395
Conc: 61.29 ng/ml

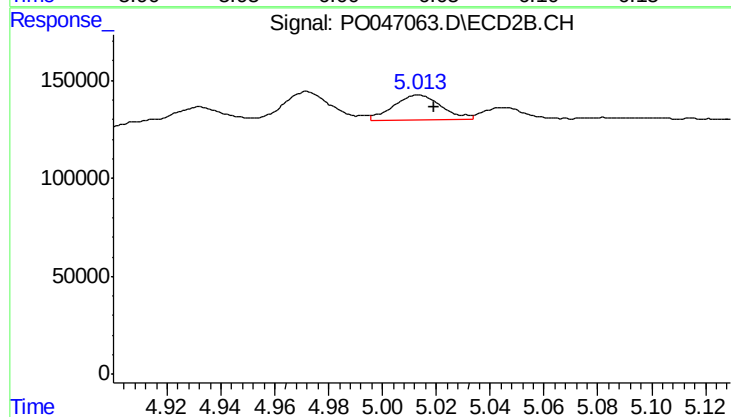

#6 AR-1016-4


R.T.: 5.013 min
Delta R.T.: -0.006 min
Response: 154589
Conc: 49.69 ng/ml

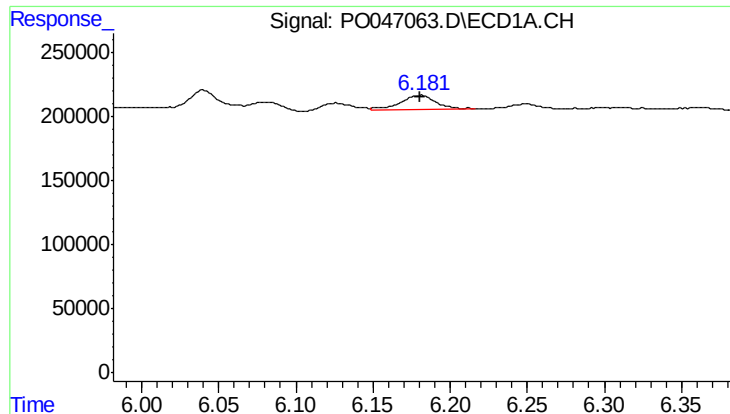

#7 AR-1016-5


R.T.: 6.180 min
Delta R.T.: 0.000 min
Response: 177044
Conc: 53.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248 MDL WATER

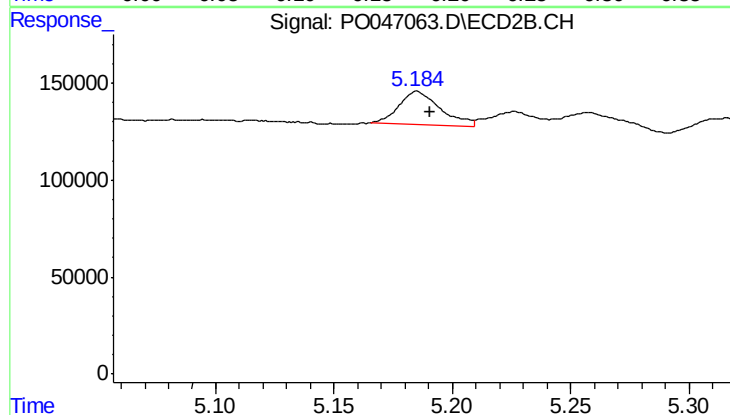


#7 AR-1016-5

R.T.: 5.185 min
Delta R.T.: -0.005 min
Response: 205372
Conc: 59.47 ng/ml

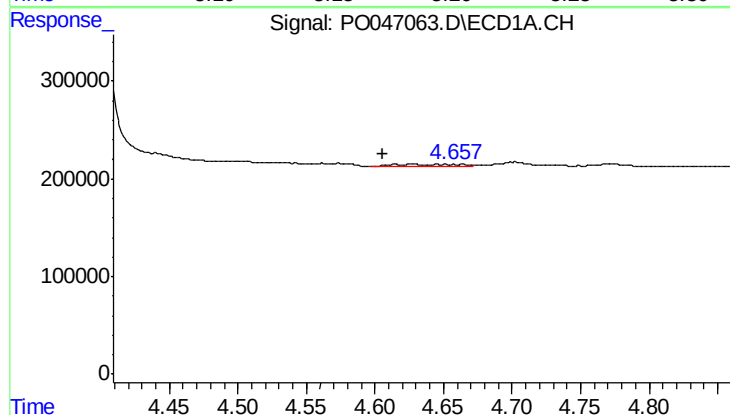


#8 AR-1221-1

R.T.: 4.645 min
Delta R.T.: 0.039 min
Response: 80859
Conc: 49.83 ng/ml

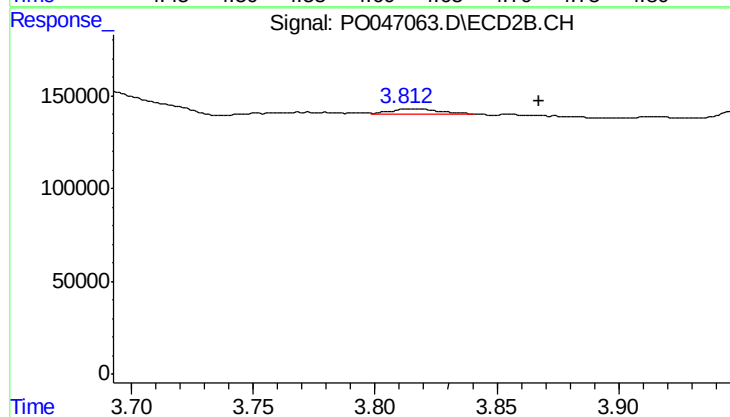

#8 AR-1221-1


R.T.: 3.815 min
Delta R.T.: -0.052 min
Response: 35873
Conc: 21.53 ng/ml

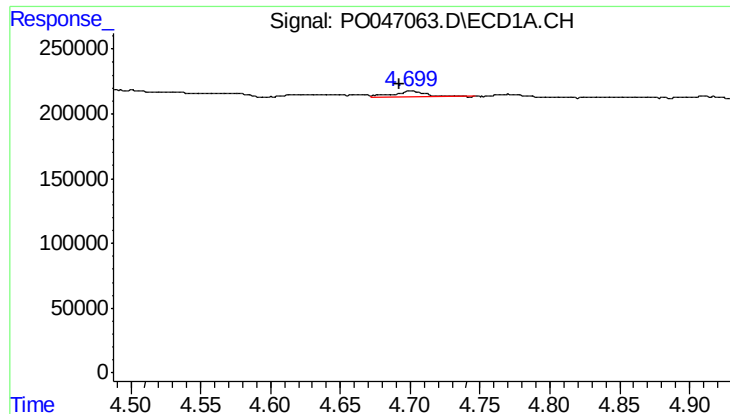

#9 AR-1221-2


R.T.: 4.702 min
Delta R.T.: 0.009 min
Response: 72320
Conc: 60.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248 MDL WATER

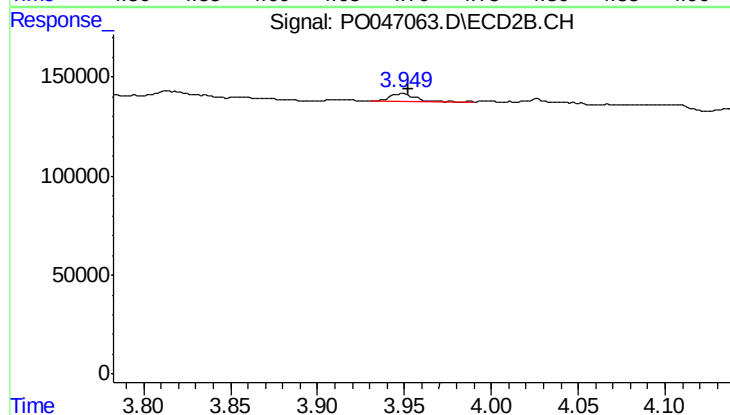


#9 AR-1221-2

R.T.: 3.948 min
Delta R.T.: -0.004 min
Response: 38677
Conc: 32.28 ng/ml

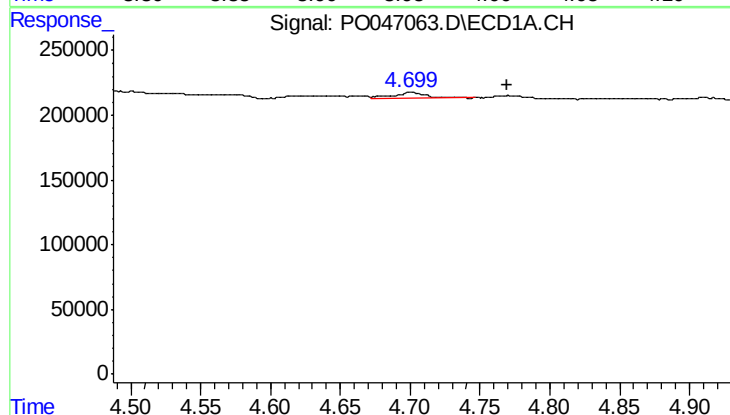


#10 AR-1221-3

R.T.: 4.702 min
Delta R.T.: -0.008 min
Response: 72320
Conc: 19.51 ng/ml

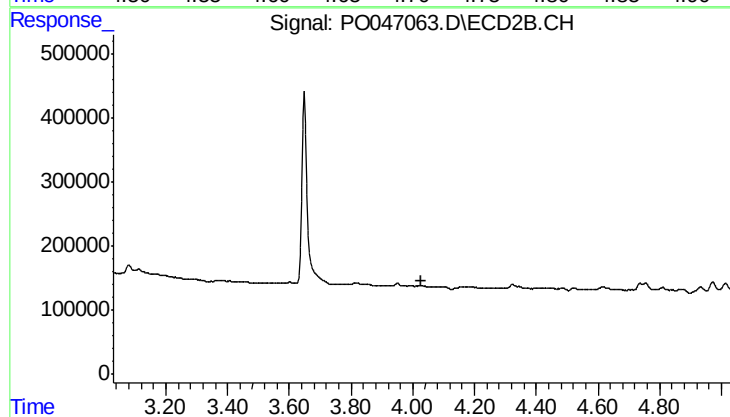

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 4.029 min
Response: 0
Conc: N.D.

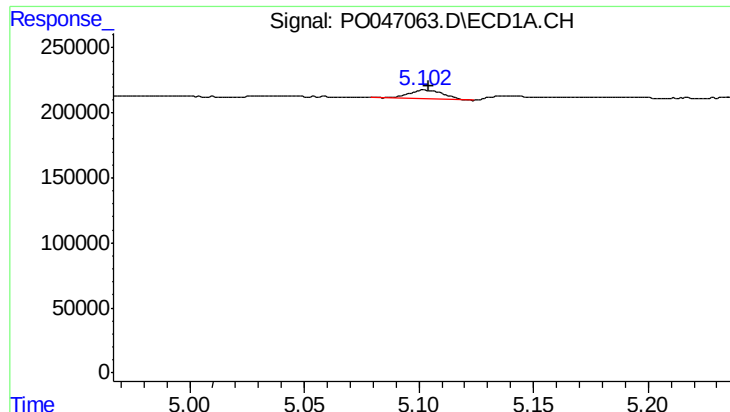

#11 AR-1232-1


R.T.: 5.103 min
Delta R.T.: -0.001 min
Response: 78049
Conc: 52.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248 MDL WATER

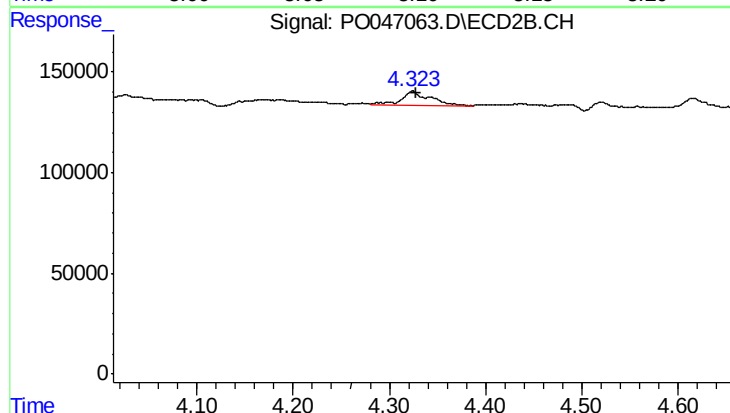


#11 AR-1232-1

R.T.: 4.324 min
Delta R.T.: -0.004 min
Response: 143576
Conc: 91.35 ng/ml

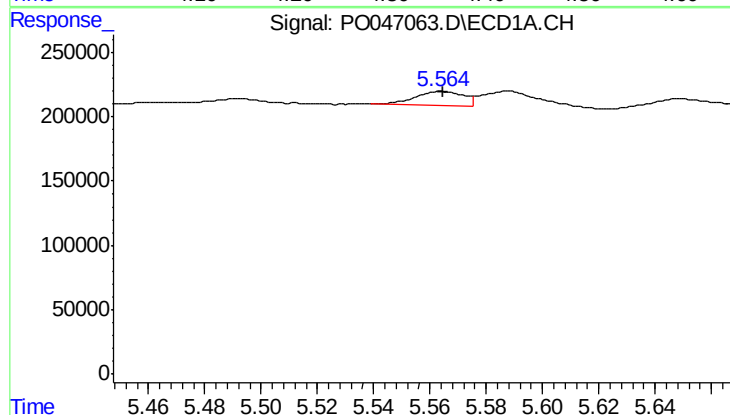


#12 AR-1232-2

R.T.: 5.564 min
Delta R.T.: 0.000 min
Response: 127397
Conc: 62.52 ng/ml

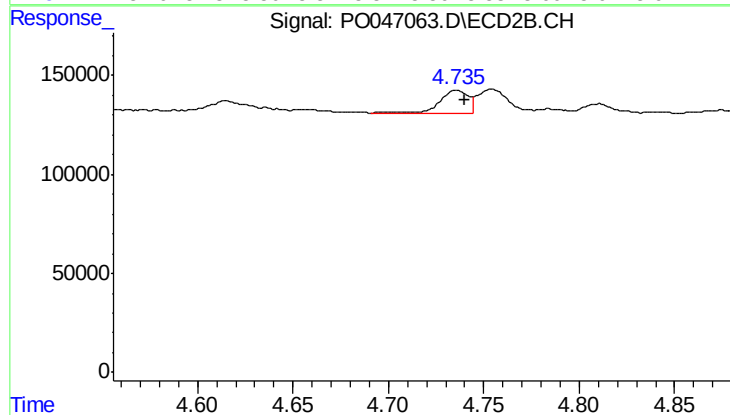

#12 AR-1232-2


R.T.: 4.736 min
Delta R.T.: -0.004 min
Response: 123311
Conc: 61.84 ng/ml

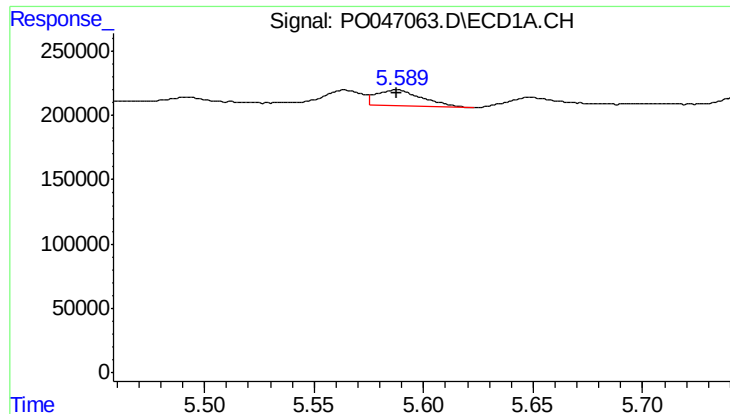

#13 AR-1232-3


R.T.: 5.587 min
Delta R.T.: 0.000 min
Response: 176346
Conc: 60.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248 MDL WATER

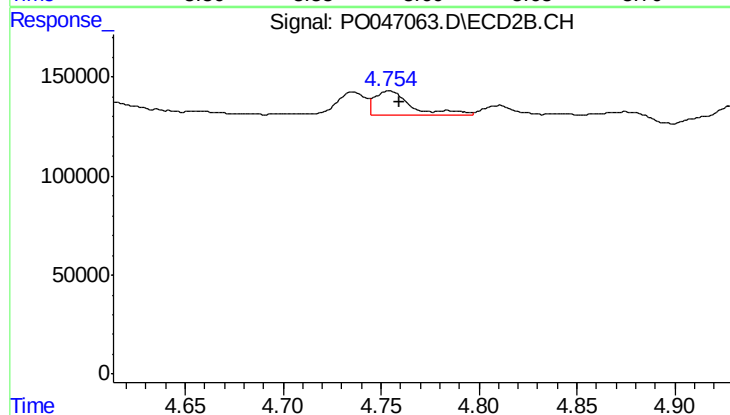


#13 AR-1232-3

R.T.: 4.754 min
Delta R.T.: -0.005 min
Response: 160269
Conc: 51.85 ng/ml

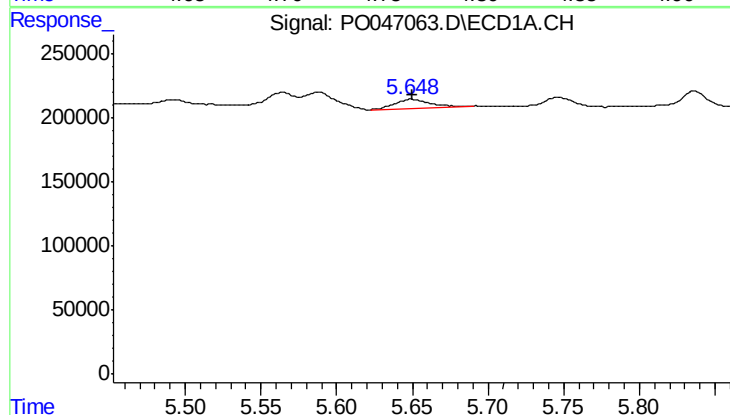


#14 AR-1232-4

R.T.: 5.649 min
Delta R.T.: 0.000 min
Response: 109114
Conc: 61.15 ng/ml

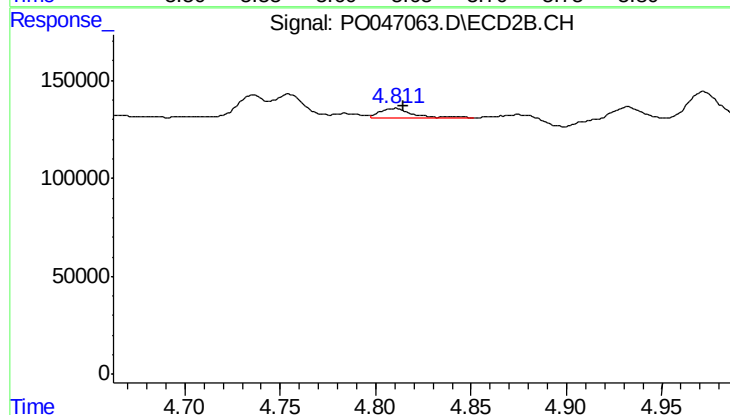

#14 AR-1232-4


R.T.: 4.810 min
Delta R.T.: -0.004 min
Response: 59780
Conc: 32.79 ng/ml

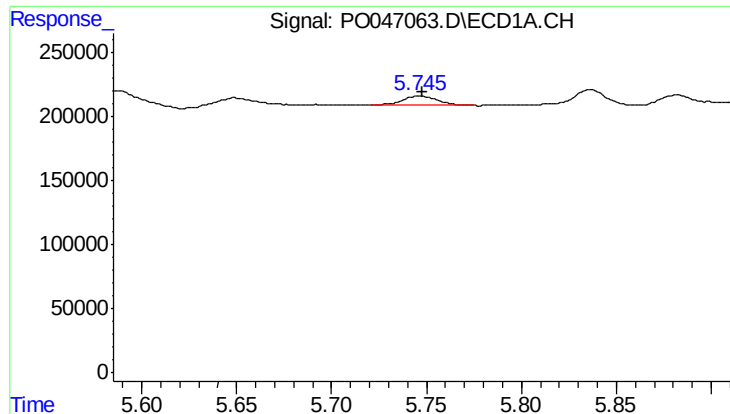

#15 AR-1232-5


R.T.: 5.746 min
Delta R.T.: -0.002 min
Response: 83209
Conc: 58.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248 MDL WATER

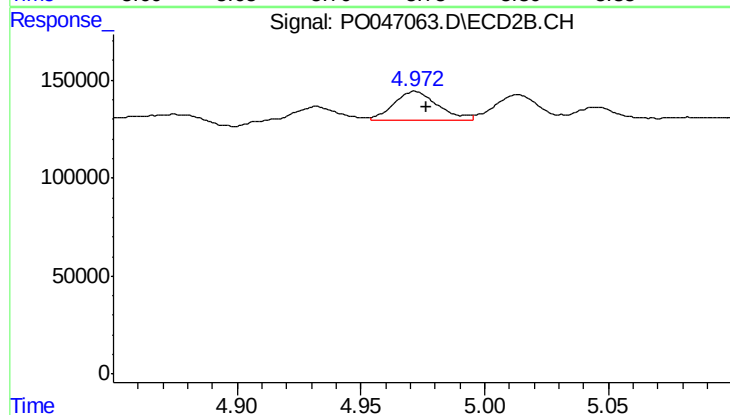


#15 AR-1232-5

R.T.: 4.972 min
Delta R.T.: -0.004 min
Response: 179308
Conc: 178.40 ng/ml

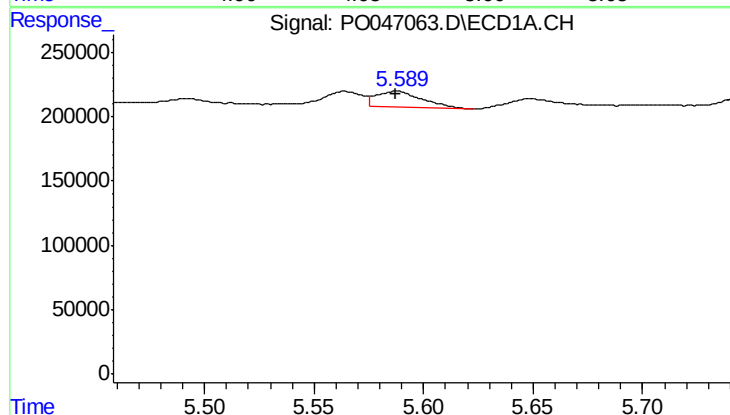


#16 AR-1242-1

R.T.: 5.587 min
Delta R.T.: 0.000 min
Response: 176346
Conc: 30.42 ng/ml

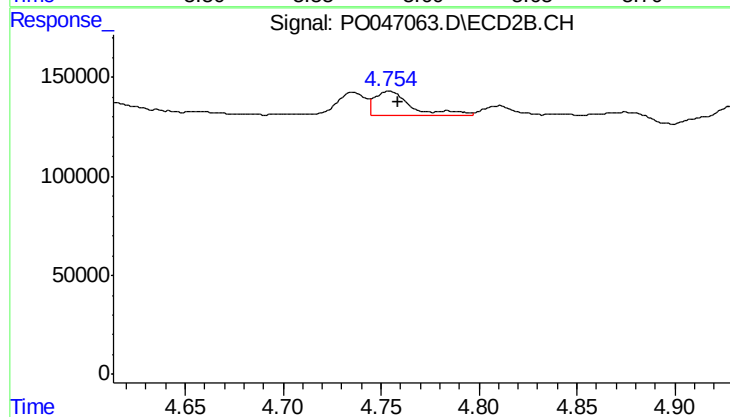

#16 AR-1242-1


R.T.: 4.754 min
Delta R.T.: -0.004 min
Response: 160269
Conc: 27.86 ng/ml

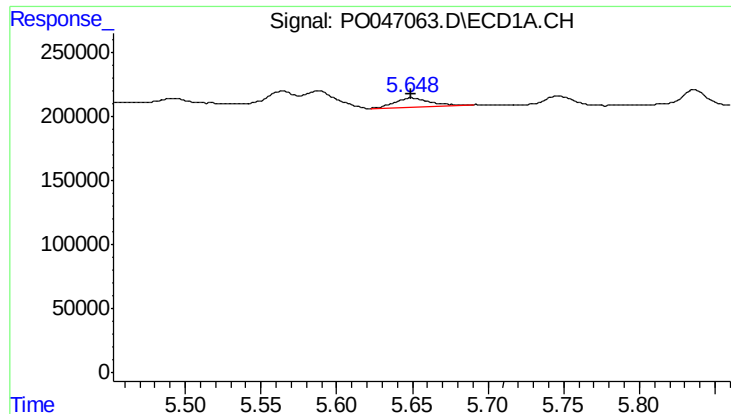

#17 AR-1242-2


R.T.: 5.649 min
Delta R.T.: 0.000 min
Response: 109114
Conc: 30.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248 MDL WATER

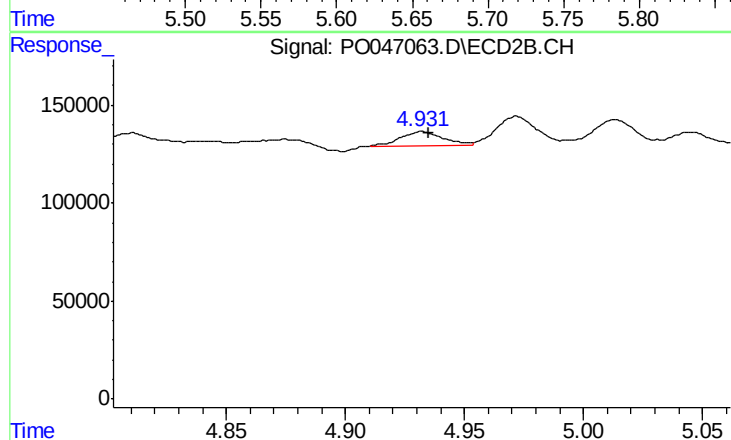


#17 AR-1242-2

R.T.: 4.932 min
Delta R.T.: -0.003 min
Response: 90312
Conc: 31.39 ng/ml

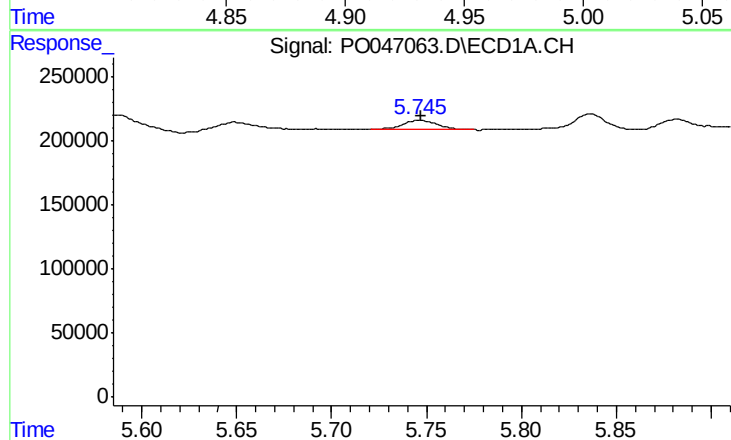


#18 AR-1242-3

R.T.: 5.746 min
Delta R.T.: -0.001 min
Response: 83209
Conc: 29.32 ng/ml

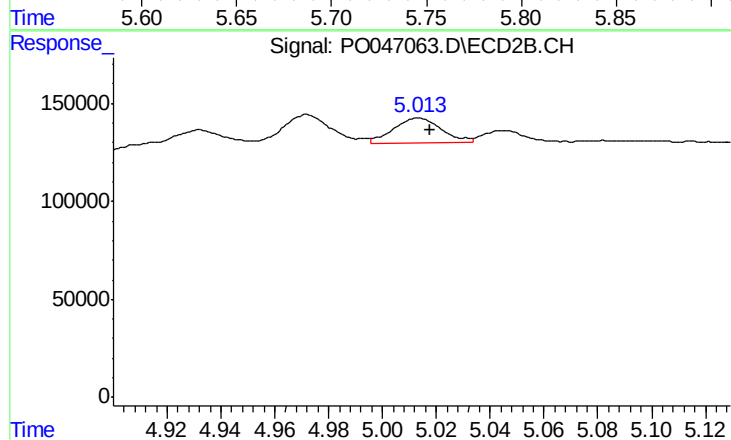

#18 AR-1242-3


R.T.: 5.013 min
Delta R.T.: -0.004 min
Response: 154589
Conc: 54.12 ng/ml

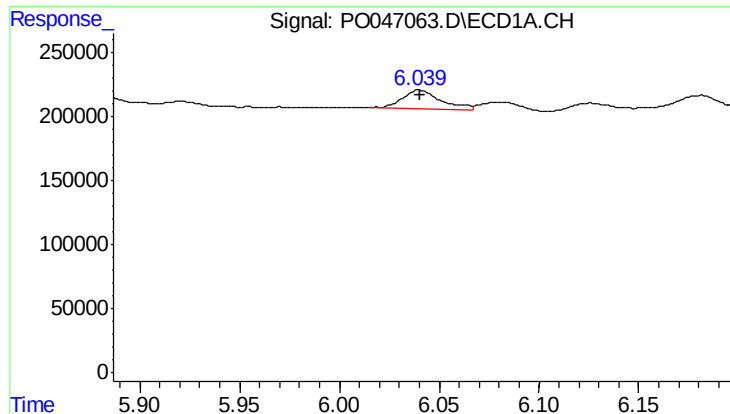

#19 AR-1242-4


R.T.: 6.040 min
Delta R.T.: 0.000 min
Response: 193395
Conc: 67.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248 MDL WATER

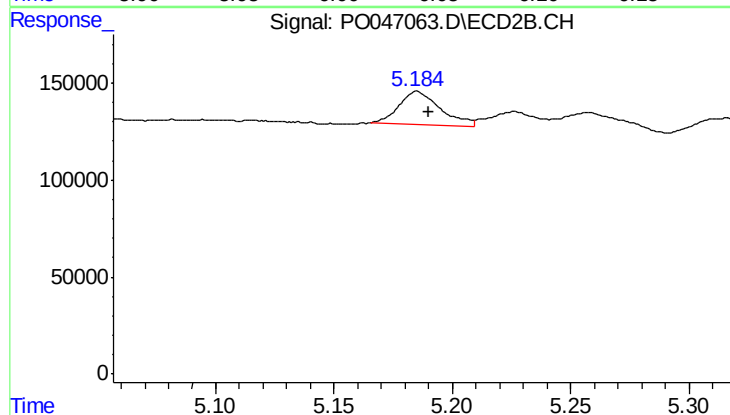


#19 AR-1242-4

R.T.: 5.185 min
Delta R.T.: -0.005 min
Response: 205372
Conc: 67.22 ng/ml

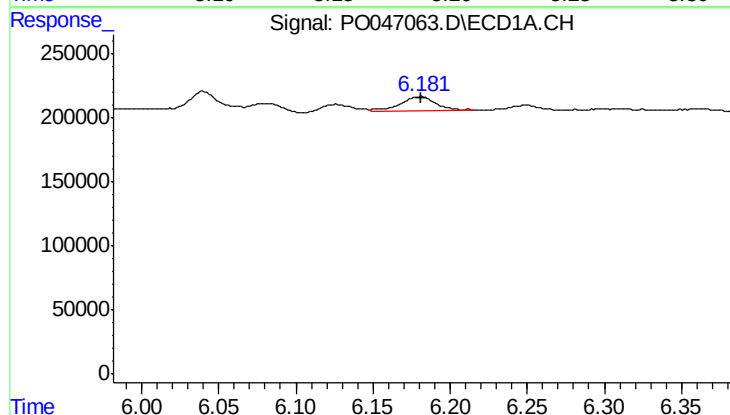


#20 AR-1242-5

R.T.: 6.180 min
Delta R.T.: 0.000 min
Response: 177044
Conc: 57.15 ng/ml

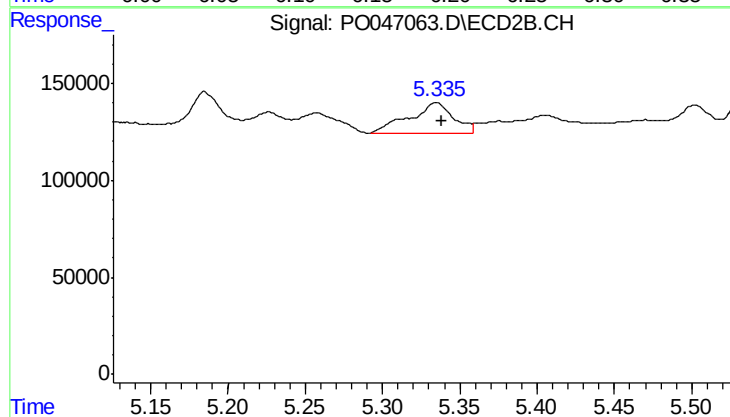

#20 AR-1242-5


R.T.: 5.335 min
Delta R.T.: -0.004 min
Response: 317154
Conc: 98.17 ng/ml

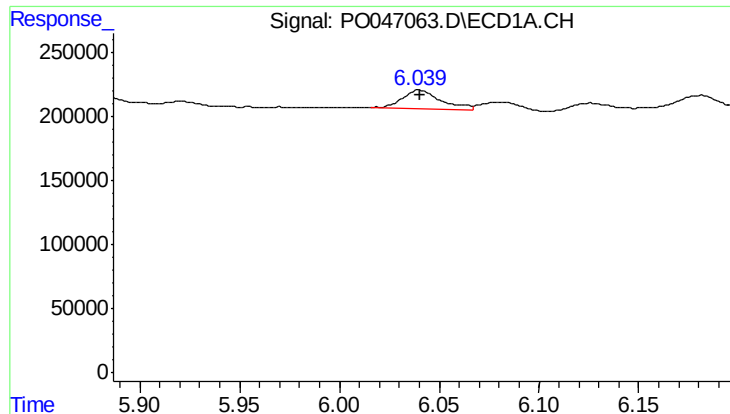

#21 AR-1248-1


R.T.: 6.040 min
Delta R.T.: 0.000 min
Response: 193395
Conc: 41.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248 MDL WATER

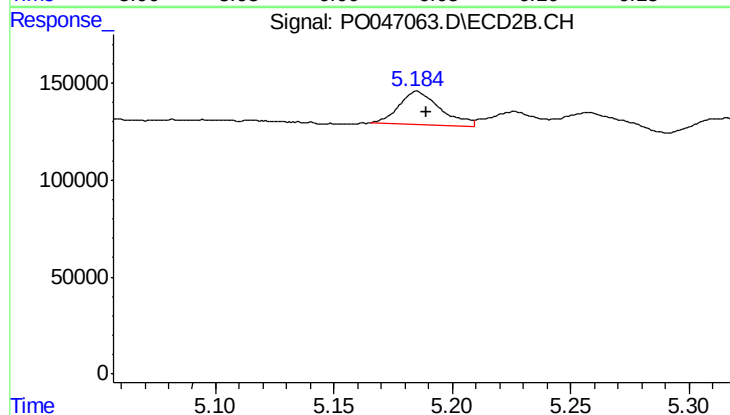


#21 AR-1248-1

R.T.: 5.185 min
Delta R.T.: -0.004 min
Response: 205372
Conc: 40.97 ng/ml

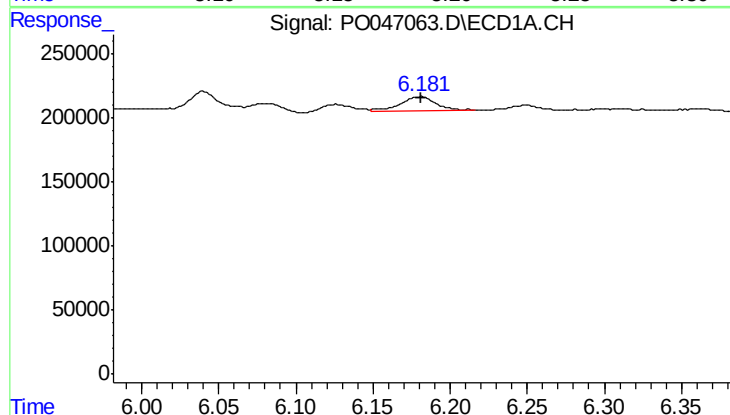


#22 AR-1248-2

R.T.: 6.180 min
Delta R.T.: 0.000 min
Response: 177044
Conc: 44.67 ng/ml

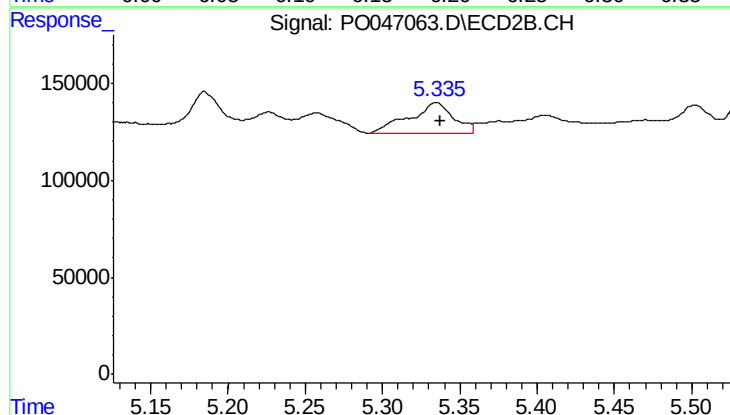

#22 AR-1248-2


R.T.: 5.335 min
Delta R.T.: -0.003 min
Response: 317154
Conc: 75.68 ng/ml

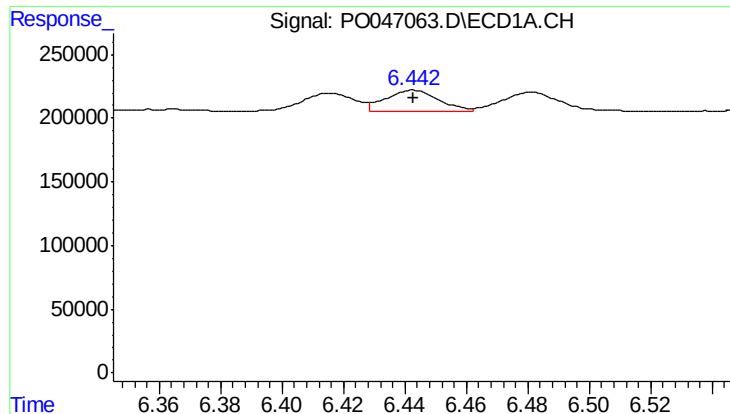

#23 AR-1248-3


R.T.: 6.443 min
Delta R.T.: 0.000 min
Response: 197607
Conc: 38.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248 MDL WATER

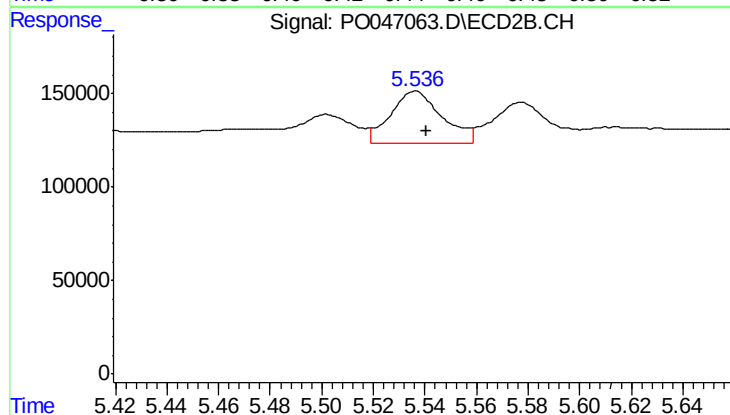


#23 AR-1248-3

R.T.: 5.536 min
Delta R.T.: -0.004 min
Response: 392027
Conc: 61.15 ng/ml

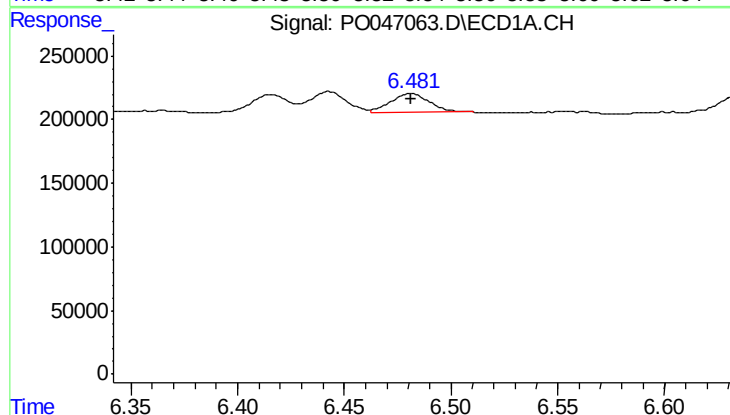


#24 AR-1248-4

R.T.: 6.481 min
Delta R.T.: 0.000 min
Response: 183311
Conc: 38.38 ng/ml

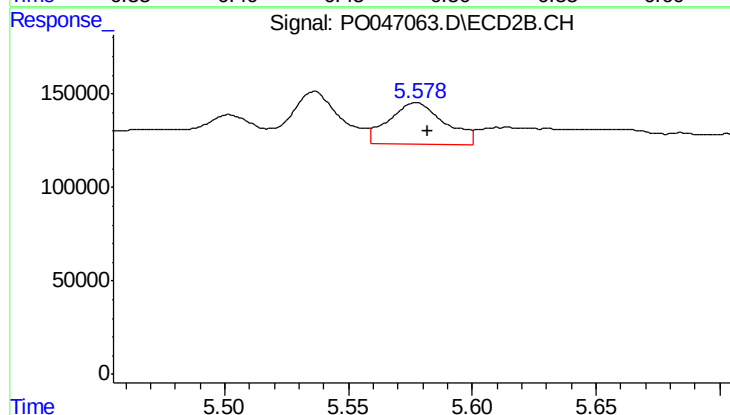

#24 AR-1248-4


R.T.: 5.577 min
Delta R.T.: -0.004 min
Response: 349101
Conc: 78.00 ng/ml

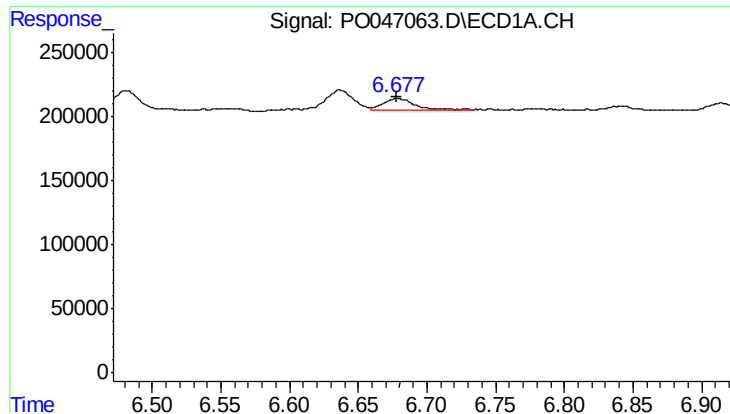

#25 AR-1248-5


R.T.: 6.678 min
Delta R.T.: 0.000 min
Response: 134002
Conc: 41.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248 MDL WATER

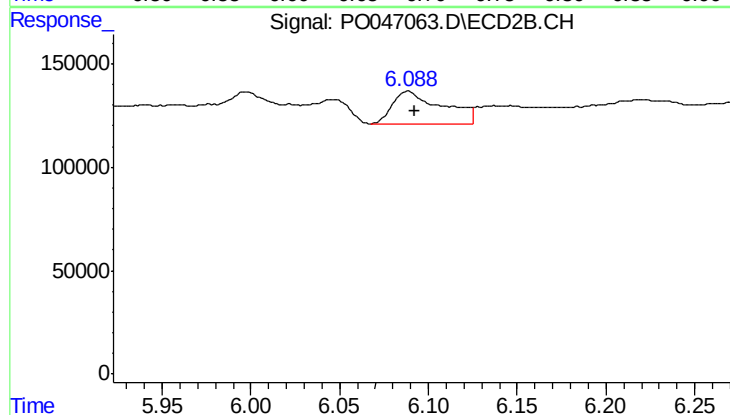


#25 AR-1248-5

R.T.: 6.088 min
Delta R.T.: -0.004 min
Response: 309503
Conc: 111.85 ng/ml

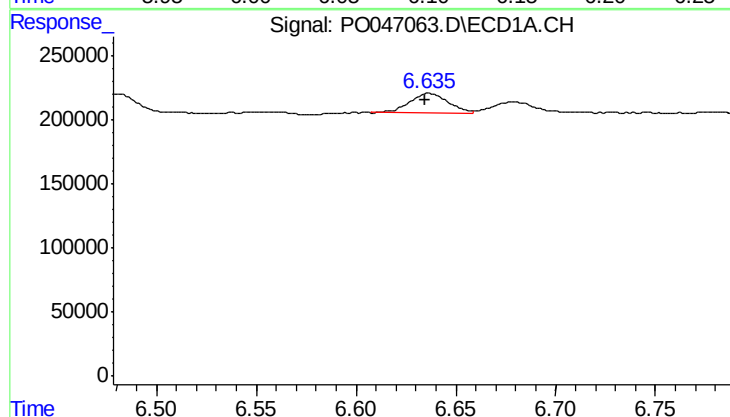


#26 AR-1254-1

R.T.: 6.637 min
Delta R.T.: 0.003 min
Response: 204539
Conc: 24.88 ng/ml

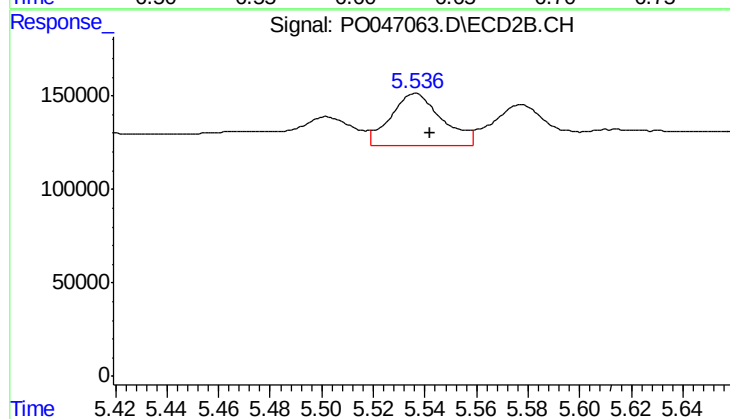

#26 AR-1254-1


R.T.: 5.536 min
Delta R.T.: -0.006 min
Response: 392027
Conc: 54.88 ng/ml

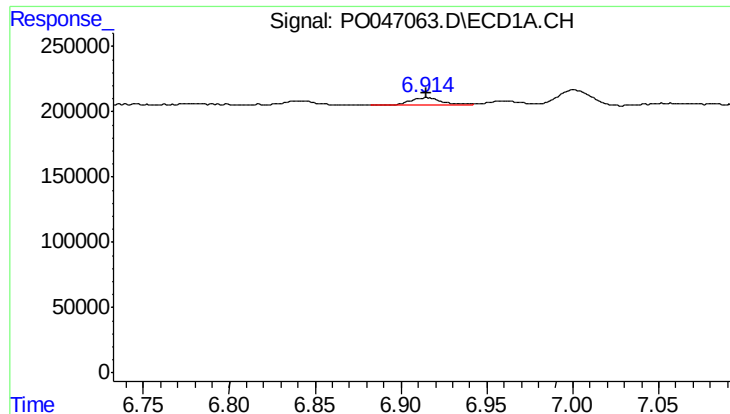

#27 AR-1254-2


R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 84731
Conc: 17.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248 MDL WATER

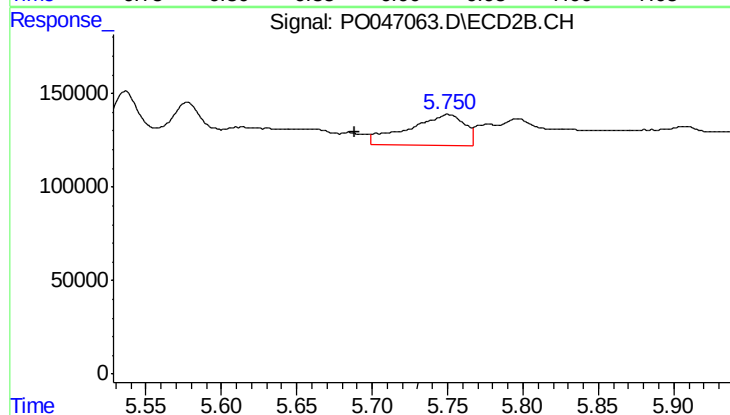


#27 AR-1254-2

R.T.: 5.750 min
Delta R.T.: 0.062 min
Response: 429908
Conc: 70.98 ng/ml

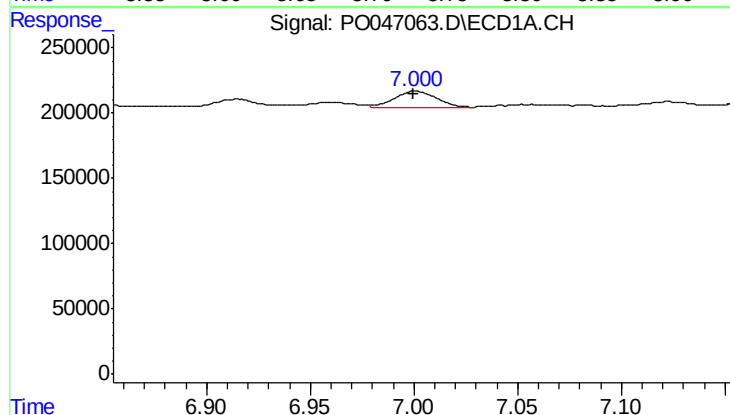


#28 AR-1254-3

R.T.: 7.001 min
Delta R.T.: 0.000 min
Response: 168341
Conc: 19.59 ng/ml

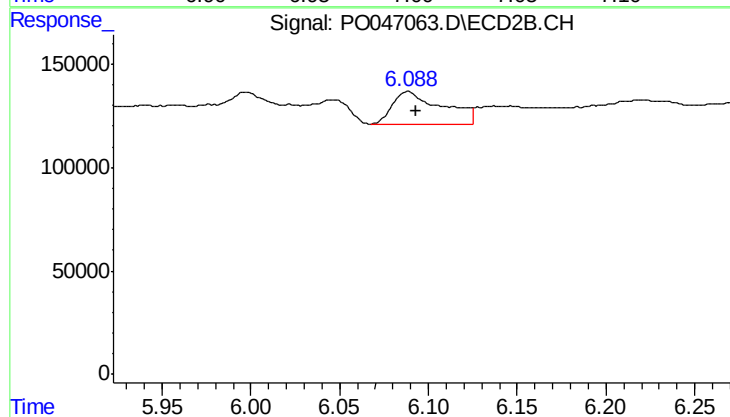

#28 AR-1254-3


R.T.: 6.088 min
Delta R.T.: -0.004 min
Response: 309503
Conc: 32.87 ng/ml

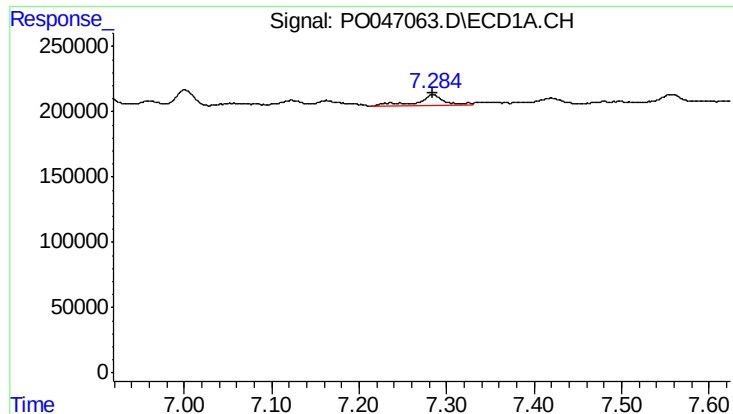

#29 AR-1254-4


R.T.: 7.284 min
Delta R.T.: 0.000 min
Response: 210030
Conc: 32.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248 MDL WATER

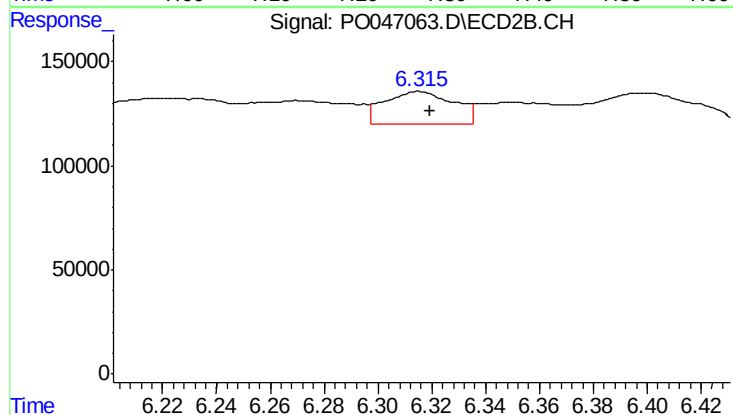


#29 AR-1254-4

R.T.: 6.315 min
Delta R.T.: -0.004 min
Response: 280143
Conc: 48.57 ng/ml

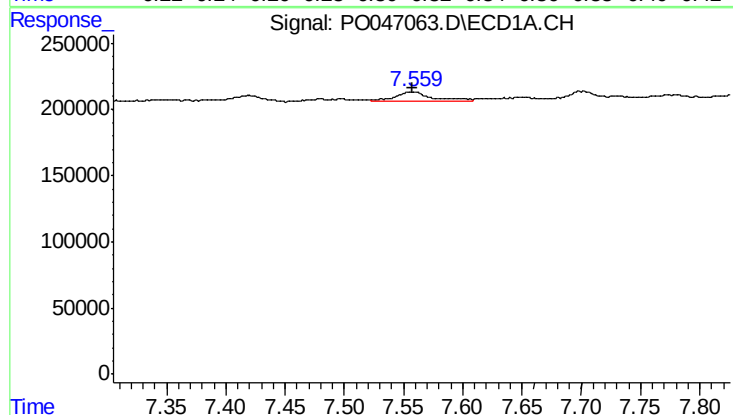


#30 AR-1254-5

R.T.: 7.557 min
Delta R.T.: 0.000 min
Response: 155746
Conc: 32.80 ng/ml

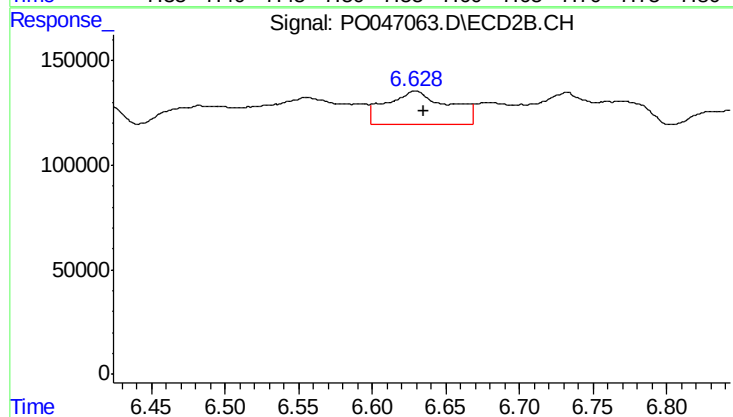

#30 AR-1254-5


R.T.: 6.629 min
Delta R.T.: -0.006 min
Response: 473677
Conc: 119.31 ng/ml

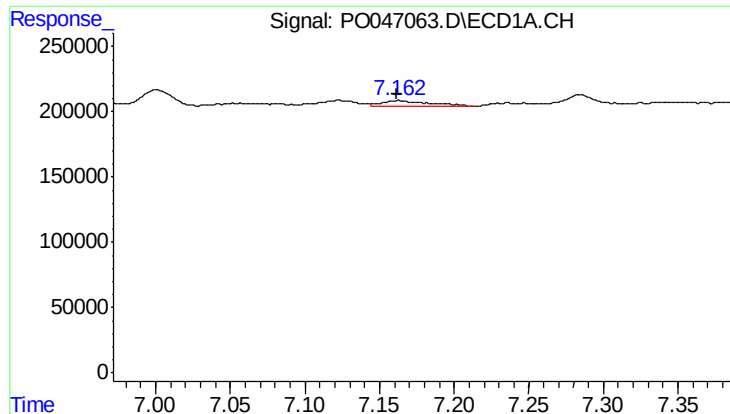

#31 AR-1260-1


R.T.: 7.162 min
Delta R.T.: 0.000 min
Response: 99921
Conc: 16.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248 MDL WATER

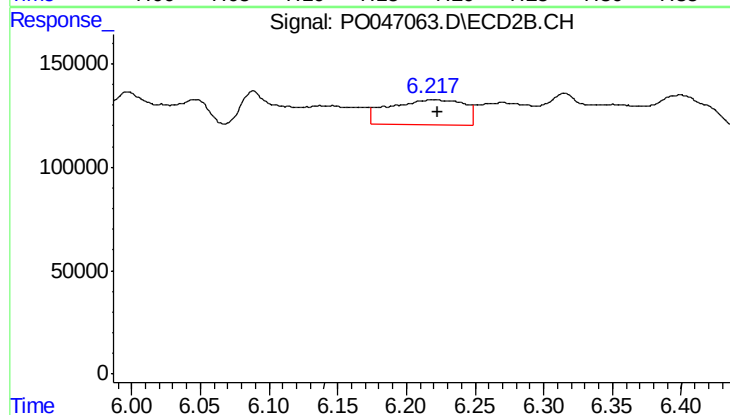


#31 AR-1260-1

R.T.: 6.219 min
Delta R.T.: -0.004 min
Response: 463276
Conc: 78.15 ng/ml

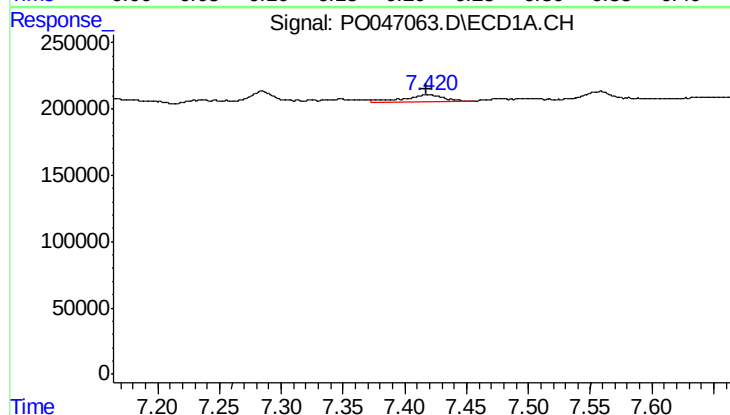


#32 AR-1260-2

R.T.: 7.419 min
Delta R.T.: 0.001 min
Response: 129249
Conc: 17.69 ng/ml

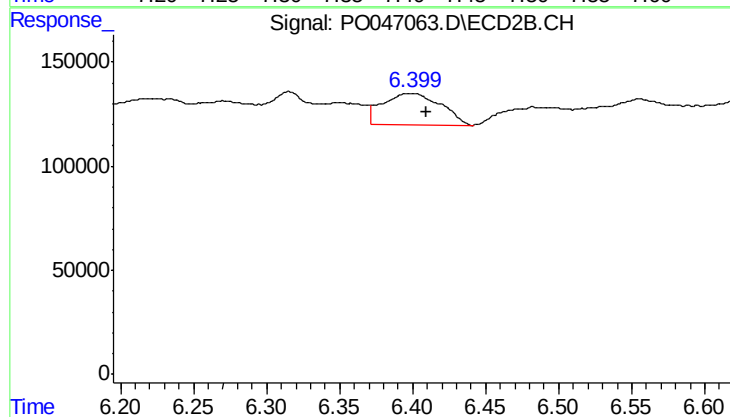

#32 AR-1260-2


R.T.: 6.399 min
Delta R.T.: -0.011 min
Response: 418960
Conc: 59.65 ng/ml

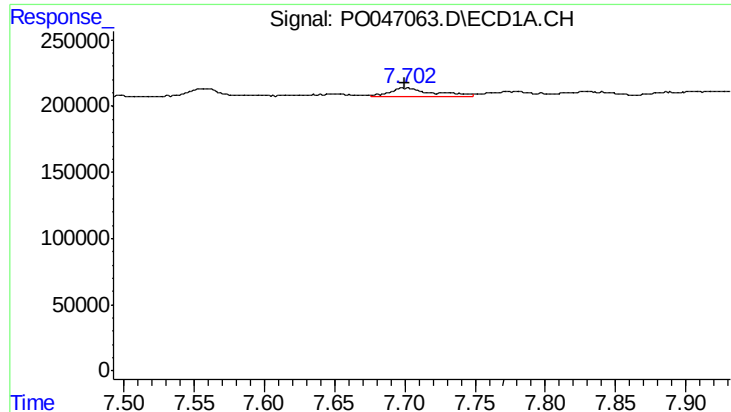

#33 AR-1260-3


R.T.: 7.701 min
Delta R.T.: 0.000 min
Response: 140689
Conc: 16.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248 MDL WATER

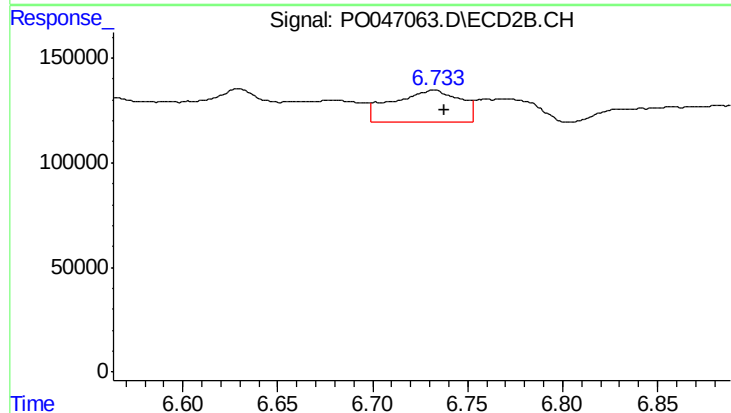


#33 AR-1260-3

R.T.: 6.732 min
Delta R.T.: -0.006 min
Response: 384318
Conc: 51.19 ng/ml

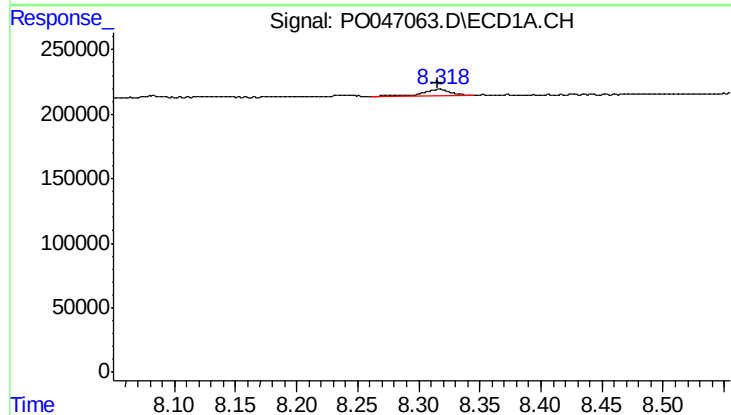


#34 AR-1260-4

R.T.: 8.316 min
Delta R.T.: 0.000 min
Response: 95346
Conc: 7.88 ng/ml

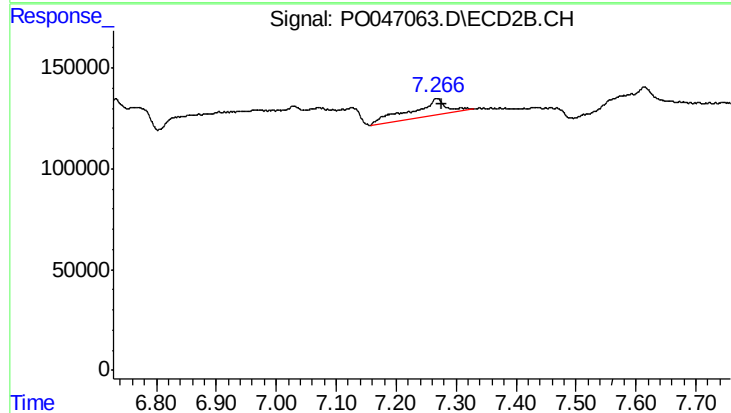

#34 AR-1260-4


R.T.: 7.268 min
Delta R.T.: -0.007 min
Response: 346915
Conc: 29.75 ng/ml

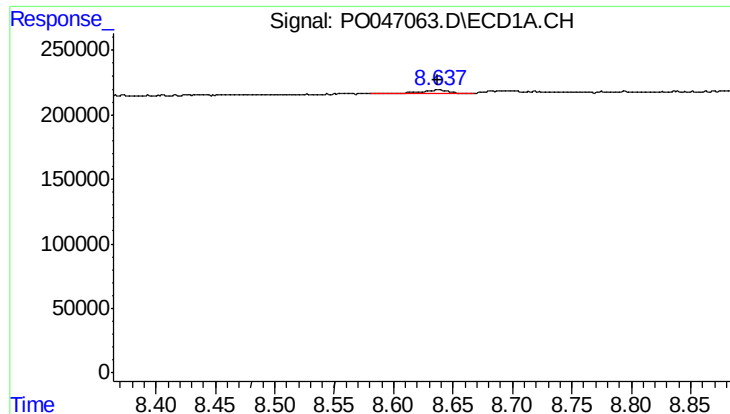

#35 AR-1260-5


R.T.: 8.637 min
Delta R.T.: 0.000 min
Response: 42489
Conc: 5.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248 MDL WATER

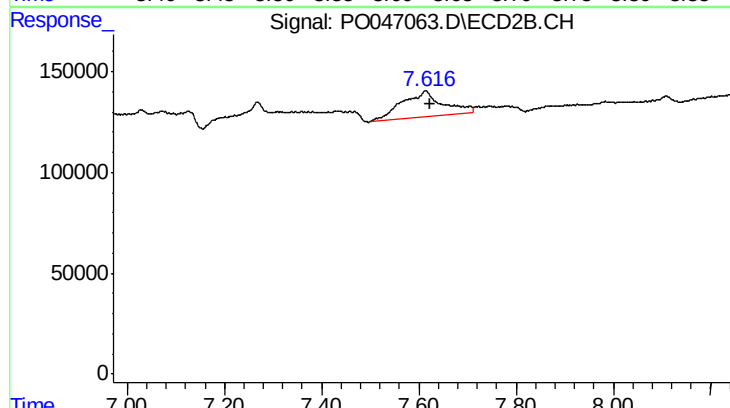


#35 AR-1260-5

R.T.: 7.614 min
Delta R.T.: -0.009 min
Response: 728293
Conc: 87.83 ng/ml

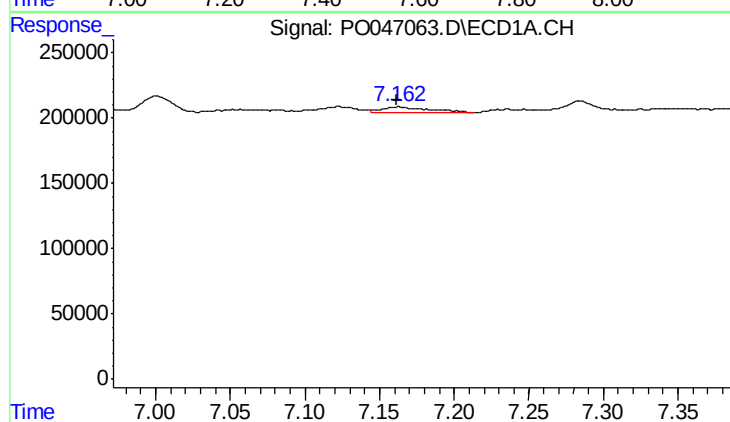


#36 AR-1262-1

R.T.: 7.162 min
Delta R.T.: 0.000 min
Response: 99921
Conc: 18.57 ng/ml

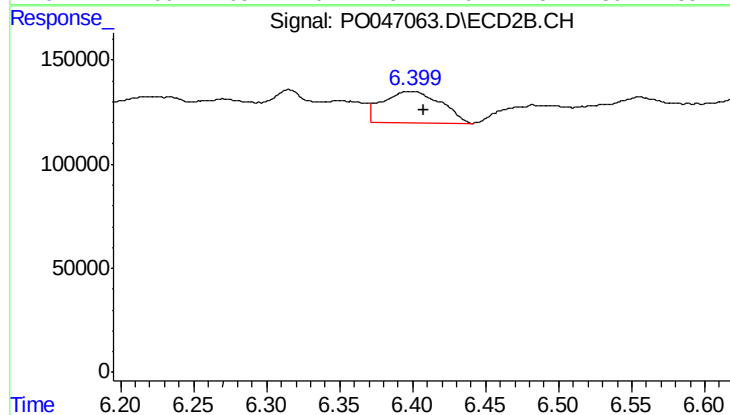

#36 AR-1262-1


R.T.: 6.399 min
Delta R.T.: -0.009 min
Response: 418960
Conc: 67.89 ng/ml

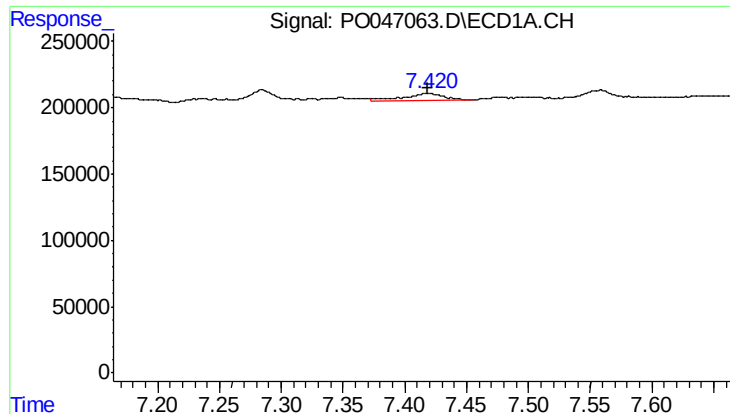

#37 AR-1262-2


R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 129249
Conc: 20.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248 MDL WATER

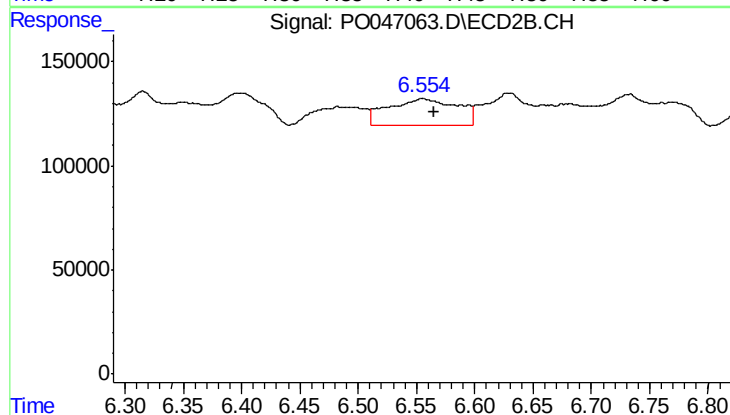


#37 AR-1262-2

R.T.: 6.556 min
Delta R.T.: -0.010 min
Response: 530420
Conc: 86.66 ng/ml

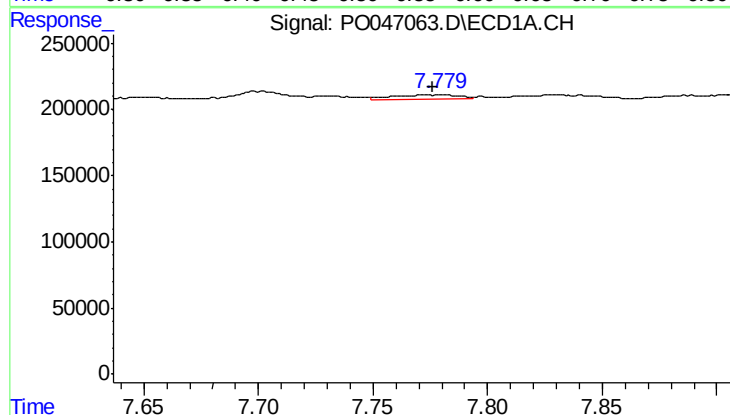


#38 AR-1262-3

R.T.: 7.778 min
Delta R.T.: 0.002 min
Response: 66492
Conc: 8.06 ng/ml

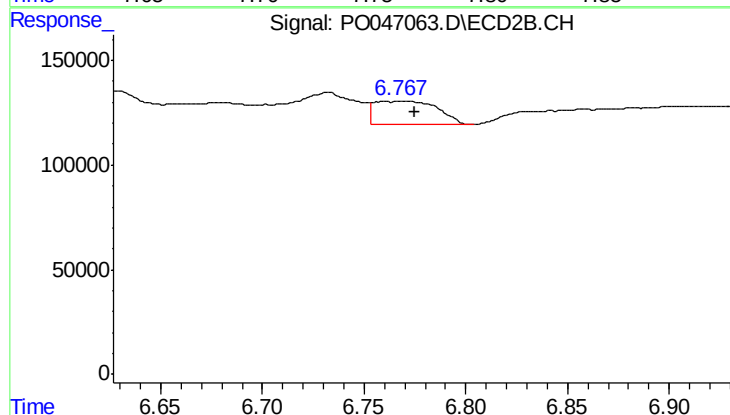

#38 AR-1262-3


R.T.: 6.769 min
Delta R.T.: -0.006 min
Response: 242940
Conc: 29.85 ng/ml

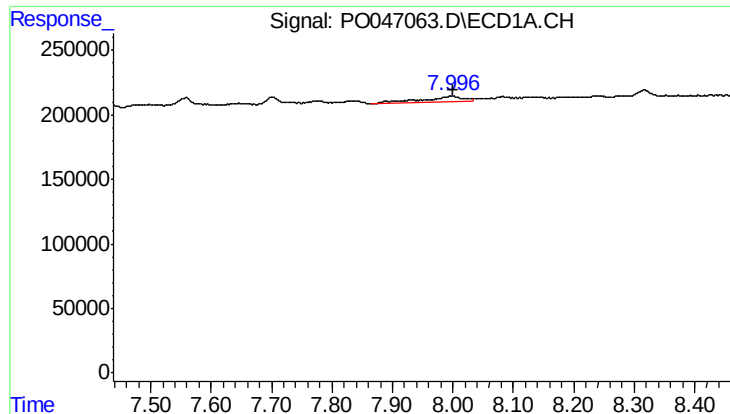

#39 AR-1262-4


R.T.: 7.998 min
Delta R.T.: -0.004 min
Response: 236136
Conc: 29.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248 MDL WATER

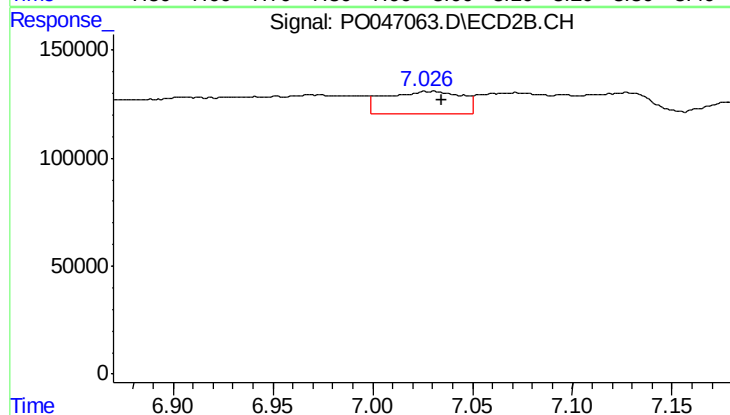


#39 AR-1262-4

R.T.: 7.029 min
Delta R.T.: -0.006 min
Response: 277769
Conc: 39.13 ng/ml

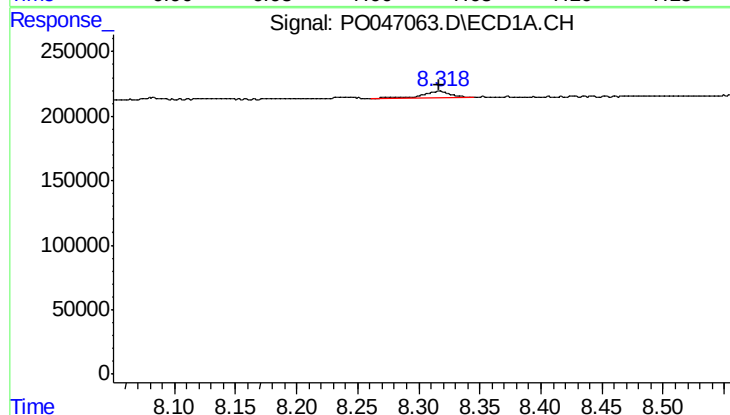


#40 AR-1262-5

R.T.: 8.316 min
Delta R.T.: 0.000 min
Response: 95346
Conc: 6.40 ng/ml

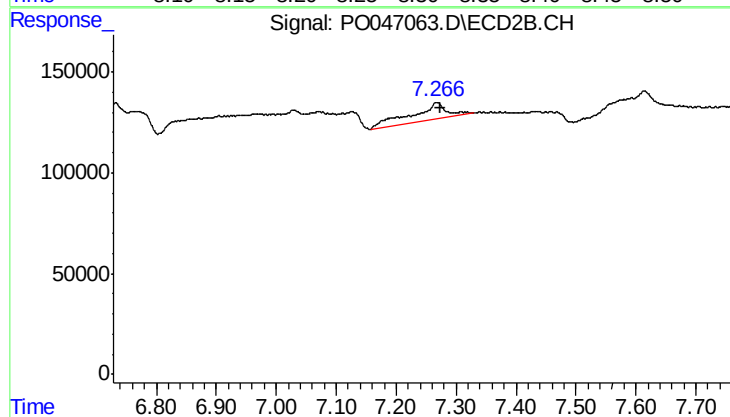

#40 AR-1262-5


R.T.: 7.268 min
Delta R.T.: -0.006 min
Response: 346915
Conc: 24.79 ng/ml

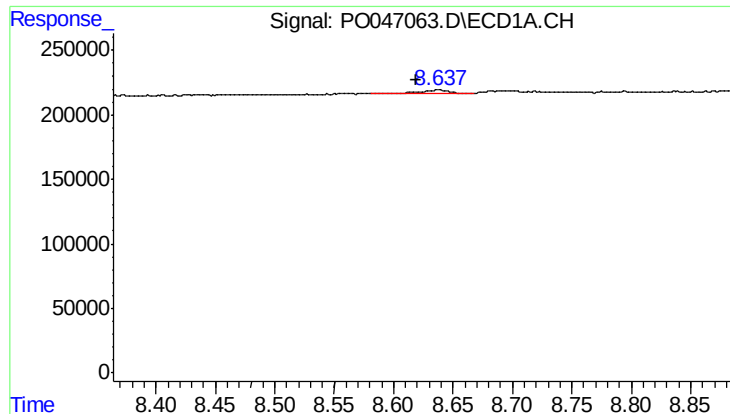

#41 AR-1268-1


R.T.: 8.637 min
Delta R.T.: 0.018 min
Response: 42489
Conc: 2.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248 MDL WATER

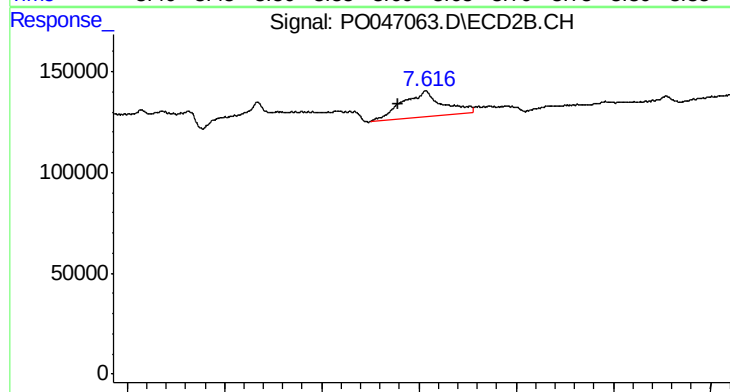


#41 AR-1268-1

R.T.: 7.614 min
Delta R.T.: 0.055 min
Response: 728293
Conc: 53.45 ng/ml

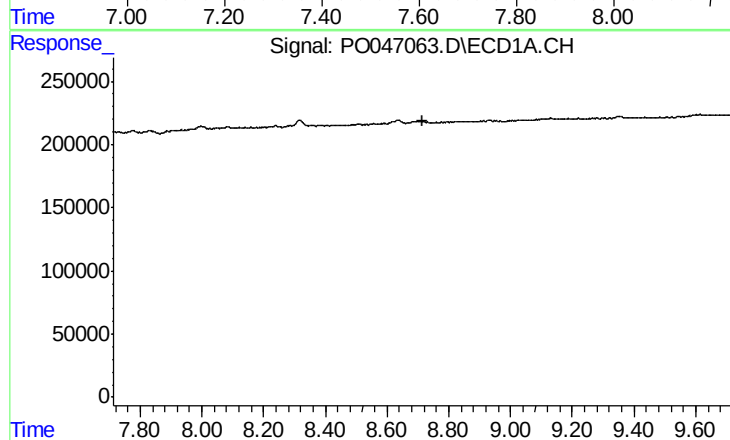


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.713 min
Response: 0
Conc: N.D.

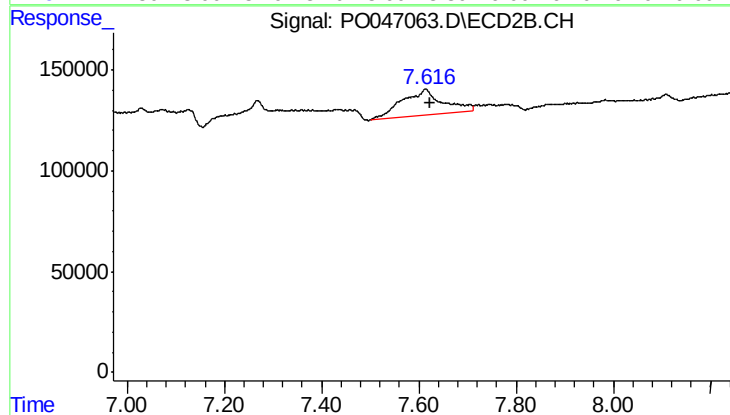

#42 AR-1268-2


R.T.: 7.614 min
Delta R.T.: -0.008 min
Response: 728293
Conc: 58.03 ng/ml

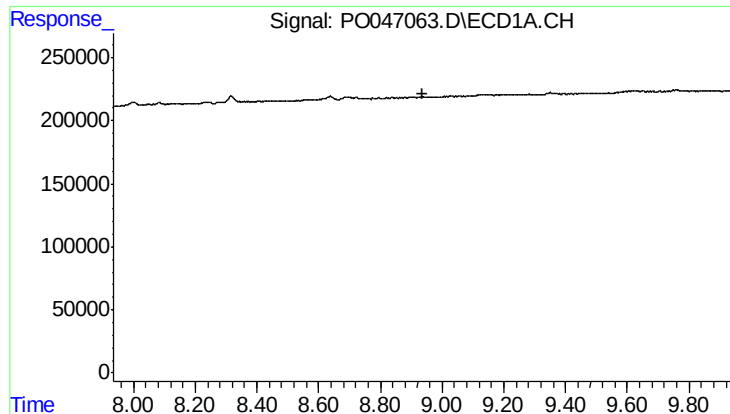

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.935 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
AR1248 MDL WATER

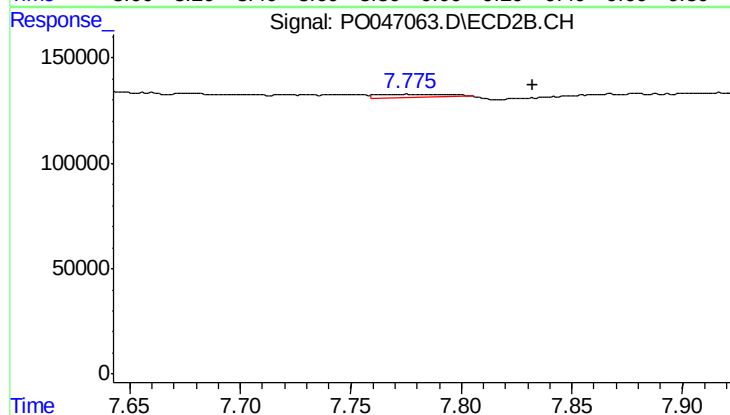


#43 AR-1268-3

R.T.: 7.780 min
Delta R.T.: -0.052 min
Response: 37735
Conc: 3.75 ng/ml

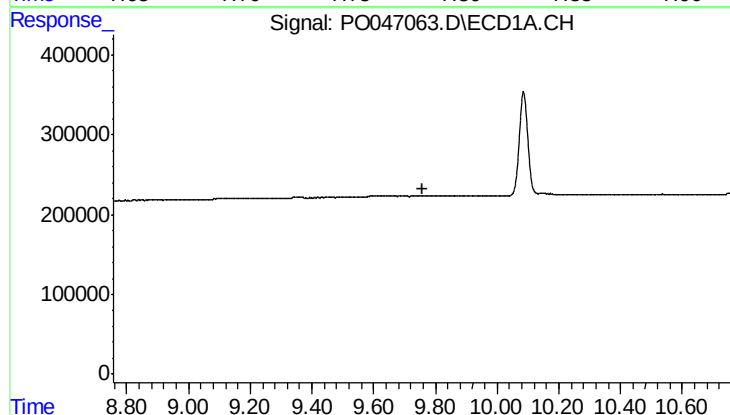

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.756 min
Response: 0
Conc: N.D.

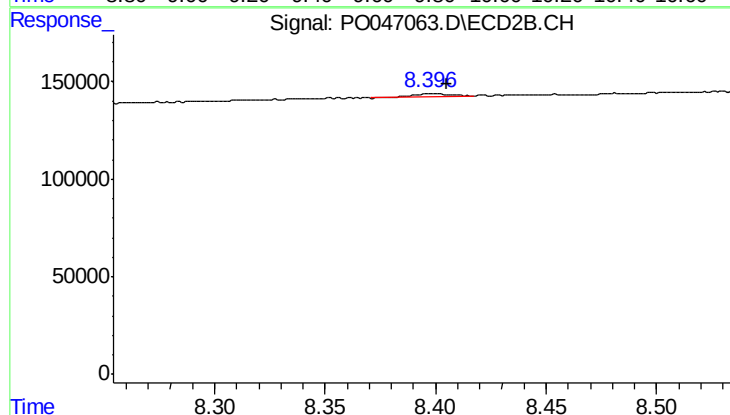

#45 AR-1268-5

R.T.: 8.398 min
Delta R.T.: -0.007 min
Response: 18534
Conc: 0.62 ng/ml