

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072318\
 Data File : P0047072.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jul 2018 7:06
 Operator : SM/SJ
 Sample : AR126 MDL WATER
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 AR1262 MDL WATER

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 07:33:07 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jul 24 03:04:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.397	3.649	3460292	3758507	20.638	19.596
2) SA Decachlor...	10.086	8.653	2869377	2404026	26.211	26.176
Target Compounds						
9) L2 AR-1221-2	4.703	3.949	39170	44367	32.967	37.028
10) L2 AR-1221-3	4.703	0.000	39170	0	10.566	N.D. #
30) L6 AR-1254-5	7.504	0.000	60319	0	12.703	N.D. #
33) L7 AR-1260-3	7.642	6.769	38815	119364	4.527	15.899 #
34) L7 AR-1260-4	8.314	7.268	117961	159151	9.744	13.647 #
35) L7 AR-1260-5	8.619	7.616	535376	560233	72.575	67.561
38) L8 AR-1262-3	7.776	6.769	140953	119364	17.081	14.666
39) L8 AR-1262-4	8.019	7.028	200242	155486	25.066	21.906
40) L8 AR-1262-5	8.314	7.268	117961	159151	7.918	11.370 #
41) L9 AR-1268-1	8.619	7.552	535376	572604	34.182	42.024
42) L9 AR-1268-2	8.711	7.616	477300	560233	34.060	44.638 #
43) L9 AR-1268-3	8.934	7.825	394815	356074	33.852	35.393
44) L9 AR-1268-4	9.353	8.108	169315	156690	33.506	35.773
45) L9 AR-1268-5	9.757	8.398	1269073	1170296	34.682	38.981



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0072318\
Data File : P0047072.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jul 2018 7:06
Operator : SM/SJ
Sample : AR126 MDL WATER
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1262 MDL WATER

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 07:33:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0072318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jul 24 03:04:21 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

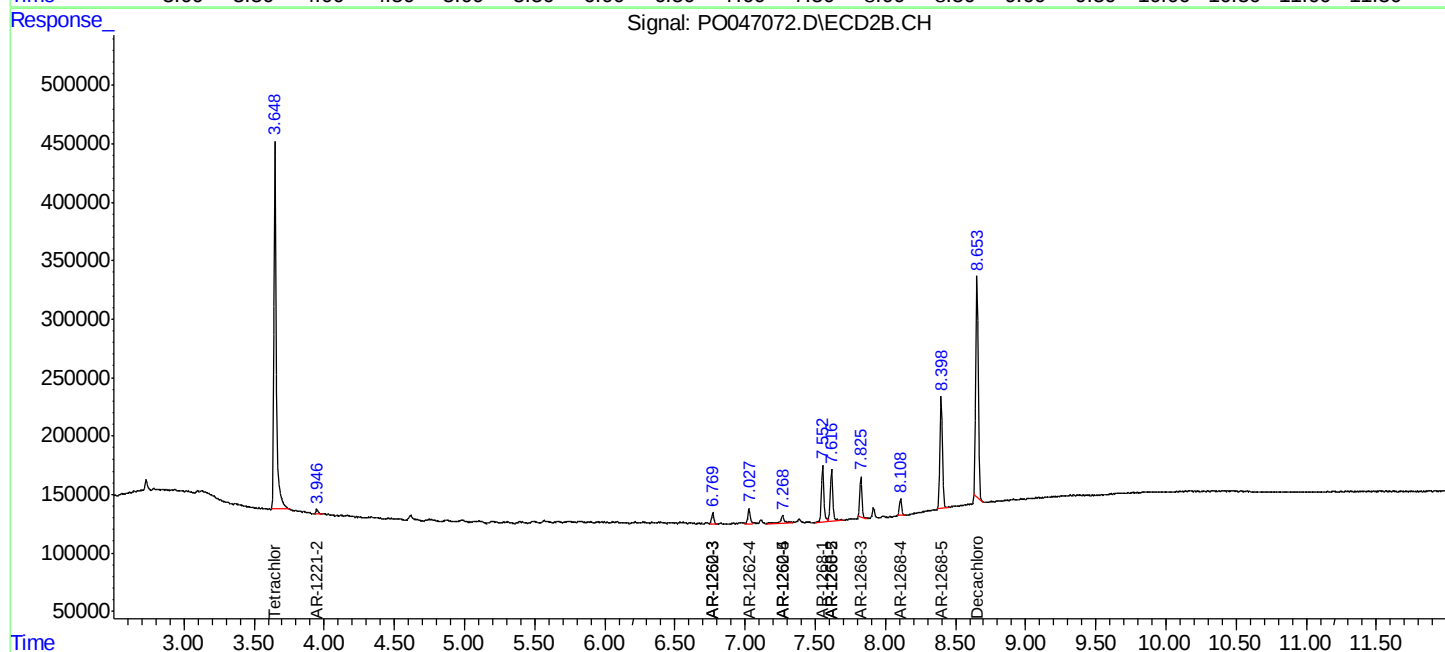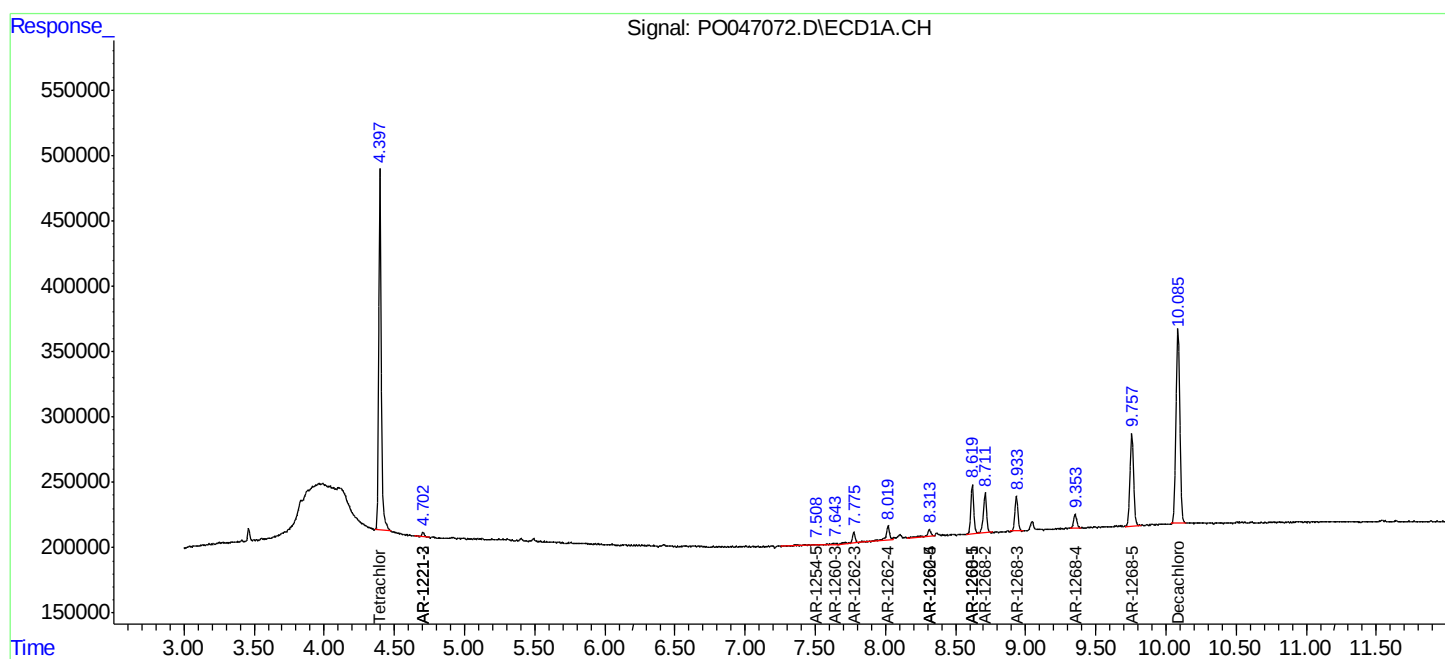


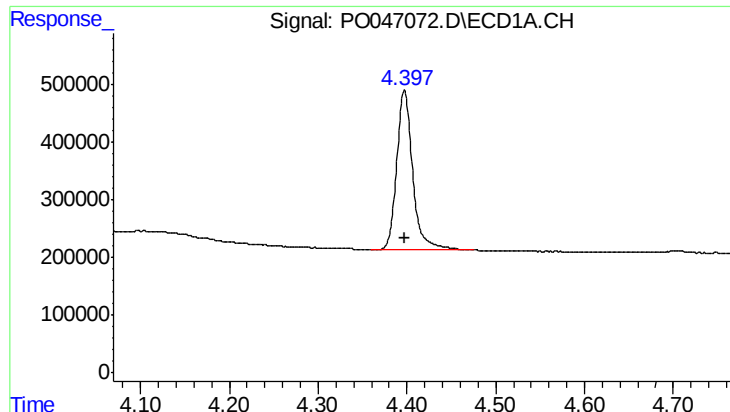

#1 Tetrachloro-m-xylene


R.T.: 4.397 min
Delta R.T.: 0.000 min
Response: 3460292
Conc: 20.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1262 MDL WATER

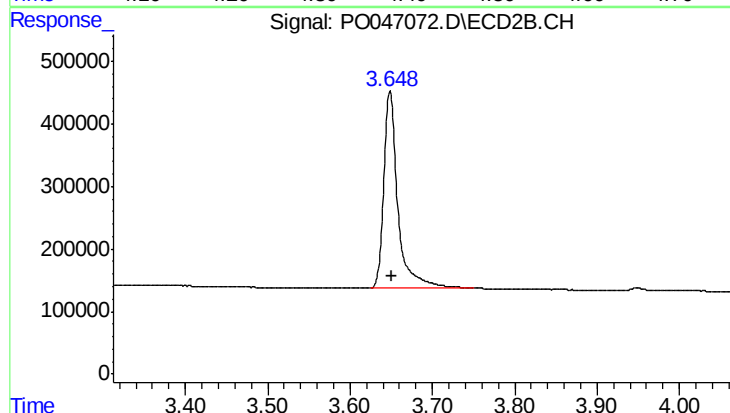


#1 Tetrachloro-m-xylene

R.T.: 3.649 min
Delta R.T.: -0.002 min
Response: 3758507
Conc: 19.60 ng/ml

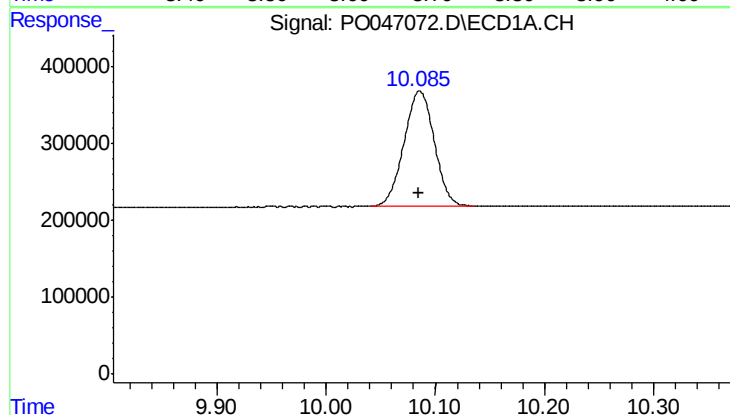


#2 Decachlorobiphenyl

R.T.: 10.086 min
Delta R.T.: 0.002 min
Response: 2869377
Conc: 26.21 ng/ml

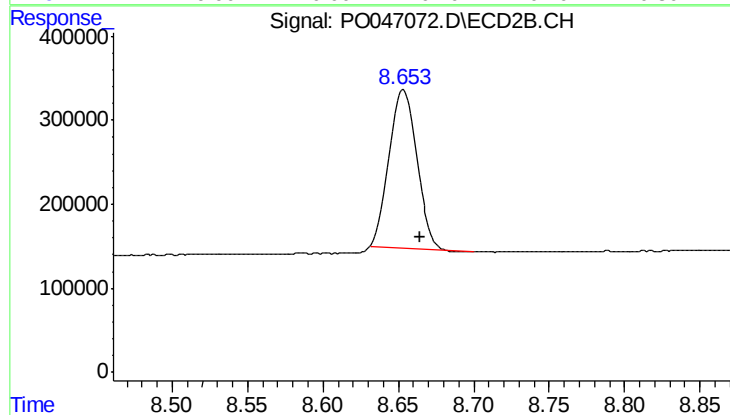

#2 Decachlorobiphenyl


R.T.: 8.653 min
Delta R.T.: -0.011 min
Response: 2404026
Conc: 26.18 ng/ml

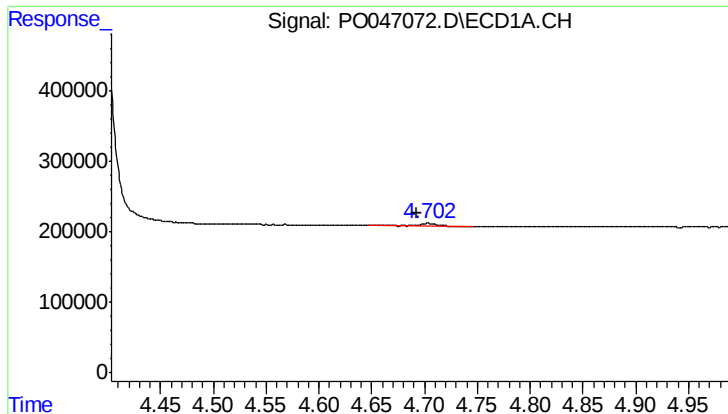

#9 AR-1221-2


R.T.: 4.703 min
Delta R.T.: 0.011 min
Response: 39170
Conc: 32.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1262 MDL WATER

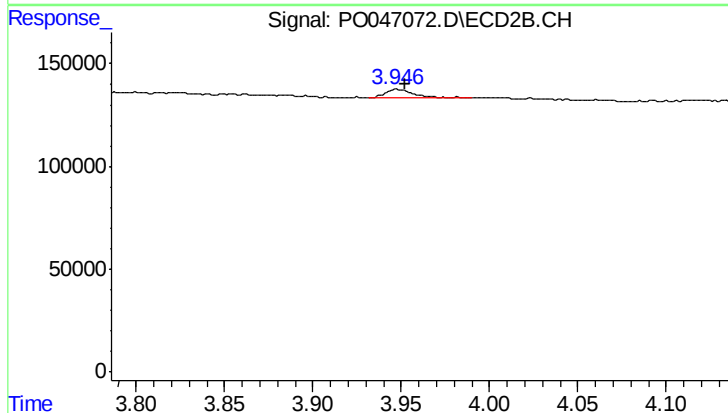


#9 AR-1221-2

R.T.: 3.949 min
Delta R.T.: -0.004 min
Response: 44367
Conc: 37.03 ng/ml

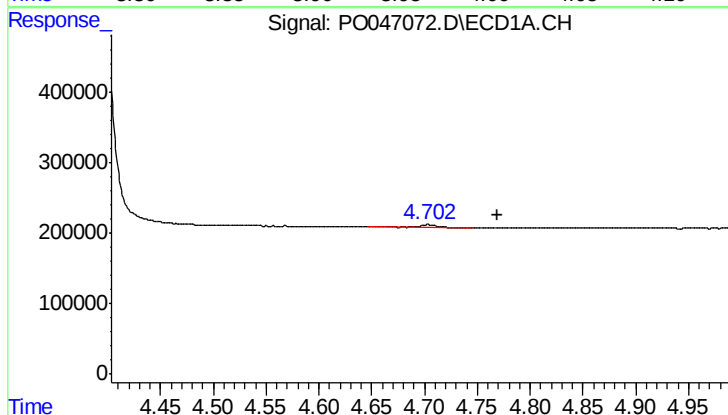


#10 AR-1221-3

R.T.: 4.703 min
Delta R.T.: -0.066 min
Response: 39170
Conc: 10.57 ng/ml

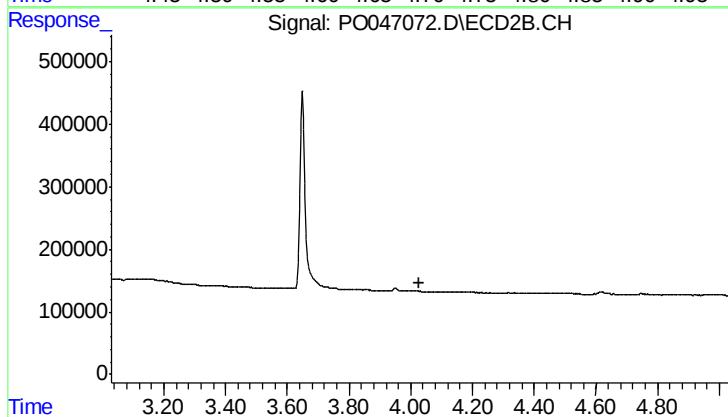

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 4.029 min
Response: 0
Conc: N.D.

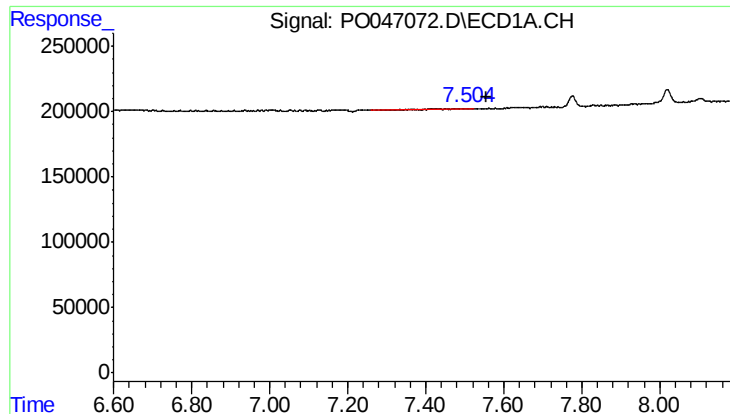

#30 AR-1254-5


R.T.: 7.504 min
Delta R.T.: -0.053 min
Response: 60319
Conc: 12.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1262 MDL WATER

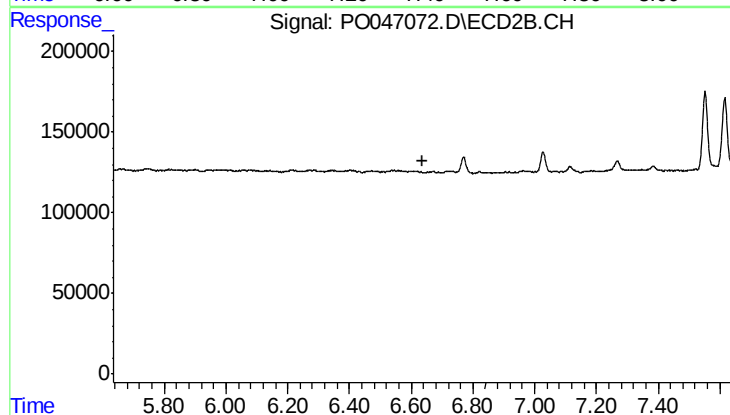


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T.: 6.635 min
Response: 0
Conc: N.D.

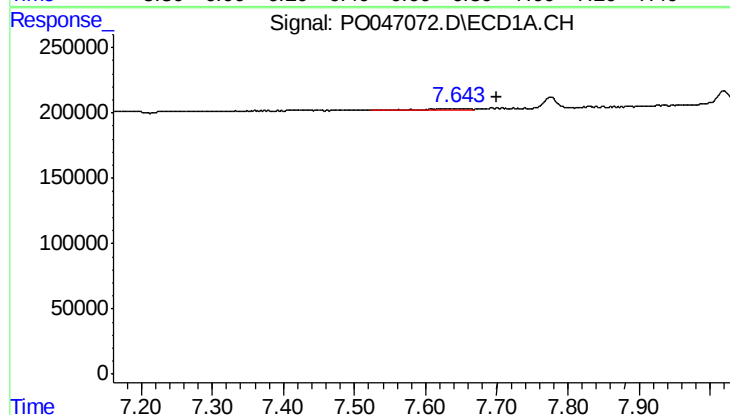


#33 AR-1260-3

R.T.: 7.642 min
Delta R.T.: -0.058 min
Response: 38815
Conc: 4.53 ng/ml

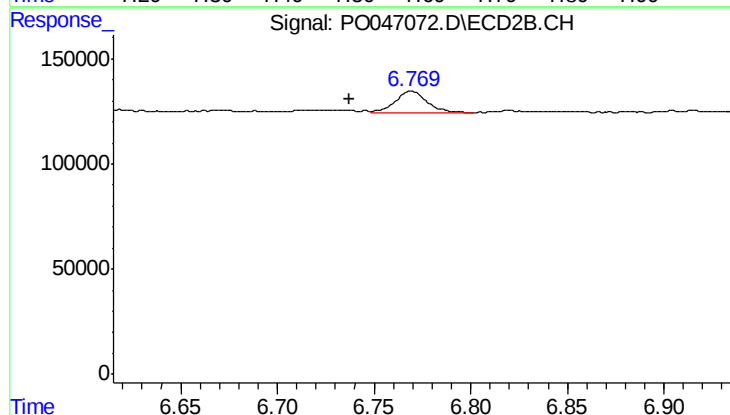

#33 AR-1260-3


R.T.: 6.769 min
Delta R.T.: 0.032 min
Response: 119364
Conc: 15.90 ng/ml

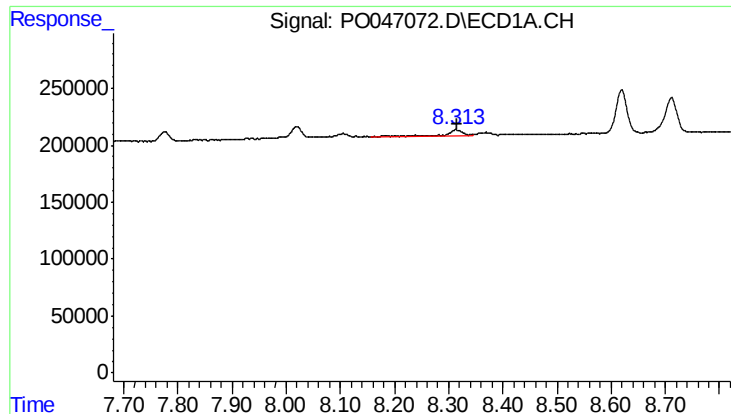

#34 AR-1260-4


R.T.: 8.314 min
Delta R.T.: -0.002 min
Response: 117961
Conc: 9.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1262 MDL WATER

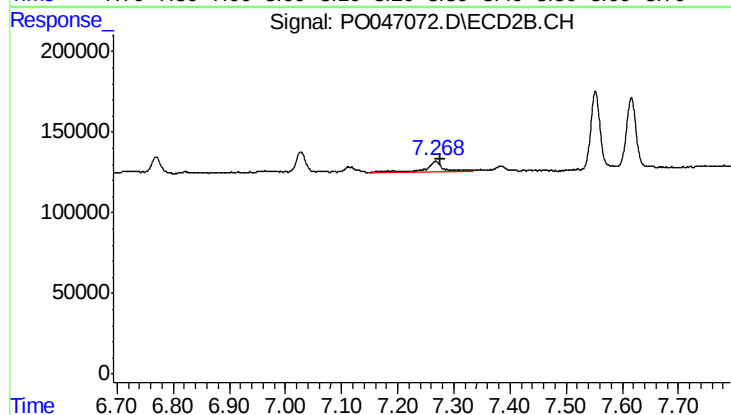


#34 AR-1260-4

R.T.: 7.268 min
Delta R.T.: -0.008 min
Response: 159151
Conc: 13.65 ng/ml

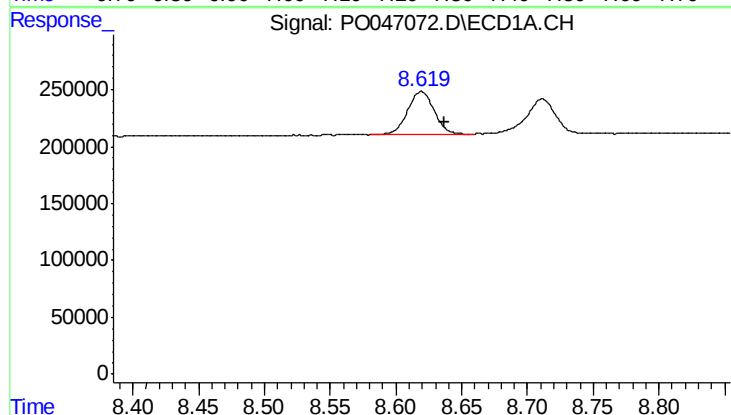


#35 AR-1260-5

R.T.: 8.619 min
Delta R.T.: -0.018 min
Response: 535376
Conc: 72.57 ng/ml

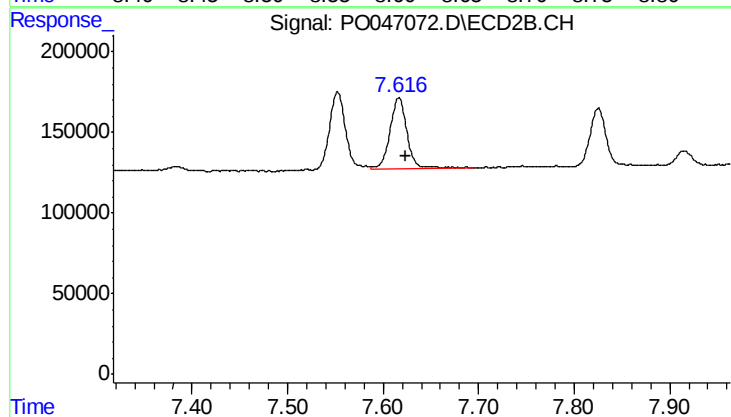

#35 AR-1260-5


R.T.: 7.616 min
Delta R.T.: -0.007 min
Response: 560233
Conc: 67.56 ng/ml

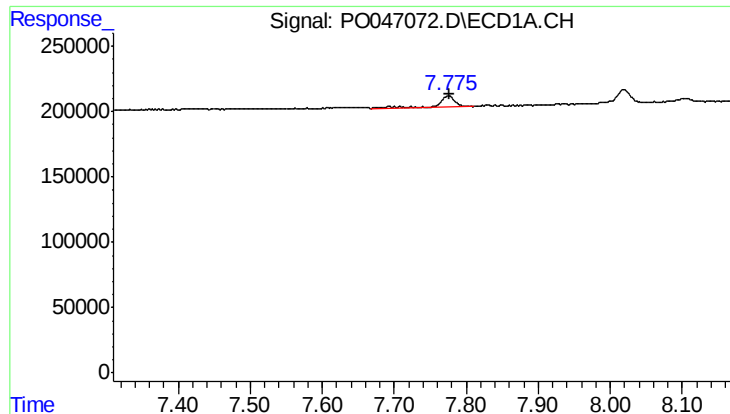

#38 AR-1262-3


R.T.: 7.776 min
Delta R.T.: 0.000 min
Response: 140953
Conc: 17.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1262 MDL WATER

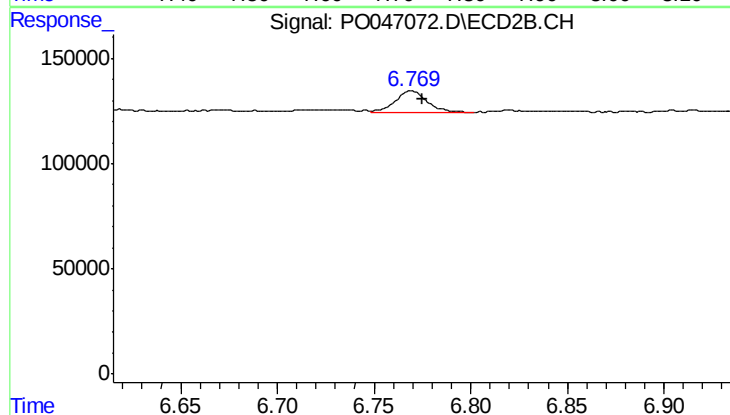


#38 AR-1262-3

R.T.: 6.769 min
Delta R.T.: -0.006 min
Response: 119364
Conc: 14.67 ng/ml

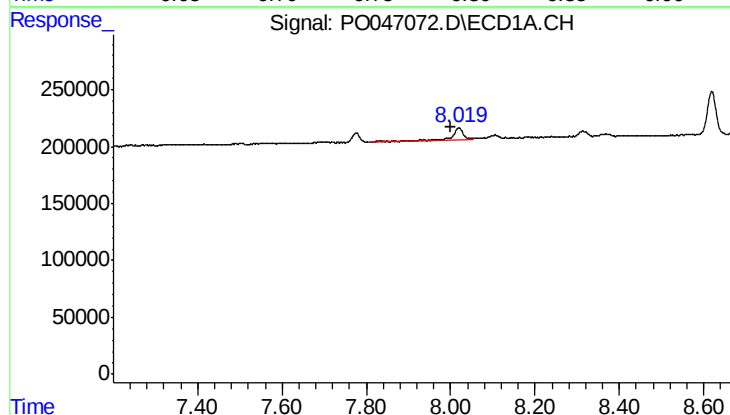


#39 AR-1262-4

R.T.: 8.019 min
Delta R.T.: 0.018 min
Response: 200242
Conc: 25.07 ng/ml

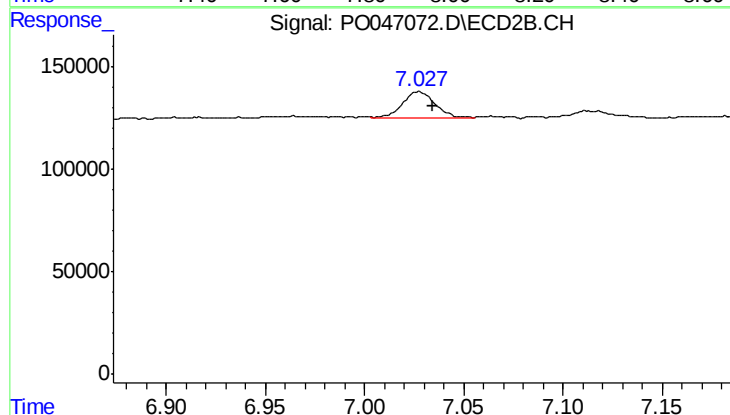

#39 AR-1262-4


R.T.: 7.028 min
Delta R.T.: -0.007 min
Response: 155486
Conc: 21.91 ng/ml

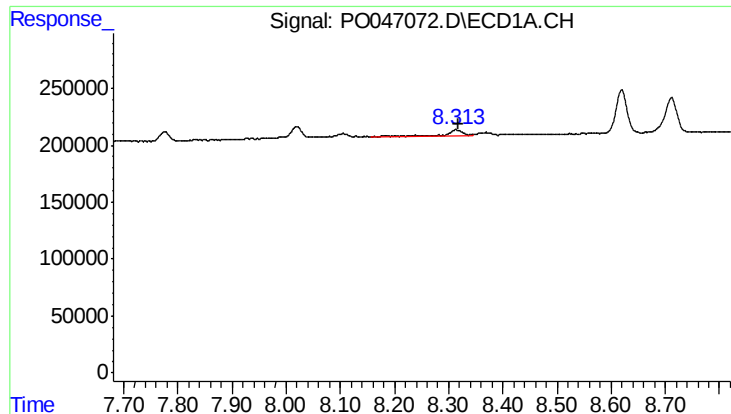

#40 AR-1262-5


R.T.: 8.314 min
Delta R.T.: -0.003 min
Response: 117961
Conc: 7.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1262 MDL WATER

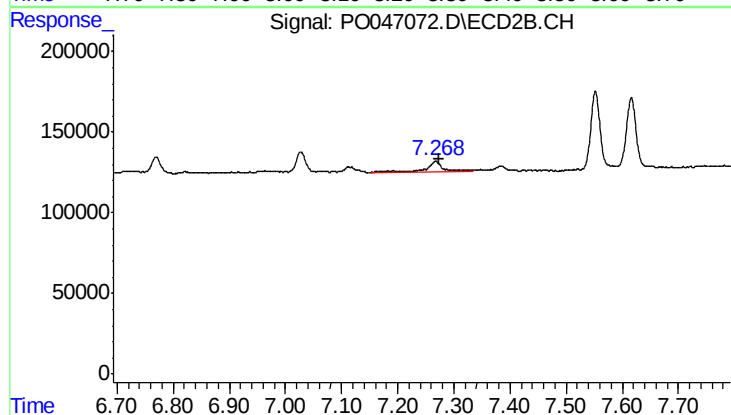


#40 AR-1262-5

R.T.: 7.268 min
Delta R.T.: -0.006 min
Response: 159151
Conc: 11.37 ng/ml

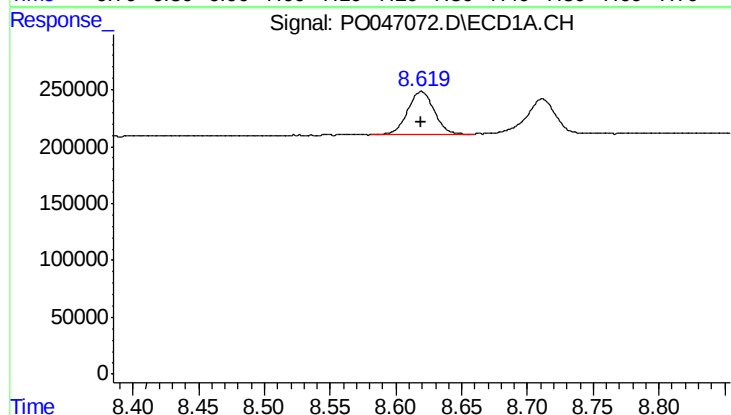


#41 AR-1268-1

R.T.: 8.619 min
Delta R.T.: 0.000 min
Response: 535376
Conc: 34.18 ng/ml

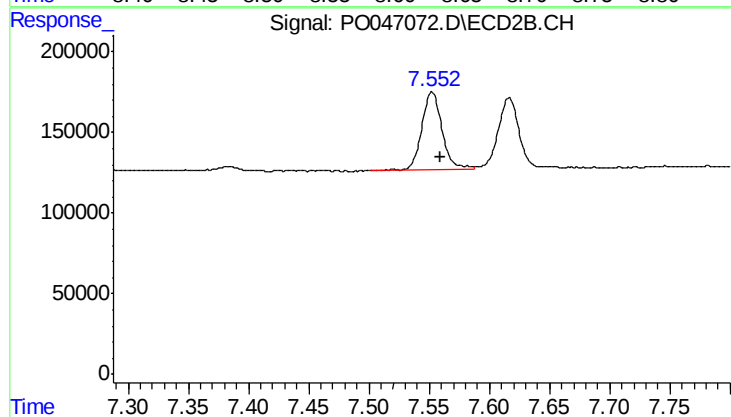

#41 AR-1268-1


R.T.: 7.552 min
Delta R.T.: -0.007 min
Response: 572604
Conc: 42.02 ng/ml

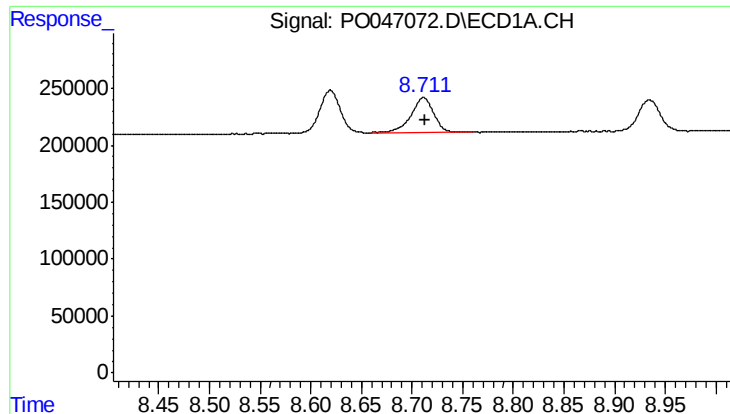

#42 AR-1268-2


R.T.: 8.711 min
Delta R.T.: -0.002 min
Response: 477300
Conc: 34.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1262 MDL WATER

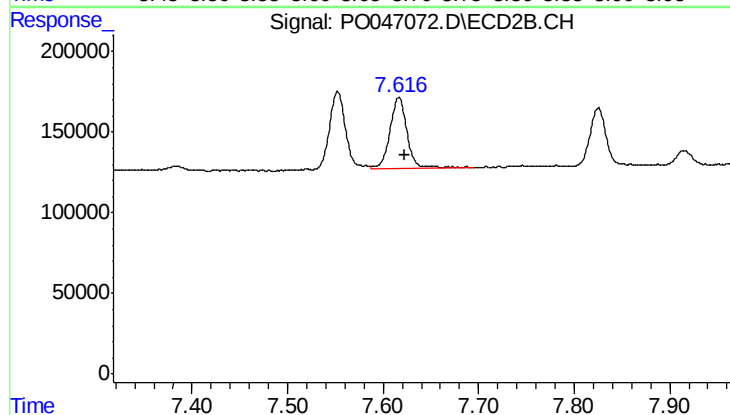


#42 AR-1268-2

R.T.: 7.616 min
Delta R.T.: -0.006 min
Response: 560233
Conc: 44.64 ng/ml

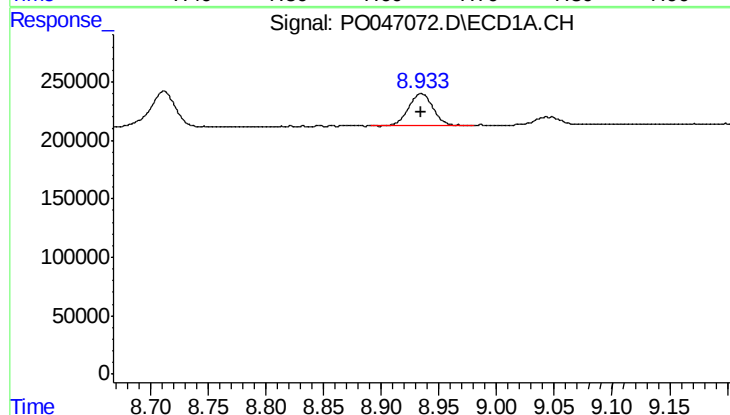


#43 AR-1268-3

R.T.: 8.934 min
Delta R.T.: 0.000 min
Response: 394815
Conc: 33.85 ng/ml

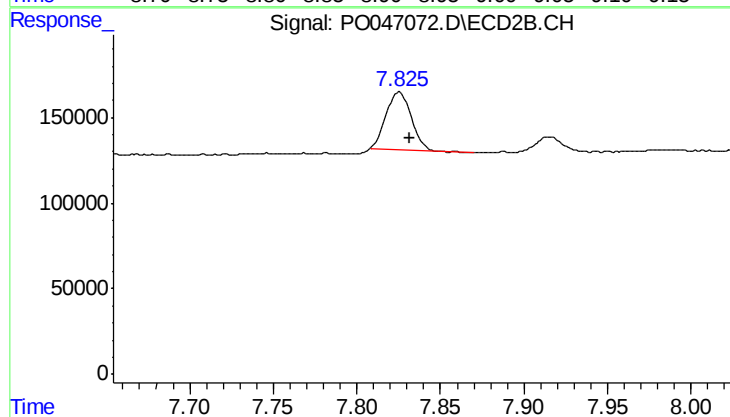

#43 AR-1268-3


R.T.: 7.825 min
Delta R.T.: -0.007 min
Response: 356074
Conc: 35.39 ng/ml

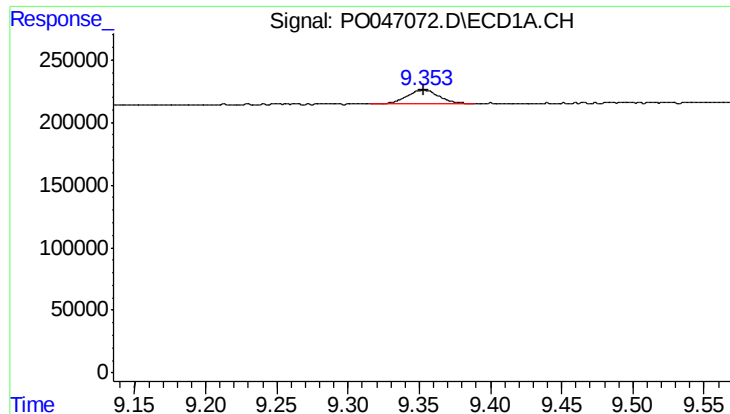

#44 AR-1268-4


R.T.: 9.353 min
Delta R.T.: 0.000 min
Response: 169315
Conc: 33.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1262 MDL WATER

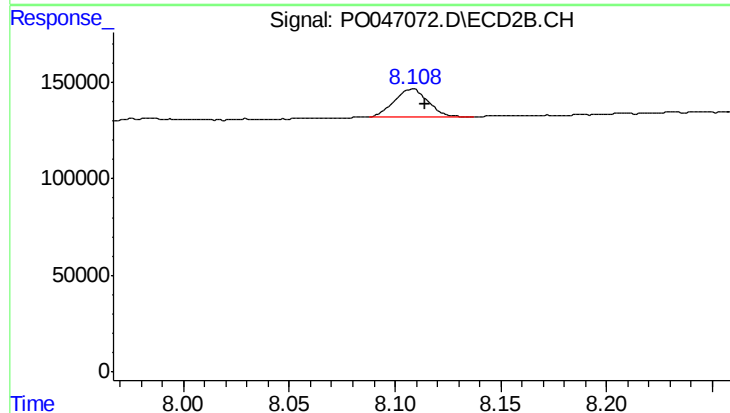


#44 AR-1268-4

R.T.: 8.108 min
Delta R.T.: -0.006 min
Response: 156690
Conc: 35.77 ng/ml

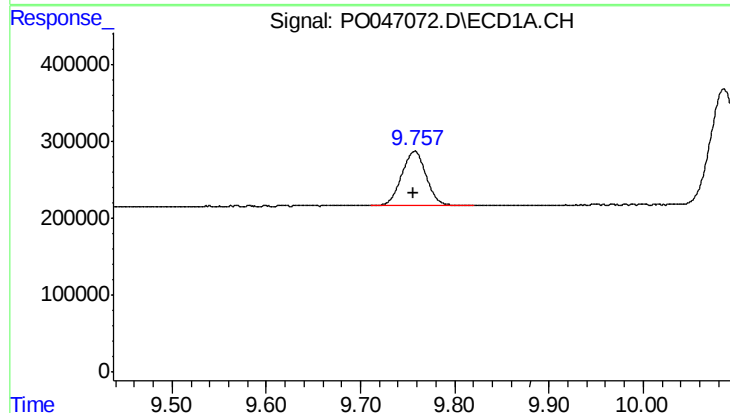

#45 AR-1268-5

R.T.: 9.757 min
Delta R.T.: 0.000 min
Response: 1269073
Conc: 34.68 ng/ml

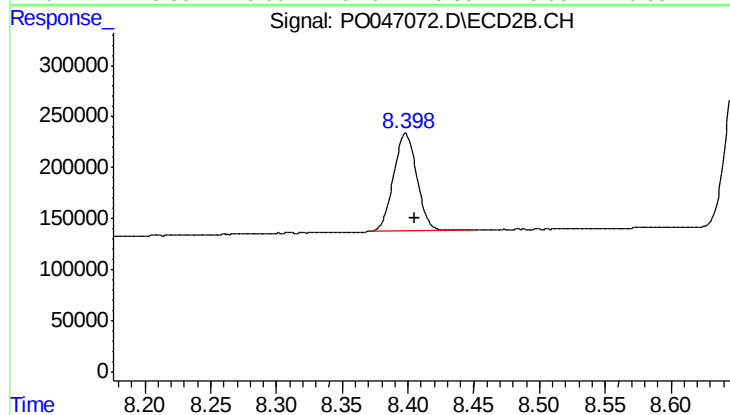

#45 AR-1268-5

R.T.: 8.398 min
Delta R.T.: -0.007 min
Response: 1170296
Conc: 38.98 ng/ml